

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031119\
 Data File : PS003500.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2019 14:35
 Operator : EI\SJ
 Sample : K1787-04
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 01:18:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.289	10.791	197.9E6	216.4E6	450.716	460.750
Target Compounds							
1) T	Dalapon	2.804	2.294	29978821	44094552	46.125	69.639 #
2) T	3,5-DICHL...	0.000	8.955	0	7125484	N.D.	11.540 #
5) T	DICAMBA	0.000	11.031	0	3546559	N.D.	2.123 #
6) T	MCP	0.000	11.274	0	312457	N.D.	0.265 #
9) T	2,4-D	13.145	12.651	5220688	2130737	11.256	4.059 #
12) T	2,4,5-T	0.000	14.392	0	6133321	N.D.	3.041 #
13) T	2,4-DB	15.480	0.000	6143046	0	25.942	N.D. #
14) T	DINOSEB	0.000	15.435	0	1213887	N.D.	0.680 #
15) T	Picloram	16.785	16.747	3468910	15378290	1.409	6.059 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031119\
Data File : PS003500.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2019 14:35
Operator : EI\SJ
Sample : K1787-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
SP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 01:18:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

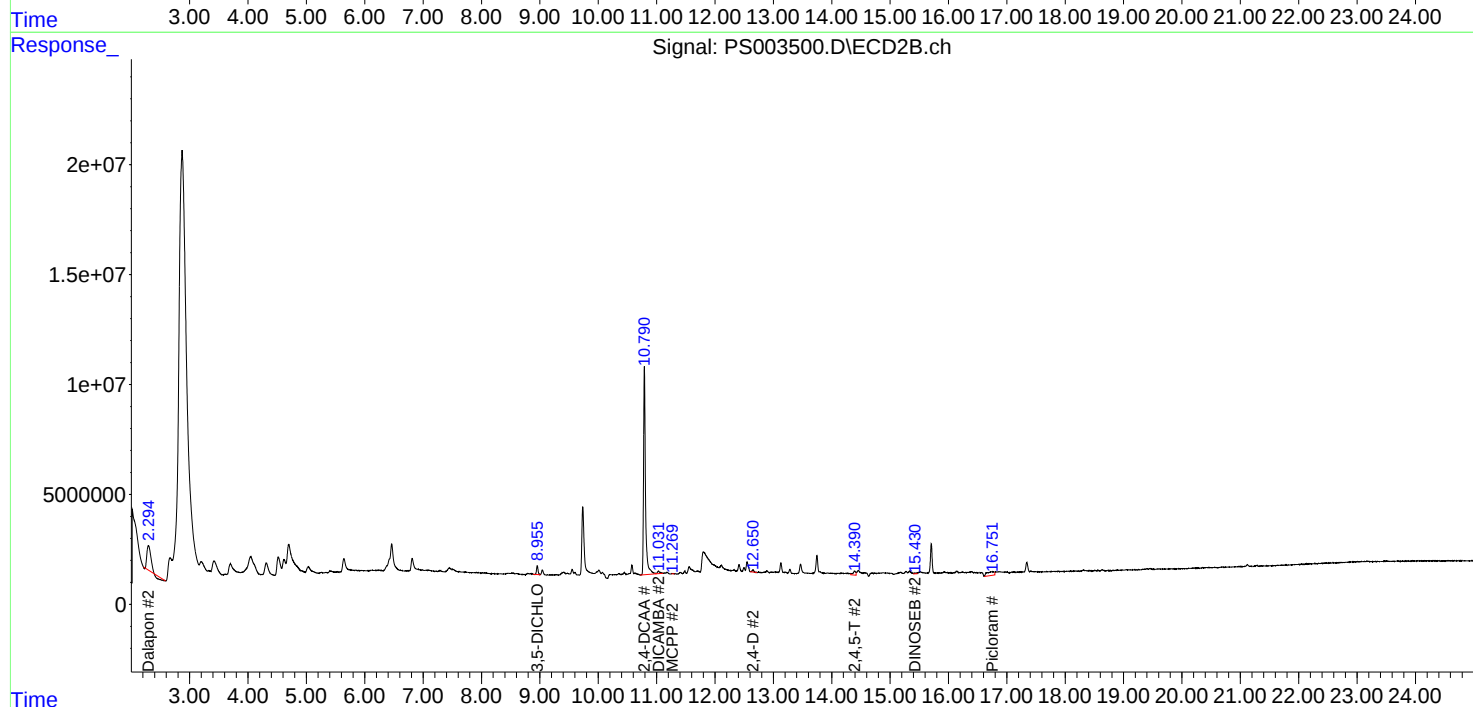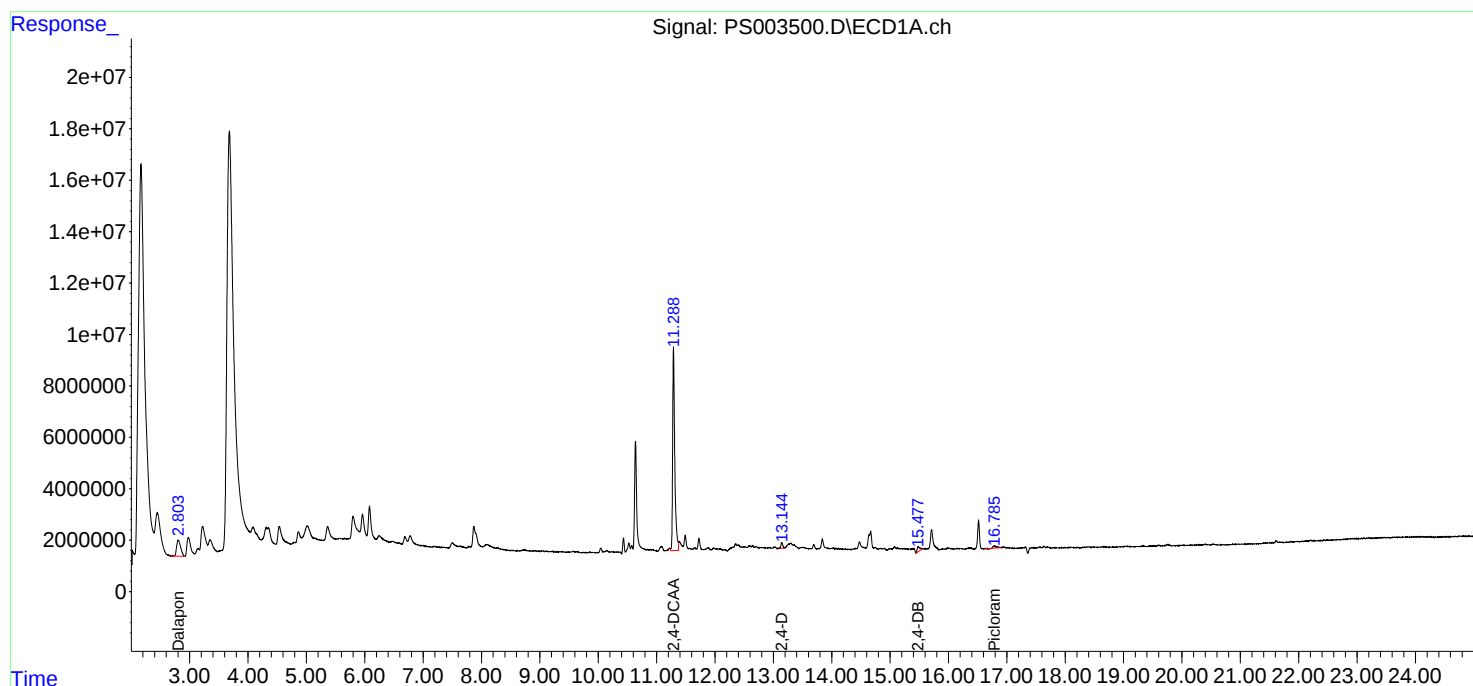


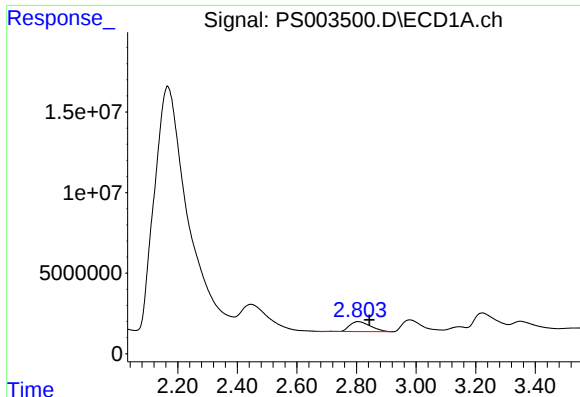

#1 Dalapon


R.T.: 2.804 min
Delta R.T.: -0.040 min
Response: 29978821
Conc: 46.13 ng/ml

Instrument :
ECD_S
ClientSampleId :
SP-1

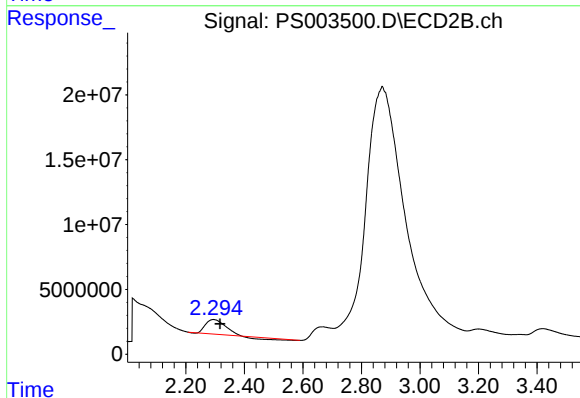


#1 Dalapon

R.T.: 2.294 min
Delta R.T.: -0.022 min
Response: 44094552
Conc: 69.64 ng/ml

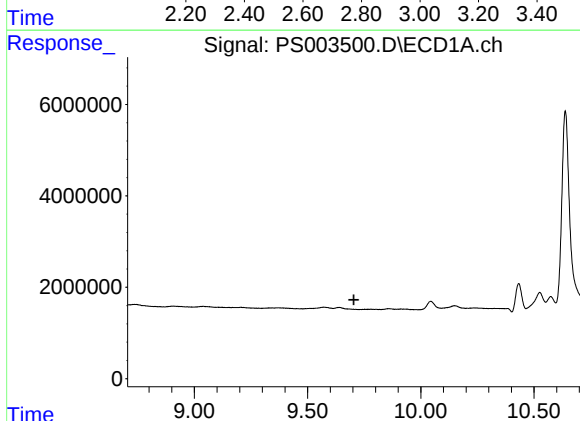


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.705 min
Response: 0
Conc: N.D.

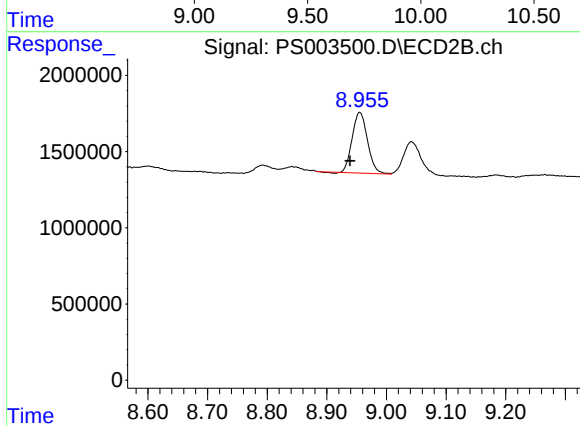

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.955 min
Delta R.T.: 0.016 min
Response: 7125484
Conc: 11.54 ng/ml

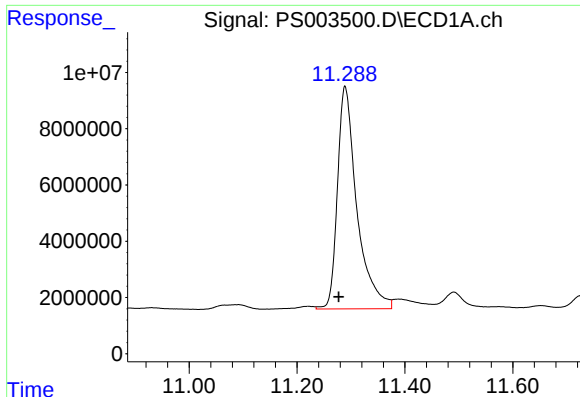

#4 2,4-DCAA


R.T.: 11.289 min
Delta R.T.: 0.012 min
Response: 197875338
Conc: 450.72 ng/ml

Instrument :
ECD_S
ClientSampleId :
SP-1

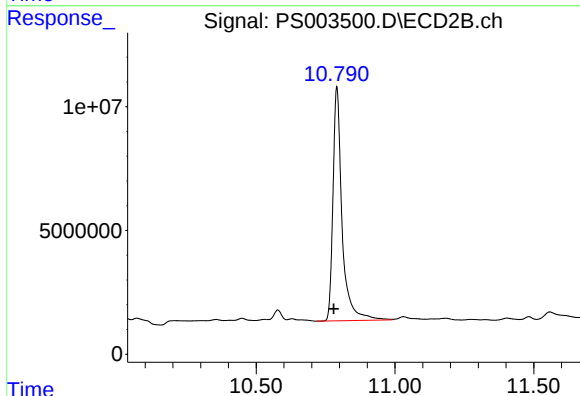


#4 2,4-DCAA

R.T.: 10.791 min
Delta R.T.: 0.011 min
Response: 216353815
Conc: 460.75 ng/ml

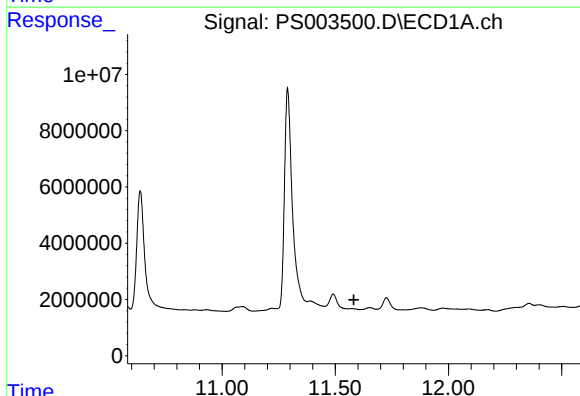


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.582 min
Response: 0
Conc: N.D.

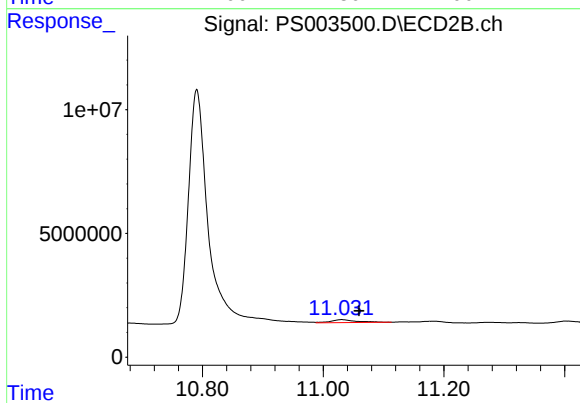

#5 DICAMBA


R.T.: 11.031 min
Delta R.T.: -0.029 min
Response: 3546559
Conc: 2.12 ng/ml

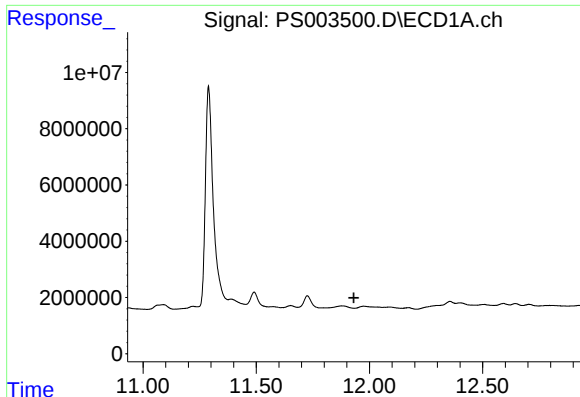

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.931 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SP-1

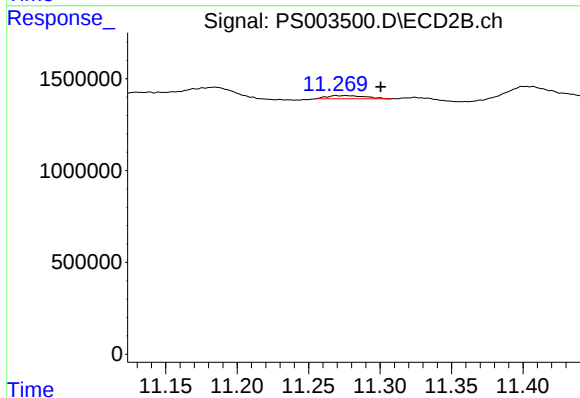


#6 MCP

R.T.: 11.274 min
Delta R.T.: -0.026 min
Response: 312457
Conc: 0.26 ug/ml

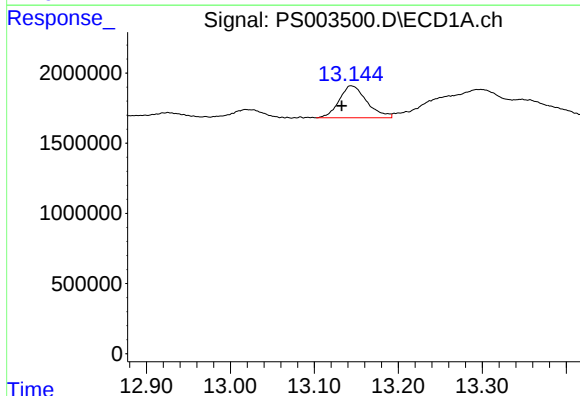


#9 2,4-D

R.T.: 13.145 min
Delta R.T.: 0.012 min
Response: 5220688
Conc: 11.26 ng/ml

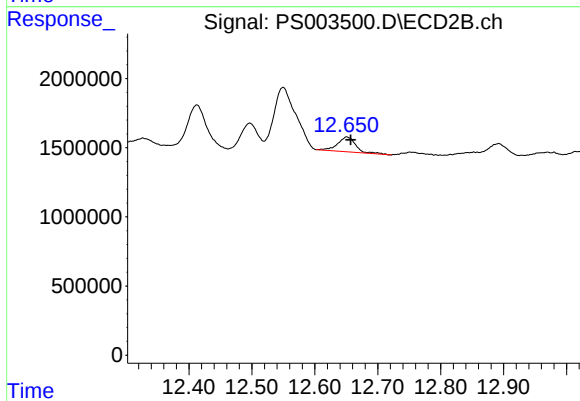

#9 2,4-D


R.T.: 12.651 min
Delta R.T.: -0.006 min
Response: 2130737
Conc: 4.06 ng/ml

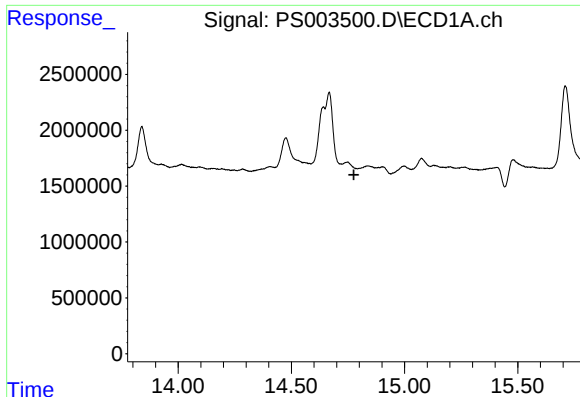

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SP-1

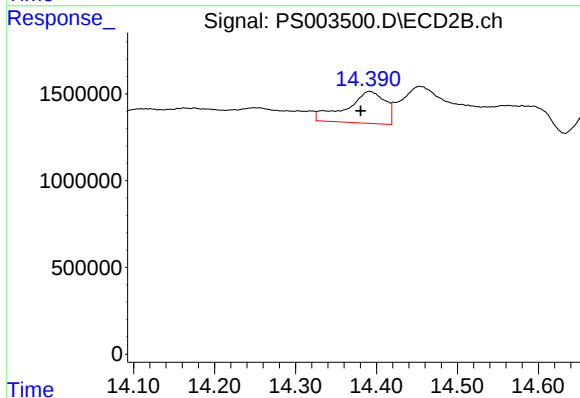


#12 2,4,5-T

R.T.: 14.392 min
Delta R.T.: 0.012 min
Response: 6133321
Conc: 3.04 ng/ml

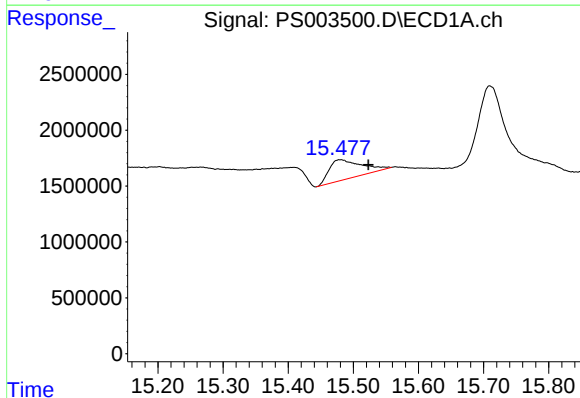


#13 2,4-DB

R.T.: 15.480 min
Delta R.T.: -0.043 min
Response: 6143046
Conc: 25.94 ng/ml

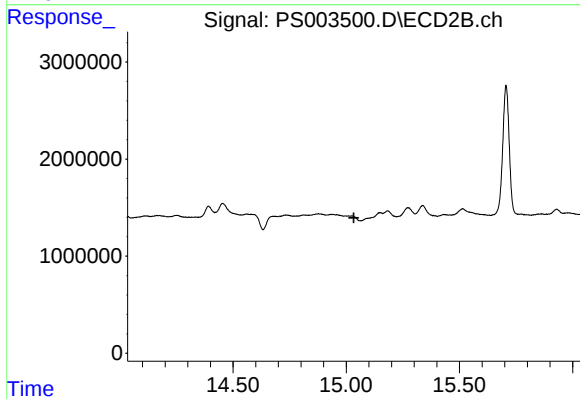

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.033 min
Response: 0
Conc: N.D.

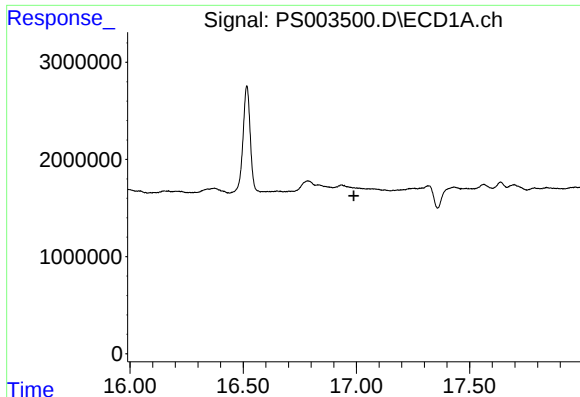

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SP-1

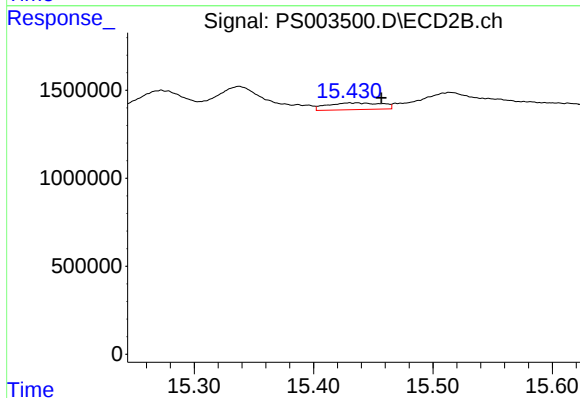


#14 DINOSEB

R.T.: 15.435 min
Delta R.T.: -0.022 min
Response: 1213887
Conc: 0.68 ng/ml

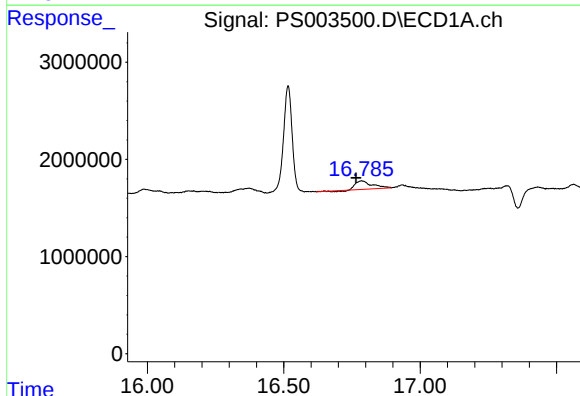

#15 Picloram

R.T.: 16.785 min
Delta R.T.: 0.020 min
Response: 3468910
Conc: 1.41 ng/ml

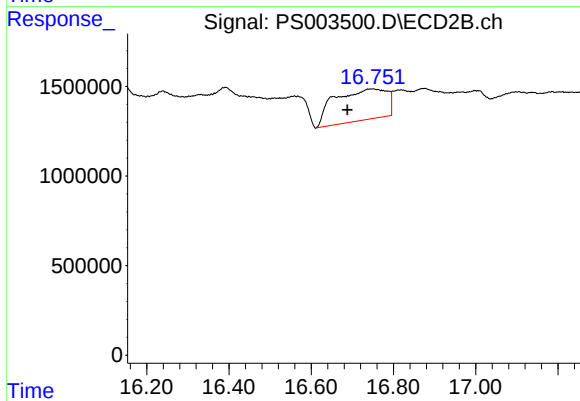

#15 Picloram

R.T.: 16.747 min
Delta R.T.: 0.059 min
Response: 15378290
Conc: 6.06 ng/ml