

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031119\
 Data File : PS003501.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2019 15:06
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 01:18:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.303	10.800	217.8E6	206.1E6	496.115	438.835
Target Compounds							
3) T	4-Nitroph...	0.000	9.949	0	44341	N.D.	0.197 #
7) T	MCPA	0.000	11.690	0	334233	N.D.	0.194 #
10) T	Pentachlo...	0.000	13.217	0	646997	N.D.	0.098 #
11) T	2,4,5-TP ...	0.000	13.770	0	229863	N.D.	0.090 #
12) T	2,4,5-T	0.000	14.370	0	70566	N.D.	0.035 #
13) T	2,4-DB	0.000	15.041	0	514340	N.D.	2.014 #
14) T	DINOSEB	0.000	15.446	0	107331	N.D.	0.060 #
15) T	Picloram	0.000	16.711	0	120377	N.D.	0.047 #
16) T	DCPA	0.000	16.653	0	735585	N.D.	0.236 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031119\
Data File : PS003501.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2019 15:06
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 01:18:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

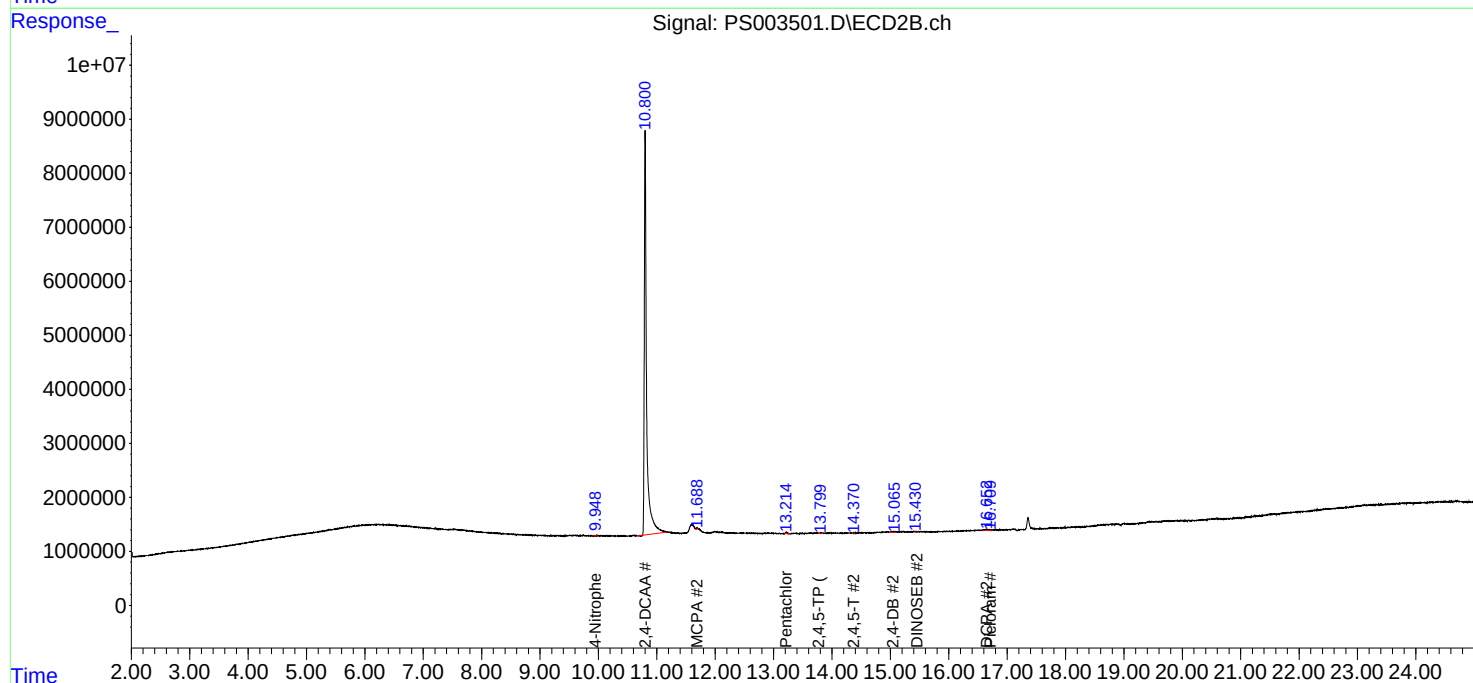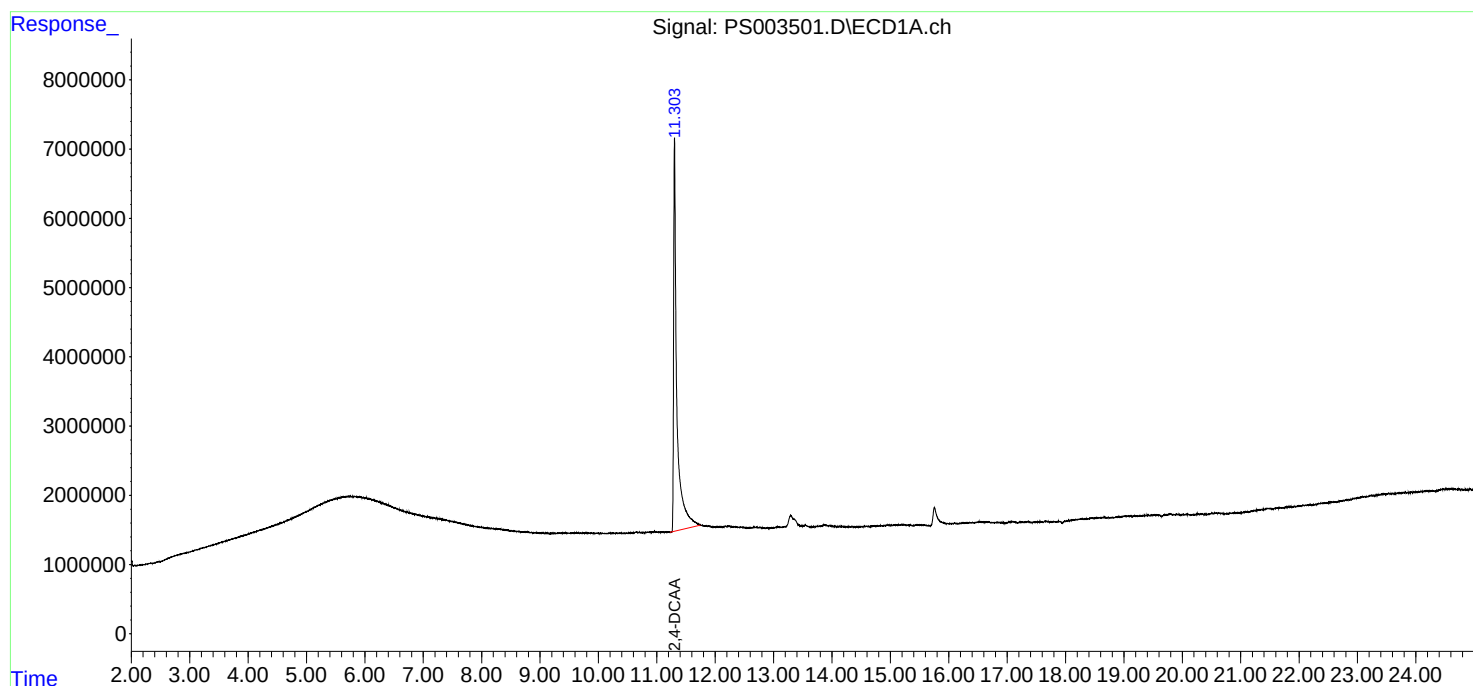


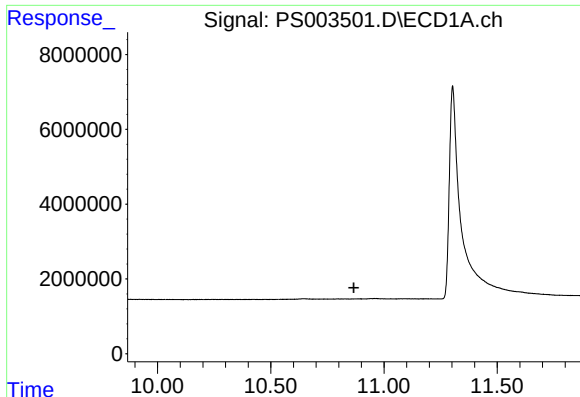

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

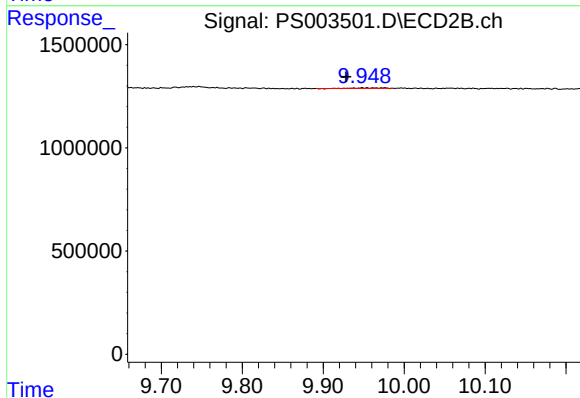


#3 4-Nitrophenol

R.T.: 9.949 min
Delta R.T.: 0.021 min
Response: 44341
Conc: 0.20 ng/ml

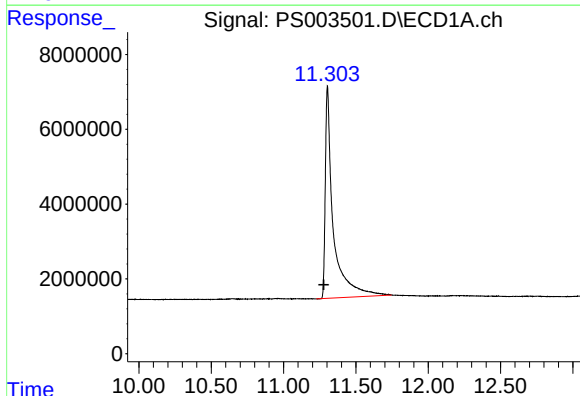


#4 2,4-DCAA

R.T.: 11.303 min
Delta R.T.: 0.026 min
Response: 217806451
Conc: 496.11 ng/ml

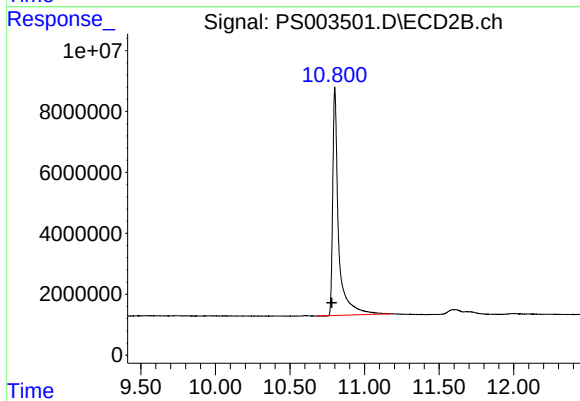

#4 2,4-DCAA


R.T.: 10.800 min
Delta R.T.: 0.020 min
Response: 206063202
Conc: 438.83 ng/ml

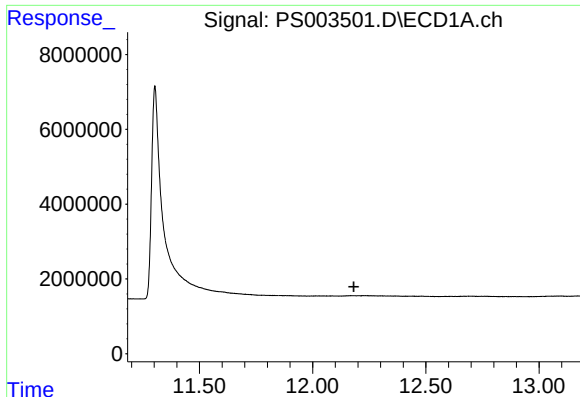

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.182 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

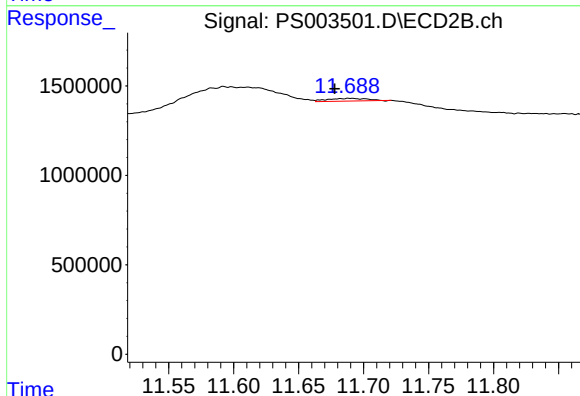


#7 MCPA

R.T.: 11.690 min
Delta R.T.: 0.012 min
Response: 334233
Conc: 0.19 ug/ml

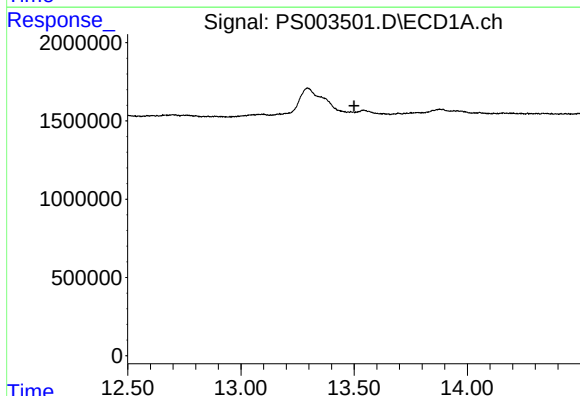


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 13.499 min
Response: 0
Conc: N.D.

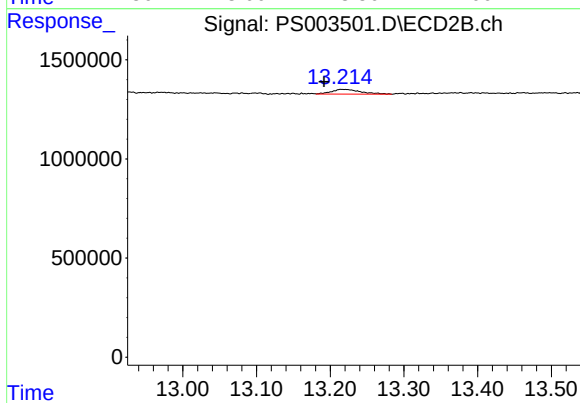

#10 Pentachlorophenol


R.T.: 13.217 min
Delta R.T.: 0.025 min
Response: 646997
Conc: 0.10 ng/ml

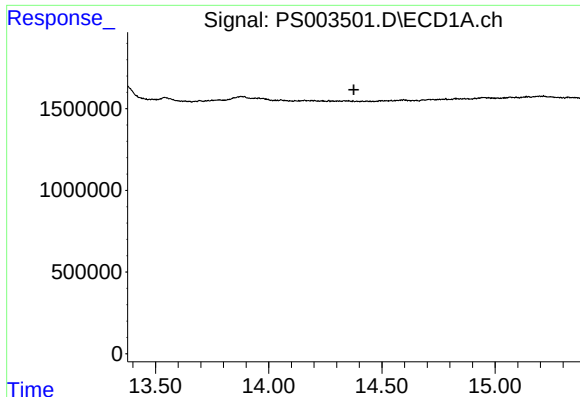

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

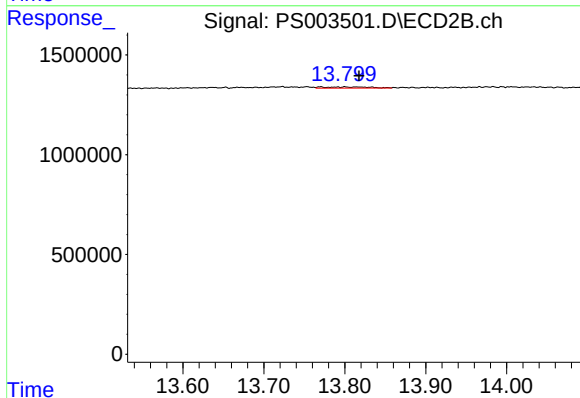


#11 2,4,5-TP (SILVEX)

R.T.: 13.770 min
Delta R.T.: -0.048 min
Response: 229863
Conc: 0.09 ng/ml

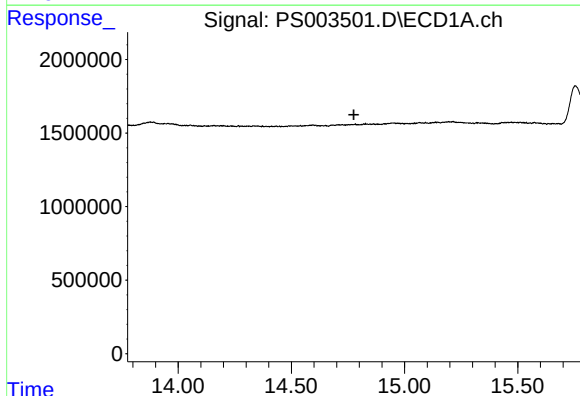


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

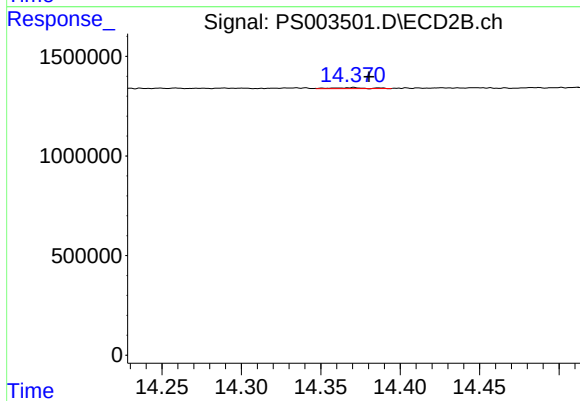

#12 2,4,5-T


R.T.: 14.370 min
Delta R.T.: -0.010 min
Response: 70566
Conc: 0.03 ng/ml

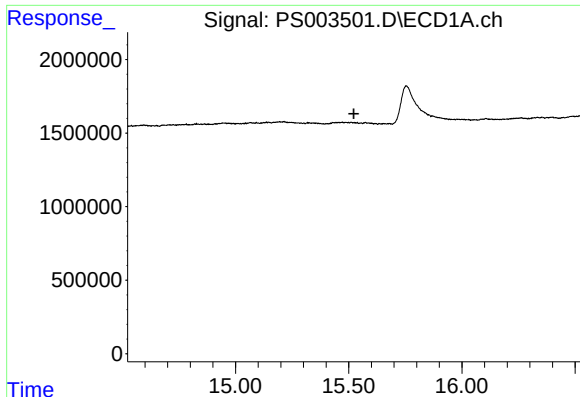

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.523 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

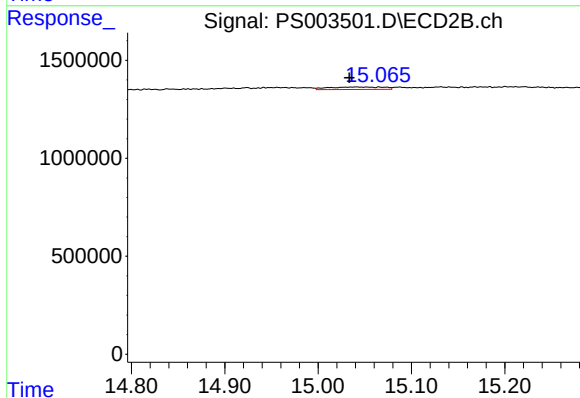


#13 2,4-DB

R.T.: 15.041 min
Delta R.T.: 0.007 min
Response: 514340
Conc: 2.01 ng/ml

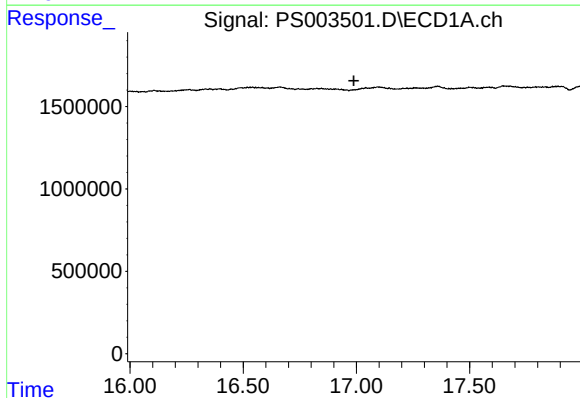


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

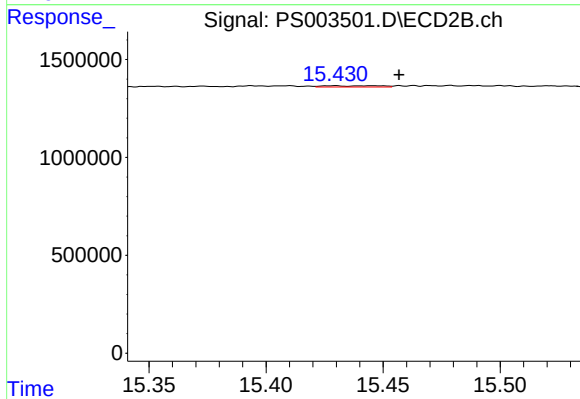

#14 DINOSEB


R.T.: 15.446 min
Delta R.T.: -0.011 min
Response: 107331
Conc: 0.06 ng/ml

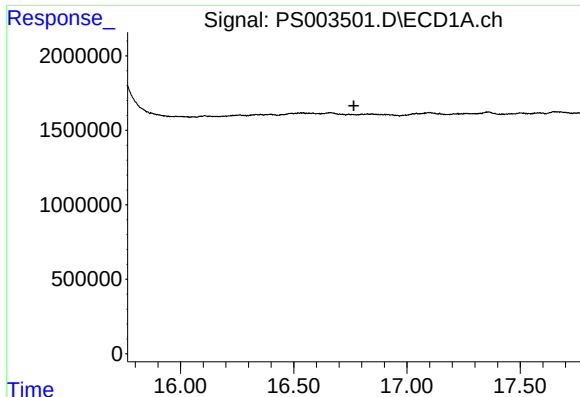

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.765 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

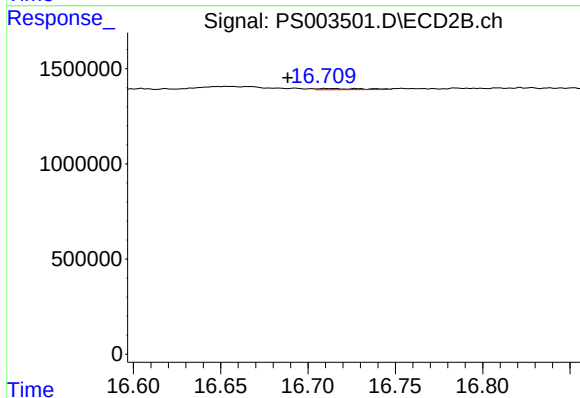


#15 Picloram

R.T.: 16.711 min
Delta R.T.: 0.023 min
Response: 120377
Conc: 0.05 ng/ml

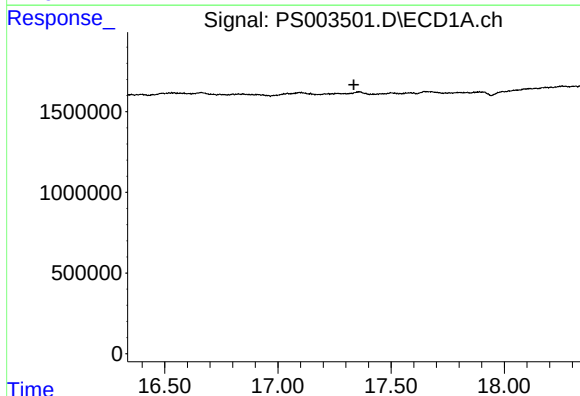

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.335 min
Response: 0
Conc: N.D.

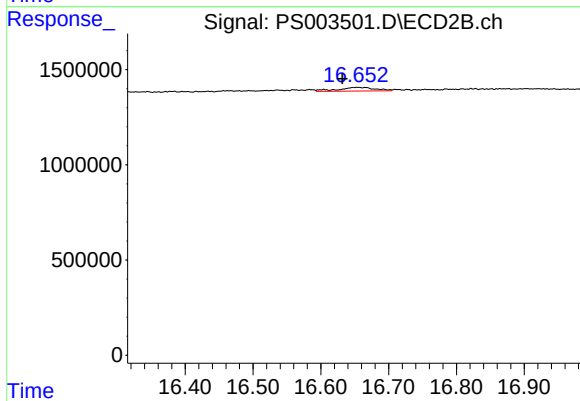

#16 DCPA

R.T.: 16.653 min
Delta R.T.: 0.021 min
Response: 735585
Conc: 0.24 ng/ml