

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031119\
 Data File : PS003504.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2019 17:10
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 01:19:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.303	10.800	219.0E6	208.0E6	498.886	442.936
Target Compounds							
3) T	4-Nitroph...	0.000	9.952	0	114852	N.D.	0.511 #
6) T	MCP	0.000	11.317	0	39477	N.D.	0.033 #
7) T	MCPA	0.000	11.688	0	496544	N.D.	0.288 #
8) T	DICHLORPROP	0.000	12.179	0	143202	N.D.	0.347 #
9) T	2,4-D	0.000	12.655	0	105619	N.D.	0.201 #
10) T	Pentachlo...	0.000	13.220	0	734646	N.D.	0.112 #
11) T	2,4,5-TP ...	0.000	13.811	0	337134	N.D.	0.132 #
12) T	2,4,5-T	0.000	14.368	0	155043	N.D.	0.077 #
13) T	2,4-DB	0.000	15.023	0	170607	N.D.	0.668 #
14) T	DINOSEB	0.000	15.500	0	227377	N.D.	0.127 #
15) T	Picloram	0.000	16.656	0	654089	N.D.	0.258 #
16) T	DCPA	0.000	16.608	0	35539	N.D.	0.011 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031119\
Data File : PS003504.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2019 17:10
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 01:19:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

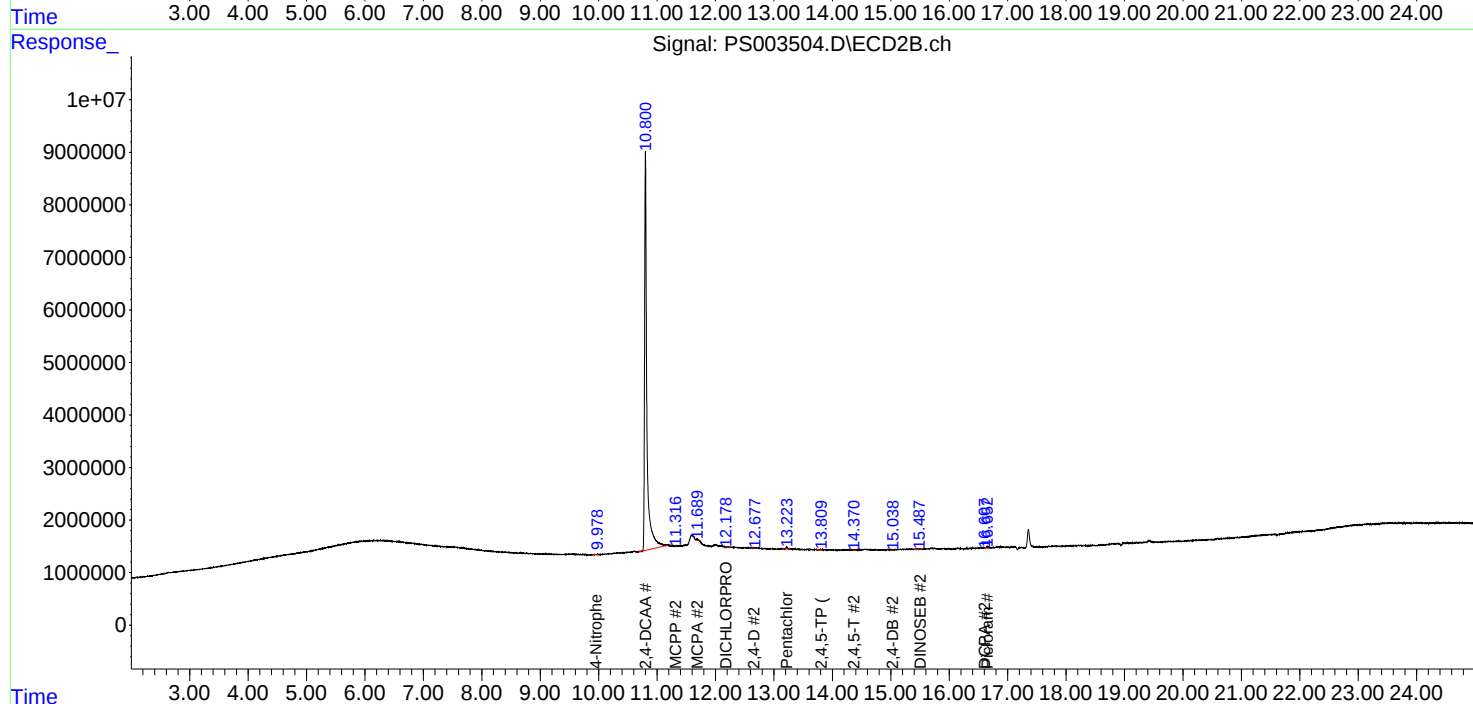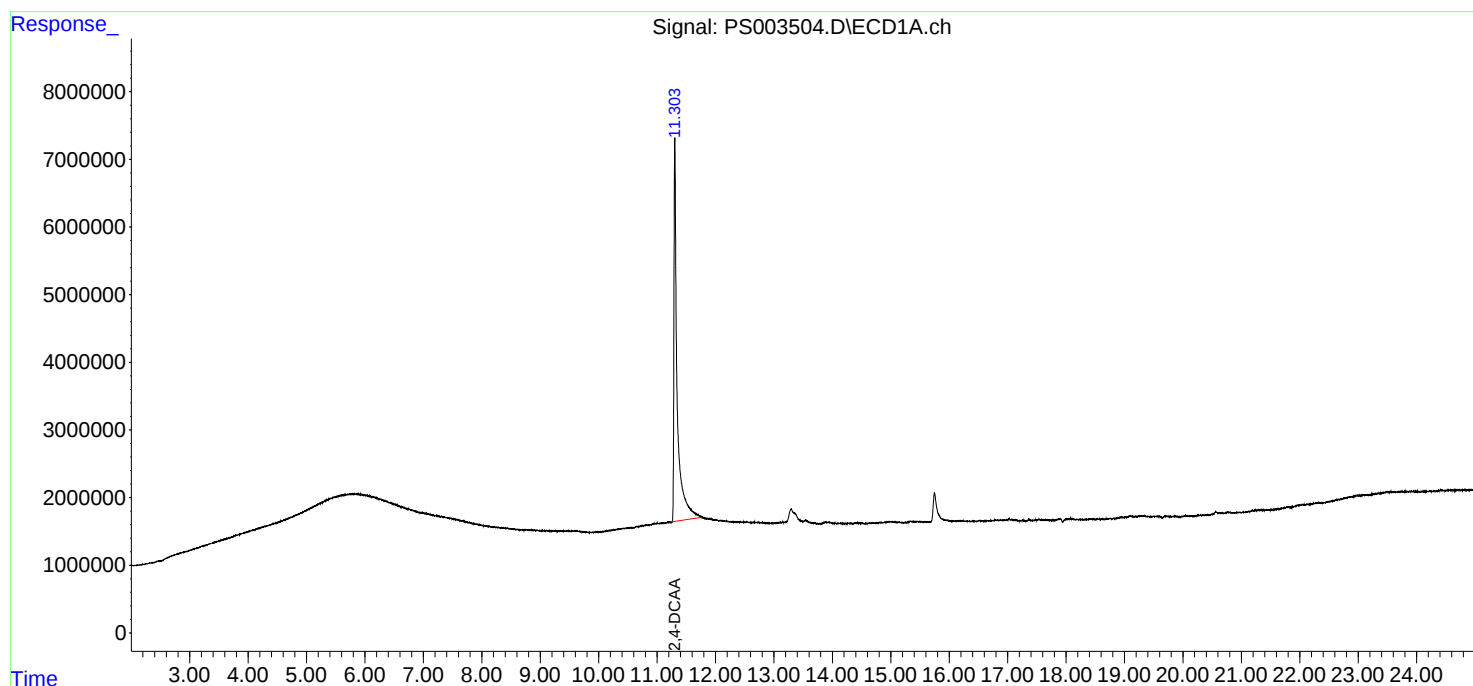


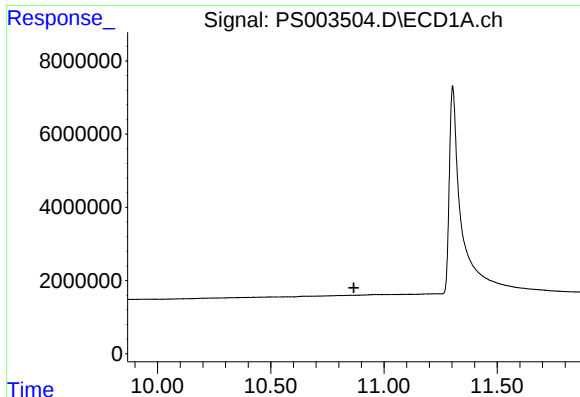

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

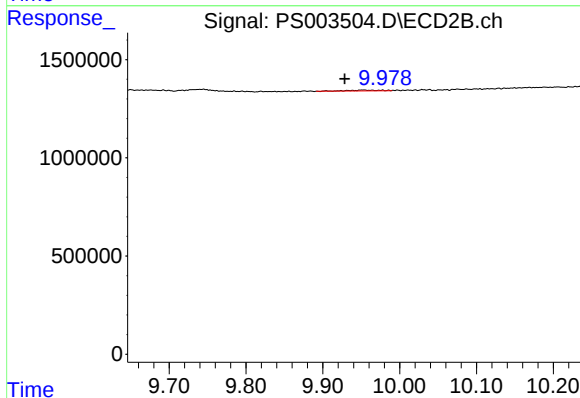


#3 4-Nitrophenol

R.T.: 9.952 min
Delta R.T.: 0.024 min
Response: 114852
Conc: 0.51 ng/ml

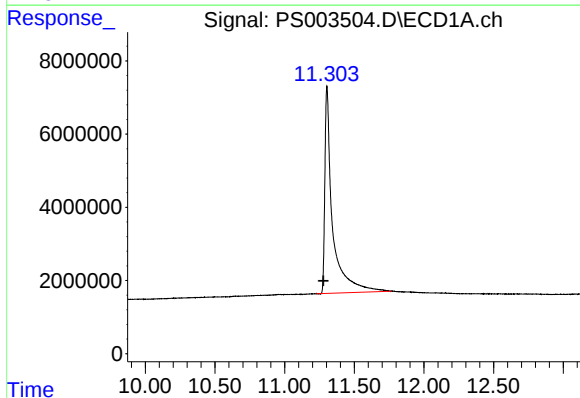


#4 2,4-DCAA

R.T.: 11.303 min
Delta R.T.: 0.026 min
Response: 219022975
Conc: 498.89 ng/ml

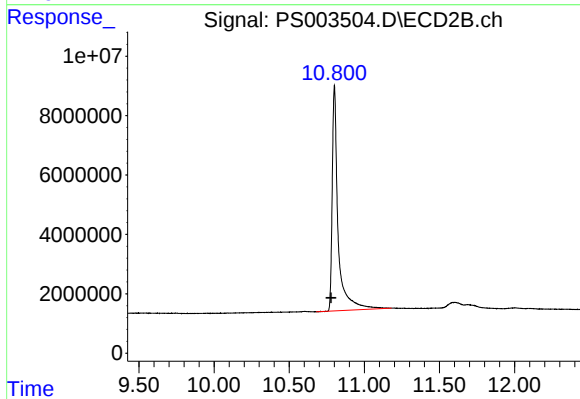

#4 2,4-DCAA


R.T.: 10.800 min
Delta R.T.: 0.021 min
Response: 207988917
Conc: 442.94 ng/ml

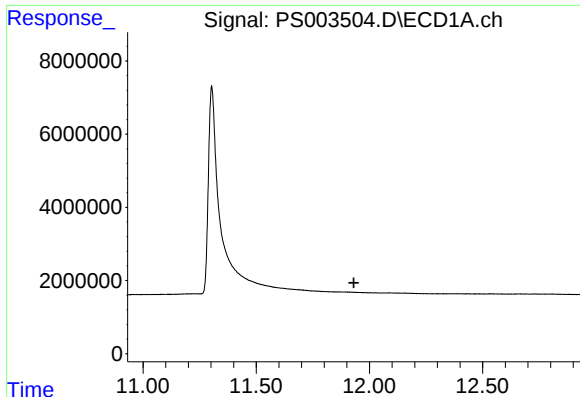

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 11.931 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

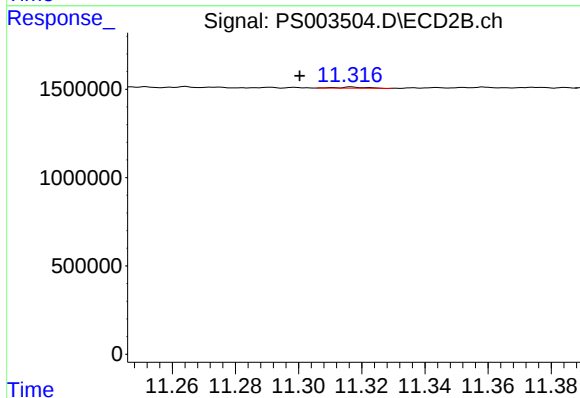


#6 MCPP

R.T.: 11.317 min
Delta R.T.: 0.017 min
Response: 39477
Conc: 0.03 ug/ml

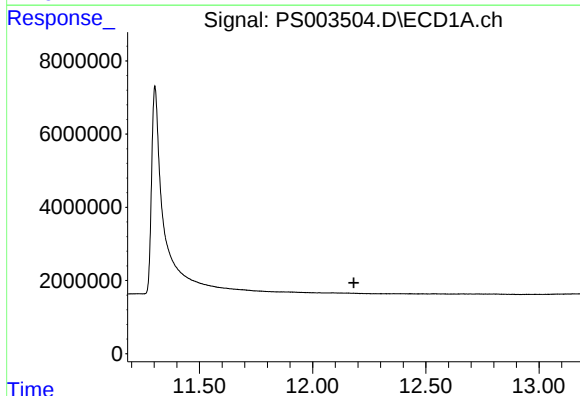


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 12.182 min
Response: 0
Conc: N.D.

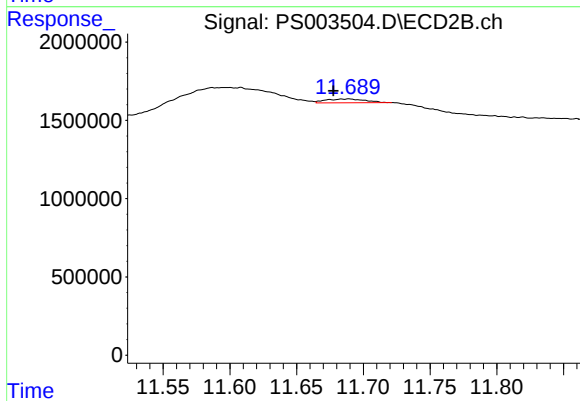

#7 MCPA


R.T.: 11.688 min
Delta R.T.: 0.010 min
Response: 496544
Conc: 0.29 ug/ml

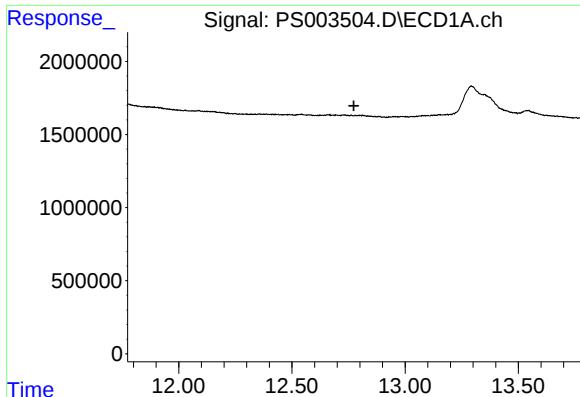

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.773 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

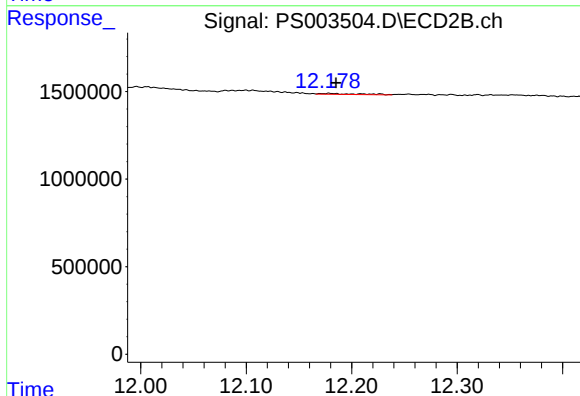


#8 DICHLORPROP

R.T.: 12.179 min
Delta R.T.: -0.006 min
Response: 143202
Conc: 0.35 ng/ml

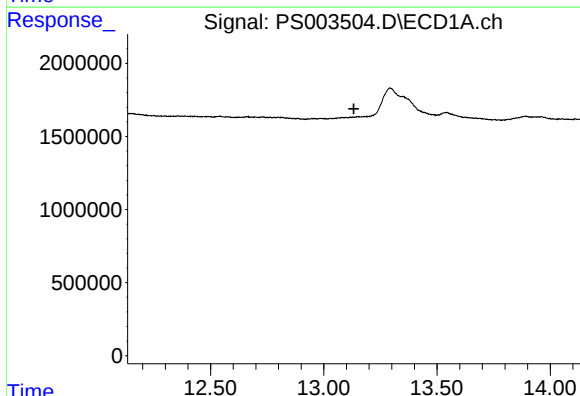


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 13.133 min
Response: 0
Conc: N.D.

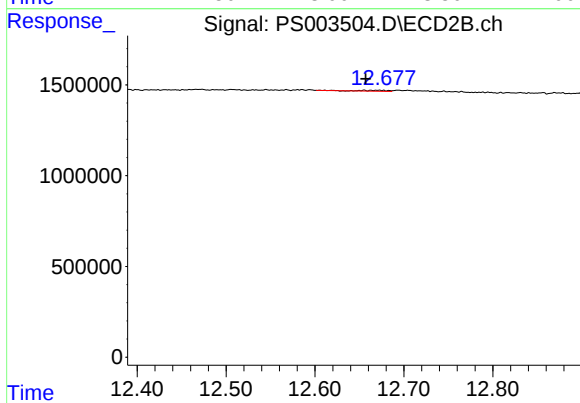

#9 2,4-D


R.T.: 12.655 min
Delta R.T.: -0.002 min
Response: 105619
Conc: 0.20 ng/ml

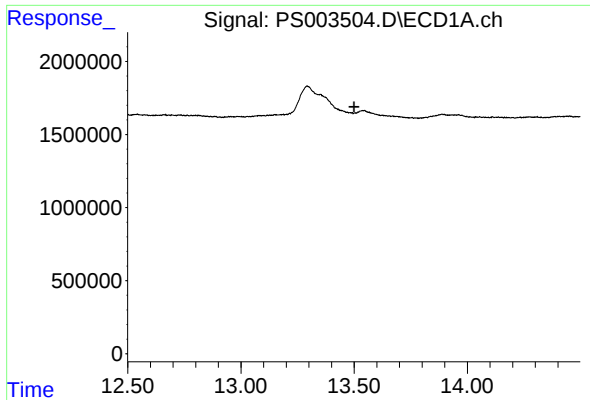

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.499 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

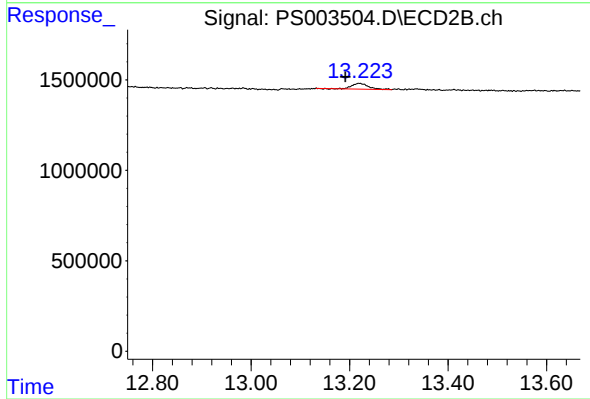


#10 Pentachlorophenol

R.T.: 13.220 min
Delta R.T.: 0.028 min
Response: 734646
Conc: 0.11 ng/ml

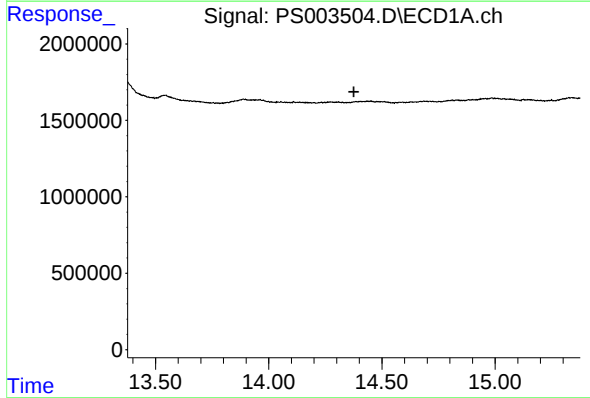


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

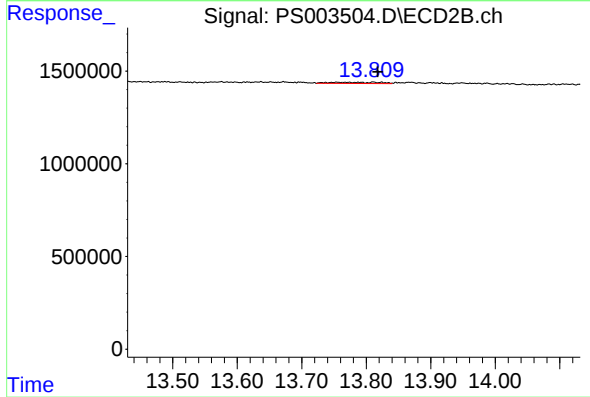

#11 2,4,5-TP (SILVEX)


R.T.: 13.811 min
Delta R.T.: -0.007 min
Response: 337134
Conc: 0.13 ng/ml

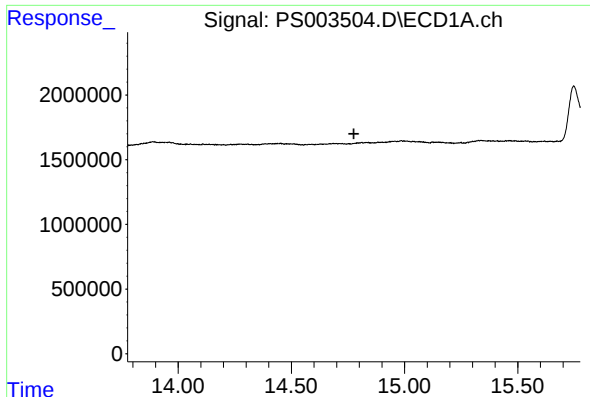

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

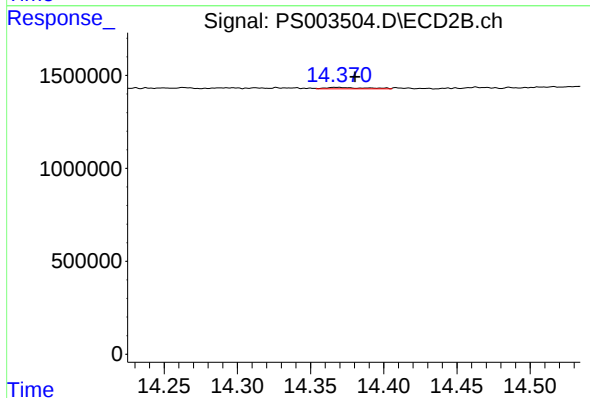


#12 2,4,5-T

R.T.: 14.368 min
Delta R.T.: -0.012 min
Response: 155043
Conc: 0.08 ng/ml

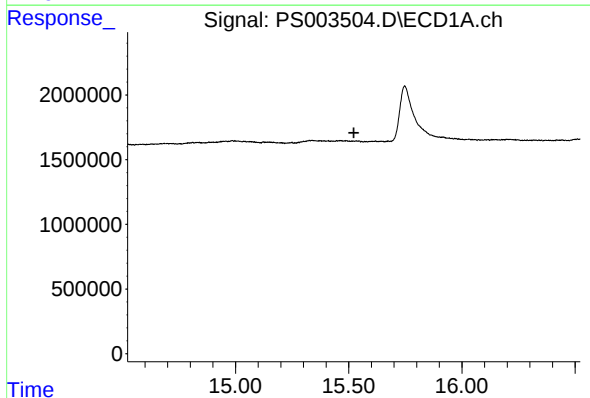


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.523 min
Response: 0
Conc: N.D.

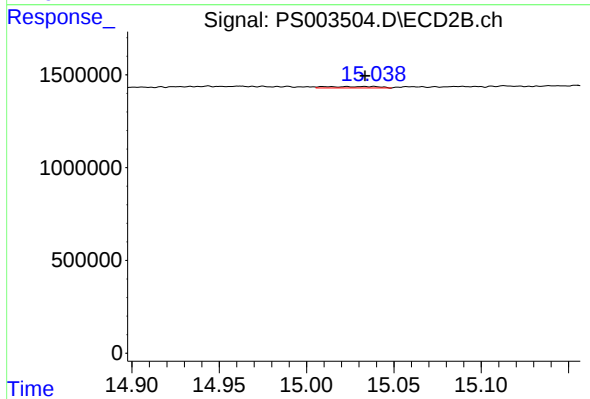

#13 2,4-DB


R.T.: 15.023 min
Delta R.T.: -0.010 min
Response: 170607
Conc: 0.67 ng/ml

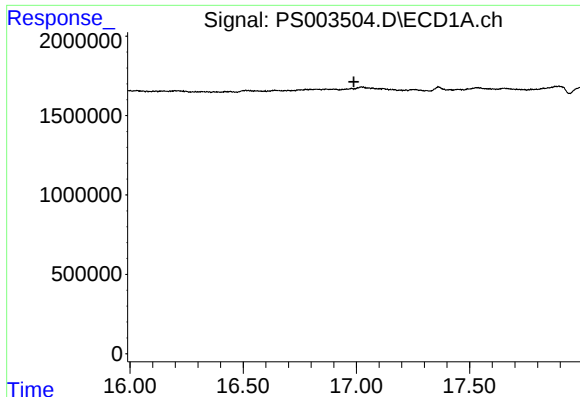

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 16.989 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

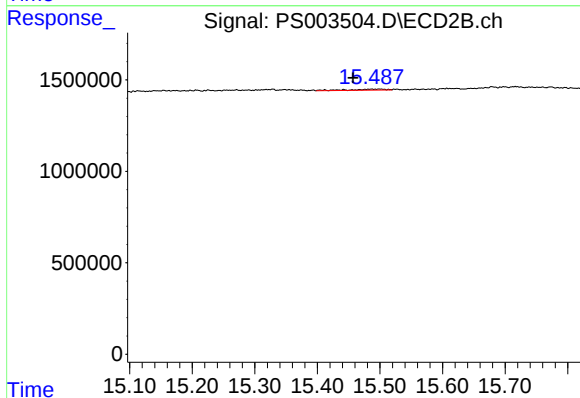


#14 DINOSEB

R.T.: 15.500 min
Delta R.T.: 0.044 min
Response: 227377
Conc: 0.13 ng/ml

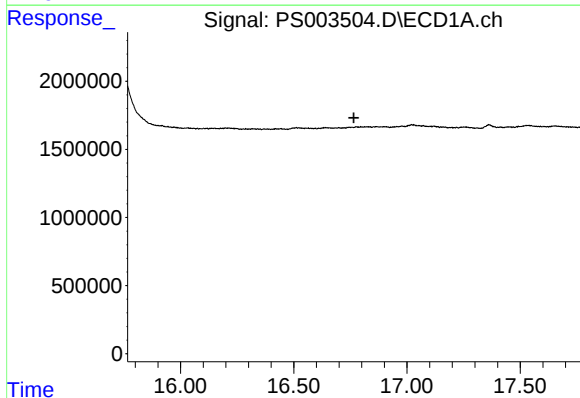


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.765 min
Response: 0
Conc: N.D.

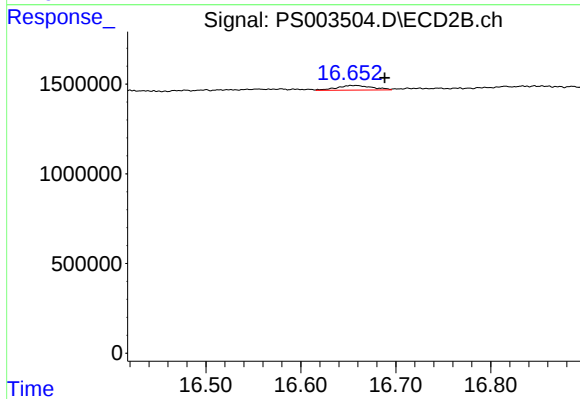

#15 Picloram


R.T.: 16.656 min
Delta R.T.: -0.032 min
Response: 654089
Conc: 0.26 ng/ml

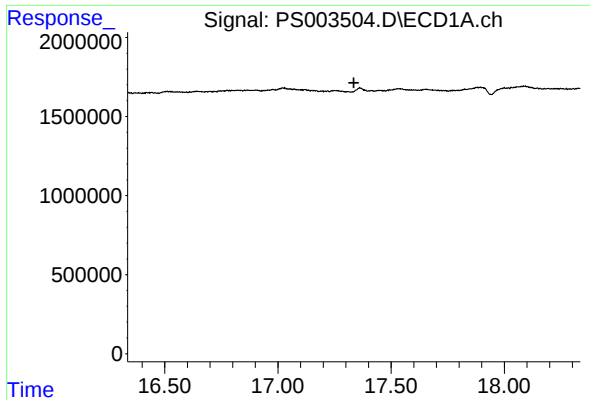

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.335 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

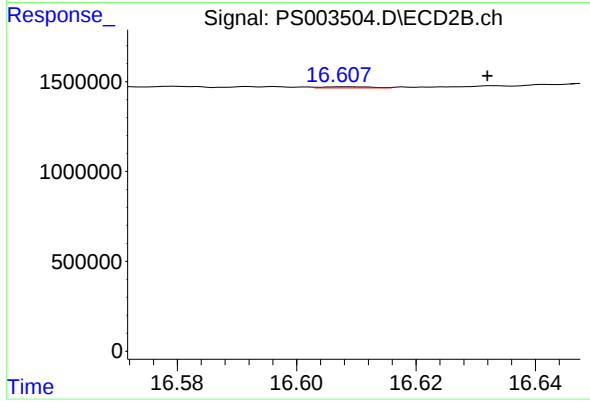

#16 DCPA

R.T.: 16.608 min
Delta R.T.: -0.024 min
Response: 35539
Conc: 0.01 ng/ml