

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031120\
 Data File : PS009200.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2020 21:30
 Operator : DD\AJ
 Sample : HSTDICC750
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 07:07:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:05:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.242	6.935	430.0E6	421.9E6	750.000	750.000
Target Compounds							
1) T	Dalapon	3.046	2.626	552.9E6	554.2E6	682.500	682.500
2) T	3,5-DICHL...	6.451	6.080	544.9E6	583.4E6	697.500	697.500
3) T	4-Nitroph...	7.071	6.536	169.0E6	224.2E6	682.500	682.500
5) T	DICAMBA	7.435	7.106	1558.7E6	1681.0E6	705.000	705.000
6) T	MCPD	7.606	7.204	177.3E6	133.9E6	70.500	70.500
7) T	MCPA	7.756	7.420	222.0E6	196.4E6	69.750	69.750
8) T	DICHLORPROP	8.129	7.733	377.9E6	401.4E6	705.000	705.000
9) T	2,4-D	8.358	8.027	386.6E6	477.1E6	705.000	705.000
10) T	Pentachlo...	8.672	8.461	5148.6E6	5551.6E6	712.500	712.500
11) T	2,4,5-TP ...	9.221	8.822	2034.2E6	2194.7E6	712.500	712.500
12) T	2,4,5-T	9.505	9.201	1884.2E6	2175.5E6	712.500	712.500
13) T	2,4-DB	10.059	9.708	257.2E6	277.7E6	712.500	712.500
14) T	DINOSEB	11.225	10.044	1498.7E6	1604.6E6	705.000	705.000
15) T	Picloram	11.037	11.023	2305.1E6	3081.7E6	712.500	712.500
16) T	DCPA	11.489	10.974	2588.6E6	2870.6E6	720.000	720.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031120\
Data File : PS009200.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2020 21:30
Operator : DD\AJ
Sample : HSTDICC750
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 07:07:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:05:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

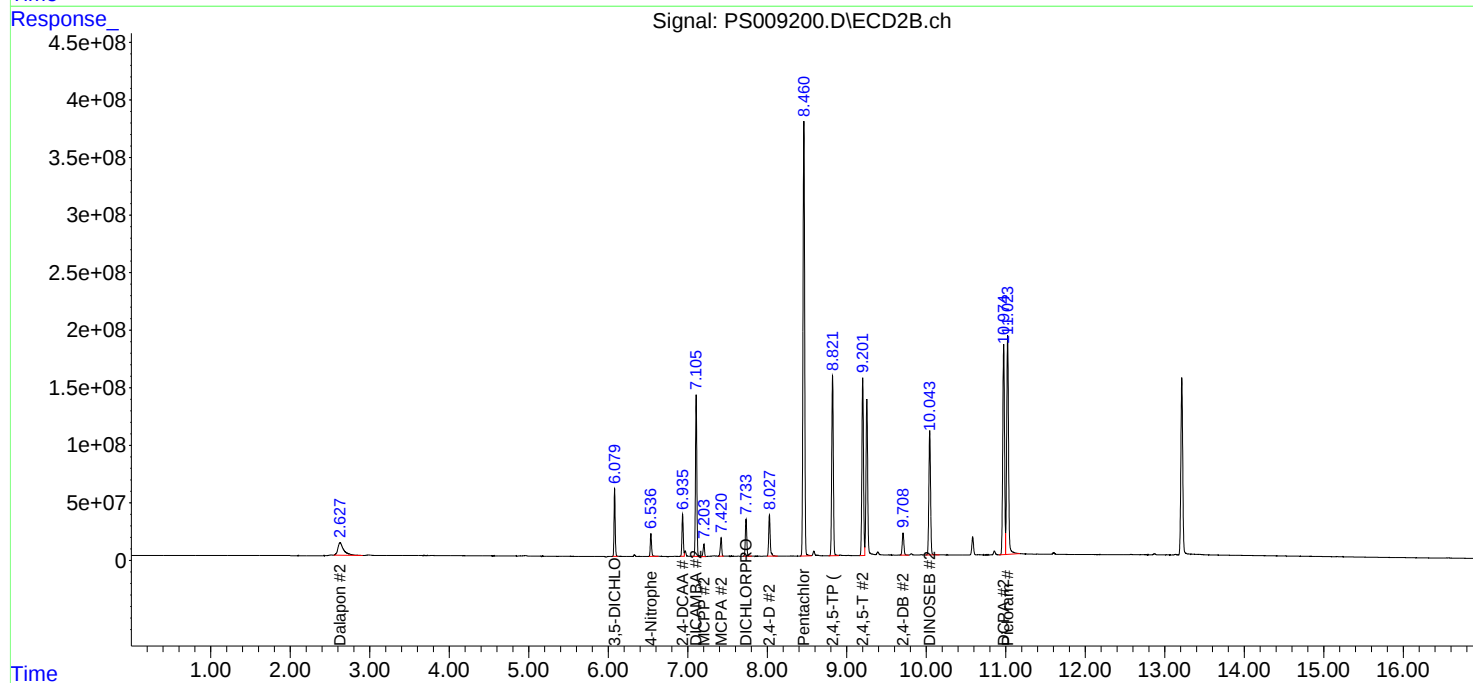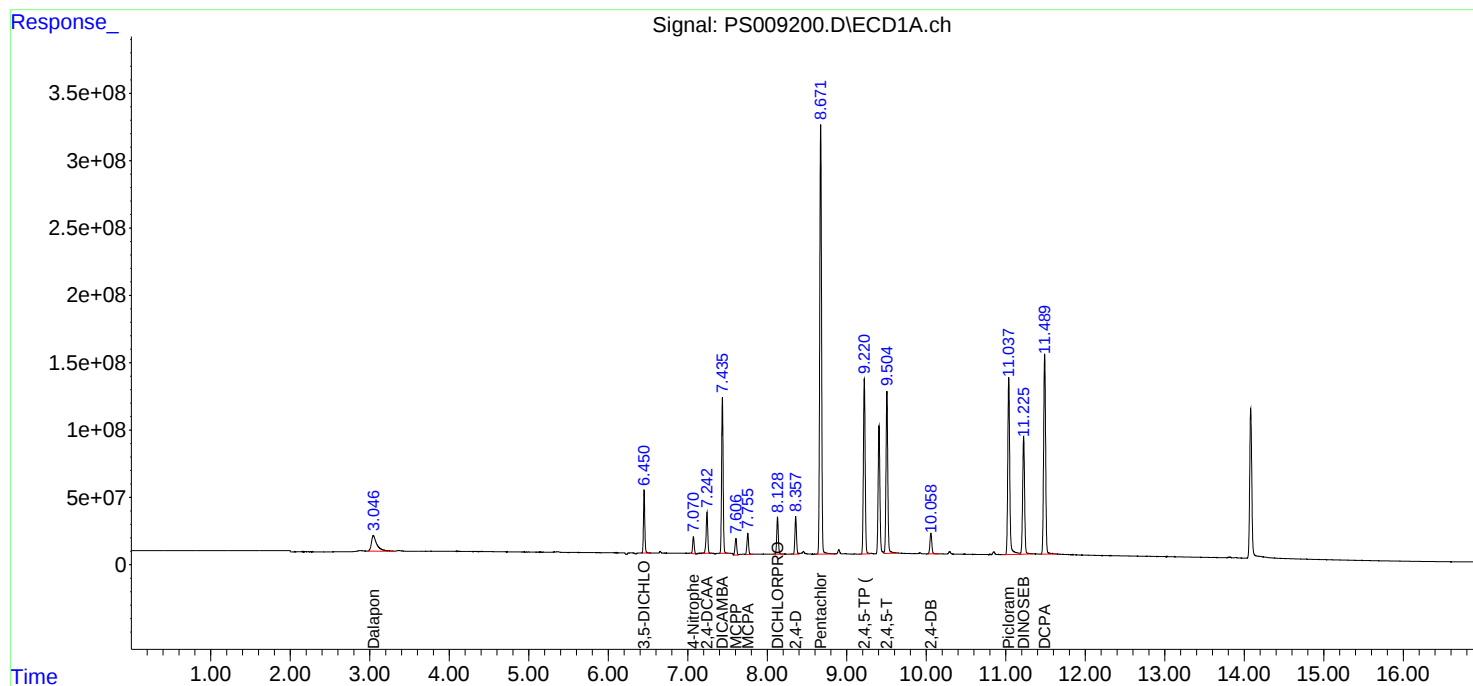


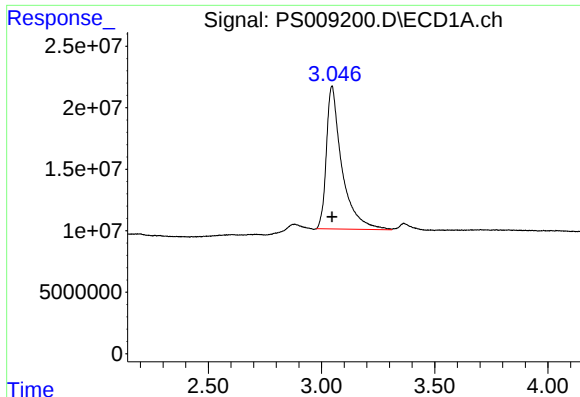

#1 Dalapon


R.T.: 3.046 min
Delta R.T.: 0.000 min
Response: 552854065
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

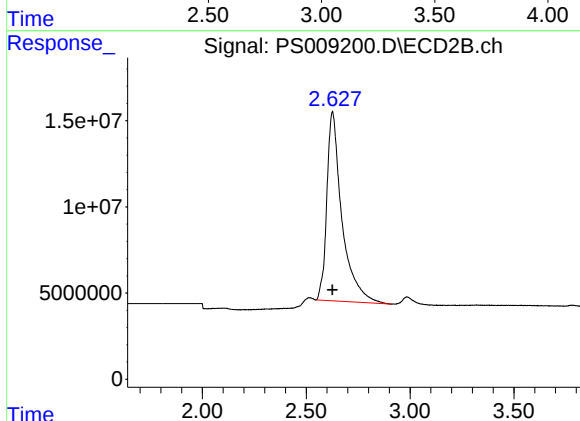


#1 Dalapon

R.T.: 2.626 min
Delta R.T.: 0.000 min
Response: 554186138
Conc: 682.50 ng/ml

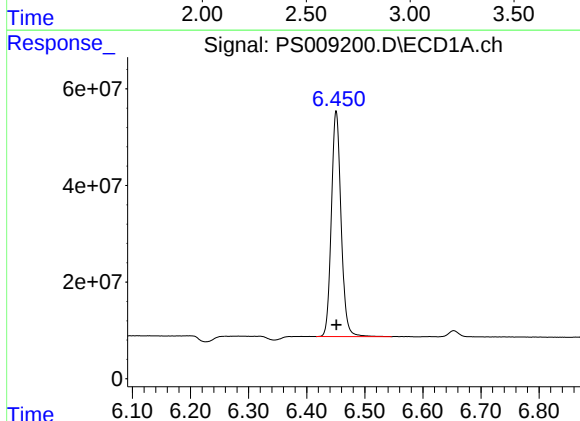


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.451 min
Delta R.T.: 0.000 min
Response: 544924451
Conc: 697.50 ng/ml

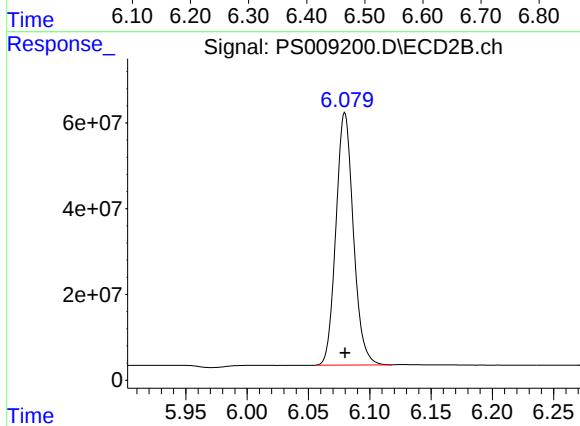

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.080 min
Delta R.T.: 0.000 min
Response: 583445717
Conc: 697.50 ng/ml

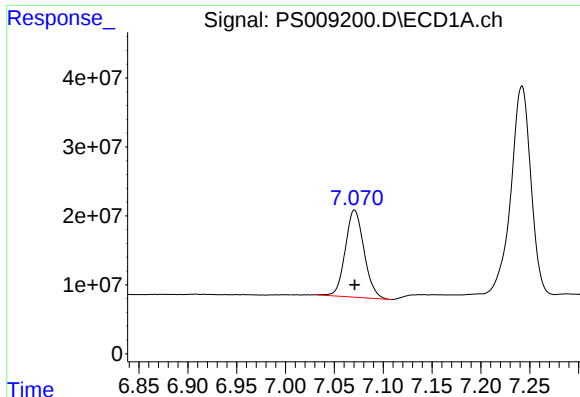

#3 4-Nitrophenol


R.T.: 7.071 min
Delta R.T.: 0.000 min
Response: 169042767
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

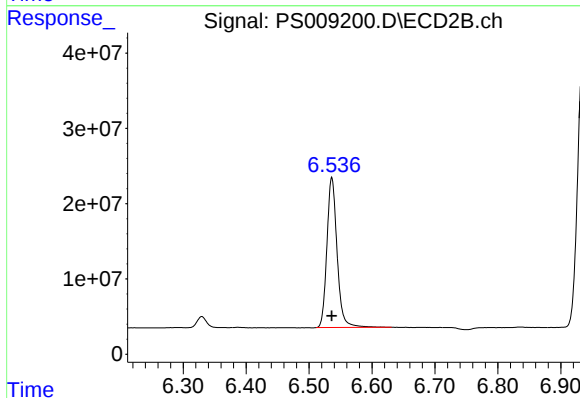


#3 4-Nitrophenol

R.T.: 6.536 min
Delta R.T.: 0.000 min
Response: 224209165
Conc: 682.50 ng/ml

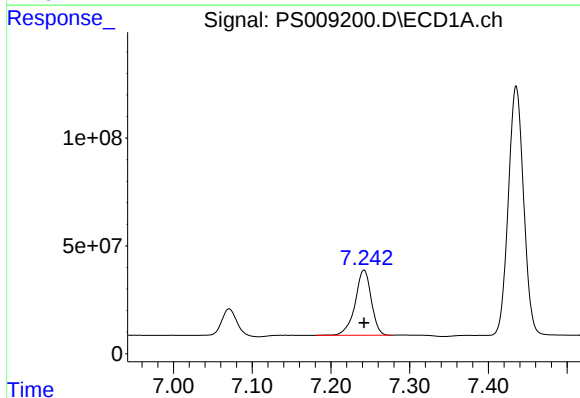


#4 2,4-DCAA

R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 429954808
Conc: 750.00 ng/ml

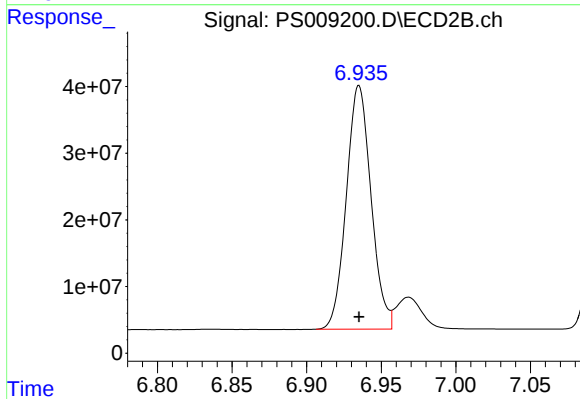

#4 2,4-DCAA


R.T.: 6.935 min
Delta R.T.: 0.000 min
Response: 421937263
Conc: 750.00 ng/ml

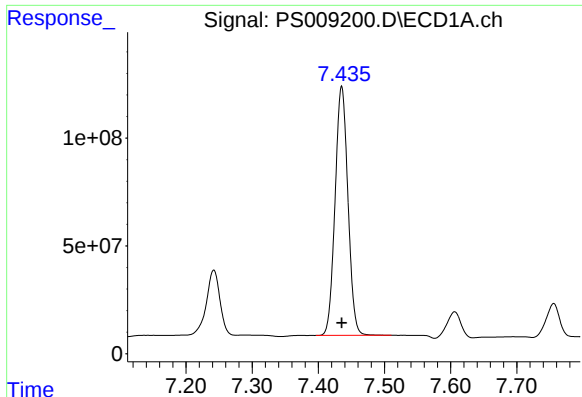

#5 DICAMBA


R.T.: 7.435 min
Delta R.T.: 0.000 min
Response: 1558678622
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

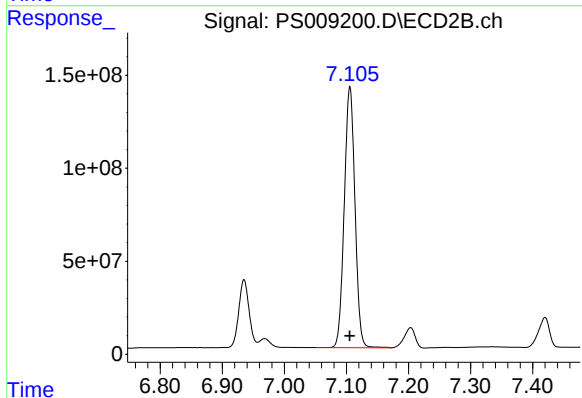


#5 DICAMBA

R.T.: 7.106 min
Delta R.T.: 0.000 min
Response: 1681019029
Conc: 705.00 ng/ml

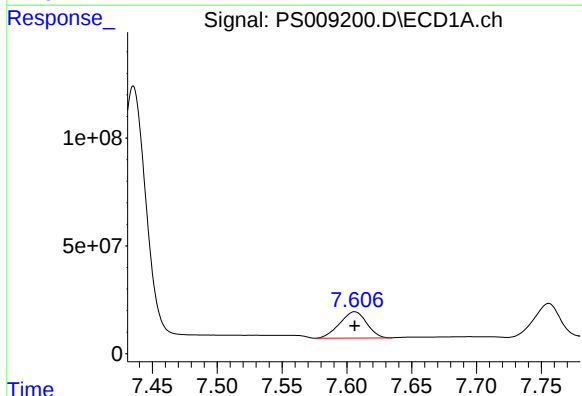


#6 MCP

R.T.: 7.606 min
Delta R.T.: 0.000 min
Response: 177256951
Conc: 70.50 ug/ml

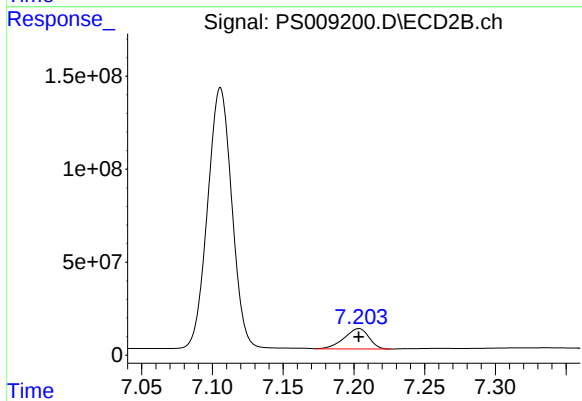

#6 MCP


R.T.: 7.204 min
Delta R.T.: 0.000 min
Response: 133947939
Conc: 70.50 ug/ml

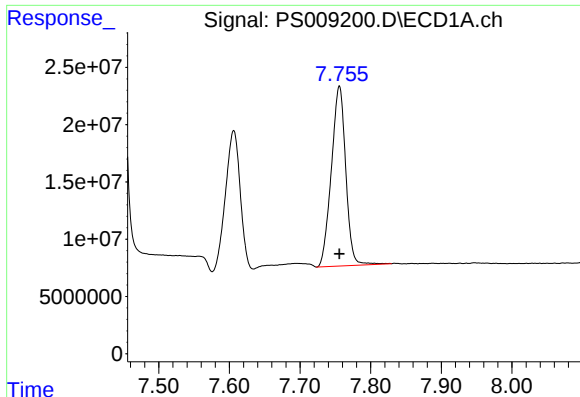

#7 MCPA


R.T.: 7.756 min
Delta R.T.: 0.000 min
Response: 222045789
Conc: 69.75 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

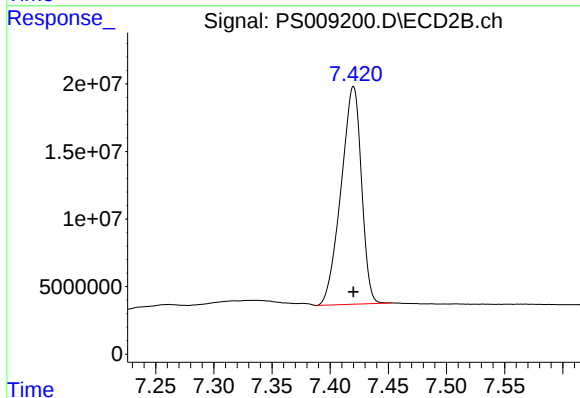


#7 MCPA

R.T.: 7.420 min
Delta R.T.: 0.000 min
Response: 196439210
Conc: 69.75 ug/ml

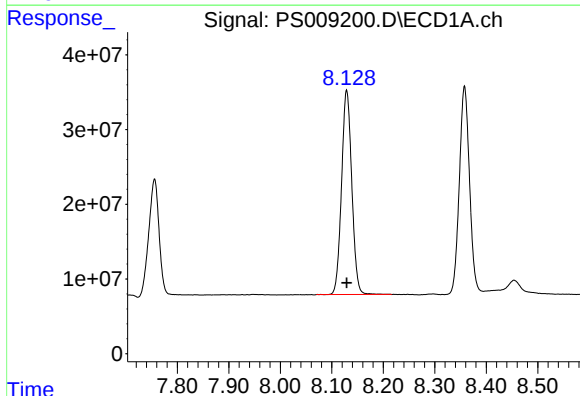


#8 DICHLORPROP

R.T.: 8.129 min
Delta R.T.: 0.000 min
Response: 377940204
Conc: 705.00 ng/ml

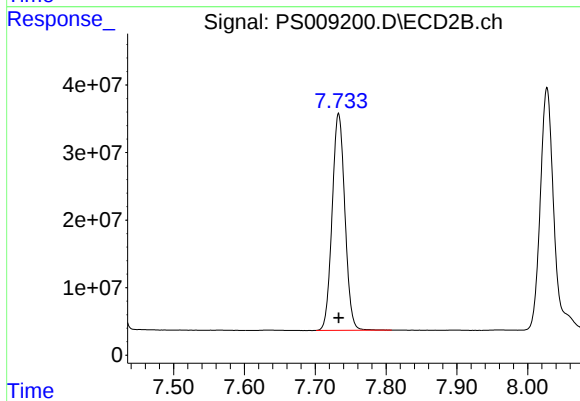

#8 DICHLORPROP


R.T.: 7.733 min
Delta R.T.: 0.000 min
Response: 401392838
Conc: 705.00 ng/ml

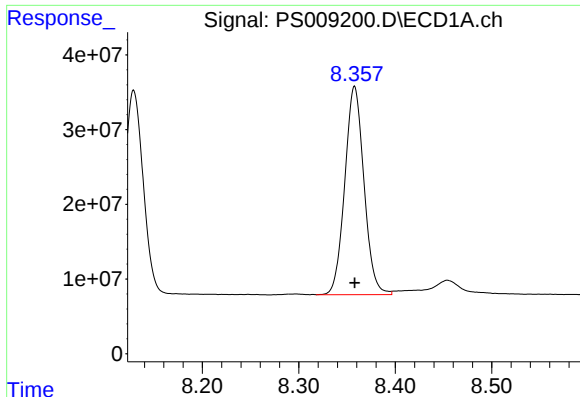

#9 2,4-D


R.T.: 8.358 min
Delta R.T.: 0.000 min
Response: 386648701
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

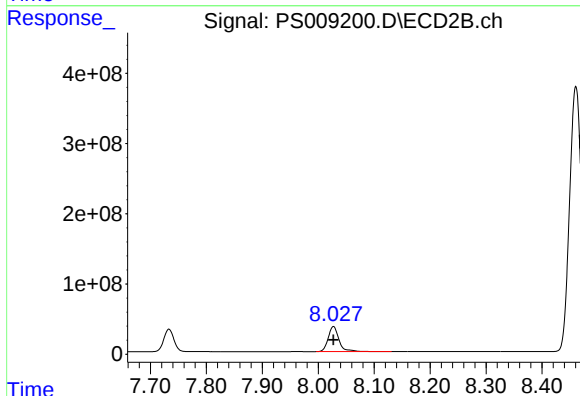


#9 2,4-D

R.T.: 8.027 min
Delta R.T.: 0.000 min
Response: 477110740
Conc: 705.00 ng/ml

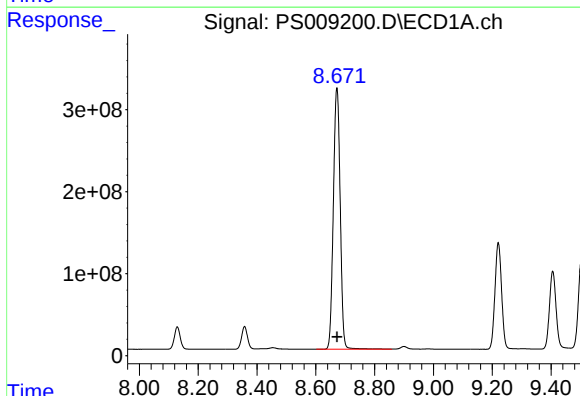


#10 Pentachlorophenol

R.T.: 8.672 min
Delta R.T.: 0.000 min
Response: 5148613159
Conc: 712.50 ng/ml

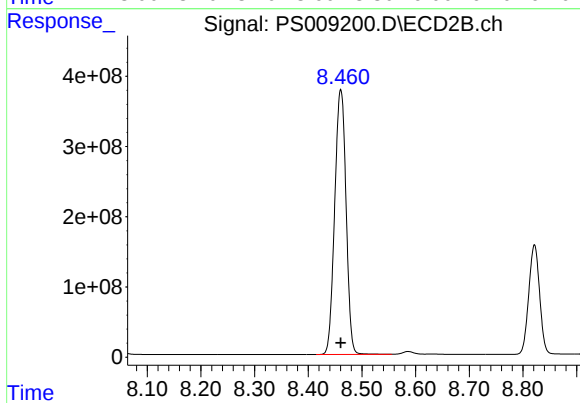

#10 Pentachlorophenol


R.T.: 8.461 min
Delta R.T.: 0.000 min
Response: 5551590547
Conc: 712.50 ng/ml

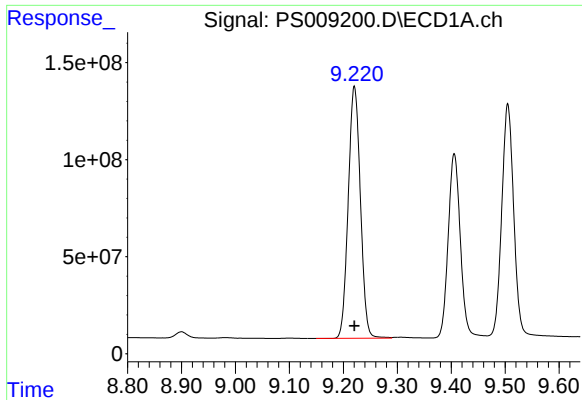

#11 2,4,5-TP (SILVEX)


R.T.: 9.221 min
Delta R.T.: 0.000 min
Response: 2034173912
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

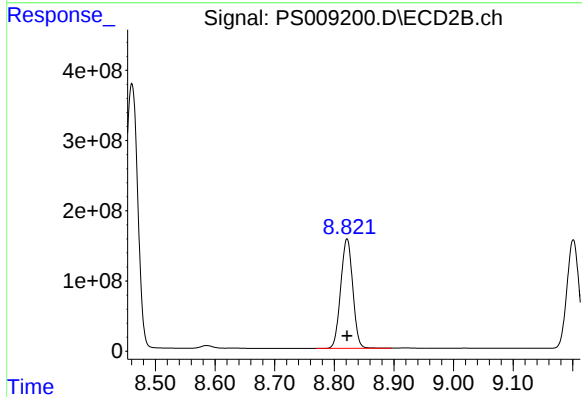


#11 2,4,5-TP (SILVEX)

R.T.: 8.822 min
Delta R.T.: 0.000 min
Response: 2194726146
Conc: 712.50 ng/ml

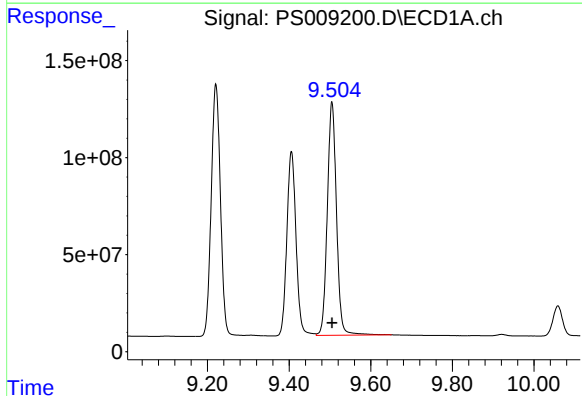


#12 2,4,5-T

R.T.: 9.505 min
Delta R.T.: 0.000 min
Response: 1884217982
Conc: 712.50 ng/ml

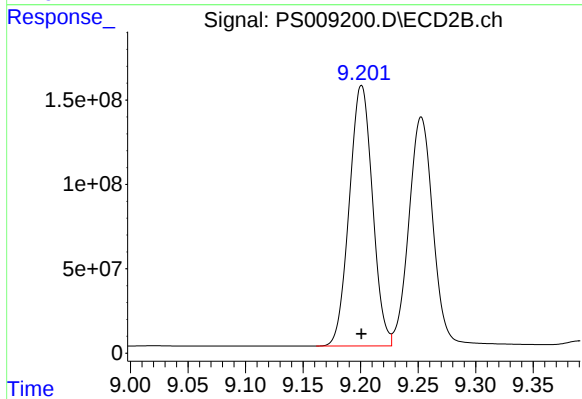

#12 2,4,5-T


R.T.: 9.201 min
Delta R.T.: 0.000 min
Response: 2175547729
Conc: 712.50 ng/ml

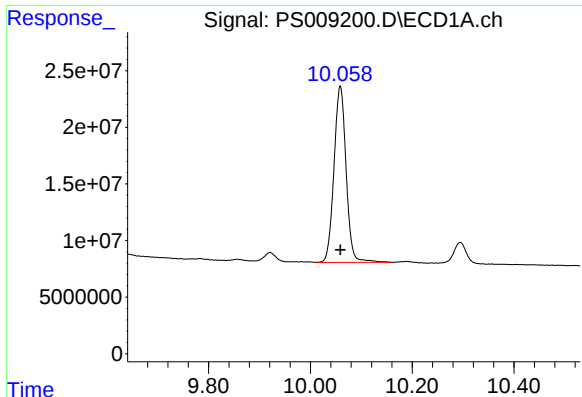

#13 2,4-DB


R.T.: 10.059 min
Delta R.T.: 0.000 min
Response: 257204179
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

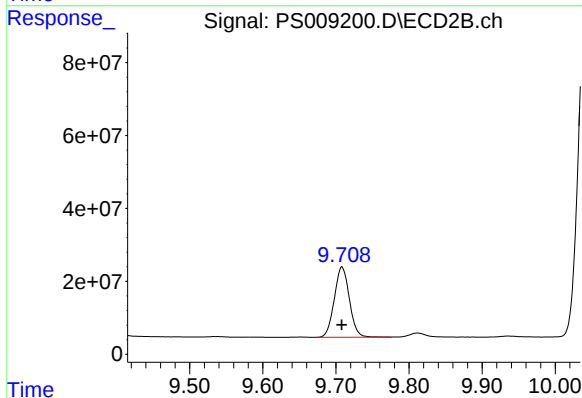


#13 2,4-DB

R.T.: 9.708 min
Delta R.T.: 0.000 min
Response: 277669737
Conc: 712.50 ng/ml

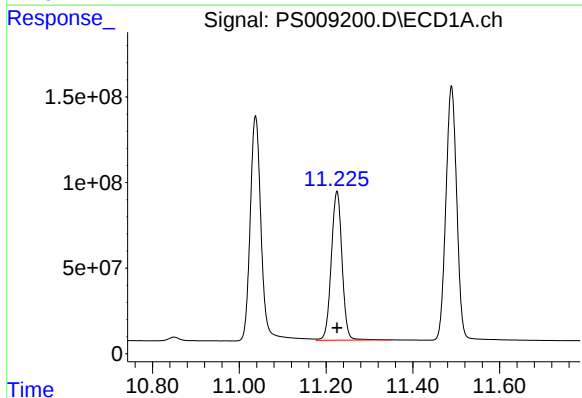


#14 DINOSEB

R.T.: 11.225 min
Delta R.T.: 0.000 min
Response: 1498658214
Conc: 705.00 ng/ml

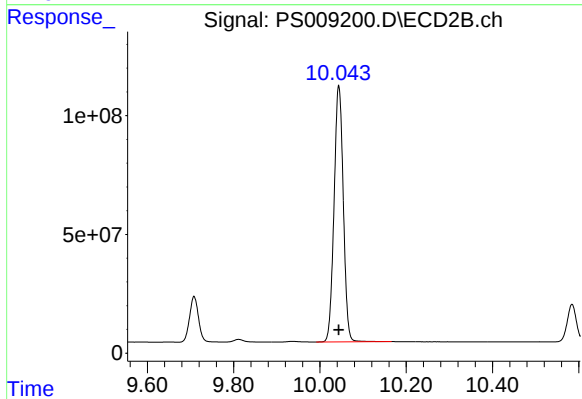

#14 DINOSEB


R.T.: 10.044 min
Delta R.T.: 0.000 min
Response: 1604571300
Conc: 705.00 ng/ml

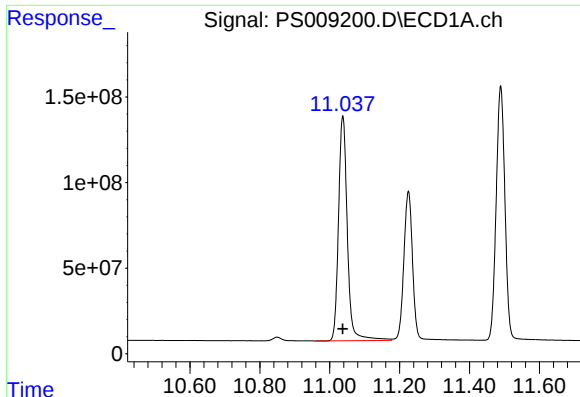

#15 Picloram


R.T.: 11.037 min
Delta R.T.: 0.000 min
Response: 2305064119
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

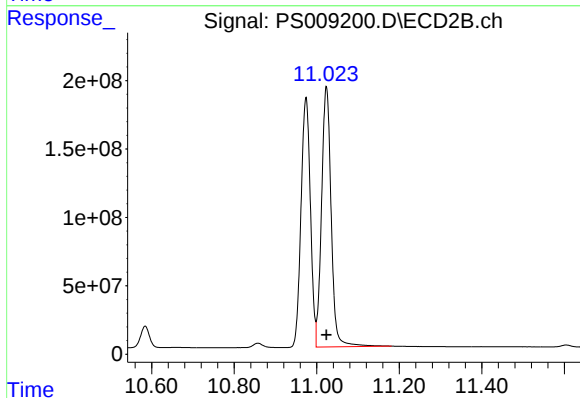


#15 Picloram

R.T.: 11.023 min
Delta R.T.: 0.000 min
Response: 3081676693
Conc: 712.50 ng/ml

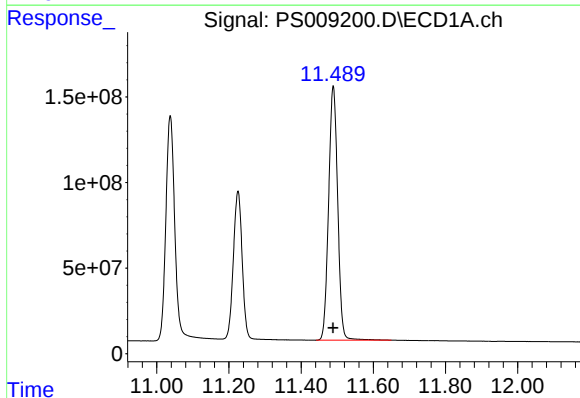

#16 DCPA

R.T.: 11.489 min
Delta R.T.: 0.000 min
Response: 2588564729
Conc: 720.00 ng/ml

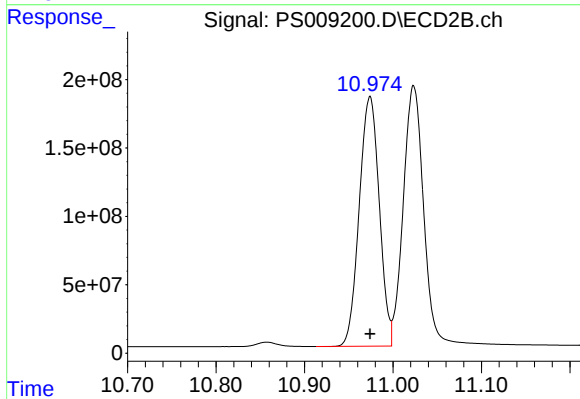

#16 DCPA

R.T.: 10.974 min
Delta R.T.: 0.000 min
Response: 2870627814
Conc: 720.00 ng/ml