

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031125\
 Data File : PS029371.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 14:03
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 04:35:13 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022125.M
 Quant Title : 8080.M
 QLast Update : Sat Feb 22 01:02:20 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.159	7.623	2049.2E6	447.5E6	497.315	475.879
Target Compounds							
1) T	Dalapon	2.647f	2.676	9331368	11728958	1.690	5.540 #
2) T	3,5-DICHL...	6.348	0.000	2660702	0	<MDL	N.D. #
3) T	4-Nitroph...	6.953	0.000	15177058	0	6.485	N.D. #
7) T	MCPA	7.702f	0.000	958240	0	<MDL	N.D. #
8) T	DICHLORPROP	8.040	0.000	752195	0	<MDL	N.D. #
9) T	2,4-D	8.233f	0.000	217385	0	<MDL	N.D. #
10) T	Pentachlo...	8.561	0.000	4733640	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.115	0.000	7537496	0	<MDL	N.D. #
12) T	2,4,5-T	9.431	0.000	1227818	0	<MDL	N.D. #
13) T	2,4-DB	10.003	0.000	426785	0	<MDL	N.D. #
14) T	DINOSEB	11.194	0.000	1286187	0	<MDL	N.D. #
15) T	Picloram	11.004	0.000	139624	0	<MDL	N.D. #
16) T	DCPA	11.482	0.000	3539546	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031125\
Data File : PS029371.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 14:03
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 04:35:13 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022125.M
Quant Title : 8080.M
QLast Update : Sat Feb 22 01:02:20 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

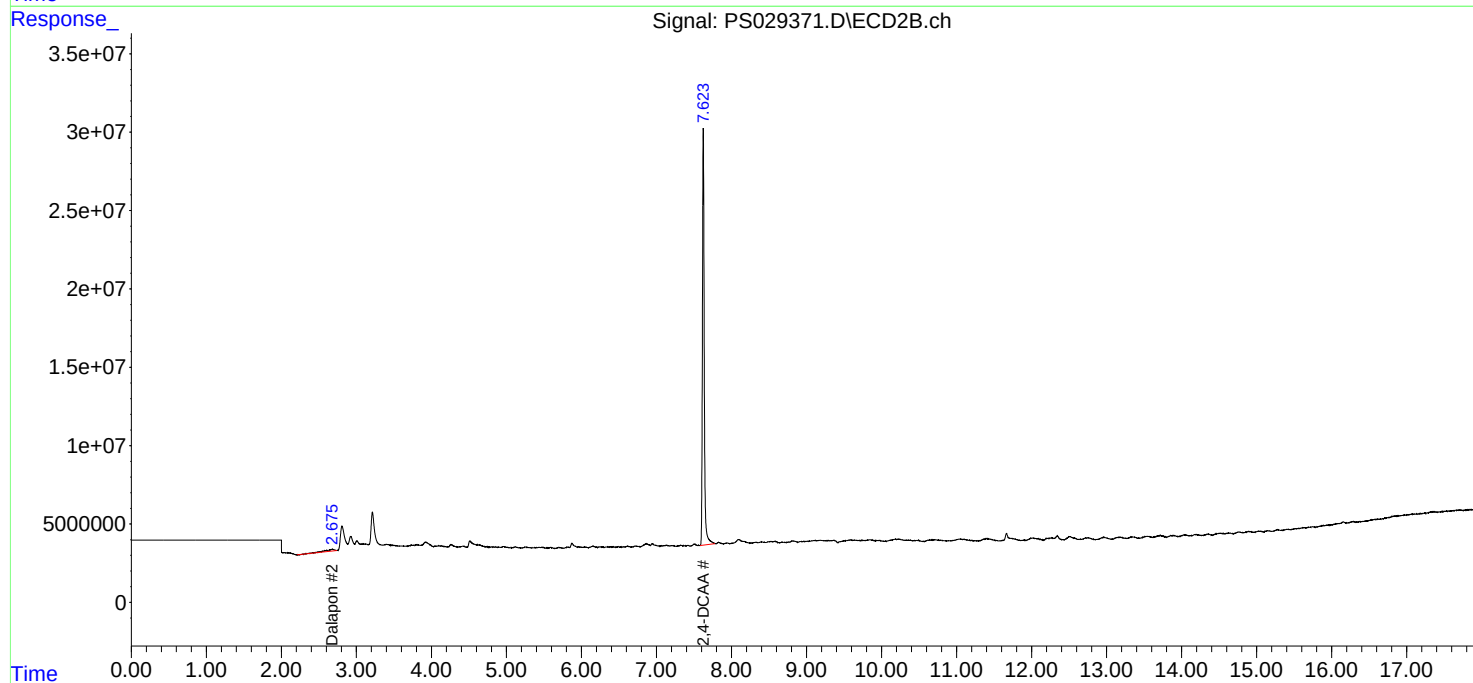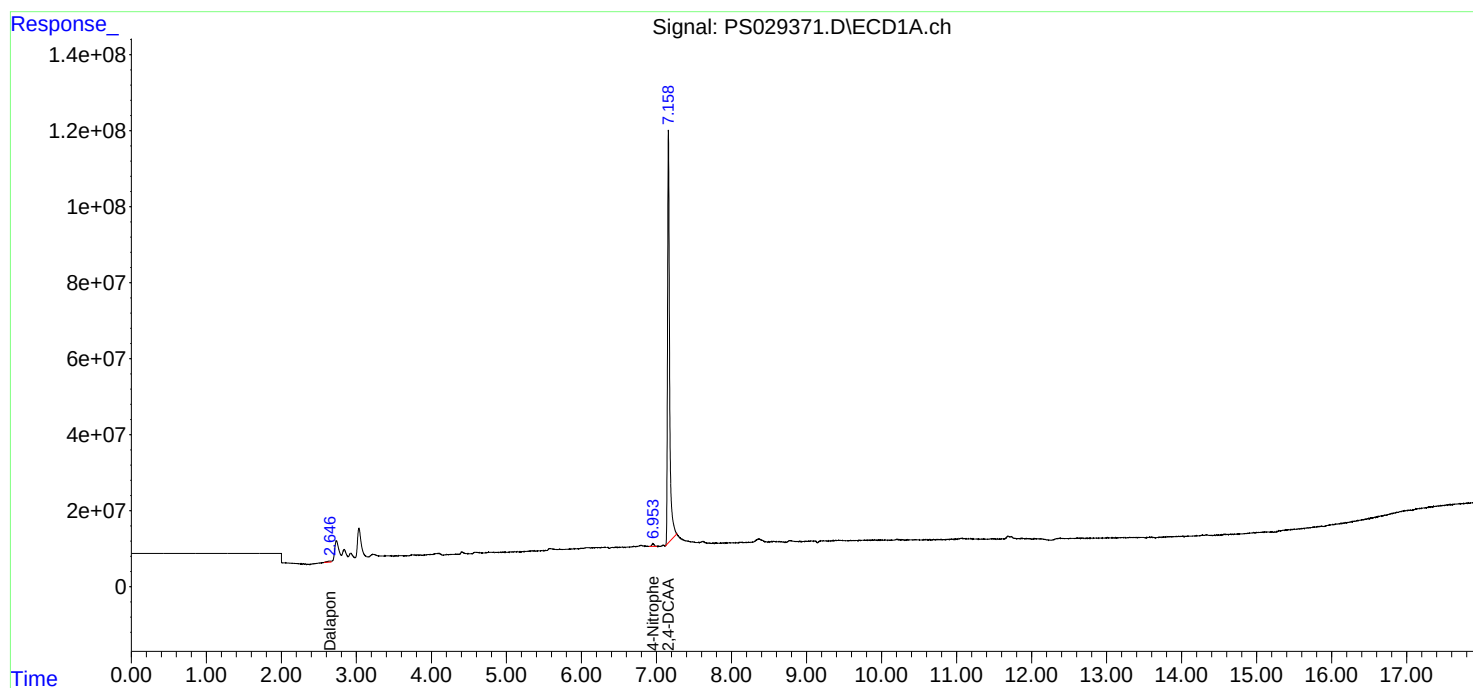


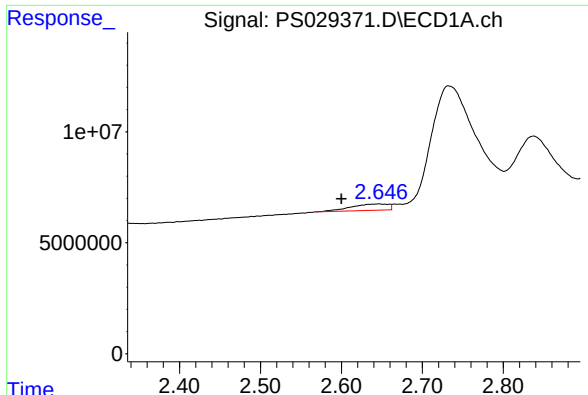

#1 Dalapon


R.T.: 2.647 min
Delta R.T.: 0.047 min
Response: 9331368
Conc: 1.69 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

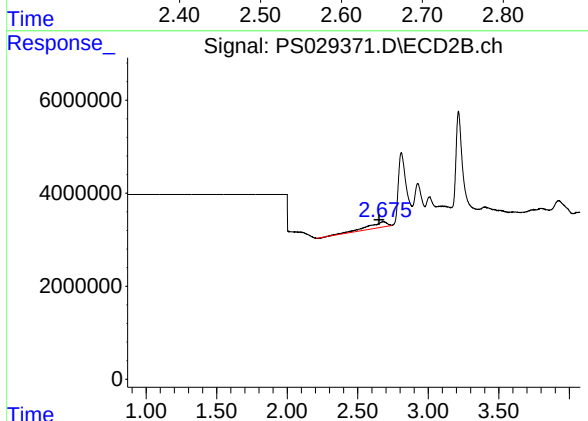


#1 Dalapon

R.T.: 2.676 min
Delta R.T.: 0.025 min
Response: 11728958
Conc: 5.54 ng/ml

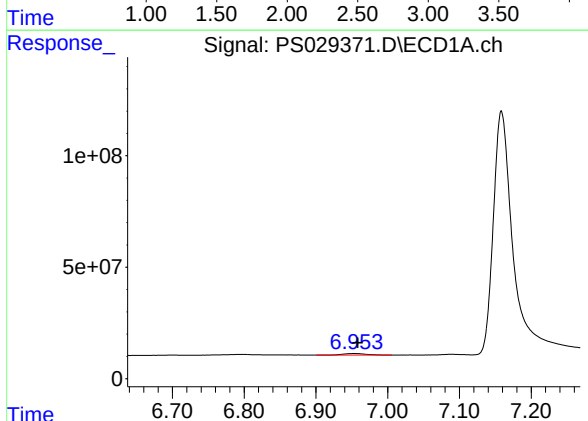


#3 4-Nitrophenol

R.T.: 6.953 min
Delta R.T.: -0.005 min
Response: 15177058
Conc: 6.49 ng/ml

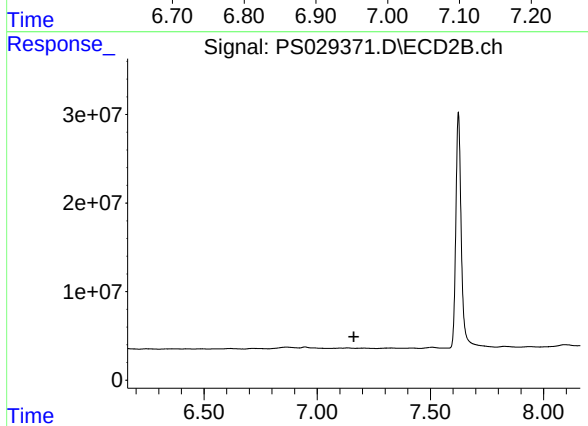

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.162 min
Response: 0
Conc: N.D.

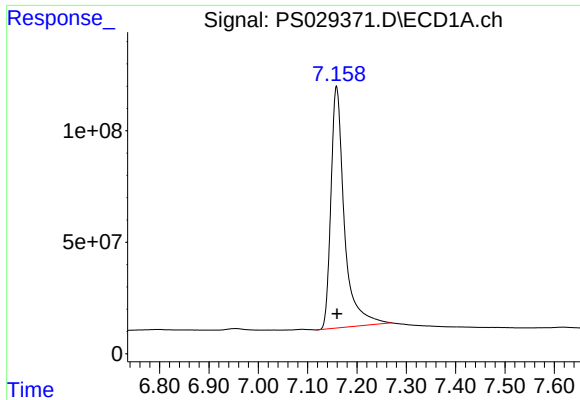

#4 2,4-DCAA

R.T.: 7.159 min
Delta R.T.: -0.001 min
Response: 2049224229
Conc: 497.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

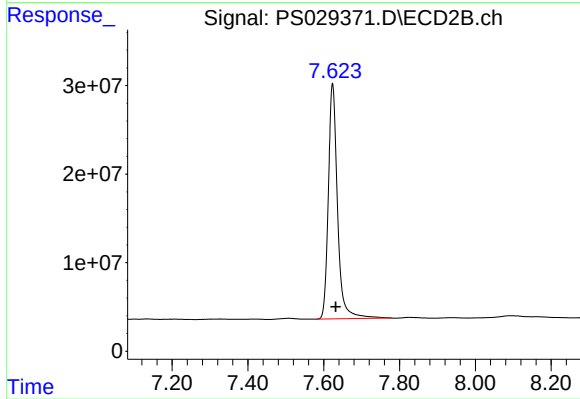

#4 2,4-DCAA

R.T.: 7.623 min
Delta R.T.: -0.008 min
Response: 447484940
Conc: 475.88 ng/ml