

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031125\
 Data File : PS029381.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 20:43
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 04:37:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022125.M
 Quant Title : 8080.M
 QLast Update : Sat Feb 22 01:02:20 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.158	7.623	2053.0E6	450.8E6	498.229	479.360
Target Compounds							
1) T	Dalapon	0.000	2.677f	0	9888470	N.D.	4.671
2) T	3,5-DICHL...	6.346	0.000	4266714	0	<MDL	N.D. #
3) T	4-Nitroph...	6.957	0.000	7814687	0	3.339	N.D. #
8) T	DICHLORPROP	8.033	8.583f	1296396	8332203	<MDL	6.516 #
10) T	Pentachlo...	8.562	9.366	6539042	19816087	<MDL	<MDL #
11) T	2,4,5-TP ...	9.116	0.000	9190152	0	<MDL	N.D. #
12) T	2,4,5-T	9.406	0.000	1468210	0	<MDL	N.D. #
13) T	2,4-DB	10.008	0.000	534258	0	<MDL	N.D. #
14) T	DINOSEB	11.200	0.000	1364470	0	<MDL	N.D. #
15) T	Picloram	11.000	0.000	1705622	0	<MDL	N.D. #
16) T	DCPA	11.485	0.000	3939028	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031125\
Data File : PS029381.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 20:43
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 04:37:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022125.M
Quant Title : 8080.M
QLast Update : Sat Feb 22 01:02:20 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

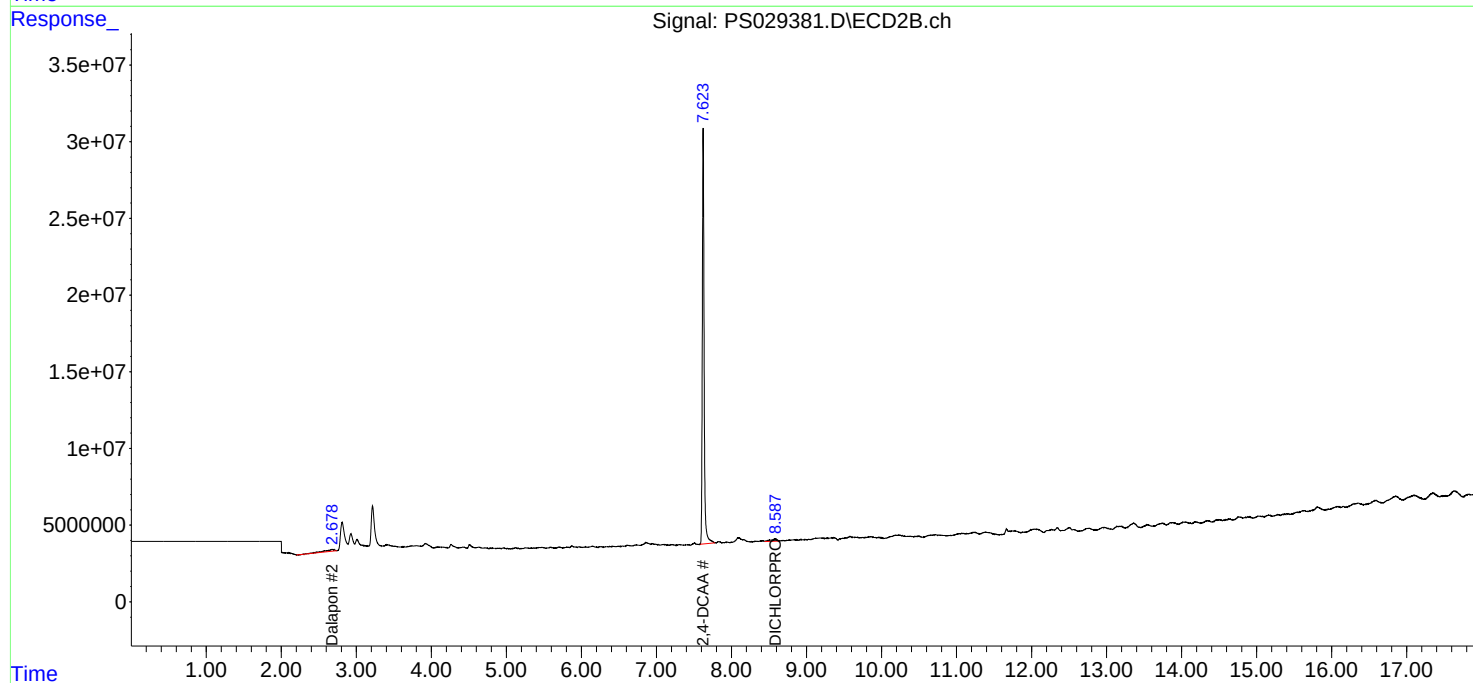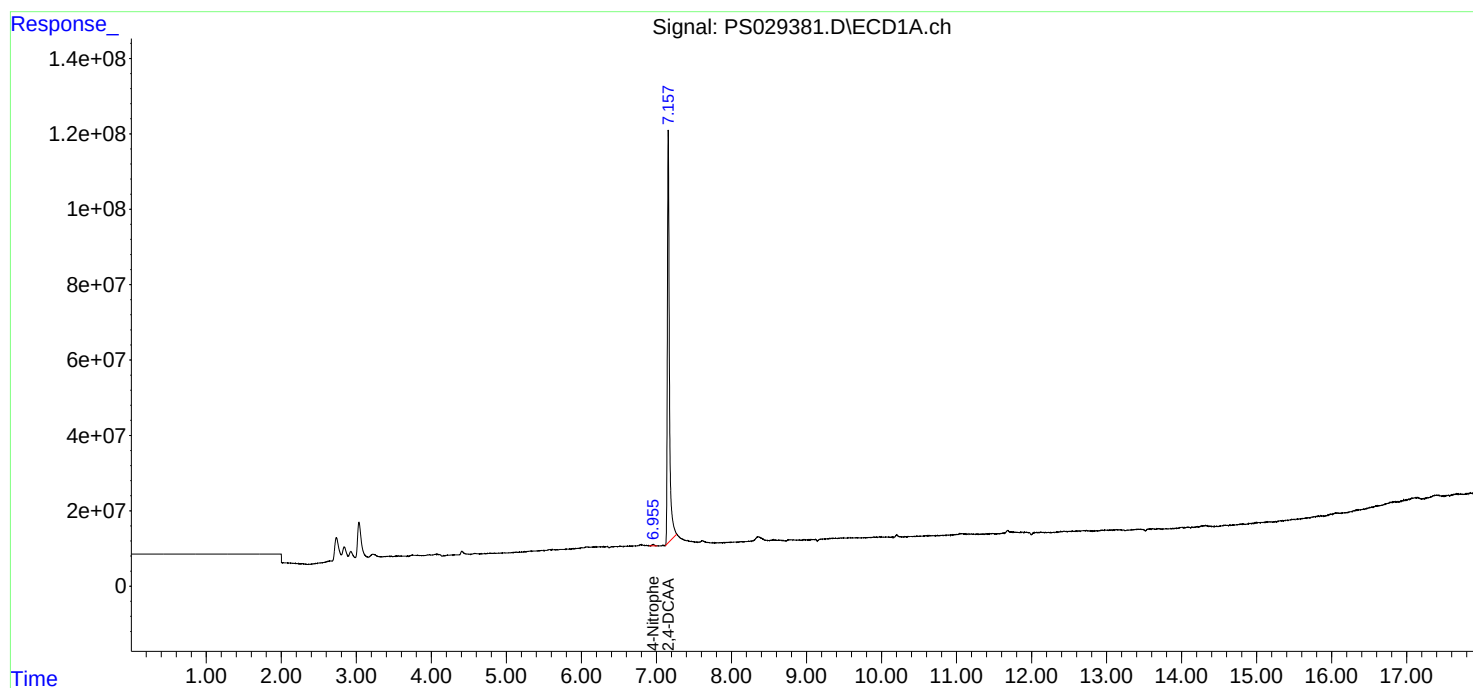


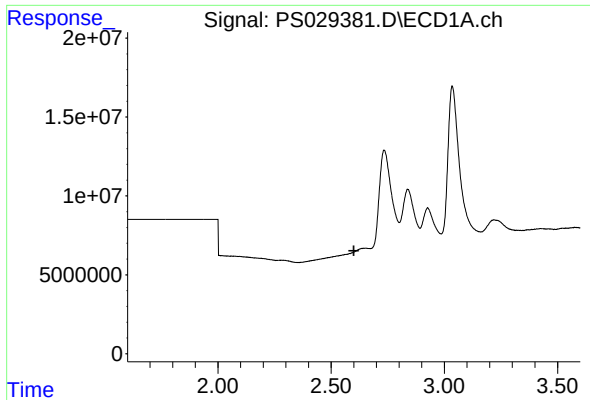

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.600 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

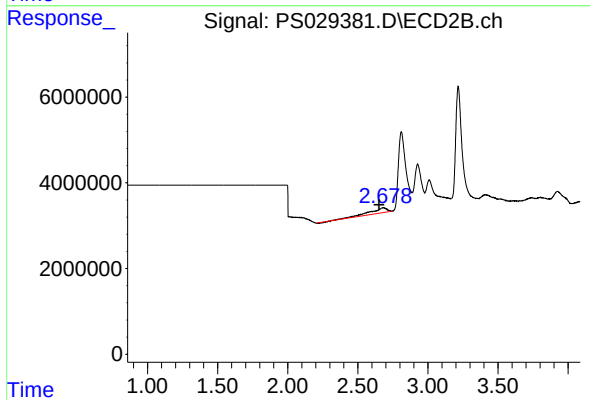


#1 Dalapon

R.T.: 2.677 min
Delta R.T.: 0.027 min
Response: 9888470
Conc: 4.67 ng/ml

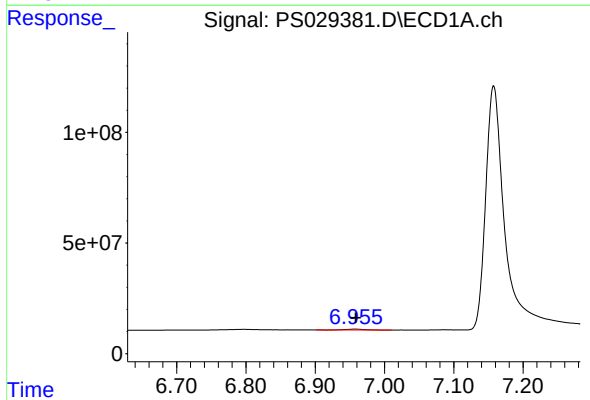


#3 4-Nitrophenol

R.T.: 6.957 min
Delta R.T.: -0.002 min
Response: 7814687
Conc: 3.34 ng/ml

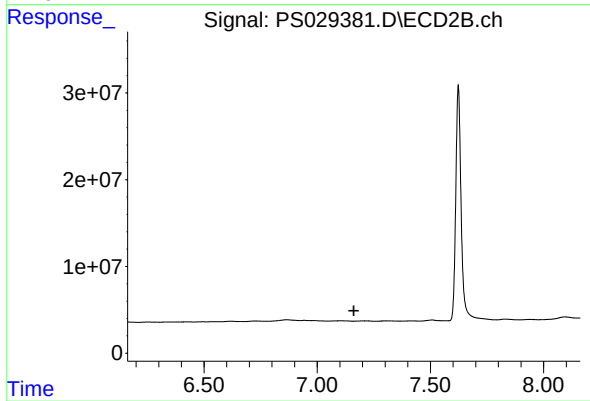

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.162 min
Response: 0
Conc: N.D.

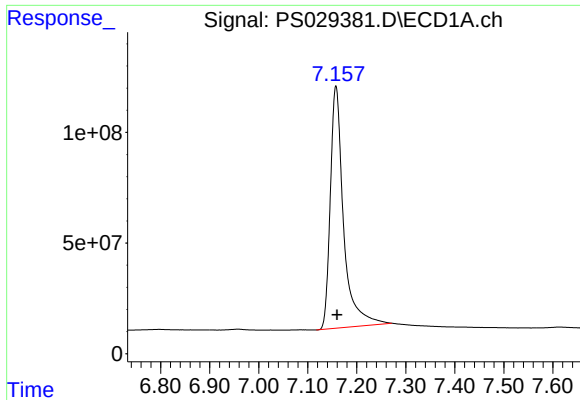

#4 2,4-DCAA


R.T.: 7.158 min
Delta R.T.: -0.002 min
Response: 2052991891
Conc: 498.23 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

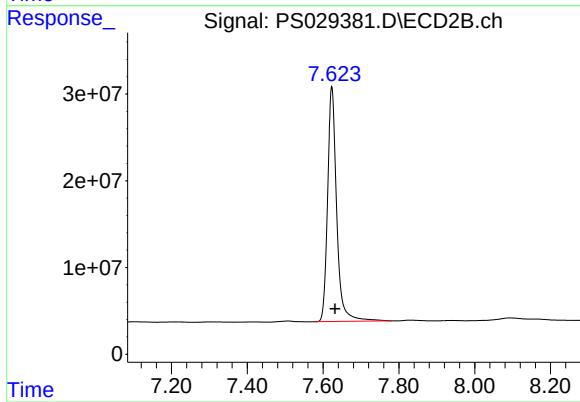


#4 2,4-DCAA

R.T.: 7.623 min
Delta R.T.: -0.009 min
Response: 450757842
Conc: 479.36 ng/ml

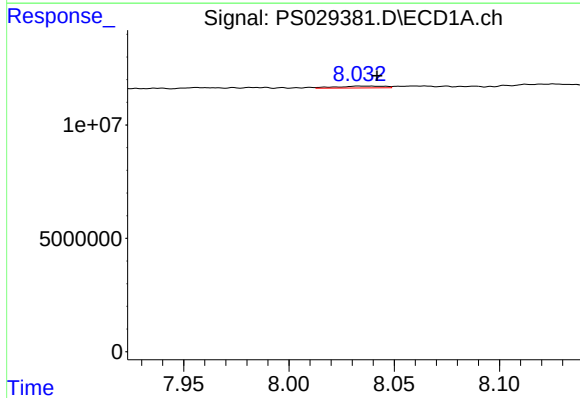

#8 DICHLORPROP

R.T.: 8.033 min
Delta R.T.: -0.009 min
Response: 1296396
Conc: N.D.

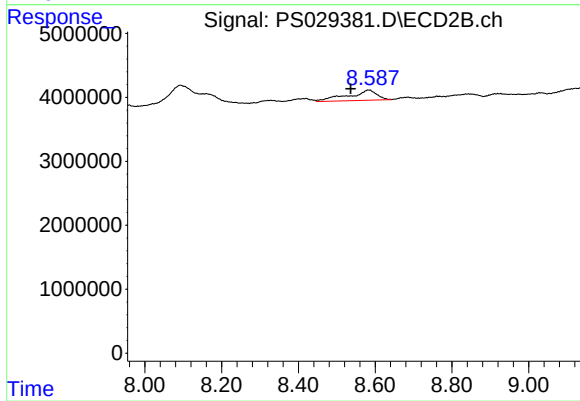

#8 DICHLORPROP

R.T.: 8.583 min
Delta R.T.: 0.047 min
Response: 8332203
Conc: 6.52 ng/ml