

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031125\
 Data File : PS029392.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2025 01:32
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 04:40:13 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022125.M
 Quant Title : 8080.M
 QLast Update : Sat Feb 22 01:02:20 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.156	7.621	2093.0E6	456.6E6	507.946	485.581
Target Compounds							
1) T	Dalapon	0.000	2.682f	0	8375852	N.D.	3.956
2) T	3,5-DICHL...	6.330	0.000	6012502	0	1.028	N.D. #
3) T	4-Nitroph...	6.954	0.000	9772788	0	4.176	N.D. #
5) T	DICAMBA	0.000	7.829	0	3011694	N.D.	<MDL
7) T	MCPA	7.701f	0.000	552805	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	8.500f	0	4019170	N.D.	3.143
10) T	Pentachlo...	8.559	0.000	1897061	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.117	9.748	14288904	15145926	<MDL	1.676 #
12) T	2,4,5-T	9.450	10.187	9133620	9190763	<MDL	1.119 #
13) T	2,4-DB	9.979	0.000	2670353	0	<MDL	N.D. #
14) T	DINOSEB	11.183	0.000	920553	0	<MDL	N.D. #
15) T	Picloram	11.034f	0.000	24738774	0	<MDL	N.D. #
16) T	DCPA	11.467	0.000	21091145	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031125\
Data File : PS029392.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2025 01:32
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 04:40:13 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022125.M
Quant Title : 8080.M
QLast Update : Sat Feb 22 01:02:20 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

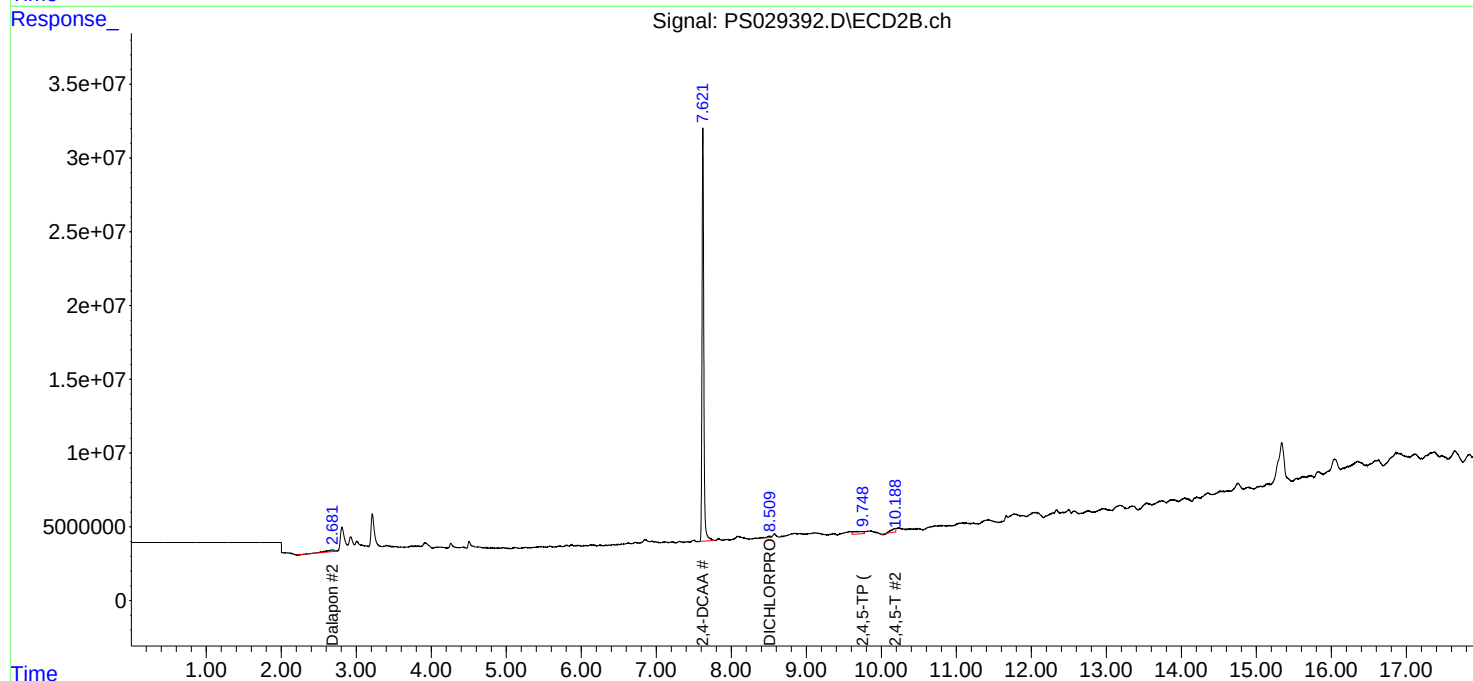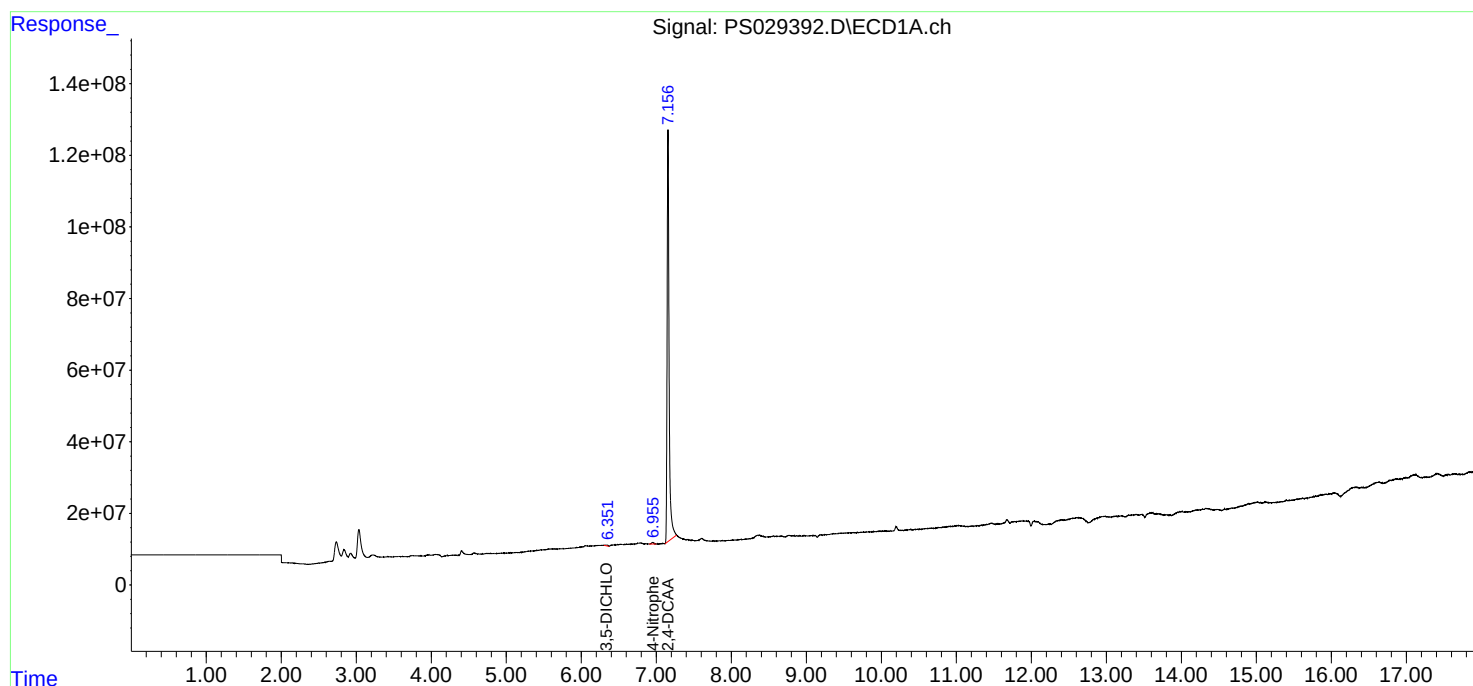


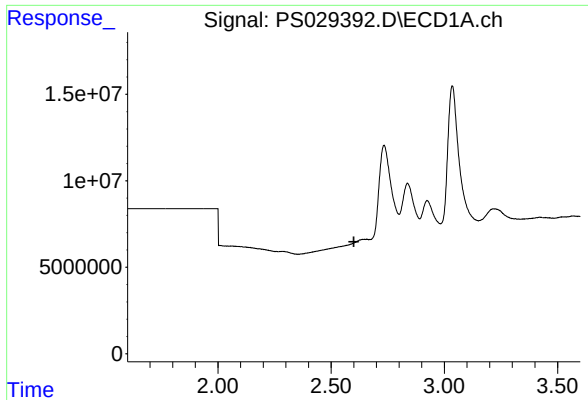

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.600 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

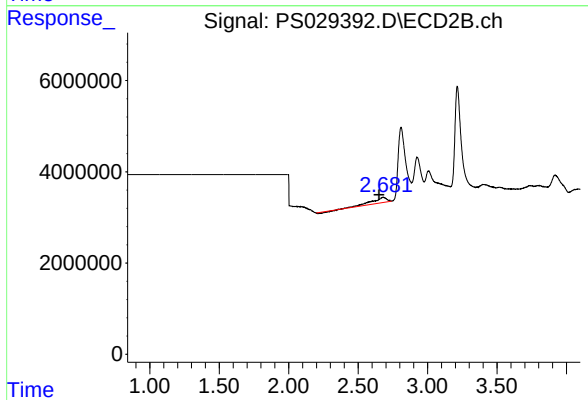


#1 Dalapon

R.T.: 2.682 min
Delta R.T.: 0.031 min
Response: 8375852
Conc: 3.96 ng/ml

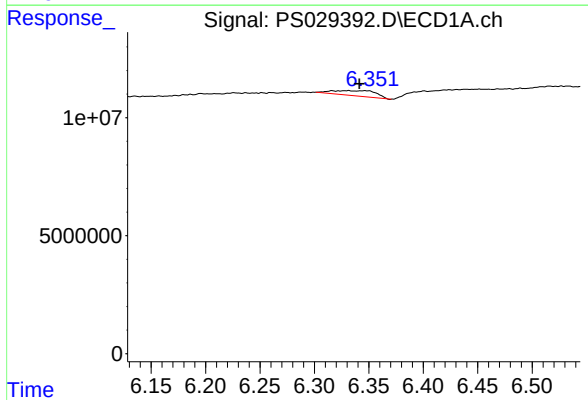


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.330 min
Delta R.T.: -0.011 min
Response: 6012502
Conc: 1.03 ng/ml

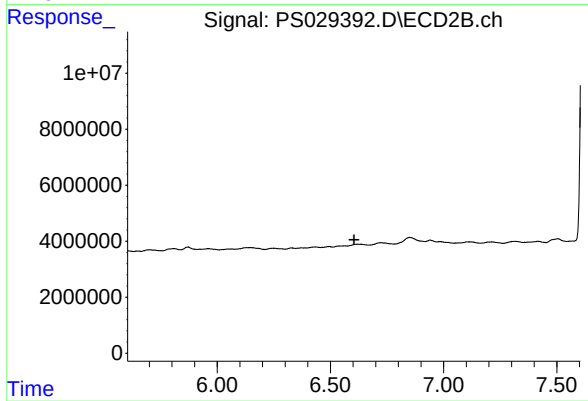

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.604 min
Response: 0
Conc: N.D.

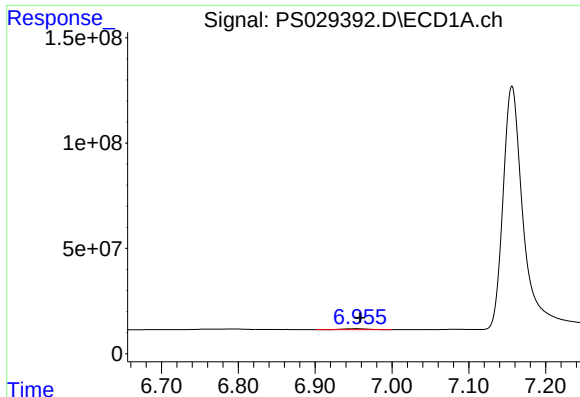

#3 4-Nitrophenol


R.T.: 6.954 min
Delta R.T.: -0.005 min
Response: 9772788
Conc: 4.18 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

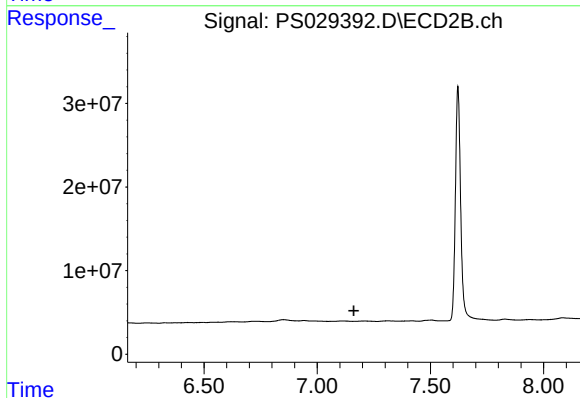


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.162 min
Response: 0
Conc: N.D.

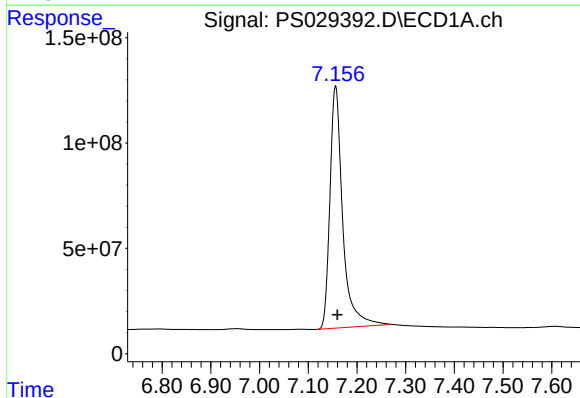


#4 2,4-DCAA

R.T.: 7.156 min
Delta R.T.: -0.004 min
Response: 2093029258
Conc: 507.95 ng/ml

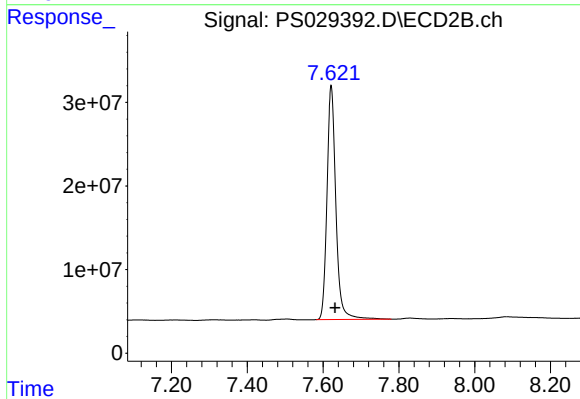

#4 2,4-DCAA


R.T.: 7.621 min
Delta R.T.: -0.011 min
Response: 456607513
Conc: 485.58 ng/ml

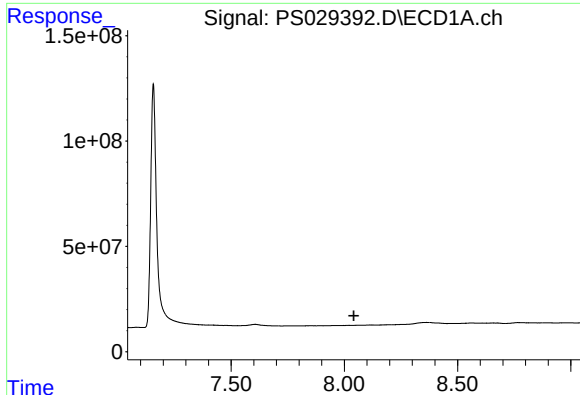

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.042 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

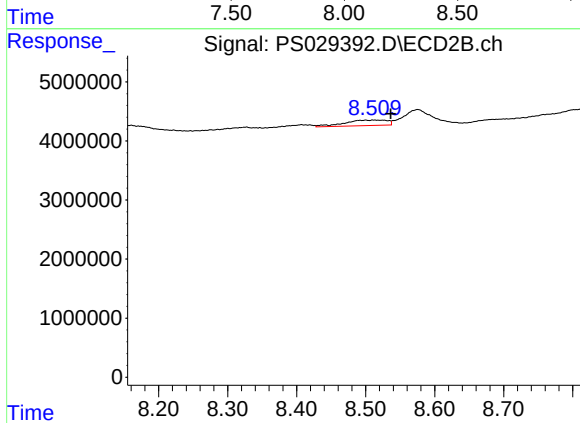


#8 DICHLORPROP

R.T.: 8.500 min
Delta R.T.: -0.036 min
Response: 4019170
Conc: 3.14 ng/ml

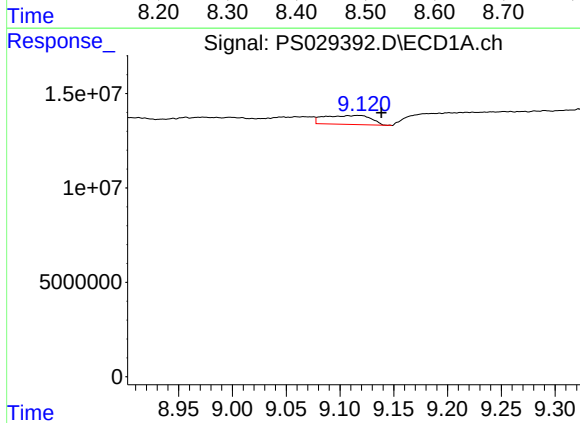


#11 2,4,5-TP (SILVEX)

R.T.: 9.117 min
Delta R.T.: -0.021 min
Response: 14288904
Conc: N.D.

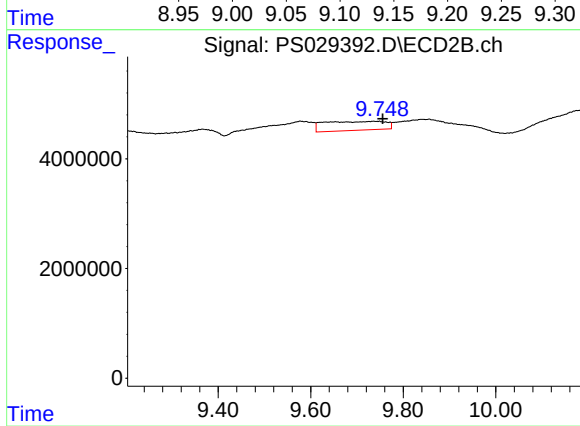

#11 2,4,5-TP (SILVEX)


R.T.: 9.748 min
Delta R.T.: -0.007 min
Response: 15145926
Conc: 1.68 ng/ml

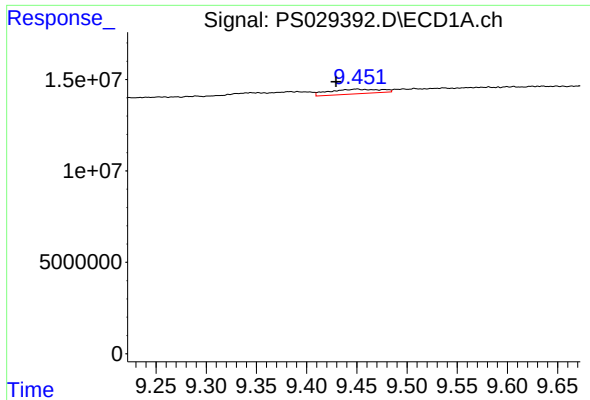

#12 2,4,5-T

R.T.: 9.450 min
Delta R.T.: 0.021 min
Response: 9133620
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

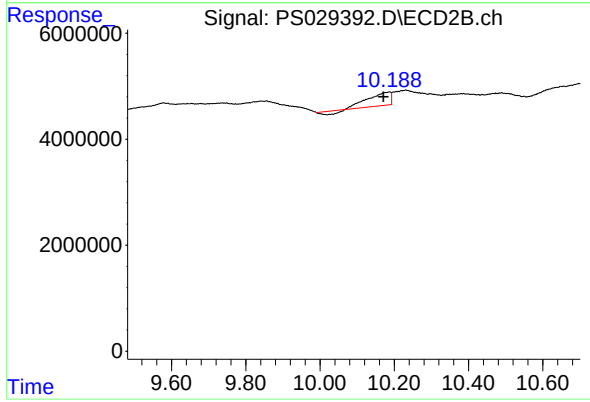

#12 2,4,5-T

R.T.: 10.187 min
Delta R.T.: 0.017 min
Response: 9190763
Conc: 1.12 ng/ml