

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031219\
 Data File : PS003512.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2019 11:38
 Operator : EI\SJ
 Sample : K1689-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 NB-07-030819

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 04:38:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.296	10.796	204.2E6	210.1E6	465.215	447.503
Target Compounds							
1) T	Dalapon	2.814	2.306	38442168	95711689	59.147	151.159 #
2) T	3,5-DICHL...	0.000	8.962	0	4214656	N.D.	6.826 #
5) T	DICAMBA	0.000	11.037	0	3918901	N.D.	2.346 #
6) T	MCP	0.000	11.278	0	374035	N.D.	0.317 #
9) T	2,4-D	13.150	12.656	3828638	881125	8.255	1.679 #
11) T	2,4,5-TP ...	0.000	13.752	0	19465542	N.D.	7.644 #
12) T	2,4,5-T	0.000	14.398	0	12240935	N.D.	6.070 #
13) T	2,4-DB	15.491	15.029	12674146	4073944	53.524	15.954 #
14) T	DINOSEB	0.000	15.519	0	11641251	N.D.	6.522 #
15) T	Picloram	16.787	16.749	6135475	26012454	2.493	10.249 #
16) T	DCPA	0.000	16.567	0	18549239	N.D.	5.964 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031219\
Data File : PS003512.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2019 11:38
Operator : EI\SJ
Sample : K1689-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
NB-07-030819

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 04:38:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

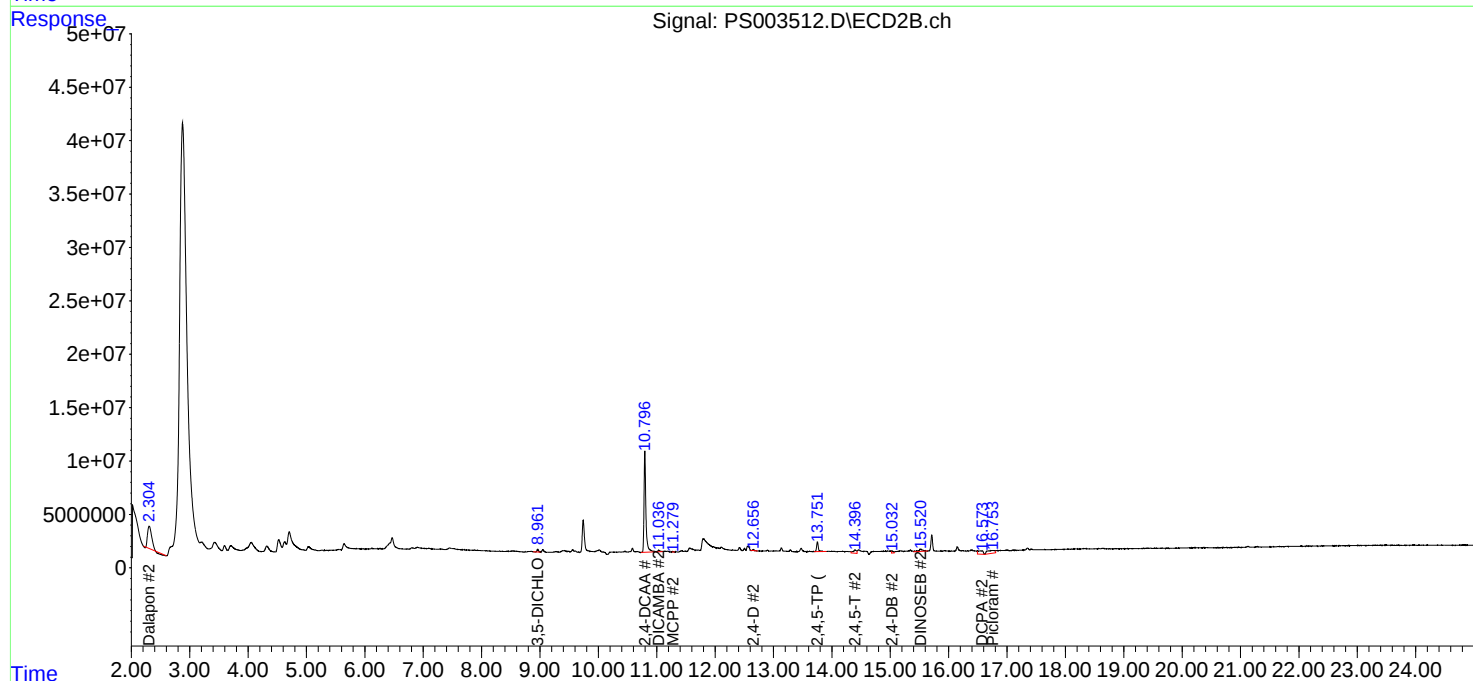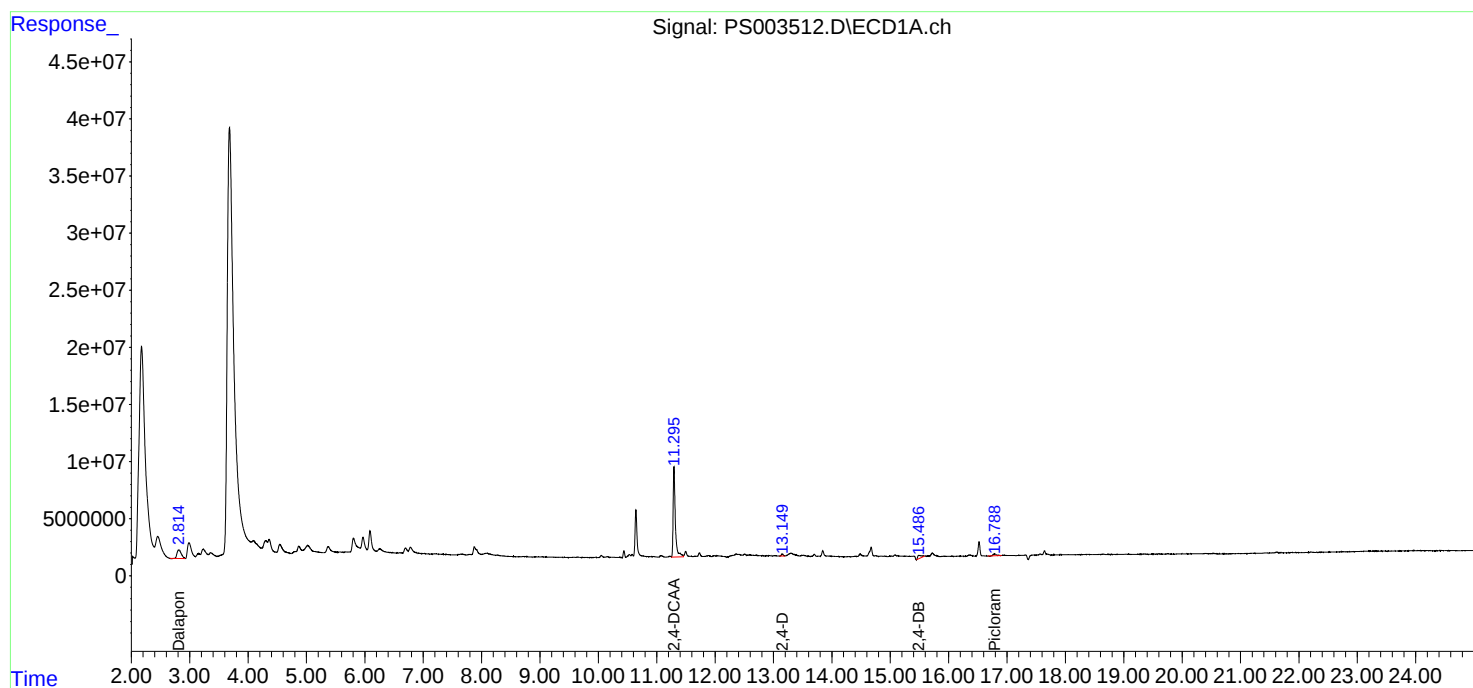


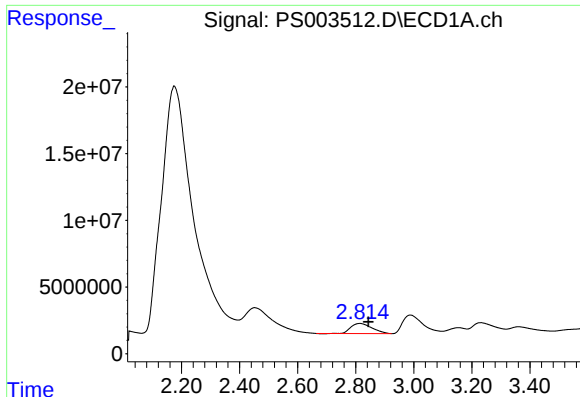

#1 Dalapon


R.T.: 2.814 min
Delta R.T.: -0.030 min
Response: 38442168
Conc: 59.15 ng/ml

Instrument :
ECD_S
ClientSampleId :
NB-07-030819

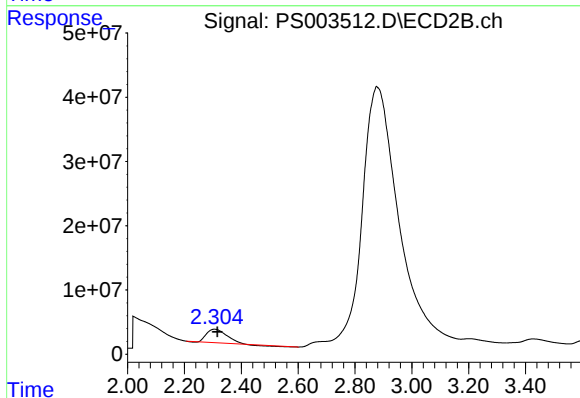


#1 Dalapon

R.T.: 2.306 min
Delta R.T.: -0.011 min
Response: 95711689
Conc: 151.16 ng/ml

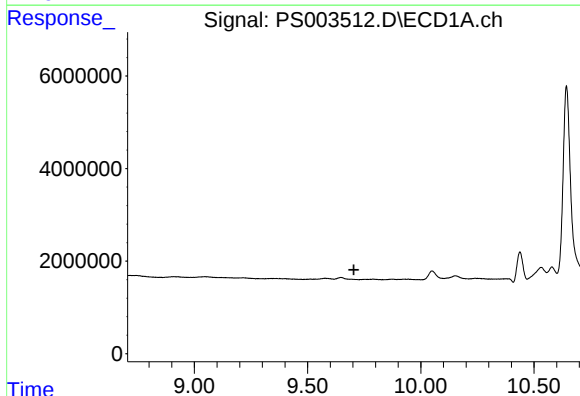


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.705 min
Response: 0
Conc: N.D.

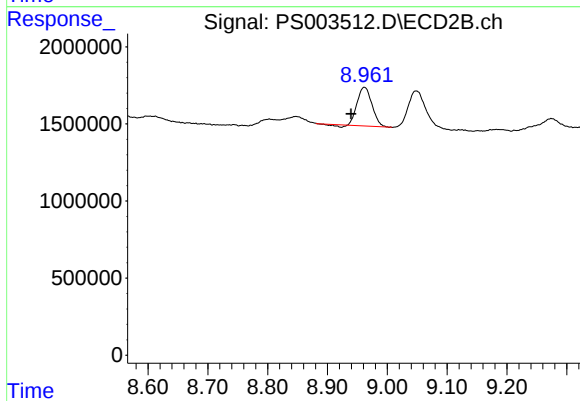

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.962 min
Delta R.T.: 0.022 min
Response: 4214656
Conc: 6.83 ng/ml

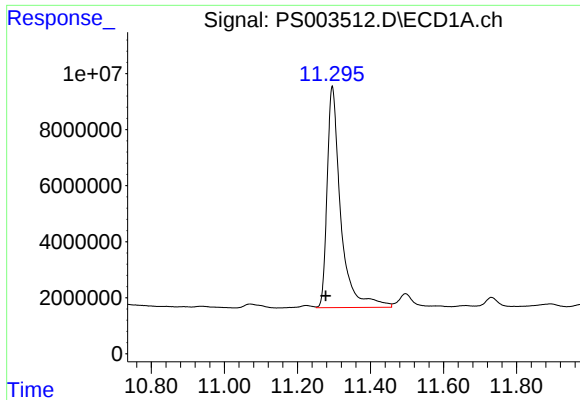

#4 2,4-DCAA


R.T.: 11.296 min
Delta R.T.: 0.018 min
Response: 204240977
Conc: 465.22 ng/ml

Instrument :
ECD_S
ClientSampleId :
NB-07-030819

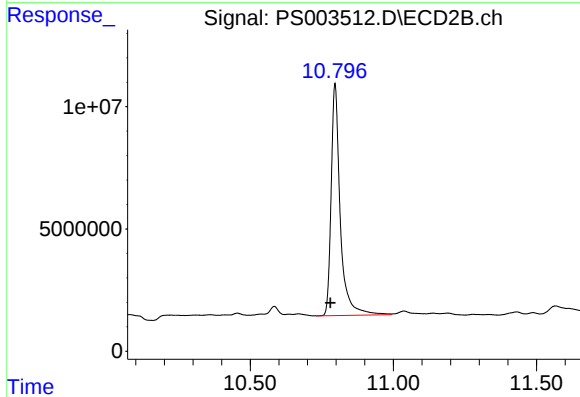


#4 2,4-DCAA

R.T.: 10.796 min
Delta R.T.: 0.016 min
Response: 210133399
Conc: 447.50 ng/ml

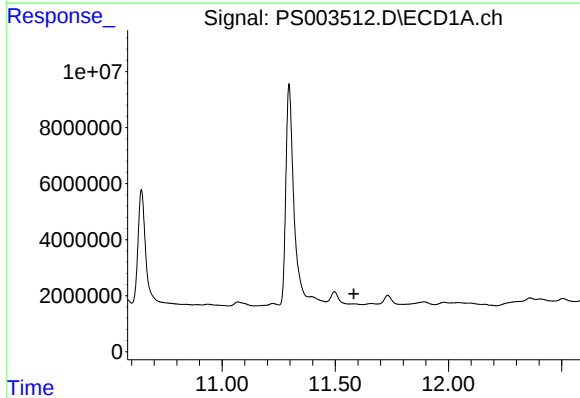


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.582 min
Response: 0
Conc: N.D.

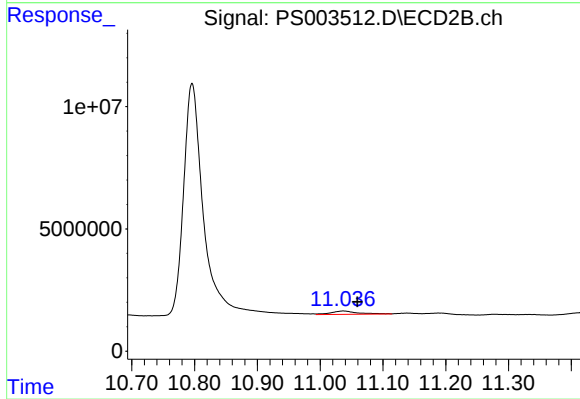

#5 DICAMBA


R.T.: 11.037 min
Delta R.T.: -0.022 min
Response: 3918901
Conc: 2.35 ng/ml

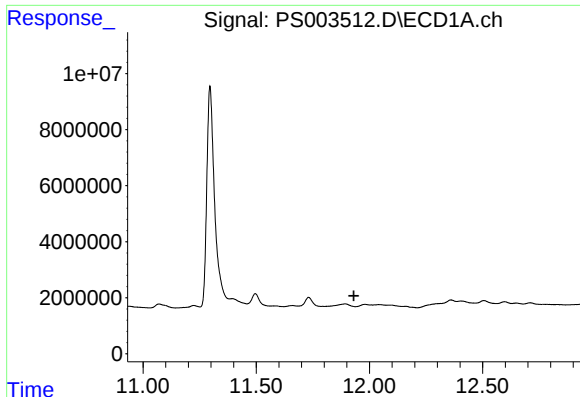

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 11.931 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
NB-07-030819

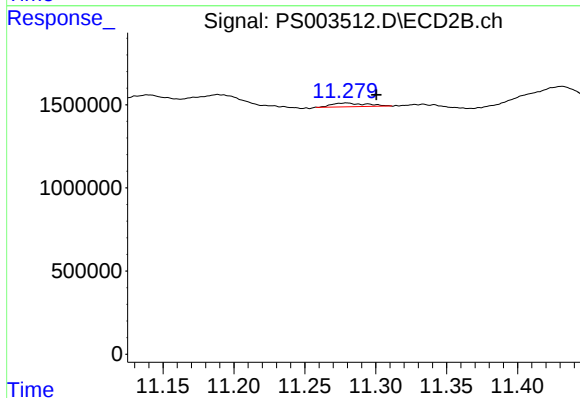


#6 MCPP

R.T.: 11.278 min
Delta R.T.: -0.022 min
Response: 374035
Conc: 0.32 ug/ml

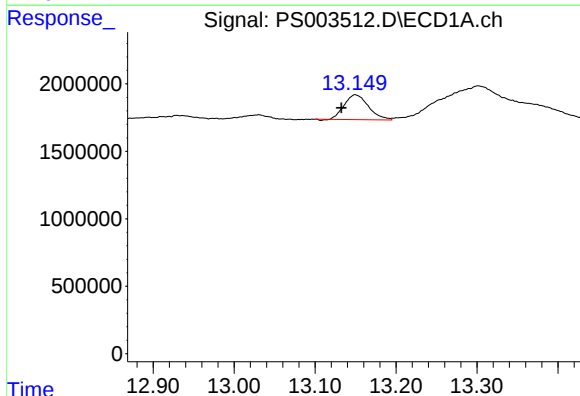


#9 2,4-D

R.T.: 13.150 min
Delta R.T.: 0.018 min
Response: 3828638
Conc: 8.25 ng/ml

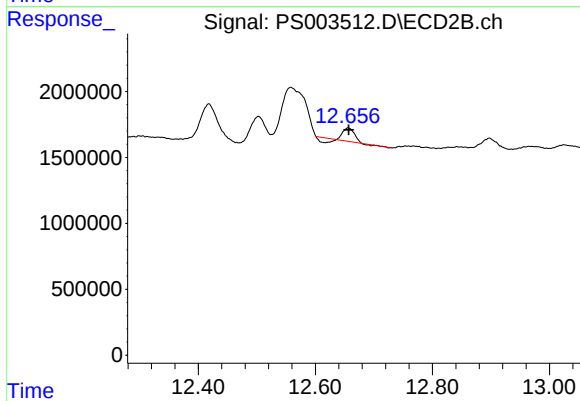

#9 2,4-D


R.T.: 12.656 min
Delta R.T.: 0.000 min
Response: 881125
Conc: 1.68 ng/ml

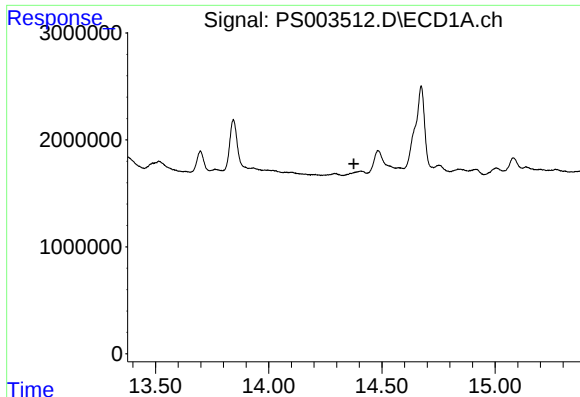

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
NB-07-030819

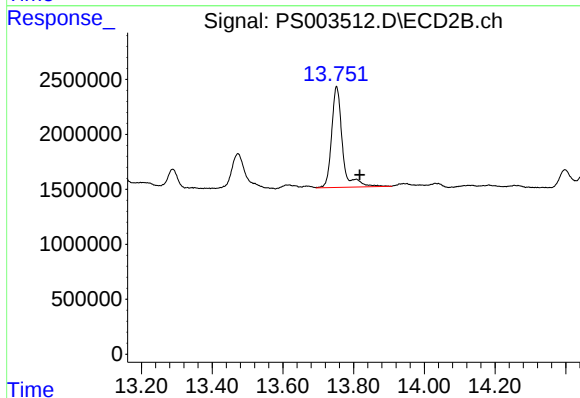


#11 2,4,5-TP (SILVEX)

R.T.: 13.752 min
Delta R.T.: -0.066 min
Response: 19465542
Conc: 7.64 ng/ml

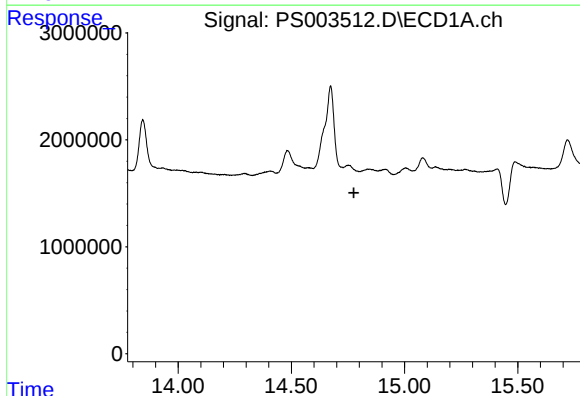


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

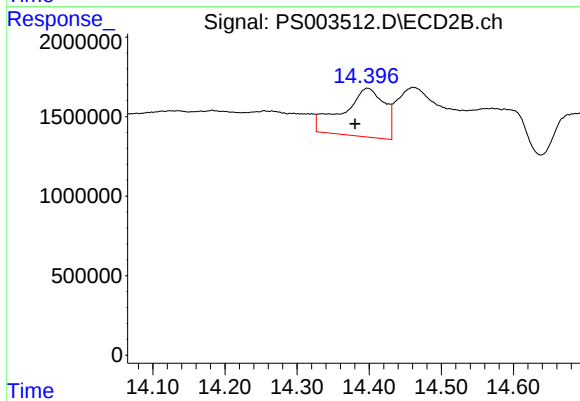

#12 2,4,5-T


R.T.: 14.398 min
Delta R.T.: 0.017 min
Response: 12240935
Conc: 6.07 ng/ml

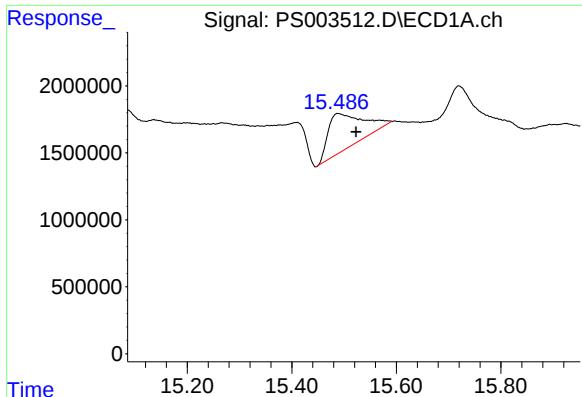

#13 2,4-DB


R.T.: 15.491 min
Delta R.T.: -0.032 min
Response: 12674146
Conc: 53.52 ng/ml

Instrument :
ECD_S
ClientSampleId :
NB-07-030819

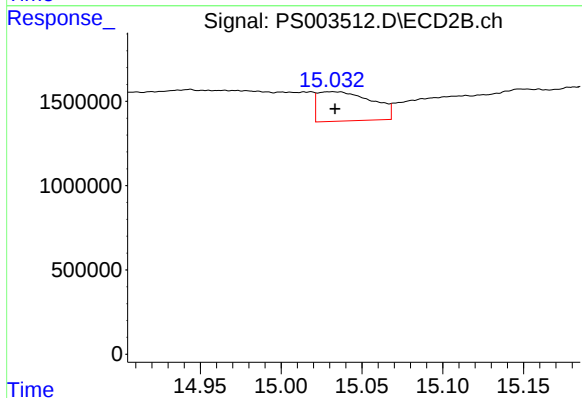


#13 2,4-DB

R.T.: 15.029 min
Delta R.T.: -0.005 min
Response: 4073944
Conc: 15.95 ng/ml

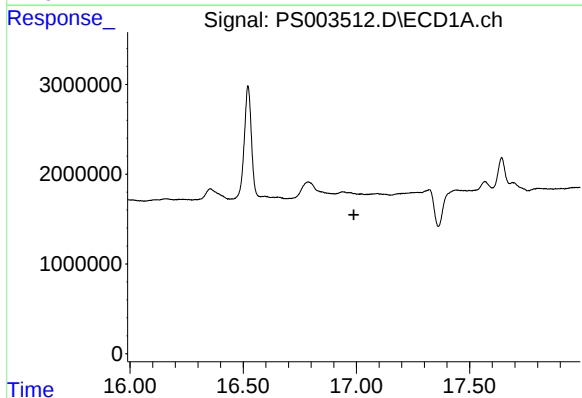


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 16.989 min
Response: 0
Conc: N.D.

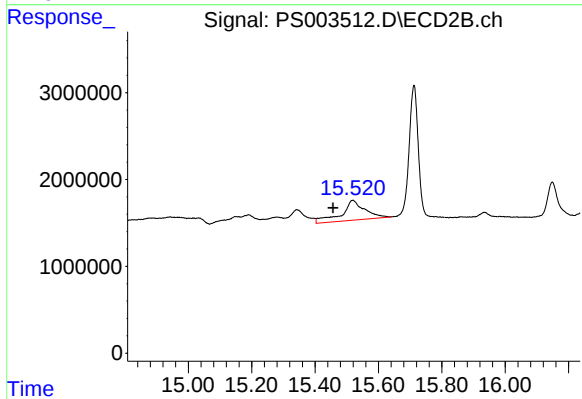

#14 DINOSEB


R.T.: 15.519 min
Delta R.T.: 0.063 min
Response: 11641251
Conc: 6.52 ng/ml

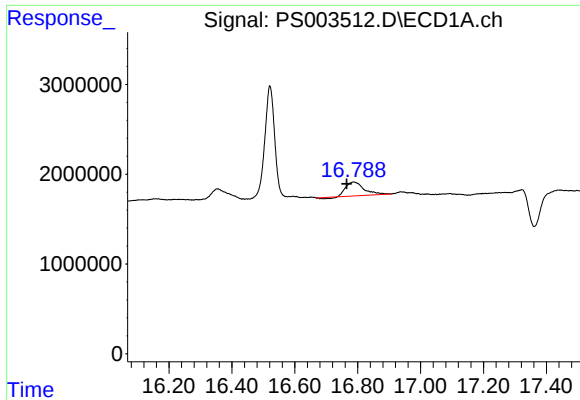

#15 Picloram


R.T.: 16.787 min
Delta R.T.: 0.022 min
Response: 6135475
Conc: 2.49 ng/ml

Instrument :
ECD_S
ClientSampleId :
NB-07-030819

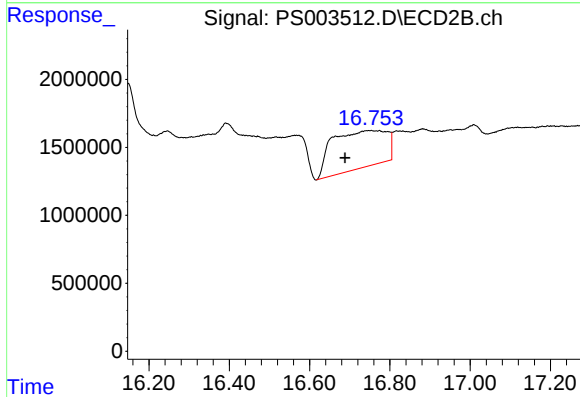


#15 Picloram

R.T.: 16.749 min
Delta R.T.: 0.061 min
Response: 26012454
Conc: 10.25 ng/ml

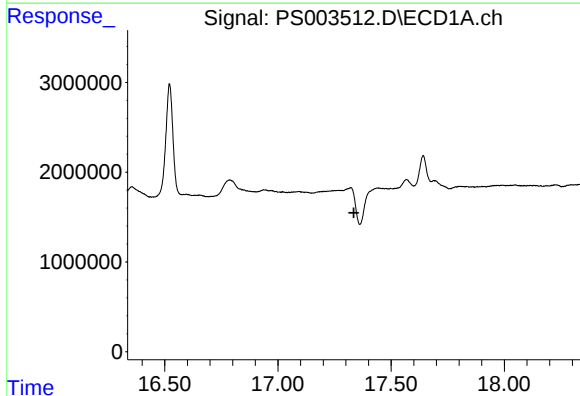

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.335 min
Response: 0
Conc: N.D.

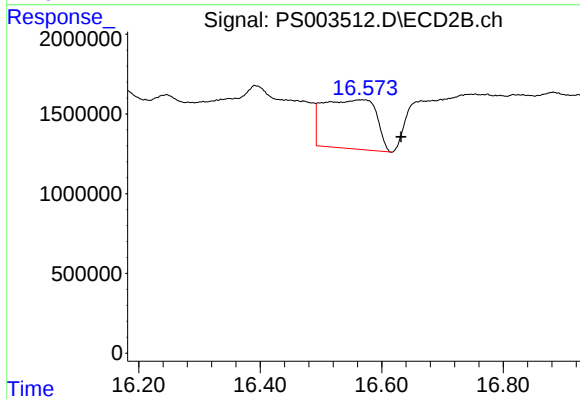

#16 DCPA

R.T.: 16.567 min
Delta R.T.: -0.065 min
Response: 18549239
Conc: 5.96 ng/ml