

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031219\
 Data File : PS003515.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2019 13:12
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 04:39:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.301	10.799	228.1E6	194.6E6	519.568	414.416
Target Compounds							
3) T	4-Nitroph...	0.000	9.956	0	247628	N.D.	1.101 #
7) T	MCPA	0.000	11.687	0	333071	N.D.	0.193 #
8) T	DICHLORPROP	0.000	12.199	0	1263690	N.D.	3.058 #
9) T	2,4-D	0.000	12.661	0	6836	N.D.	0.013 #
10) T	Pentachlo...	0.000	13.215	0	1071107	N.D.	0.163 #
11) T	2,4,5-TP ...	0.000	13.866	0	2170297	N.D.	0.852 #
13) T	2,4-DB	0.000	15.011	0	180487	N.D.	0.707 #
14) T	DINOSEB	0.000	15.483	0	81471	N.D.	0.046 #
15) T	Picloram	0.000	16.651	0	902044	N.D.	0.355 #
16) T	DCPA	0.000	16.651	0	902044	N.D.	0.290 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031219\
Data File : PS003515.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2019 13:12
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 04:39:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

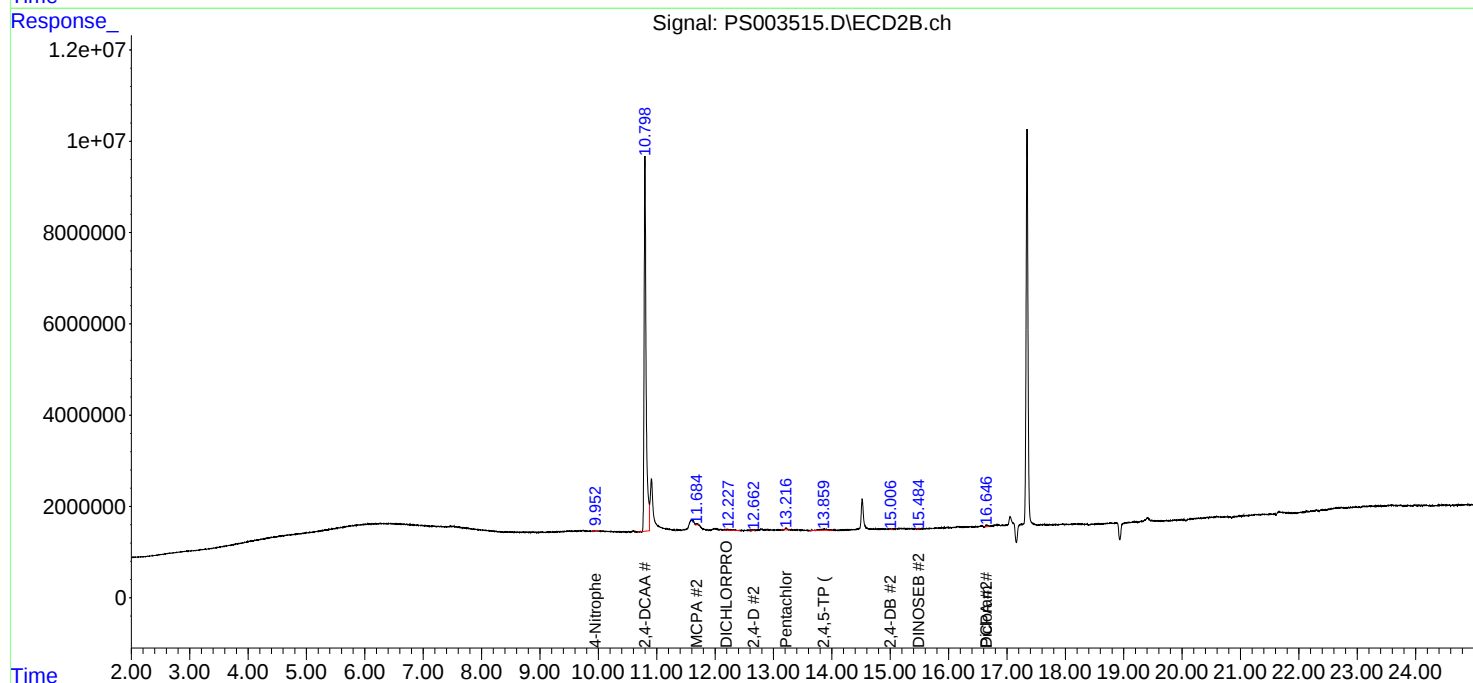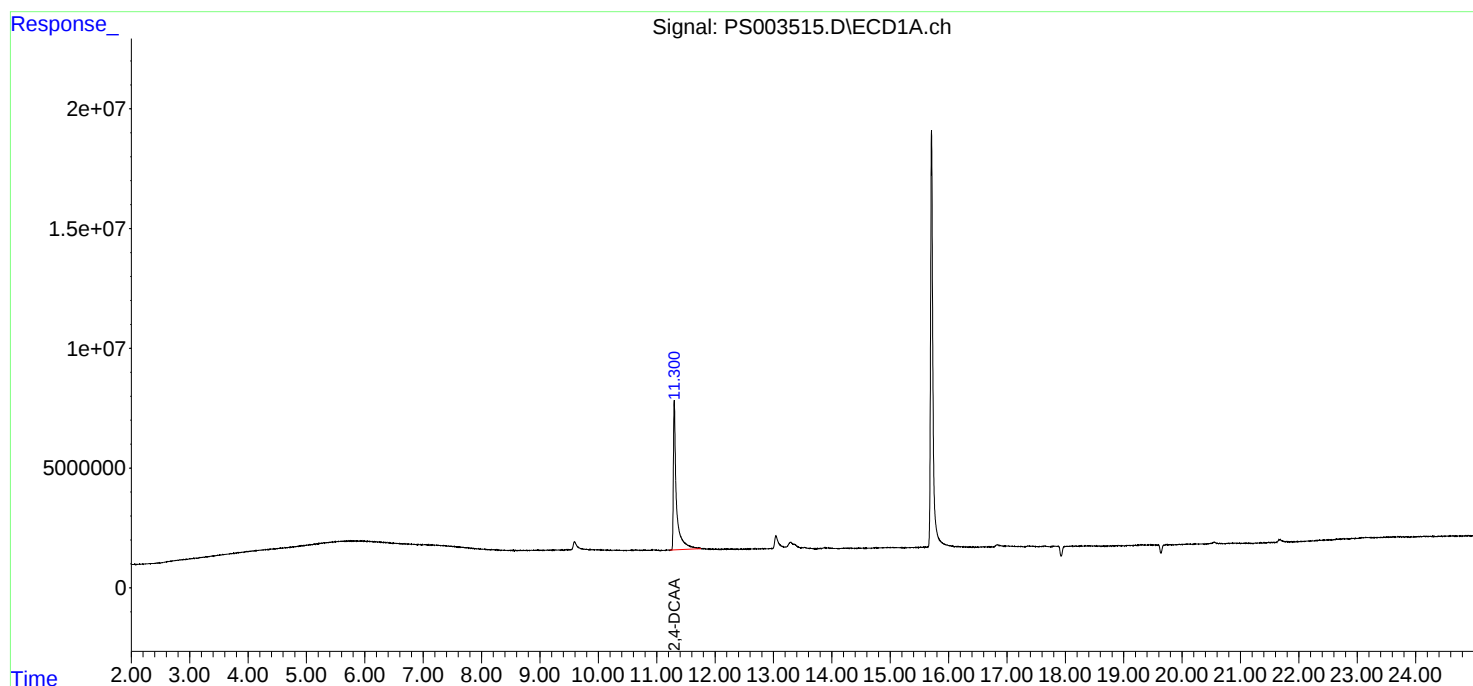


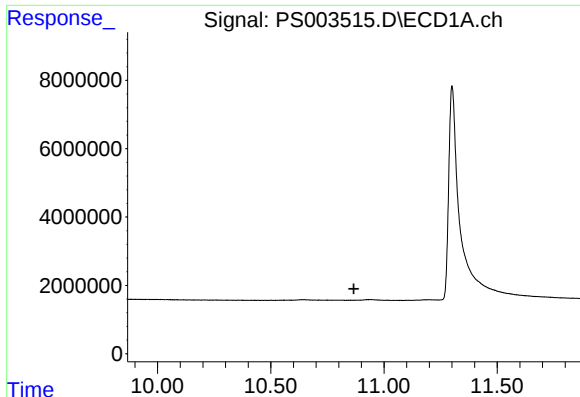

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

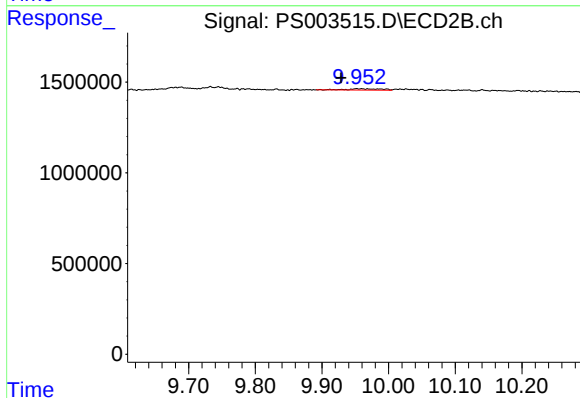


#3 4-Nitrophenol

R.T.: 9.956 min
Delta R.T.: 0.028 min
Response: 247628
Conc: 1.10 ng/ml

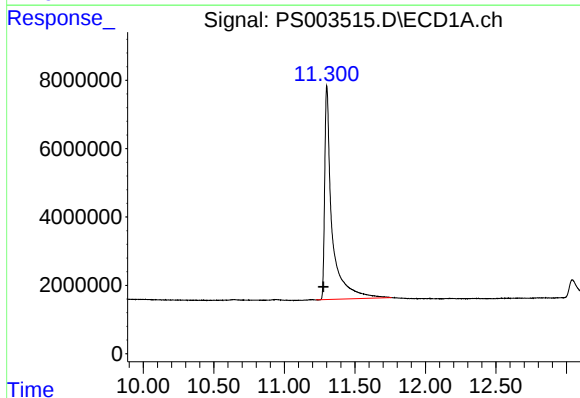


#4 2,4-DCAA

R.T.: 11.301 min
Delta R.T.: 0.023 min
Response: 228103290
Conc: 519.57 ng/ml

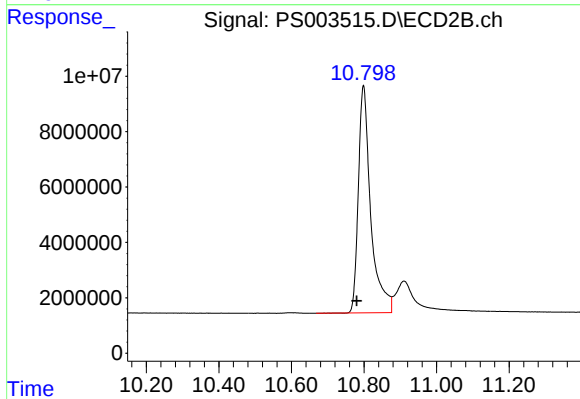

#4 2,4-DCAA


R.T.: 10.799 min
Delta R.T.: 0.019 min
Response: 194596894
Conc: 414.42 ng/ml

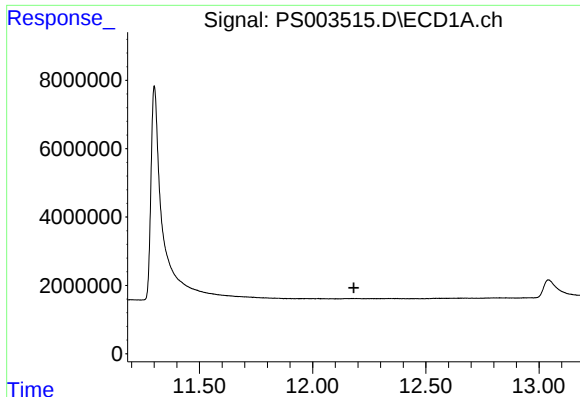

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.182 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

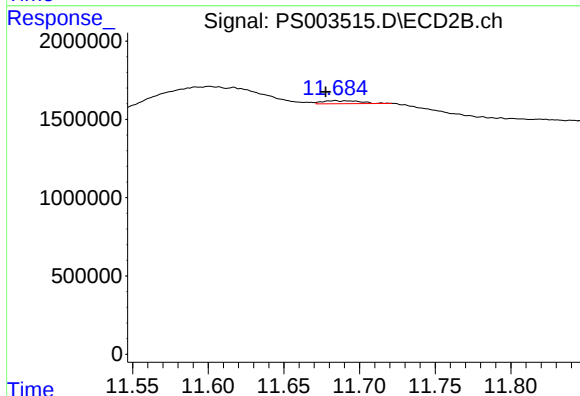


#7 MCPA

R.T.: 11.687 min
Delta R.T.: 0.009 min
Response: 333071
Conc: 0.19 ug/ml

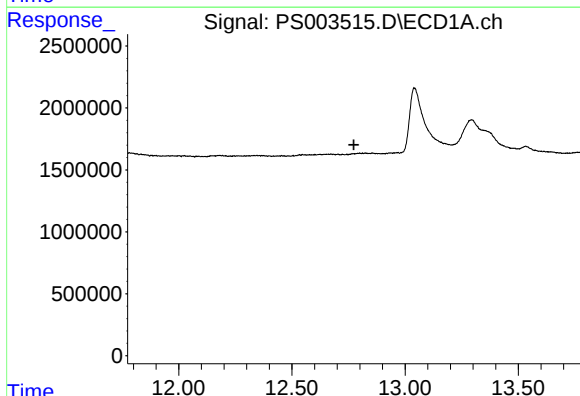


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 12.773 min
Response: 0
Conc: N.D.

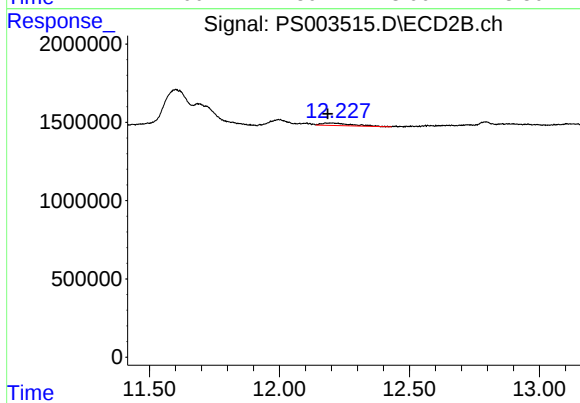

#8 DICHLORPROP


R.T.: 12.199 min
Delta R.T.: 0.014 min
Response: 1263690
Conc: 3.06 ng/ml

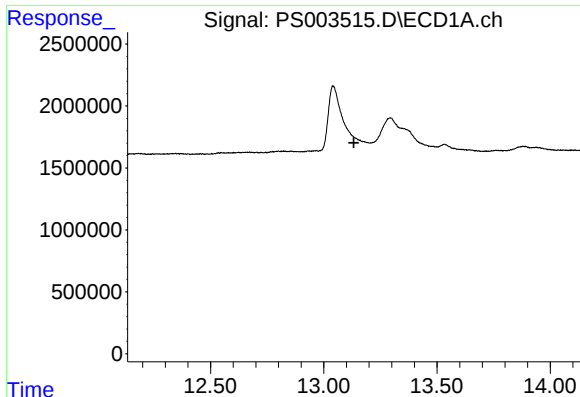

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.133 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

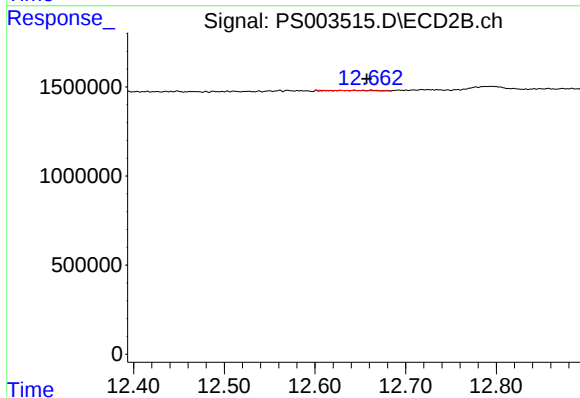


#9 2,4-D

R.T.: 12.661 min
Delta R.T.: 0.004 min
Response: 6836
Conc: 0.01 ng/ml

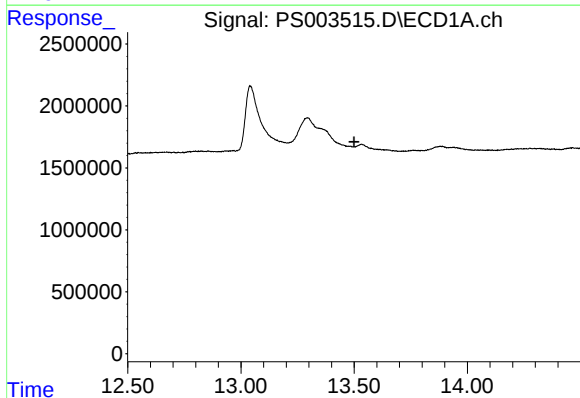


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 13.499 min
Response: 0
Conc: N.D.

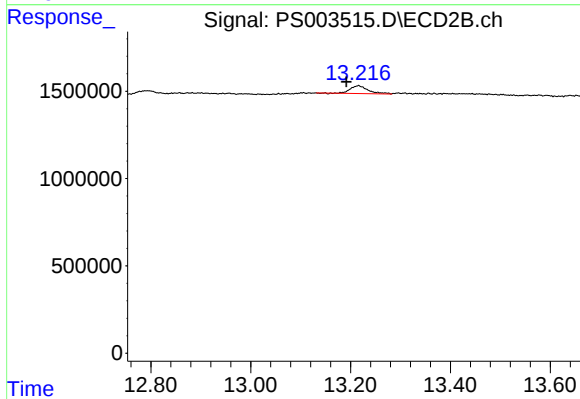

#10 Pentachlorophenol


R.T.: 13.215 min
Delta R.T.: 0.024 min
Response: 1071107
Conc: 0.16 ng/ml

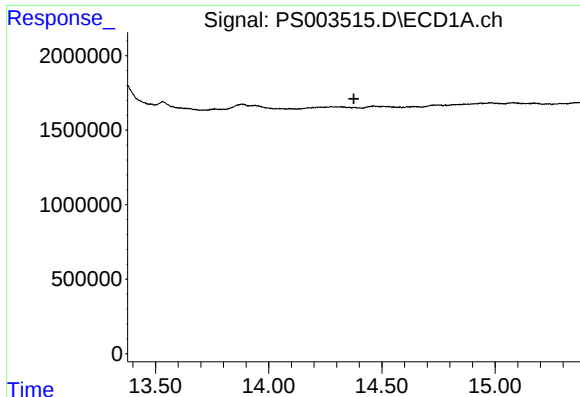

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

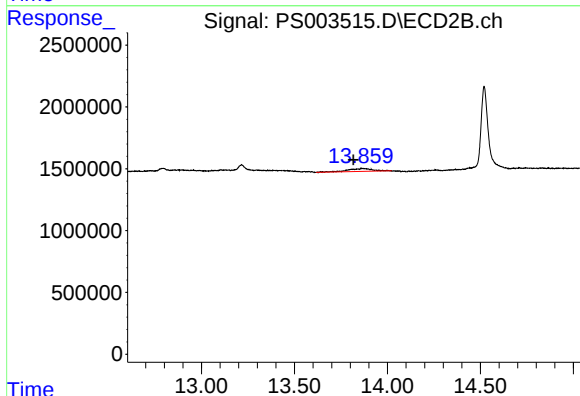


#11 2,4,5-TP (SILVEX)

R.T.: 13.866 min
Delta R.T.: 0.048 min
Response: 2170297
Conc: 0.85 ng/ml

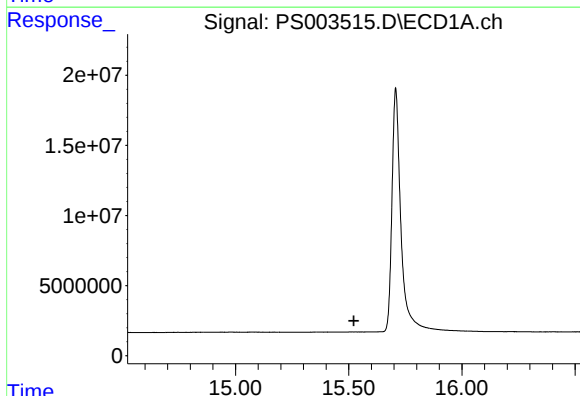


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.523 min
Response: 0
Conc: N.D.

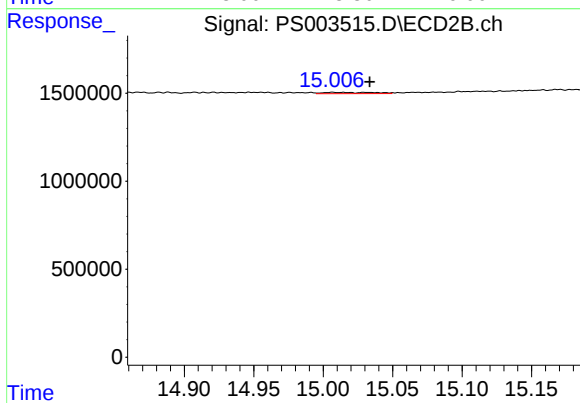

#13 2,4-DB


R.T.: 15.011 min
Delta R.T.: -0.022 min
Response: 180487
Conc: 0.71 ng/ml

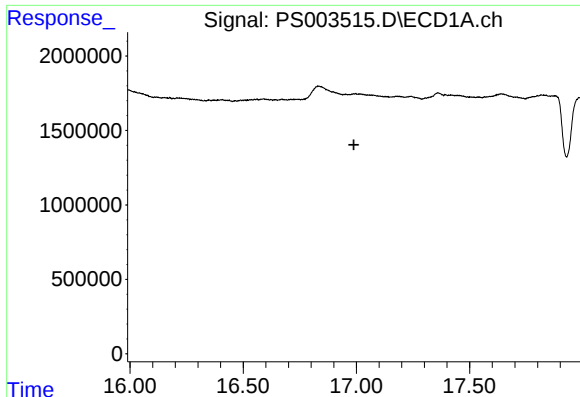

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 16.989 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

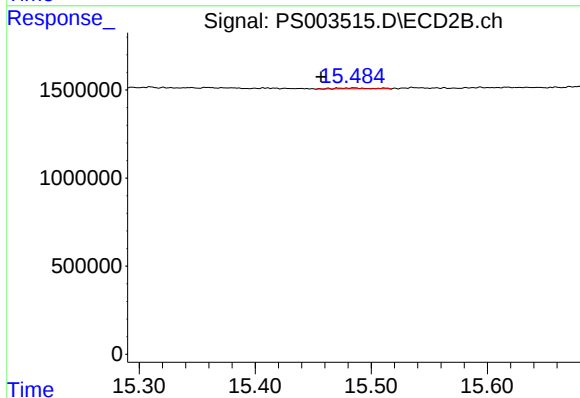


#14 DINOSEB

R.T.: 15.483 min
Delta R.T.: 0.026 min
Response: 81471
Conc: 0.05 ng/ml

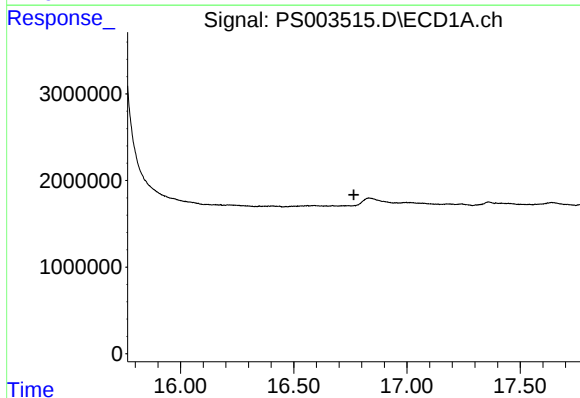


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.765 min
Response: 0
Conc: N.D.

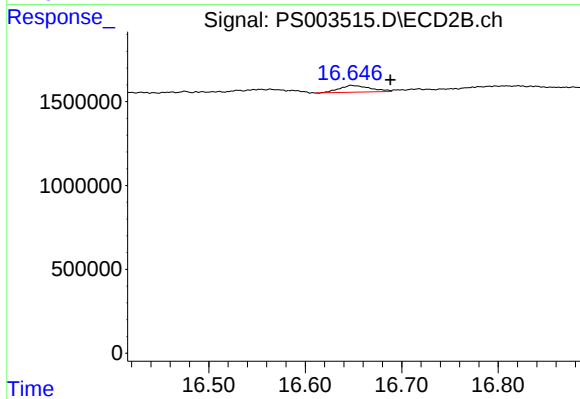

#15 Picloram


R.T.: 16.651 min
Delta R.T.: -0.038 min
Response: 902044
Conc: 0.36 ng/ml

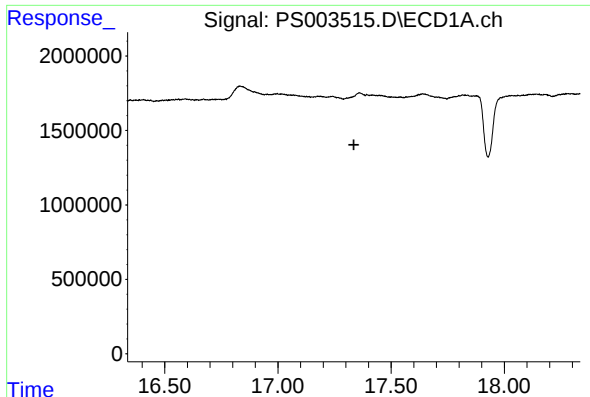

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.335 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

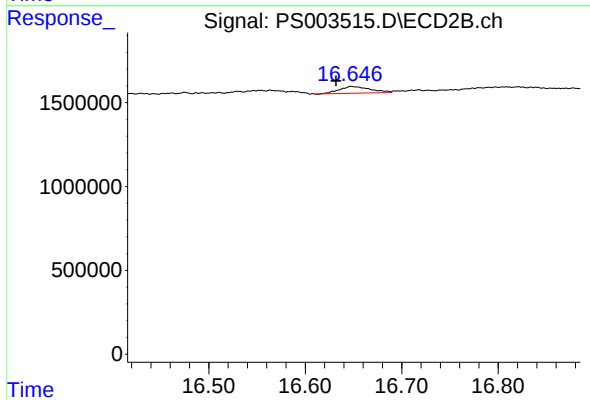

#16 DCPA

R.T.: 16.651 min
Delta R.T.: 0.019 min
Response: 902044
Conc: 0.29 ng/ml