

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031219\
 Data File : PS003517.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2019 14:14
 Operator : EI\SJ
 Sample : K1691-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CL-02-030819-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 04:40:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.310	10.811	257.7E6	259.0E6	587.033	551.637
Target Compounds							
1) T	Dalapon	2.827	2.324	50470421	120.9E6	77.654	190.998 #
2) T	3,5-DICHL...	0.000	8.977	0	4445395	N.D.	7.200 #
5) T	DICAMBA	0.000	11.051	0	4958147	N.D.	2.968 #
6) T	MCP	0.000	11.293	0	249497	N.D.	0.211 #
8) T	DICHLORPROP	0.000	12.118	0	25161031	N.D.	60.887 #
9) T	2,4-D	13.166	12.673	5924266	-6145519	12.773	N.D. #
10) T	Pentachlo...	0.000	13.225	0	784149	N.D.	0.119 #
11) T	2,4,5-TP ...	0.000	13.766	0	48255819	N.D.	18.950 #
12) T	2,4,5-T	0.000	14.354	0	2528983	N.D.	1.254 #
13) T	2,4-DB	15.501	15.034	12309220	2892350	51.982	11.327 #
15) T	Picloram	16.800	16.670	6988195	5908107	2.839	2.328
16) T	DCPA	0.000	16.670	0	5908107	N.D.	1.899 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031219\
Data File : PS003517.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2019 14:14
Operator : EI\SJ
Sample : K1691-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
CL-02-030819-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 04:40:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

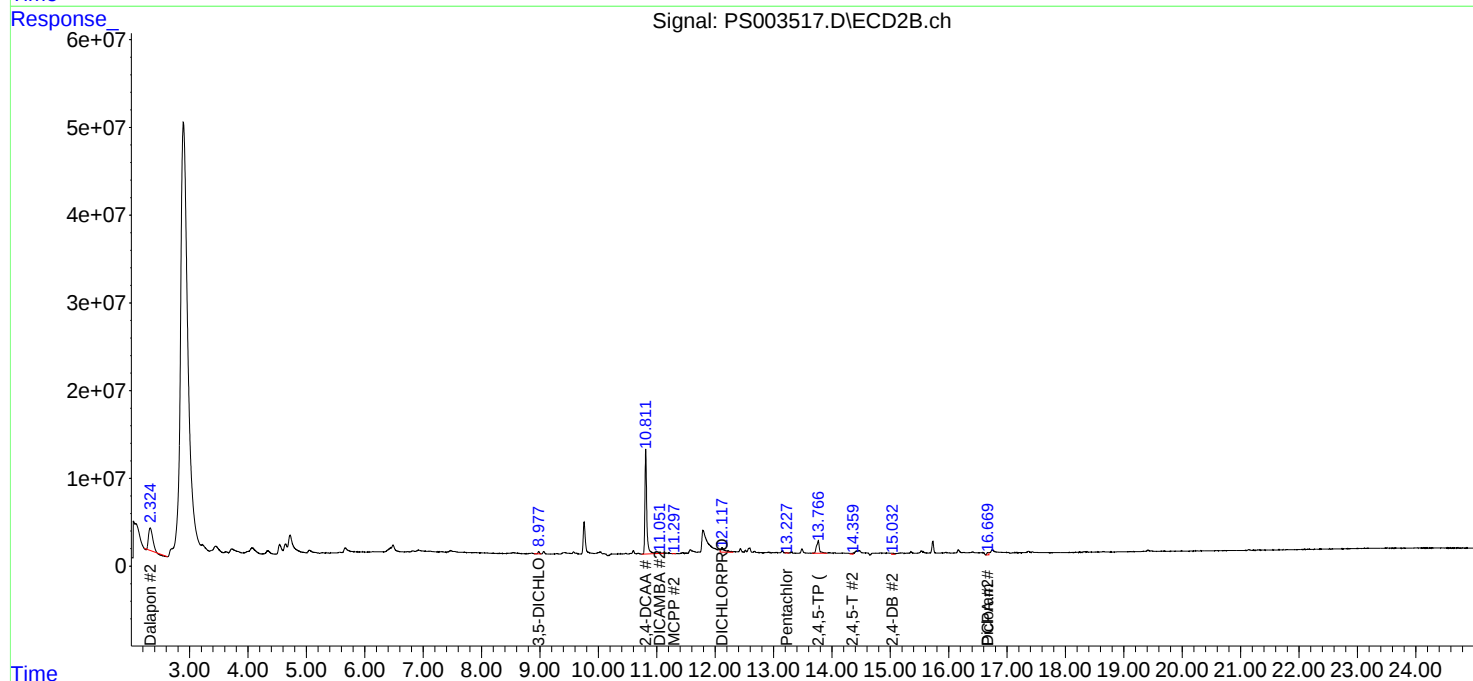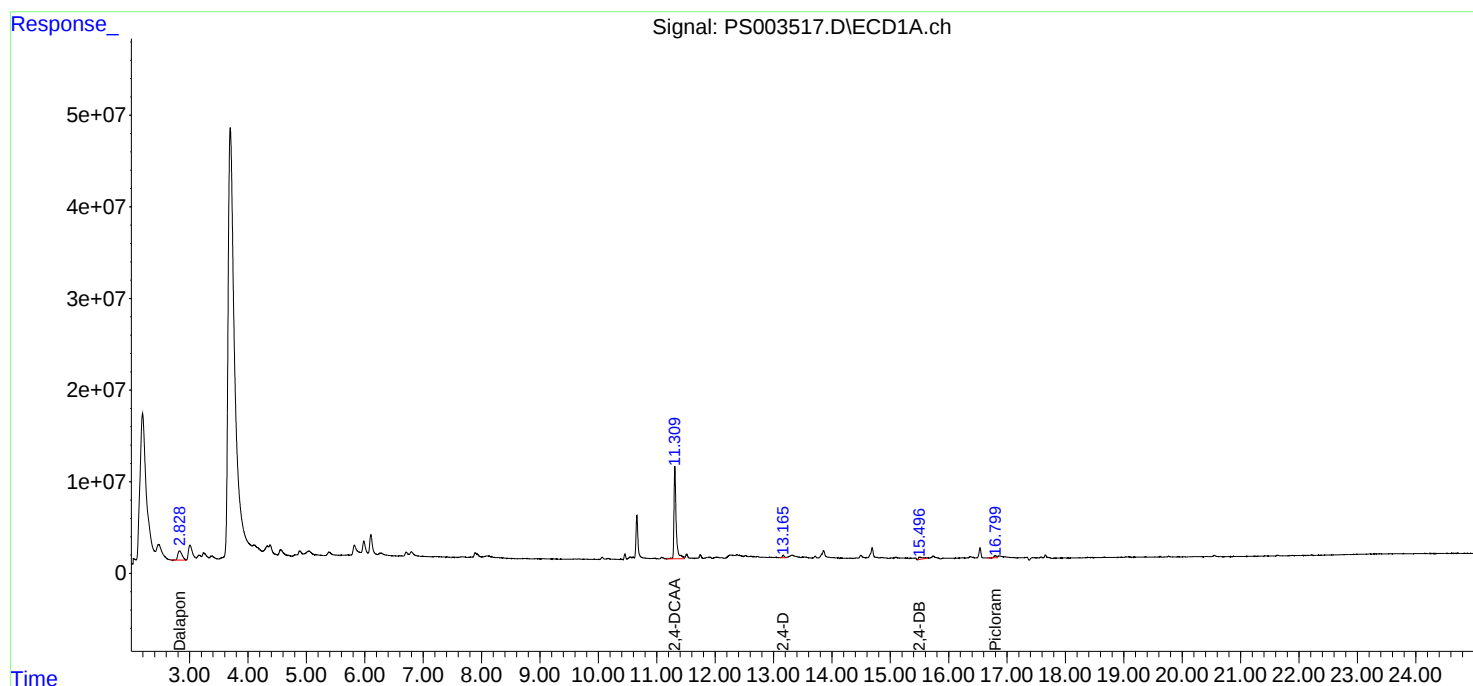


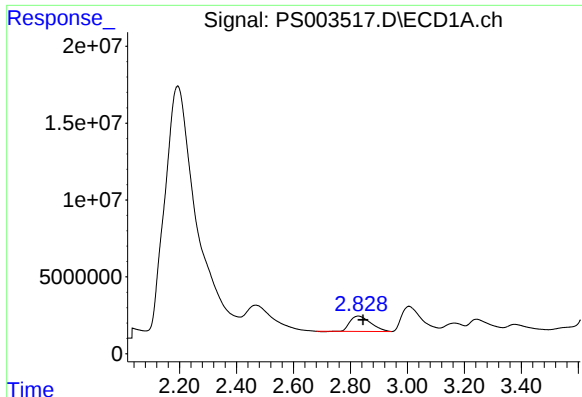

#1 Dalapon


R.T.: 2.827 min
Delta R.T.: -0.017 min
Response: 50470421
Conc: 77.65 ng/ml

Instrument :
ECD_S
ClientSampleId :
CL-02-030819-A

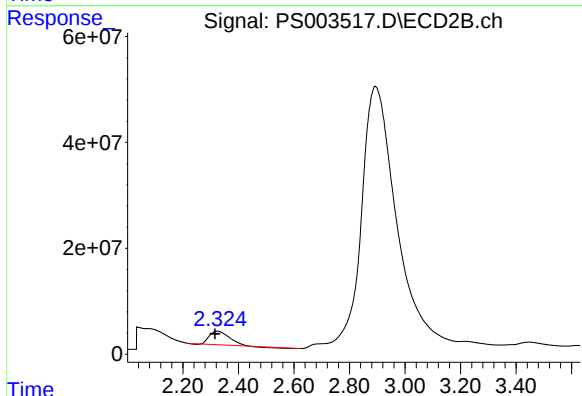


#1 Dalapon

R.T.: 2.324 min
Delta R.T.: 0.007 min
Response: 120937054
Conc: 191.00 ng/ml

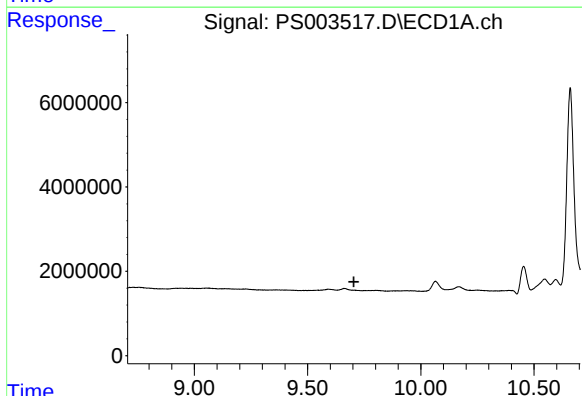


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.705 min
Response: 0
Conc: N.D.

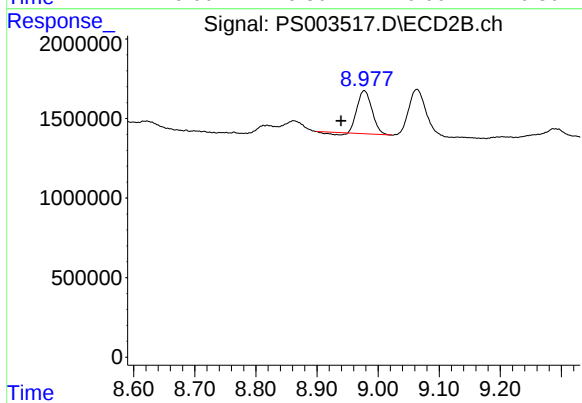

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.977 min
Delta R.T.: 0.038 min
Response: 4445395
Conc: 7.20 ng/ml

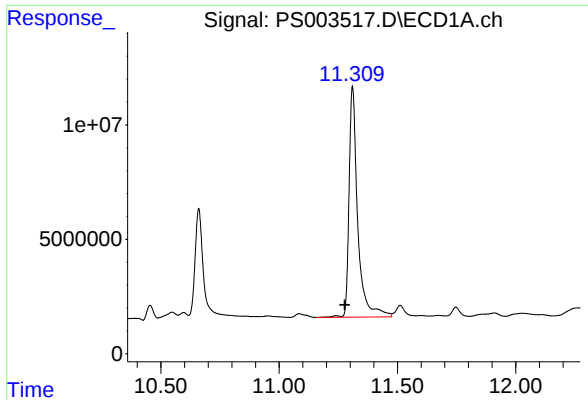

#4 2,4-DCAA


R.T.: 11.310 min
Delta R.T.: 0.033 min
Response: 257721882
Conc: 587.03 ng/ml

Instrument :
ECD_S
ClientSampleId :
CL-02-030819-A

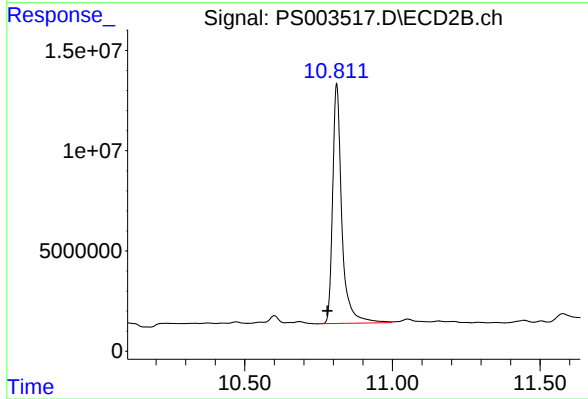


#4 2,4-DCAA

R.T.: 10.811 min
Delta R.T.: 0.031 min
Response: 259031580
Conc: 551.64 ng/ml

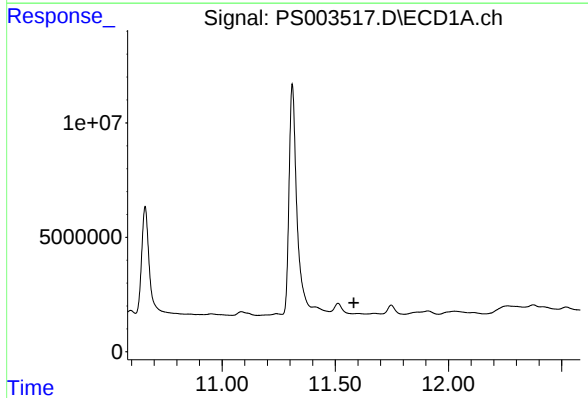


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.582 min
Response: 0
Conc: N.D.

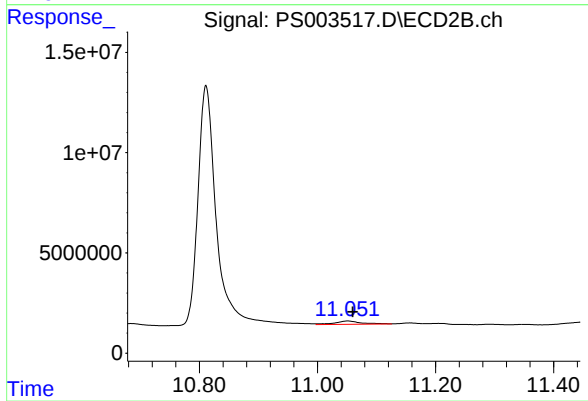

#5 DICAMBA


R.T.: 11.051 min
Delta R.T.: -0.008 min
Response: 4958147
Conc: 2.97 ng/ml

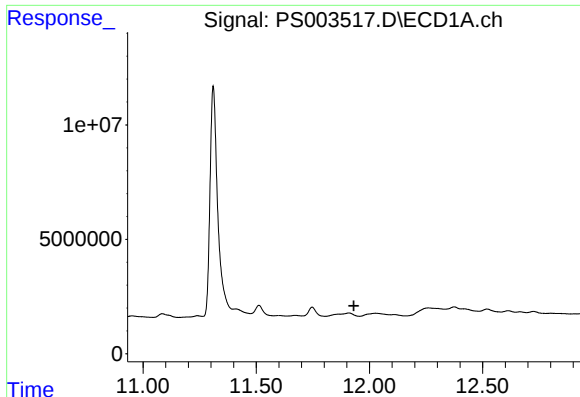

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.931 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-02-030819-A

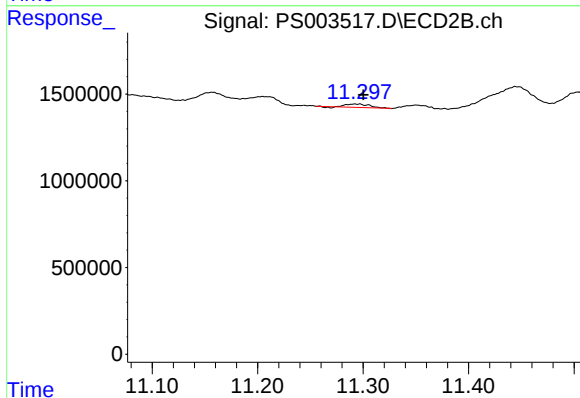


#6 MCP

R.T.: 11.293 min
Delta R.T.: -0.007 min
Response: 249497
Conc: 0.21 ug/ml

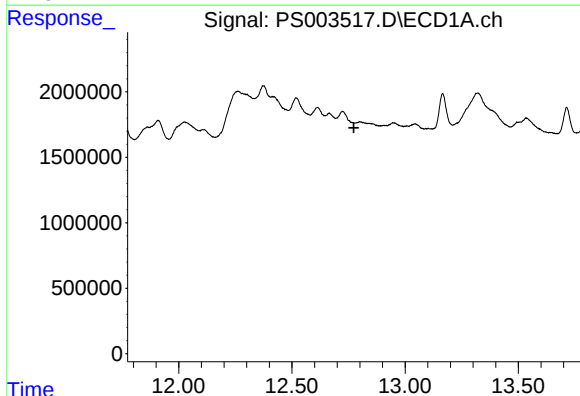


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 12.773 min
Response: 0
Conc: N.D.

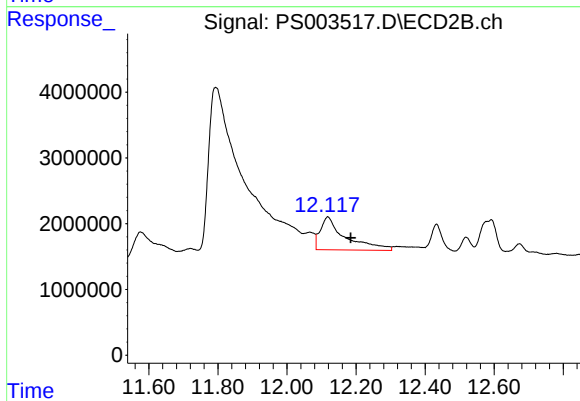

#8 DICHLORPROP


R.T.: 12.118 min
Delta R.T.: -0.067 min
Response: 25161031
Conc: 60.89 ng/ml

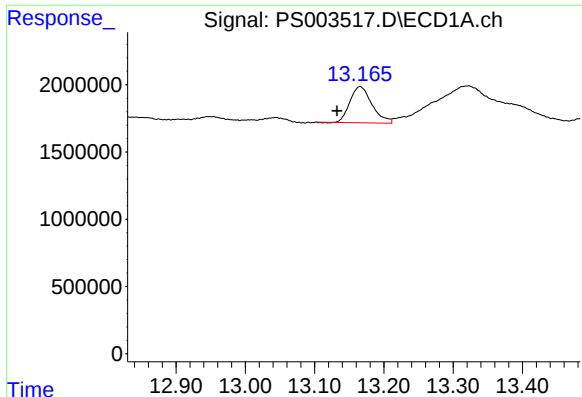

#9 2,4-D


R.T.: 13.166 min
Delta R.T.: 0.033 min
Response: 5924266
Conc: 12.77 ng/ml

Instrument :
ECD_S
ClientSampleId :
CL-02-030819-A

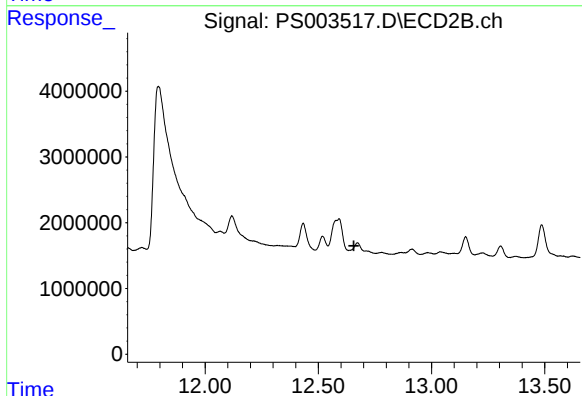


#9 2,4-D

R.T.: 12.673 min
Delta R.T.: 0.016 min
Response: -6145519
Conc: N.D.

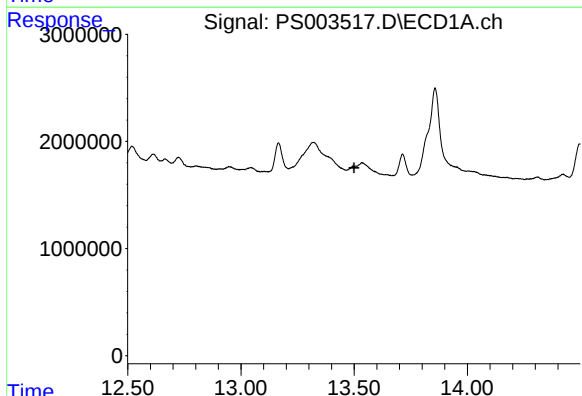


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.499 min
Response: 0
Conc: N.D.

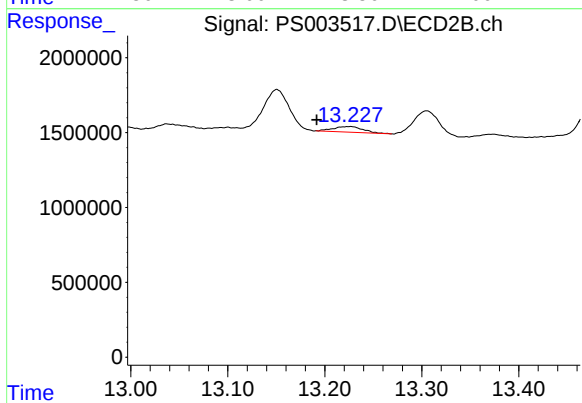

#10 Pentachlorophenol


R.T.: 13.225 min
Delta R.T.: 0.033 min
Response: 784149
Conc: 0.12 ng/ml

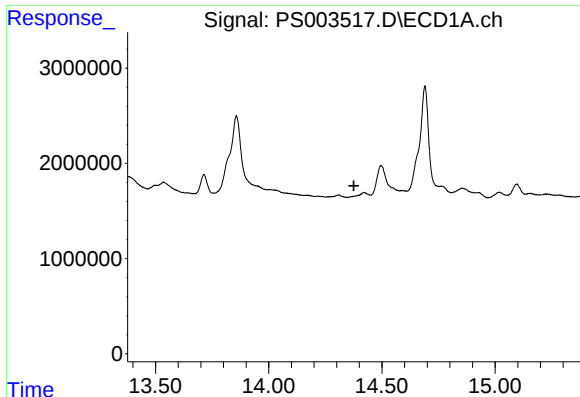

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-02-030819-A

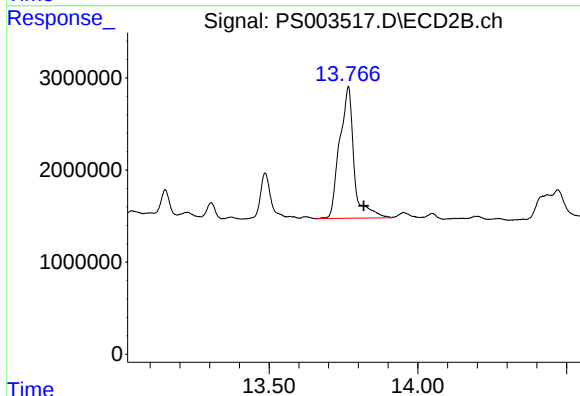


#11 2,4,5-TP (SILVEX)

R.T.: 13.766 min
Delta R.T.: -0.052 min
Response: 48255819
Conc: 18.95 ng/ml

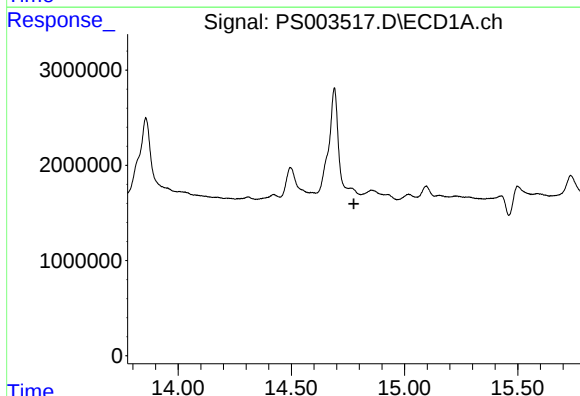


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

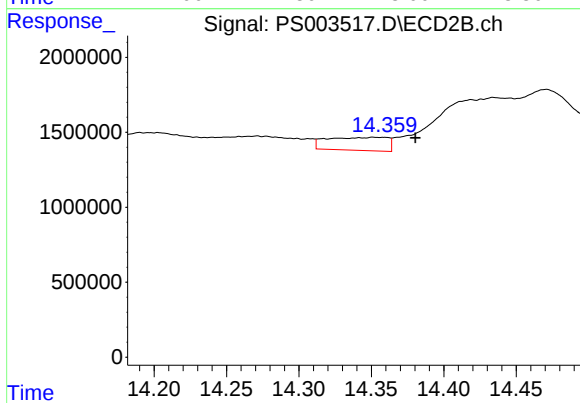

#12 2,4,5-T


R.T.: 14.354 min
Delta R.T.: -0.026 min
Response: 2528983
Conc: 1.25 ng/ml

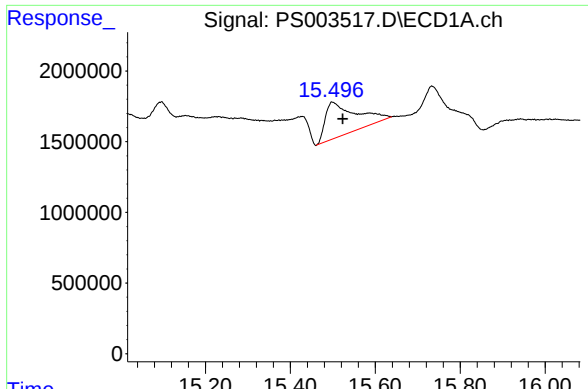

#13 2,4-DB


R.T.: 15.501 min
Delta R.T.: -0.022 min
Response: 12309220
Conc: 51.98 ng/ml

Instrument :
ECD_S
ClientSampleId :
CL-02-030819-A

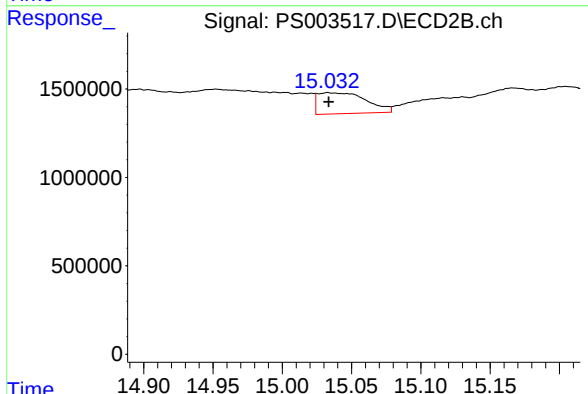


#13 2,4-DB

R.T.: 15.034 min
Delta R.T.: 0.000 min
Response: 2892350
Conc: 11.33 ng/ml

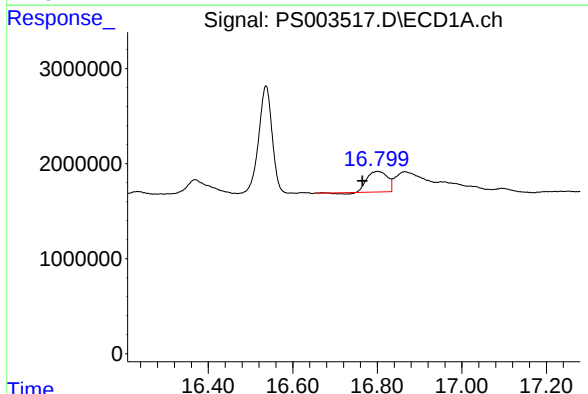


#15 Picloram

R.T.: 16.800 min
Delta R.T.: 0.035 min
Response: 6988195
Conc: 2.84 ng/ml

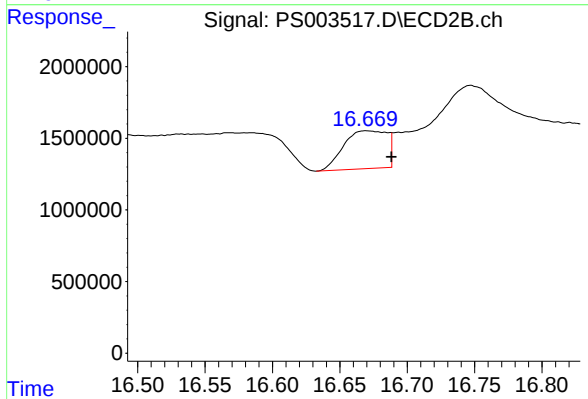

#15 Picloram


R.T.: 16.670 min
Delta R.T.: -0.018 min
Response: 5908107
Conc: 2.33 ng/ml

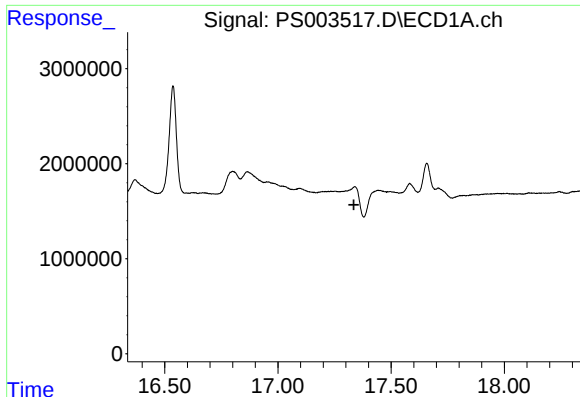

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.335 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-02-030819-A

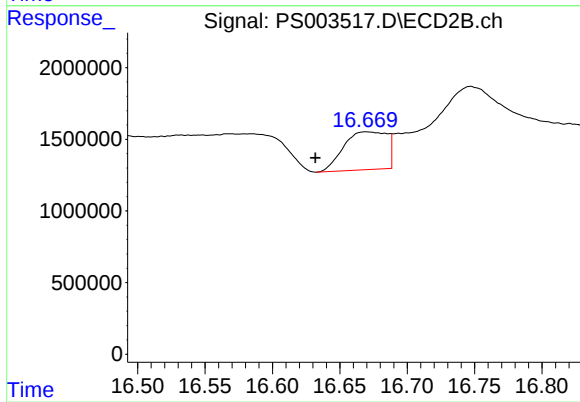

#16 DCPA

R.T.: 16.670 min
Delta R.T.: 0.038 min
Response: 5908107
Conc: 1.90 ng/ml