

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031219\
 Data File : PS003519.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2019 15:16
 Operator : EI\SJ
 Sample : K1691-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CL-02-030819-C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 04:40:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.293	10.794	259.4E6	261.2E6	590.767	556.269
Target Compounds							
1) T	Dalapon	2.813	2.307	54009404	120.5E6	83.099	190.238 #
2) T	3,5-DICHL...	0.000	8.960	0	4510154	N.D.	7.304 #
5) T	DICAMBA	0.000	11.034	0	4156986	N.D.	2.488 #
6) T	MCP	0.000	11.276	0	393571	N.D.	0.333 #
7) T	MCPA	12.225	0.000	37185333	0	18.747	N.D. #
9) T	2,4-D	13.148	12.655	6202864	548440	13.374	1.045 #
11) T	2,4,5-TP ...	0.000	13.750	0	25215235	N.D.	9.902 #
12) T	2,4,5-T	0.000	14.396	0	8374295	N.D.	4.152 #
13) T	2,4-DB	15.485	0.000	10702602	0	45.198	N.D. #
14) T	DINOSEB	0.000	15.442	0	1301205	N.D.	0.729 #
15) T	Picloram	16.773	16.738	6344458	22005134	2.578	8.670 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031219\
Data File : PS003519.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2019 15:16
Operator : EI\SJ
Sample : K1691-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
CL-02-030819-C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 04:40:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

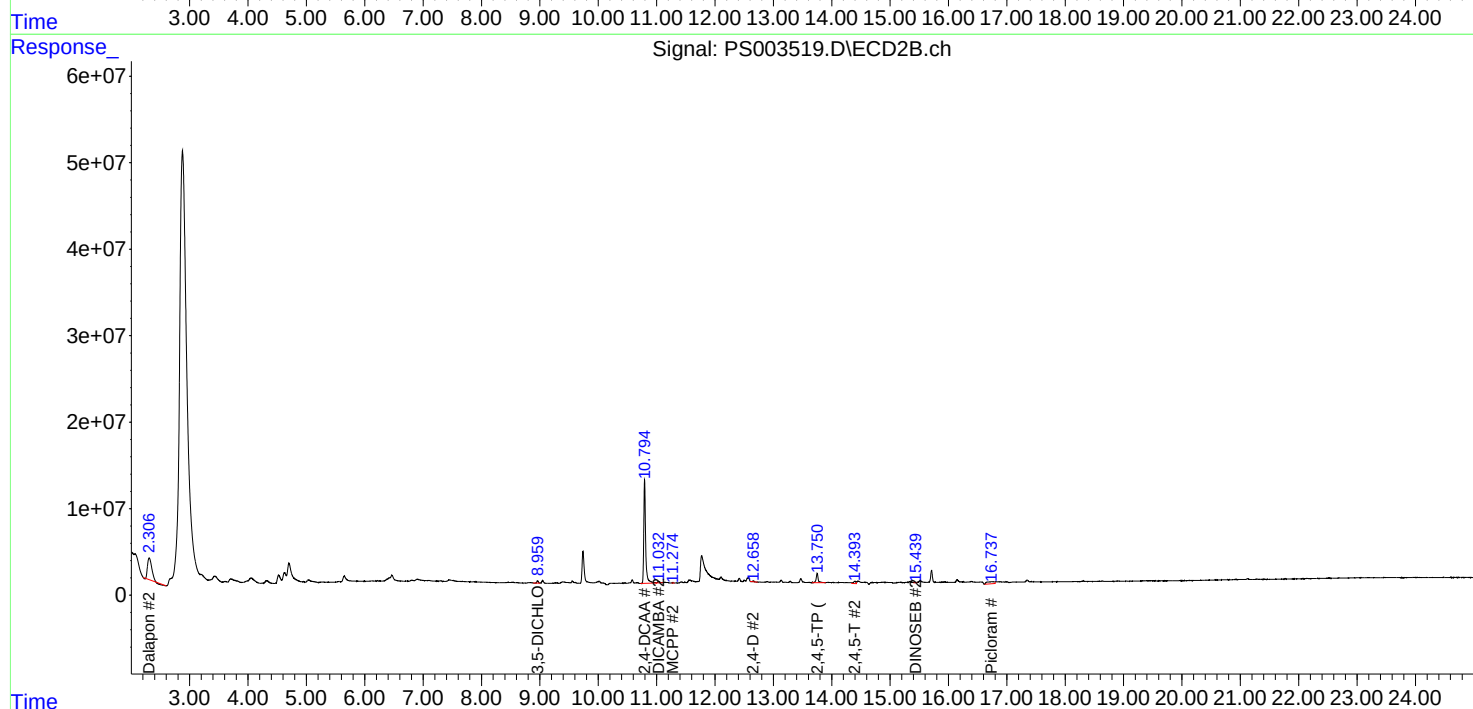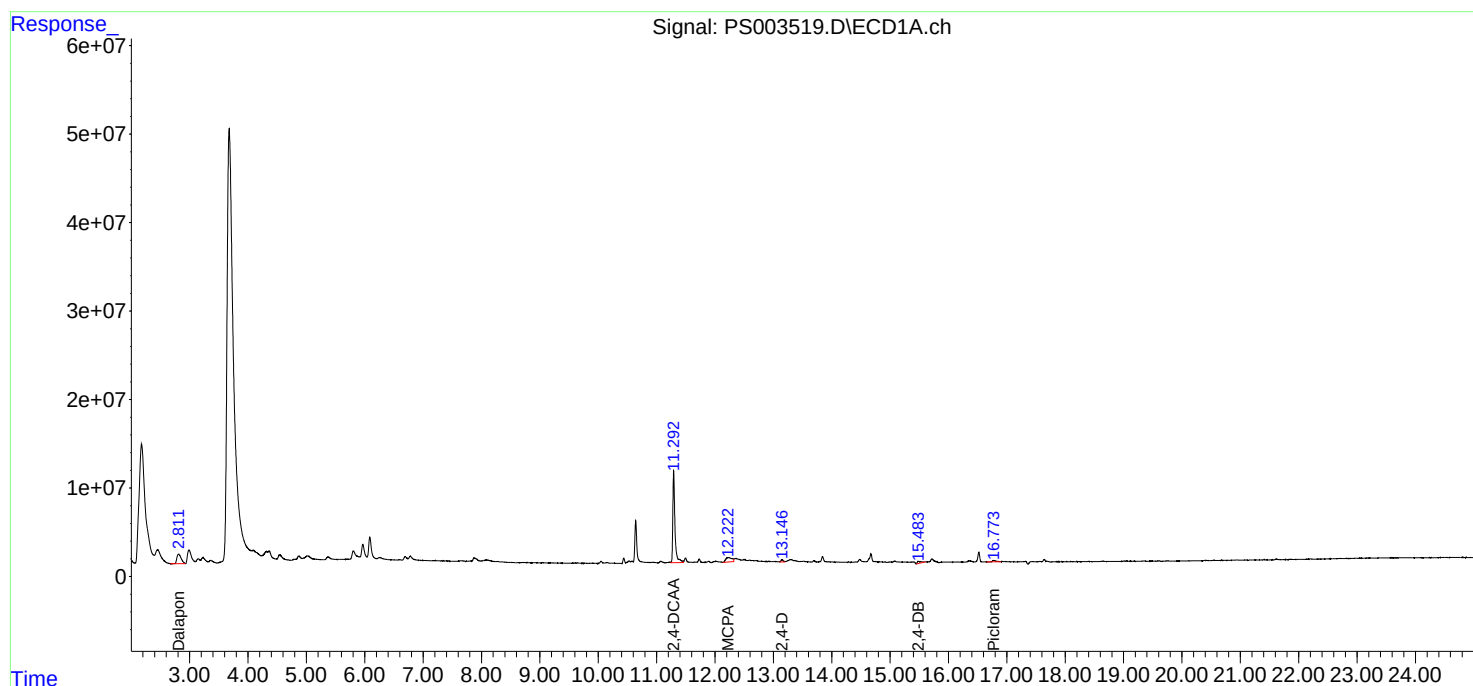


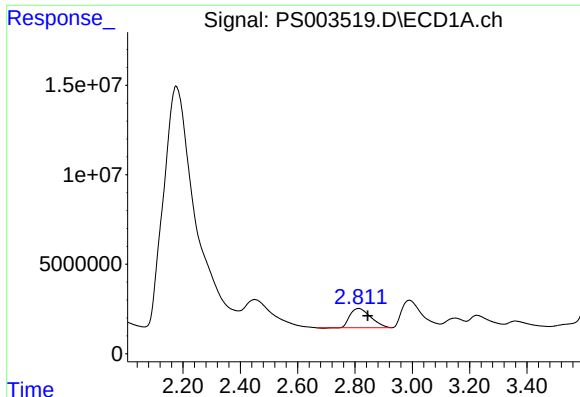

#1 Dalapon


R.T.: 2.813 min
Delta R.T.: -0.031 min
Response: 54009404
Conc: 83.10 ng/ml

Instrument :
ECD_S
ClientSampleId :
CL-02-030819-C

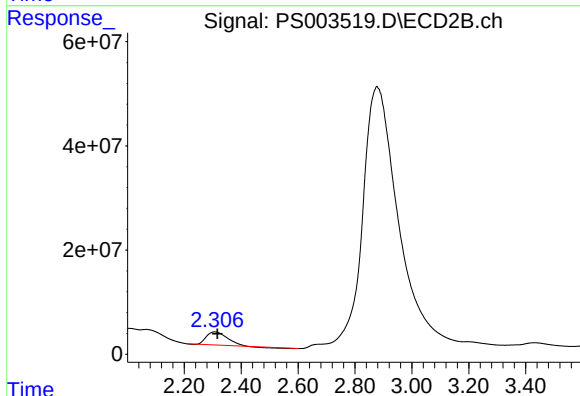


#1 Dalapon

R.T.: 2.307 min
Delta R.T.: -0.010 min
Response: 120455725
Conc: 190.24 ng/ml

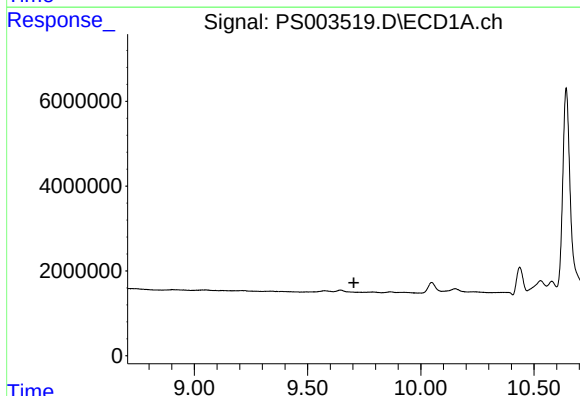


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.705 min
Response: 0
Conc: N.D.

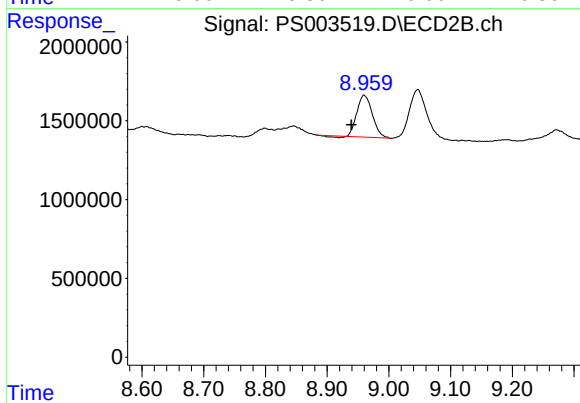

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.960 min
Delta R.T.: 0.021 min
Response: 4510154
Conc: 7.30 ng/ml

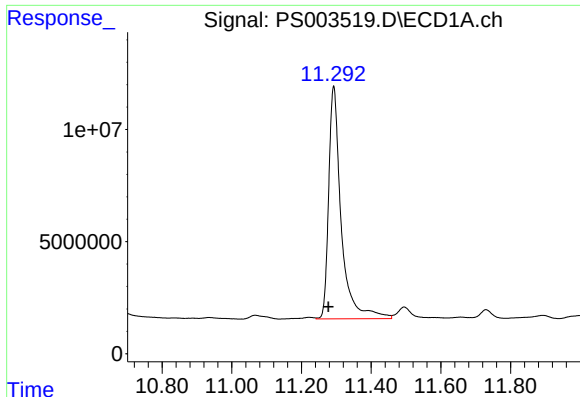

#4 2,4-DCAA


R.T.: 11.293 min
Delta R.T.: 0.015 min
Response: 259361296
Conc: 590.77 ng/ml

Instrument :
ECD_S
ClientSampleId :
CL-02-030819-C

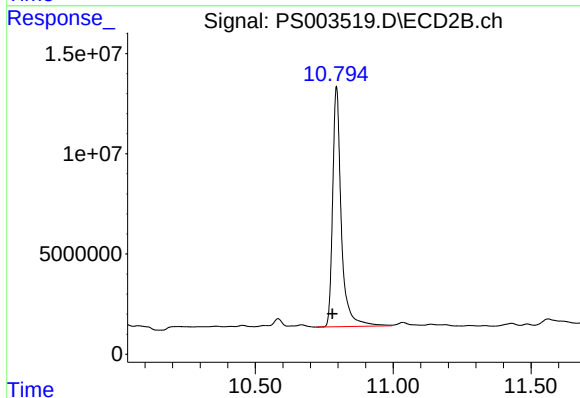


#4 2,4-DCAA

R.T.: 10.794 min
Delta R.T.: 0.015 min
Response: 261206940
Conc: 556.27 ng/ml

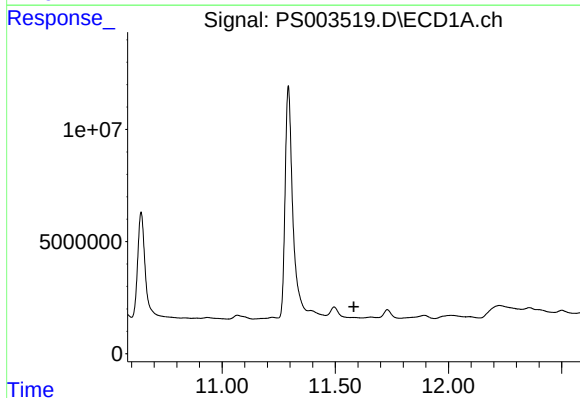


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.582 min
Response: 0
Conc: N.D.

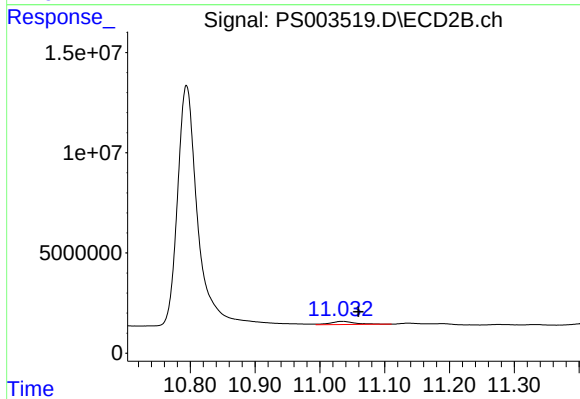

#5 DICAMBA


R.T.: 11.034 min
Delta R.T.: -0.025 min
Response: 4156986
Conc: 2.49 ng/ml

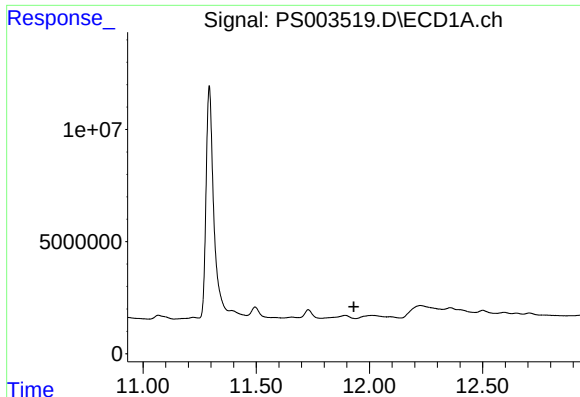

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 11.931 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-02-030819-C

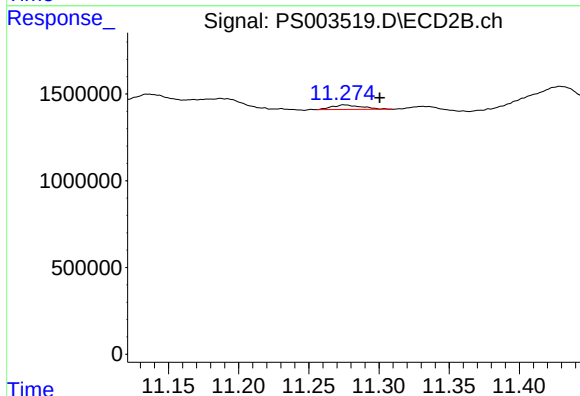


#6 MCPP

R.T.: 11.276 min
Delta R.T.: -0.024 min
Response: 393571
Conc: 0.33 ug/ml

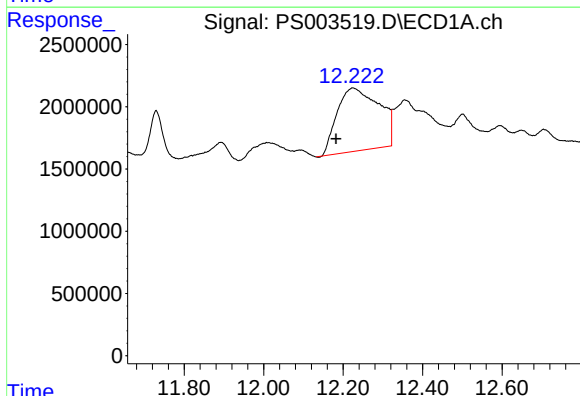


#7 MCPA

R.T.: 12.225 min
Delta R.T.: 0.043 min
Response: 37185333
Conc: 18.75 ug/ml

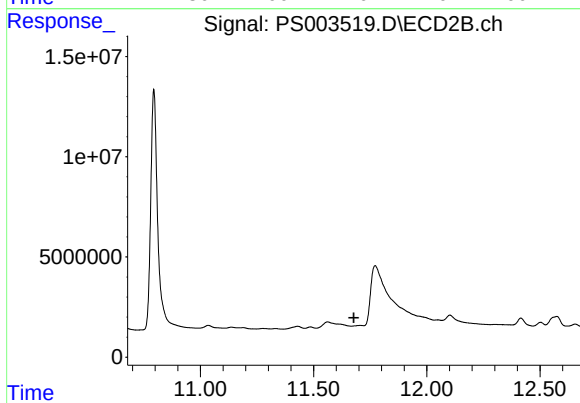

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 11.678 min
Response: 0
Conc: N.D.

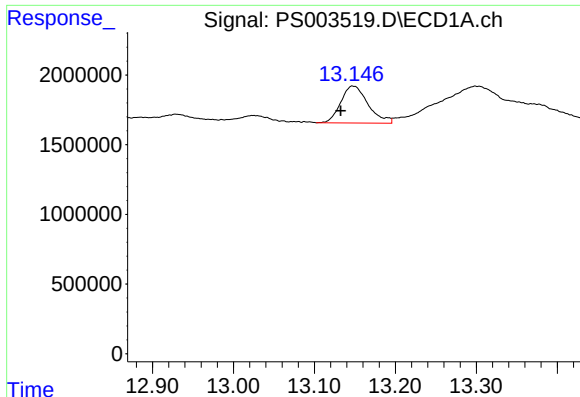

#9 2,4-D


R.T.: 13.148 min
Delta R.T.: 0.016 min
Response: 6202864
Conc: 13.37 ng/ml

Instrument :
ECD_S
ClientSampleId :
CL-02-030819-C

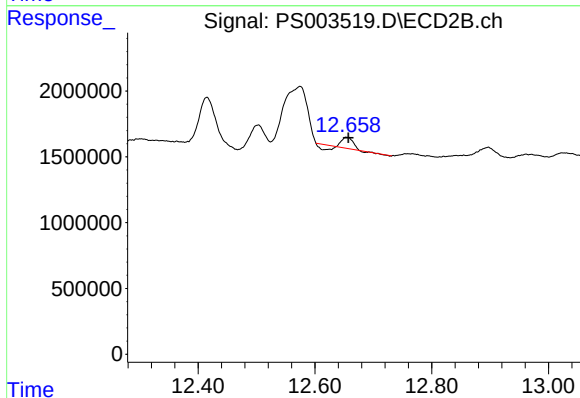


#9 2,4-D

R.T.: 12.655 min
Delta R.T.: -0.002 min
Response: 548440
Conc: 1.04 ng/ml

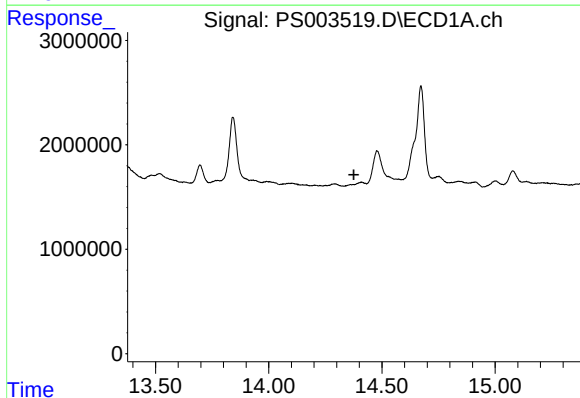


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.376 min
Response: 0
Conc: N.D.

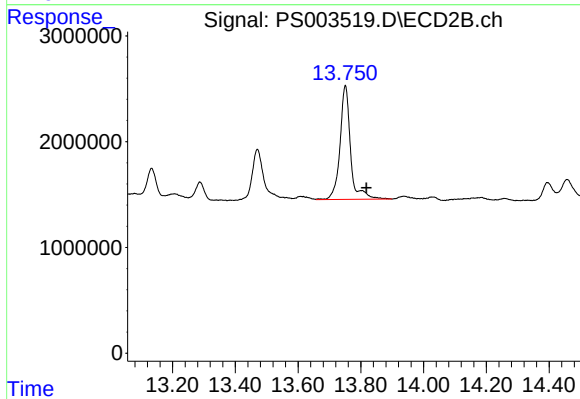

#11 2,4,5-TP (SILVEX)


R.T.: 13.750 min
Delta R.T.: -0.067 min
Response: 25215235
Conc: 9.90 ng/ml

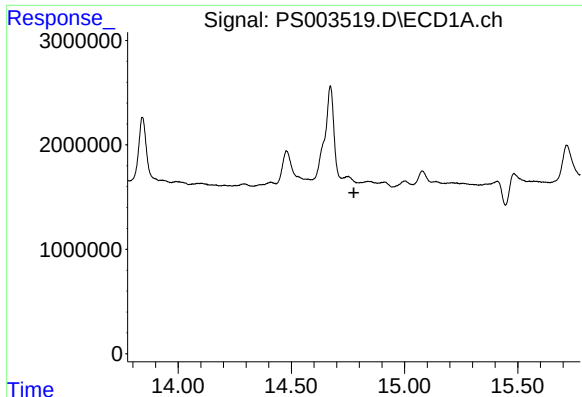

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-02-030819-C

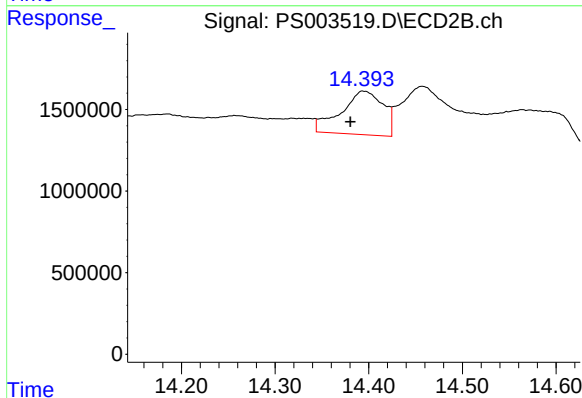


#12 2,4,5-T

R.T.: 14.396 min
Delta R.T.: 0.015 min
Response: 8374295
Conc: 4.15 ng/ml

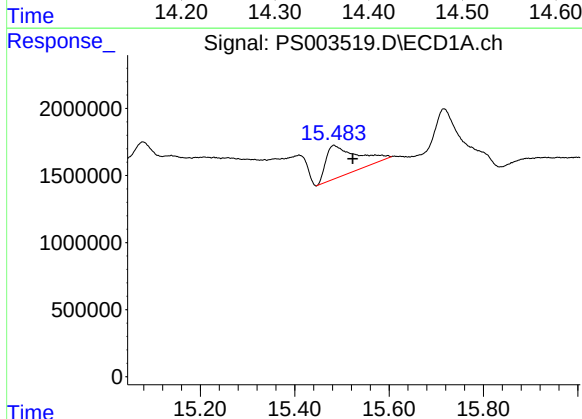


#13 2,4-DB

R.T.: 15.485 min
Delta R.T.: -0.038 min
Response: 10702602
Conc: 45.20 ng/ml

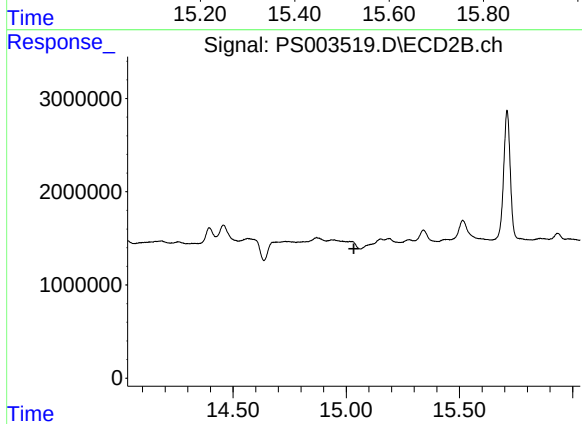

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.033 min
Response: 0
Conc: N.D.

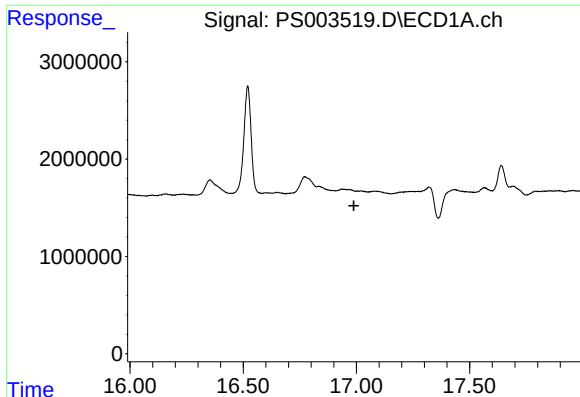

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-02-030819-C

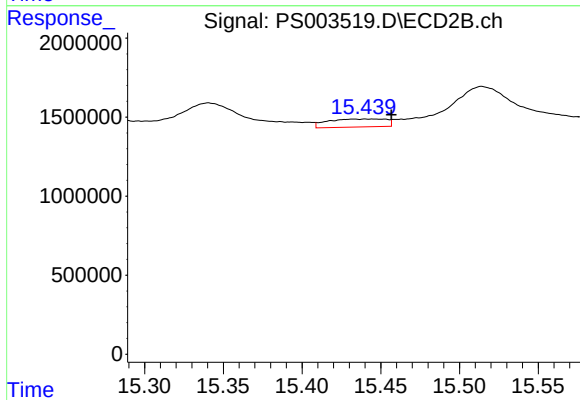


#14 DINOSEB

R.T.: 15.442 min
Delta R.T.: -0.014 min
Response: 1301205
Conc: 0.73 ng/ml

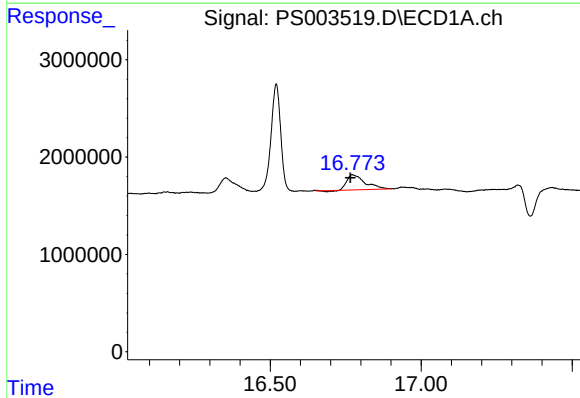

#15 Picloram

R.T.: 16.773 min
Delta R.T.: 0.008 min
Response: 6344458
Conc: 2.58 ng/ml

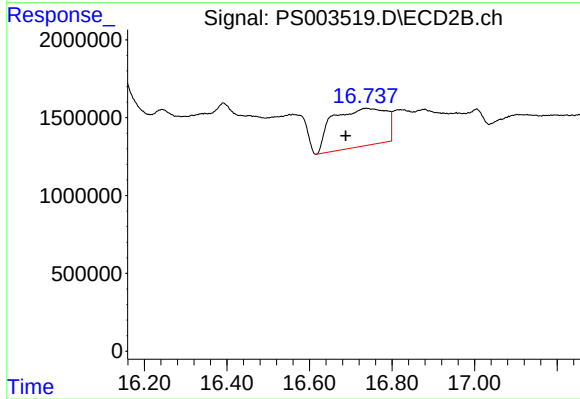

#15 Picloram

R.T.: 16.738 min
Delta R.T.: 0.050 min
Response: 22005134
Conc: 8.67 ng/ml