

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031219\
 Data File : PS003520.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2019 15:47
 Operator : EI\SJ
 Sample : K1691-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CL-02-030819-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 04:40:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.276	10.777	242.7E6	241.4E6	552.883	514.117
Target Compounds							
1) T	Dalapon	2.793	2.288	46470335	110.3E6	71.499	174.130 #
2) T	3,5-DICHL...	0.000	8.943	0	5375747	N.D.	8.706 #
3) T	4-Nitroph...	0.000	9.996	0	11356429	N.D.	50.512 #
5) T	DICAMBA	0.000	11.017	0	3976584	N.D.	2.380 #
6) T	MCPD	0.000	11.314	0	41307	N.D.	0.035 #
7) T	MCPA	12.216	11.689	31347110	-811843	15.803	N.D. #
9) T	2,4-D	13.131	12.638	5834016	2317336	12.578	4.415 #
12) T	2,4,5-T	0.000	14.379	0	7855792	N.D.	3.895 #
13) T	2,4-DB	15.467	0.000	9932472	0	41.945	N.D. #
14) T	DINOSEB	0.000	15.500	0	11430521	N.D.	6.404 #
15) T	Picloram	16.765	16.724	8667421	16332478	3.522	6.435 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031219\
Data File : PS003520.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2019 15:47
Operator : EI\SJ
Sample : K1691-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
CL-02-030819-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 04:40:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

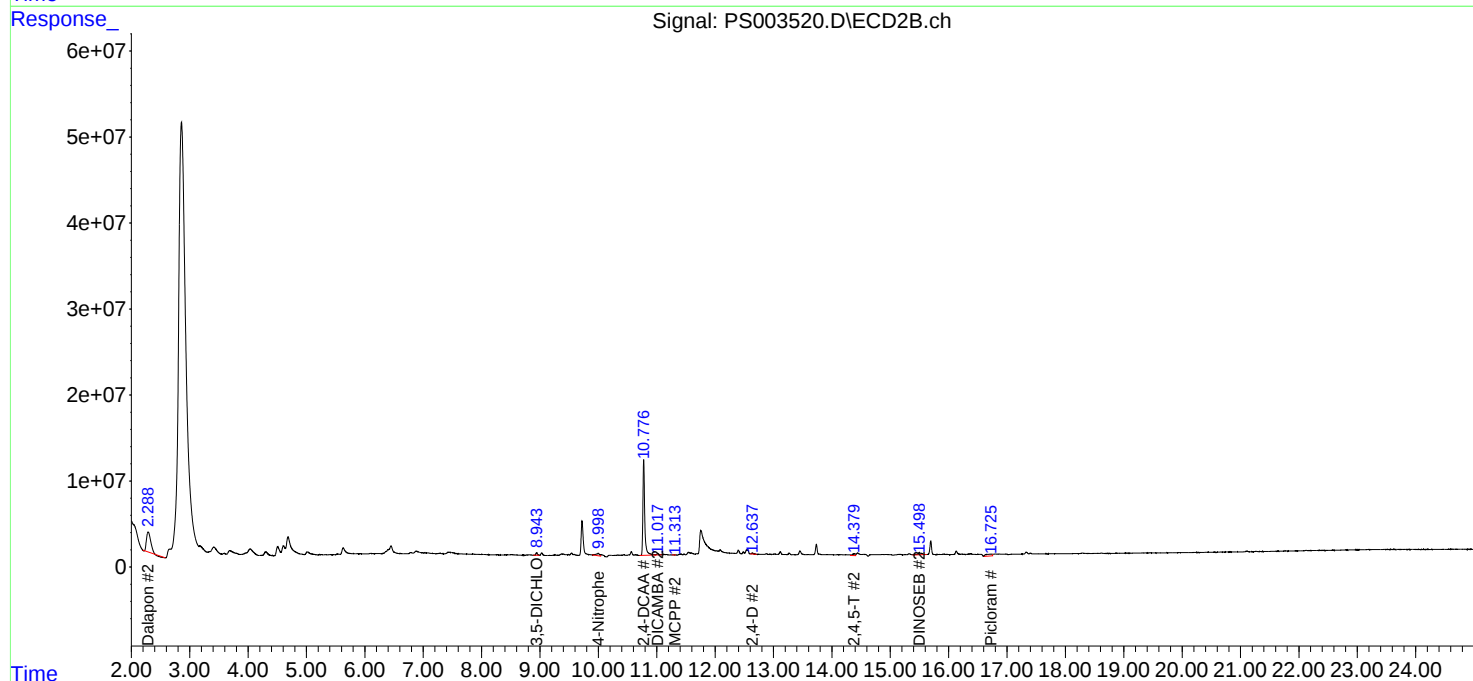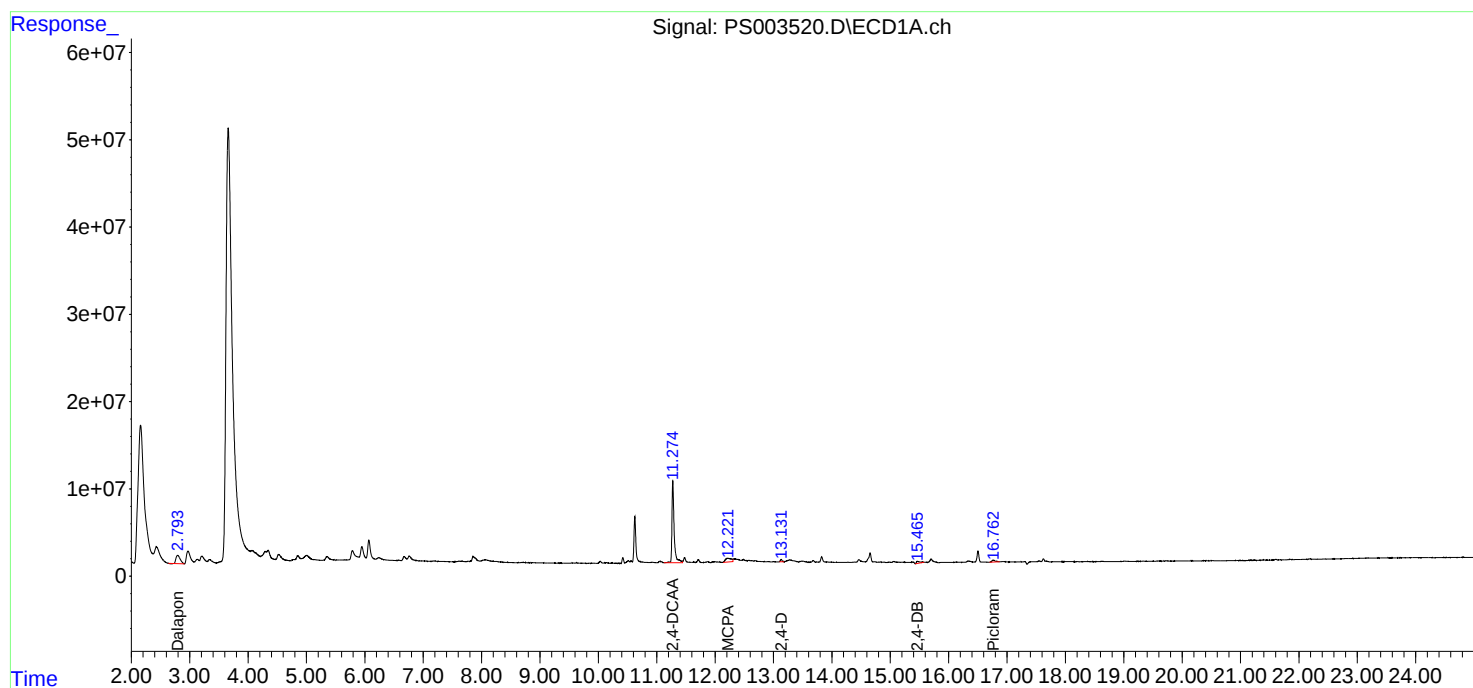


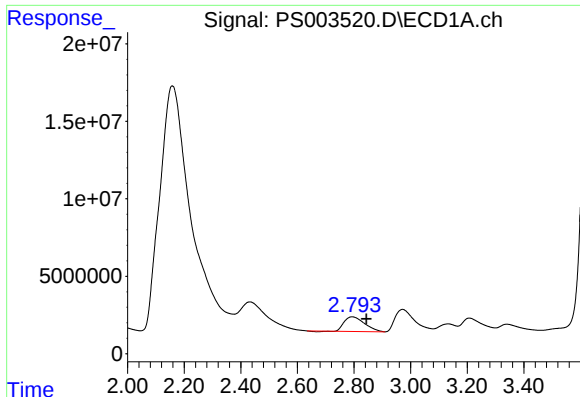

#1 Dalapon


R.T.: 2.793 min
Delta R.T.: -0.051 min
Response: 46470335
Conc: 71.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
CL-02-030819-D

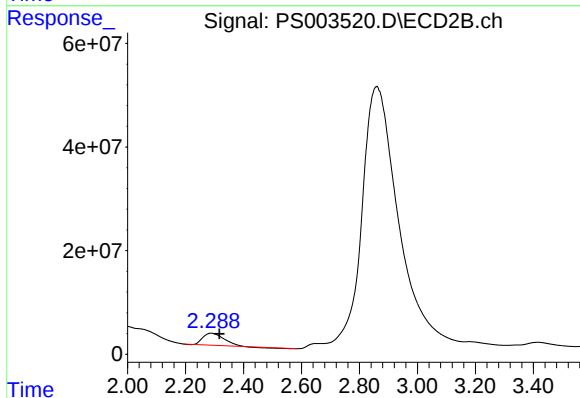


#1 Dalapon

R.T.: 2.288 min
Delta R.T.: -0.029 min
Response: 110256256
Conc: 174.13 ng/ml

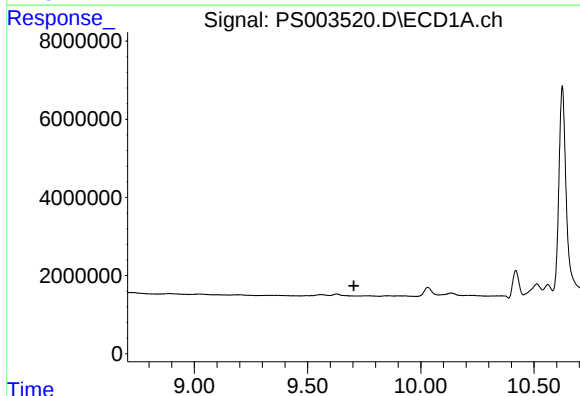


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.705 min
Response: 0
Conc: N.D.

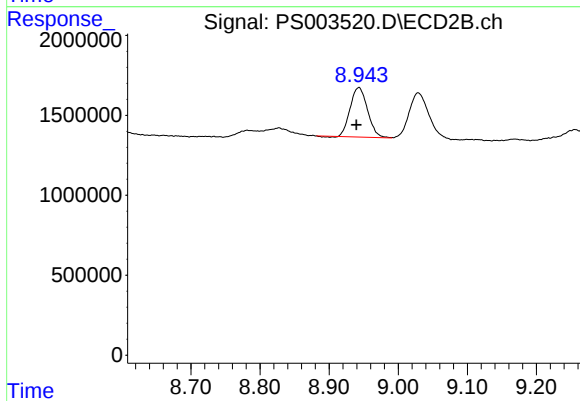

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.943 min
Delta R.T.: 0.004 min
Response: 5375747
Conc: 8.71 ng/ml

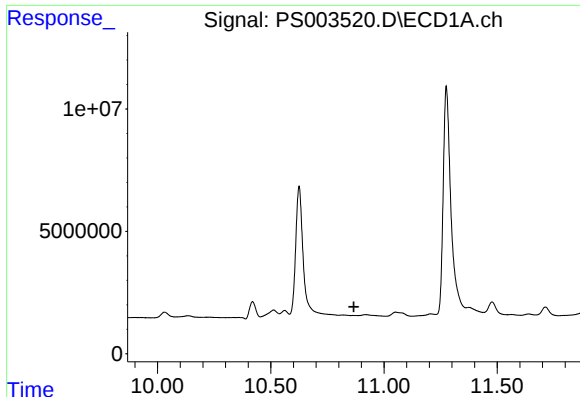

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-02-030819-D

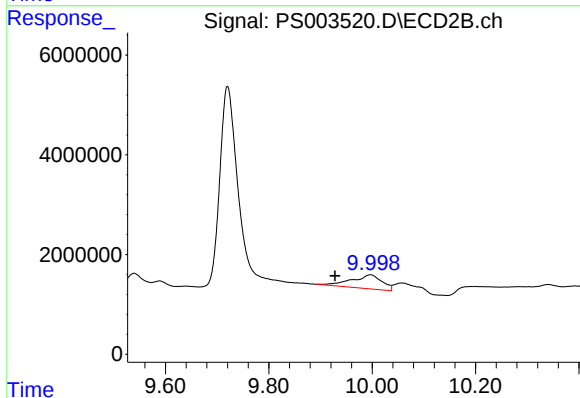


#3 4-Nitrophenol

R.T.: 9.996 min
Delta R.T.: 0.068 min
Response: 11356429
Conc: 50.51 ng/ml

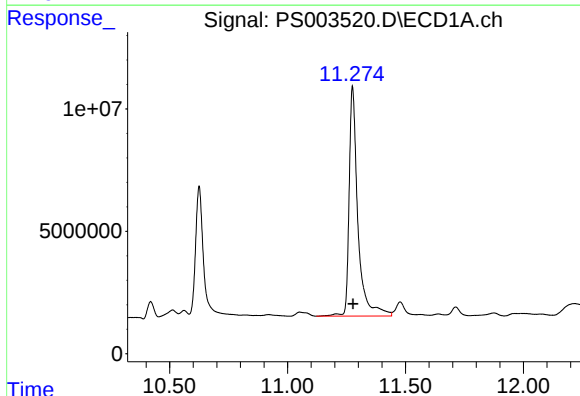


#4 2,4-DCAA

R.T.: 11.276 min
Delta R.T.: -0.002 min
Response: 242729050
Conc: 552.88 ng/ml

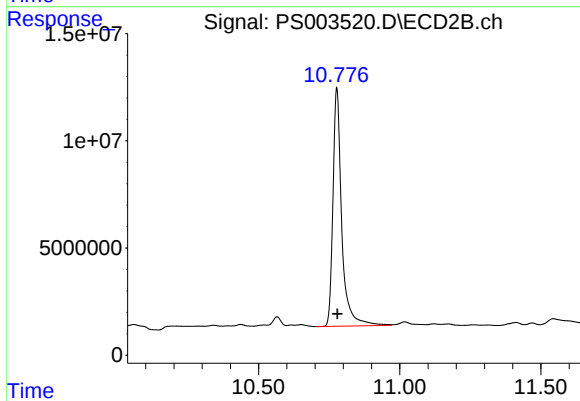

#4 2,4-DCAA


R.T.: 10.777 min
Delta R.T.: -0.003 min
Response: 241413473
Conc: 514.12 ng/ml

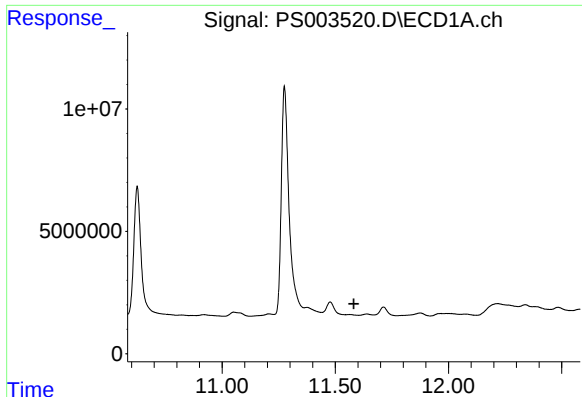

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.582 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-02-030819-D

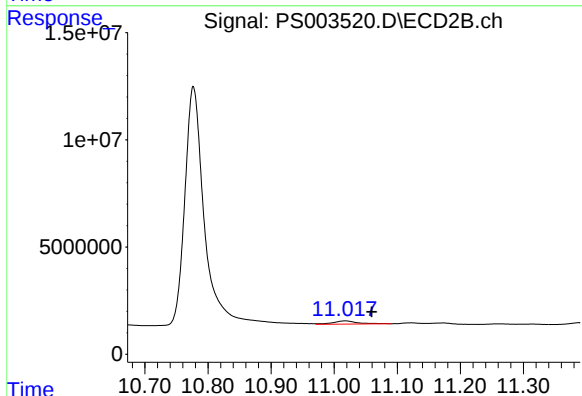


#5 DICAMBA

R.T.: 11.017 min
Delta R.T.: -0.042 min
Response: 3976584
Conc: 2.38 ng/ml

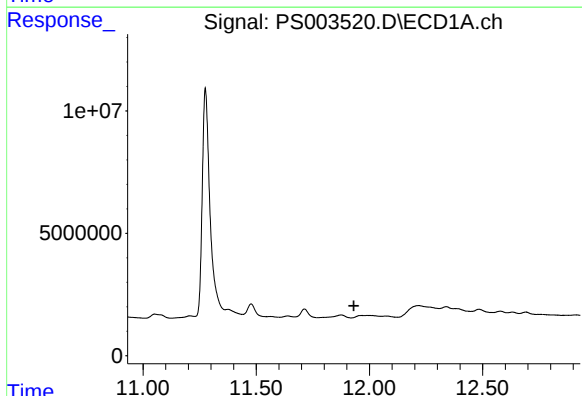


#6 MCP

R.T.: 0.000 min
Exp R.T.: 11.931 min
Response: 0
Conc: N.D.

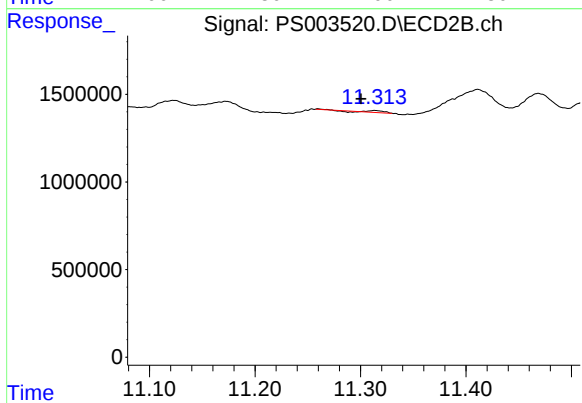

#6 MCP


R.T.: 11.314 min
Delta R.T.: 0.013 min
Response: 41307
Conc: 0.03 ug/ml

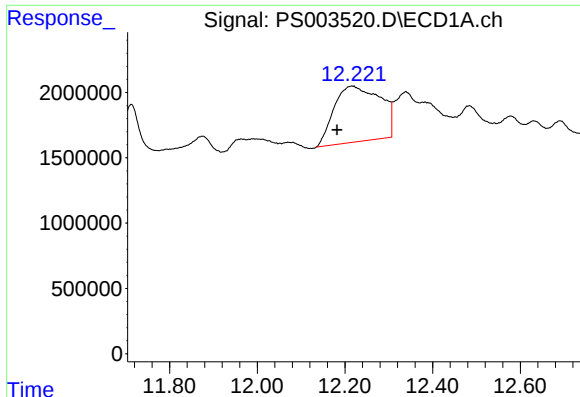

#7 MCPA


R.T.: 12.216 min
Delta R.T.: 0.034 min
Response: 31347110
Conc: 15.80 ug/ml

Instrument :
ECD_S
ClientSampleId :
CL-02-030819-D

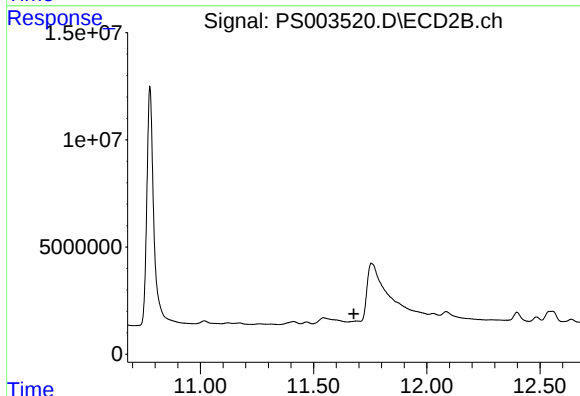


#7 MCPA

R.T.: 11.689 min
Delta R.T.: 0.011 min
Response: -811843
Conc: N.D.

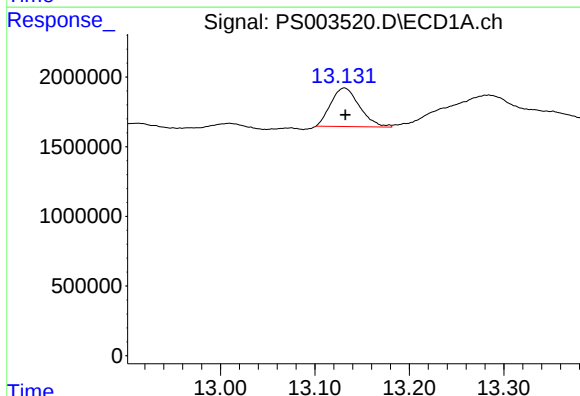


#9 2,4-D

R.T.: 13.131 min
Delta R.T.: -0.001 min
Response: 5834016
Conc: 12.58 ng/ml

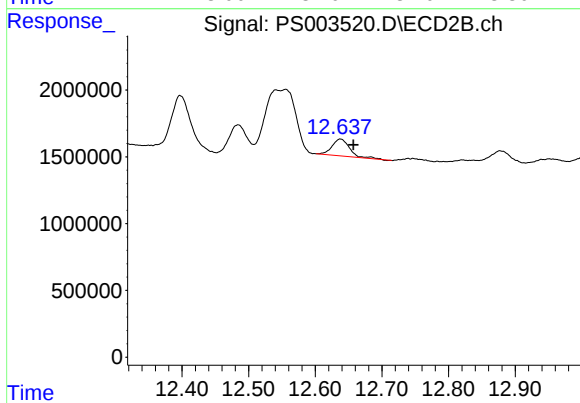

#9 2,4-D


R.T.: 12.638 min
Delta R.T.: -0.019 min
Response: 2317336
Conc: 4.41 ng/ml

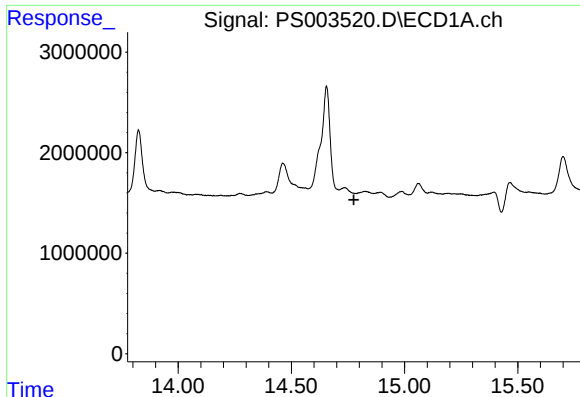

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-02-030819-D

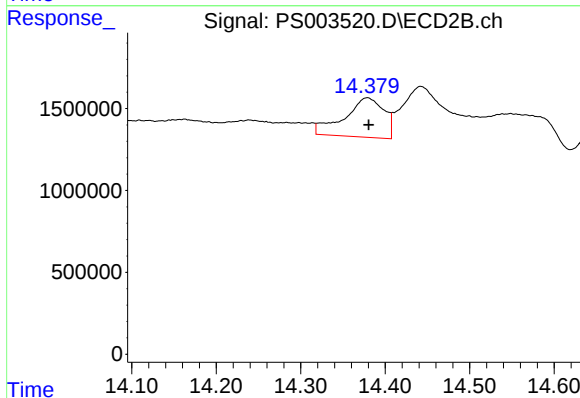


#12 2,4,5-T

R.T.: 14.379 min
Delta R.T.: -0.001 min
Response: 7855792
Conc: 3.90 ng/ml

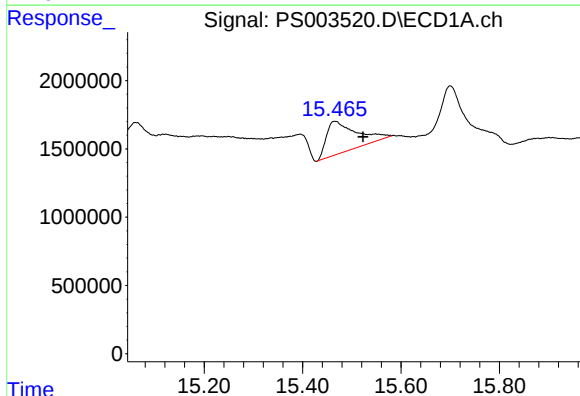


#13 2,4-DB

R.T.: 15.467 min
Delta R.T.: -0.056 min
Response: 9932472
Conc: 41.95 ng/ml

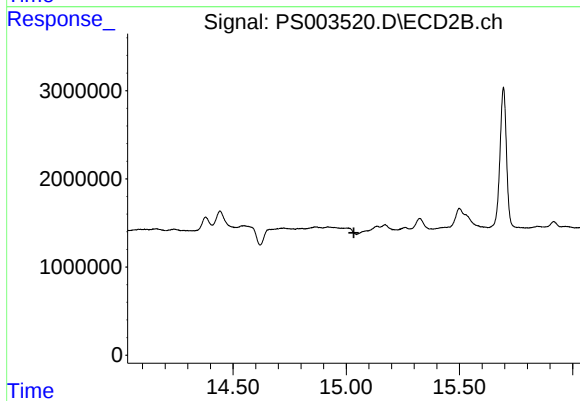

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.033 min
Response: 0
Conc: N.D.

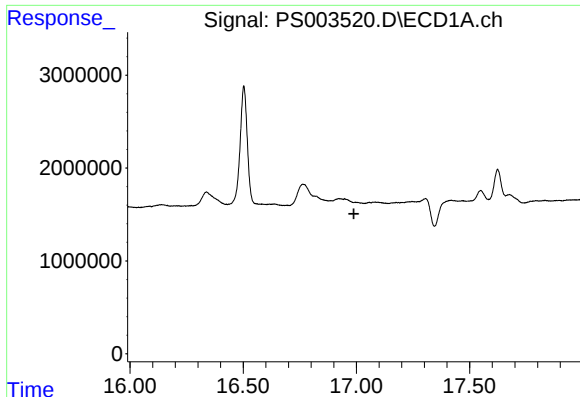

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-02-030819-D

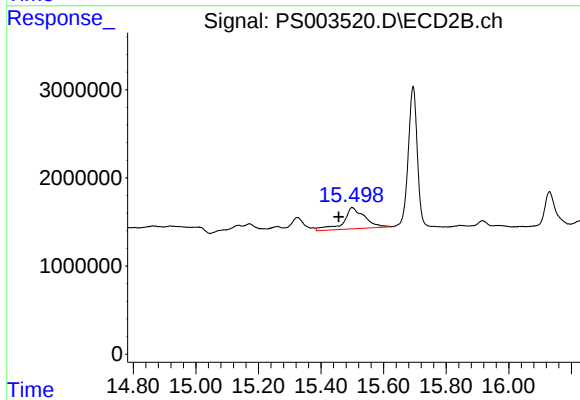


#14 DINOSEB

R.T.: 15.500 min
Delta R.T.: 0.043 min
Response: 11430521
Conc: 6.40 ng/ml

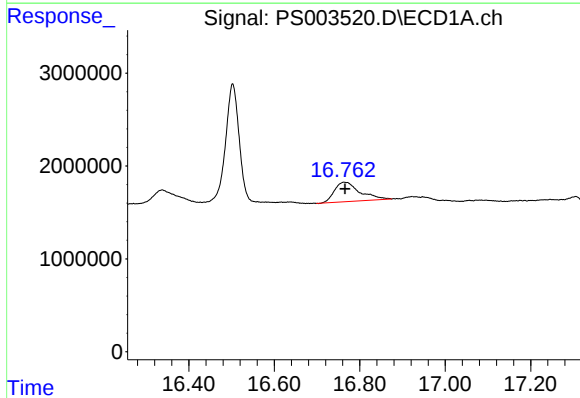

#15 Picloram

R.T.: 16.765 min
Delta R.T.: 0.000 min
Response: 8667421
Conc: 3.52 ng/ml

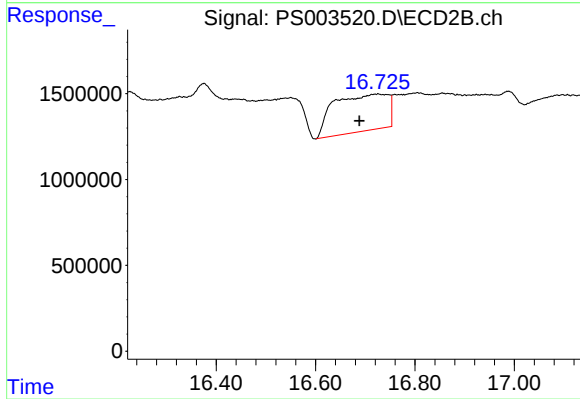

#15 Picloram

R.T.: 16.724 min
Delta R.T.: 0.036 min
Response: 16332478
Conc: 6.43 ng/ml