

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031219\
 Data File : PS003523.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2019 17:20
 Operator : EI\SJ
 Sample : K1835-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 04:41:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.295	10.796	302.4E6	299.2E6	688.751	637.091
Target Compounds							
1) T	Dalapon	2.812	2.309	52197024	152.6E6	80.310	241.066 #
2) T	3,5-DICHL...	0.000	8.963	0	2606308	N.D.	4.221 #
5) T	DICAMBA	0.000	11.037	0	4314849	N.D.	2.583 #
6) T	MCPD	0.000	11.279	0	274727	N.D.	0.233 #
7) T	MCPA	0.000	11.707	0	1120854	N.D.	0.650 #
9) T	2,4-D	13.151	12.658	7128242	-787213	15.369	N.D. #
11) T	2,4,5-TP ...	0.000	13.805	0	1625046	N.D.	0.638 #
12) T	2,4,5-T	0.000	14.398	0	9617710	N.D.	4.769 #
13) T	2,4-DB	15.489	15.030	15223568	3471663	64.290	13.595 #
14) T	DINOSEB	0.000	15.519	0	10926456	N.D.	6.122 #
15) T	Picloram	16.785	16.748	7489454	17631835	3.043	6.947 #
16) T	DCPA	0.000	16.572	0	10332300	N.D.	3.322 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031219\
Data File : PS003523.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2019 17:20
Operator : EI\SJ
Sample : K1835-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 04:41:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

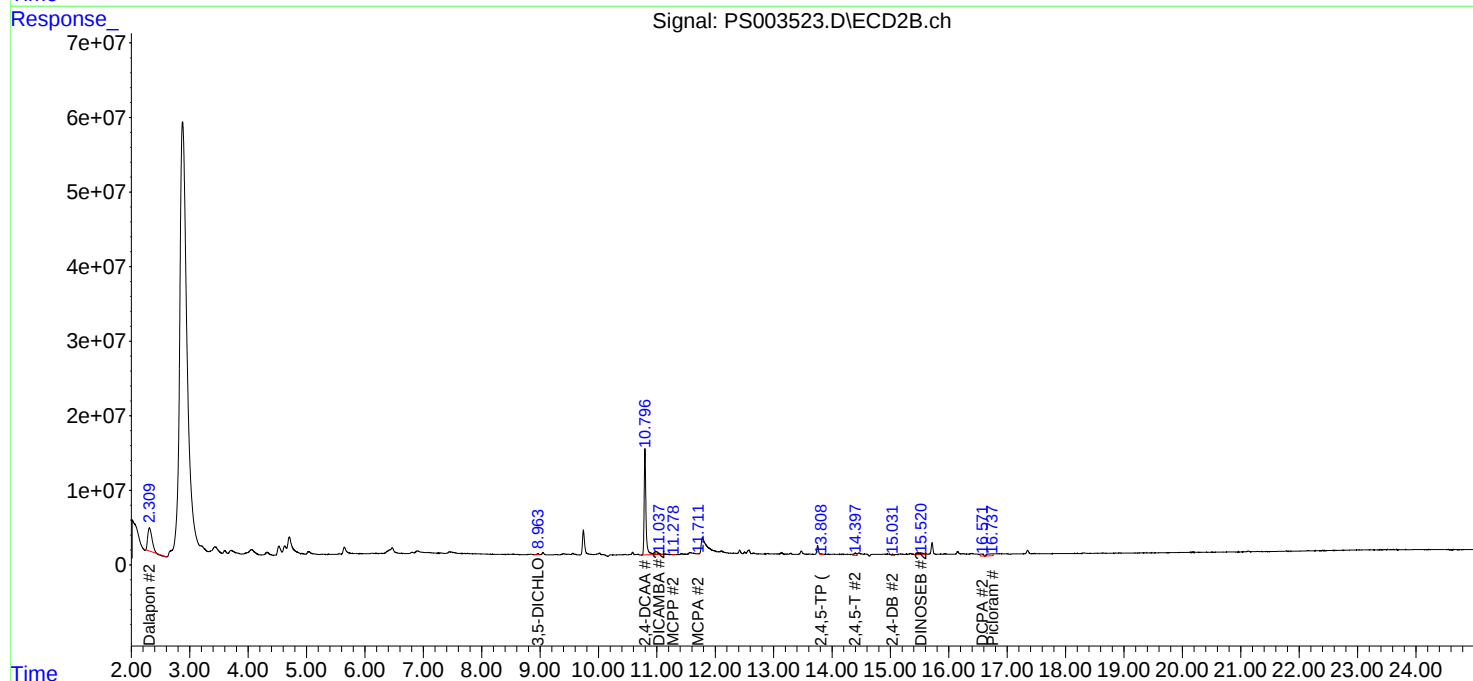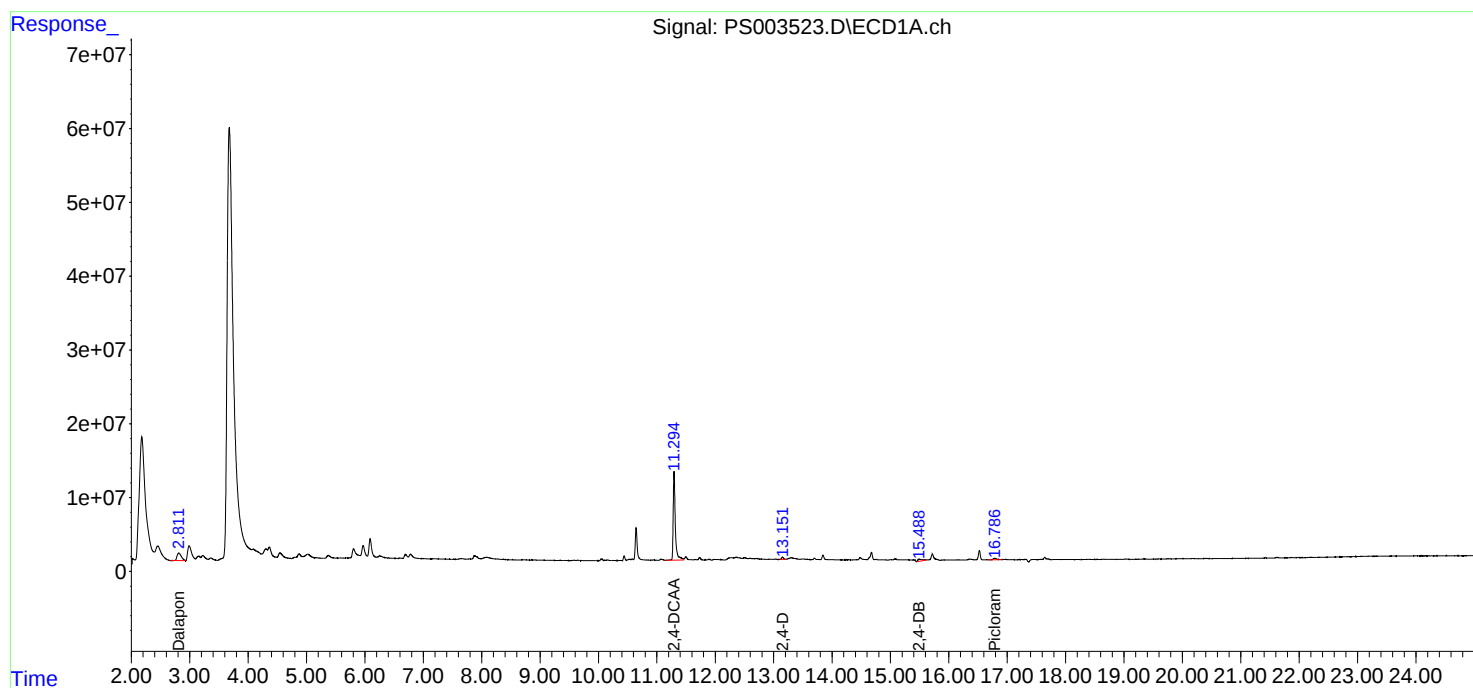


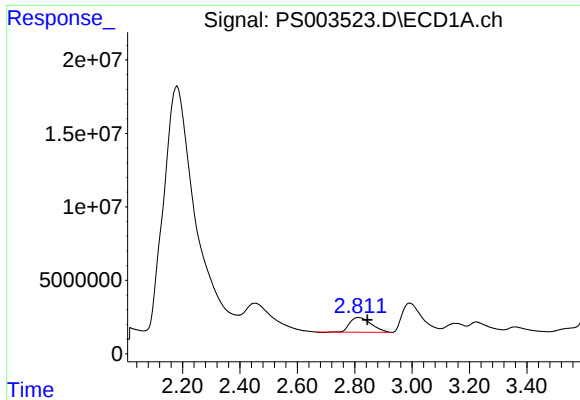

#1 Dalapon


R.T.: 2.812 min
Delta R.T.: -0.032 min
Response: 52197024
Conc: 80.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3

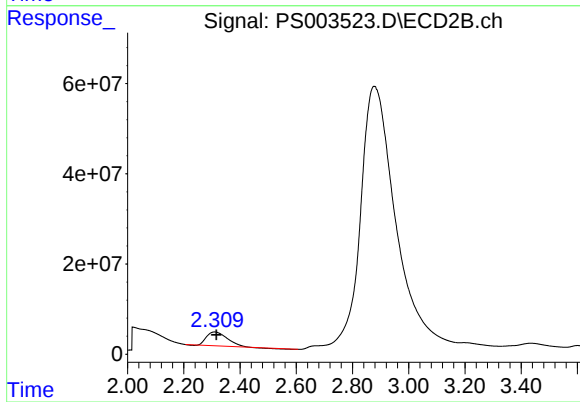


#1 Dalapon

R.T.: 2.309 min
Delta R.T.: -0.007 min
Response: 152639532
Conc: 241.07 ng/ml

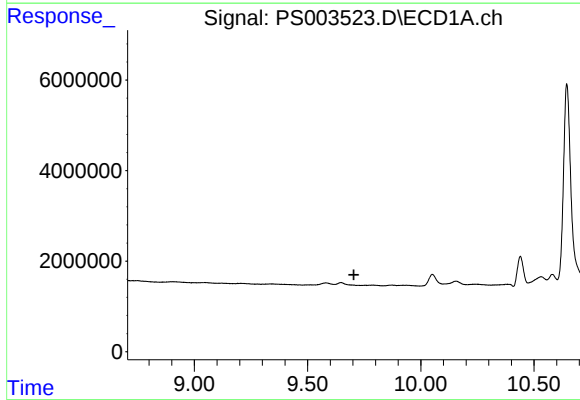


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.705 min
Response: 0
Conc: N.D.

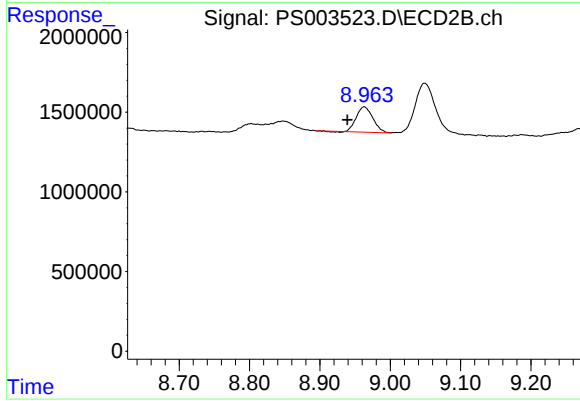

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.963 min
Delta R.T.: 0.024 min
Response: 2606308
Conc: 4.22 ng/ml

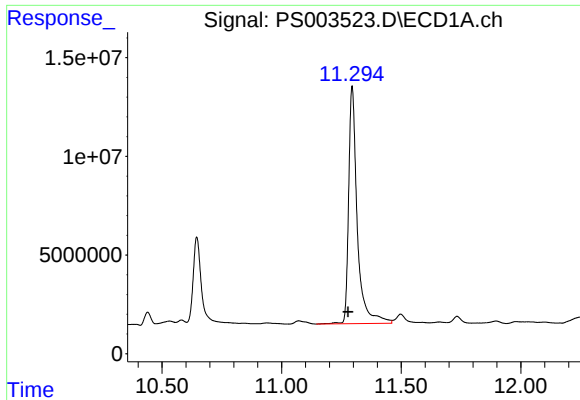

#4 2,4-DCAA


R.T.: 11.295 min
Delta R.T.: 0.017 min
Response: 302378674
Conc: 688.75 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3

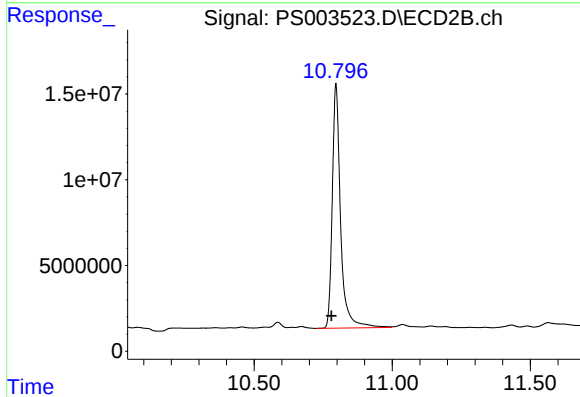


#4 2,4-DCAA

R.T.: 10.796 min
Delta R.T.: 0.016 min
Response: 299158360
Conc: 637.09 ng/ml

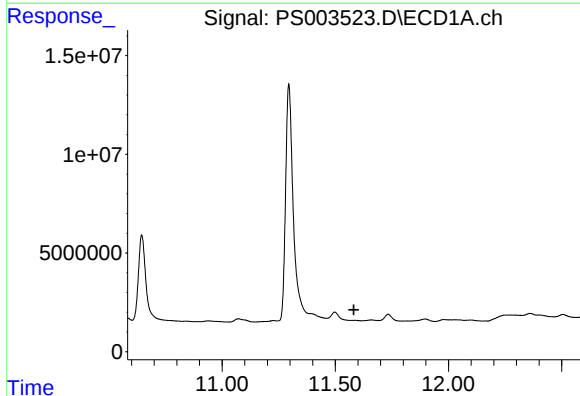


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.582 min
Response: 0
Conc: N.D.

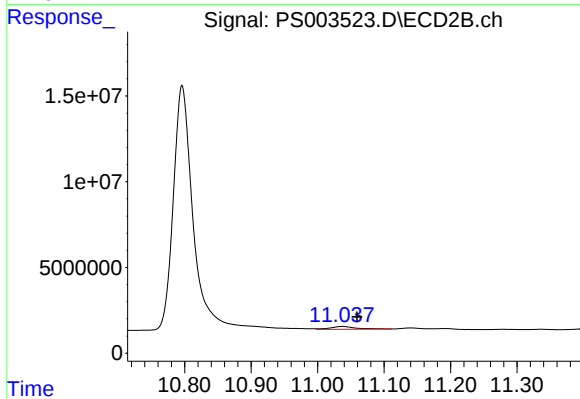

#5 DICAMBA


R.T.: 11.037 min
Delta R.T.: -0.022 min
Response: 4314849
Conc: 2.58 ng/ml

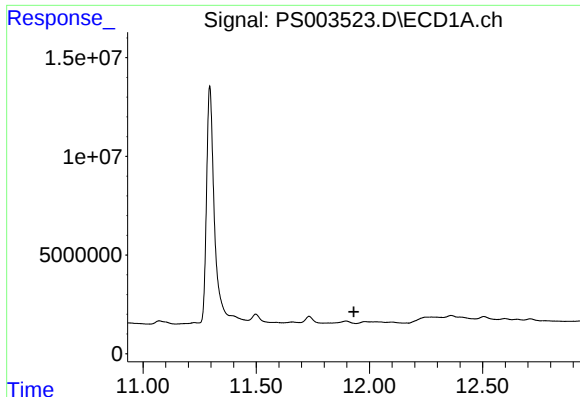

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 11.931 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-3

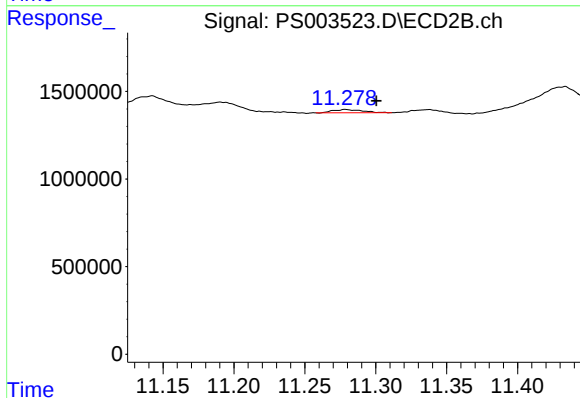


#6 MCPP

R.T.: 11.279 min
Delta R.T.: -0.021 min
Response: 274727
Conc: 0.23 ug/ml

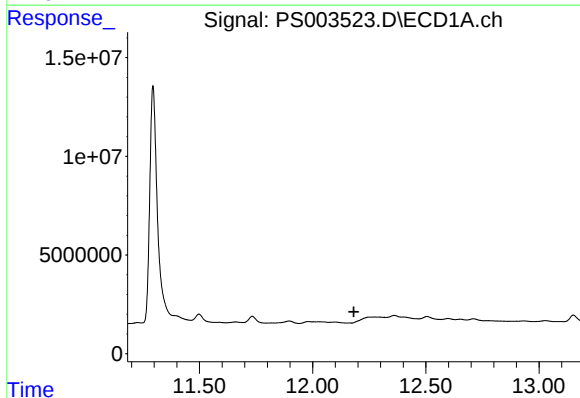


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 12.182 min
Response: 0
Conc: N.D.

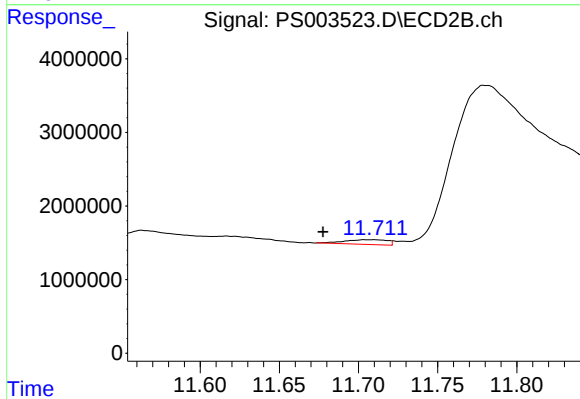

#7 MCPA


R.T.: 11.707 min
Delta R.T.: 0.030 min
Response: 1120854
Conc: 0.65 ug/ml

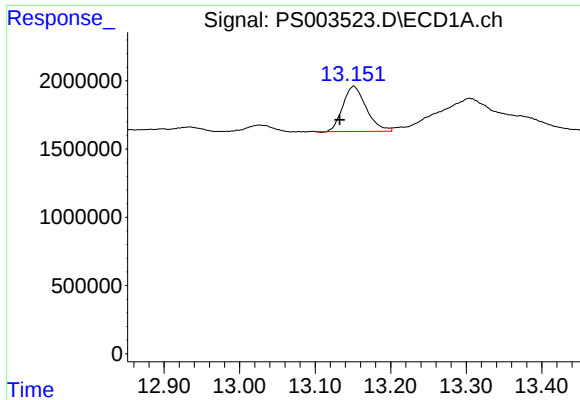

#9 2,4-D


R.T.: 13.151 min
Delta R.T.: 0.019 min
Response: 7128242
Conc: 15.37 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3

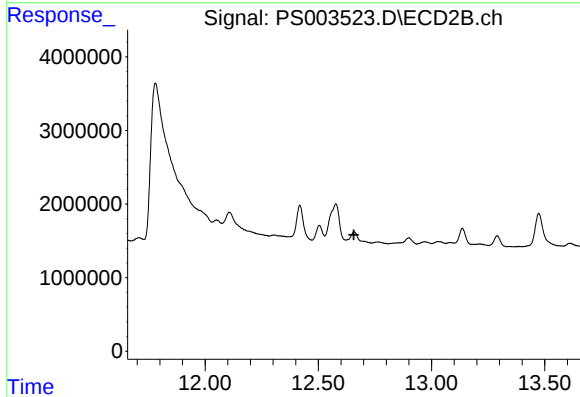


#9 2,4-D

R.T.: 12.658 min
Delta R.T.: 0.001 min
Response: -787213
Conc: N.D.

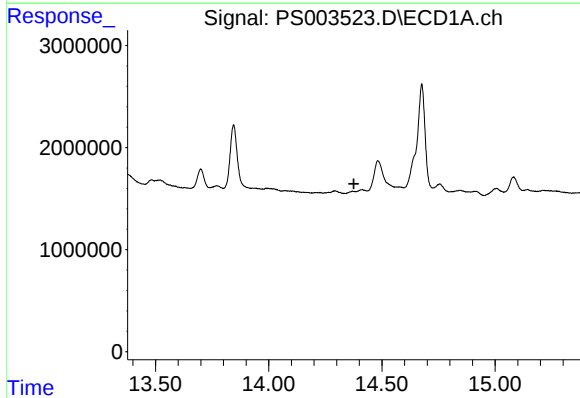


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.376 min
Response: 0
Conc: N.D.

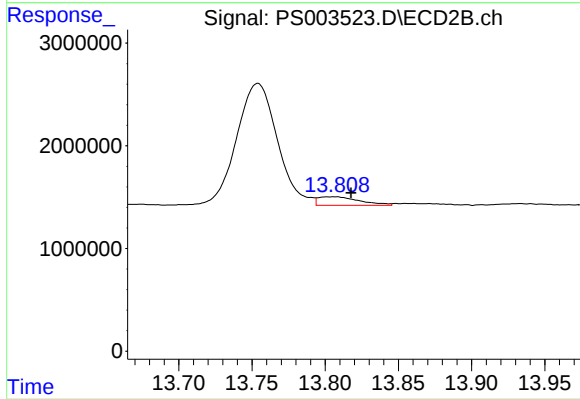

#11 2,4,5-TP (SILVEX)


R.T.: 13.805 min
Delta R.T.: -0.013 min
Response: 1625046
Conc: 0.64 ng/ml

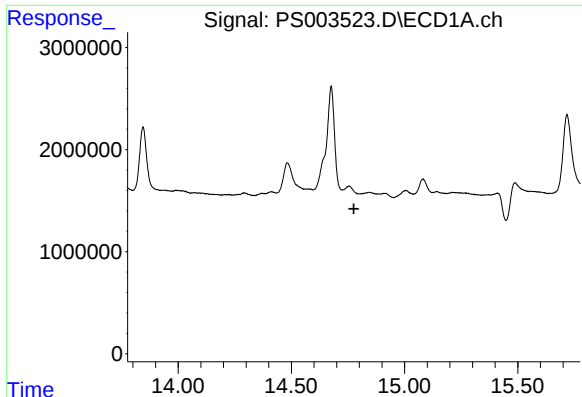

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-3

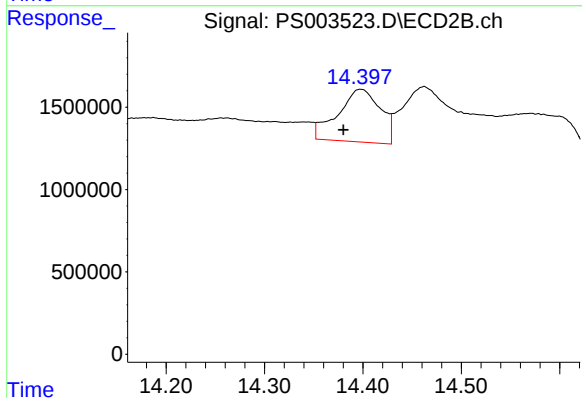


#12 2,4,5-T

R.T.: 14.398 min
Delta R.T.: 0.017 min
Response: 9617710
Conc: 4.77 ng/ml

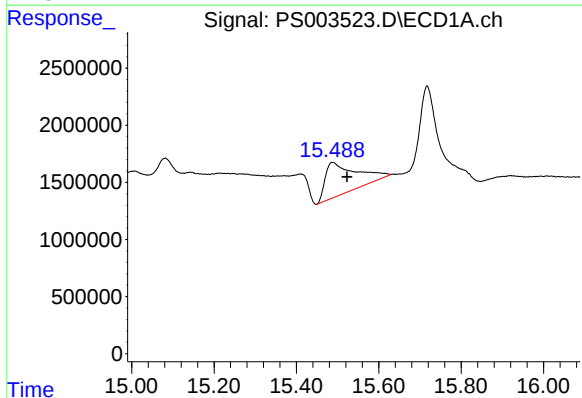


#13 2,4-DB

R.T.: 15.489 min
Delta R.T.: -0.034 min
Response: 15223568
Conc: 64.29 ng/ml

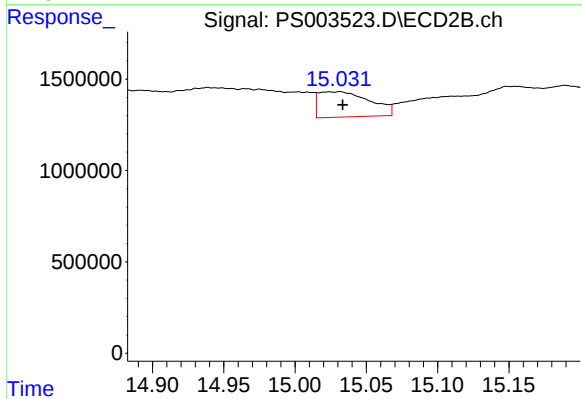

#13 2,4-DB


R.T.: 15.030 min
Delta R.T.: -0.004 min
Response: 3471663
Conc: 13.60 ng/ml

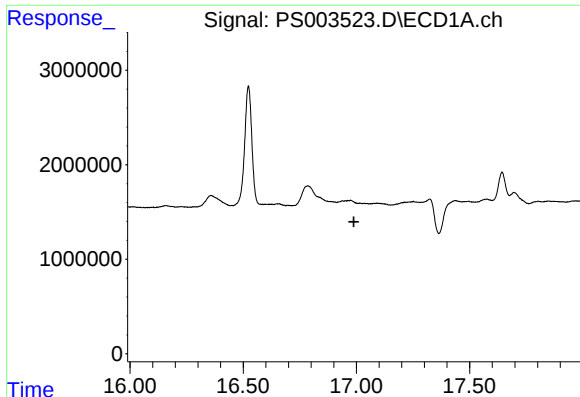

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-3

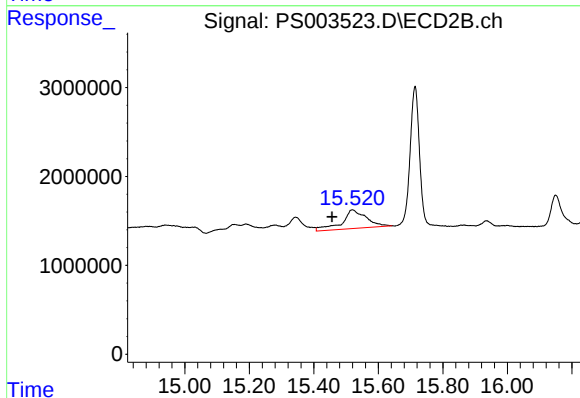


#14 DINOSEB

R.T.: 15.519 min
Delta R.T.: 0.063 min
Response: 10926456
Conc: 6.12 ng/ml

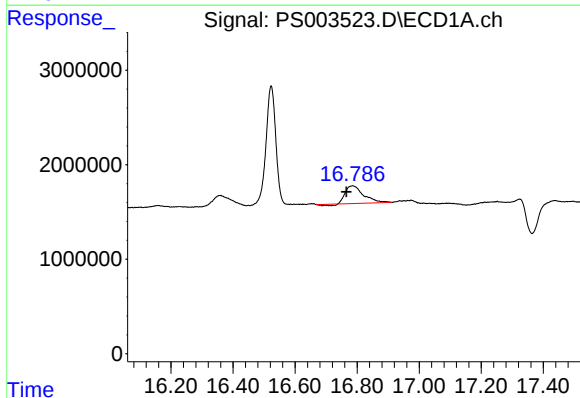


#15 Picloram

R.T.: 16.785 min
Delta R.T.: 0.020 min
Response: 7489454
Conc: 3.04 ng/ml

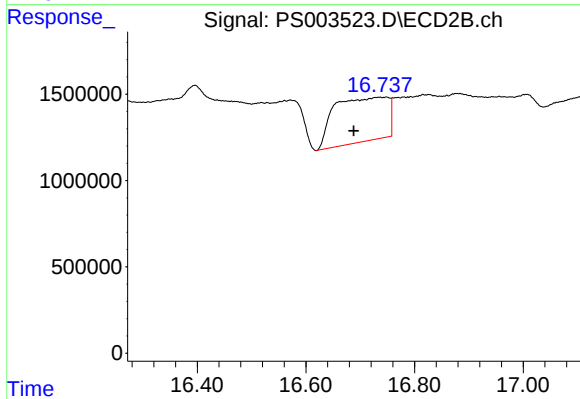

#15 Picloram


R.T.: 16.748 min
Delta R.T.: 0.059 min
Response: 17631835
Conc: 6.95 ng/ml

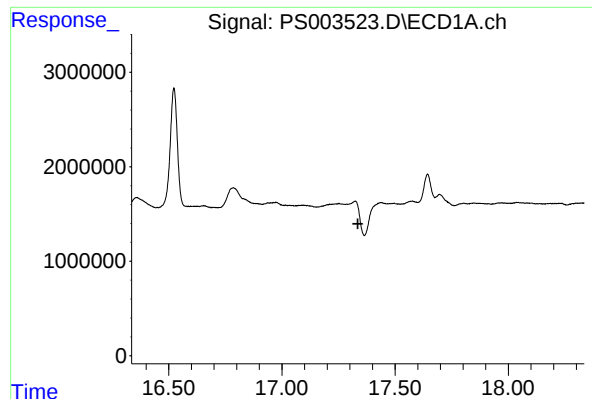

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.335 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-3

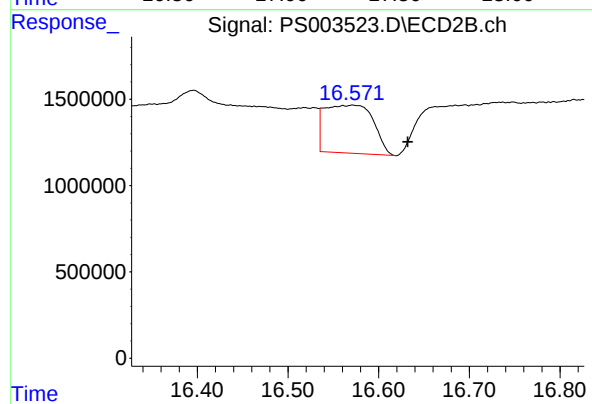

#16 DCPA

R.T.: 16.572 min
Delta R.T.: -0.060 min
Response: 10332300
Conc: 3.32 ng/ml