

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031219\
 Data File : PS003524.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2019 17:51
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 04:42:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.322	10.799	232.0E6	197.2E6	528.415	419.935
Target Compounds							
2) T	3,5-DICHL...	0.000	8.996	0	85981	N.D.	0.139 #
3) T	4-Nitroph...	0.000	9.859	0	32744	N.D.	0.146 #
7) T	MCPA	0.000	11.673	0	397264	N.D.	0.230 #
8) T	DICHLORPROP	0.000	12.206	0	635386	N.D.	1.538 #
9) T	2,4-D	13.063	12.681	7878556	55016	16.986	0.105 #
10) T	Pentachlo...	0.000	13.217	0	629838	N.D.	0.096 #
12) T	2,4,5-T	0.000	14.314	0	50881	N.D.	0.025 #
14) T	DINOSEB	0.000	15.439	0	339655	N.D.	0.190 #
15) T	Picloram	0.000	16.650	0	949916	N.D.	0.374 #
16) T	DCPA	0.000	16.650	0	949916	N.D.	0.305 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031219\
Data File : PS003524.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2019 17:51
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 04:42:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

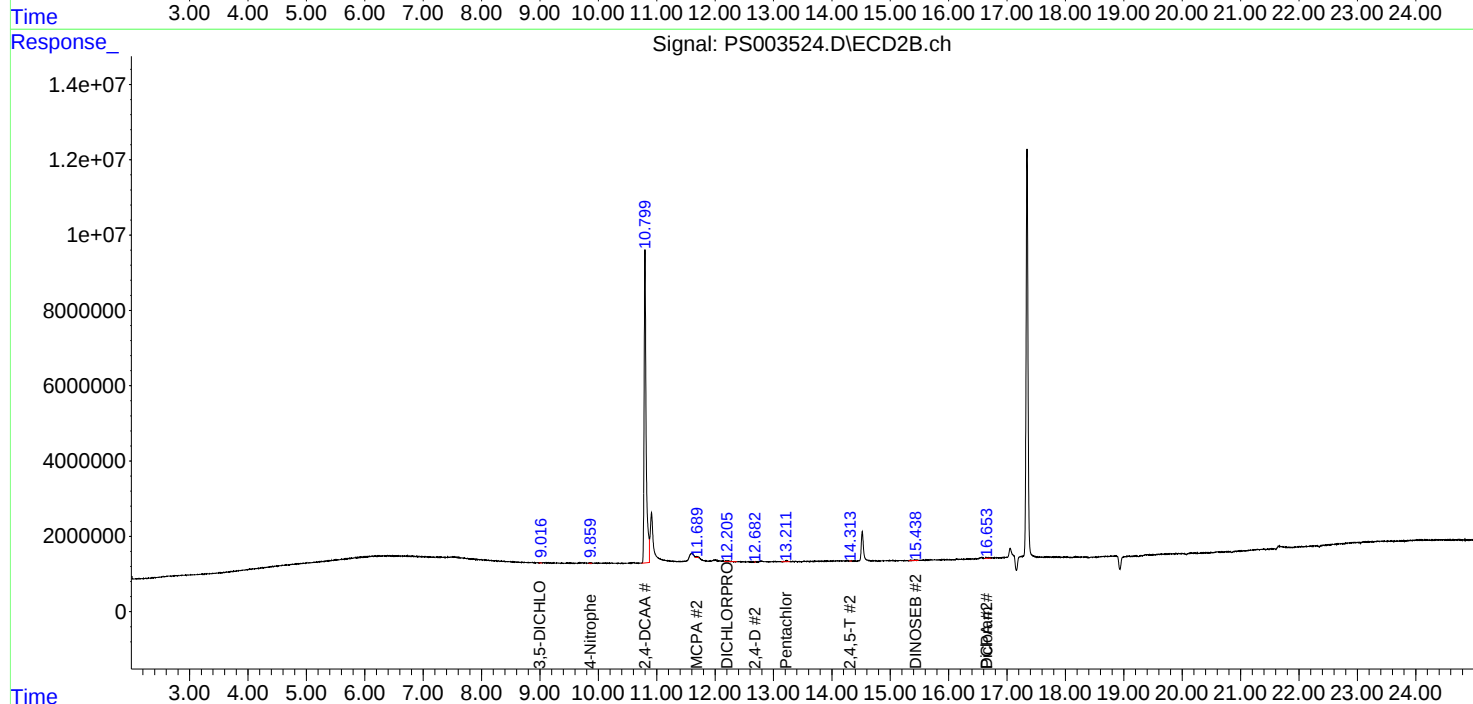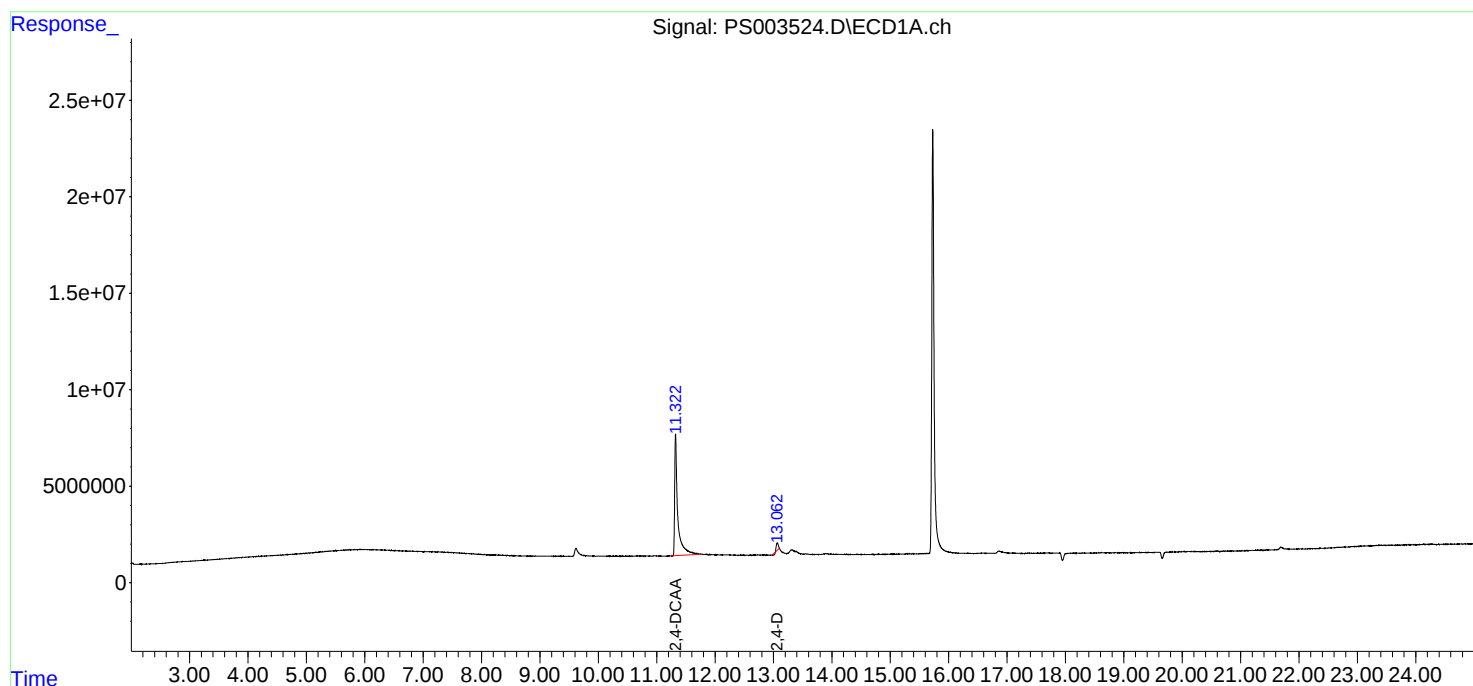


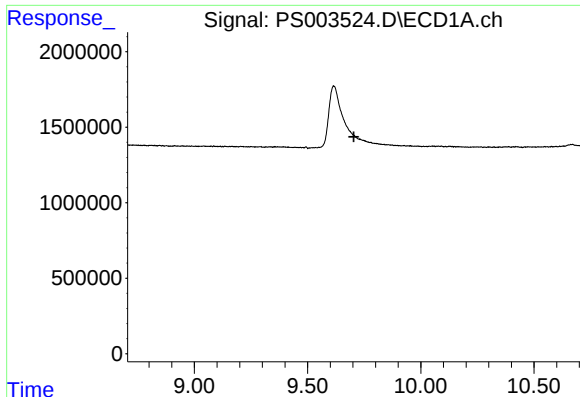

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.705 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

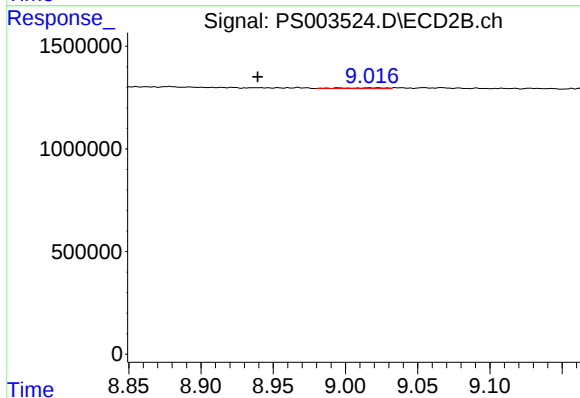


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 8.996 min
Delta R.T.: 0.056 min
Response: 85981
Conc: 0.14 ng/ml

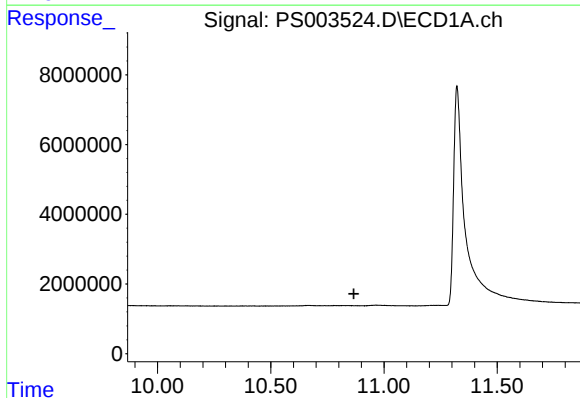


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

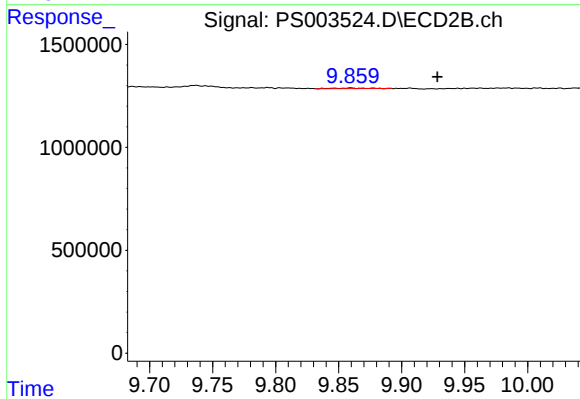

#3 4-Nitrophenol


R.T.: 9.859 min
Delta R.T.: -0.069 min
Response: 32744
Conc: 0.15 ng/ml

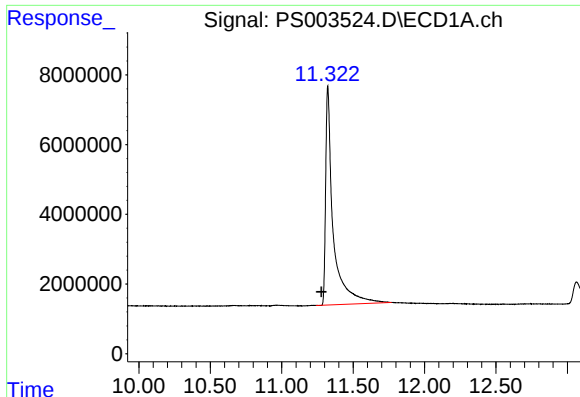

#4 2,4-DCAA


R.T.: 11.322 min
Delta R.T.: 0.045 min
Response: 231986973
Conc: 528.41 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

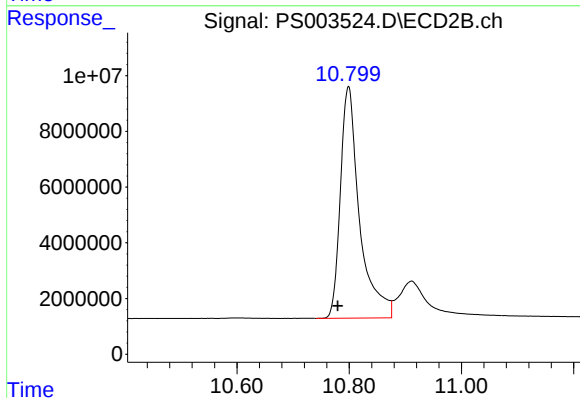


#4 2,4-DCAA

R.T.: 10.799 min
Delta R.T.: 0.019 min
Response: 197188664
Conc: 419.94 ng/ml

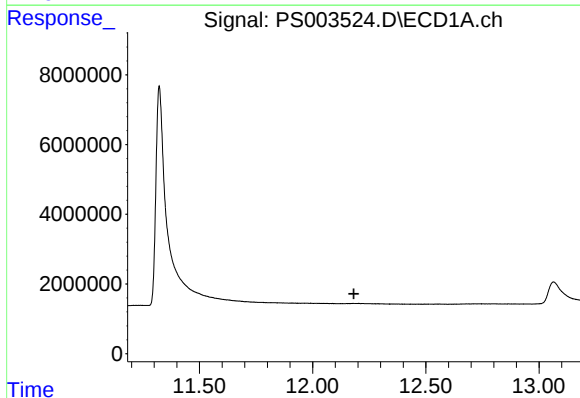


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.182 min
Response: 0
Conc: N.D.

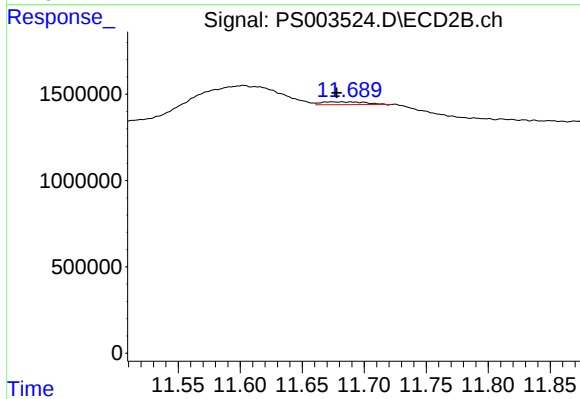

#7 MCPA


R.T.: 11.673 min
Delta R.T.: -0.004 min
Response: 397264
Conc: 0.23 ug/ml

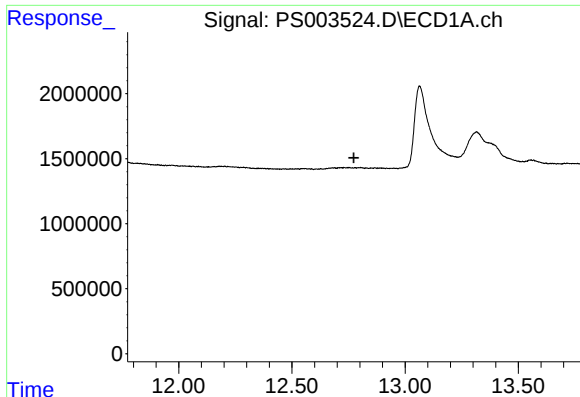

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.773 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

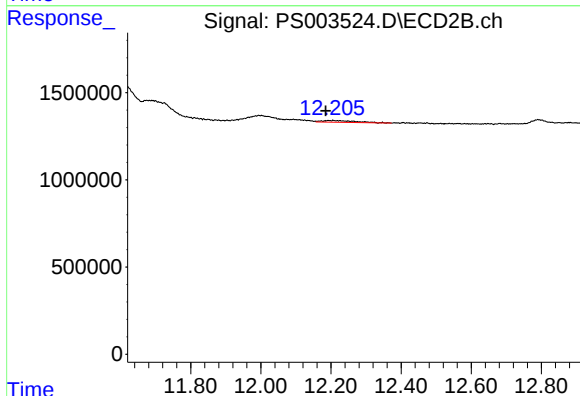


#8 DICHLORPROP

R.T.: 12.206 min
Delta R.T.: 0.021 min
Response: 635386
Conc: 1.54 ng/ml

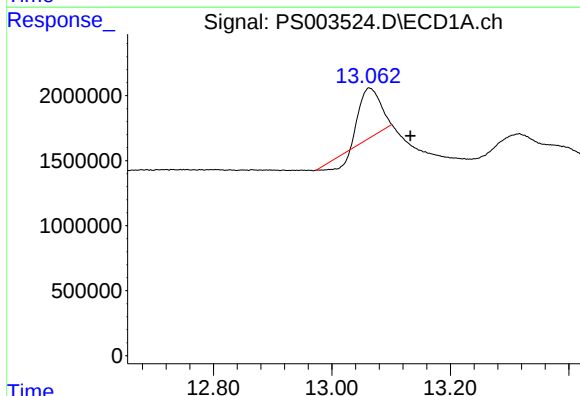


#9 2,4-D

R.T.: 13.063 min
Delta R.T.: -0.069 min
Response: 7878556
Conc: 16.99 ng/ml

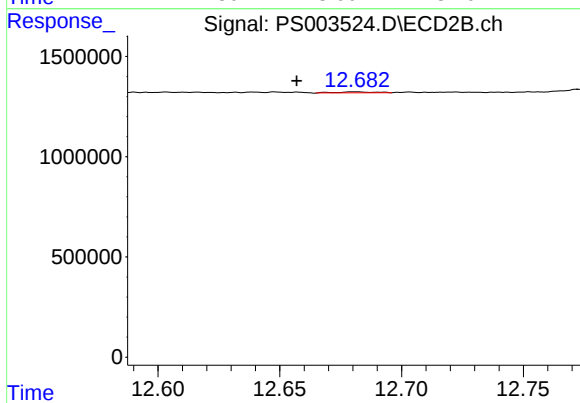

#9 2,4-D


R.T.: 12.681 min
Delta R.T.: 0.024 min
Response: 55016
Conc: 0.10 ng/ml

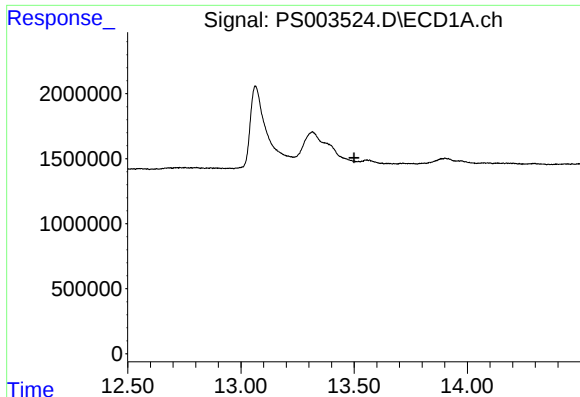

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.499 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

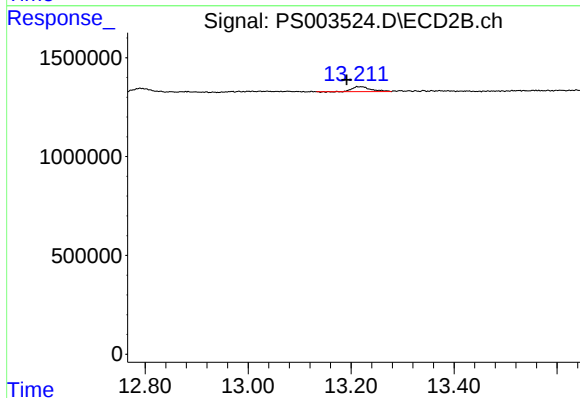


#10 Pentachlorophenol

R.T.: 13.217 min
Delta R.T.: 0.026 min
Response: 629838
Conc: 0.10 ng/ml

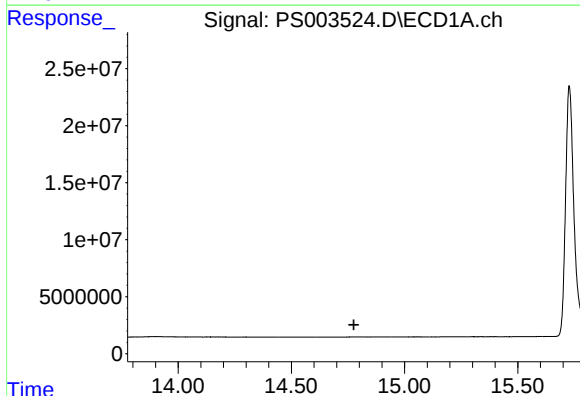


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

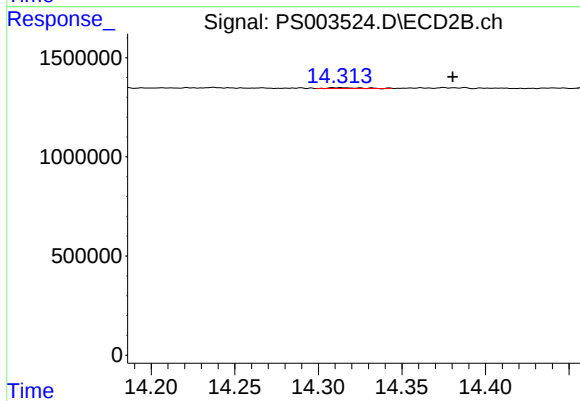

#12 2,4,5-T


R.T.: 14.314 min
Delta R.T.: -0.066 min
Response: 50881
Conc: 0.03 ng/ml

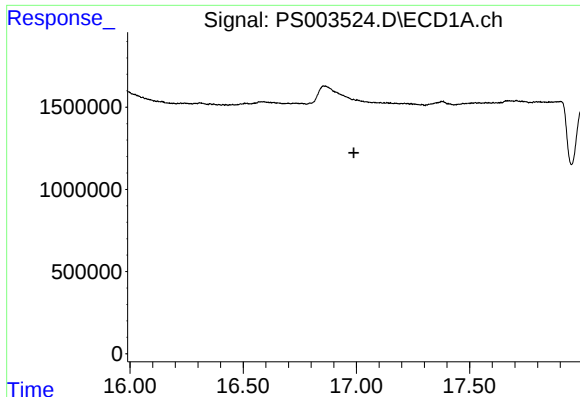

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 16.989 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

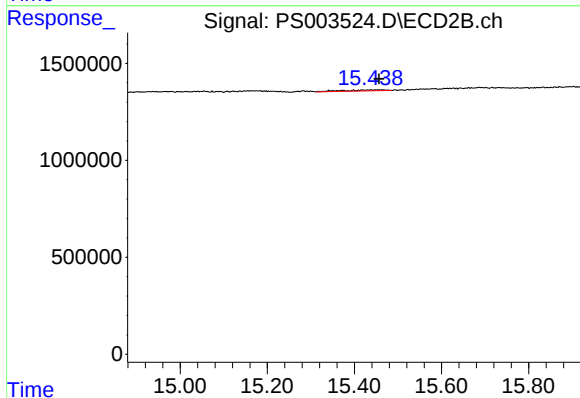


#14 DINOSEB

R.T.: 15.439 min
Delta R.T.: -0.018 min
Response: 339655
Conc: 0.19 ng/ml

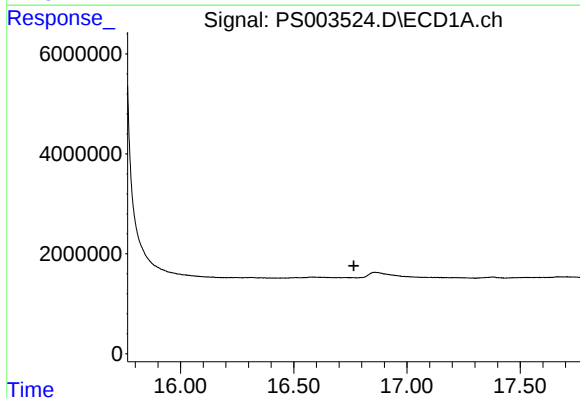


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.765 min
Response: 0
Conc: N.D.

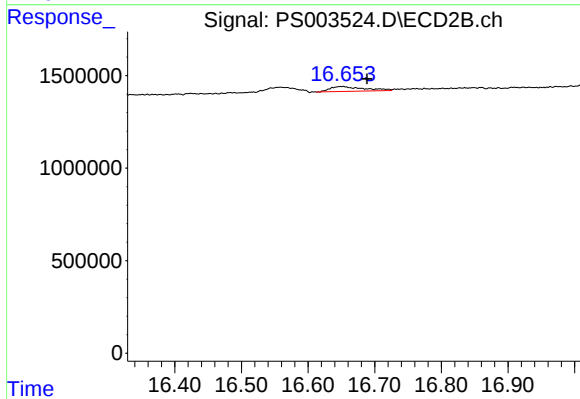

#15 Picloram


R.T.: 16.650 min
Delta R.T.: -0.038 min
Response: 949916
Conc: 0.37 ng/ml

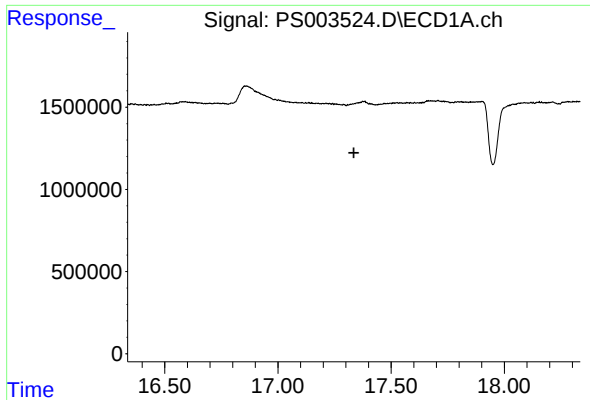

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.335 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

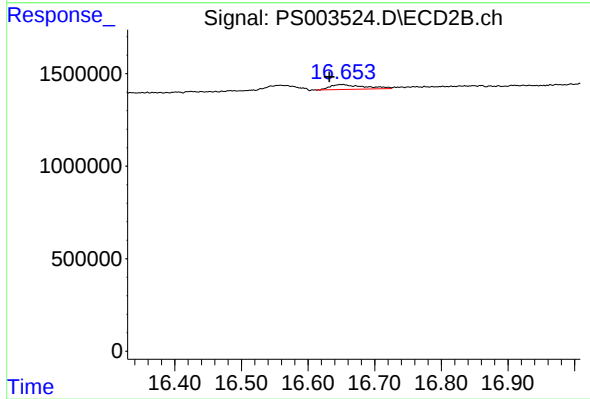

#16 DCPA

R.T.: 16.650 min
Delta R.T.: 0.018 min
Response: 949916
Conc: 0.31 ng/ml