

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031220\
 Data File : PS009210.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2020 13:44
 Operator : DD\AJ
 Sample : PB127469BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 04:11:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.246	6.933	301.6E6	276.5E6	545.227	503.457
Target Compounds							
1) T	Dalapon	3.012	2.582	17589247	108.6E6	22.555	137.976 #
2) T	3,5-DICHL...	0.000	6.108	0	47562592	N.D.	58.481
3) T	4-Nitroph...	7.086	6.590	2256174	54644311	9.451	171.730 #
5) T	DICAMBA	7.366	0.000	18587347	0	8.734	N.D. #
7) T	MCPA	7.798	7.401	8597850	52961291	2.823	19.625 #
8) T	DICHLORPROP	8.127	7.754	11141368	36905286	21.603	66.517 #
11) T	2,4,5-TP ...	0.000	8.787	0	26115588	N.D.	8.760
14) T	DINOSEB	0.000	10.048	0	9565847	N.D.	4.355
15) T	Picloram	0.000	11.022	0	43405811	N.D.	10.659
16) T	DCPA	0.000	11.022	0	43405811	N.D.	11.207



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031220\
Data File : PS009210.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2020 13:44
Operator : DD\AJ
Sample : PB127469BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 04:11:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

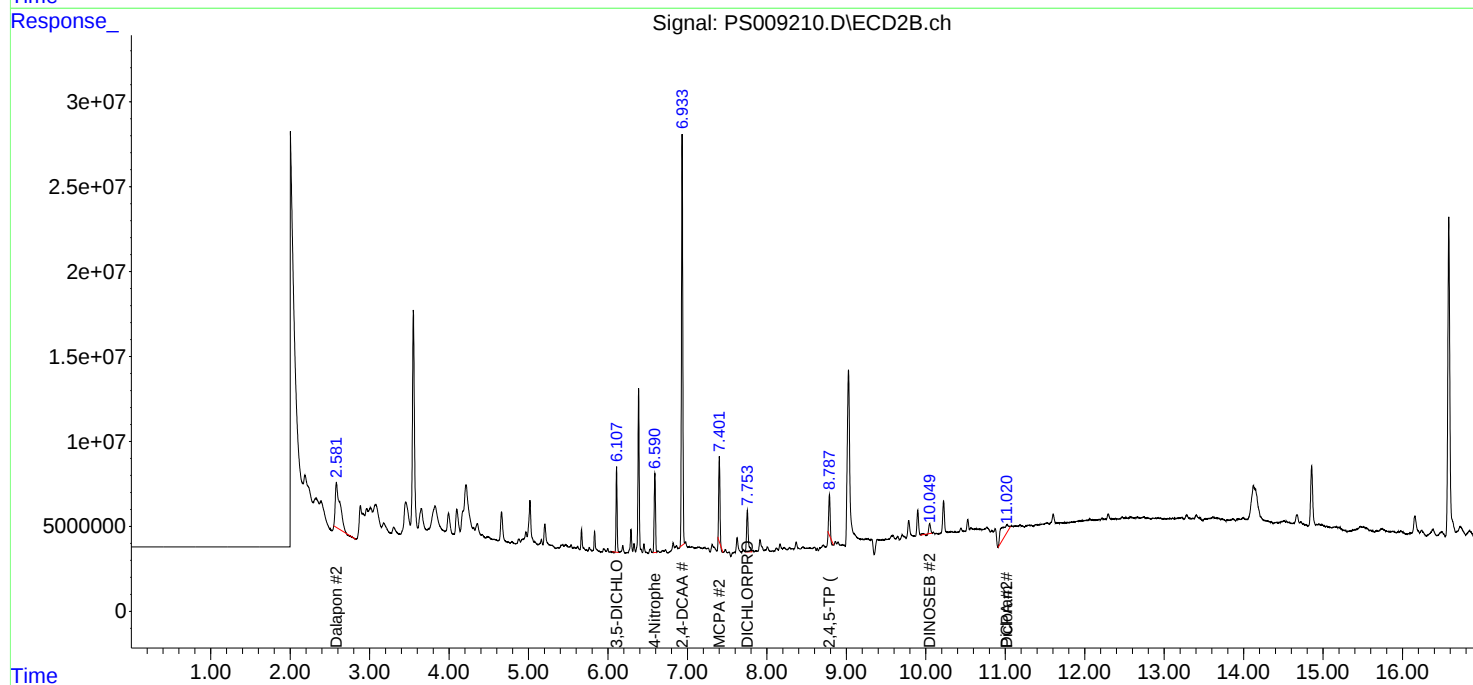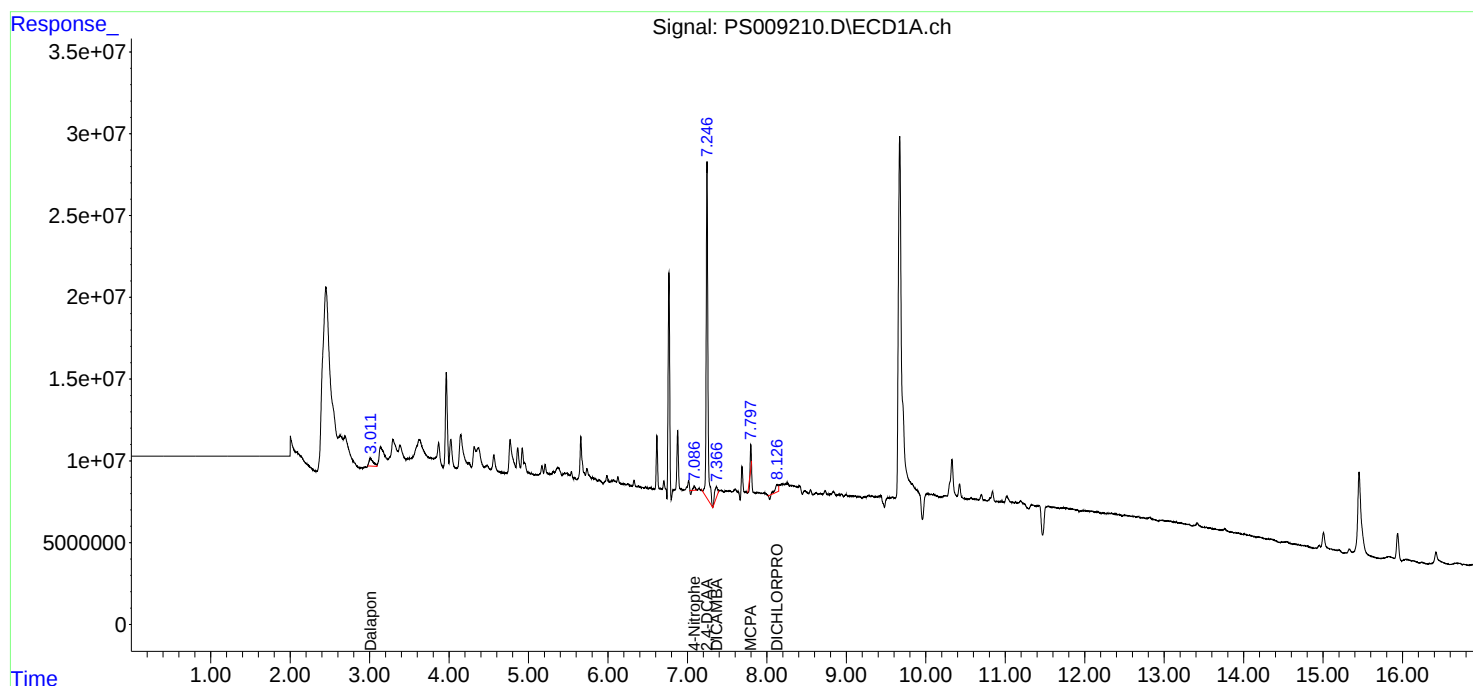


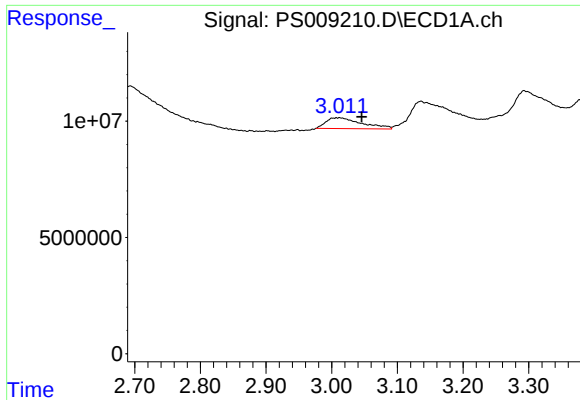

#1 Dalapon


R.T.: 3.012 min
Delta R.T.: -0.034 min
Response: 17589247
Conc: 22.56 ng/ml

Instrument :
ECD_S
ClientSampleId :

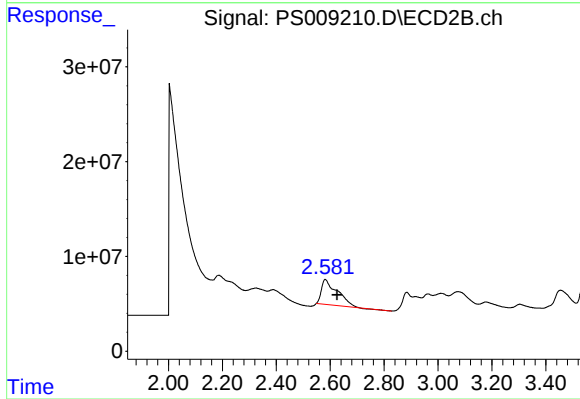


#1 Dalapon

R.T.: 2.582 min
Delta R.T.: -0.045 min
Response: 108637052
Conc: 137.98 ng/ml

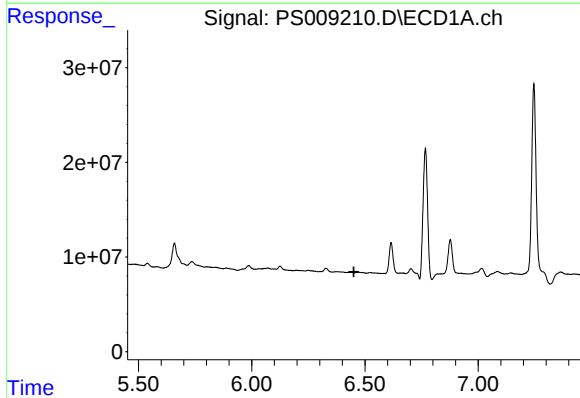


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

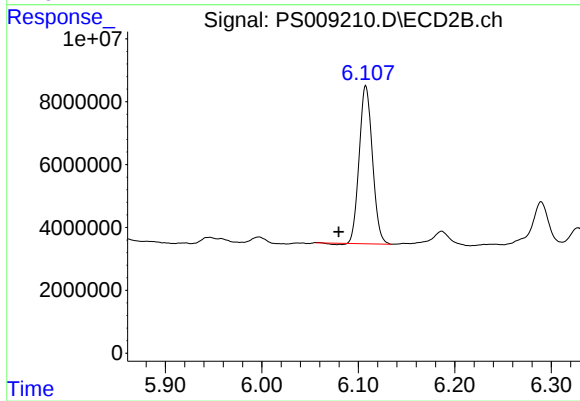

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.108 min
Delta R.T.: 0.028 min
Response: 47562592
Conc: 58.48 ng/ml

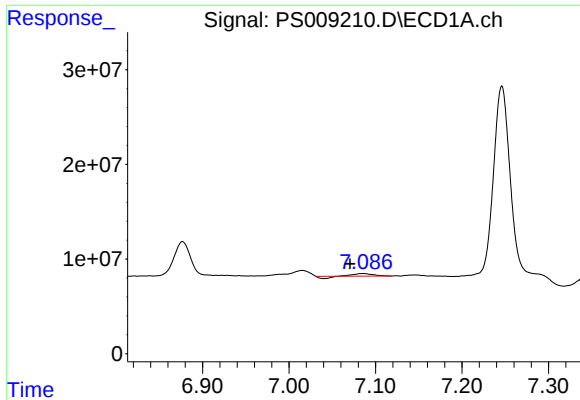

#3 4-Nitrophenol


R.T.: 7.086 min
Delta R.T.: 0.016 min
Response: 2256174
Conc: 9.45 ng/ml

Instrument :
ECD_S
ClientSampleId :

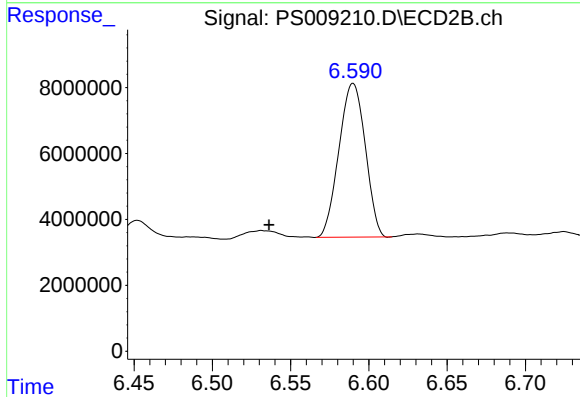


#3 4-Nitrophenol

R.T.: 6.590 min
Delta R.T.: 0.054 min
Response: 54644311
Conc: 171.73 ng/ml

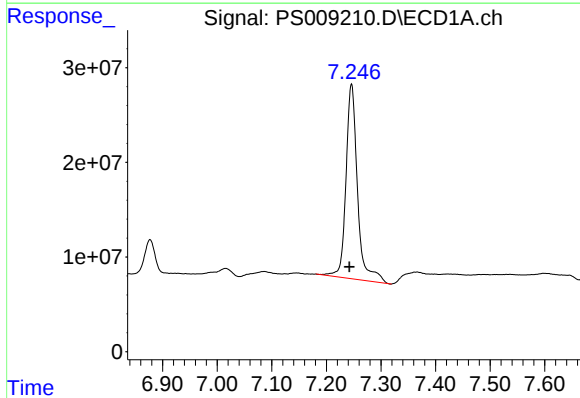


#4 2,4-DCAA

R.T.: 7.246 min
Delta R.T.: 0.004 min
Response: 301603300
Conc: 545.23 ng/ml

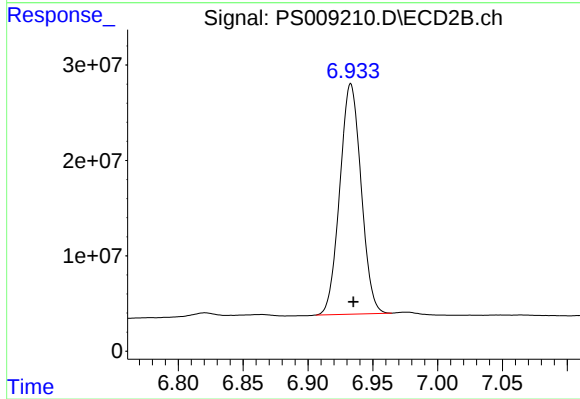

#4 2,4-DCAA


R.T.: 6.933 min
Delta R.T.: -0.002 min
Response: 276497689
Conc: 503.46 ng/ml

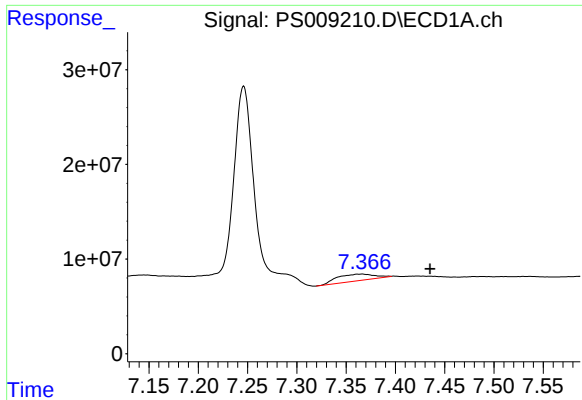

#5 DICAMBA


R.T.: 7.366 min
Delta R.T.: -0.069 min
Response: 18587347
Conc: 8.73 ng/ml

Instrument :
ECD_S
ClientSampleId :

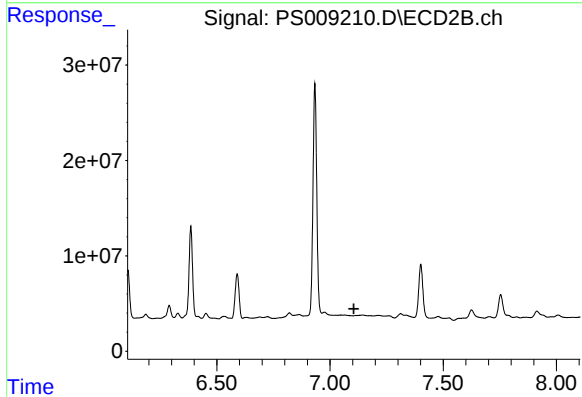


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.106 min
Response: 0
Conc: N.D.

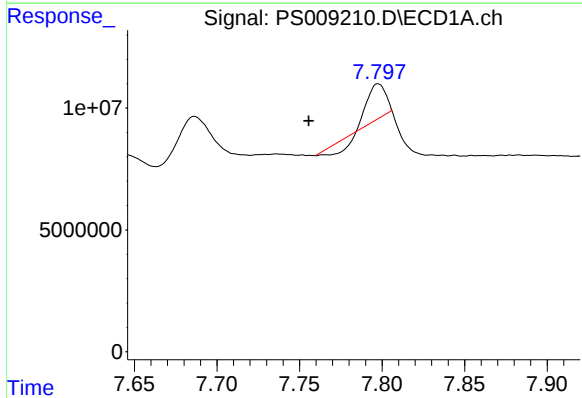


#7 MCPA

R.T.: 7.798 min
Delta R.T.: 0.042 min
Response: 8597850
Conc: 2.82 ug/ml

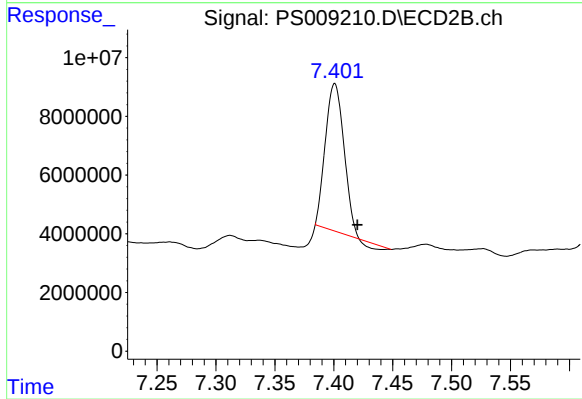

#7 MCPA


R.T.: 7.401 min
Delta R.T.: -0.019 min
Response: 52961291
Conc: 19.63 ug/ml

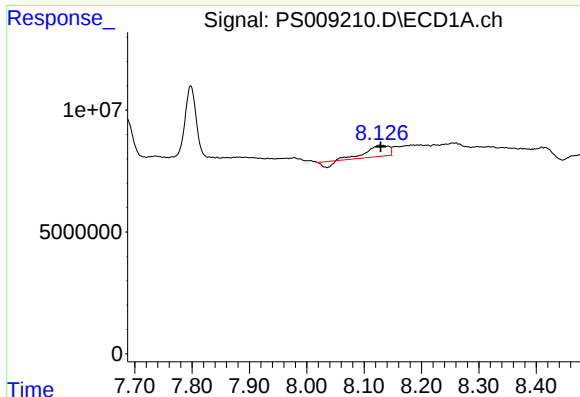

#8 DICHLORPROP


R.T.: 8.127 min
Delta R.T.: -0.002 min
Response: 11141368
Conc: 21.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

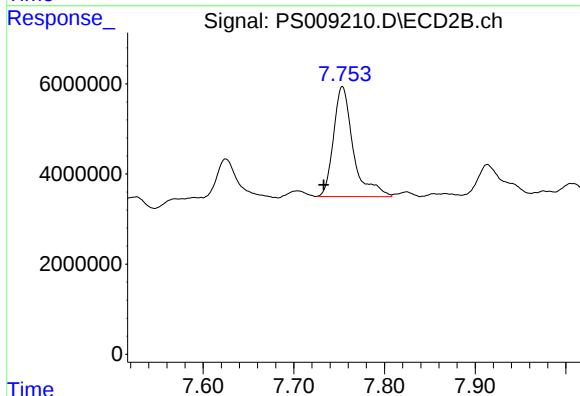


#8 DICHLORPROP

R.T.: 7.754 min
Delta R.T.: 0.021 min
Response: 36905286
Conc: 66.52 ng/ml

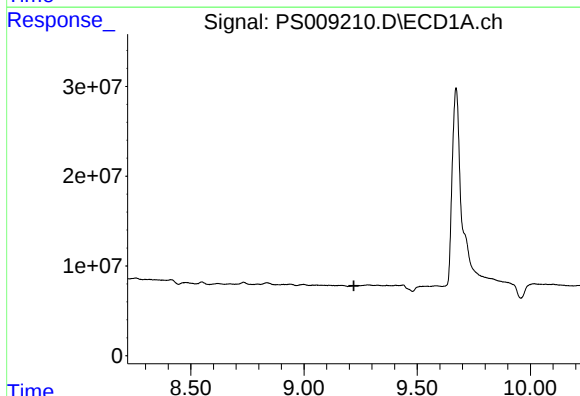


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.221 min
Response: 0
Conc: N.D.

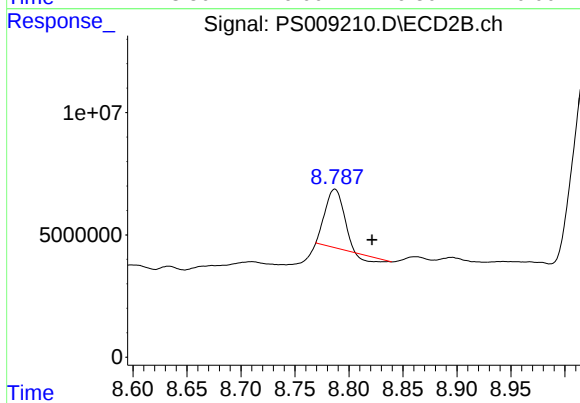

#11 2,4,5-TP (SILVEX)


R.T.: 8.787 min
Delta R.T.: -0.035 min
Response: 26115588
Conc: 8.76 ng/ml

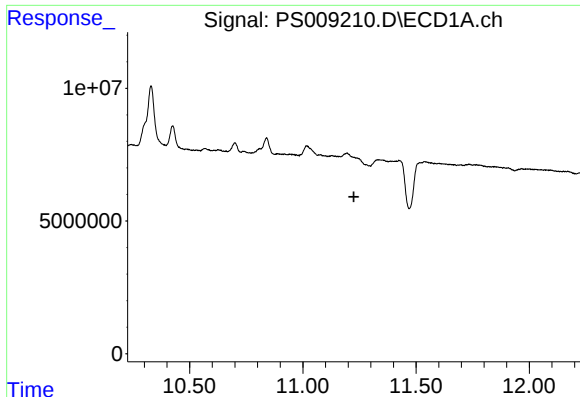

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 11.225 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

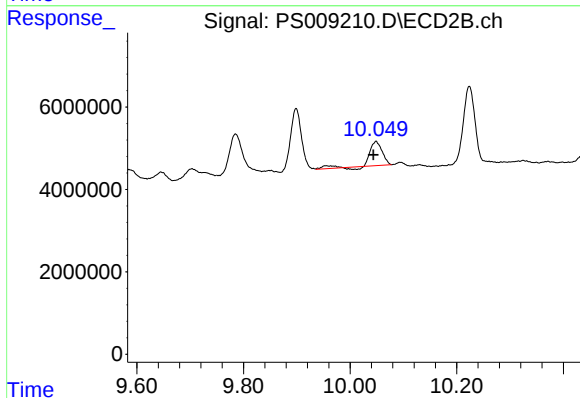


#14 DINOSEB

R.T.: 10.048 min
Delta R.T.: 0.005 min
Response: 9565847
Conc: 4.36 ng/ml

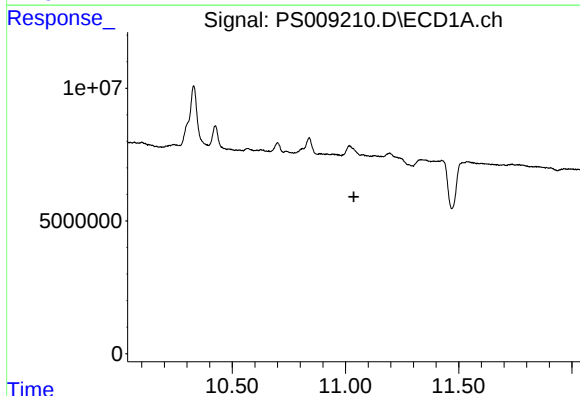


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.037 min
Response: 0
Conc: N.D.

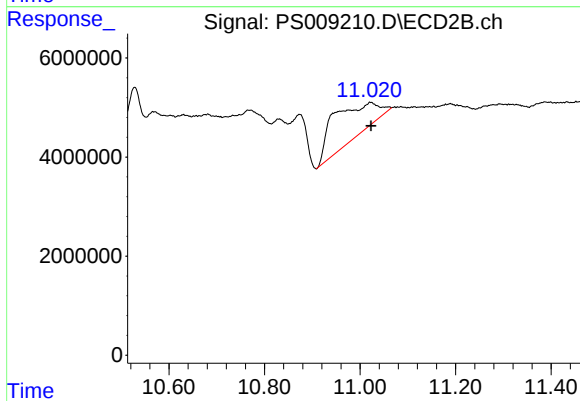

#15 Picloram


R.T.: 11.022 min
Delta R.T.: -0.001 min
Response: 43405811
Conc: 10.66 ng/ml

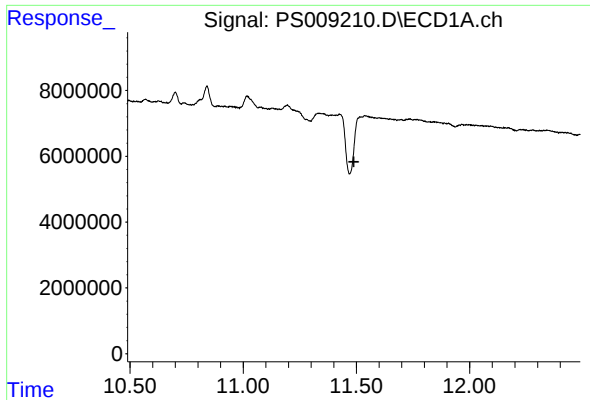

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.489 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

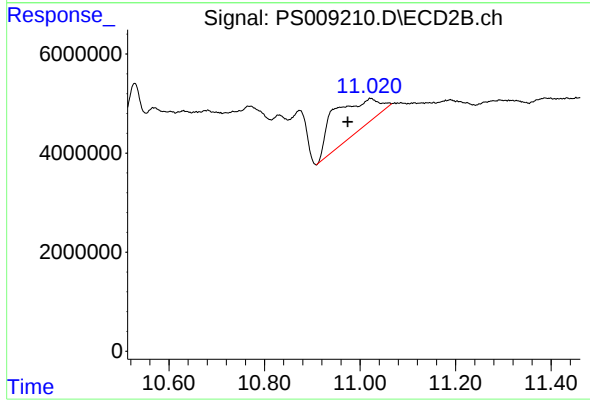

#16 DCPA

R.T.: 11.022 min
Delta R.T.: 0.048 min
Response: 43405811
Conc: 11.21 ng/ml