

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031220\
 Data File : PS009212.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2020 14:29
 Operator : DD\AJ
 Sample : PB127449BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 04:12:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.242	6.934	312.1E6	287.0E6	564.139	522.661
Target Compounds							
1) T	Dalapon	3.009	2.587	20297052	232.6E6	26.027	295.414 #
2) T	3,5-DICHL...	0.000	6.110	0	66538054	N.D.	81.812
3) T	4-Nitroph...	7.011	6.592	16423373	41968710	68.800	131.895 #
7) T	MCPA	7.793	7.401	4083807	29769092	1.341	11.031 #
8) T	DICHLORPROP	8.118	7.754	1672537	37722442	3.243	67.990 #
10) T	Pentachlo...	8.670	8.458	9206103	8417740	1.309	1.109
12) T	2,4,5-T	9.503	0.000	11411311	0	4.486	N.D. #
13) T	2,4-DB	0.000	9.703	0	17035158	N.D.	44.875
14) T	DINOSEB	0.000	10.046	0	12729129	N.D.	5.795
15) T	Picloram	0.000	11.023	0	13711103	N.D.	3.367
16) T	DCPA	0.000	10.973	0	31138430	N.D.	8.040



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031220\
Data File : PS009212.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2020 14:29
Operator : DD\AJ
Sample : PB127449BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 04:12:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

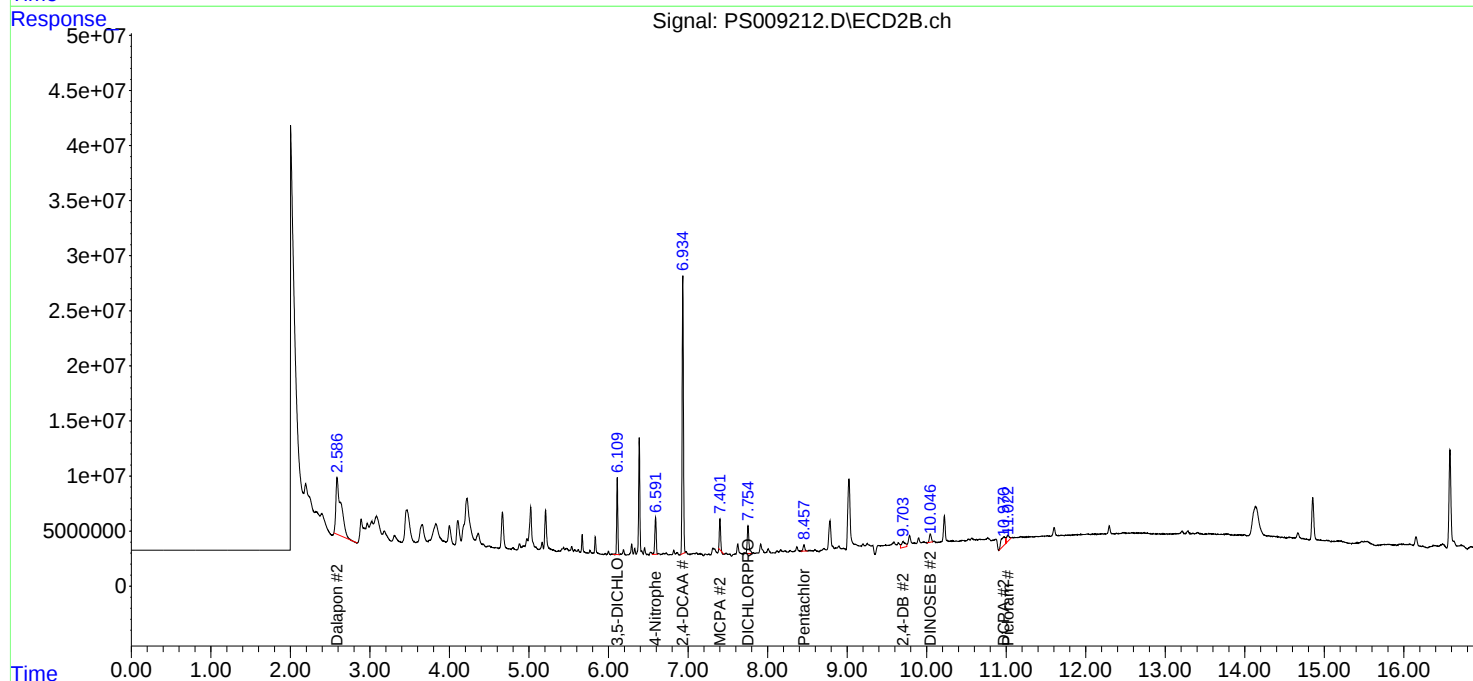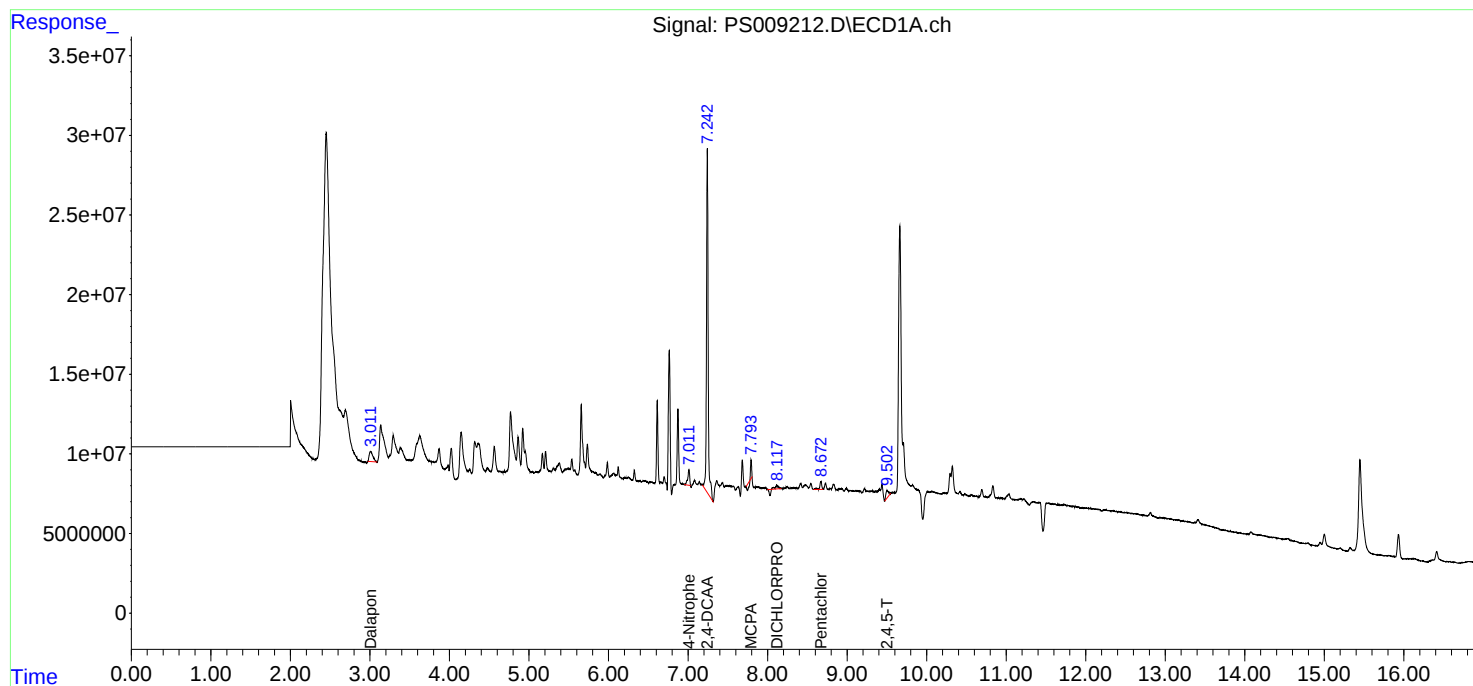


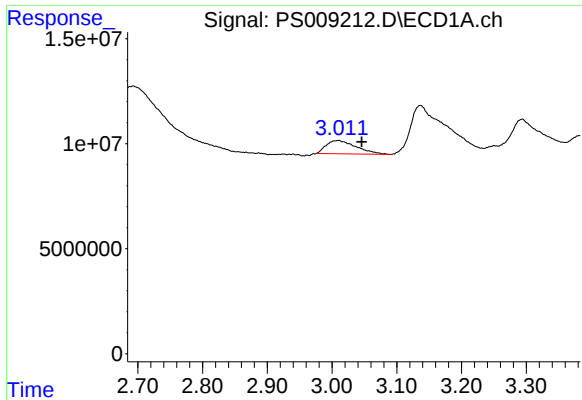

#1 Dalapon


R.T.: 3.009 min
Delta R.T.: -0.037 min
Response: 20297052
Conc: 26.03 ng/ml

Instrument :
ECD_S
ClientSampleId :

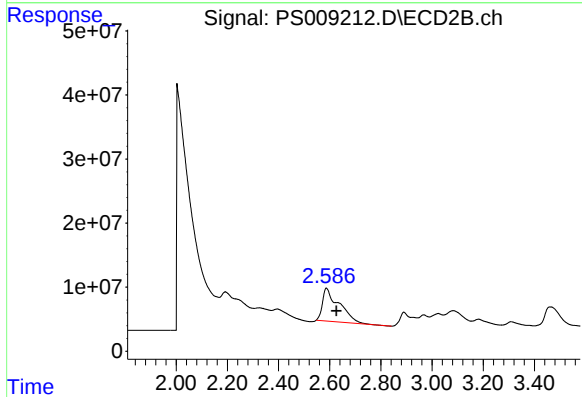


#1 Dalapon

R.T.: 2.587 min
Delta R.T.: -0.039 min
Response: 232597752
Conc: 295.41 ng/ml

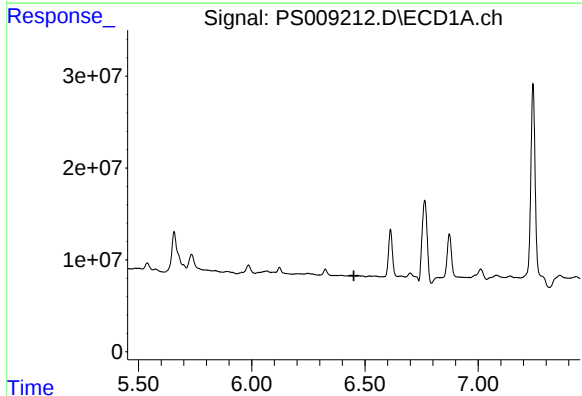


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

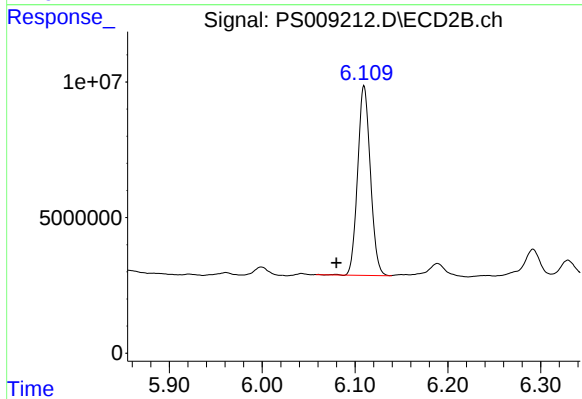

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.110 min
Delta R.T.: 0.030 min
Response: 66538054
Conc: 81.81 ng/ml

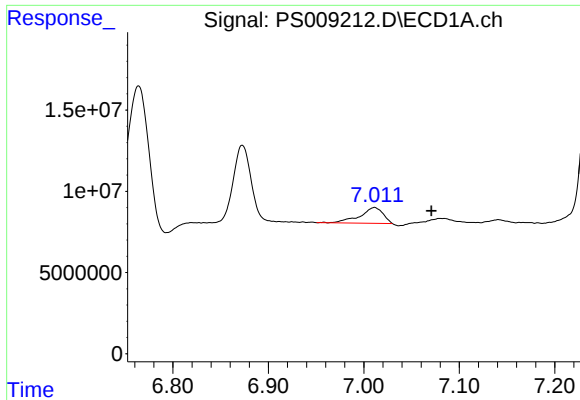

#3 4-Nitrophenol


R.T.: 7.011 min
Delta R.T.: -0.060 min
Response: 16423373
Conc: 68.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

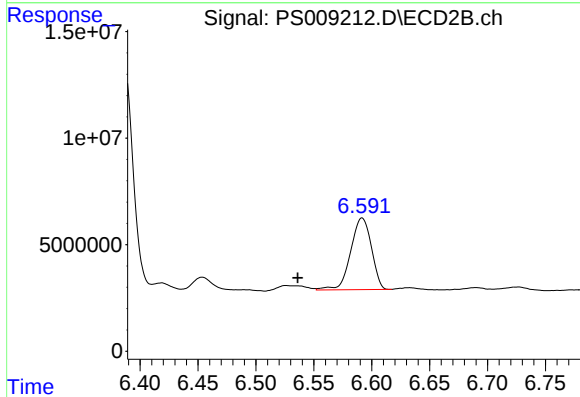


#3 4-Nitrophenol

R.T.: 6.592 min
Delta R.T.: 0.055 min
Response: 41968710
Conc: 131.89 ng/ml

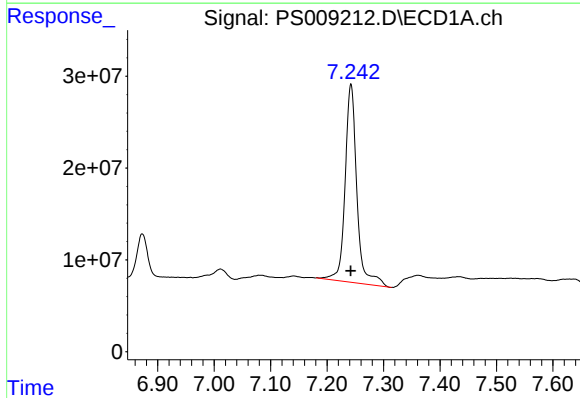


#4 2,4-DCAA

R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 312064756
Conc: 564.14 ng/ml

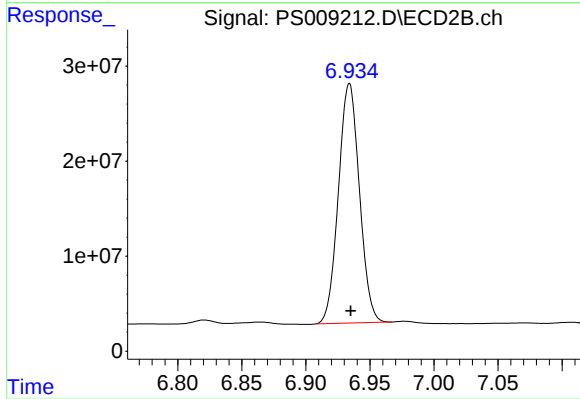

#4 2,4-DCAA


R.T.: 6.934 min
Delta R.T.: -0.001 min
Response: 287044330
Conc: 522.66 ng/ml

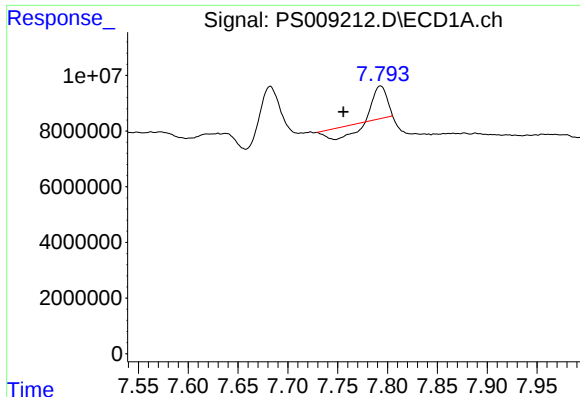

#7 MCPA


R.T.: 7.793 min
Delta R.T.: 0.037 min
Response: 4083807
Conc: 1.34 ug/ml

Instrument :
ECD_S
ClientSampleId :

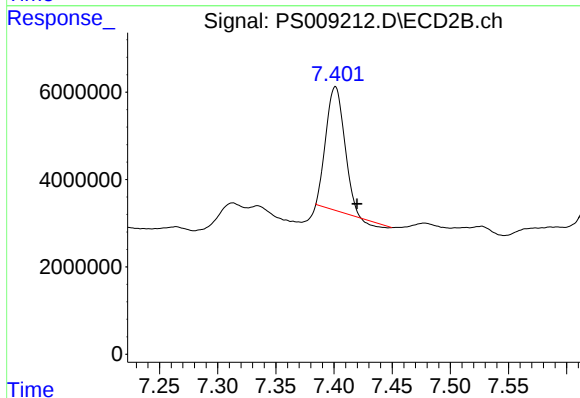


#7 MCPA

R.T.: 7.401 min
Delta R.T.: -0.019 min
Response: 29769092
Conc: 11.03 ug/ml

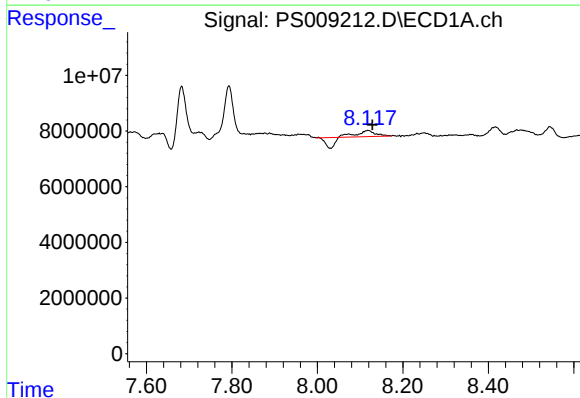


#8 DICHLORPROP

R.T.: 8.118 min
Delta R.T.: -0.011 min
Response: 1672537
Conc: 3.24 ng/ml

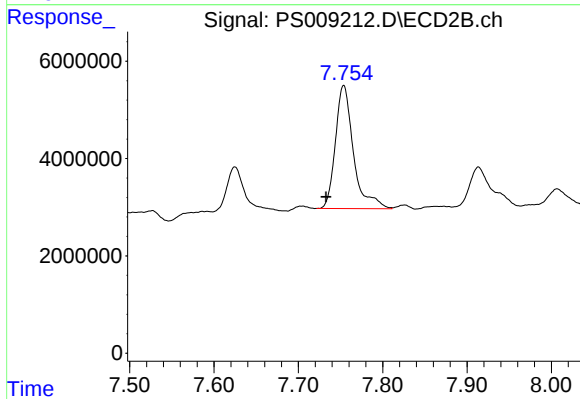

#8 DICHLORPROP


R.T.: 7.754 min
Delta R.T.: 0.021 min
Response: 37722442
Conc: 67.99 ng/ml

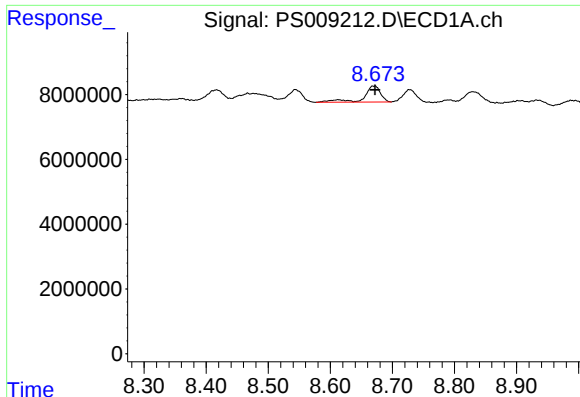

#10 Pentachlorophenol


R.T.: 8.670 min
Delta R.T.: -0.002 min
Response: 9206103
Conc: 1.31 ng/ml

Instrument :
ECD_S
ClientSampleId :

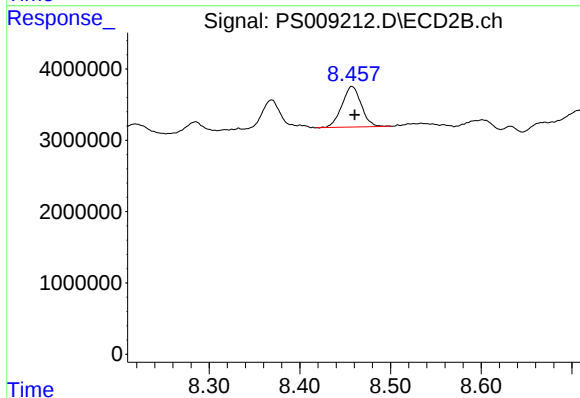


#10 Pentachlorophenol

R.T.: 8.458 min
Delta R.T.: -0.003 min
Response: 8417740
Conc: 1.11 ng/ml

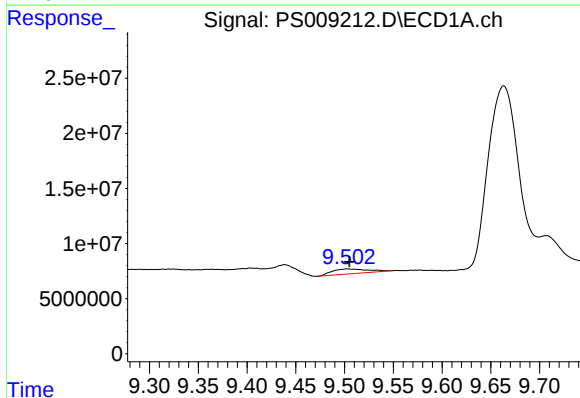


#12 2,4,5-T

R.T.: 9.503 min
Delta R.T.: -0.002 min
Response: 11411311
Conc: 4.49 ng/ml

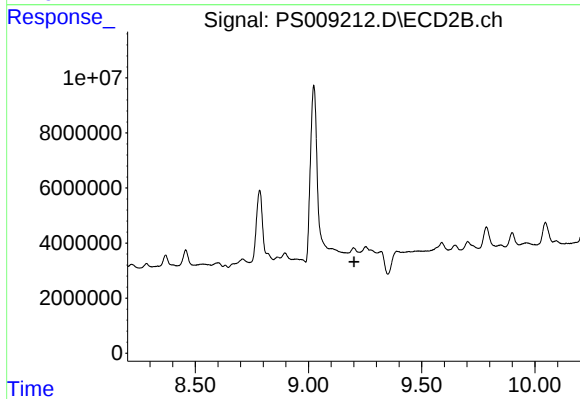

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.201 min
Response: 0
Conc: N.D.

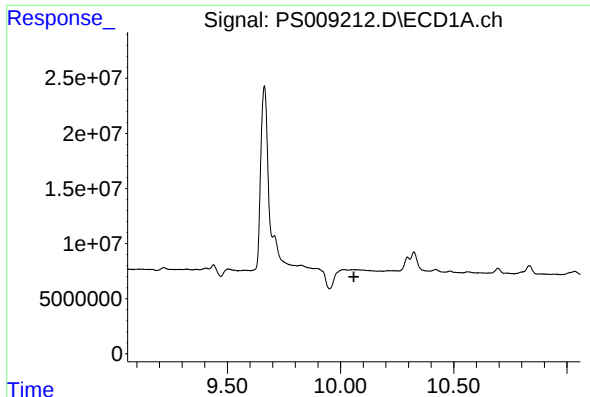

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.059 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

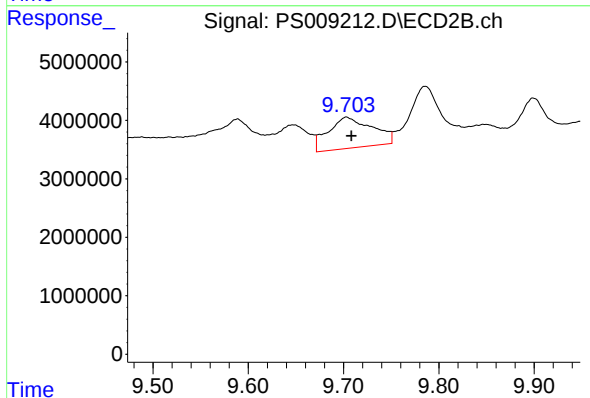


#13 2,4-DB

R.T.: 9.703 min
Delta R.T.: -0.005 min
Response: 17035158
Conc: 44.87 ng/ml

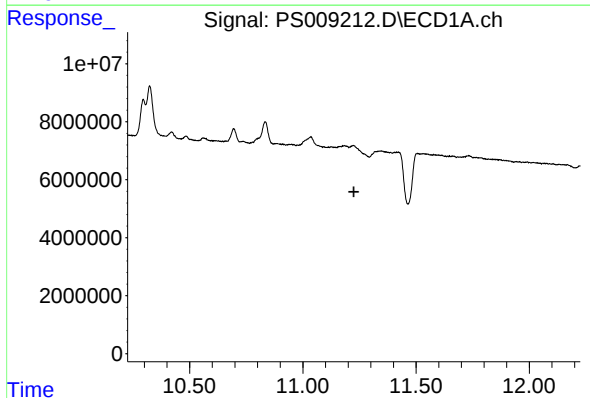


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 11.225 min
Response: 0
Conc: N.D.

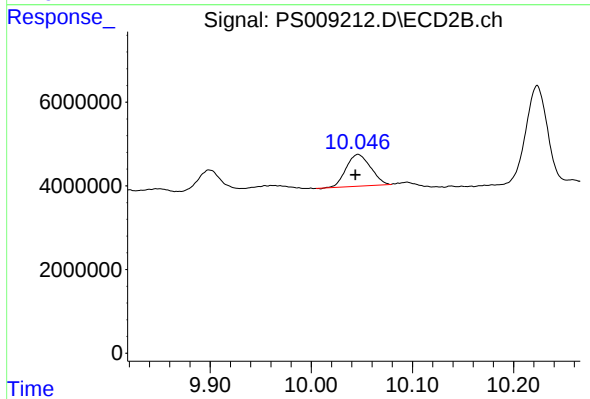

#14 DINOSEB


R.T.: 10.046 min
Delta R.T.: 0.003 min
Response: 12729129
Conc: 5.80 ng/ml

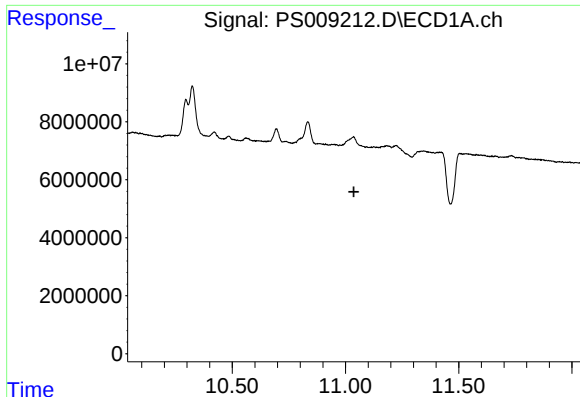

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 11.037 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

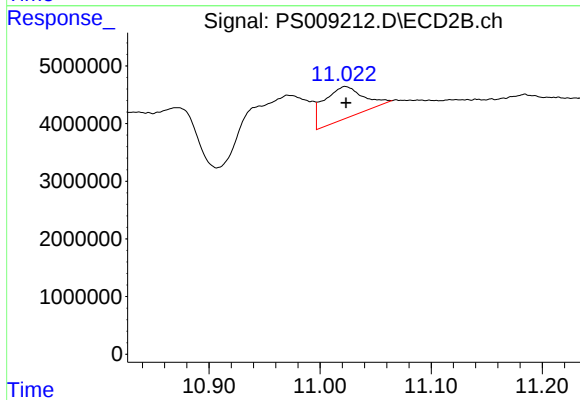


#15 Picloram

R.T.: 11.023 min
Delta R.T.: 0.000 min
Response: 13711103
Conc: 3.37 ng/ml

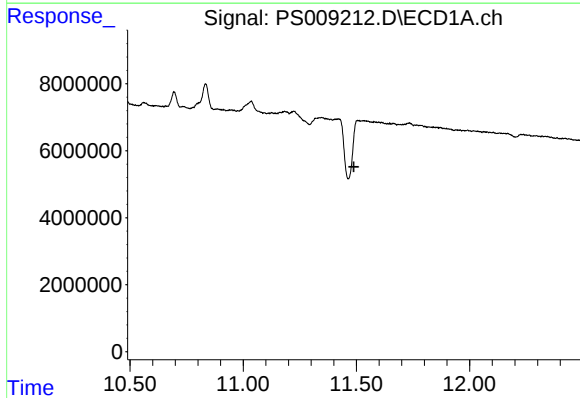

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.489 min
Response: 0
Conc: N.D.

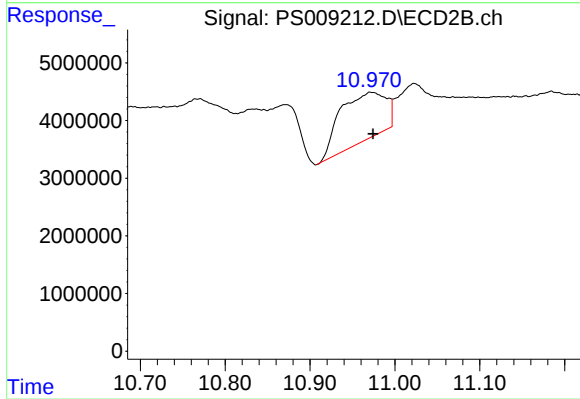

#16 DCPA

R.T.: 10.973 min
Delta R.T.: -0.002 min
Response: 31138430
Conc: 8.04 ng/ml