

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031220\
 Data File : PS009216.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2020 16:01
 Operator : DD\AJ
 Sample : L1852-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 04:13:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.242	6.934	222.7E6	196.3E6	402.651	357.419
Target Compounds							
1) T	Dalapon	3.006	2.590	19777327	170.7E6	25.361	216.771 #
2) T	3,5-DICHL...	0.000	6.110	0	63514956	N.D.	78.095
3) T	4-Nitroph...	7.010	6.592	17461490	30394014	73.149	95.519 #
8) T	DICHLORPROP	8.119	7.754	-1202333	37825874	N.D.	68.177
9) T	2,4-D	8.295	0.000	11151989	0	21.152	N.D. #
12) T	2,4,5-T	9.441	0.000	24004224	0	9.436	N.D. #
13) T	2,4-DB	0.000	9.704	0	7610926	N.D.	20.049
15) T	Picloram	11.011	0.000	20533072	0	6.766	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031220\
Data File : PS009216.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2020 16:01
Operator : DD\AJ
Sample : L1852-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 04:13:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

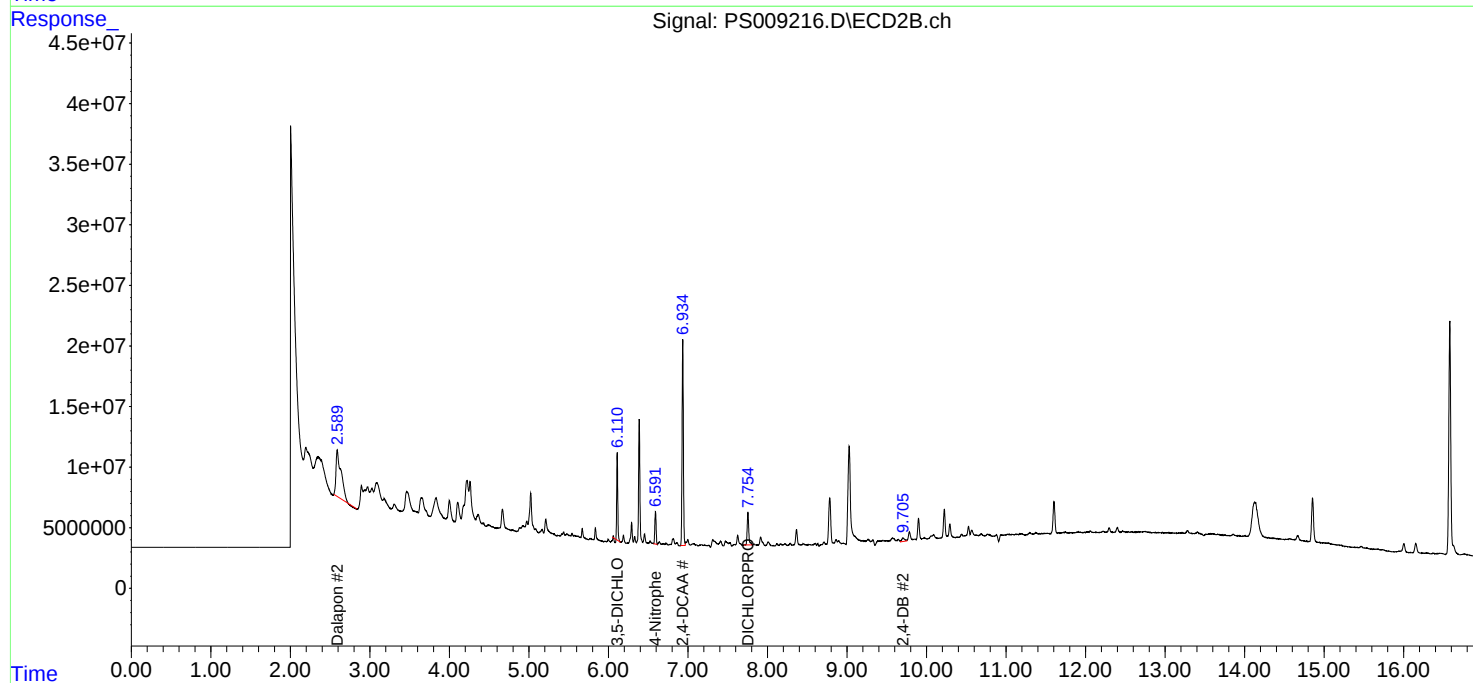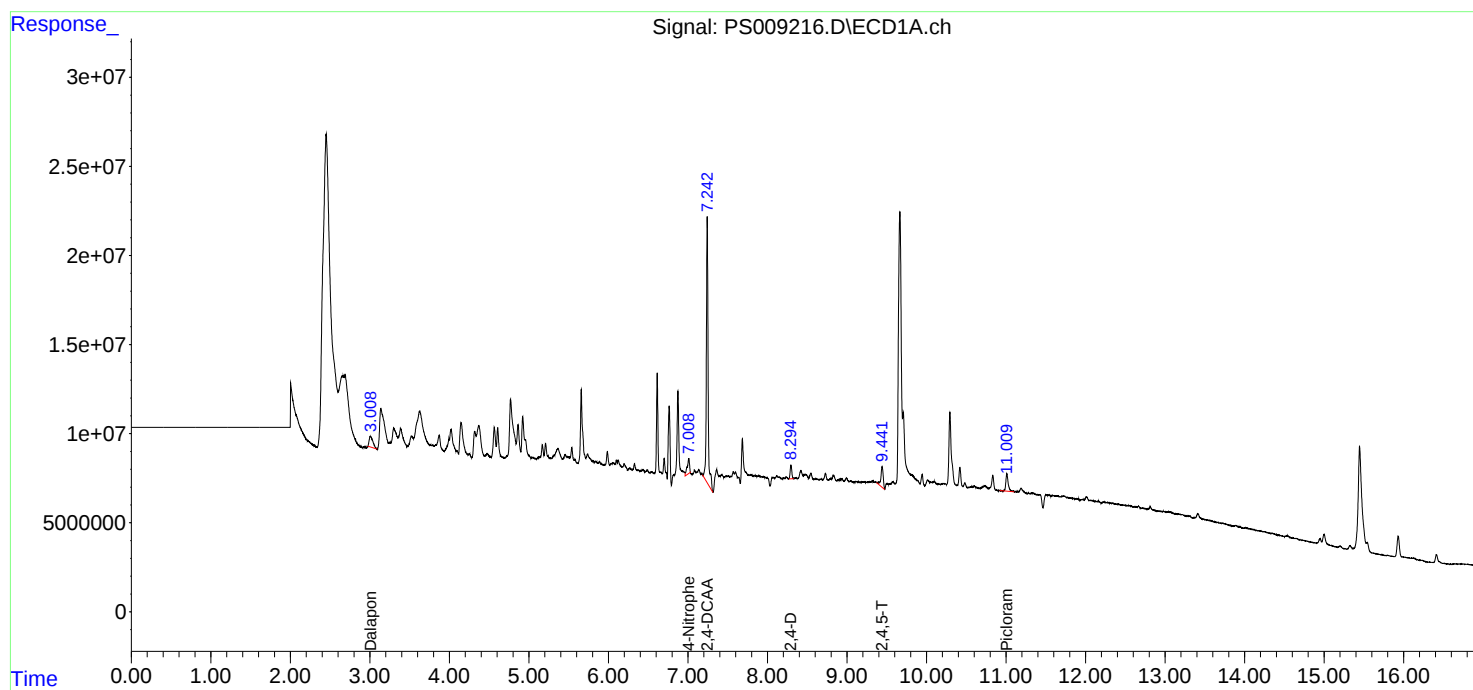


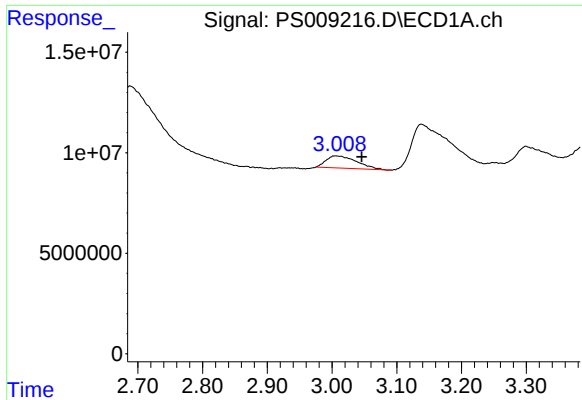

#1 Dalapon


R.T.: 3.006 min
Delta R.T.: -0.040 min
Response: 19777327
Conc: 25.36 ng/ml

Instrument :
ECD_S
ClientSampleId :

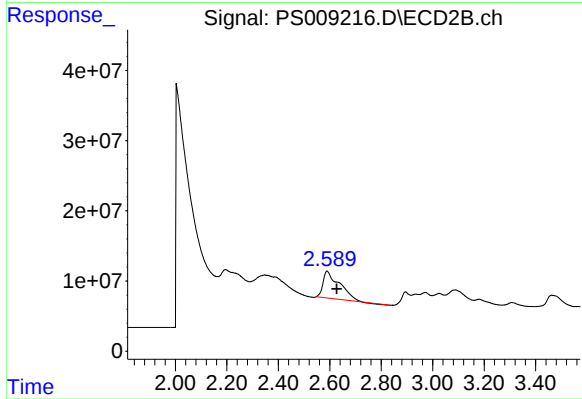


#1 Dalapon

R.T.: 2.590 min
Delta R.T.: -0.037 min
Response: 170677504
Conc: 216.77 ng/ml

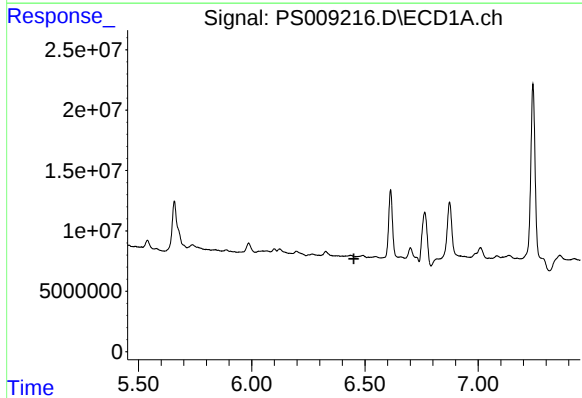


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

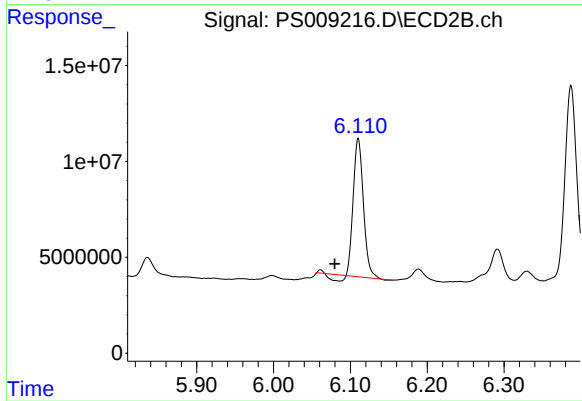

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.110 min
Delta R.T.: 0.031 min
Response: 63514956
Conc: 78.09 ng/ml

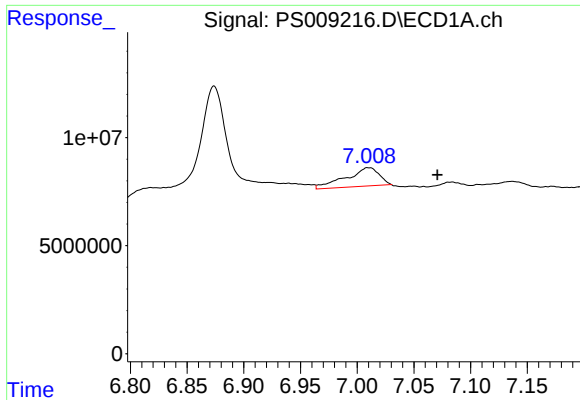

#3 4-Nitrophenol


R.T.: 7.010 min
Delta R.T.: -0.061 min
Response: 17461490
Conc: 73.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

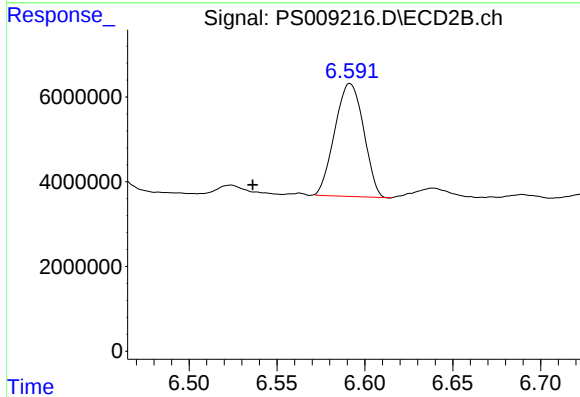


#3 4-Nitrophenol

R.T.: 6.592 min
Delta R.T.: 0.055 min
Response: 30394014
Conc: 95.52 ng/ml

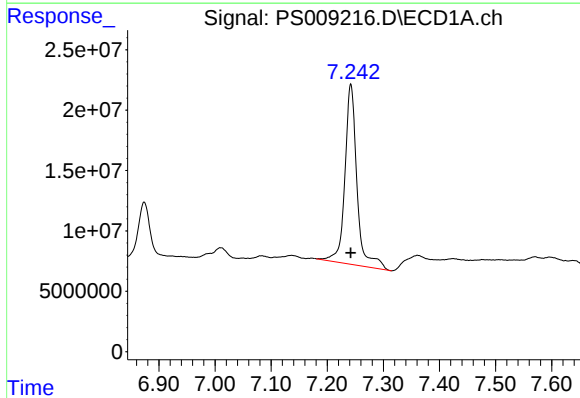


#4 2,4-DCAA

R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 222734482
Conc: 402.65 ng/ml

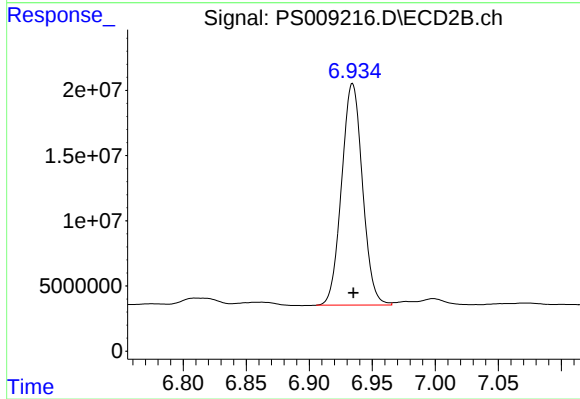

#4 2,4-DCAA


R.T.: 6.934 min
Delta R.T.: 0.000 min
Response: 196293644
Conc: 357.42 ng/ml

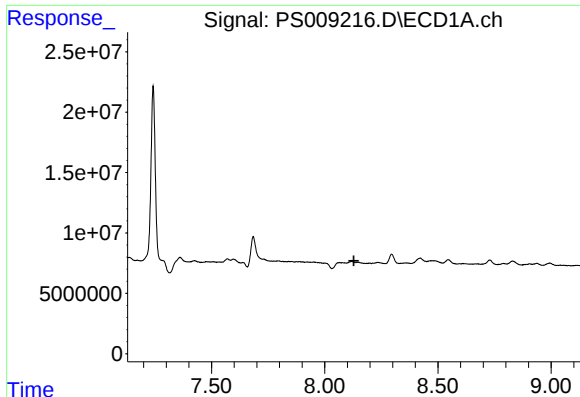

#8 DICHLORPROP


R.T.: 8.119 min
Delta R.T.: -0.010 min
Response: -1202333
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

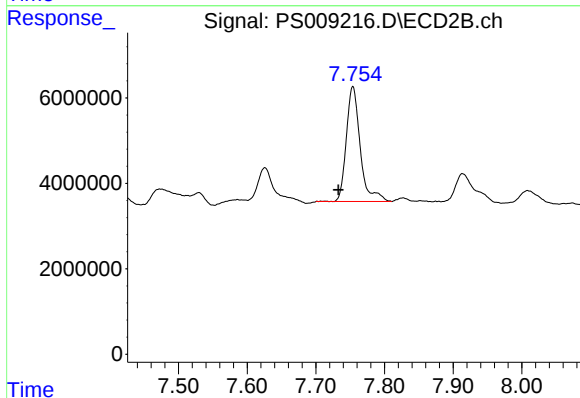


#8 DICHLORPROP

R.T.: 7.754 min
Delta R.T.: 0.021 min
Response: 37825874
Conc: 68.18 ng/ml

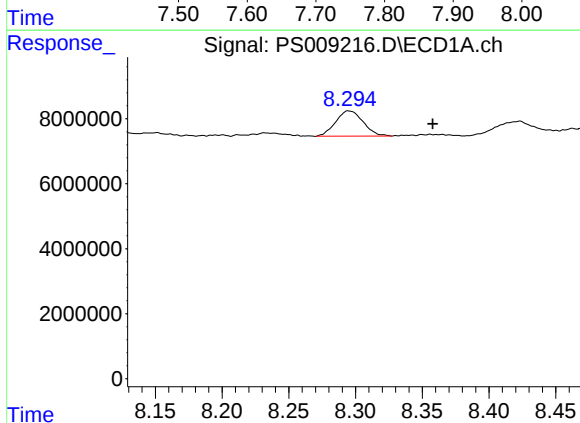


#9 2,4-D

R.T.: 8.295 min
Delta R.T.: -0.062 min
Response: 11151989
Conc: 21.15 ng/ml

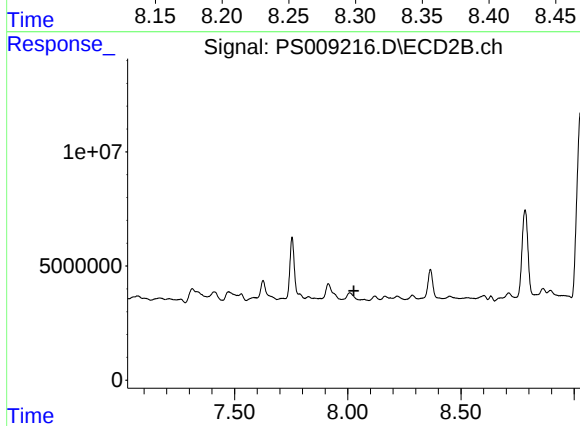

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.027 min
Response: 0
Conc: N.D.

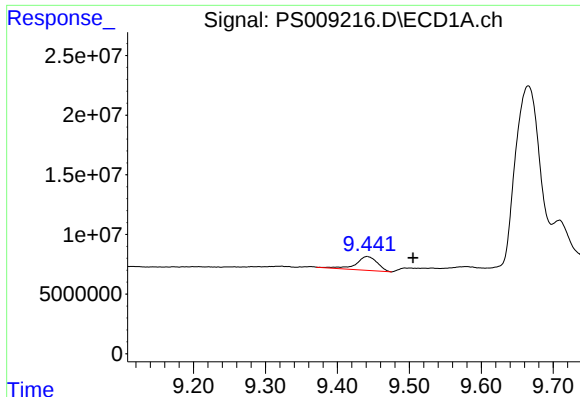

#12 2,4,5-T


R.T.: 9.441 min
Delta R.T.: -0.064 min
Response: 24004224
Conc: 9.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

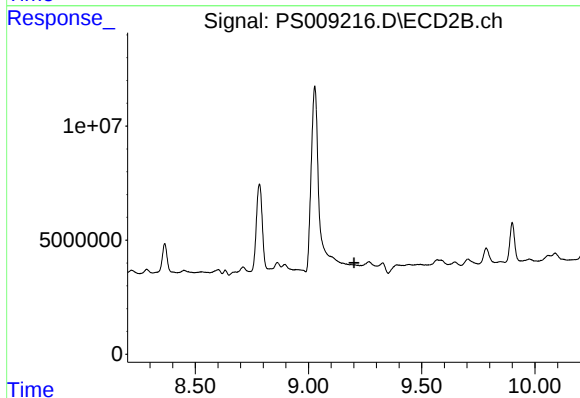


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.201 min
Response: 0
Conc: N.D.

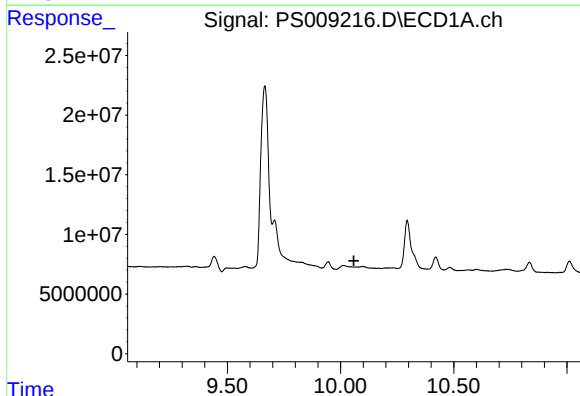


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.059 min
Response: 0
Conc: N.D.

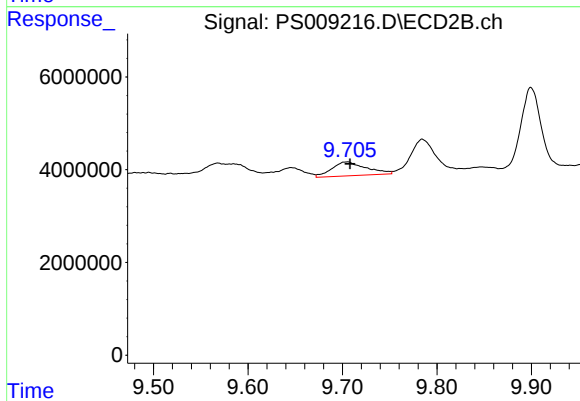

#13 2,4-DB


R.T.: 9.704 min
Delta R.T.: -0.004 min
Response: 7610926
Conc: 20.05 ng/ml

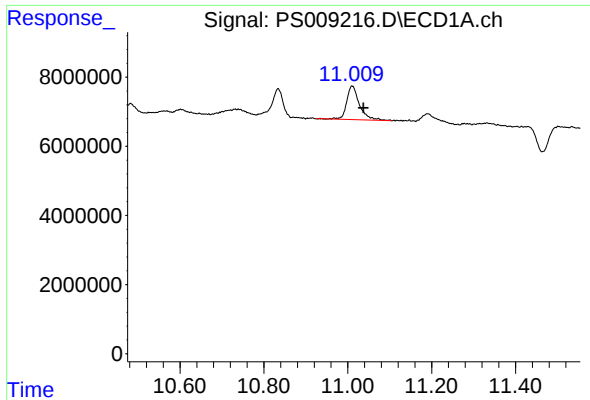

#15 Picloram

R.T.: 11.011 min
Delta R.T.: -0.027 min
Response: 20533072
Conc: 6.77 ng/ml

Instrument :
ECD_S
ClientSampleId :

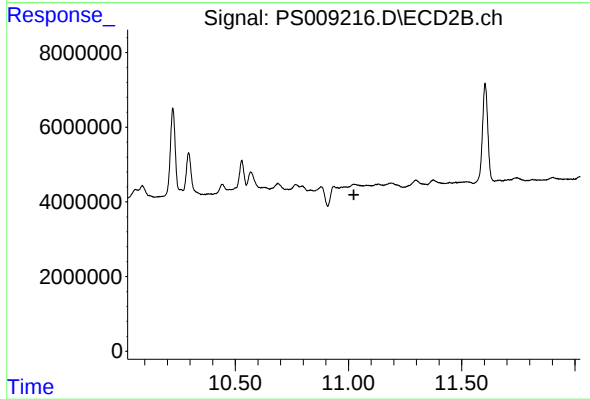

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.023 min
Response: 0
Conc: N.D.