

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031220\
 Data File : PS009228.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2020 20:36
 Operator : DD\AJ
 Sample : L1755-04
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 04:22:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.242	6.934	236.4E6	208.0E6	427.306	378.794
Target Compounds							
1) T	Dalapon	3.008	2.589	19932967	121.7E6	25.561	154.514 #
2) T	3,5-DICHL...	0.000	6.110	0	80610203	N.D.	99.114
3) T	4-Nitroph...	7.010	6.592	20252717	21785942	84.841	68.467
8) T	DICHLORPROP	8.118	7.753	3440795	38852341	6.672	70.027 #
9) T	2,4-D	8.295	0.000	7536040	0	14.294	N.D. #
10) T	Pentachlo...	8.669	8.458	13966619	15886336	1.986	2.093
12) T	2,4,5-T	9.443	0.000	25874532	0	10.171	N.D. #
13) T	2,4-DB	0.000	9.703	0	6519244	N.D.	17.173
15) T	Picloram	11.012	0.000	11647283	0	3.838	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031220\
Data File : PS009228.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2020 20:36
Operator : DD\AJ
Sample : L1755-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 04:22:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

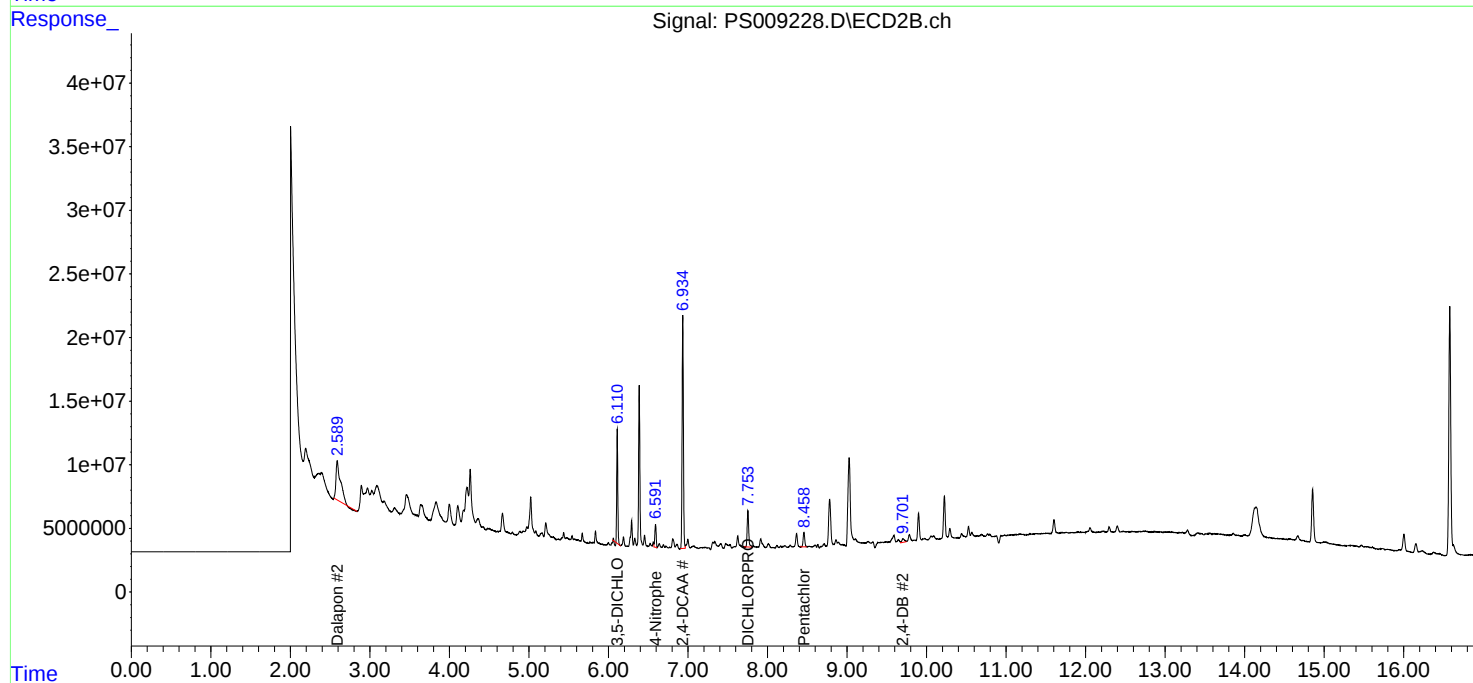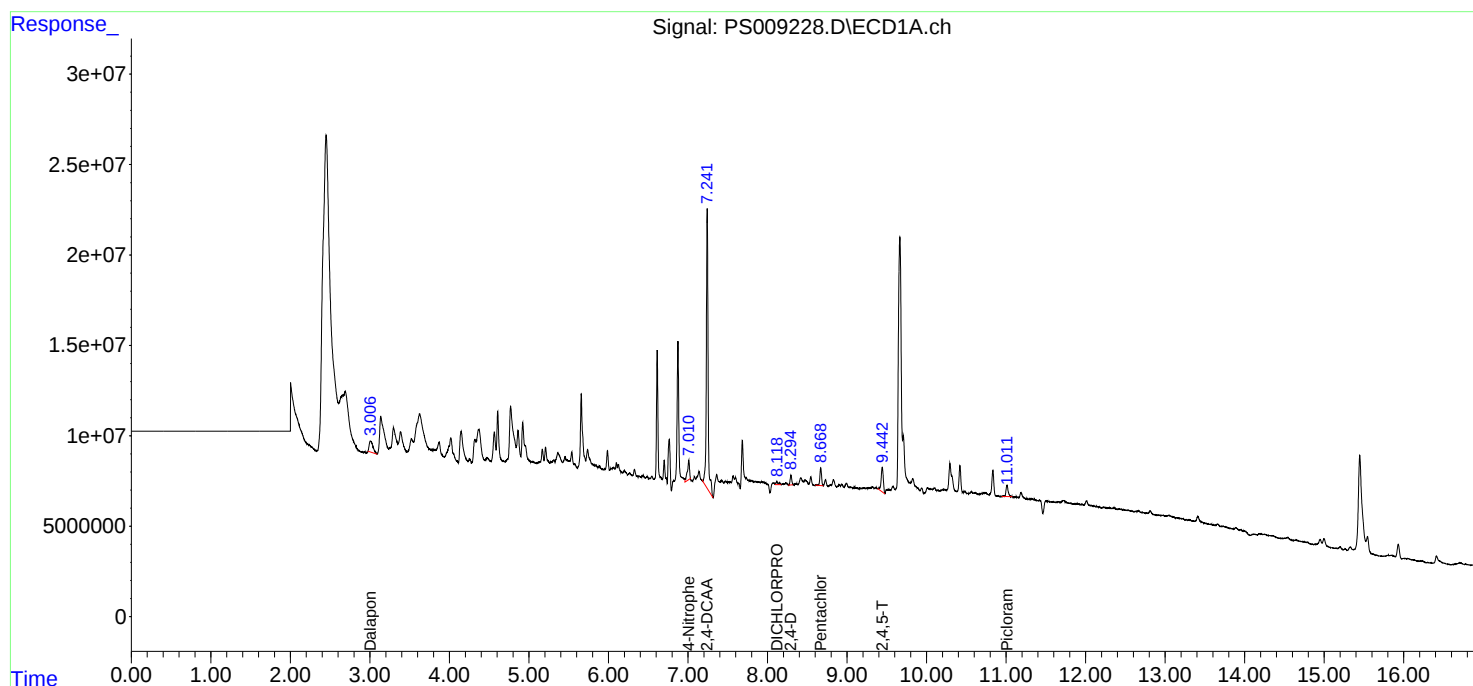


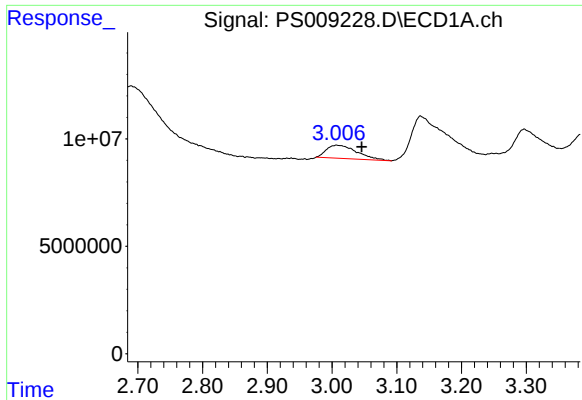

#1 Dalapon


R.T.: 3.008 min
Delta R.T.: -0.038 min
Response: 19932967
Conc: 25.56 ng/ml

Instrument :
ECD_S
ClientSampleId :

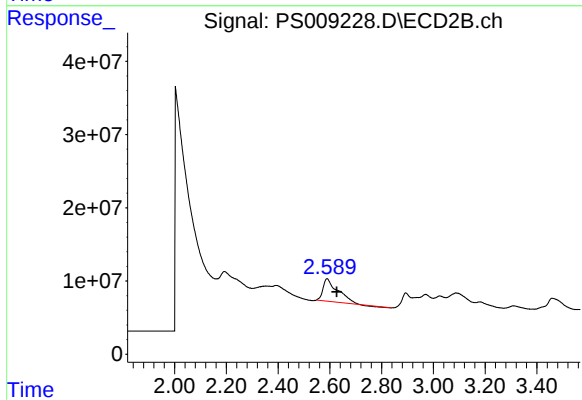


#1 Dalapon

R.T.: 2.589 min
Delta R.T.: -0.037 min
Response: 121658276
Conc: 154.51 ng/ml

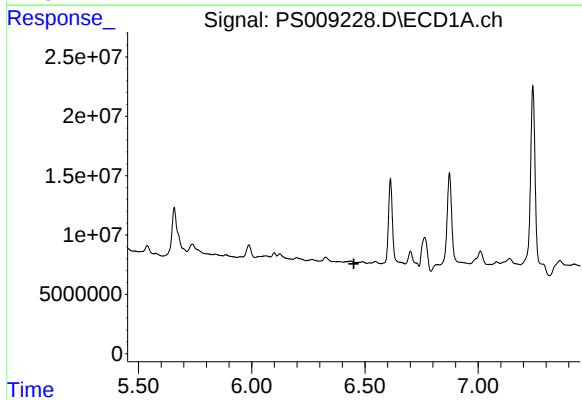


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

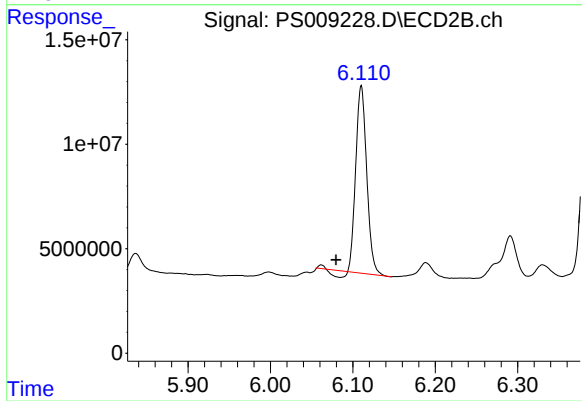

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.110 min
Delta R.T.: 0.031 min
Response: 80610203
Conc: 99.11 ng/ml

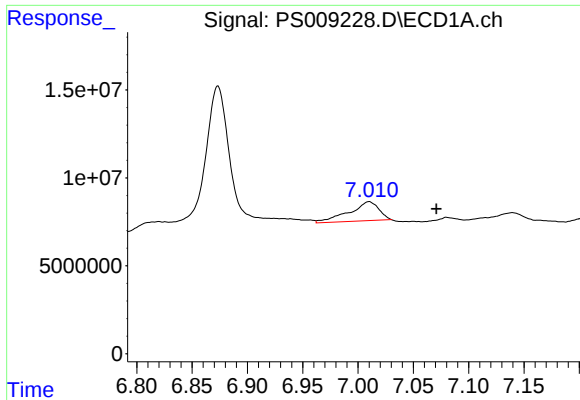

#3 4-Nitrophenol


R.T.: 7.010 min
Delta R.T.: -0.061 min
Response: 20252717
Conc: 84.84 ng/ml

Instrument :
ECD_S
ClientSampleId :

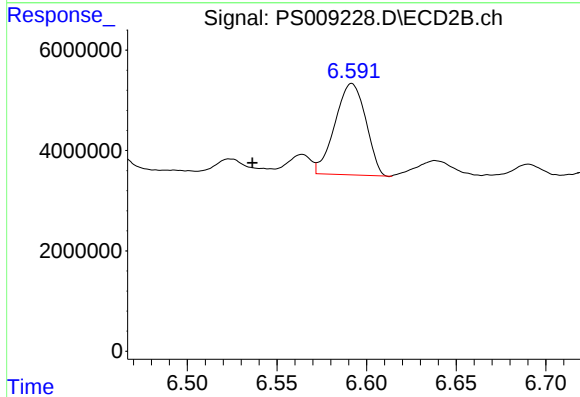


#3 4-Nitrophenol

R.T.: 6.592 min
Delta R.T.: 0.056 min
Response: 21785942
Conc: 68.47 ng/ml

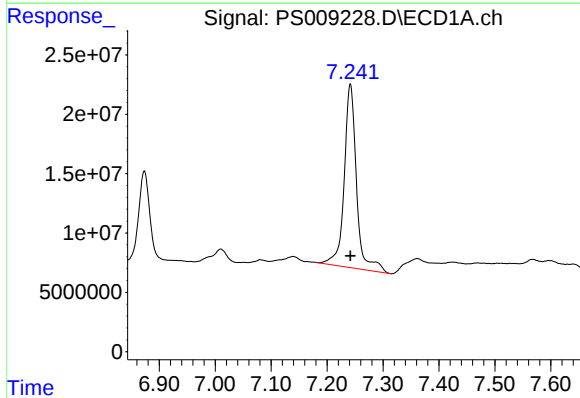


#4 2,4-DCAA

R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 236372923
Conc: 427.31 ng/ml

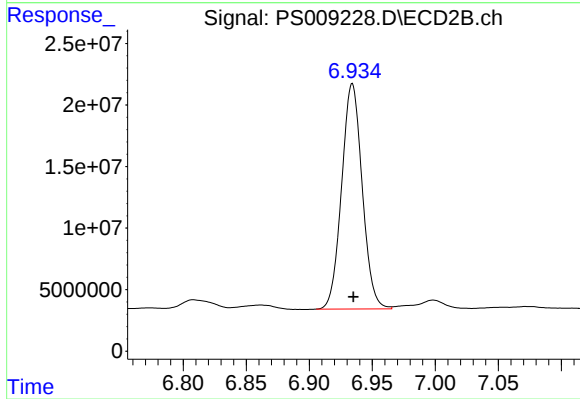

#4 2,4-DCAA


R.T.: 6.934 min
Delta R.T.: 0.000 min
Response: 208032845
Conc: 378.79 ng/ml

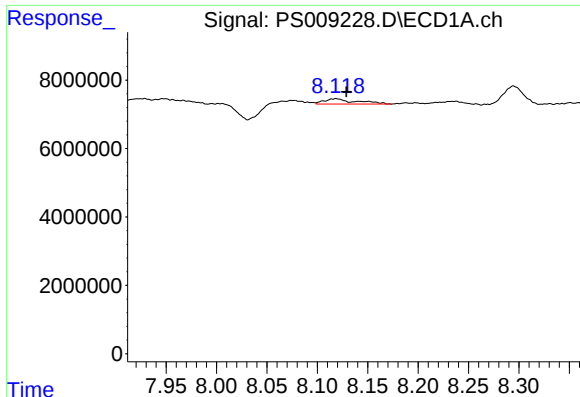

#8 DICHLORPROP


R.T.: 8.118 min
Delta R.T.: -0.011 min
Response: 3440795
Conc: 6.67 ng/ml

Instrument :
ECD_S
ClientSampleId :

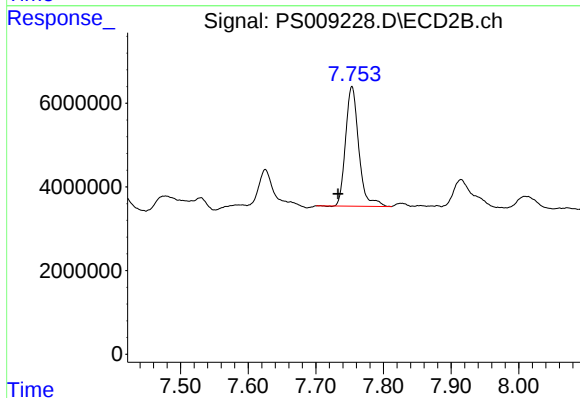


#8 DICHLORPROP

R.T.: 7.753 min
Delta R.T.: 0.020 min
Response: 38852341
Conc: 70.03 ng/ml

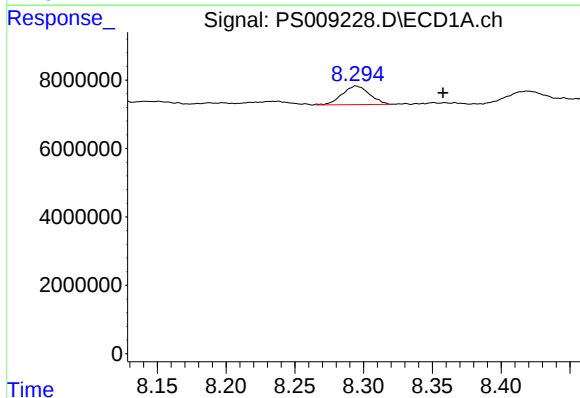


#9 2,4-D

R.T.: 8.295 min
Delta R.T.: -0.063 min
Response: 7536040
Conc: 14.29 ng/ml

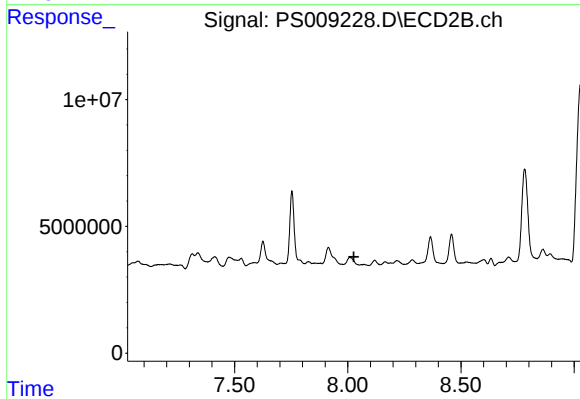

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.027 min
Response: 0
Conc: N.D.

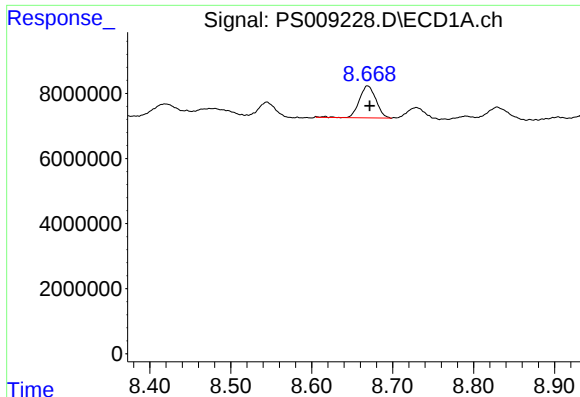

#10 Pentachlorophenol


R.T.: 8.669 min
Delta R.T.: -0.003 min
Response: 13966619
Conc: 1.99 ng/ml

Instrument :
ECD_S
ClientSampleId :

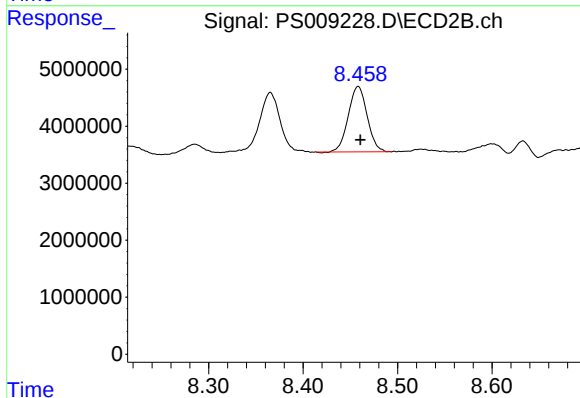


#10 Pentachlorophenol

R.T.: 8.458 min
Delta R.T.: -0.002 min
Response: 15886336
Conc: 2.09 ng/ml

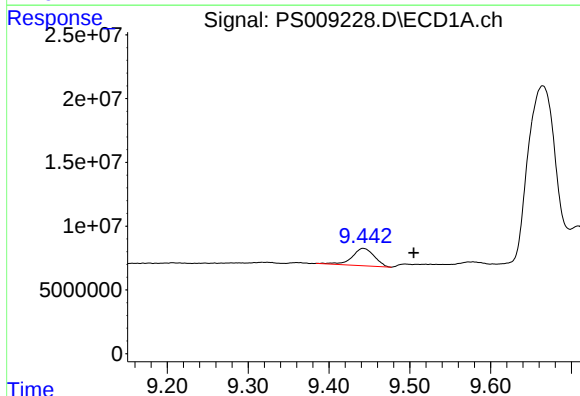


#12 2,4,5-T

R.T.: 9.443 min
Delta R.T.: -0.062 min
Response: 25874532
Conc: 10.17 ng/ml

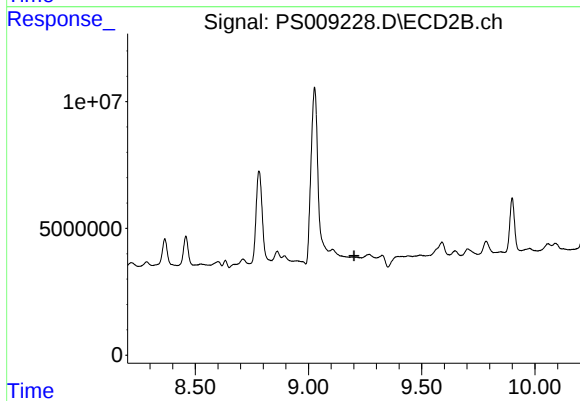

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.201 min
Response: 0
Conc: N.D.

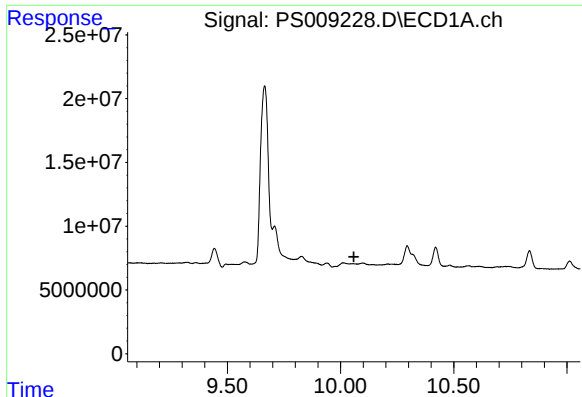

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.059 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

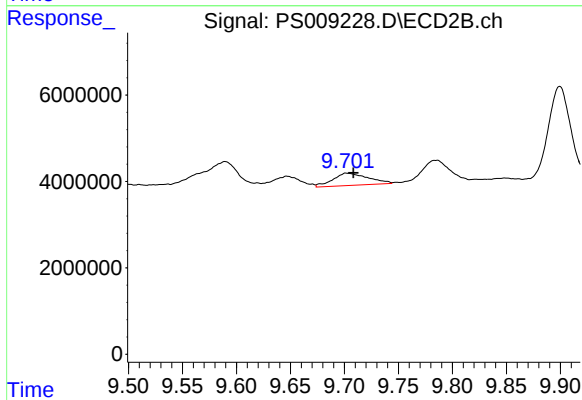


#13 2,4-DB

R.T.: 9.703 min
Delta R.T.: -0.005 min
Response: 6519244
Conc: 17.17 ng/ml

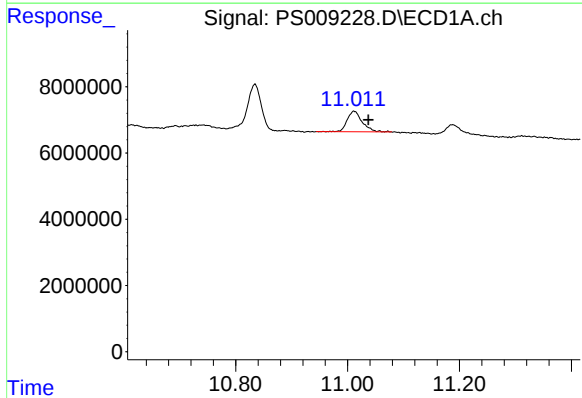

#15 Picloram

R.T.: 11.012 min
Delta R.T.: -0.026 min
Response: 11647283
Conc: 3.84 ng/ml

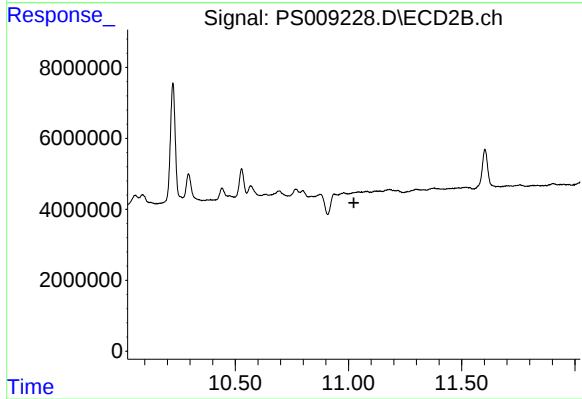

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 11.023 min
Response: 0
Conc: N.D.