

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031220\
 Data File : PS009234.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2020 23:16
 Operator : DD\AJ
 Sample : PB127461BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 04:24:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.241	6.934	325.8E6	305.1E6	588.994	555.459
Target Compounds							
1) T	Dalapon	3.004	2.587	20199179	196.9E6	25.902	250.129 #
2) T	3,5-DICHL...	0.000	6.110	0	65149512	N.D.	80.104
3) T	4-Nitroph...	7.011	6.593	15946120	16857069	66.800	52.977
7) T	MCPA	7.793	7.401	11073722	62956259	3.636	23.329 #
8) T	DICHLORPROP	8.118	7.754	156178	39834969	<MDL	71.798 #
11) T	2,4,5-TP ...	0.000	8.787	0	28795577	N.D.	9.659
13) T	2,4-DB	0.000	9.703	0	8865014	N.D.	23.353
14) T	DINOSEB	0.000	10.047	0	14234212	N.D.	6.480
15) T	Picloram	11.013	11.022	10231978	12641343	3.371	3.104
16) T	DCPA	0.000	10.973	0	25678826	N.D.	6.630



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031220\
Data File : PS009234.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2020 23:16
Operator : DD\AJ
Sample : PB127461BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 04:24:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

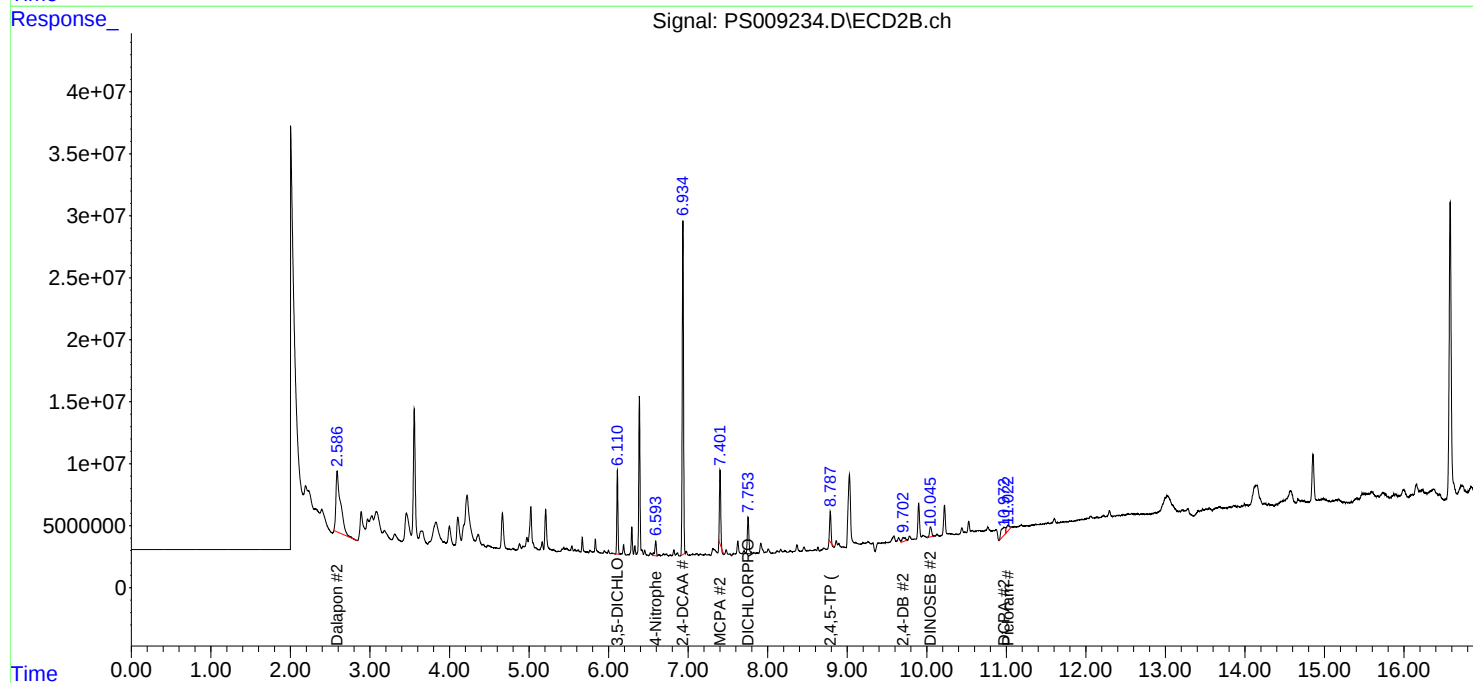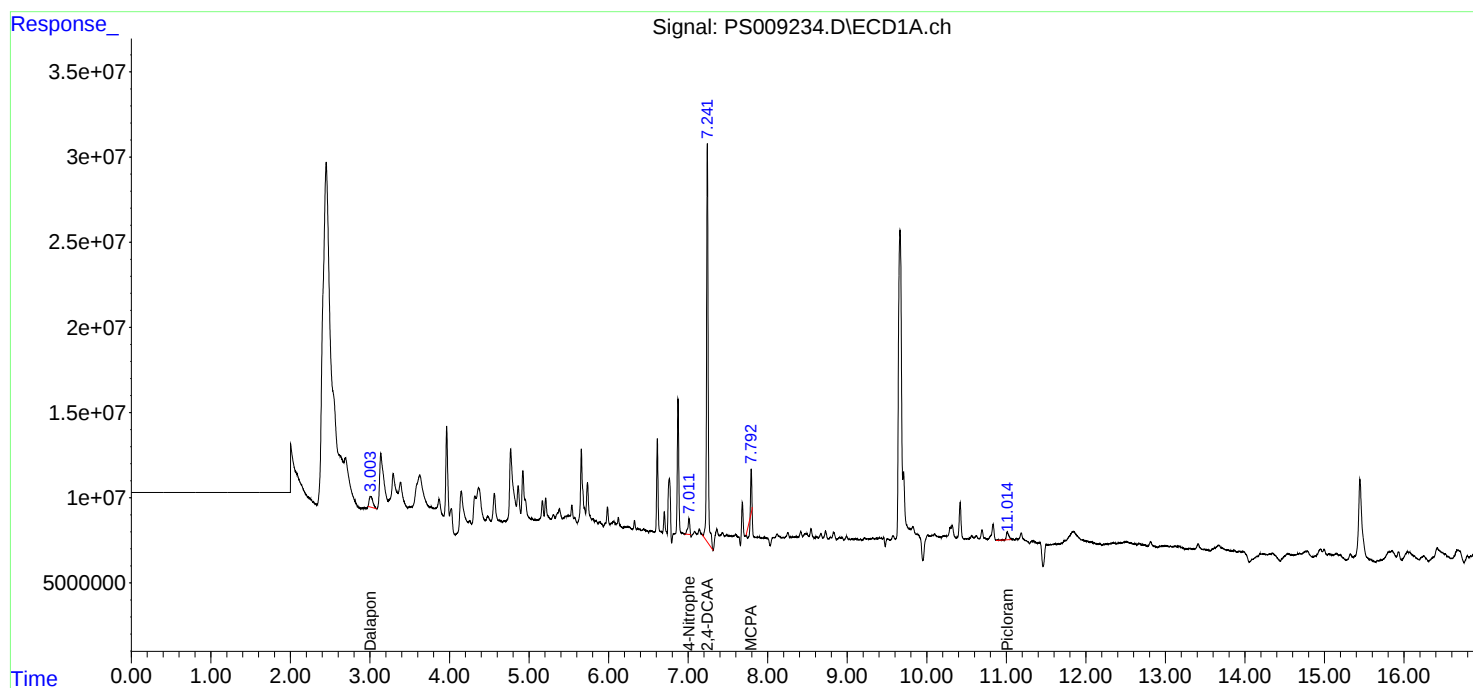


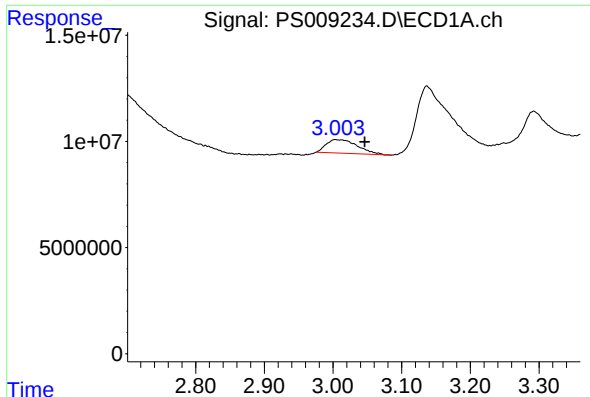

#1 Dalapon


R.T.: 3.004 min
Delta R.T.: -0.042 min
Response: 20199179
Conc: 25.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

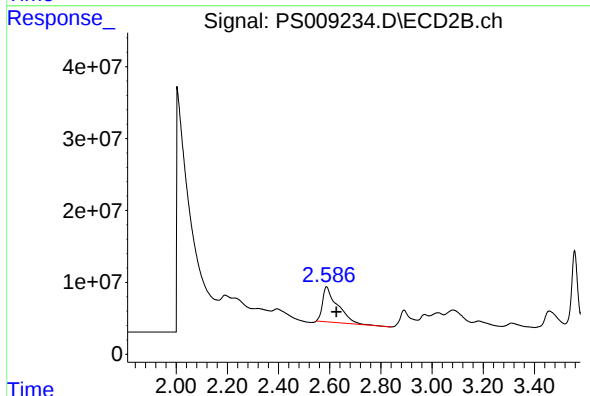


#1 Dalapon

R.T.: 2.587 min
Delta R.T.: -0.039 min
Response: 196941965
Conc: 250.13 ng/ml

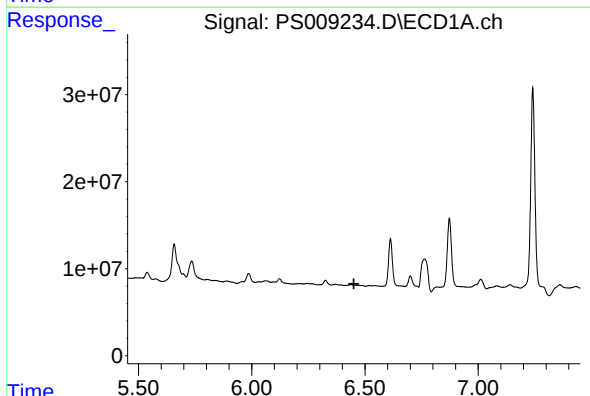


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

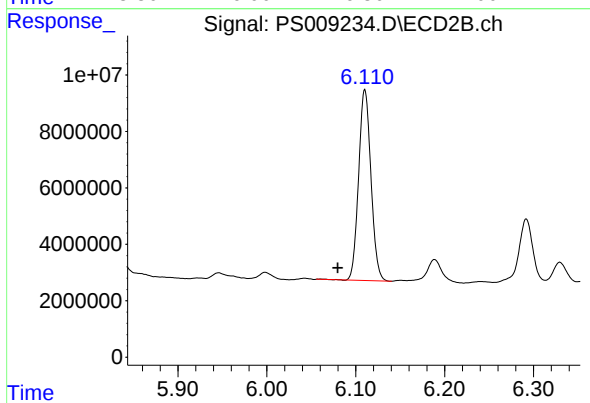

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.110 min
Delta R.T.: 0.031 min
Response: 65149512
Conc: 80.10 ng/ml

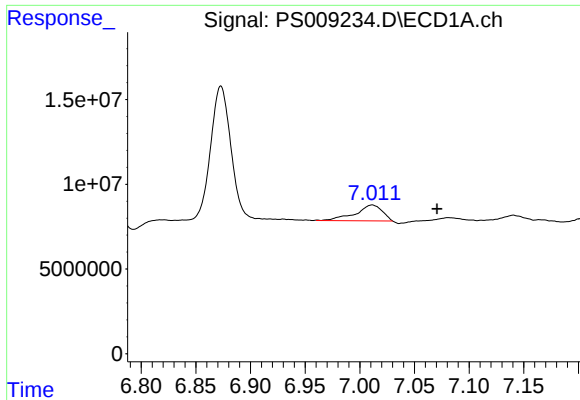

#3 4-Nitrophenol


R.T.: 7.011 min
Delta R.T.: -0.059 min
Response: 15946120
Conc: 66.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

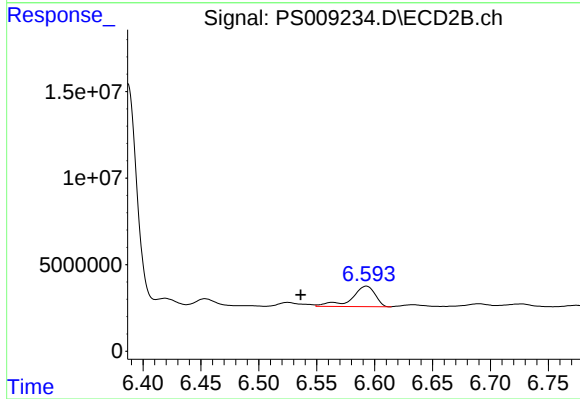


#3 4-Nitrophenol

R.T.: 6.593 min
Delta R.T.: 0.056 min
Response: 16857069
Conc: 52.98 ng/ml

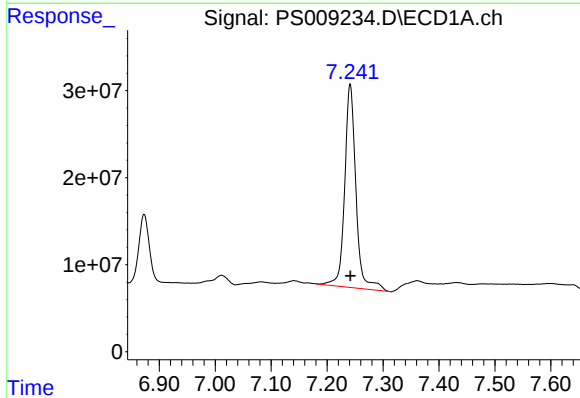


#4 2,4-DCAA

R.T.: 7.241 min
Delta R.T.: 0.000 min
Response: 325813966
Conc: 588.99 ng/ml

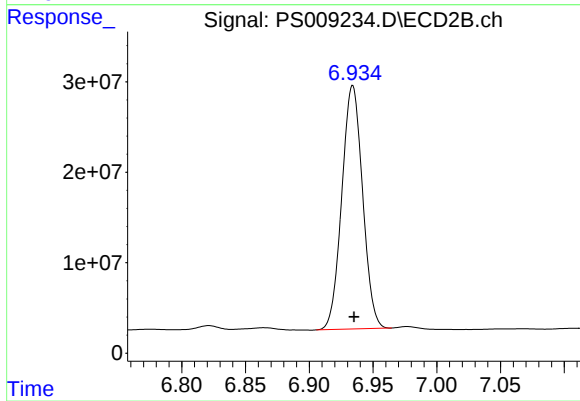

#4 2,4-DCAA


R.T.: 6.934 min
Delta R.T.: -0.001 min
Response: 305056807
Conc: 555.46 ng/ml

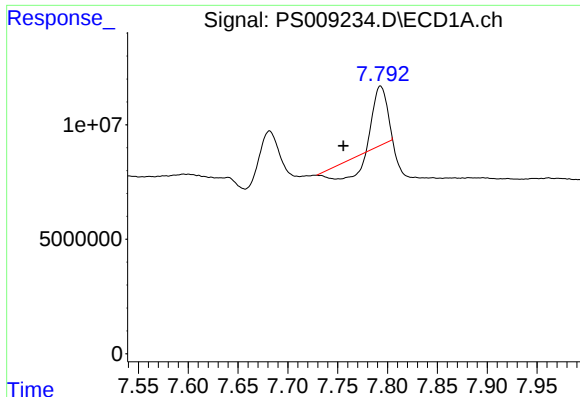

#7 MCPA


R.T.: 7.793 min
Delta R.T.: 0.038 min
Response: 11073722
Conc: 3.64 ug/ml

Instrument :
ECD_S
ClientSampleId :

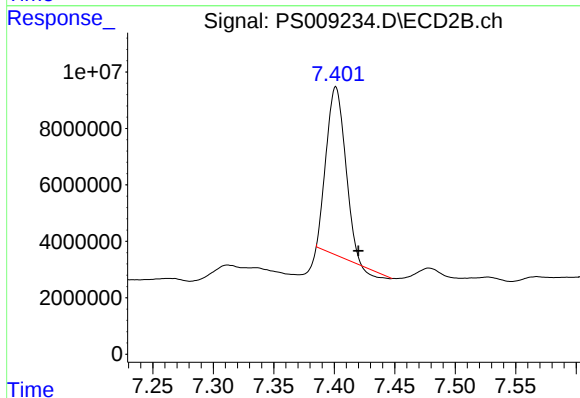


#7 MCPA

R.T.: 7.401 min
Delta R.T.: -0.019 min
Response: 62956259
Conc: 23.33 ug/ml

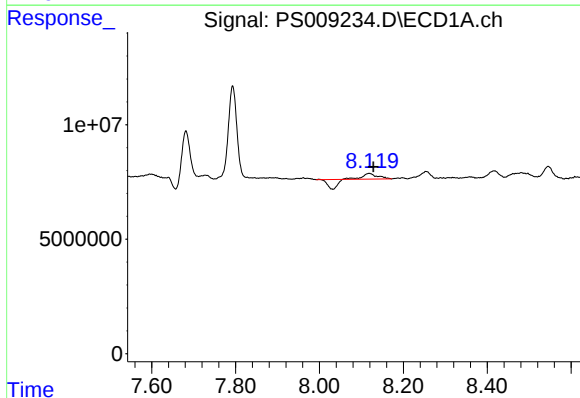


#8 DICHLORPROP

R.T.: 8.118 min
Delta R.T.: -0.011 min
Response: 156178
Conc: N.D.

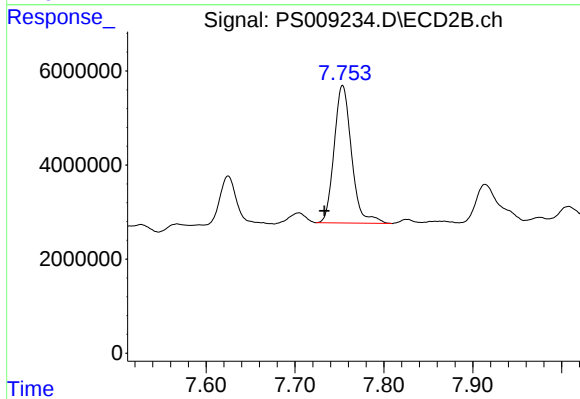

#8 DICHLORPROP


R.T.: 7.754 min
Delta R.T.: 0.021 min
Response: 39834969
Conc: 71.80 ng/ml

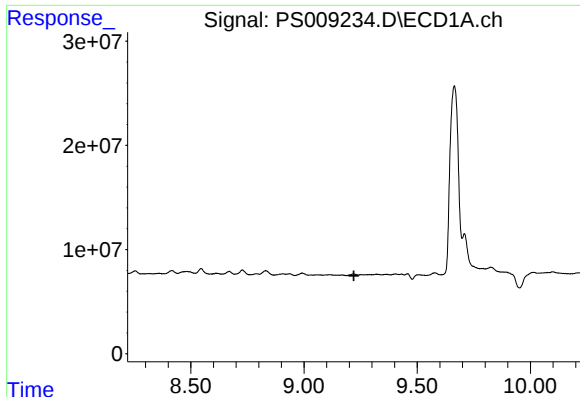

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.221 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

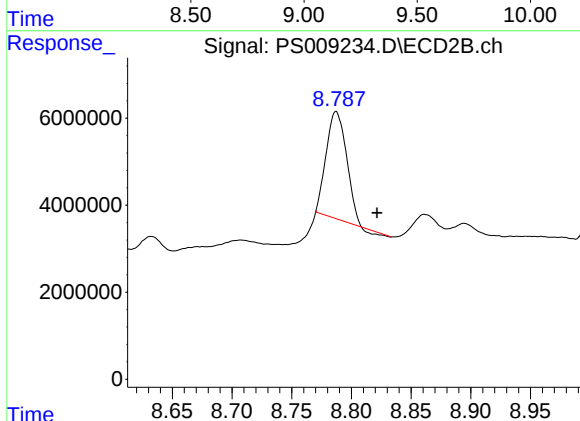


#11 2,4,5-TP (SILVEX)

R.T.: 8.787 min
Delta R.T.: -0.034 min
Response: 28795577
Conc: 9.66 ng/ml

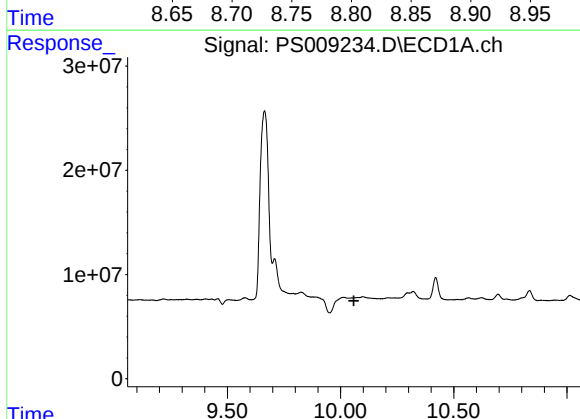


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 10.059 min
Response: 0
Conc: N.D.

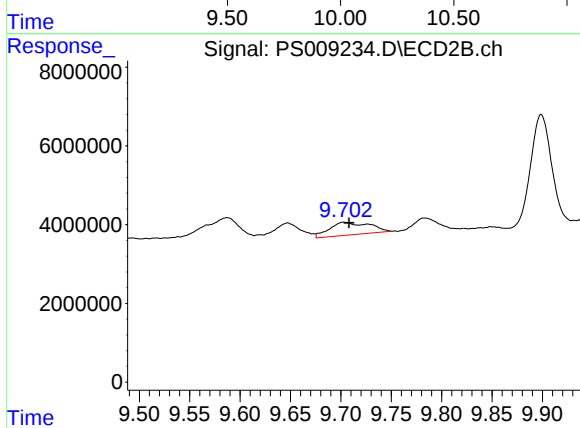

#13 2,4-DB


R.T.: 9.703 min
Delta R.T.: -0.005 min
Response: 8865014
Conc: 23.35 ng/ml

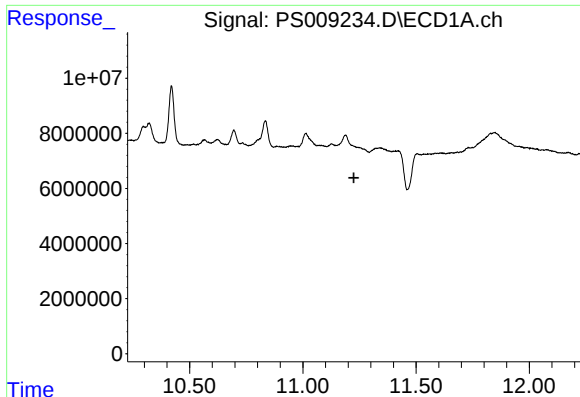

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 11.225 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

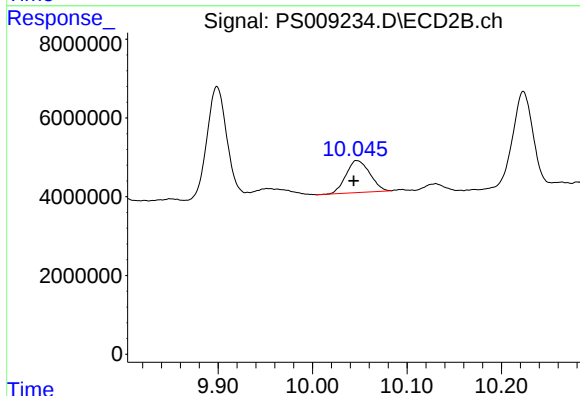


#14 DINOSEB

R.T.: 10.047 min
Delta R.T.: 0.004 min
Response: 14234212
Conc: 6.48 ng/ml

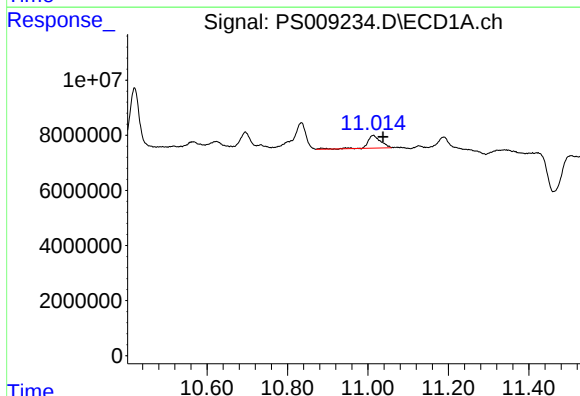


#15 Picloram

R.T.: 11.013 min
Delta R.T.: -0.025 min
Response: 10231978
Conc: 3.37 ng/ml

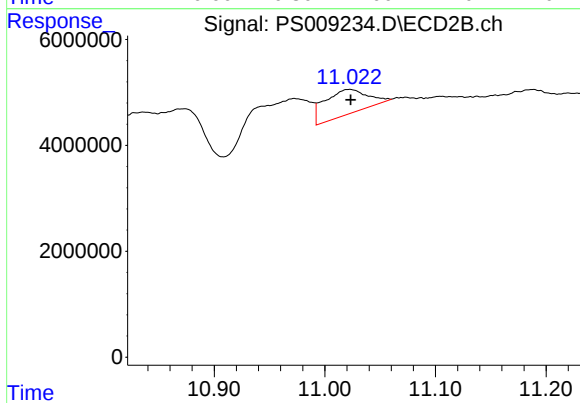

#15 Picloram


R.T.: 11.022 min
Delta R.T.: -0.001 min
Response: 12641343
Conc: 3.10 ng/ml

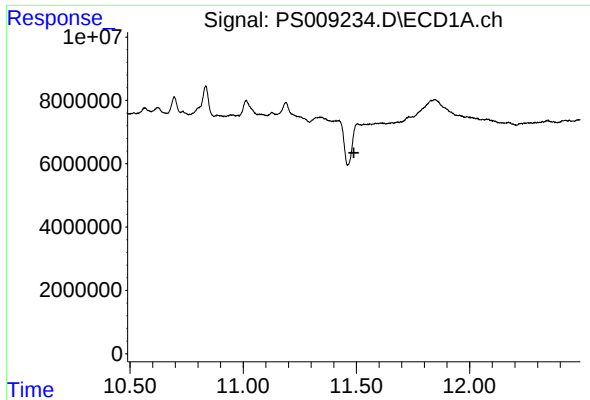

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.489 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

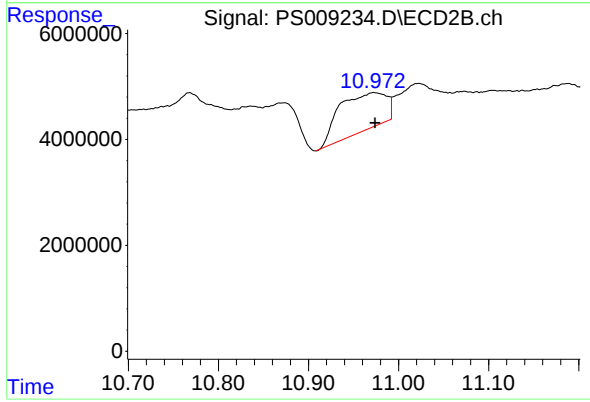

#16 DCPA

R.T.: 10.973 min
Delta R.T.: -0.001 min
Response: 25678826
Conc: 6.63 ng/ml