

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031220\
 Data File : PS009236.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2020 00:02
 Operator : DD\AJ
 Sample : PB127461TB
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 04:24:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.242	6.934	245.7E6	219.0E6	444.098	398.824
Target Compounds							
1) T	Dalapon	3.006	2.589	21579271	150.3E6	27.672	190.913 #
2) T	3,5-DICHL...	0.000	6.110	0	74801834	N.D.	91.972
3) T	4-Nitroph...	7.010	6.592	18628074	18458090	78.036	58.008 #
7) T	MCPA	0.000	7.467	0	18576066	N.D.	6.884
8) T	DICHLORPROP	8.120	7.753	-2368536	46680319	N.D.	84.136
10) T	Pentachlo...	0.000	8.458	0	7823669	N.D.	1.031
12) T	2,4,5-T	9.444	0.000	30418796	0	11.958	N.D. #
13) T	2,4-DB	0.000	9.704	0	6962360	N.D.	18.341
15) T	Picloram	11.013	11.022	14552189	5333819	4.795	1.310 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031220\
Data File : PS009236.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2020 00:02
Operator : DD\AJ
Sample : PB127461TB
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 04:24:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

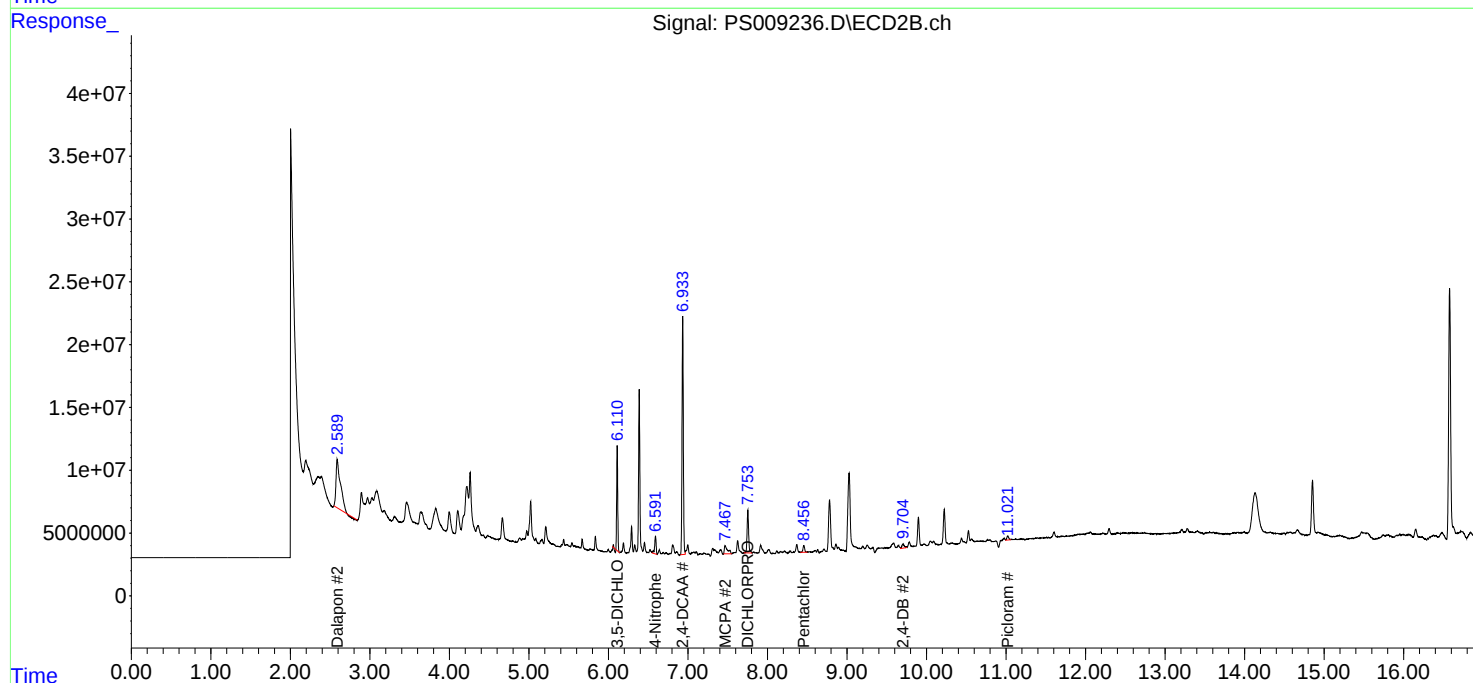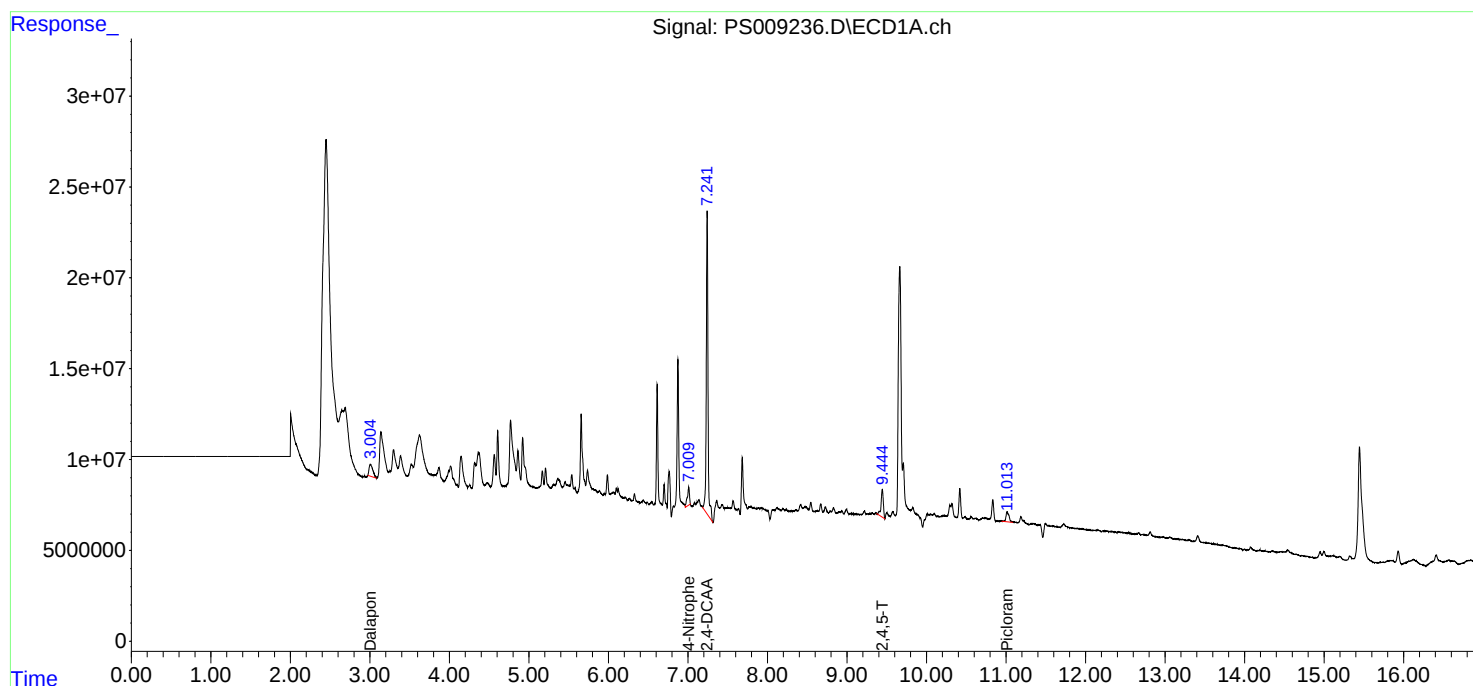


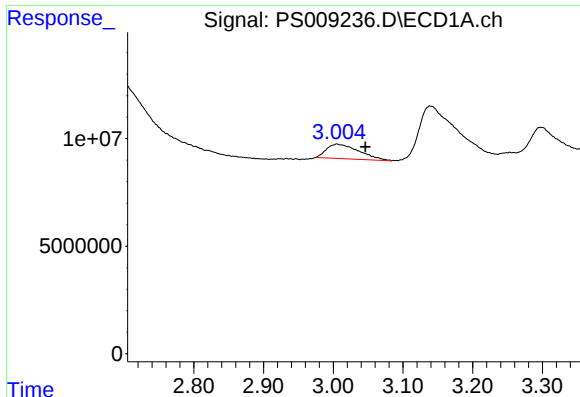

#1 Dalapon


R.T.: 3.006 min
Delta R.T.: -0.040 min
Response: 21579271
Conc: 27.67 ng/ml

Instrument :
ECD_S
ClientSampleId :

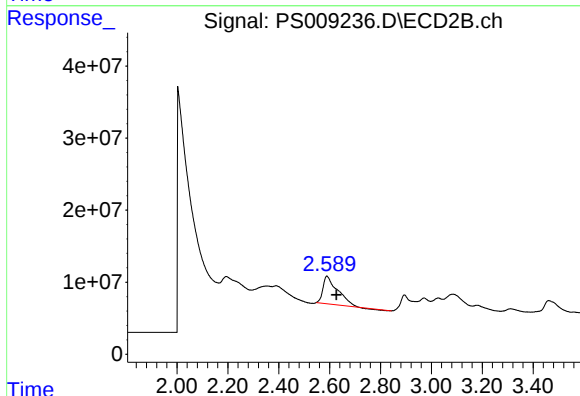


#1 Dalapon

R.T.: 2.589 min
Delta R.T.: -0.037 min
Response: 150317369
Conc: 190.91 ng/ml

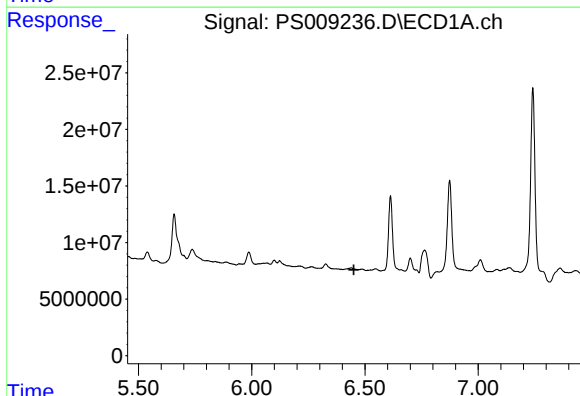


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

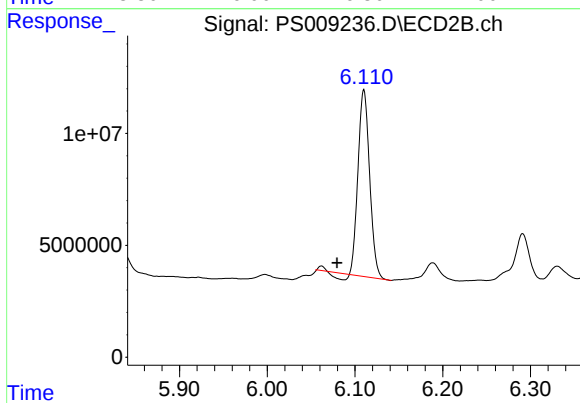

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.110 min
Delta R.T.: 0.030 min
Response: 74801834
Conc: 91.97 ng/ml

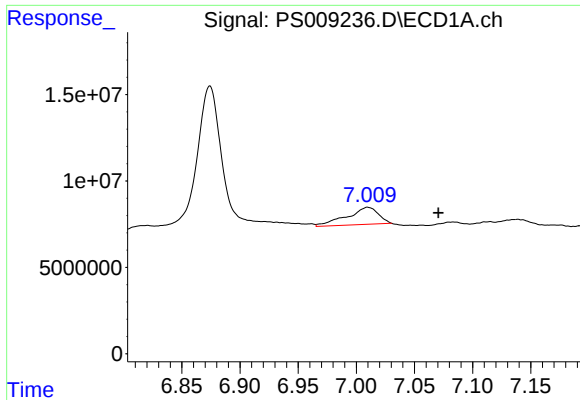

#3 4-Nitrophenol


R.T.: 7.010 min
Delta R.T.: -0.061 min
Response: 18628074
Conc: 78.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

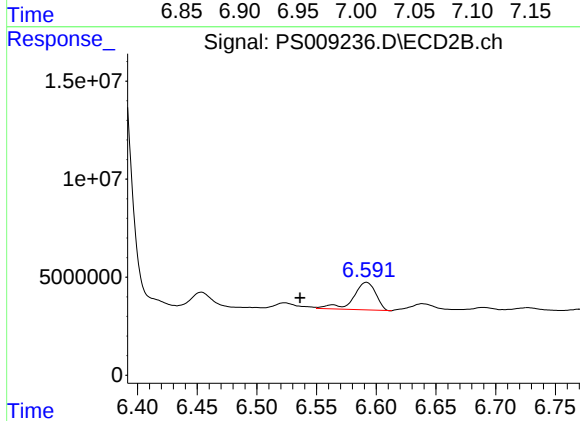


#3 4-Nitrophenol

R.T.: 6.592 min
Delta R.T.: 0.056 min
Response: 18458090
Conc: 58.01 ng/ml

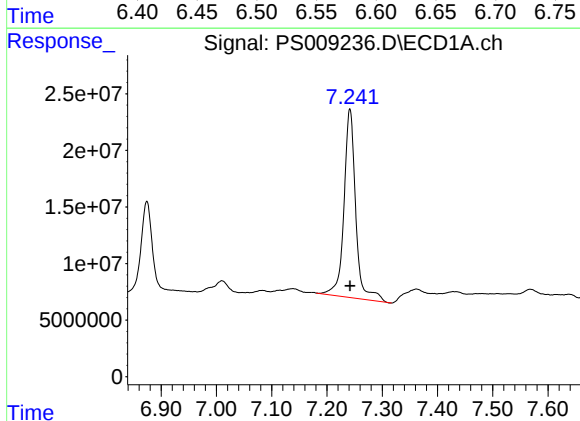


#4 2,4-DCAA

R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 245661708
Conc: 444.10 ng/ml

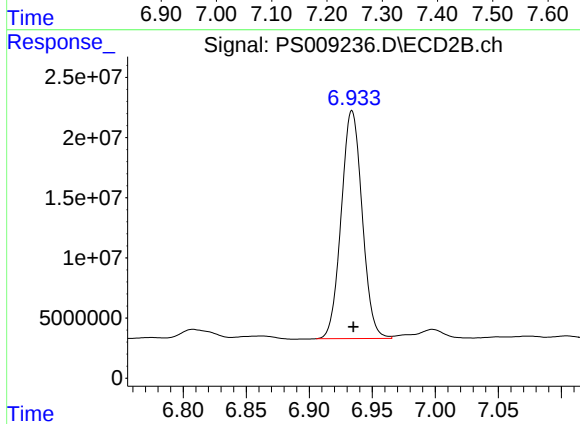

#4 2,4-DCAA


R.T.: 6.934 min
Delta R.T.: -0.001 min
Response: 219033273
Conc: 398.82 ng/ml

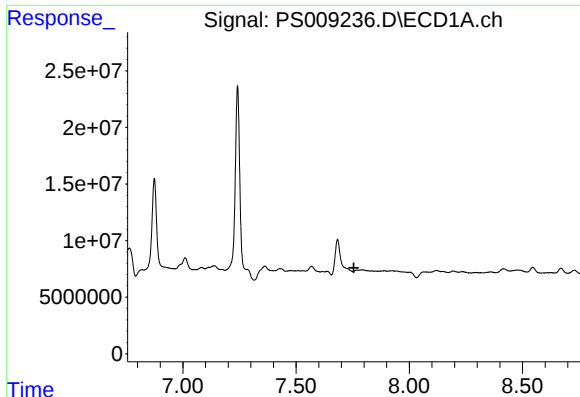

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.756 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

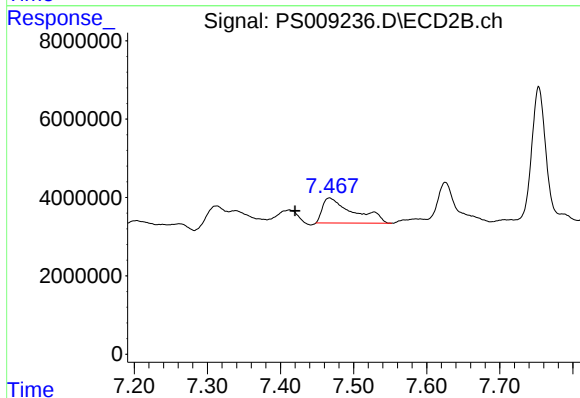


#7 MCPA

R.T.: 7.467 min
Delta R.T.: 0.047 min
Response: 18576066
Conc: 6.88 ug/ml

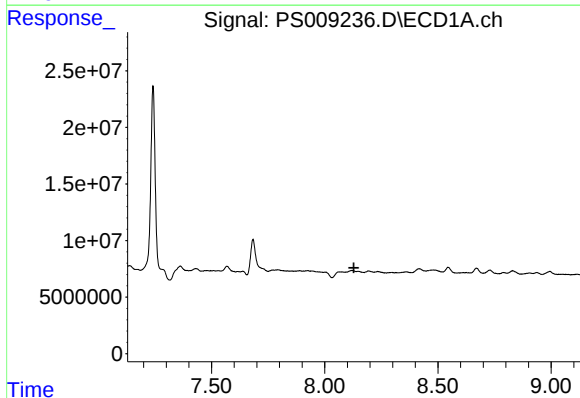


#8 DICHLORPROP

R.T.: 8.120 min
Delta R.T.: -0.009 min
Response: -2368536
Conc: N.D.

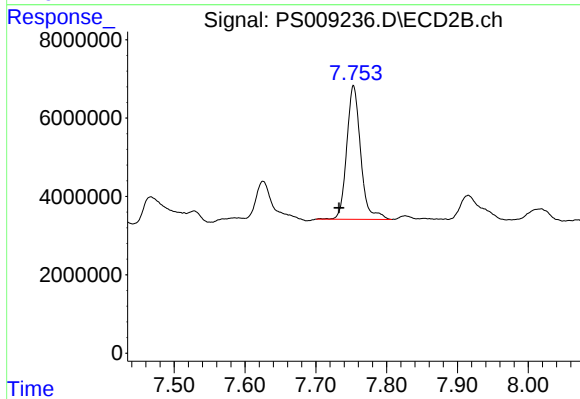

#8 DICHLORPROP


R.T.: 7.753 min
Delta R.T.: 0.020 min
Response: 46680319
Conc: 84.14 ng/ml

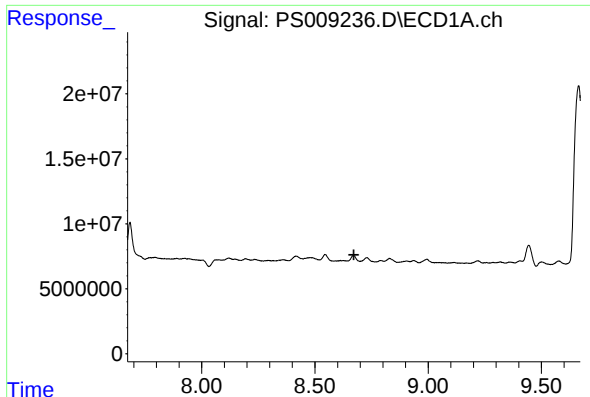

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 8.672 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

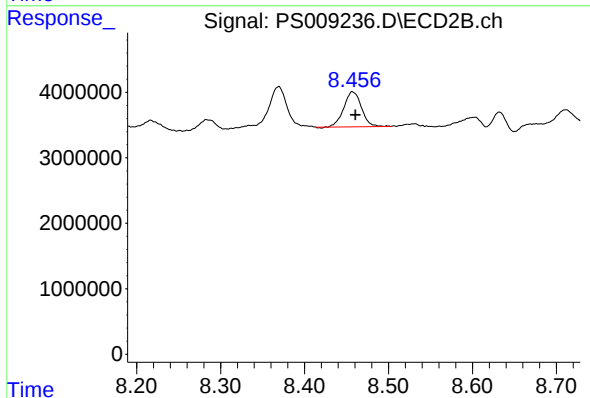


#10 Pentachlorophenol

R.T.: 8.458 min
Delta R.T.: -0.003 min
Response: 7823669
Conc: 1.03 ng/ml

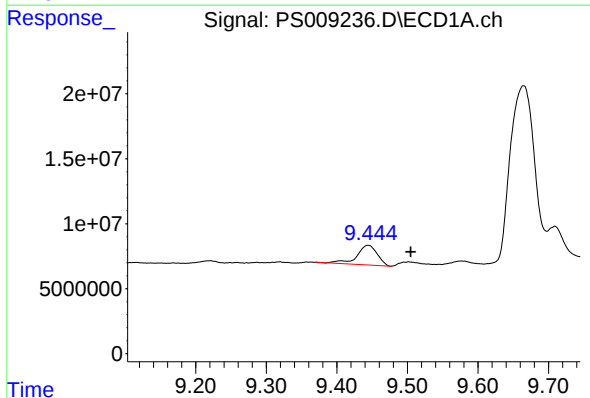


#12 2,4,5-T

R.T.: 9.444 min
Delta R.T.: -0.061 min
Response: 30418796
Conc: 11.96 ng/ml

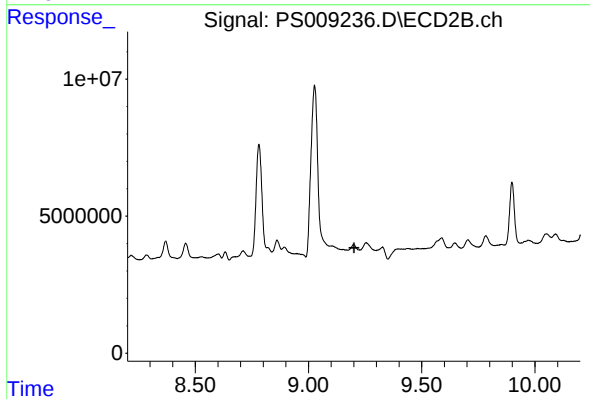

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.201 min
Response: 0
Conc: N.D.

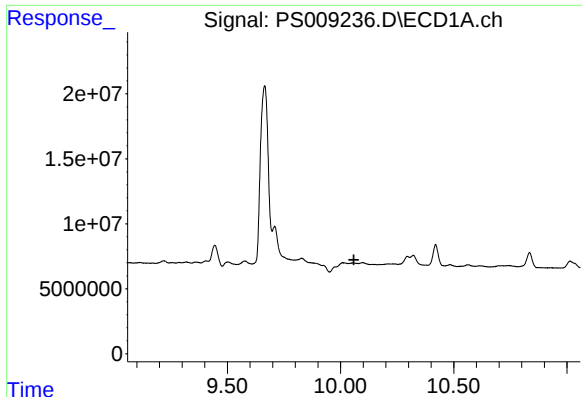

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.059 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

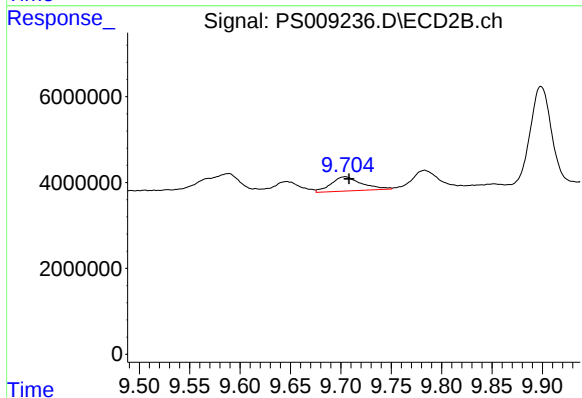


#13 2,4-DB

R.T.: 9.704 min
Delta R.T.: -0.004 min
Response: 6962360
Conc: 18.34 ng/ml

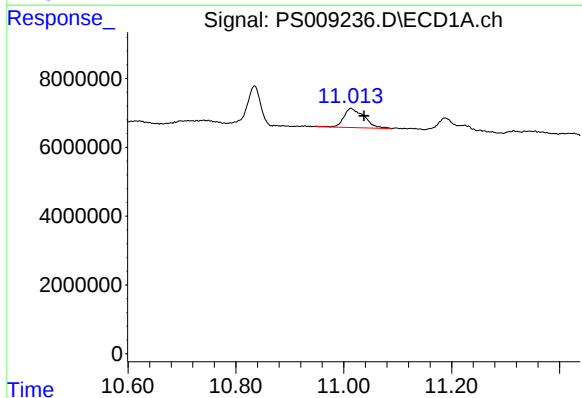

#15 Picloram

R.T.: 11.013 min
Delta R.T.: -0.024 min
Response: 14552189
Conc: 4.79 ng/ml

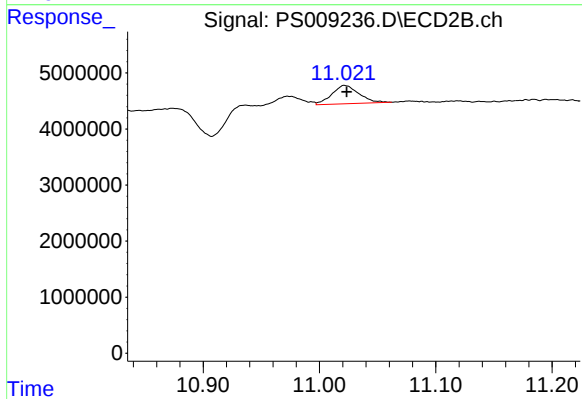

#15 Picloram

R.T.: 11.022 min
Delta R.T.: -0.001 min
Response: 5333819
Conc: 1.31 ng/ml