

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031220\
 Data File : PS009240.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2020 01:34
 Operator : DD\AJ
 Sample : L1853-03
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 04:25:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.242	6.934	263.8E6	230.5E6	476.826	419.697
Target Compounds							
1) T	Dalapon	3.005	2.590	21851694	199.7E6	28.021	253.658 #
2) T	3,5-DICHL...	0.000	6.110	0	77862065	N.D.	95.735
3) T	4-Nitroph...	7.011	6.564	19233316	3662856	80.571	11.511 #
5) T	DICAMBA	7.456	0.000	20114624	0	9.452	N.D. #
8) T	DICHLORPROP	8.115	7.753	3464532	36523546	6.718	65.829 #
9) T	2,4-D	8.416	0.000	23554829	0	44.677	N.D. #
10) T	Pentachlo...	0.000	8.456	0	6617989	N.D.	<MDL
12) T	2,4,5-T	9.445	0.000	32167497	0	12.645	N.D. #
13) T	2,4-DB	0.000	9.704	0	8443385	N.D.	22.242
15) T	Picloram	11.012	0.000	8412297	0	2.772	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031220\
Data File : PS009240.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2020 01:34
Operator : DD\AJ
Sample : L1853-03
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 04:25:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

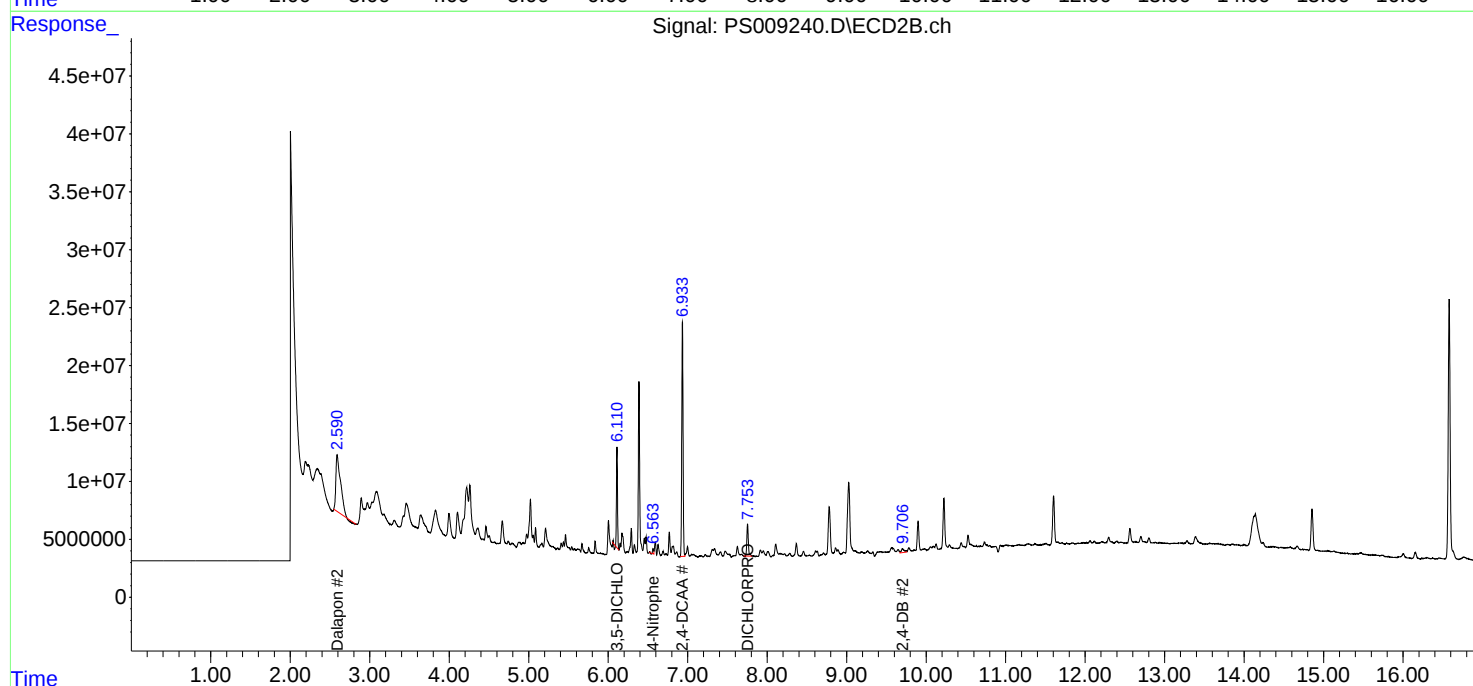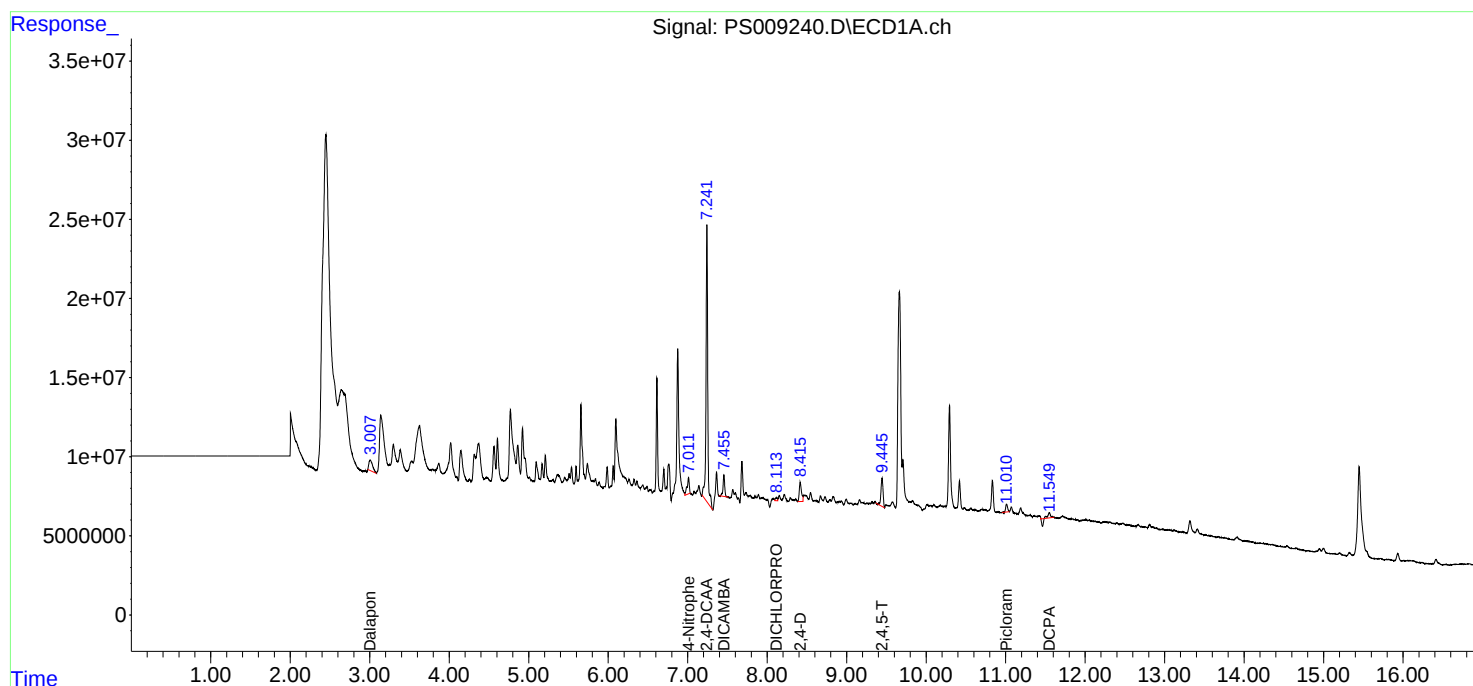


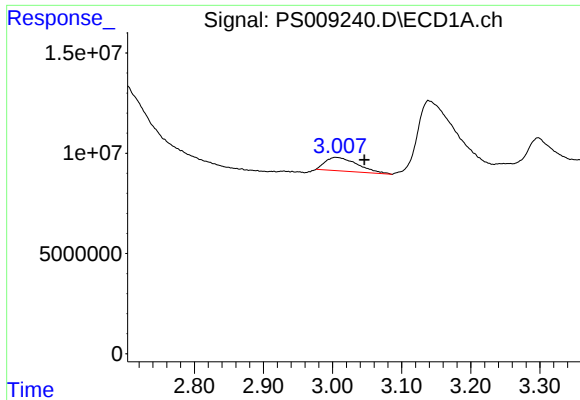

#1 Dalapon


R.T.: 3.005 min
Delta R.T.: -0.041 min
Response: 21851694
Conc: 28.02 ng/ml

Instrument :
ECD_S
ClientSampleId :

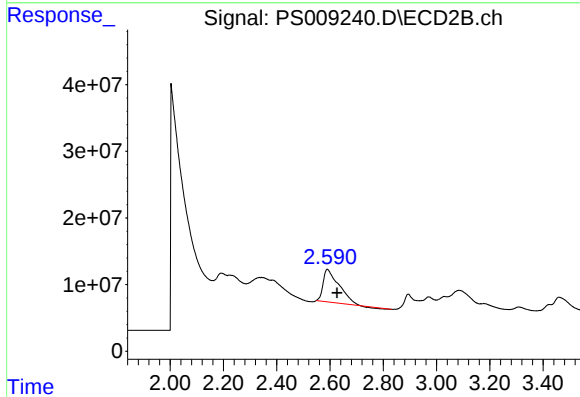


#1 Dalapon

R.T.: 2.590 min
Delta R.T.: -0.036 min
Response: 199721146
Conc: 253.66 ng/ml

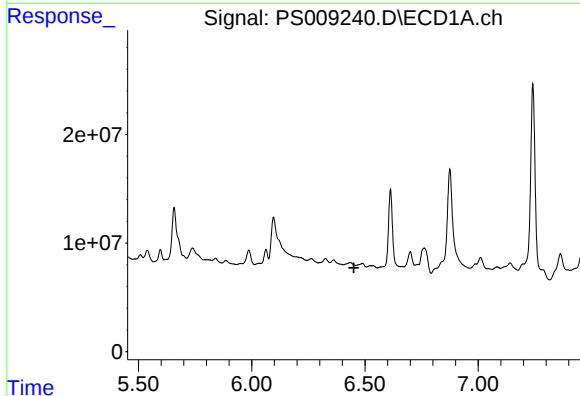


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

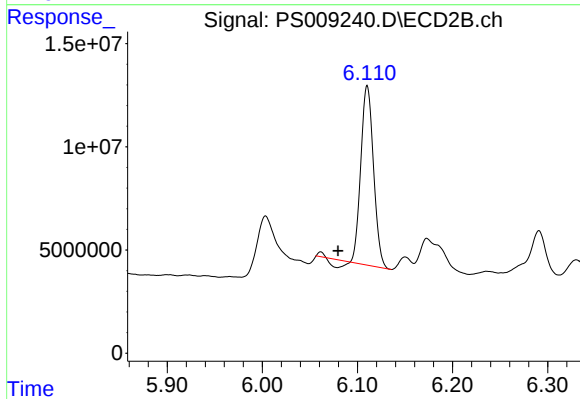

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.110 min
Delta R.T.: 0.031 min
Response: 77862065
Conc: 95.74 ng/ml

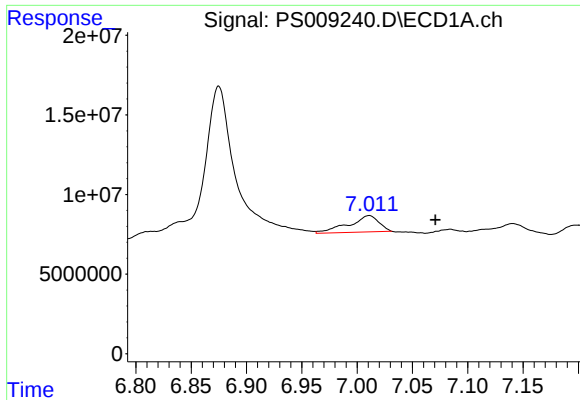

#3 4-Nitrophenol


R.T.: 7.011 min
Delta R.T.: -0.060 min
Response: 19233316
Conc: 80.57 ng/ml

Instrument :
ECD_S
ClientSampleId :

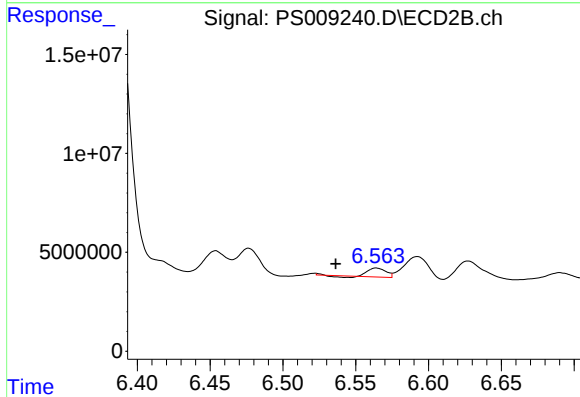


#3 4-Nitrophenol

R.T.: 6.564 min
Delta R.T.: 0.028 min
Response: 3662856
Conc: 11.51 ng/ml

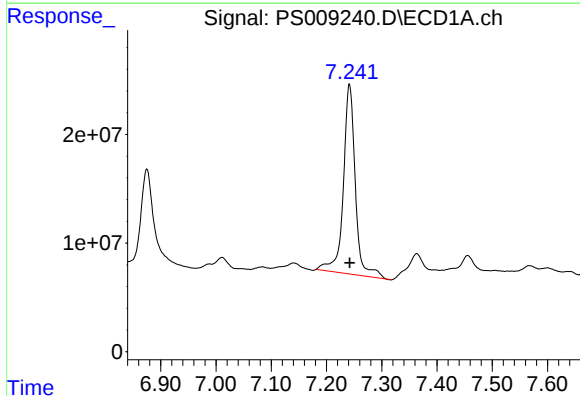


#4 2,4-DCAA

R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 263765631
Conc: 476.83 ng/ml

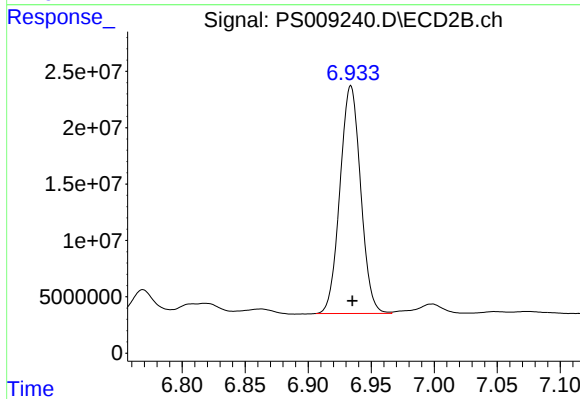

#4 2,4-DCAA


R.T.: 6.934 min
Delta R.T.: -0.001 min
Response: 230496817
Conc: 419.70 ng/ml

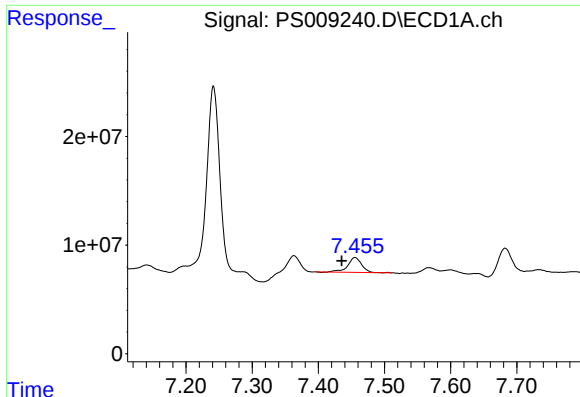

#5 DICAMBA


R.T.: 7.456 min
Delta R.T.: 0.020 min
Response: 20114624
Conc: 9.45 ng/ml

Instrument :
ECD_S
ClientSampleId :

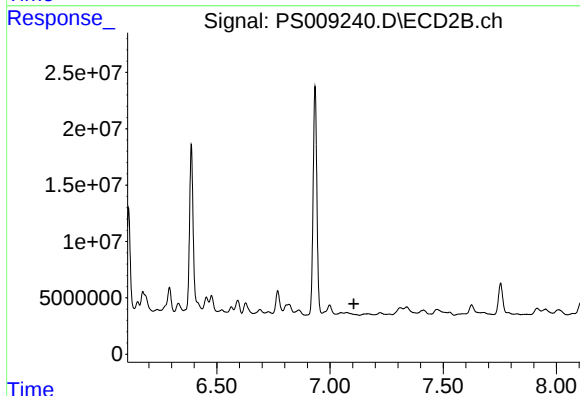


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 7.106 min
Response: 0
Conc: N.D.

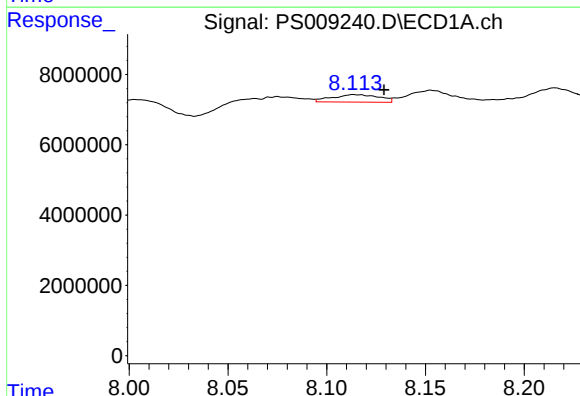


#8 DICHLORPROP

R.T.: 8.115 min
Delta R.T.: -0.014 min
Response: 3464532
Conc: 6.72 ng/ml

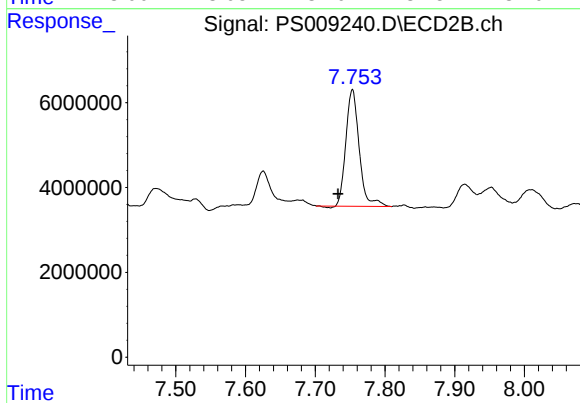

#8 DICHLORPROP


R.T.: 7.753 min
Delta R.T.: 0.020 min
Response: 36523546
Conc: 65.83 ng/ml

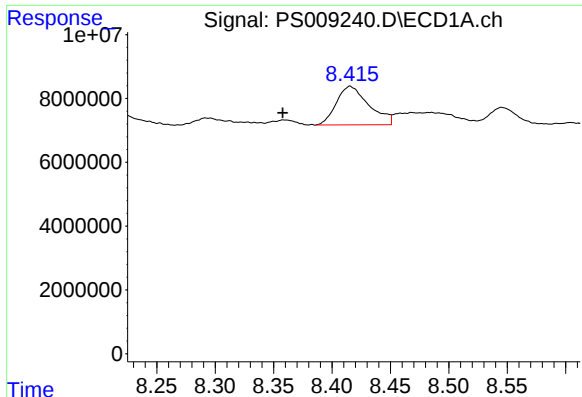

#9 2,4-D


R.T.: 8.416 min
Delta R.T.: 0.058 min
Response: 23554829
Conc: 44.68 ng/ml

Instrument :
ECD_S
ClientSampleId :

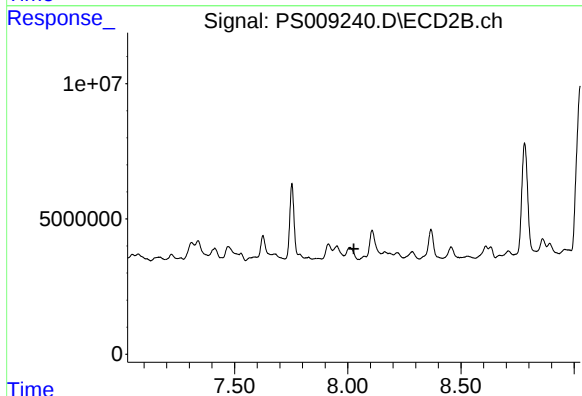


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.027 min
Response: 0
Conc: N.D.

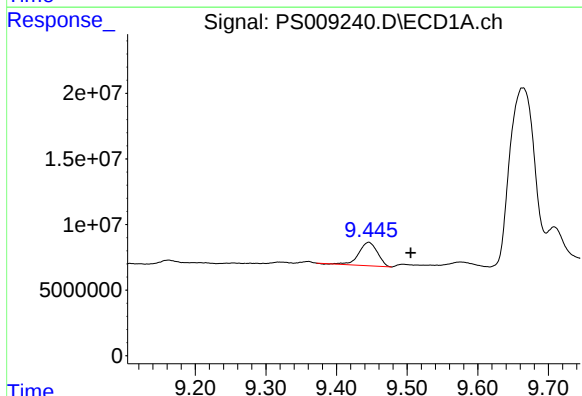


#12 2,4,5-T

R.T.: 9.445 min
Delta R.T.: -0.060 min
Response: 32167497
Conc: 12.65 ng/ml

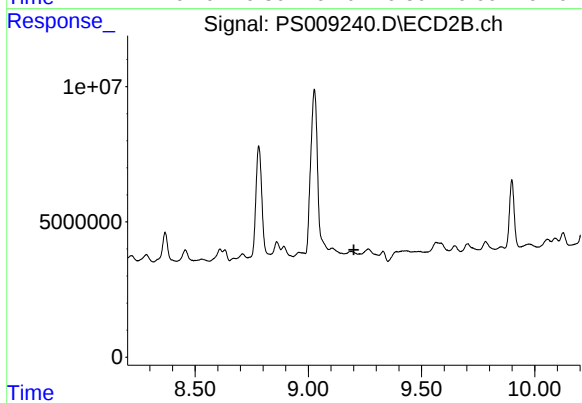

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 9.201 min
Response: 0
Conc: N.D.

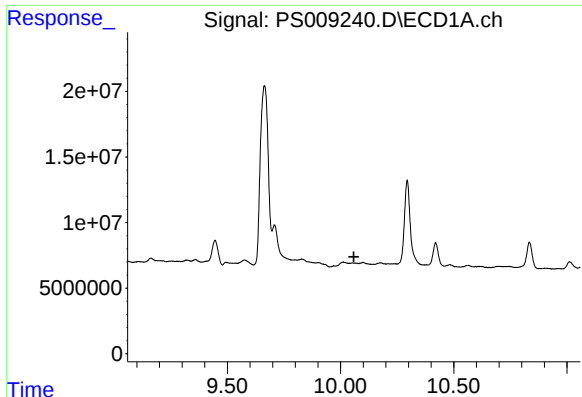

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.059 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

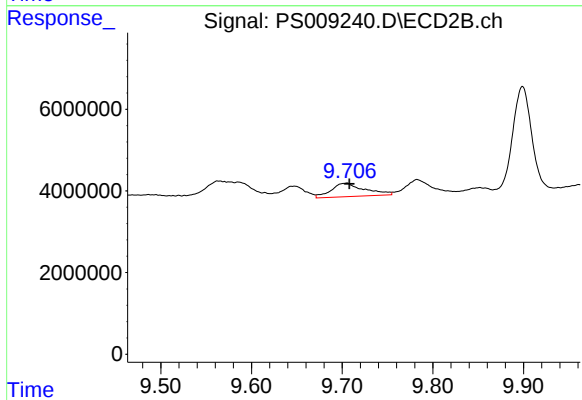


#13 2,4-DB

R.T.: 9.704 min
Delta R.T.: -0.005 min
Response: 8443385
Conc: 22.24 ng/ml

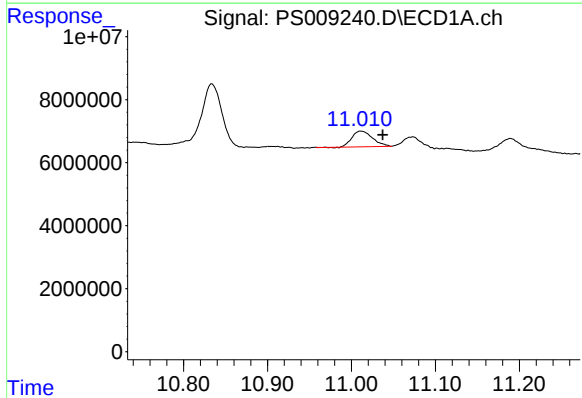


#15 Picloram

R.T.: 11.012 min
Delta R.T.: -0.026 min
Response: 8412297
Conc: 2.77 ng/ml

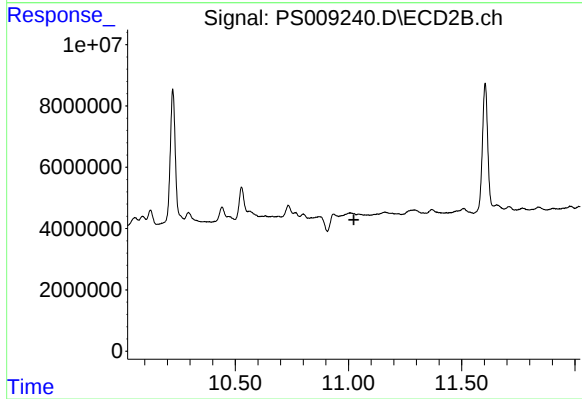

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 11.023 min
Response: 0
Conc: N.D.

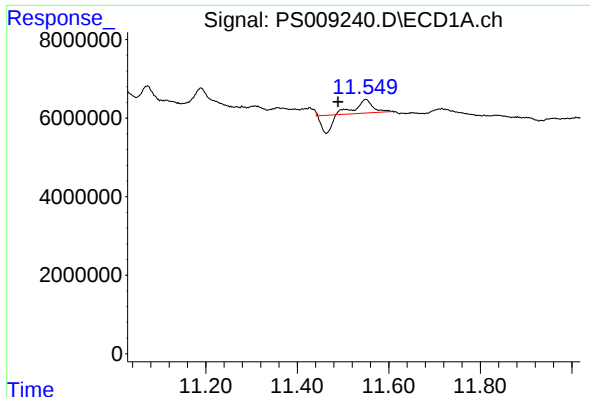

#16 DCPA

R.T.: 11.550 min
Delta R.T.: 0.061 min
Response: 3822605
Conc: 1.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

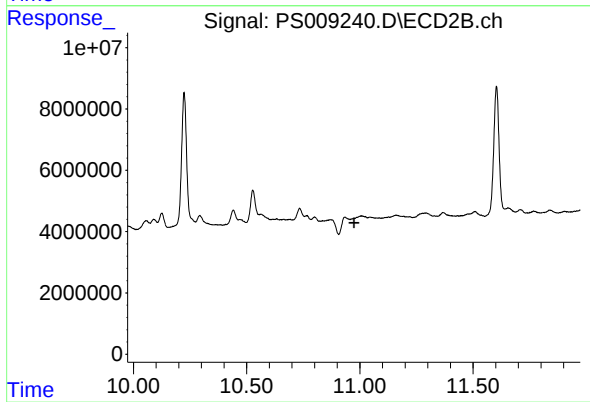

#16 DCPA

R.T.: 10.934 min
Delta R.T.: -0.040 min
Response: -6070798
Conc: N.D.