

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031220\
 Data File : PS009243.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2020 02:42
 Operator : DD\AJ
 Sample : L1853-06
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 04:26:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.242	6.933	252.1E6	222.1E6	455.739	404.437
Target Compounds							
1) T	Dalapon	3.007	2.588	20006110	127.0E6	25.654	161.311 #
2) T	3,5-DICHL...	0.000	6.110	0	77092911	N.D.	94.789
3) T	4-Nitroph...	7.010	6.591	24792507	19650605	103.859	61.756 #
8) T	DICHLORPROP	8.117	7.754	5320342	39924307	10.316	71.959 #
9) T	2,4-D	8.421	0.000	7493255	0	14.213	N.D. #
10) T	Pentachlo...	8.670	8.458	14955165	16185053	2.127	2.132
12) T	2,4,5-T	9.503	9.252	11396094	36576088	4.480	12.390 #
13) T	2,4-DB	0.000	9.704	0	9541589	N.D.	25.135
15) T	Picloram	11.036	11.022	82231317	116.3E6	27.095	28.549
16) T	DCPA	11.493	10.972	438210	21443834	<MDL	5.537 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031220\
Data File : PS009243.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2020 02:42
Operator : DD\AJ
Sample : L1853-06
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 04:26:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

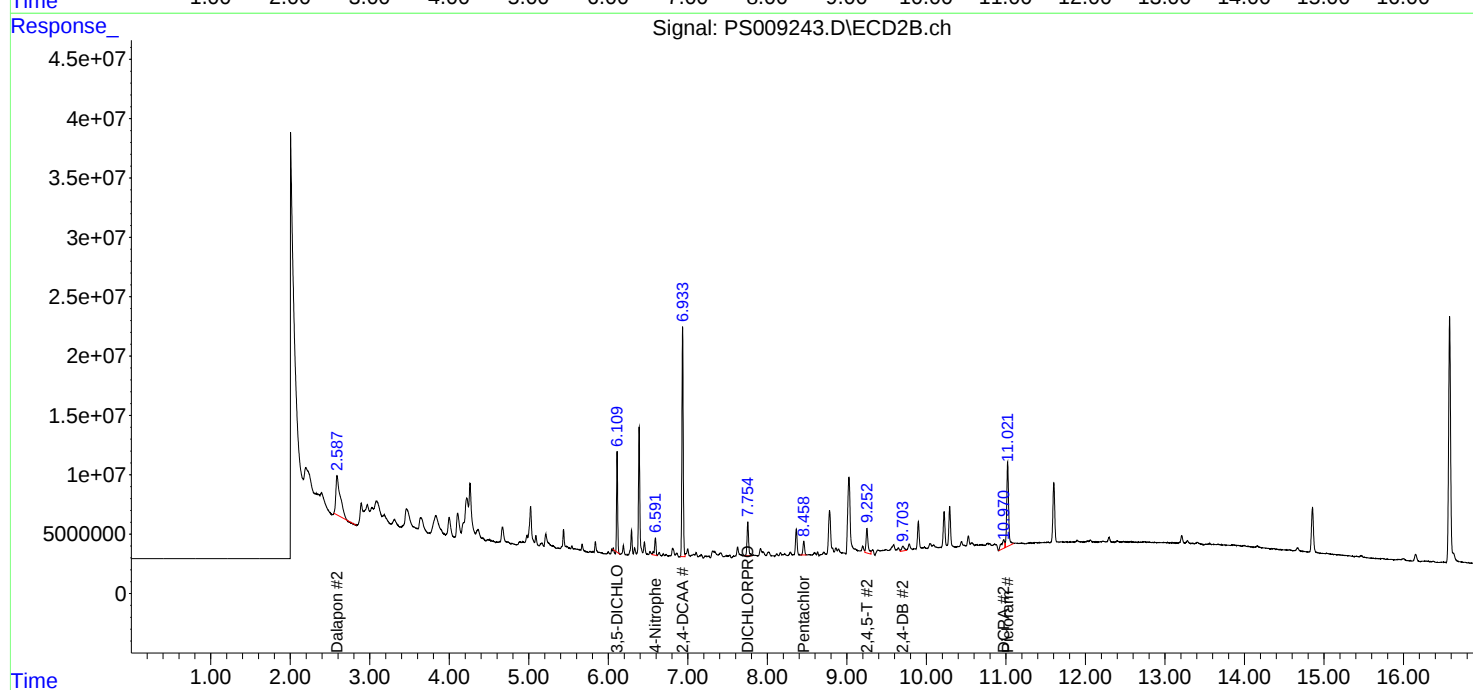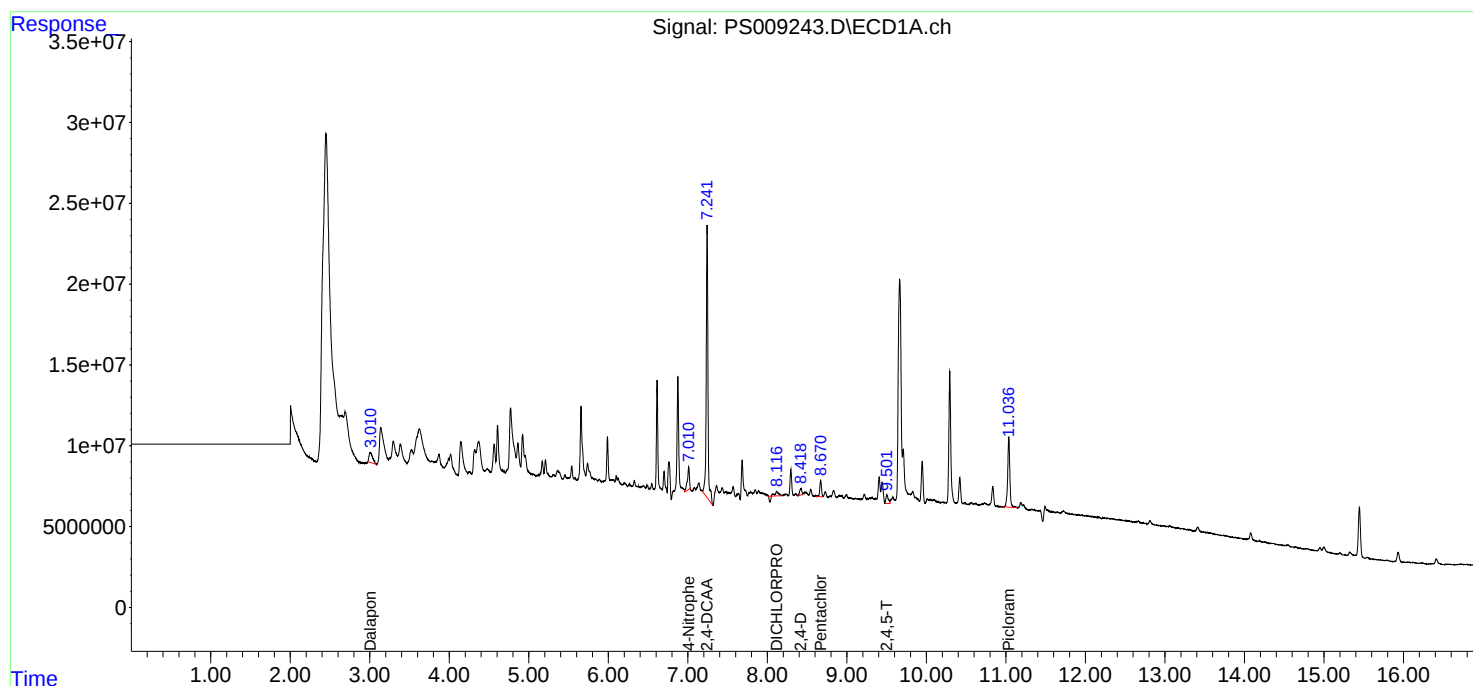


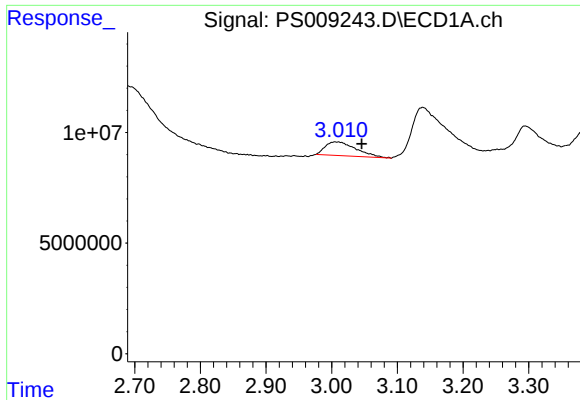

#1 Dalapon


R.T.: 3.007 min
Delta R.T.: -0.039 min
Response: 20006110
Conc: 25.65 ng/ml

Instrument :
ECD_S
ClientSampleId :

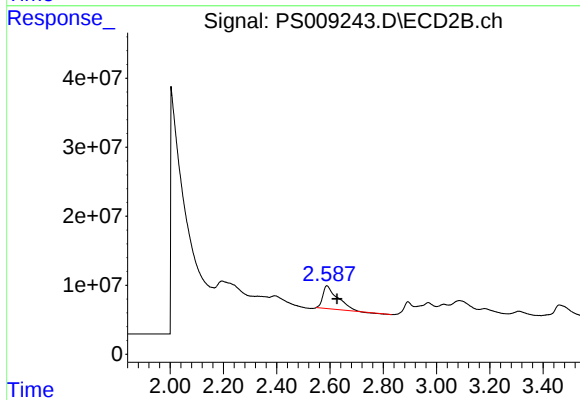


#1 Dalapon

R.T.: 2.588 min
Delta R.T.: -0.038 min
Response: 127010251
Conc: 161.31 ng/ml

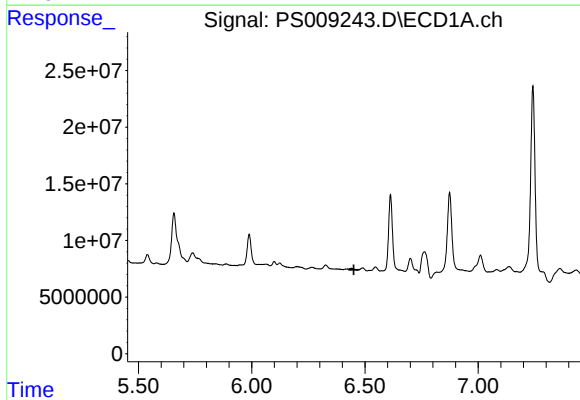


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

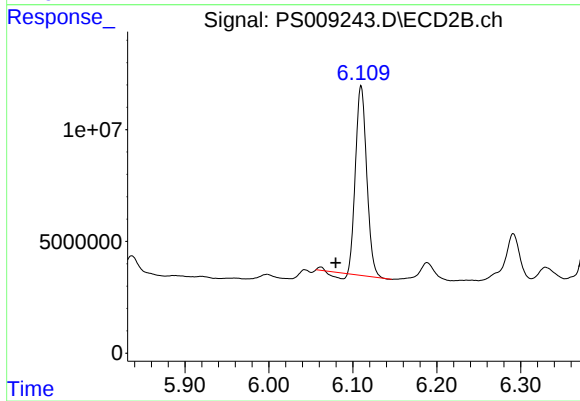

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.110 min
Delta R.T.: 0.030 min
Response: 77092911
Conc: 94.79 ng/ml

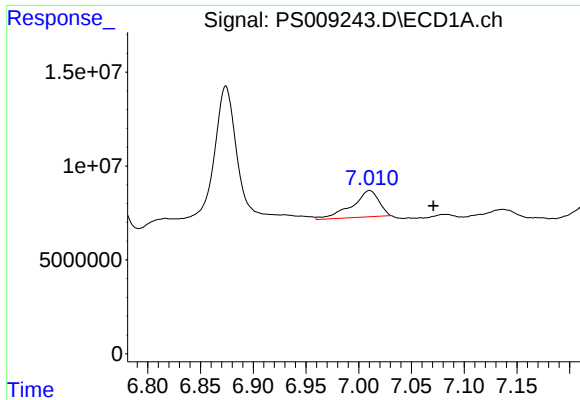

#3 4-Nitrophenol


R.T.: 7.010 min
Delta R.T.: -0.061 min
Response: 24792507
Conc: 103.86 ng/ml

Instrument :
ECD_S
ClientSampleId :

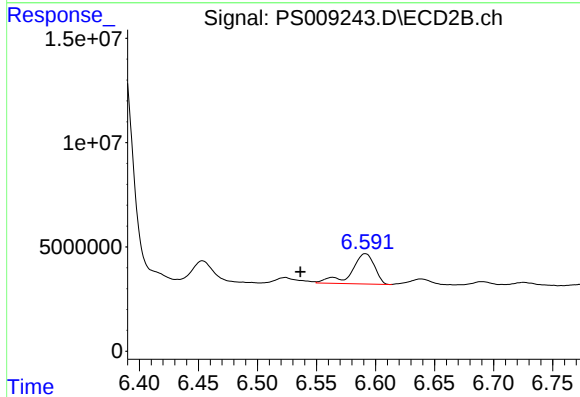


#3 4-Nitrophenol

R.T.: 6.591 min
Delta R.T.: 0.055 min
Response: 19650605
Conc: 61.76 ng/ml

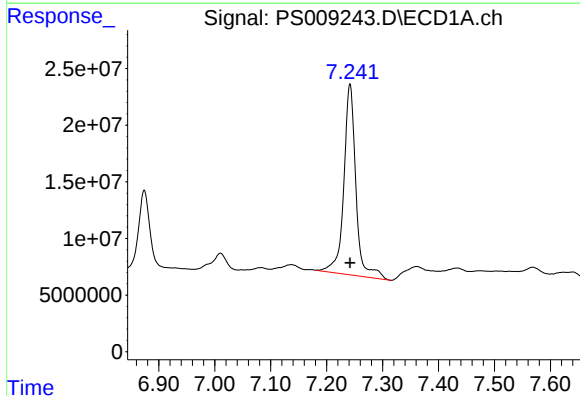


#4 2,4-DCAA

R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 252101437
Conc: 455.74 ng/ml

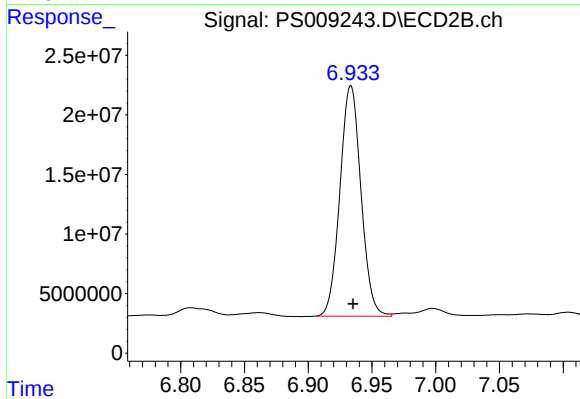

#4 2,4-DCAA


R.T.: 6.933 min
Delta R.T.: -0.002 min
Response: 222115755
Conc: 404.44 ng/ml

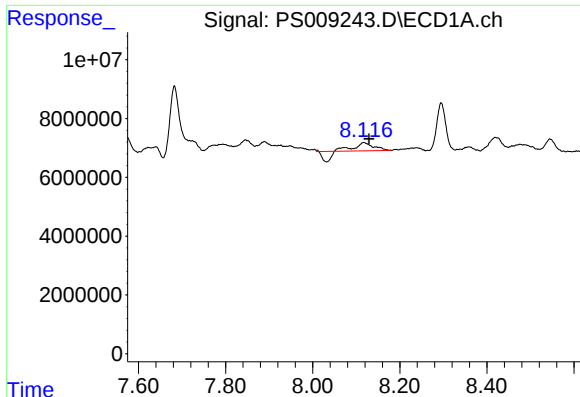

#8 DICHLORPROP


R.T.: 8.117 min
Delta R.T.: -0.012 min
Response: 5320342
Conc: 10.32 ng/ml

Instrument :
ECD_S
ClientSampleId :

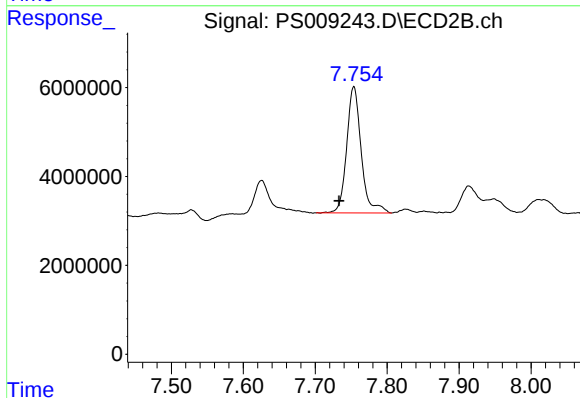


#8 DICHLORPROP

R.T.: 7.754 min
Delta R.T.: 0.021 min
Response: 39924307
Conc: 71.96 ng/ml

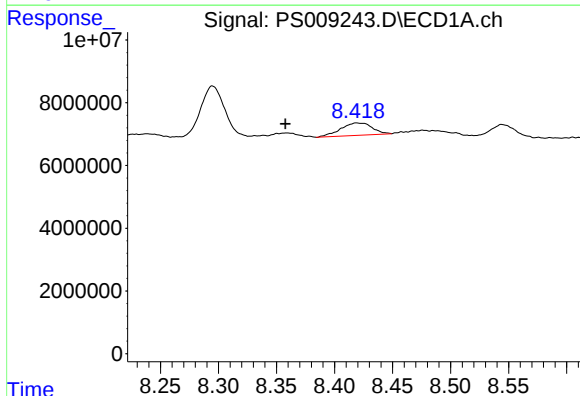


#9 2,4-D

R.T.: 8.421 min
Delta R.T.: 0.063 min
Response: 7493255
Conc: 14.21 ng/ml

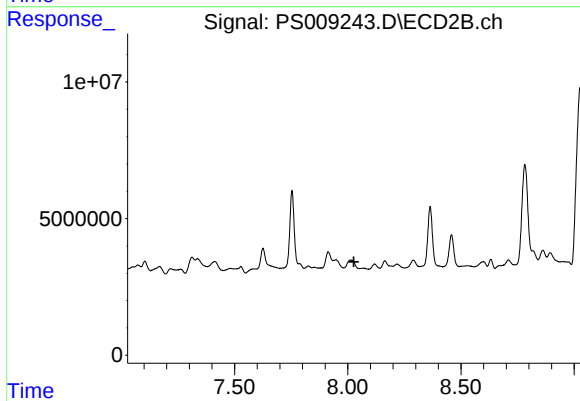

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.027 min
Response: 0
Conc: N.D.

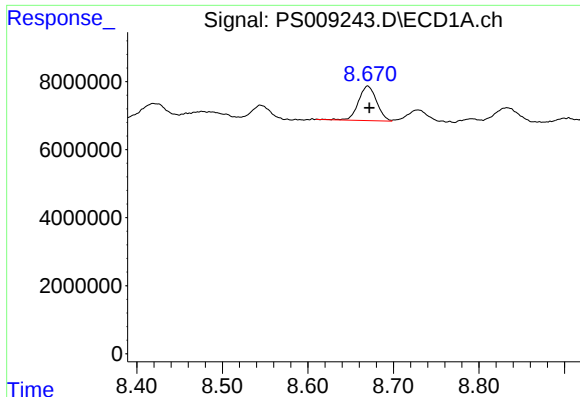

#10 Pentachlorophenol


R.T.: 8.670 min
Delta R.T.: -0.002 min
Response: 14955165
Conc: 2.13 ng/ml

Instrument :
ECD_S
ClientSampleId :

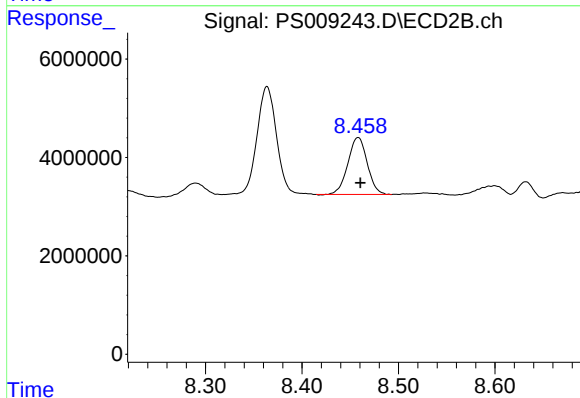


#10 Pentachlorophenol

R.T.: 8.458 min
Delta R.T.: -0.003 min
Response: 16185053
Conc: 2.13 ng/ml

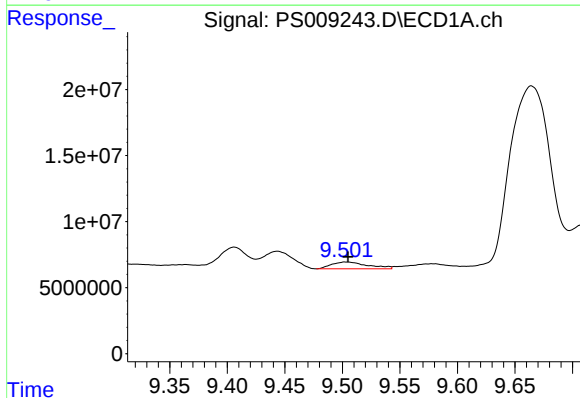


#12 2,4,5-T

R.T.: 9.503 min
Delta R.T.: -0.002 min
Response: 11396094
Conc: 4.48 ng/ml

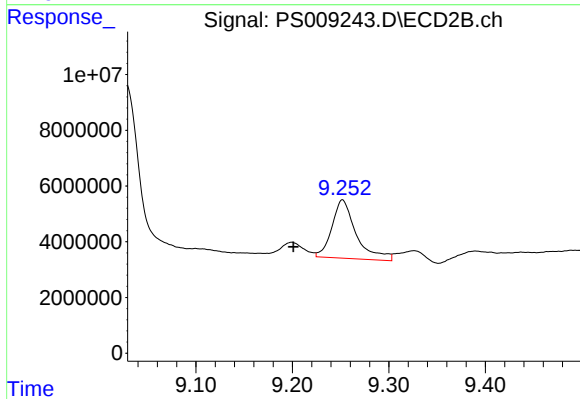

#12 2,4,5-T


R.T.: 9.252 min
Delta R.T.: 0.051 min
Response: 36576088
Conc: 12.39 ng/ml

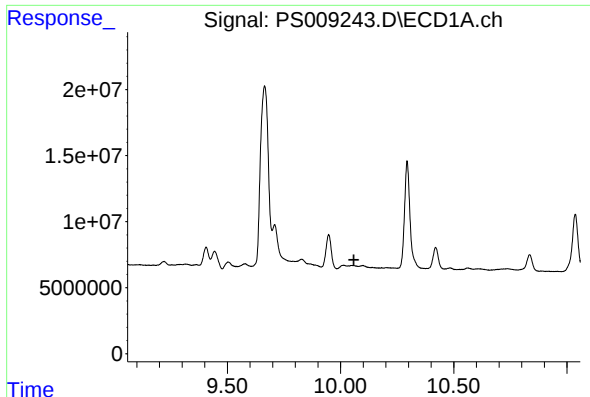

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.059 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

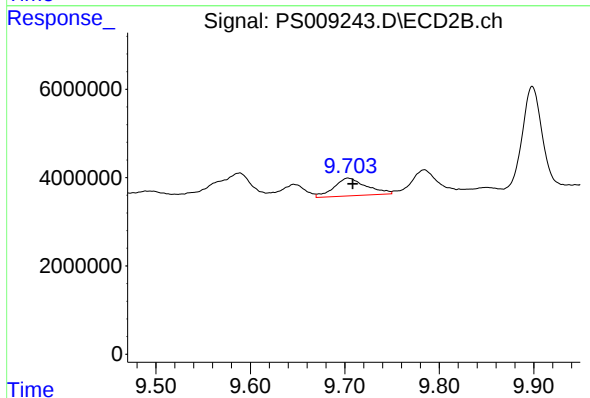


#13 2,4-DB

R.T.: 9.704 min
Delta R.T.: -0.004 min
Response: 9541589
Conc: 25.13 ng/ml

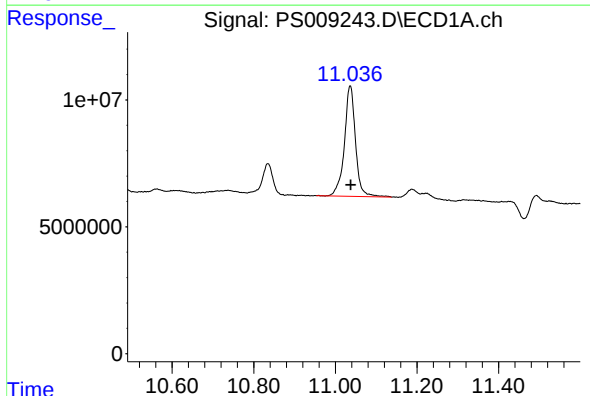


#15 Picloram

R.T.: 11.036 min
Delta R.T.: -0.001 min
Response: 82231317
Conc: 27.09 ng/ml

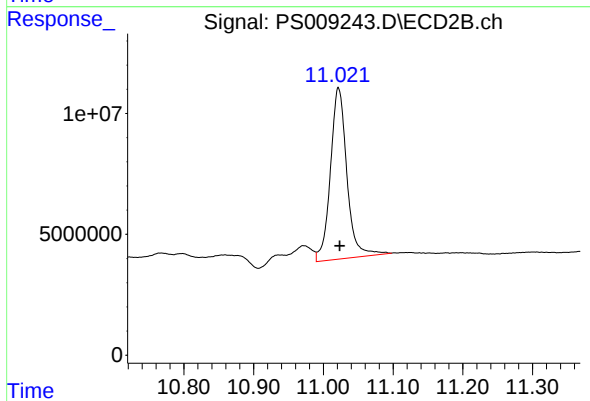

#15 Picloram


R.T.: 11.022 min
Delta R.T.: -0.002 min
Response: 116254866
Conc: 28.55 ng/ml

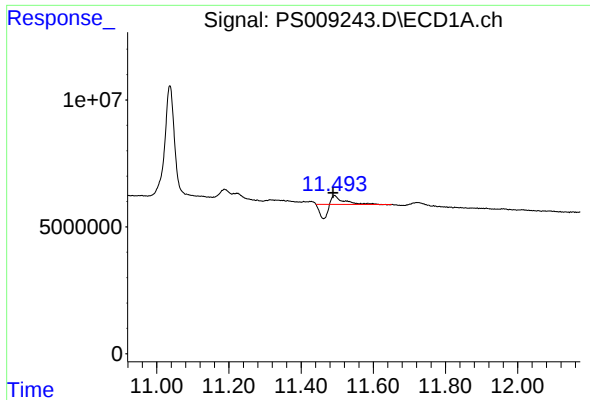

#16 DCPA

R.T.: 11.493 min
Delta R.T.: 0.004 min
Response: 438210
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

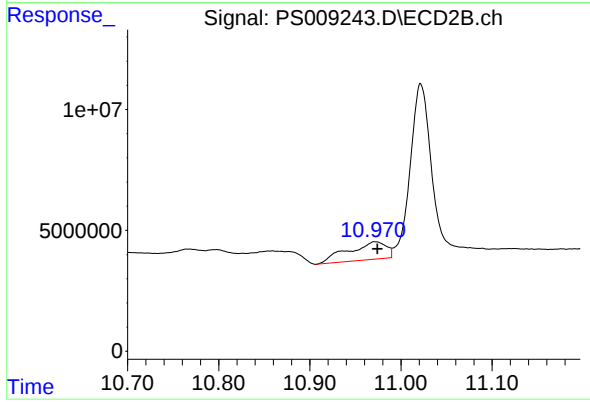

#16 DCPA

R.T.: 10.972 min
Delta R.T.: -0.002 min
Response: 21443834
Conc: 5.54 ng/ml