

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031220\
 Data File : PS009260.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2020 09:12
 Operator : DD\AJ
 Sample : PB127490BL
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 11:06:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.242	6.933	349.8E6	376.1E6	632.381	684.904
Target Compounds							
1) T	Dalapon	3.005	2.589	14681788	104.1E6	18.827	132.170 #
2) T	3,5-DICHL...	0.000	6.110	0	24257643	N.D.	29.826
3) T	4-Nitroph...	7.015	6.591	13143221	16699802	55.059	52.482
7) T	MCPA	7.793	7.401	33175911	66175474	10.893	24.522 #
8) T	DICHLORPROP	8.124	7.753	-3630553	35641817	N.D.	64.240
11) T	2,4,5-TP ...	0.000	8.788	0	7465211	N.D.	2.504
13) T	2,4-DB	0.000	9.729	0	9288231	N.D.	24.467
14) T	DINOSEB	0.000	10.052	0	10282681	N.D.	4.681
15) T	Picloram	0.000	10.973	0	12479546	N.D.	3.065
16) T	DCPA	11.507	10.973	-9840746	12479546	N.D.	3.222



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031220\
Data File : PS009260.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2020 09:12
Operator : DD\AJ
Sample : PB127490BL
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 11:06:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

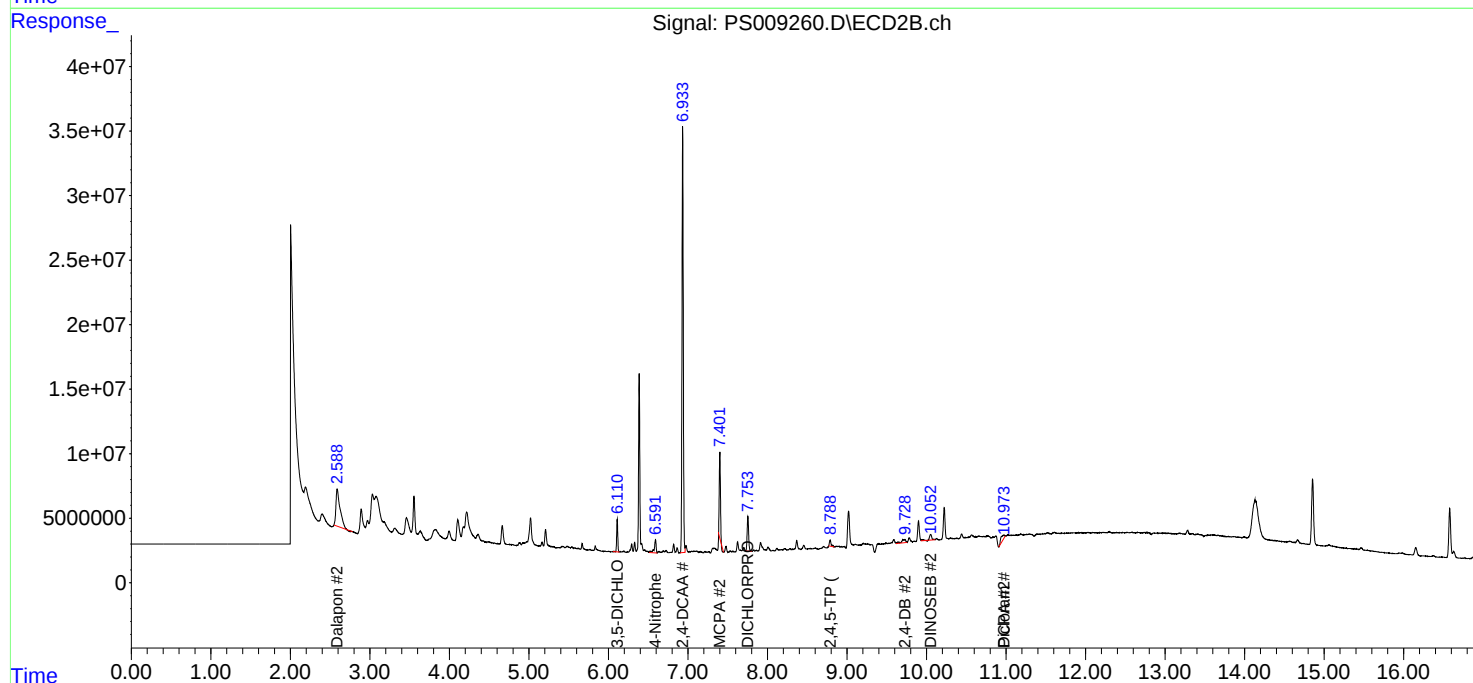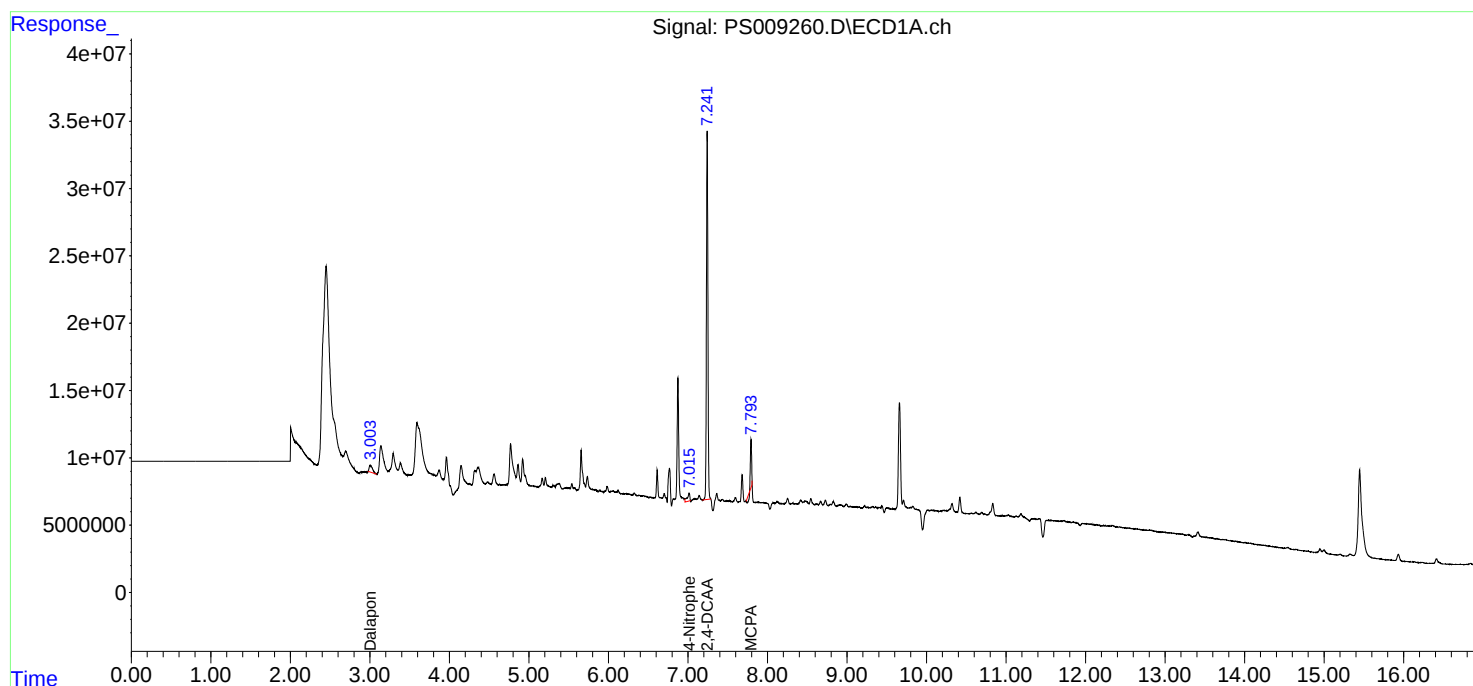


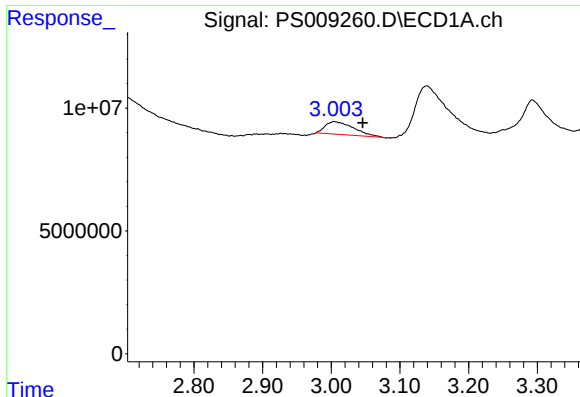

#1 Dalapon


R.T.: 3.005 min
Delta R.T.: -0.041 min
Response: 14681788
Conc: 18.83 ng/ml

Instrument :
ECD_S
ClientSampleId :

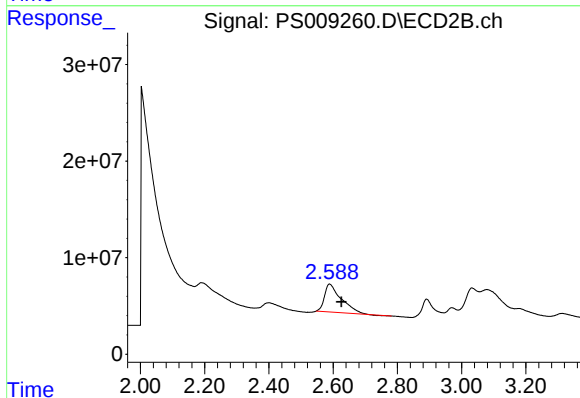


#1 Dalapon

R.T.: 2.589 min
Delta R.T.: -0.037 min
Response: 104065976
Conc: 132.17 ng/ml

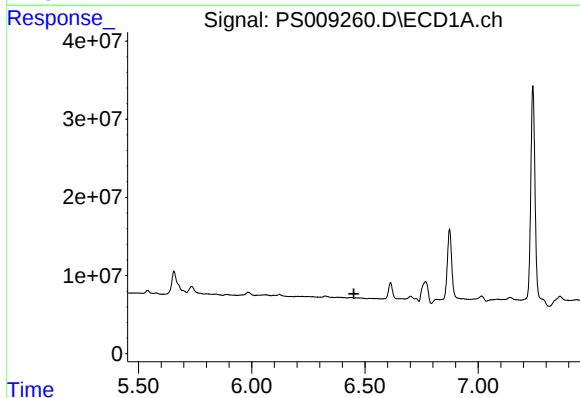


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

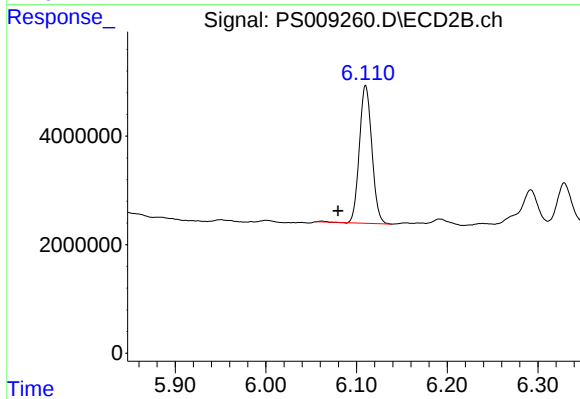

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.110 min
Delta R.T.: 0.030 min
Response: 24257643
Conc: 29.83 ng/ml

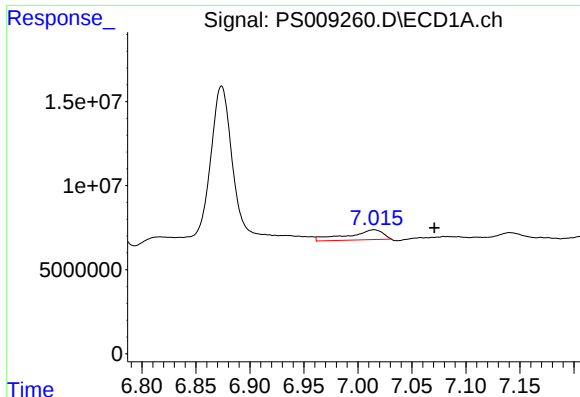

#3 4-Nitrophenol


R.T.: 7.015 min
Delta R.T.: -0.056 min
Response: 13143221
Conc: 55.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

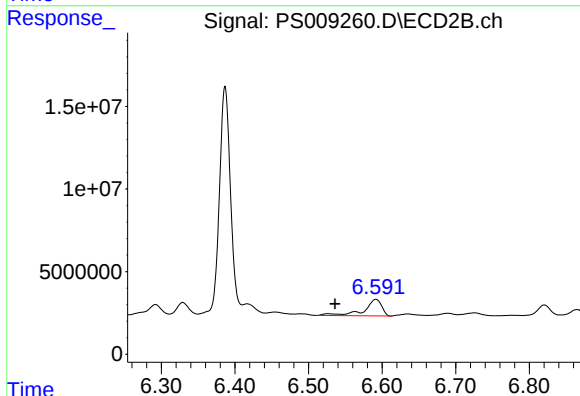


#3 4-Nitrophenol

R.T.: 6.591 min
Delta R.T.: 0.055 min
Response: 16699802
Conc: 52.48 ng/ml

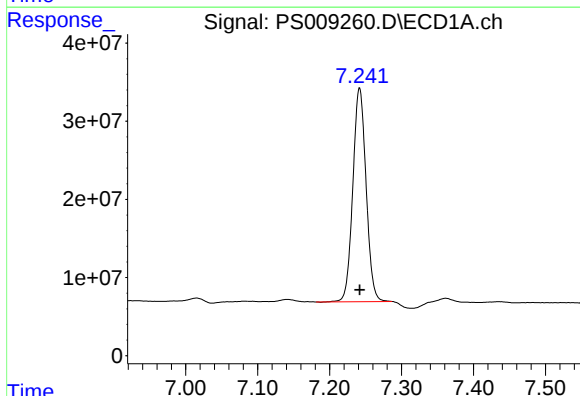


#4 2,4-DCAA

R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 349814324
Conc: 632.38 ng/ml

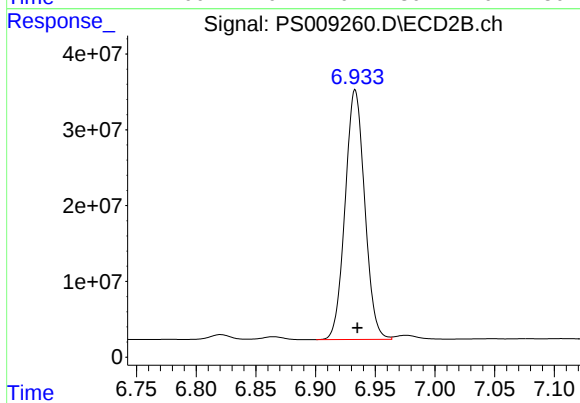

#4 2,4-DCAA


R.T.: 6.933 min
Delta R.T.: -0.002 min
Response: 376147972
Conc: 684.90 ng/ml

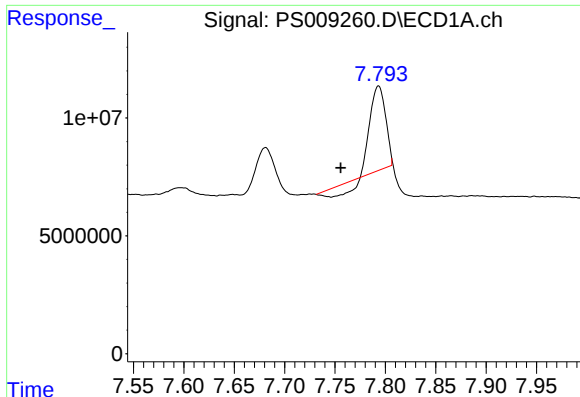

#7 MCPA


R.T.: 7.793 min
Delta R.T.: 0.038 min
Response: 33175911
Conc: 10.89 ug/ml

Instrument :
ECD_S
ClientSampleId :

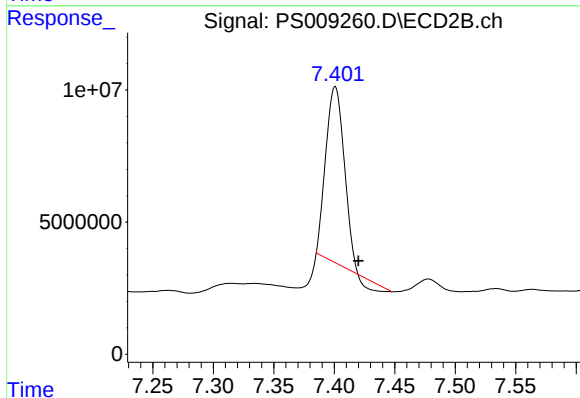


#7 MCPA

R.T.: 7.401 min
Delta R.T.: -0.019 min
Response: 66175474
Conc: 24.52 ug/ml

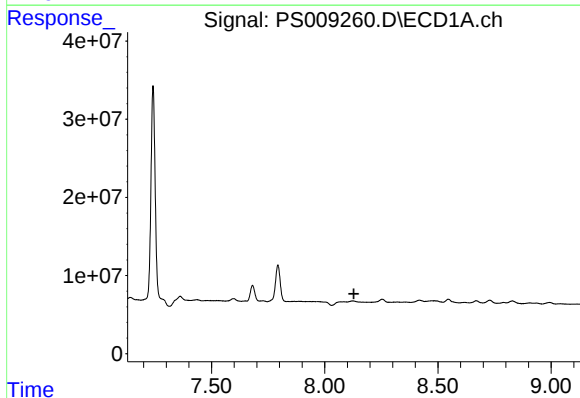


#8 DICHLORPROP

R.T.: 8.124 min
Delta R.T.: -0.005 min
Response: -3630553
Conc: N.D.

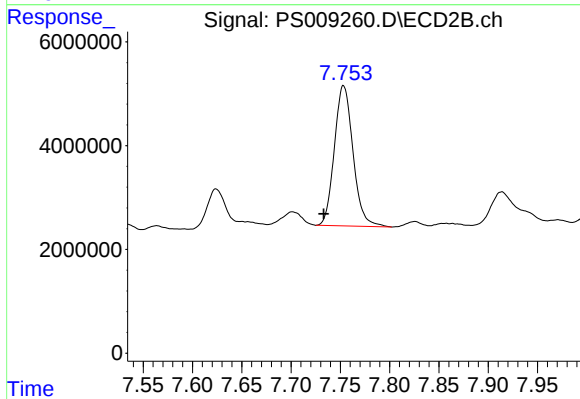

#8 DICHLORPROP


R.T.: 7.753 min
Delta R.T.: 0.020 min
Response: 35641817
Conc: 64.24 ng/ml

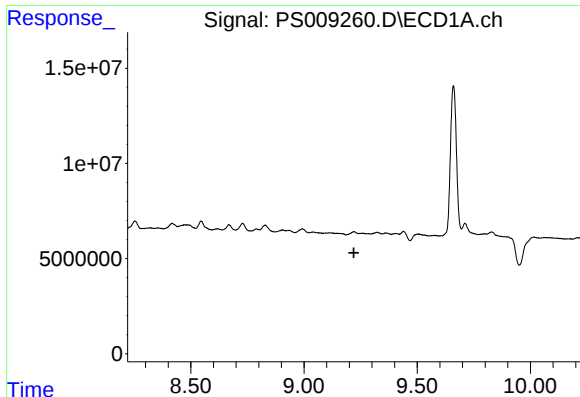

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 9.221 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

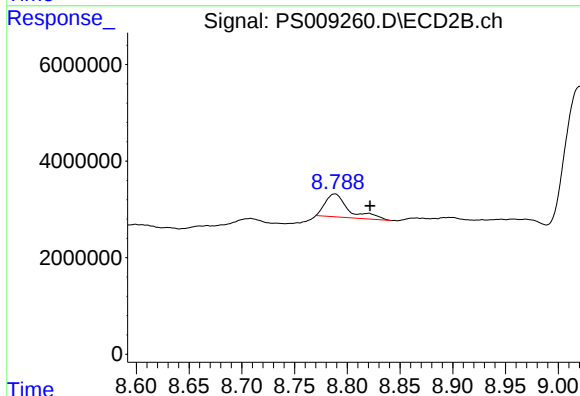


#11 2,4,5-TP (SILVEX)

R.T.: 8.788 min
Delta R.T.: -0.033 min
Response: 7465211
Conc: 2.50 ng/ml

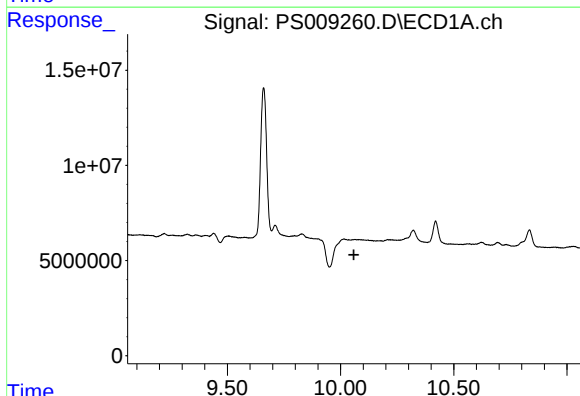


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.059 min
Response: 0
Conc: N.D.

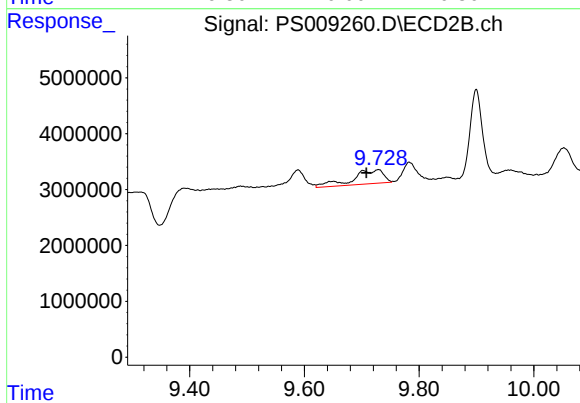

#13 2,4-DB


R.T.: 9.729 min
Delta R.T.: 0.021 min
Response: 9288231
Conc: 24.47 ng/ml

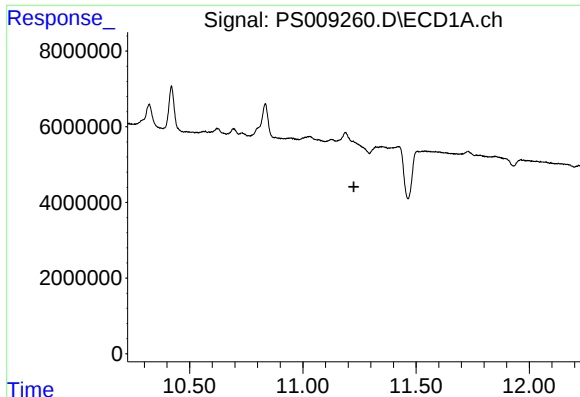

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 11.225 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

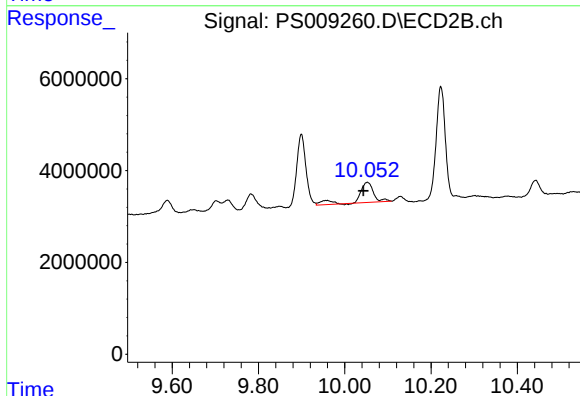


#14 DINOSEB

R.T.: 10.052 min
Delta R.T.: 0.009 min
Response: 10282681
Conc: 4.68 ng/ml

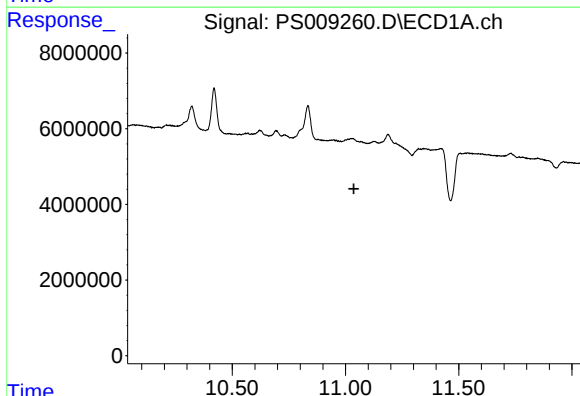


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.037 min
Response: 0
Conc: N.D.

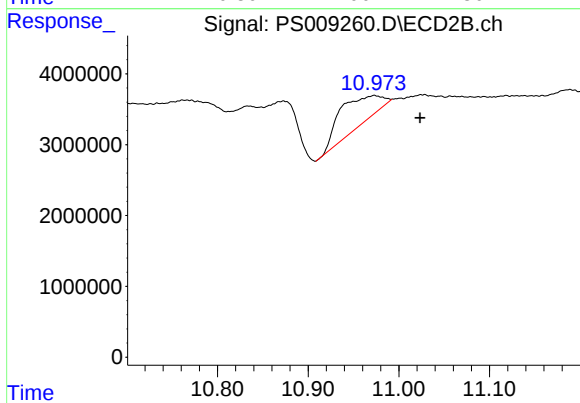

#15 Picloram


R.T.: 10.973 min
Delta R.T.: -0.050 min
Response: 12479546
Conc: 3.06 ng/ml

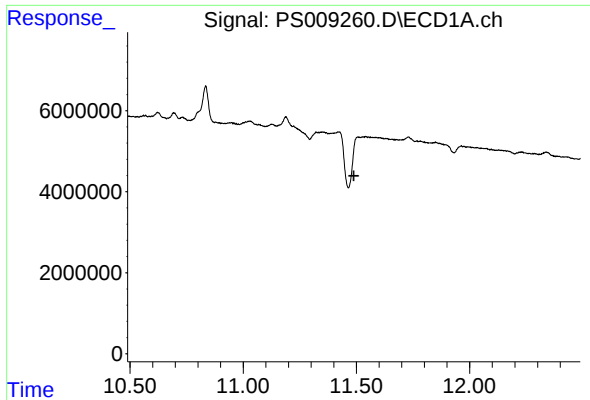

#16 DCPA

R.T.: 11.507 min
Delta R.T.: 0.018 min
Response: -9840746
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

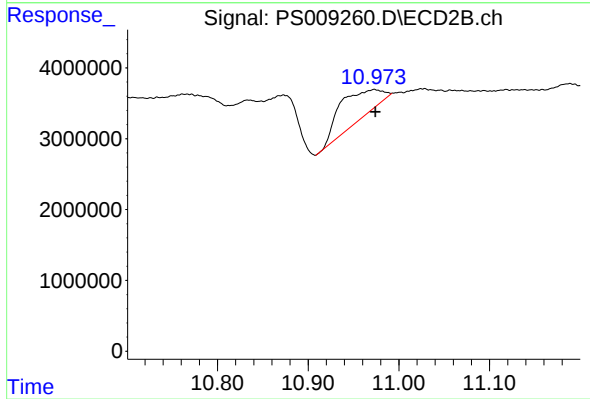

#16 DCPA

R.T.: 10.973 min
Delta R.T.: -0.001 min
Response: 12479546
Conc: 3.22 ng/ml