

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031220\
 Data File : PS009264.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2020 10:43
 Operator : DD\AJ
 Sample : L1797-04
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 11:07:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.242	6.934	243.3E6	246.4E6	439.819	448.739
Target Compounds							
1) T	Dalapon	3.010	2.589	16662533	91560517	21.367	116.288 #
2) T	3,5-DICHL...	0.000	6.110	0	67856954	N.D.	83.433
3) T	4-Nitroph...	7.010	6.592	17445485	12281779	73.081	38.598 #
8) T	DICHLORPROP	8.118	7.753	-1989687	33814866	N.D.	60.947
12) T	2,4,5-T	9.443	0.000	12357978	0	4.858	N.D. #
15) T	Picloram	0.000	11.025	0	22849461	N.D.	5.611
16) T	DCPA	0.000	11.025	0	22849461	N.D.	5.900



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031220\
Data File : PS009264.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2020 10:43
Operator : DD\AJ
Sample : L1797-04
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 11:07:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

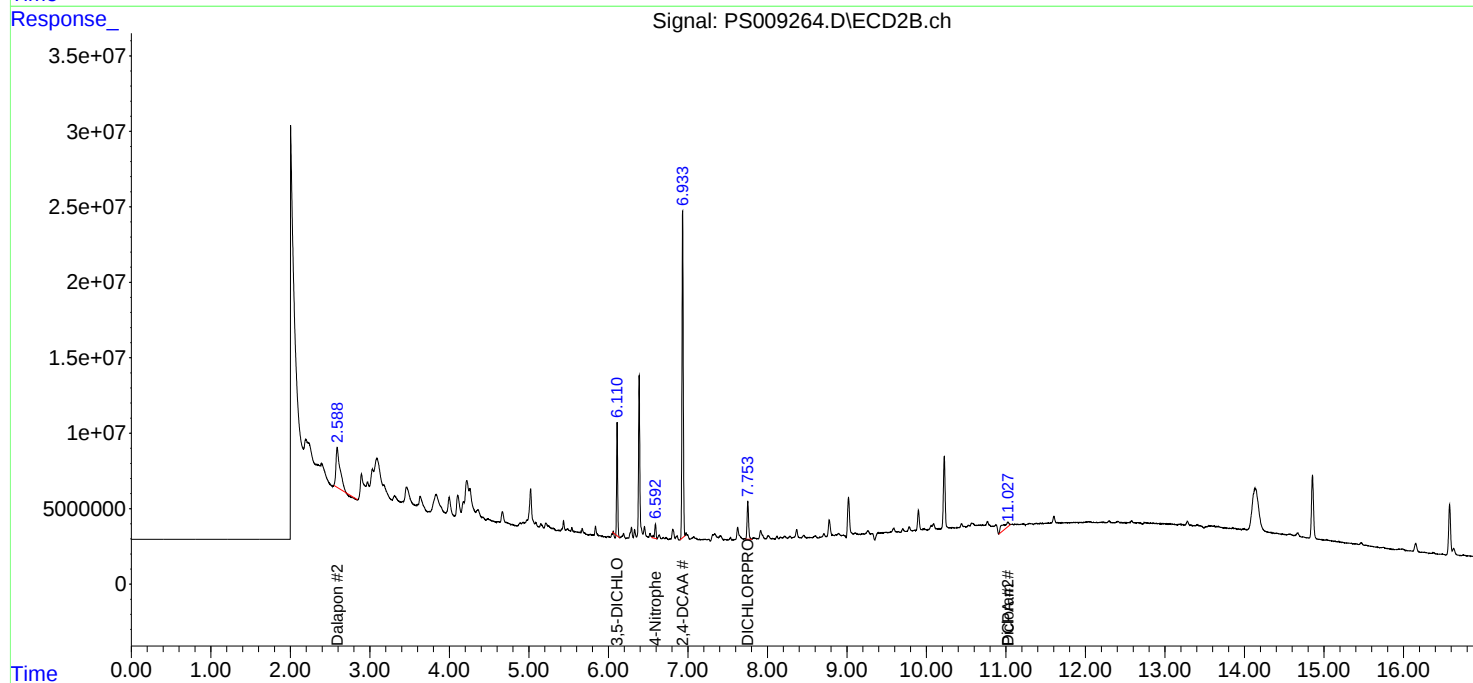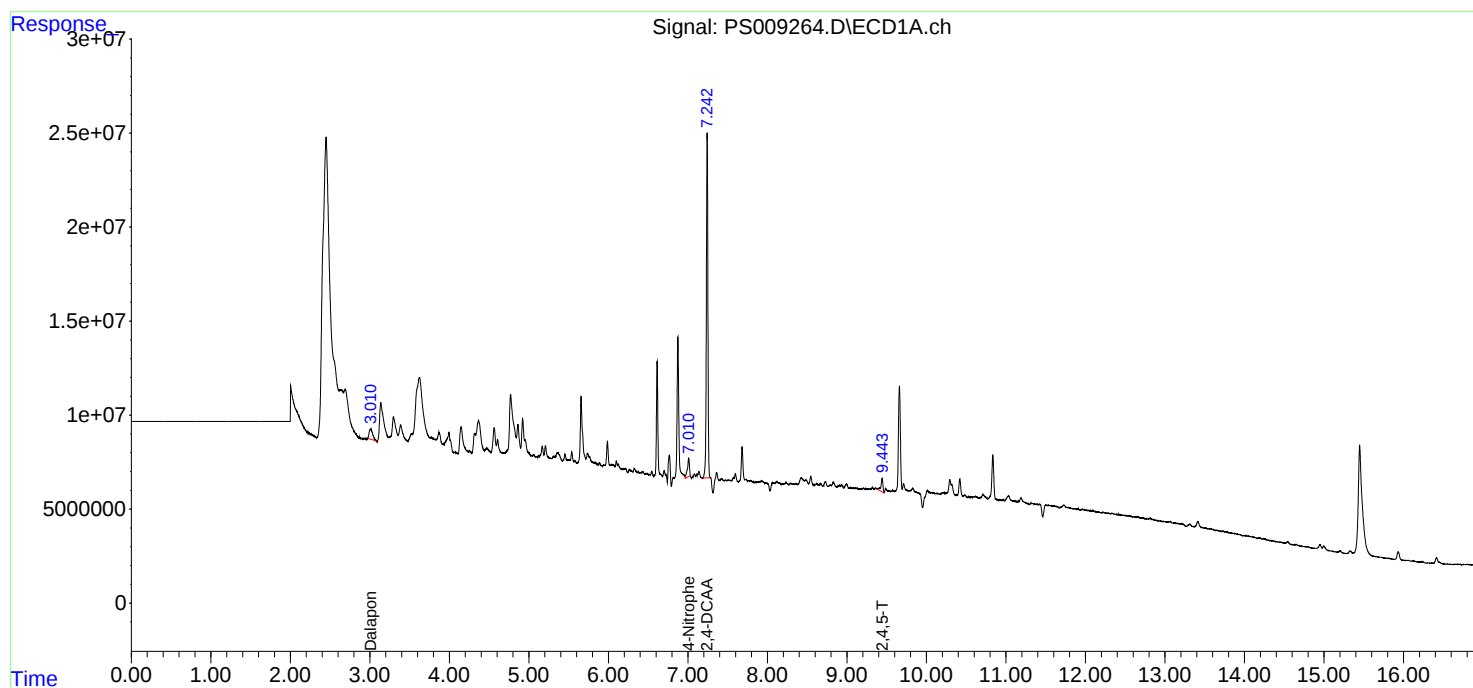


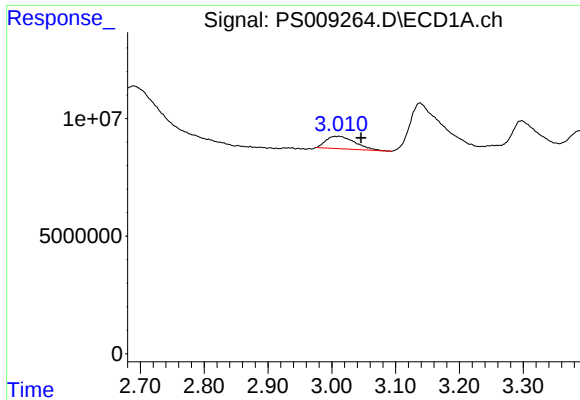

#1 Dalapon


R.T.: 3.010 min
Delta R.T.: -0.036 min
Response: 16662533
Conc: 21.37 ng/ml

Instrument :
ECD_S
ClientSampleId :

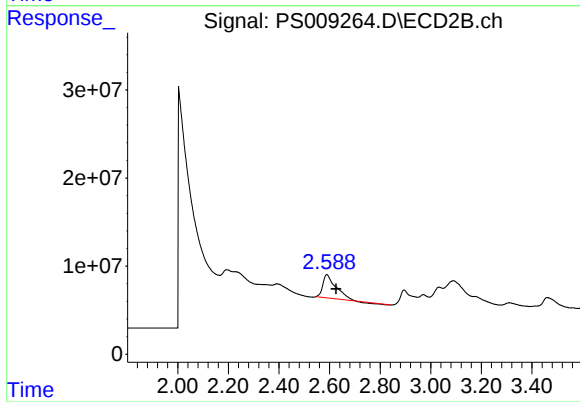


#1 Dalapon

R.T.: 2.589 min
Delta R.T.: -0.037 min
Response: 91560517
Conc: 116.29 ng/ml

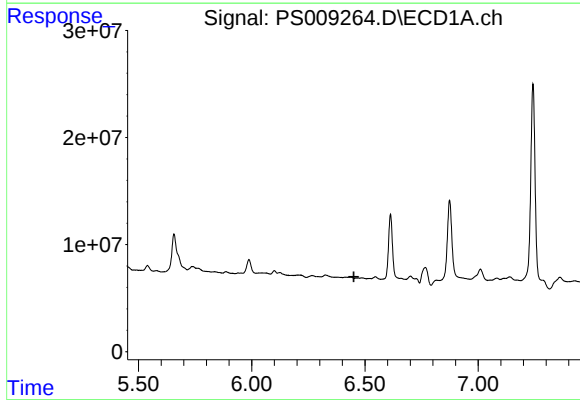


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

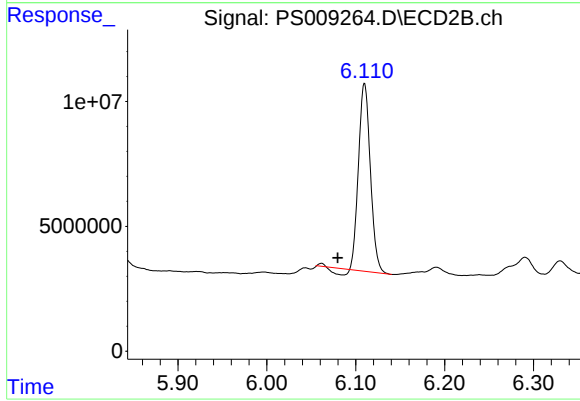

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.110 min
Delta R.T.: 0.030 min
Response: 67856954
Conc: 83.43 ng/ml

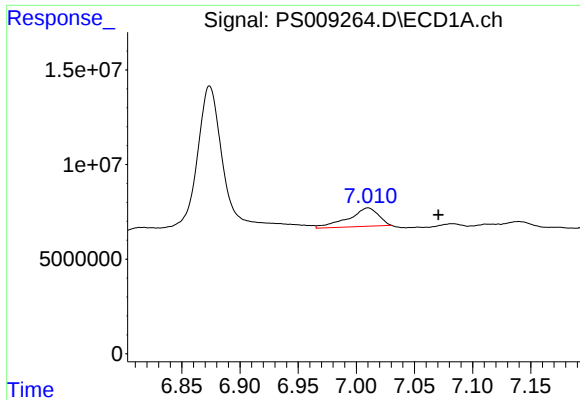

#3 4-Nitrophenol


R.T.: 7.010 min
Delta R.T.: -0.061 min
Response: 17445485
Conc: 73.08 ng/ml

Instrument :
ECD_S
ClientSampleId :

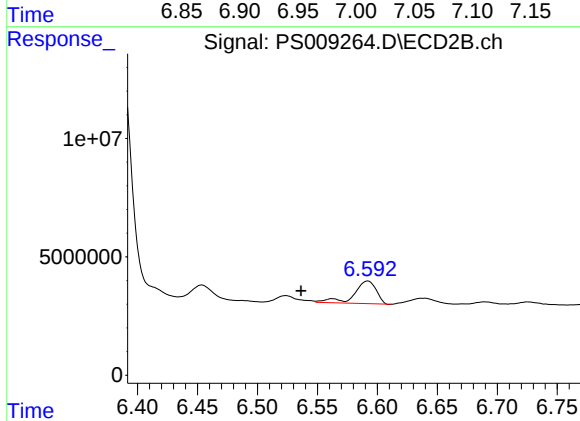


#3 4-Nitrophenol

R.T.: 6.592 min
Delta R.T.: 0.056 min
Response: 12281779
Conc: 38.60 ng/ml

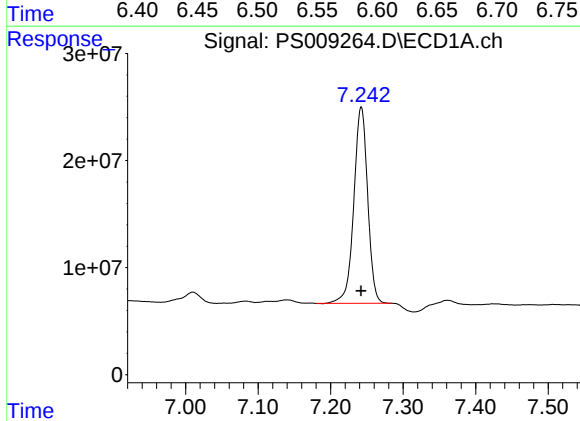


#4 2,4-DCAA

R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 243294758
Conc: 439.82 ng/ml

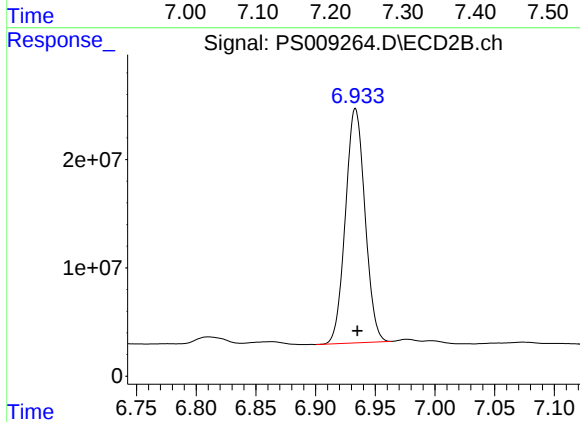

#4 2,4-DCAA


R.T.: 6.934 min
Delta R.T.: -0.002 min
Response: 246446391
Conc: 448.74 ng/ml

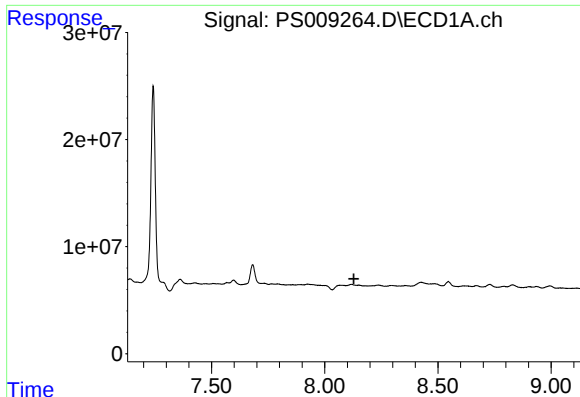

#8 DICHLORPROP


R.T.: 8.118 min
Delta R.T.: -0.011 min
Response: -1989687
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

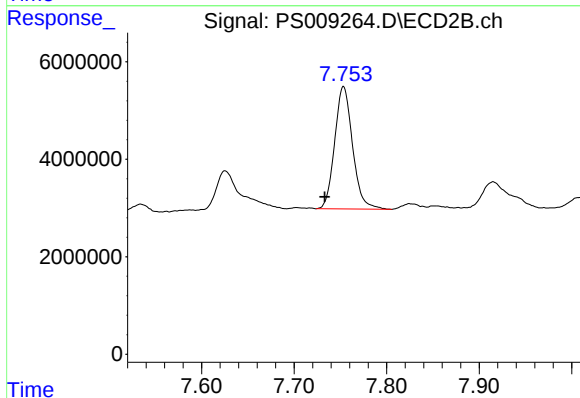


#8 DICHLORPROP

R.T.: 7.753 min
Delta R.T.: 0.020 min
Response: 33814866
Conc: 60.95 ng/ml

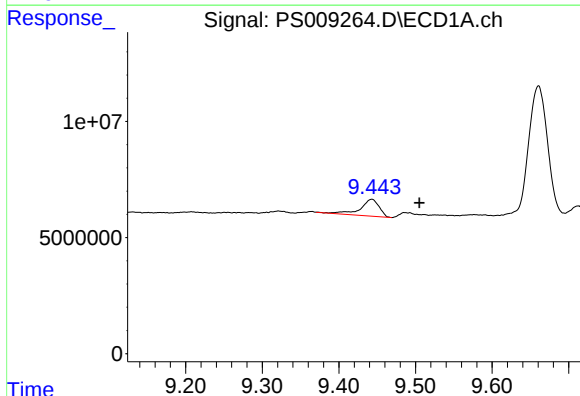


#12 2,4,5-T

R.T.: 9.443 min
Delta R.T.: -0.062 min
Response: 12357978
Conc: 4.86 ng/ml

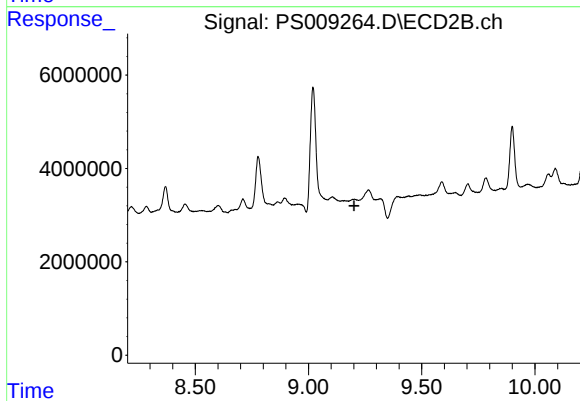

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.201 min
Response: 0
Conc: N.D.

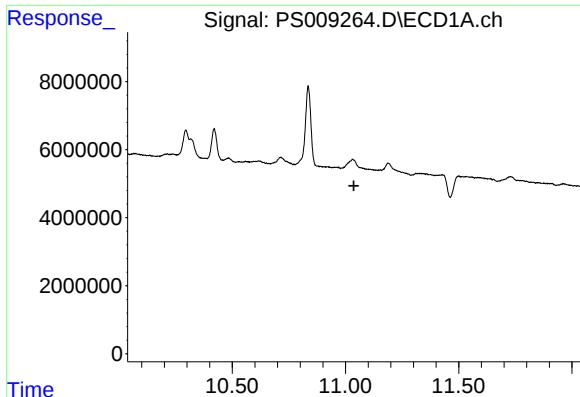

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 11.037 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

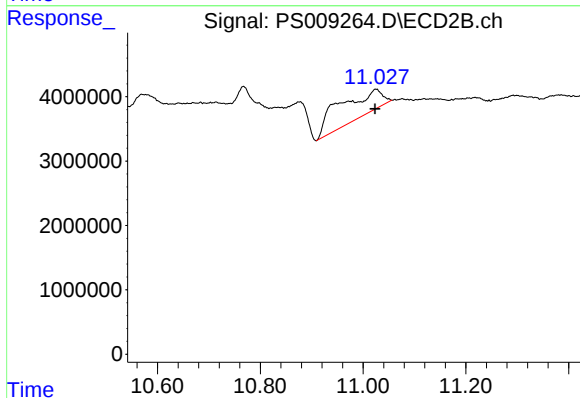


#15 Picloram

R.T.: 11.025 min
Delta R.T.: 0.002 min
Response: 22849461
Conc: 5.61 ng/ml

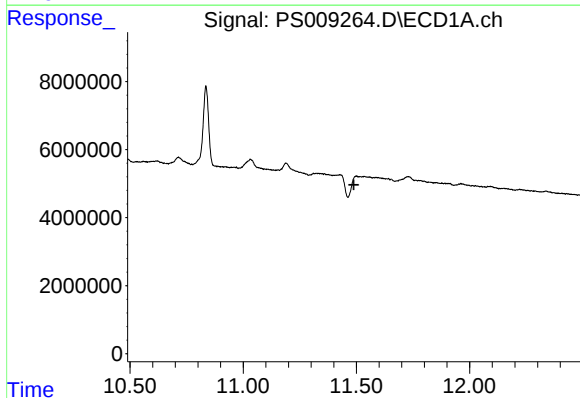

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.489 min
Response: 0
Conc: N.D.

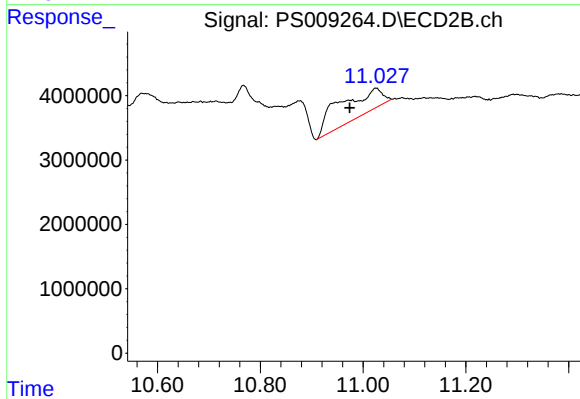

#16 DCPA

R.T.: 11.025 min
Delta R.T.: 0.051 min
Response: 22849461
Conc: 5.90 ng/ml