

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031220\
 Data File : PS009267.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2020 11:52
 Operator : DD\AJ
 Sample : L1752-04
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 14:06:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.242	6.934	227.1E6	232.0E6	410.600	422.449
Target Compounds							
1) T	Dalapon	3.006	2.590	14407801	62383369	18.475	79.231 #
2) T	3,5-DICHL...	0.000	6.111	0	60879729	N.D.	74.855
3) T	4-Nitroph...	7.010	6.592	16090688	13059789	67.406	41.043 #
8) T	DICHLORPROP	8.121	7.754	1261795	36048344	2.447	64.973 #
12) T	2,4,5-T	9.444	9.254	23383479	15330506	9.192	5.193 #
15) T	Picloram	11.037	11.024	51447939	100.5E6	16.952	24.684 #
16) T	DCPA	0.000	11.024	0	100.5E6	N.D.	25.953



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031220\
Data File : PS009267.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2020 11:52
Operator : DD\AJ
Sample : L1752-04
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 14:06:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

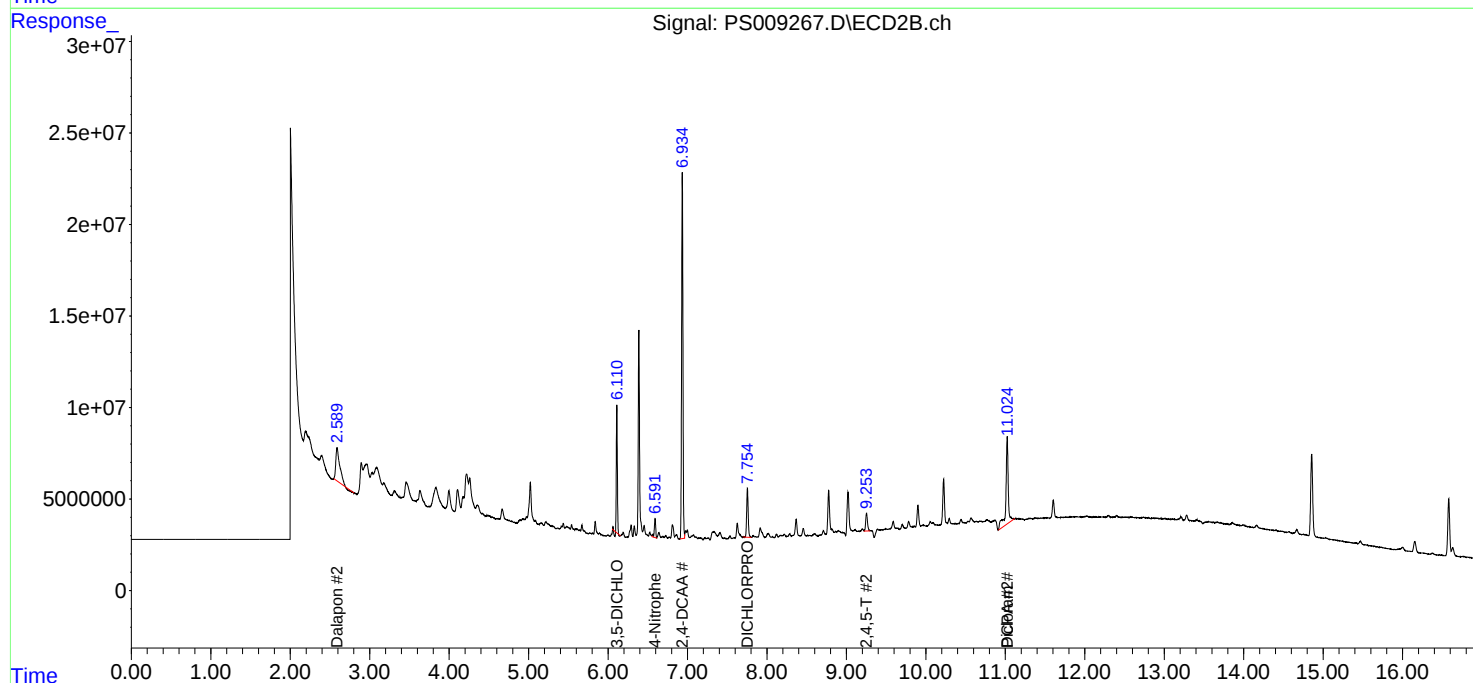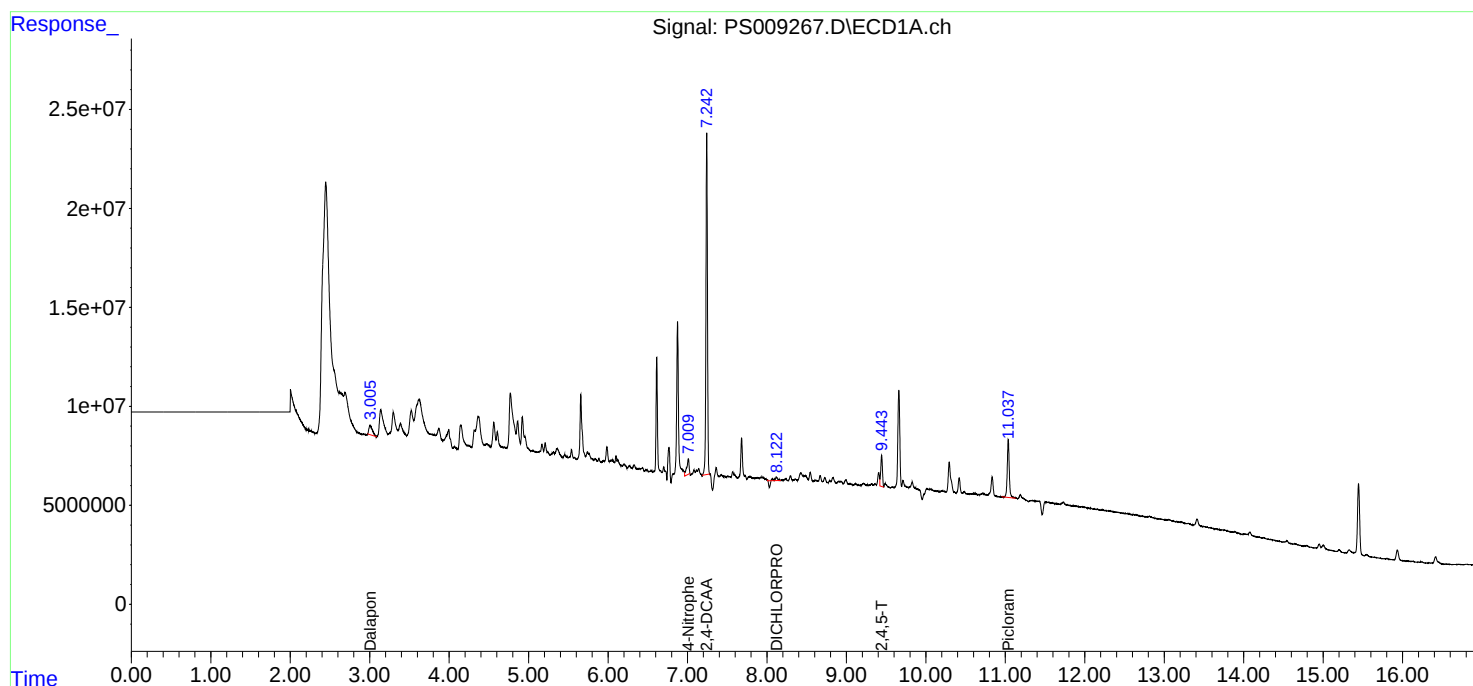


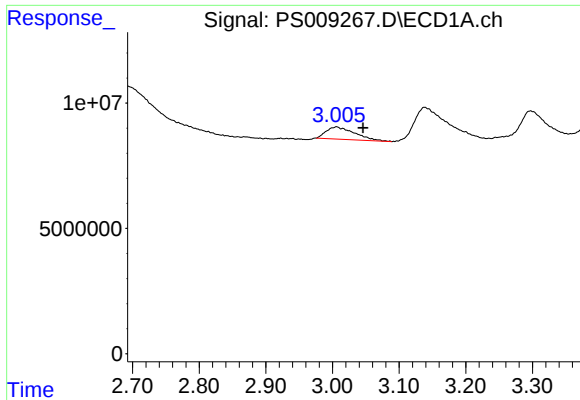

#1 Dalapon


R.T.: 3.006 min
Delta R.T.: -0.040 min
Response: 14407801
Conc: 18.48 ng/ml

Instrument :
ECD_S
ClientSampleId :

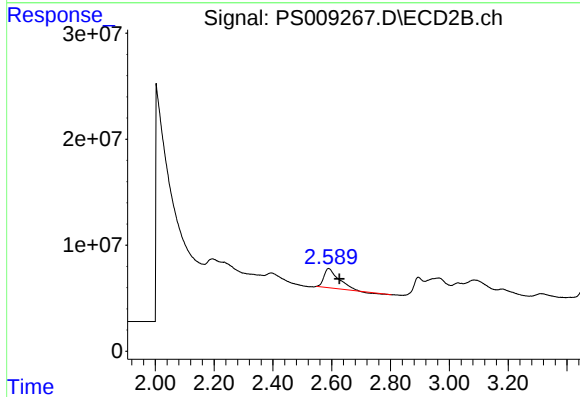


#1 Dalapon

R.T.: 2.590 min
Delta R.T.: -0.037 min
Response: 62383369
Conc: 79.23 ng/ml

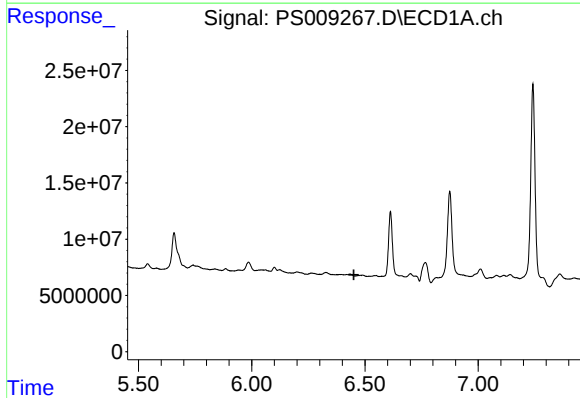


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

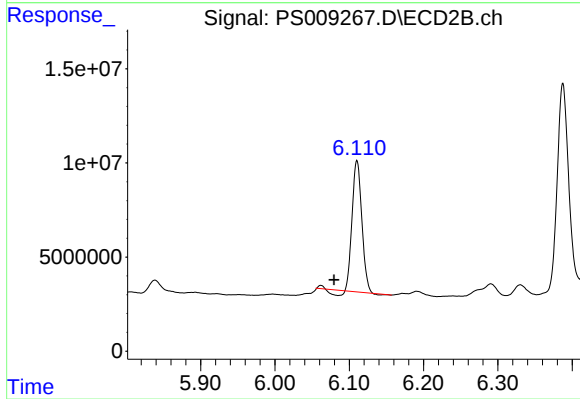

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.111 min
Delta R.T.: 0.031 min
Response: 60879729
Conc: 74.85 ng/ml

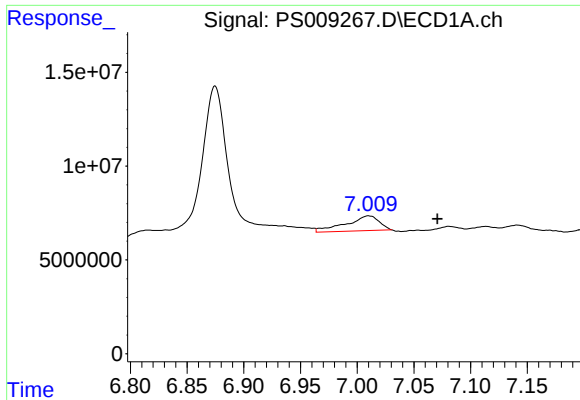

#3 4-Nitrophenol


R.T.: 7.010 min
Delta R.T.: -0.061 min
Response: 16090688
Conc: 67.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

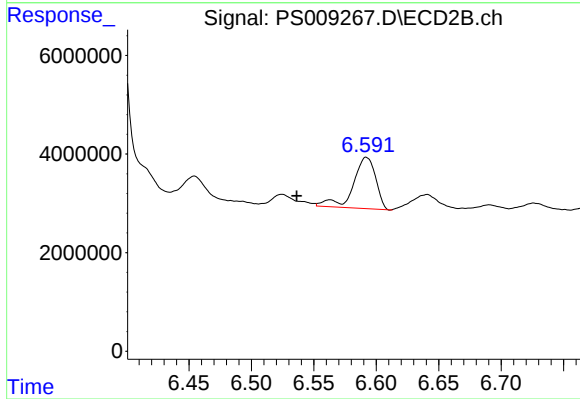


#3 4-Nitrophenol

R.T.: 6.592 min
Delta R.T.: 0.056 min
Response: 13059789
Conc: 41.04 ng/ml

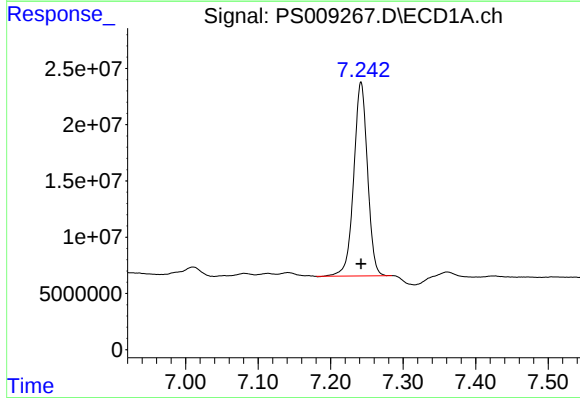


#4 2,4-DCAA

R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 227131505
Conc: 410.60 ng/ml

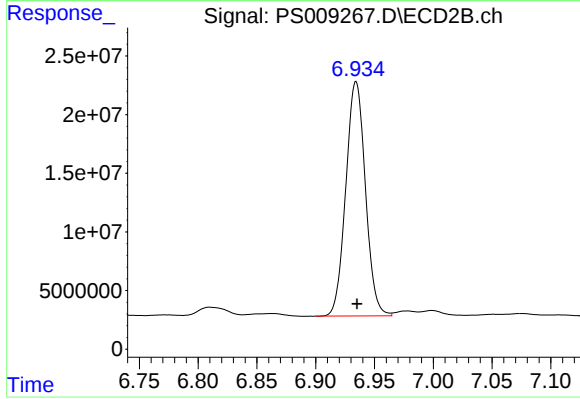

#4 2,4-DCAA


R.T.: 6.934 min
Delta R.T.: 0.000 min
Response: 232007890
Conc: 422.45 ng/ml

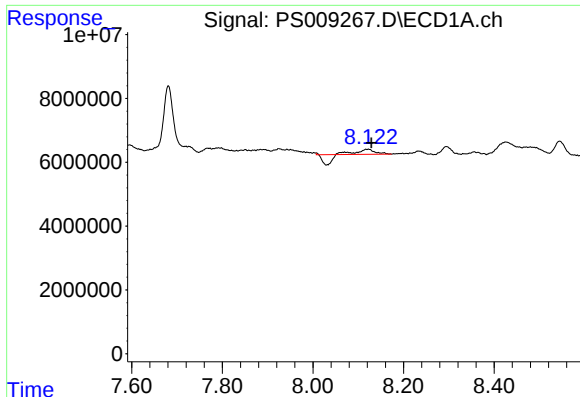

#8 DICHLORPROP


R.T.: 8.121 min
Delta R.T.: -0.008 min
Response: 1261795
Conc: 2.45 ng/ml

Instrument :
ECD_S
ClientSampleId :

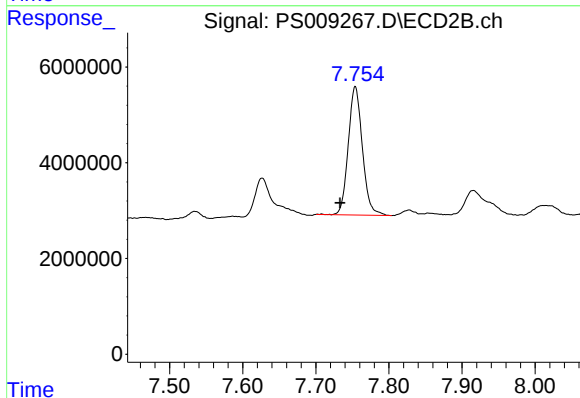


#8 DICHLORPROP

R.T.: 7.754 min
Delta R.T.: 0.021 min
Response: 36048344
Conc: 64.97 ng/ml

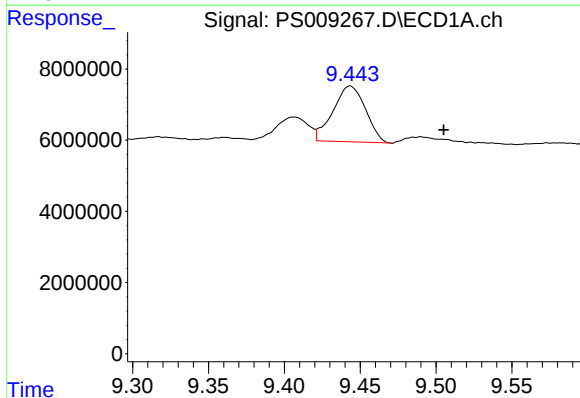


#12 2,4,5-T

R.T.: 9.444 min
Delta R.T.: -0.062 min
Response: 23383479
Conc: 9.19 ng/ml

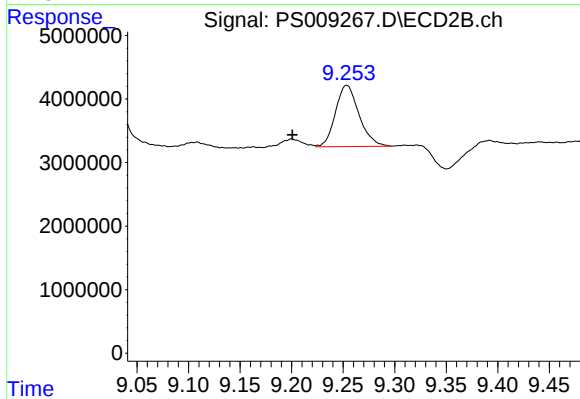

#12 2,4,5-T


R.T.: 9.254 min
Delta R.T.: 0.053 min
Response: 15330506
Conc: 5.19 ng/ml

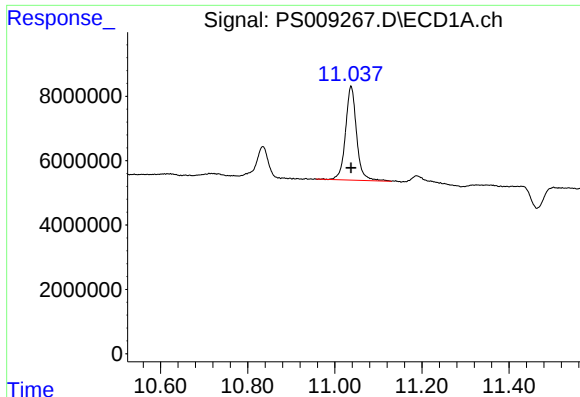

#15 Picloram


R.T.: 11.037 min
Delta R.T.: 0.000 min
Response: 51447939
Conc: 16.95 ng/ml

Instrument :
ECD_S
ClientSampleId :

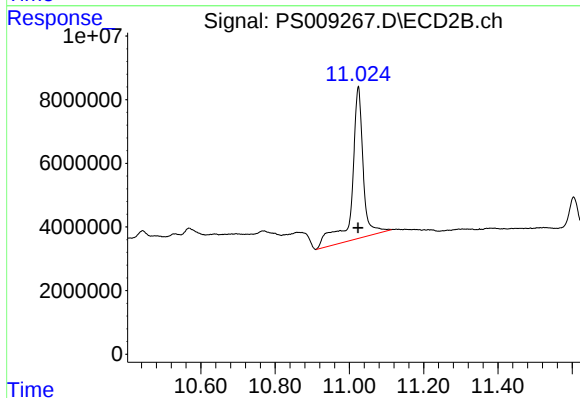


#15 Picloram

R.T.: 11.024 min
Delta R.T.: 0.000 min
Response: 100516332
Conc: 24.68 ng/ml

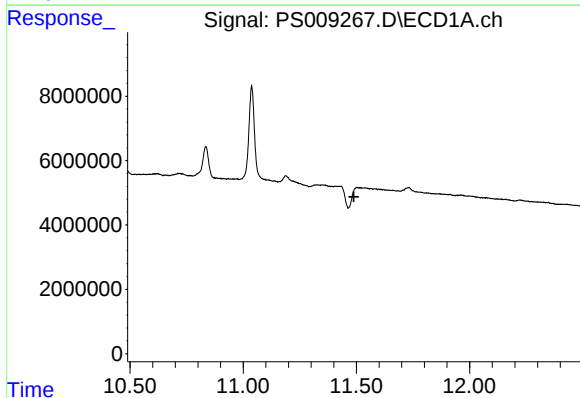

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.489 min
Response: 0
Conc: N.D.

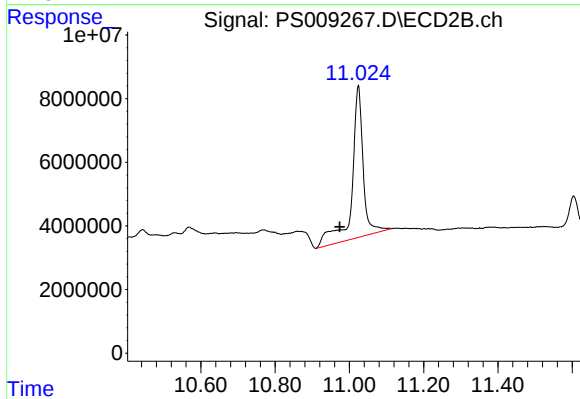

#16 DCPA

R.T.: 11.024 min
Delta R.T.: 0.050 min
Response: 100516332
Conc: 25.95 ng/ml