

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031220\
 Data File : PS009270.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2020 13:01
 Operator : DD\AJ
 Sample : L1797-03
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 14:06:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.242	6.935	220.6E6	219.0E6	398.837	398.795
Target Compounds							
1) T	Dalapon	3.007	2.589	14486394	77745558	18.576	98.742 #
2) T	3,5-DICHL...	0.000	6.110	0	65344351	N.D.	80.344
3) T	4-Nitroph...	7.010	6.593	15374503	11395384	64.406	35.812 #
6) T	MCP	7.564	0.000	948463	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.755	0	38166898	N.D.	68.791
12) T	2,4,5-T	9.444	0.000	17043493	0	6.700	N.D. #
15) T	Picloram	11.036	11.024	12125555	32270567	3.995	7.925 #
16) T	DCPA	0.000	11.024	0	32270567	N.D.	8.332



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031220\
Data File : PS009270.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2020 13:01
Operator : DD\AJ
Sample : L1797-03
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 14:06:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

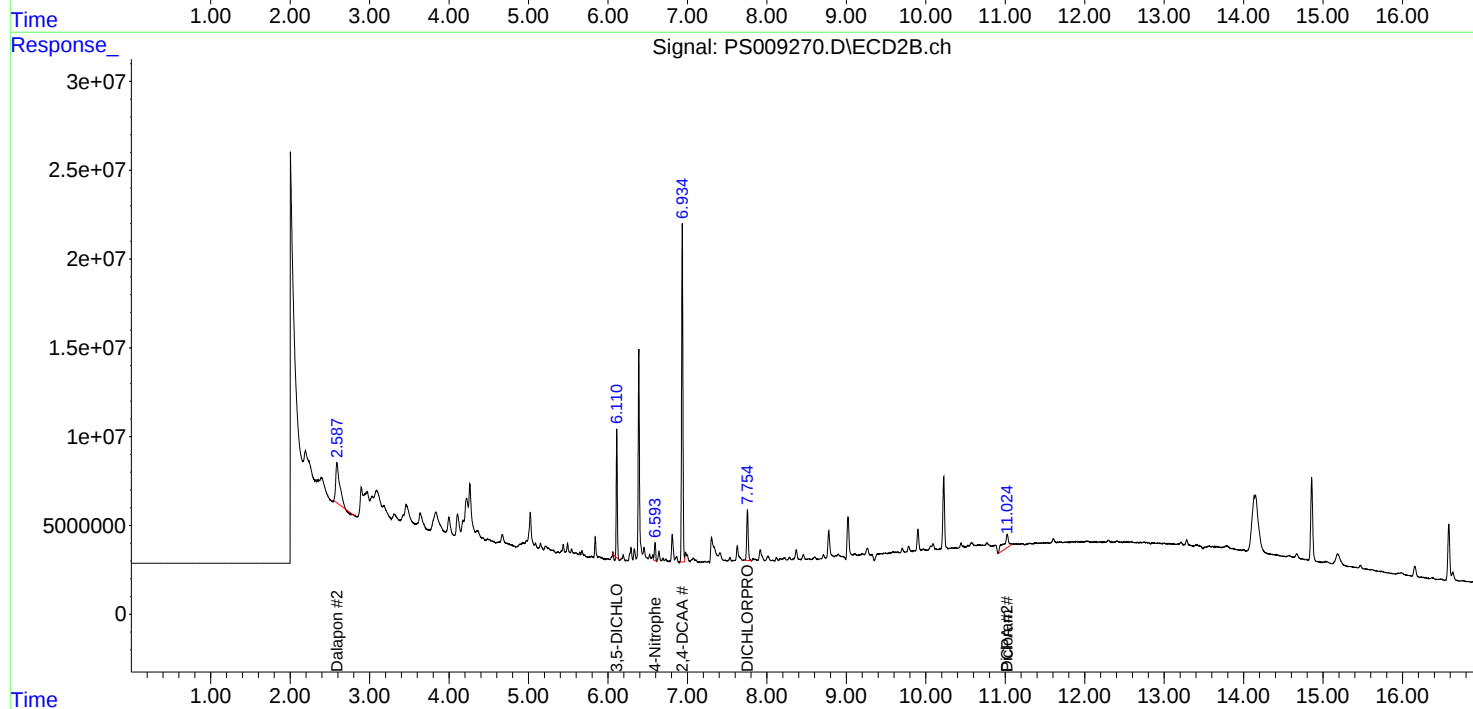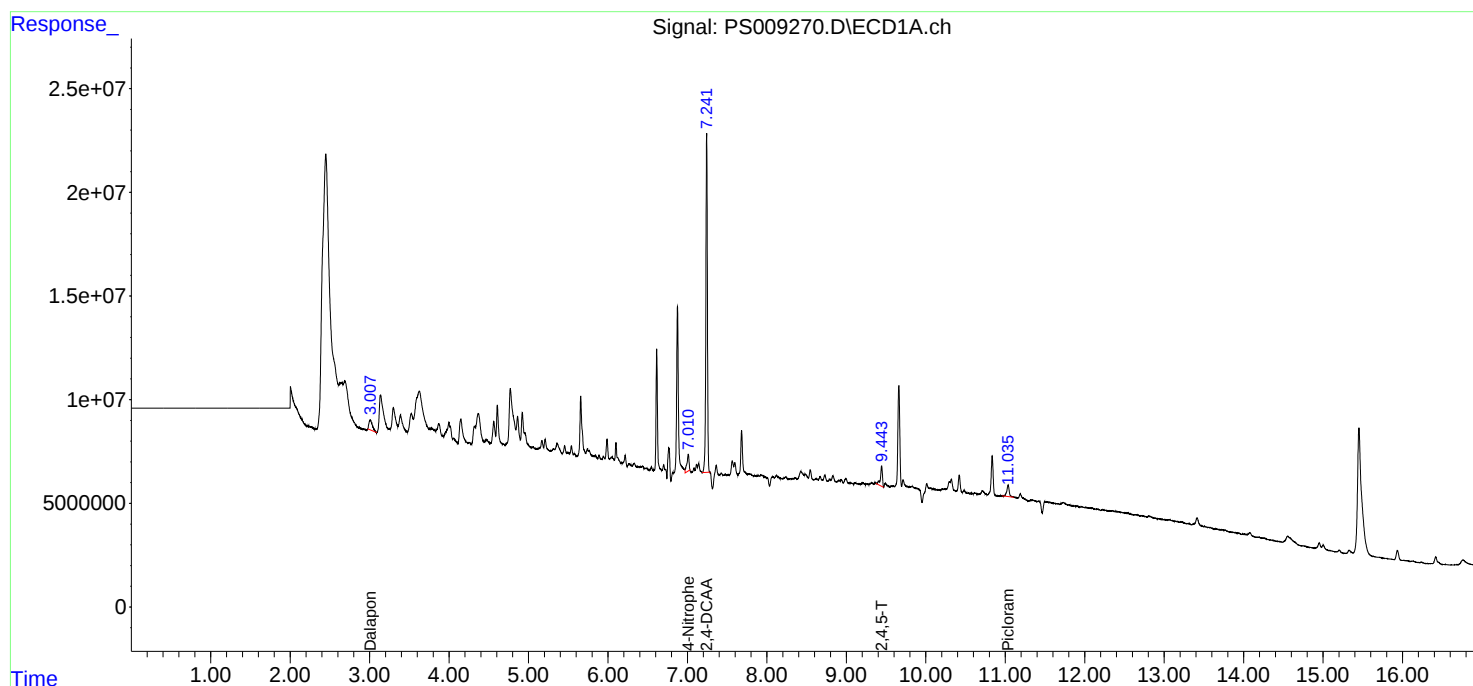


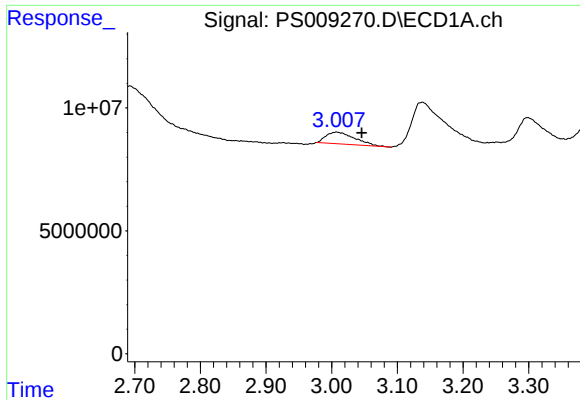

#1 Dalapon


R.T.: 3.007 min
Delta R.T.: -0.039 min
Response: 14486394
Conc: 18.58 ng/ml

Instrument :
ECD_S
ClientSampleId :

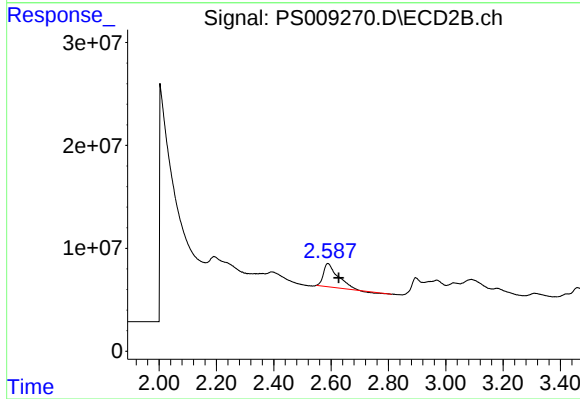


#1 Dalapon

R.T.: 2.589 min
Delta R.T.: -0.038 min
Response: 77745558
Conc: 98.74 ng/ml

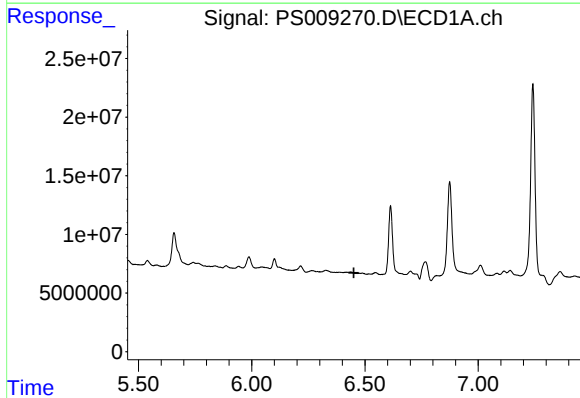


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

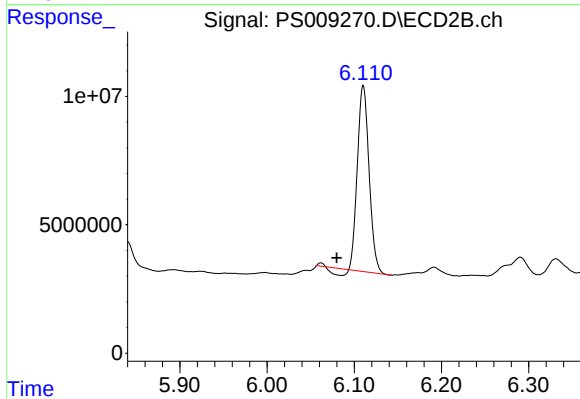

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.110 min
Delta R.T.: 0.031 min
Response: 65344351
Conc: 80.34 ng/ml

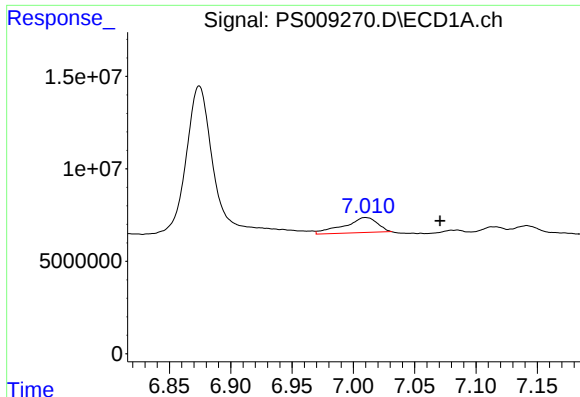

#3 4-Nitrophenol


R.T.: 7.010 min
Delta R.T.: -0.061 min
Response: 15374503
Conc: 64.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

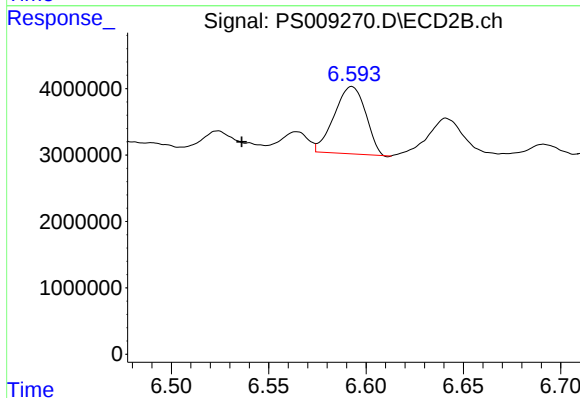


#3 4-Nitrophenol

R.T.: 6.593 min
Delta R.T.: 0.056 min
Response: 11395384
Conc: 35.81 ng/ml

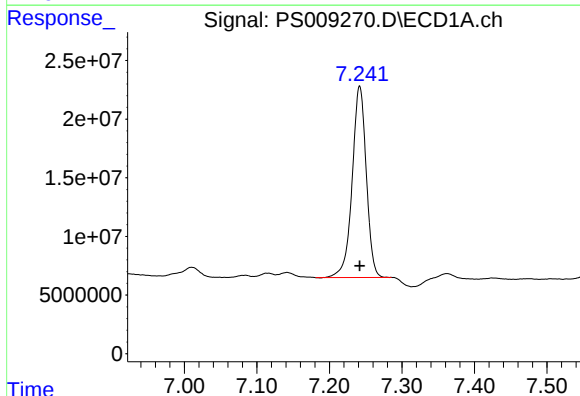


#4 2,4-DCAA

R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 220624734
Conc: 398.84 ng/ml

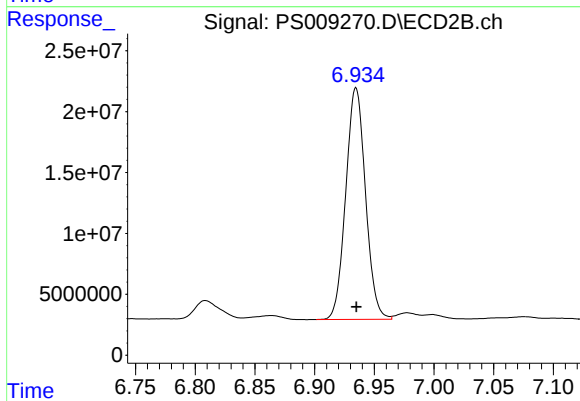

#4 2,4-DCAA


R.T.: 6.935 min
Delta R.T.: 0.000 min
Response: 219017563
Conc: 398.80 ng/ml

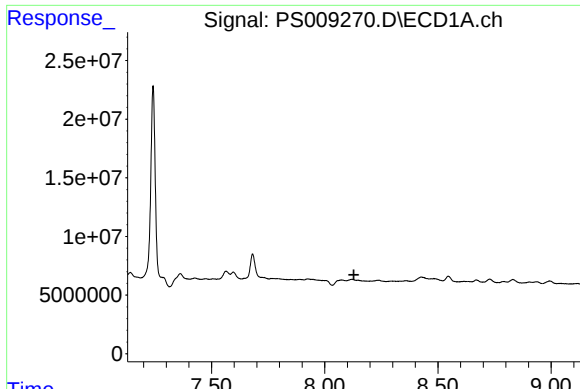

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.129 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

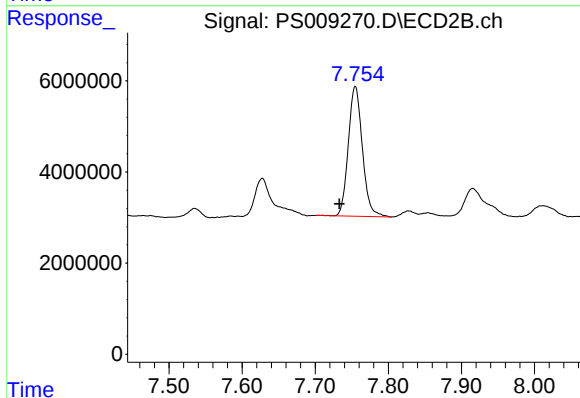


#8 DICHLORPROP

R.T.: 7.755 min
Delta R.T.: 0.022 min
Response: 38166898
Conc: 68.79 ng/ml

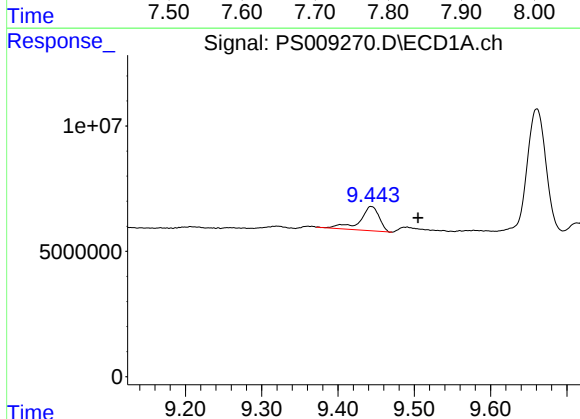


#12 2,4,5-T

R.T.: 9.444 min
Delta R.T.: -0.061 min
Response: 17043493
Conc: 6.70 ng/ml

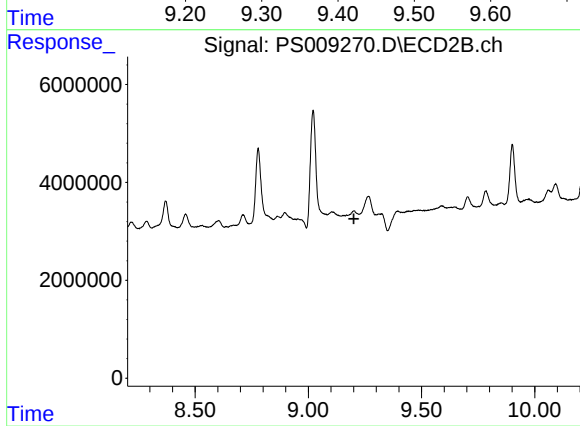

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.201 min
Response: 0
Conc: N.D.

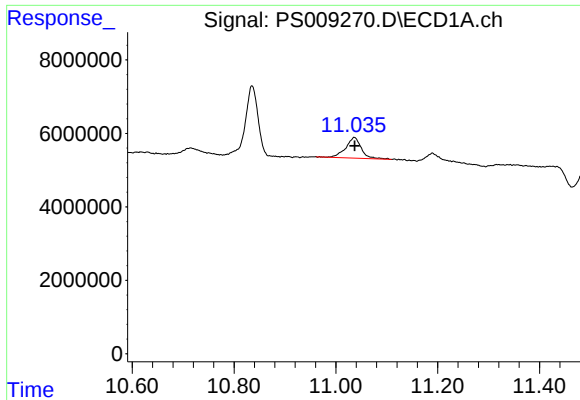

#15 Picloram


R.T.: 11.036 min
Delta R.T.: -0.001 min
Response: 12125555
Conc: 4.00 ng/ml

Instrument :
ECD_S
ClientSampleId :

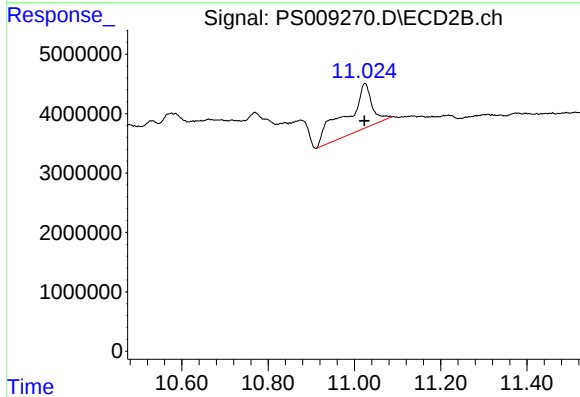


#15 Picloram

R.T.: 11.024 min
Delta R.T.: 0.001 min
Response: 32270567
Conc: 7.92 ng/ml

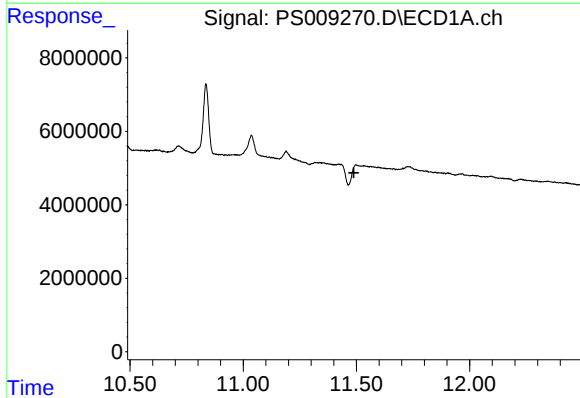

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.489 min
Response: 0
Conc: N.D.

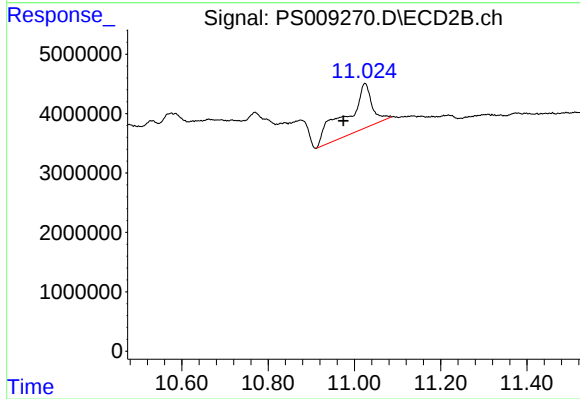

#16 DCPA

R.T.: 11.024 min
Delta R.T.: 0.050 min
Response: 32270567
Conc: 8.33 ng/ml