

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031220\
 Data File : PS009271.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2020 13:24
 Operator : DD\AJ
 Sample : L1893-04
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 14:07:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.243	6.935	232.2E6	239.8E6	419.716	436.703
Target Compounds							
1) T	Dalapon	3.006	2.590	15866042	95594605	20.345	121.411 #
2) T	3,5-DICHL...	0.000	6.111	0	65146677	N.D.	80.101
3) T	4-Nitroph...	7.011	6.593	15096776	10156186	63.242	31.918 #
8) T	DICHLORPROP	8.119	7.755	3323143	34083147	6.443	61.431 #
9) T	2,4-D	8.428	0.000	4740773	0	8.992	N.D. #
12) T	2,4,5-T	9.445	0.000	15550552	0	6.113	N.D. #
15) T	Picloram	0.000	11.026	0	28370663	N.D.	6.967
16) T	DCPA	0.000	11.026	0	28370663	N.D.	7.325



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031220\
Data File : PS009271.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2020 13:24
Operator : DD\AJ
Sample : L1893-04
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 14:07:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

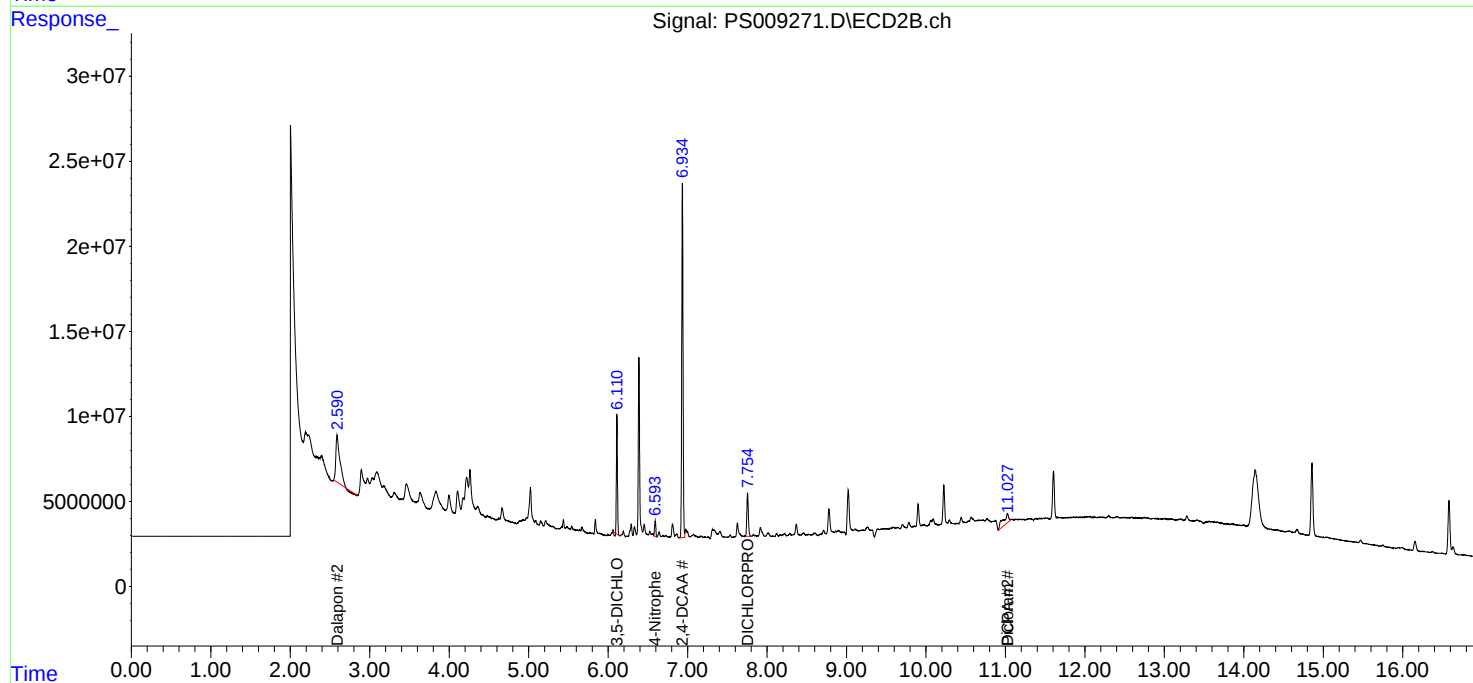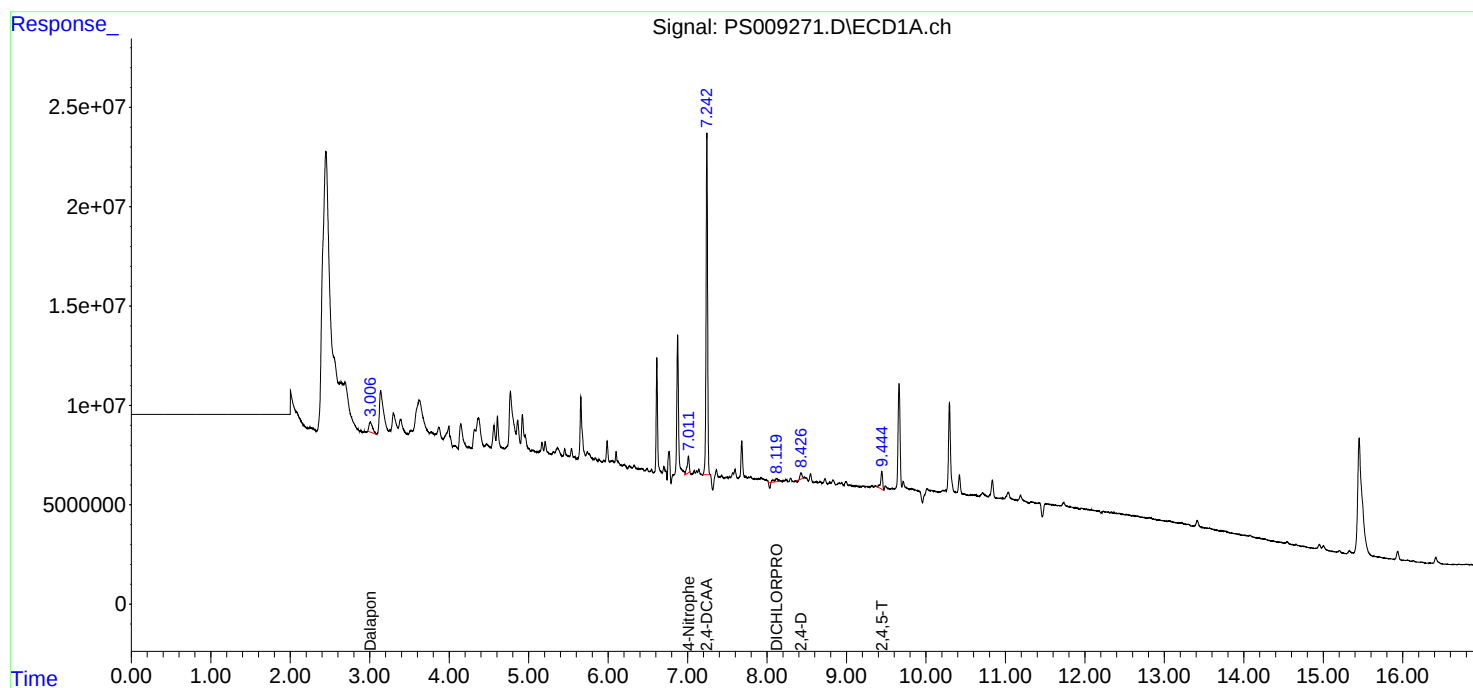


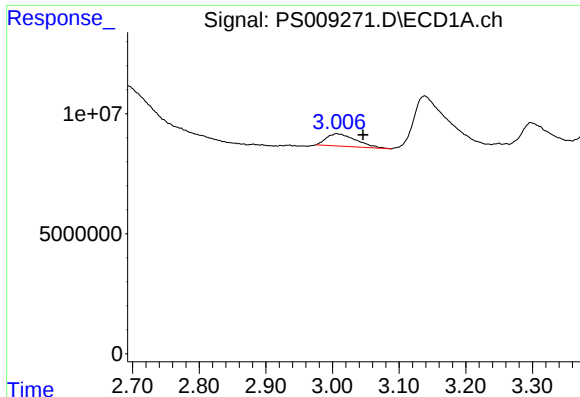

#1 Dalapon


R.T.: 3.006 min
Delta R.T.: -0.040 min
Response: 15866042
Conc: 20.35 ng/ml

Instrument :
ECD_S
ClientSampleId :

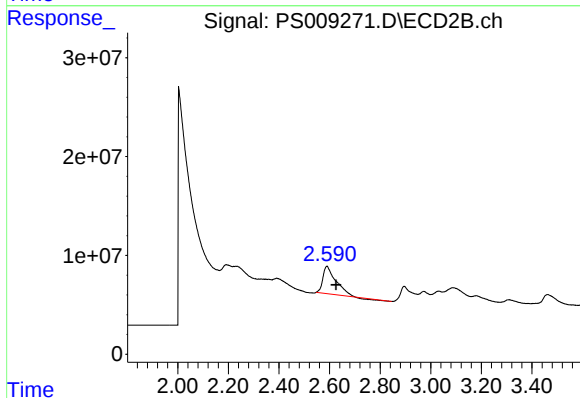


#1 Dalapon

R.T.: 2.590 min
Delta R.T.: -0.037 min
Response: 95594605
Conc: 121.41 ng/ml

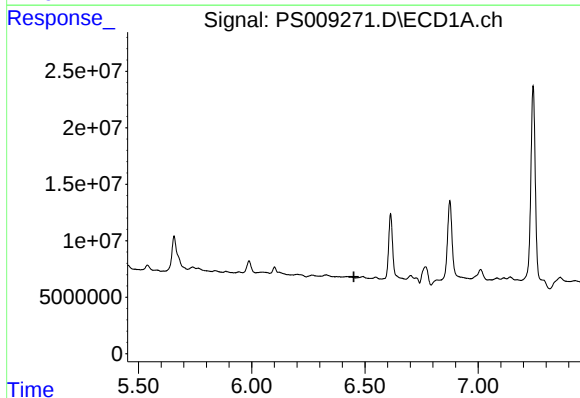


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

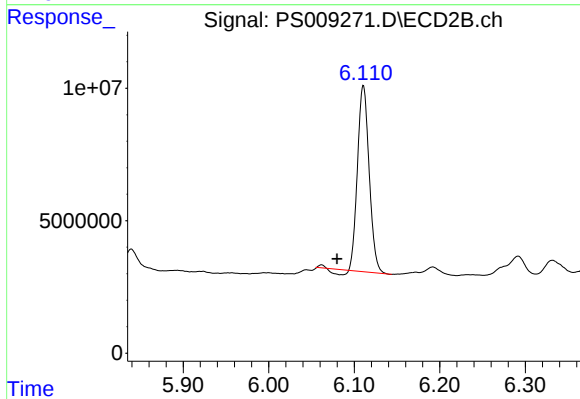

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.111 min
Delta R.T.: 0.031 min
Response: 65146677
Conc: 80.10 ng/ml

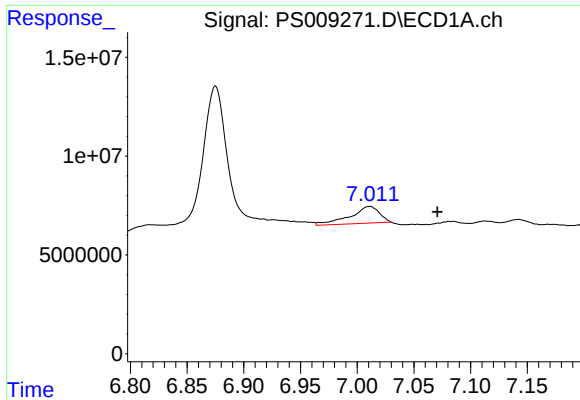

#3 4-Nitrophenol


R.T.: 7.011 min
Delta R.T.: -0.060 min
Response: 15096776
Conc: 63.24 ng/ml

Instrument :
ECD_S
ClientSampleId :

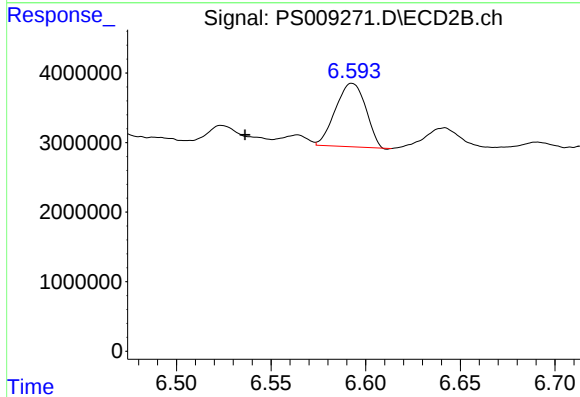


#3 4-Nitrophenol

R.T.: 6.593 min
Delta R.T.: 0.057 min
Response: 10156186
Conc: 31.92 ng/ml

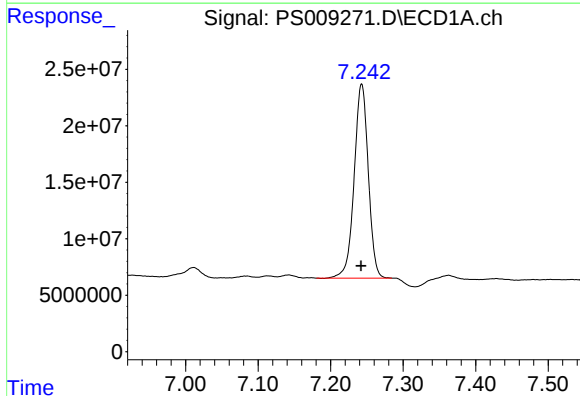


#4 2,4-DCAA

R.T.: 7.243 min
Delta R.T.: 0.000 min
Response: 232174317
Conc: 419.72 ng/ml

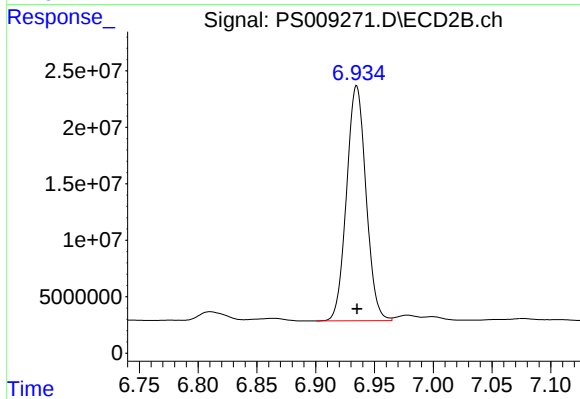

#4 2,4-DCAA


R.T.: 6.935 min
Delta R.T.: 0.000 min
Response: 239836264
Conc: 436.70 ng/ml

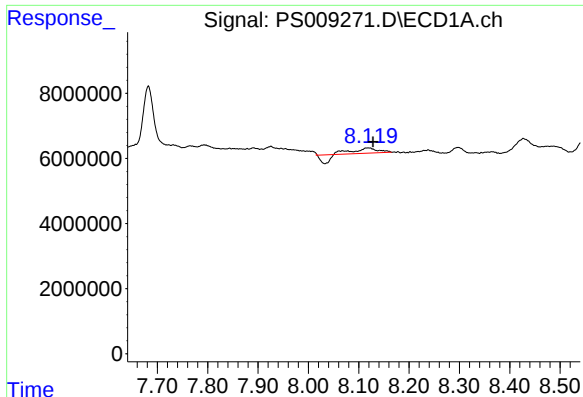

#8 DICHLORPROP


R.T.: 8.119 min
Delta R.T.: -0.010 min
Response: 3323143
Conc: 6.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

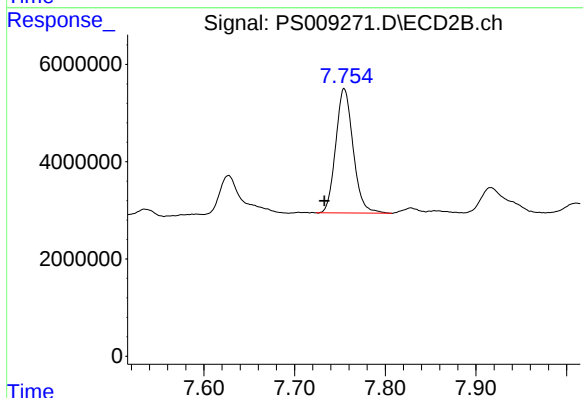


#8 DICHLORPROP

R.T.: 7.755 min
Delta R.T.: 0.022 min
Response: 34083147
Conc: 61.43 ng/ml

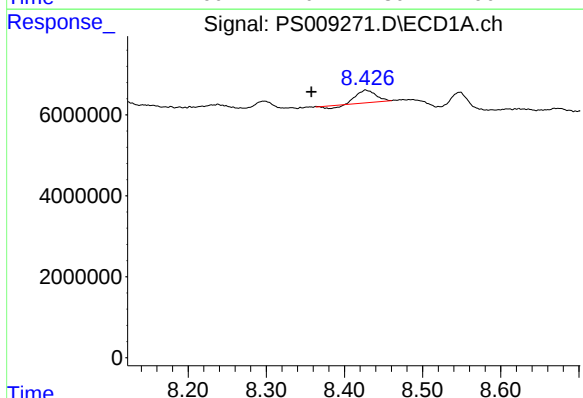


#9 2,4-D

R.T.: 8.428 min
Delta R.T.: 0.070 min
Response: 4740773
Conc: 8.99 ng/ml

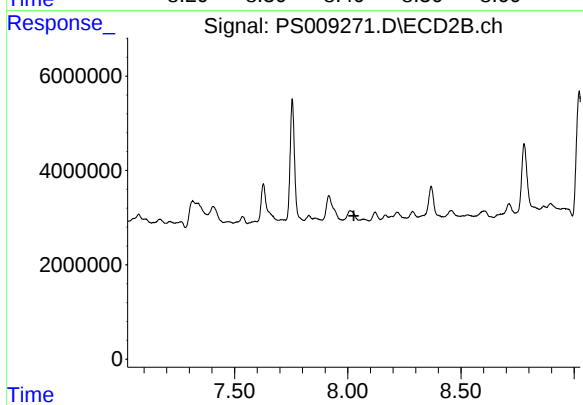

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.027 min
Response: 0
Conc: N.D.

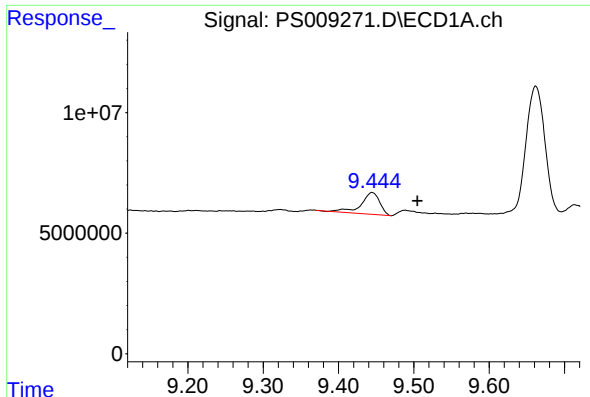

#12 2,4,5-T


R.T.: 9.445 min
Delta R.T.: -0.060 min
Response: 15550552
Conc: 6.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

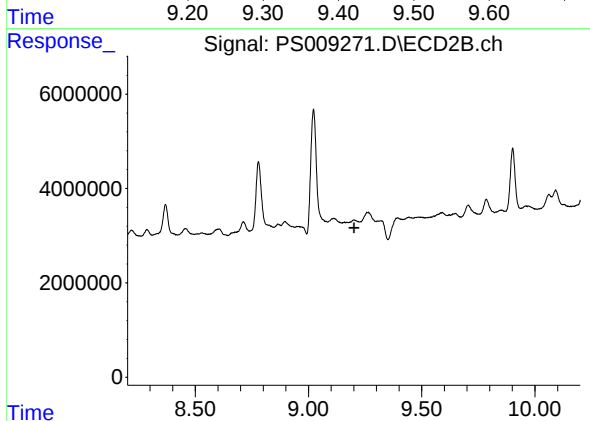


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.201 min
Response: 0
Conc: N.D.

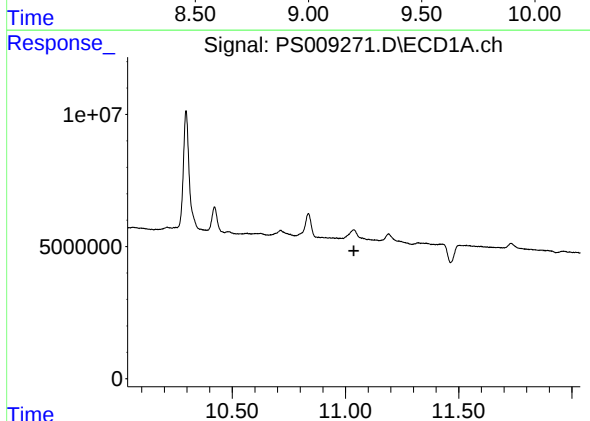


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.037 min
Response: 0
Conc: N.D.

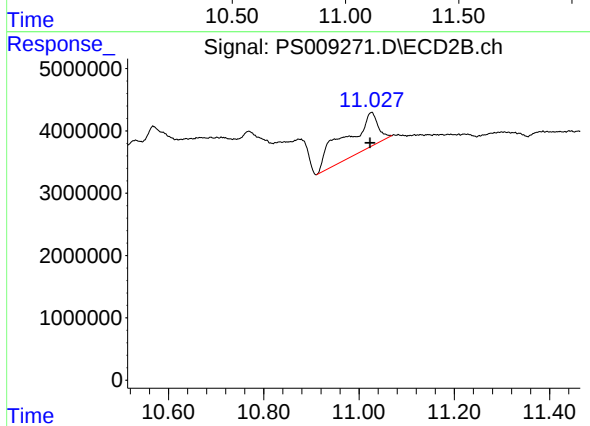

#15 Picloram


R.T.: 11.026 min
Delta R.T.: 0.003 min
Response: 28370663
Conc: 6.97 ng/ml

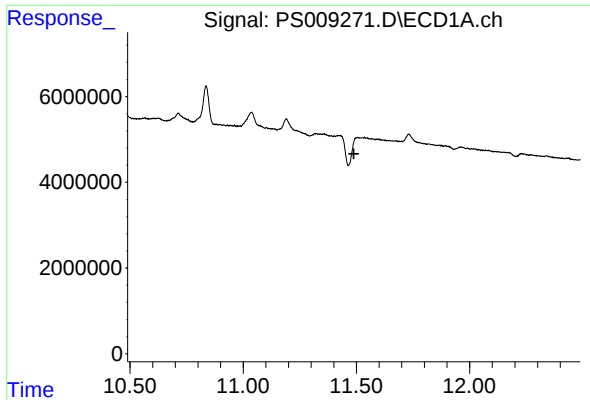

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.489 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

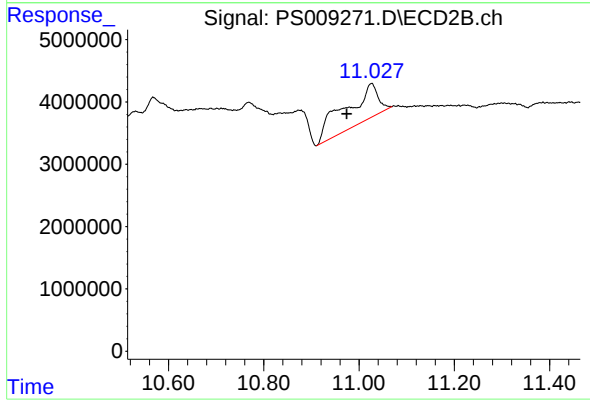

#16 DCPA

R.T.: 11.026 min
Delta R.T.: 0.052 min
Response: 28370663
Conc: 7.33 ng/ml