

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031220\
 Data File : PS009273.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2020 14:09
 Operator : DD\AJ
 Sample : L1893-12
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 14:32:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.243	6.935	216.4E6	217.8E6	391.238	396.493
Target Compounds							
1) T	Dalapon	0.000	2.589	0 62517242		N.D.	79.401
2) T	3,5-DICHL...	0.000	6.111	0 52895600		N.D.	65.038
3) T	4-Nitroph...	7.011	6.593	13424108	10331650	56.235	32.469 #
8) T	DICHLORPROP	8.118	7.755	-409720	38800968	N.D.	69.934
10) T	Pentachlo...	8.671	8.460	195.8E6	211.4E6	27.849	27.851
12) T	2,4,5-T	9.444	0.000	15530316	0	6.105	N.D. #
15) T	Picloram	0.000	11.026	0 26380887		N.D.	6.478
16) T	DCPA	0.000	11.026	0 26380887		N.D.	6.811



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031220\
Data File : PS009273.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2020 14:09
Operator : DD\AJ
Sample : L1893-12
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 14:32:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

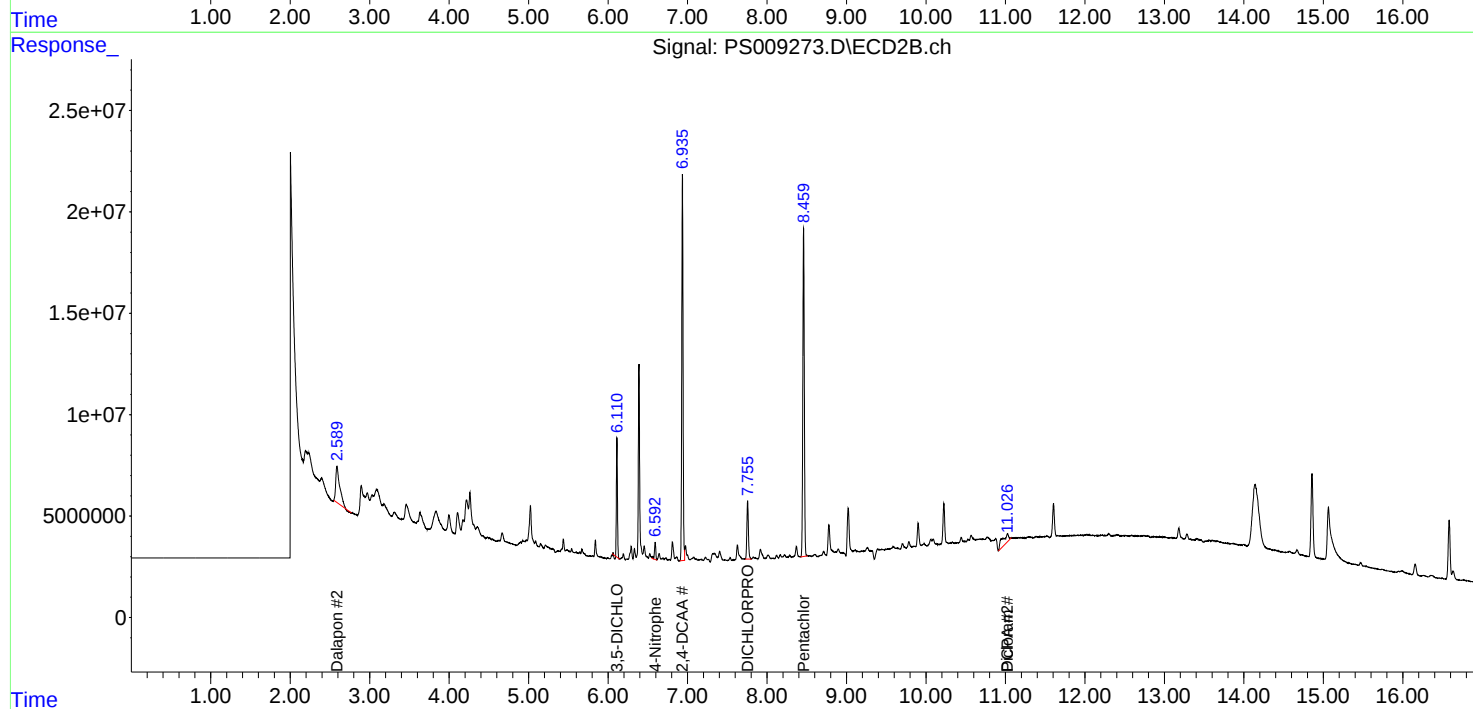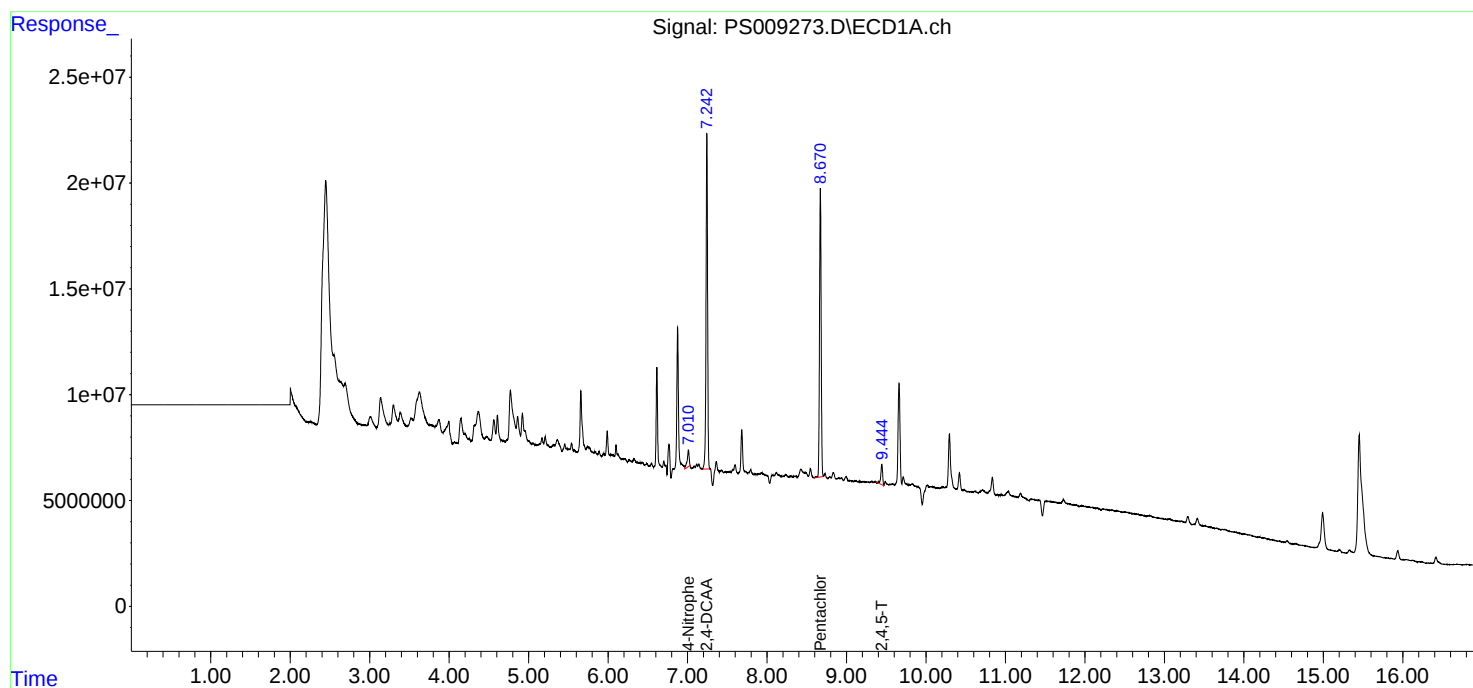


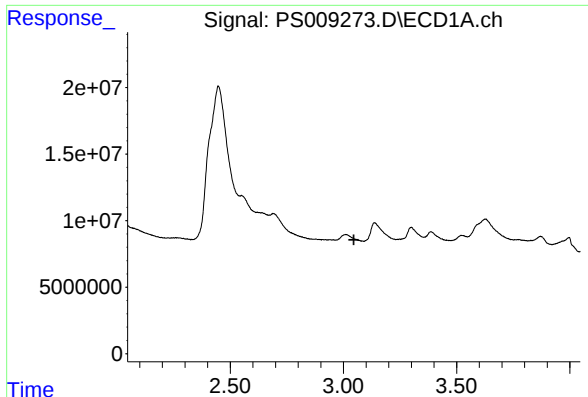

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.046 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

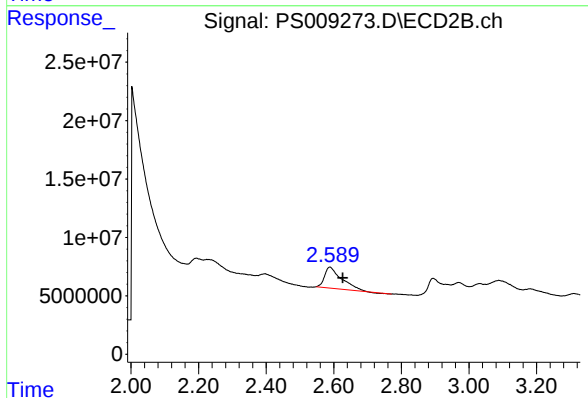


#1 Dalapon

R.T.: 2.589 min
Delta R.T.: -0.038 min
Response: 62517242
Conc: 79.40 ng/ml

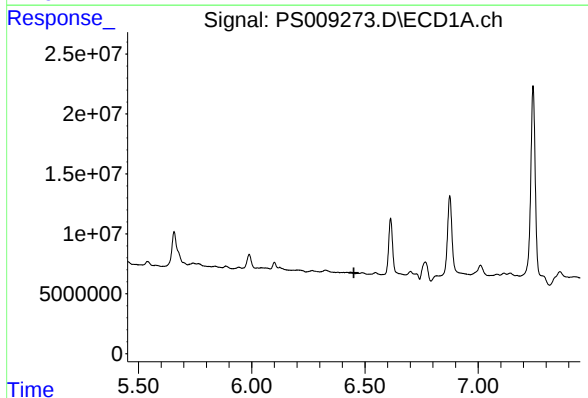


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.451 min
Response: 0
Conc: N.D.

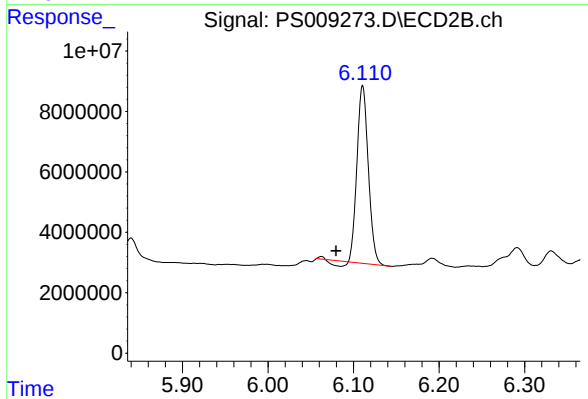

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.111 min
Delta R.T.: 0.031 min
Response: 52895600
Conc: 65.04 ng/ml

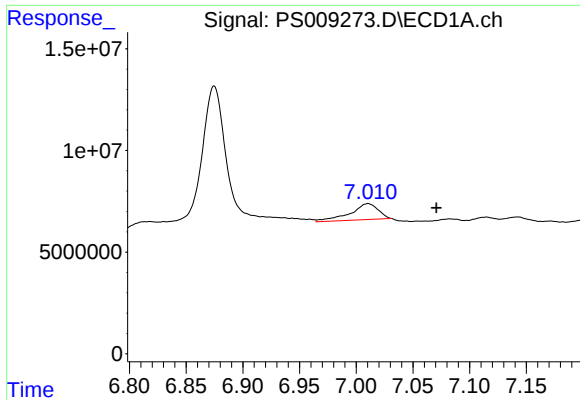

#3 4-Nitrophenol


R.T.: 7.011 min
Delta R.T.: -0.060 min
Response: 13424108
Conc: 56.24 ng/ml

Instrument :
ECD_S
ClientSampleId :

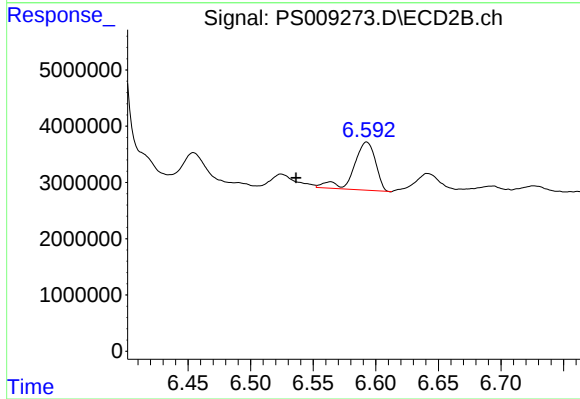


#3 4-Nitrophenol

R.T.: 6.593 min
Delta R.T.: 0.056 min
Response: 10331650
Conc: 32.47 ng/ml

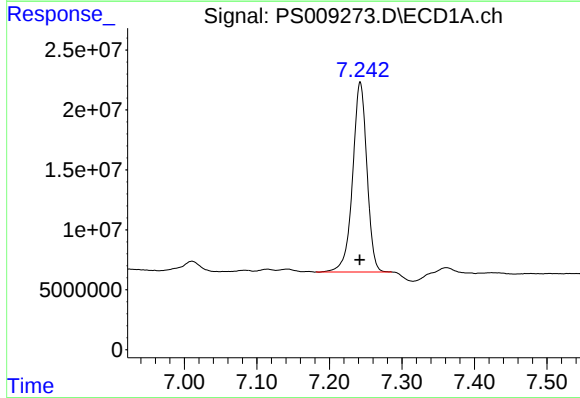


#4 2,4-DCAA

R.T.: 7.243 min
Delta R.T.: 0.000 min
Response: 216421382
Conc: 391.24 ng/ml

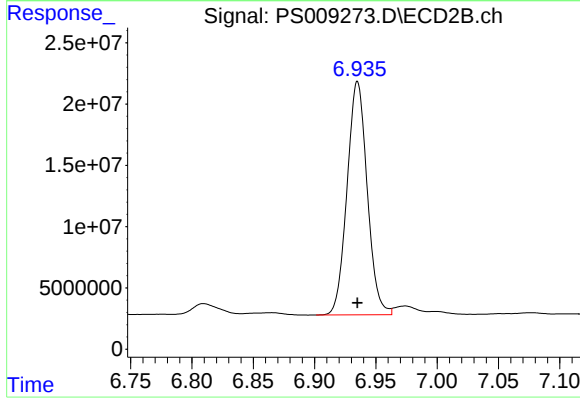

#4 2,4-DCAA


R.T.: 6.935 min
Delta R.T.: 0.000 min
Response: 217753153
Conc: 396.49 ng/ml

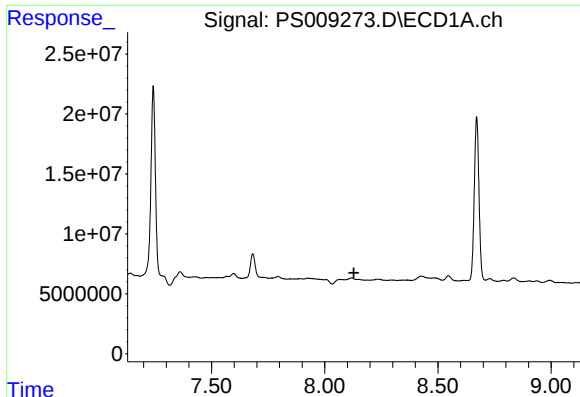

#8 DICHLORPROP


R.T.: 8.118 min
Delta R.T.: -0.011 min
Response: -409720
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

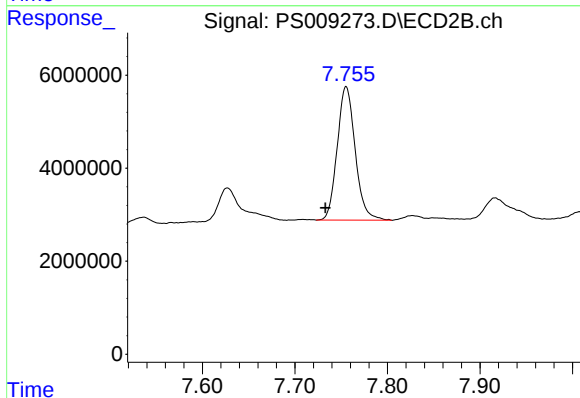


#8 DICHLORPROP

R.T.: 7.755 min
Delta R.T.: 0.022 min
Response: 38800968
Conc: 69.93 ng/ml

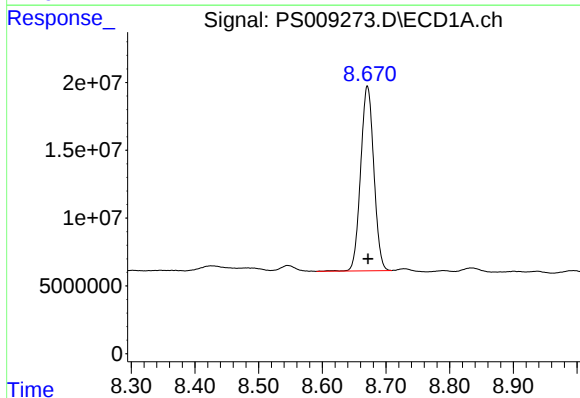


#10 Pentachlorophenol

R.T.: 8.671 min
Delta R.T.: 0.000 min
Response: 195809656
Conc: 27.85 ng/ml

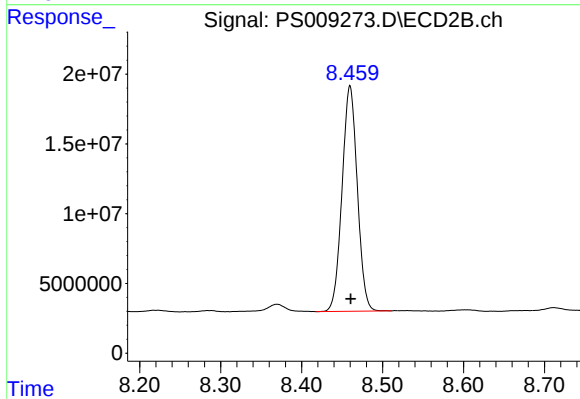

#10 Pentachlorophenol


R.T.: 8.460 min
Delta R.T.: 0.000 min
Response: 211390202
Conc: 27.85 ng/ml

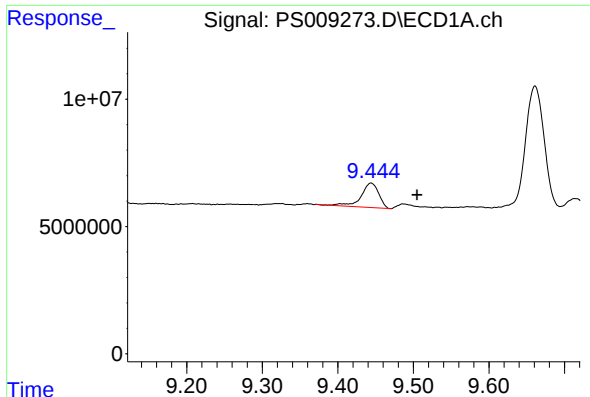

#12 2,4,5-T


R.T.: 9.444 min
Delta R.T.: -0.061 min
Response: 15530316
Conc: 6.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

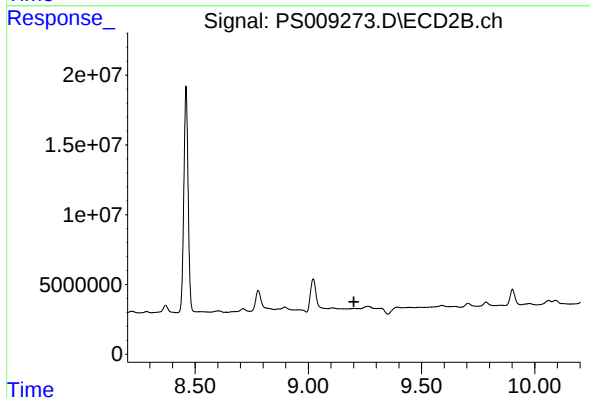


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.201 min
Response: 0
Conc: N.D.

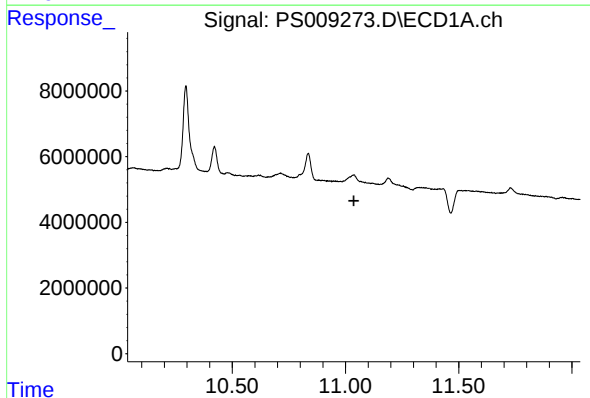


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.037 min
Response: 0
Conc: N.D.

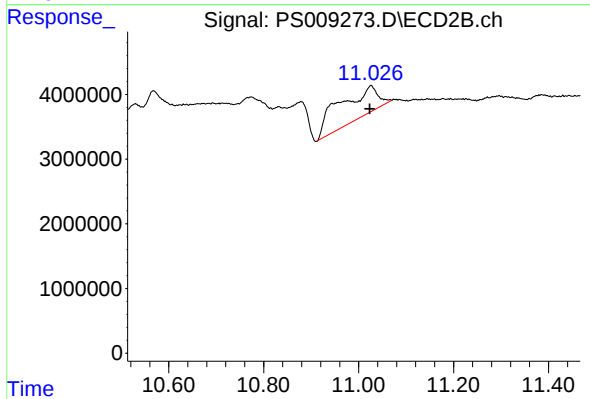

#15 Picloram


R.T.: 11.026 min
Delta R.T.: 0.003 min
Response: 26380887
Conc: 6.48 ng/ml

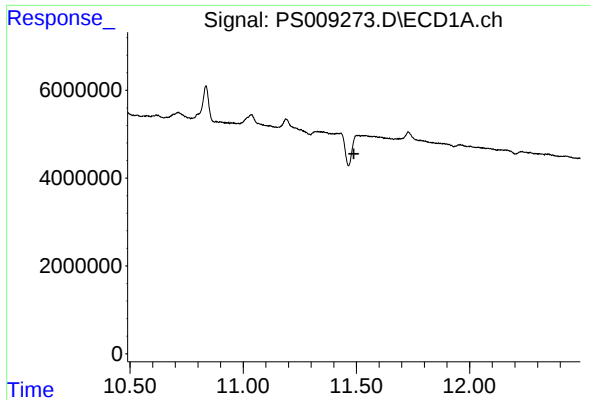

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.489 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

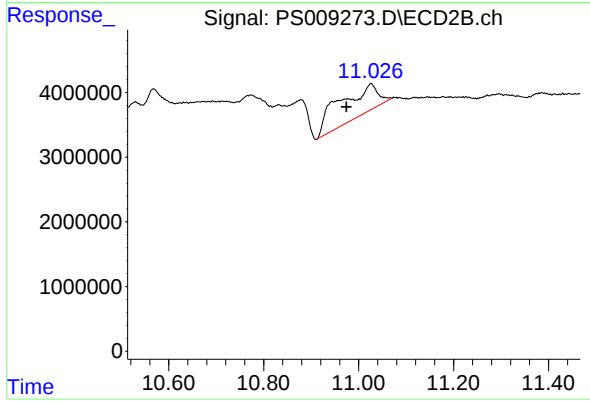

#16 DCPA

R.T.: 11.026 min
Delta R.T.: 0.052 min
Response: 26380887
Conc: 6.81 ng/ml