

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031221\
 Data File : PS014220.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2021 16:54
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 03:34:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS030521.M
 Quant Title : 8080.M
 QLast Update : Sat Mar 06 03:17:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	6.852f	0	617385	N.D.	1.623
Target Compounds							
1) T	Dalapon	2.958f	0.000	534570	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.466f	0.000	269.2E6	0	194.691	N.D. #
3) T	4-Nitroph...	6.998f	0.000	851630	0	1.640	N.D. #
5) T	DICAMBA	0.000	7.087	0	306124	N.D.	<MDL
6) T	MCP	0.000	7.137	0	140.4E6	N.D.	105.912
8) T	DICHLORPROP	0.000	7.745f	0	150648	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.845f	0	730755	N.D.	<MDL
14) T	DINOSEB	0.000	10.006	0	1854740	N.D.	1.178
15) T	Picloram	11.070f	11.065f	28864397	13241604	3.616	4.011
16) T	DCPA	0.000	10.856f	0	9897454	N.D.	2.949



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031221\
Data File : PS014220.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2021 16:54
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 03:34:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS030521.M
Quant Title : 8080.M
QLast Update : Sat Mar 06 03:17:26 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

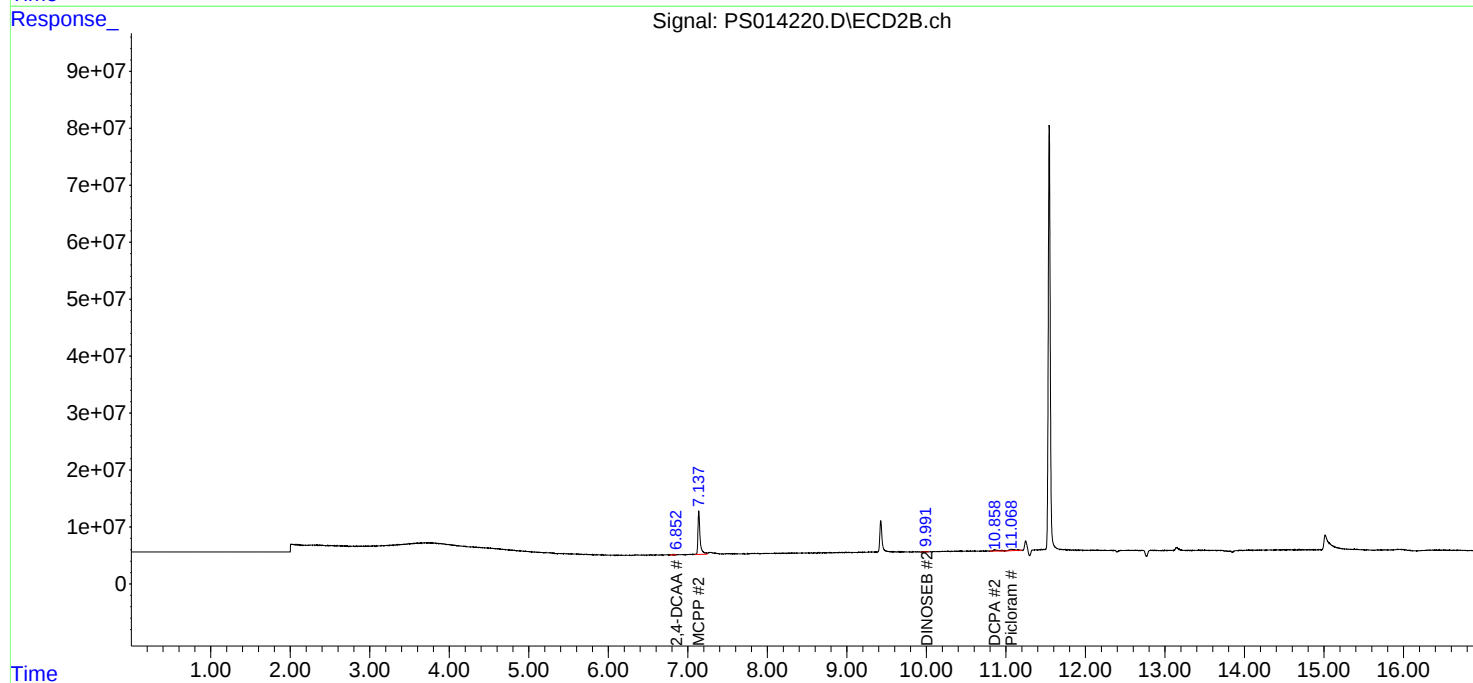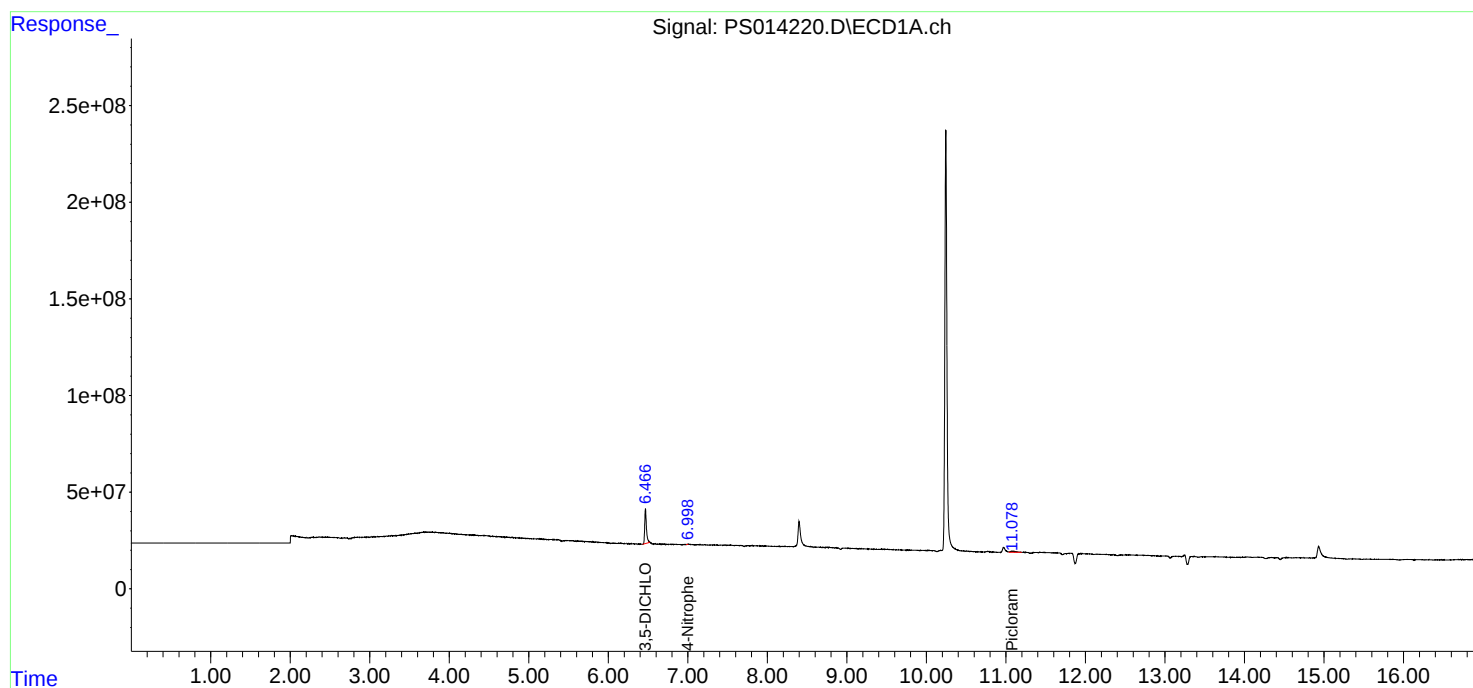


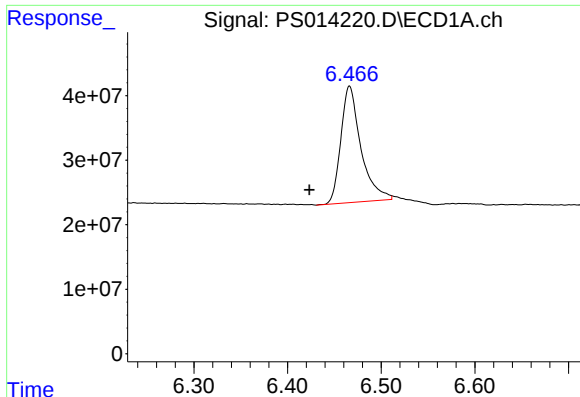

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.466 min
Delta R.T.: 0.043 min
Response: 269238956
Conc: 194.69 ng/ml

Instrument :
ECD_S
ClientSampleId :

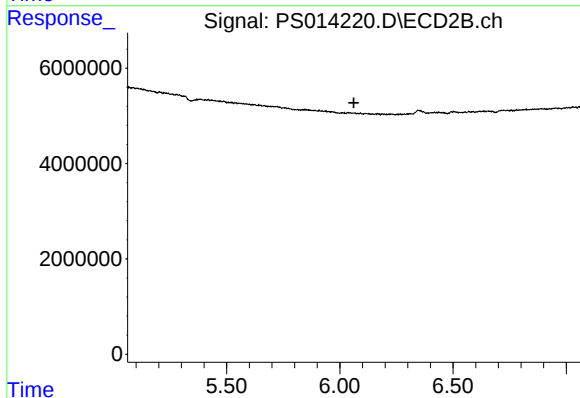


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.062 min
Response: 0
Conc: N.D.

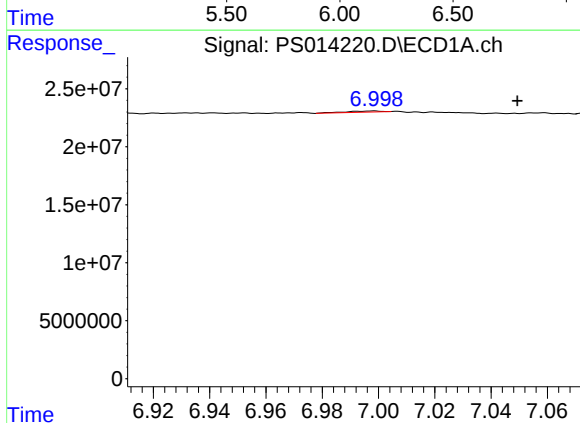


#3 4-Nitrophenol

R.T.: 6.998 min
Delta R.T.: -0.051 min
Response: 851630
Conc: 1.64 ng/ml

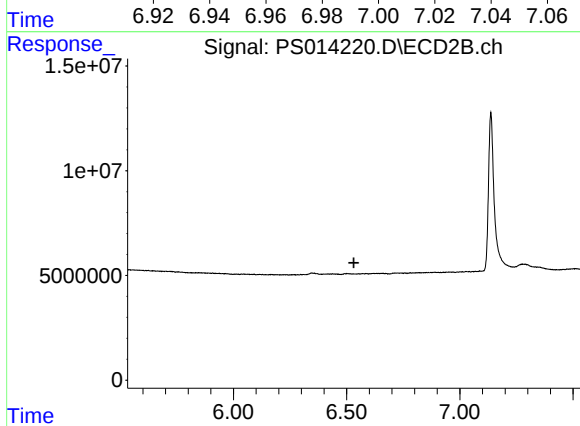

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.532 min
Response: 0
Conc: N.D.

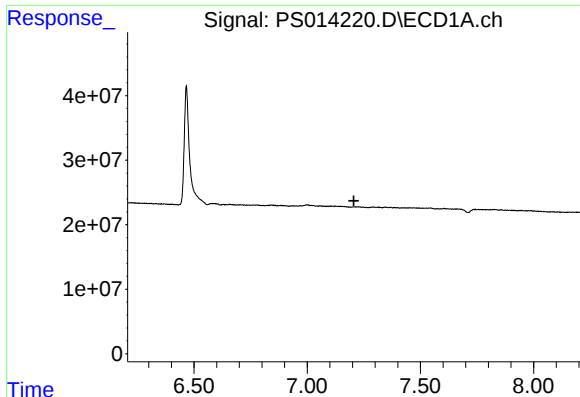

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.206 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

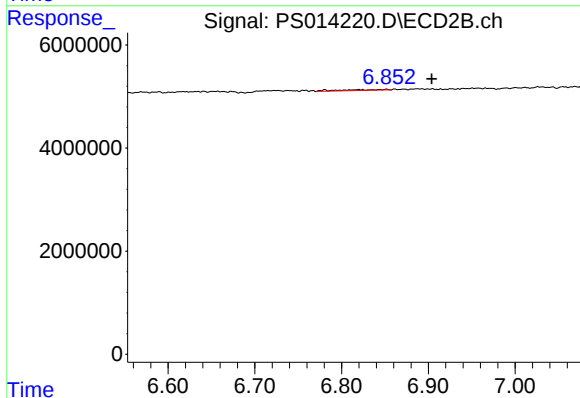


#4 2,4-DCAA

R.T.: 6.852 min
Delta R.T.: -0.052 min
Response: 617385
Conc: 1.62 ng/ml

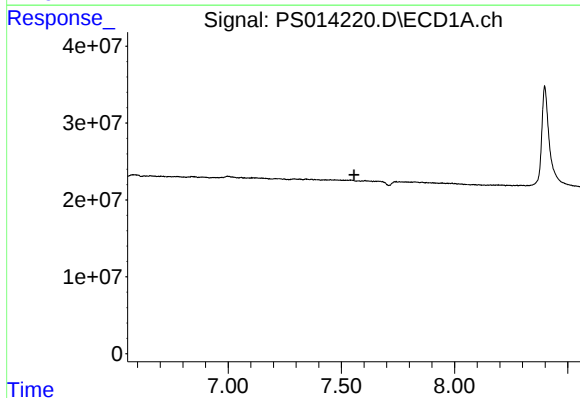


#6 MCP

R.T.: 0.000 min
Exp R.T.: 7.556 min
Response: 0
Conc: N.D.

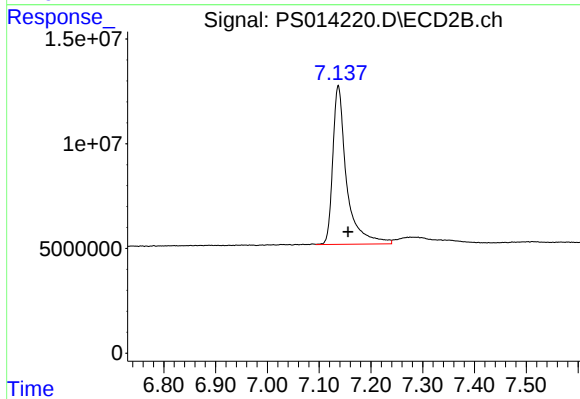

#6 MCP


R.T.: 7.137 min
Delta R.T.: -0.019 min
Response: 140383044
Conc: 105.91 ug/ml

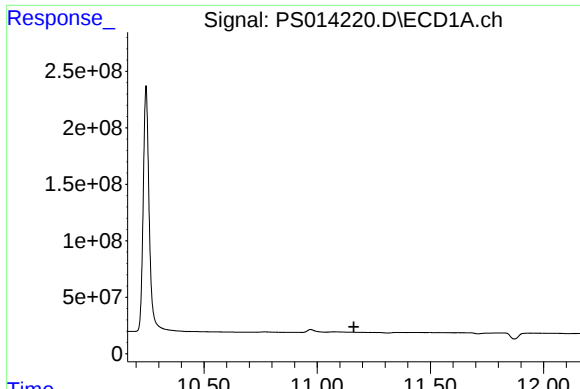

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 11.162 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

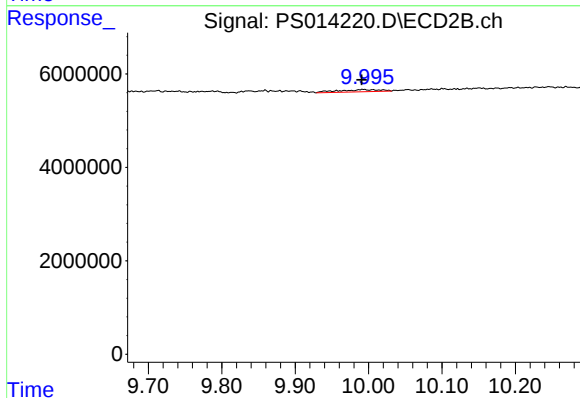


#14 DINOSEB

R.T.: 10.006 min
Delta R.T.: 0.015 min
Response: 1854740
Conc: 1.18 ng/ml

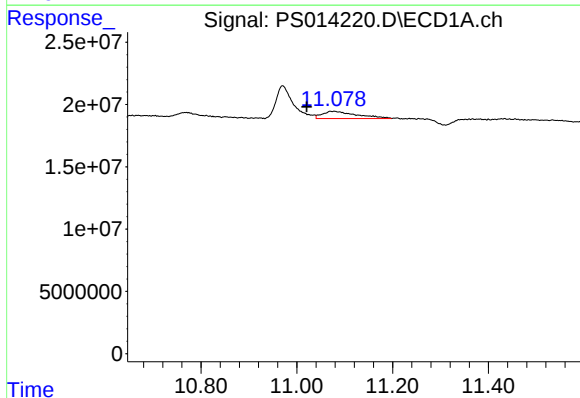


#15 Picloram

R.T.: 11.070 min
Delta R.T.: 0.049 min
Response: 28864397
Conc: 3.62 ng/ml

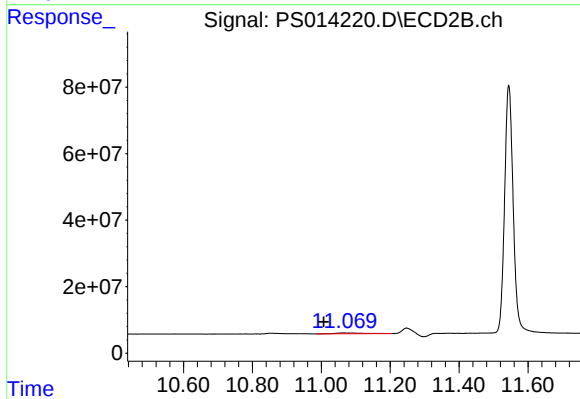

#15 Picloram


R.T.: 11.065 min
Delta R.T.: 0.058 min
Response: 13241604
Conc: 4.01 ng/ml

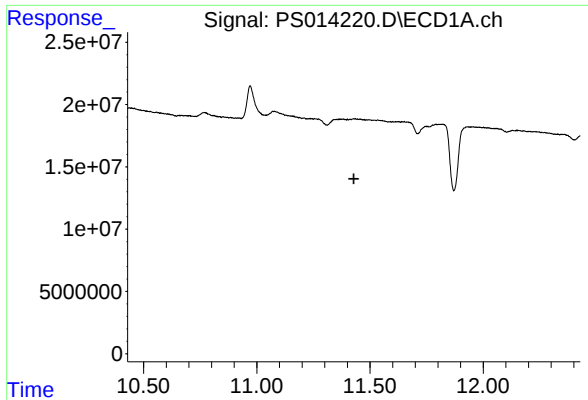

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.428 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

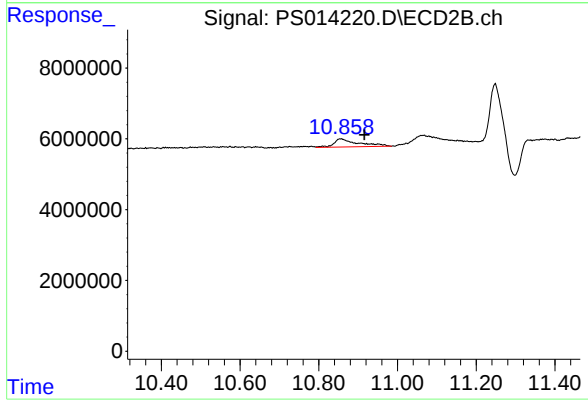

#16 DCPA

R.T.: 10.856 min
Delta R.T.: -0.060 min
Response: 9897454
Conc: 2.95 ng/ml