

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031225\
 Data File : PS029394.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2025 08:39
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 02:27:54 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022125.M
 Quant Title : 8080.M
 QLast Update : Sat Feb 22 01:02:20 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.177	0.000	741934	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	0.000	2.672	0	3376632	N.D.	1.595
2) T	3,5-DICHL...	6.347	0.000	3261802	0	<MDL	N.D. #
3) T	4-Nitroph...	6.941	0.000	2352169	0	1.005	N.D. #
5) T	DICAMBA	7.342	0.000	1485317	0	<MDL	N.D. #
7) T	MCPA	7.696	0.000	652972	0	<MDL	N.D. #
8) T	DICHLORPROP	8.042	0.000	512107	0	<MDL	N.D. #
9) T	2,4-D	8.279	0.000	185186	0	<MDL	N.D. #
10) T	Pentachlo...	8.562	0.000	8211962	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.138	0.000	5957720	0	<MDL	N.D. #
12) T	2,4,5-T	9.445	10.159	8797611	6418168	<MDL	<MDL #
13) T	2,4-DB	10.030f	0.000	2174361	0	<MDL	N.D. #
15) T	Picloram	11.030	12.177	47797078	45058355	1.565	3.897 #
16) T	DCPA	11.519f	12.177f	15726894	45058355	<MDL	3.807 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031225\
Data File : PS029394.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2025 08:39
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 02:27:54 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022125.M
Quant Title : 8080.M
QLast Update : Sat Feb 22 01:02:20 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

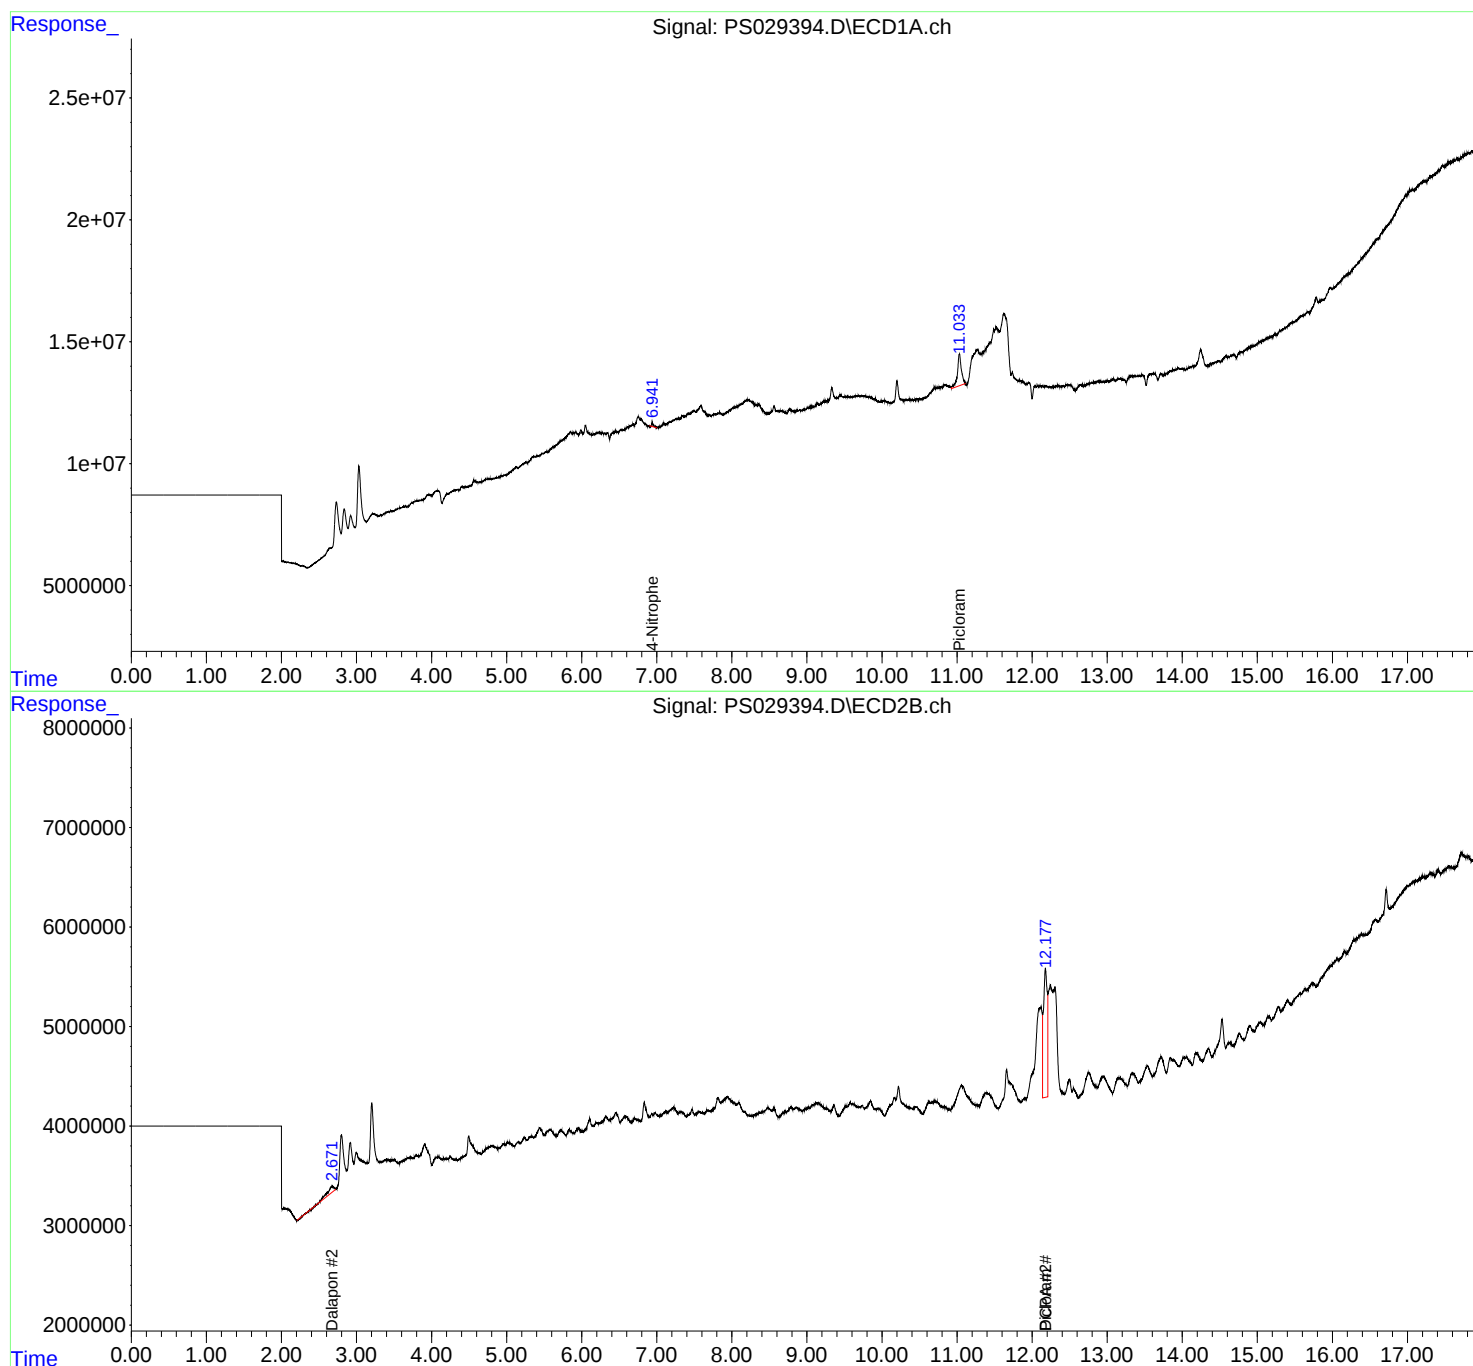


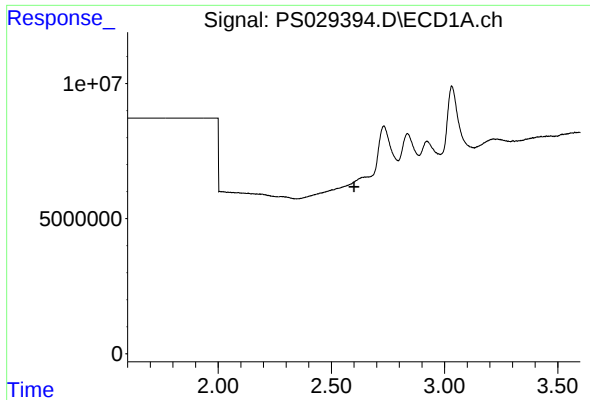

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.600 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

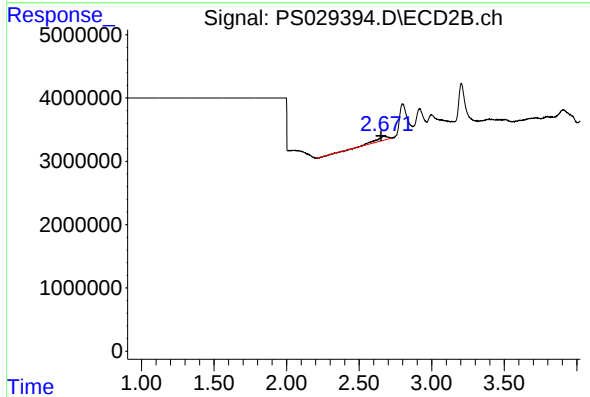


#1 Dalapon

R.T.: 2.672 min
Delta R.T.: 0.022 min
Response: 3376632
Conc: 1.59 ng/ml

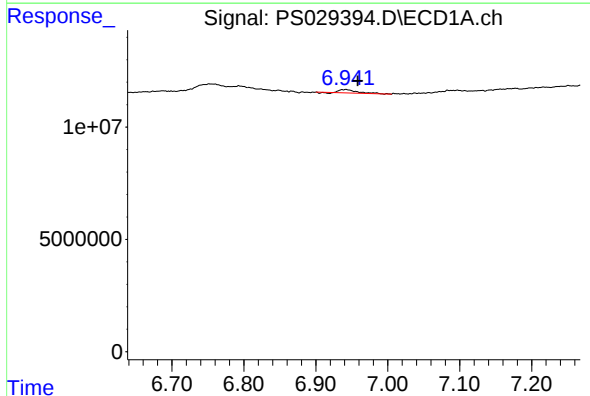


#3 4-Nitrophenol

R.T.: 6.941 min
Delta R.T.: -0.018 min
Response: 2352169
Conc: 1.01 ng/ml

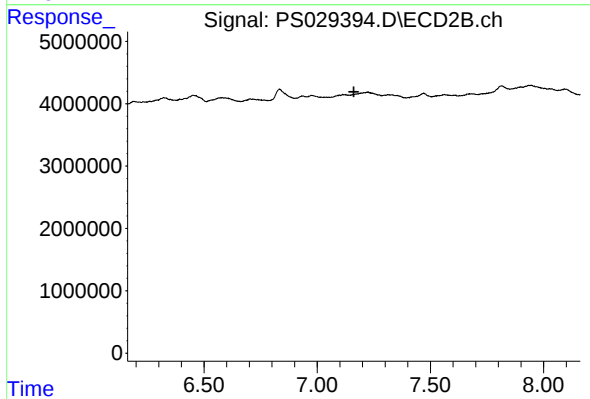

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.162 min
Response: 0
Conc: N.D.

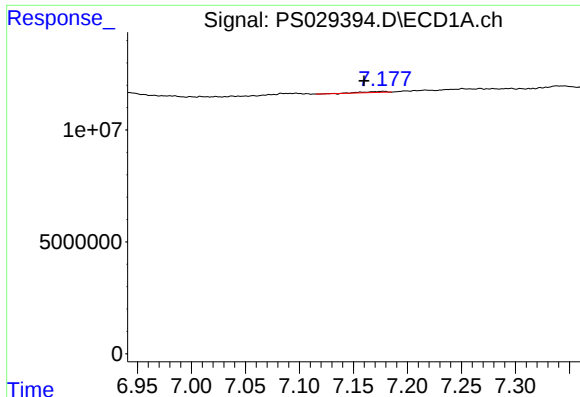

#4 2,4-DCAA


R.T.: 7.177 min
Delta R.T.: 0.017 min
Response: 741934
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

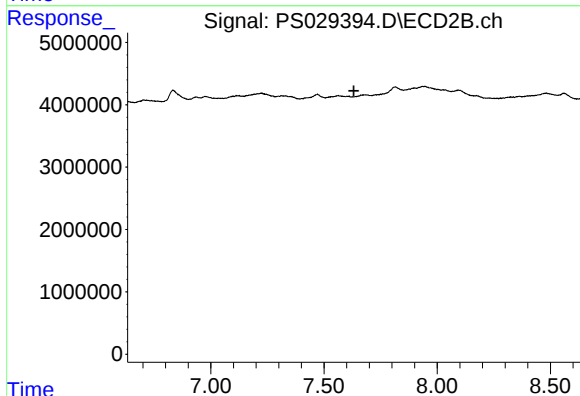


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.632 min
Response: 0
Conc: N.D.

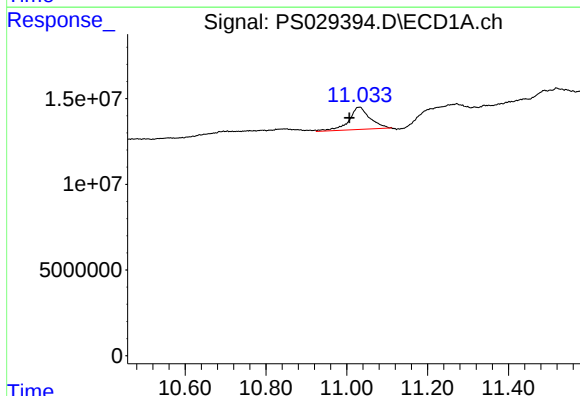


#15 Picloram

R.T.: 11.030 min
Delta R.T.: 0.024 min
Response: 47797078
Conc: 1.56 ng/ml

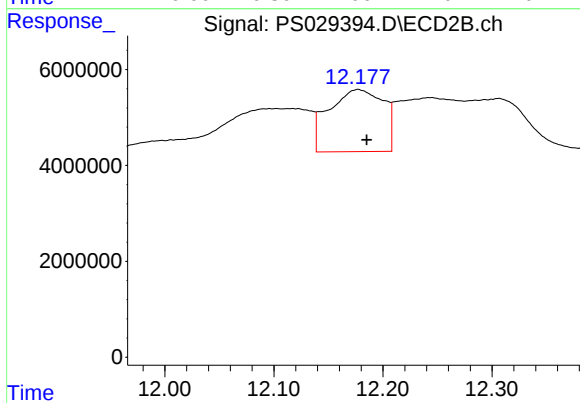

#15 Picloram


R.T.: 12.177 min
Delta R.T.: -0.008 min
Response: 45058355
Conc: 3.90 ng/ml

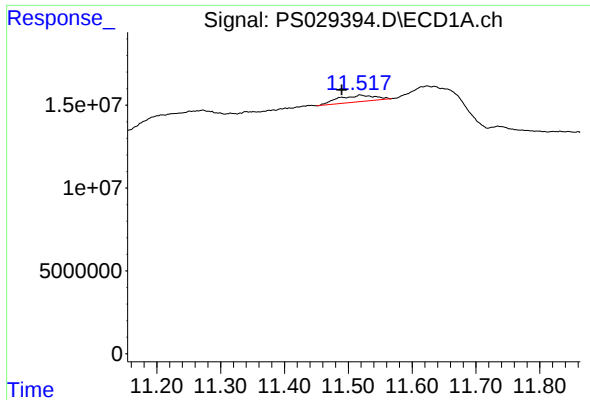

#16 DCPA

R.T.: 11.519 min
Delta R.T.: 0.029 min
Response: 15726894
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

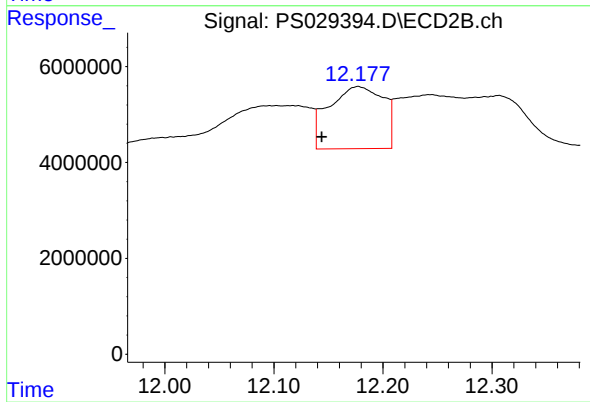

#16 DCPA

R.T.: 12.177 min
Delta R.T.: 0.033 min
Response: 45058355
Conc: 3.81 ng/ml