

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031319\
 Data File : PS003526.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2019 08:24
 Operator : EI\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 15:10:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.803	0	350199	N.D.	0.746 #
Target Compounds							
2) T	3,5-DICHL...	0.000	8.959	0	55215	N.D.	0.089 #
3) T	4-Nitroph...	0.000	9.966	0	275093	N.D.	1.224 #
5) T	DICAMBA	0.000	11.070	0	470128	N.D.	0.281 #
7) T	MCPA	0.000	11.616	0	3377435	N.D.	1.958 #
8) T	DICHLORPROP	0.000	12.178	0	685319	N.D.	1.658 #
11) T	2,4,5-TP ...	0.000	13.833	0	363196	N.D.	0.143 #
12) T	2,4,5-T	0.000	14.415	0	995304	N.D.	0.494 #
13) T	2,4-DB	0.000	15.063	0	730195	N.D.	2.860 #
14) T	DINOSEB	0.000	15.450	0	158924	N.D.	0.089 #
15) T	Picloram	16.781	16.699	17048831	409331	6.927	0.161 #
16) T	DCPA	0.000	16.653	0	1606667	N.D.	0.517 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031319\
Data File : PS003526.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2019 08:24
Operator : EI\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 15:10:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

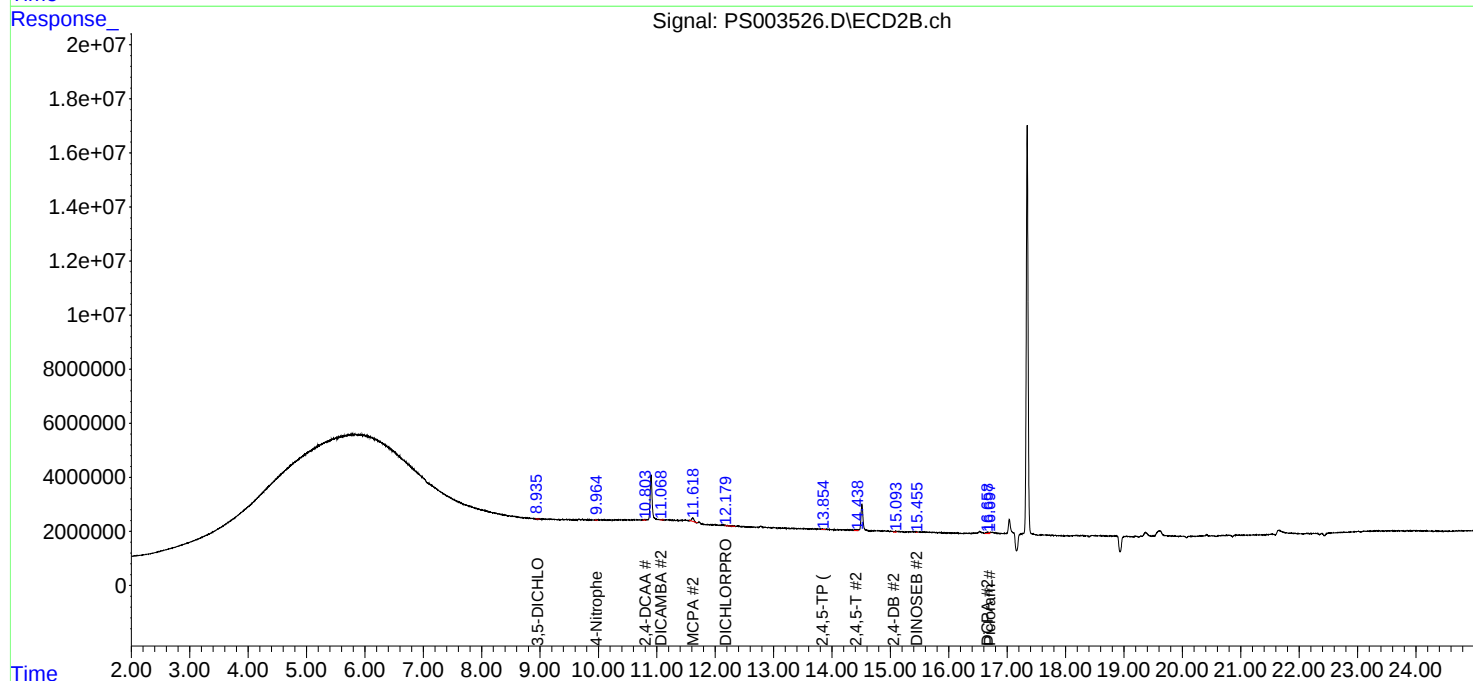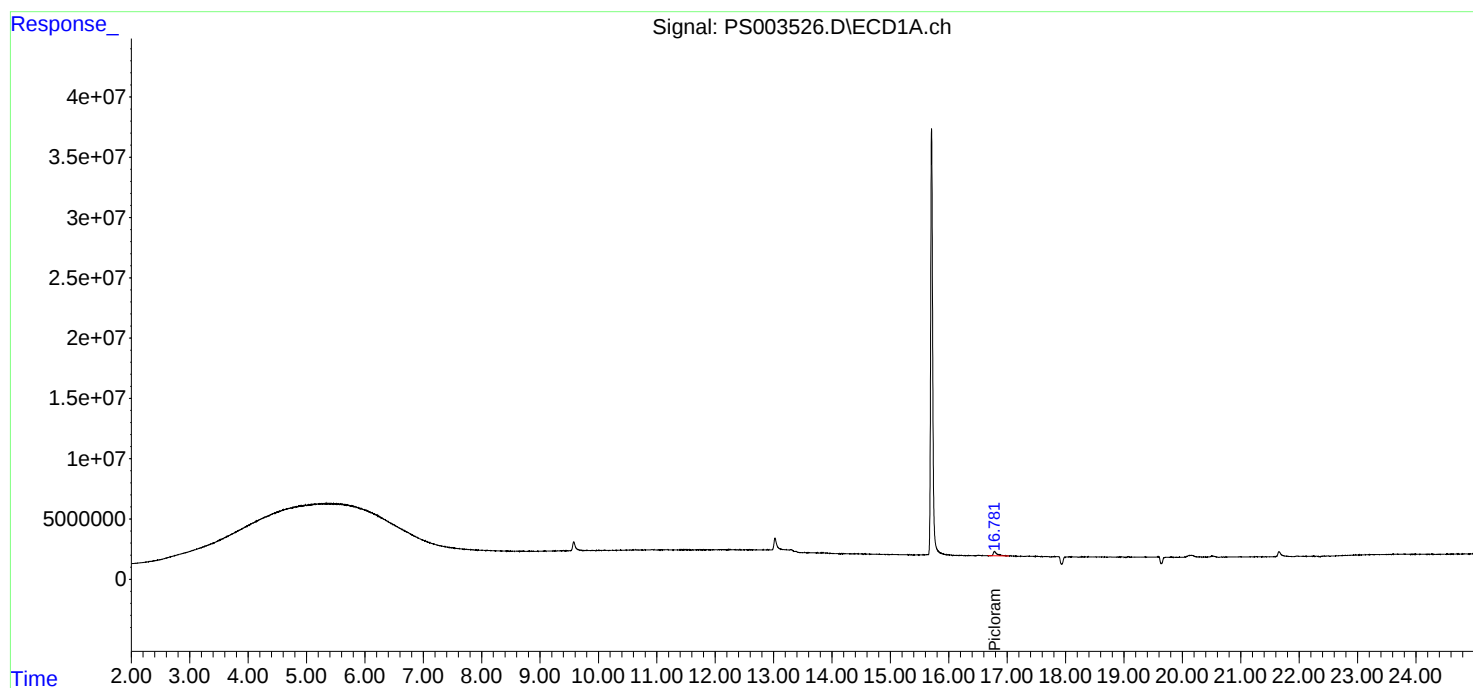


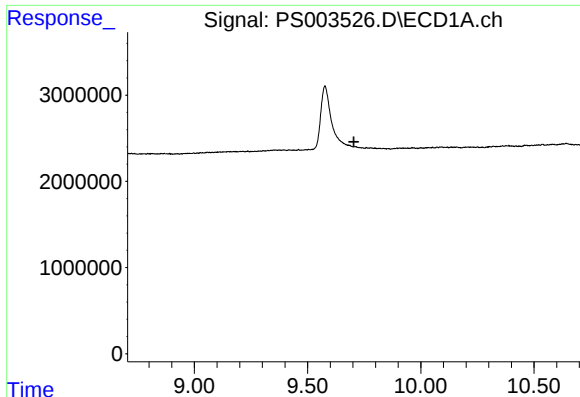

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.705 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

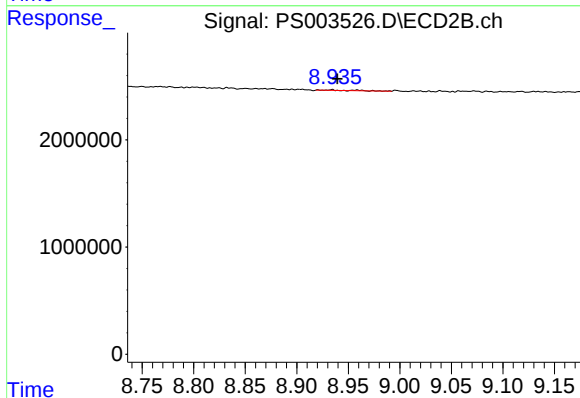


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 8.959 min
Delta R.T.: 0.019 min
Response: 55215
Conc: 0.09 ng/ml

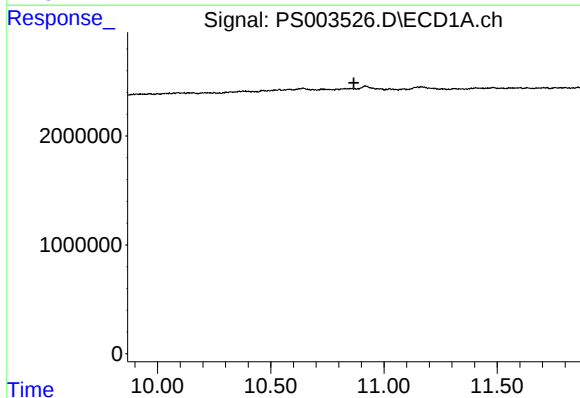


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

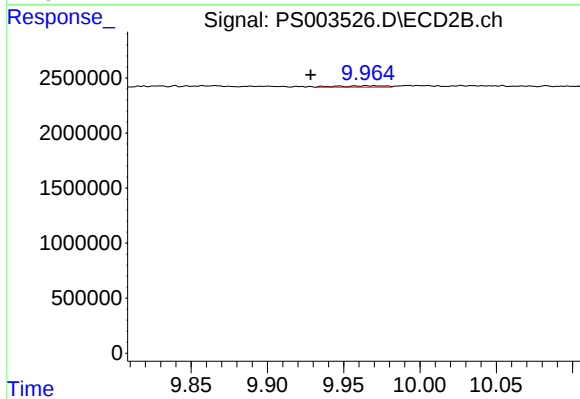

#3 4-Nitrophenol


R.T.: 9.966 min
Delta R.T.: 0.038 min
Response: 275093
Conc: 1.22 ng/ml

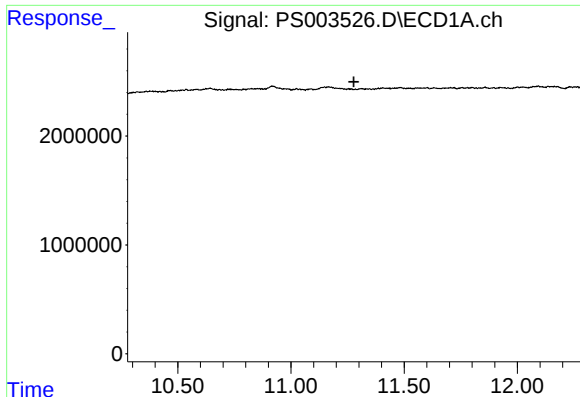

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 11.278 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

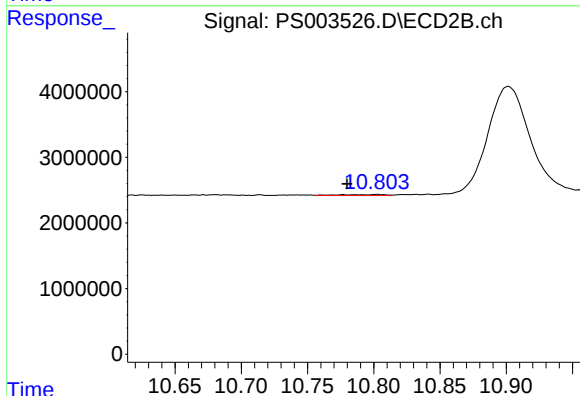


#4 2,4-DCAA

R.T.: 10.803 min
Delta R.T.: 0.023 min
Response: 350199
Conc: 0.75 ng/ml

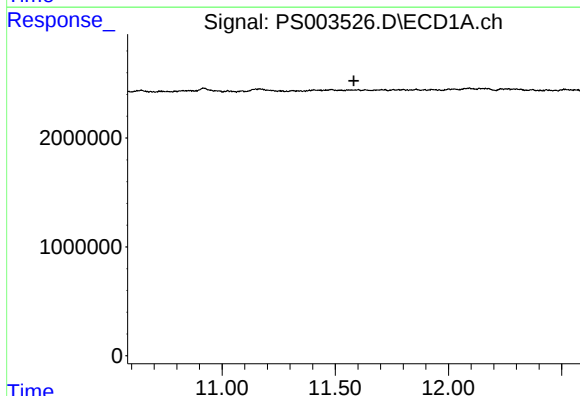


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 11.582 min
Response: 0
Conc: N.D.

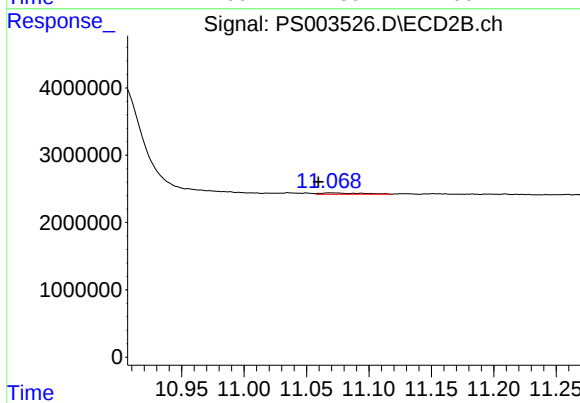

#5 DICAMBA


R.T.: 11.070 min
Delta R.T.: 0.010 min
Response: 470128
Conc: 0.28 ng/ml

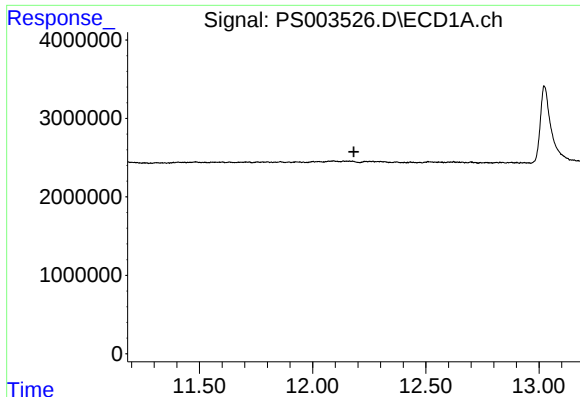

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.182 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

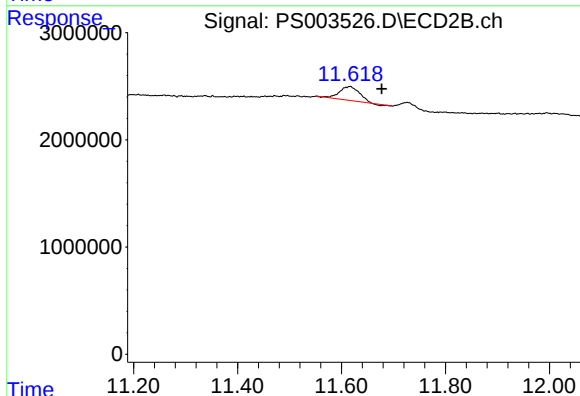


#7 MCPA

R.T.: 11.616 min
Delta R.T.: -0.062 min
Response: 3377435
Conc: 1.96 ug/ml

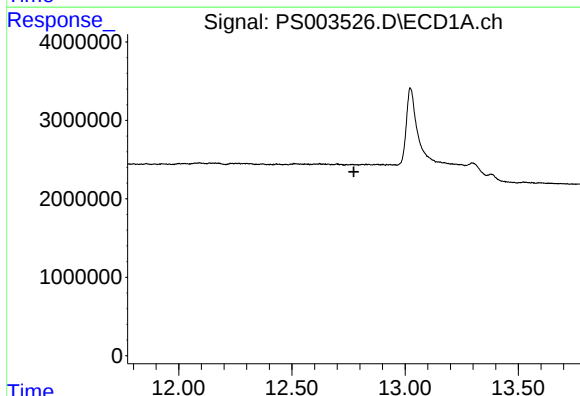


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 12.773 min
Response: 0
Conc: N.D.

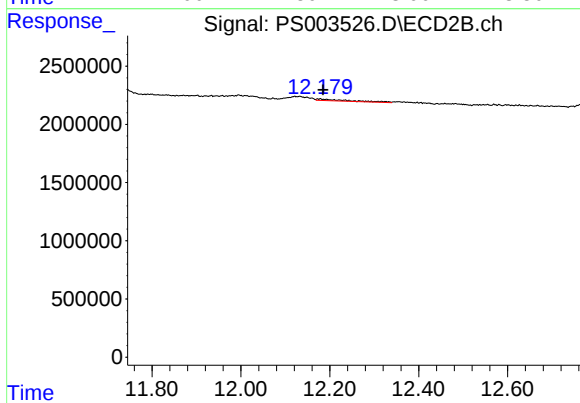

#8 DICHLORPROP


R.T.: 12.178 min
Delta R.T.: -0.008 min
Response: 685319
Conc: 1.66 ng/ml

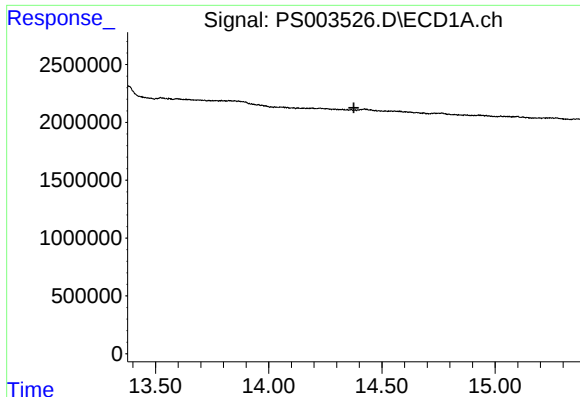

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

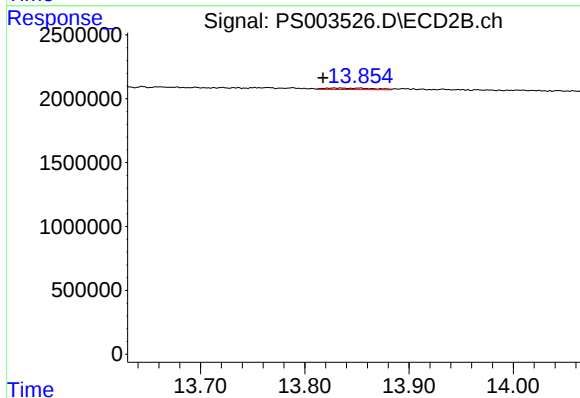


#11 2,4,5-TP (SILVEX)

R.T.: 13.833 min
Delta R.T.: 0.016 min
Response: 363196
Conc: 0.14 ng/ml

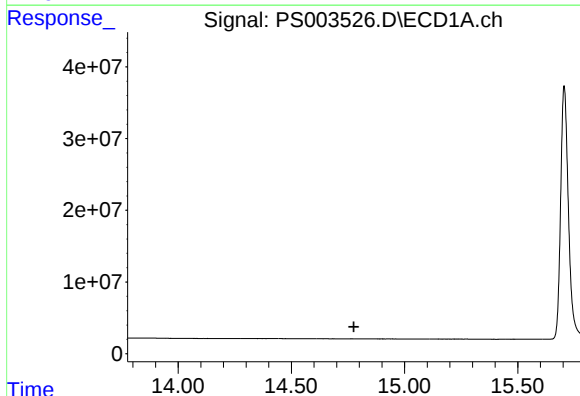


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

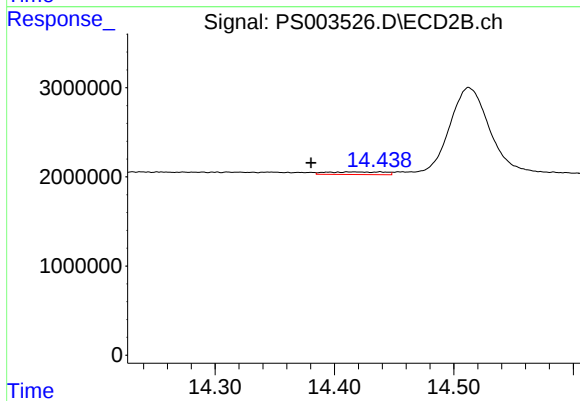

#12 2,4,5-T


R.T.: 14.415 min
Delta R.T.: 0.035 min
Response: 995304
Conc: 0.49 ng/ml

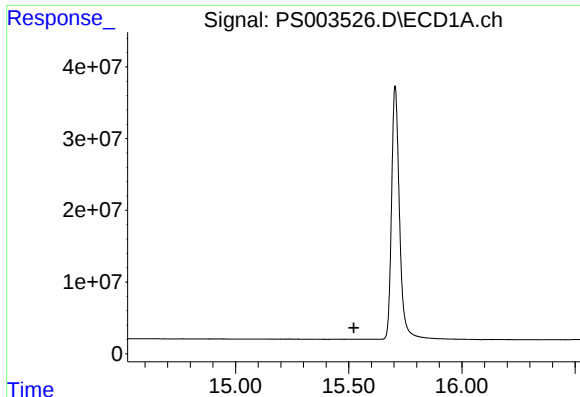

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.523 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

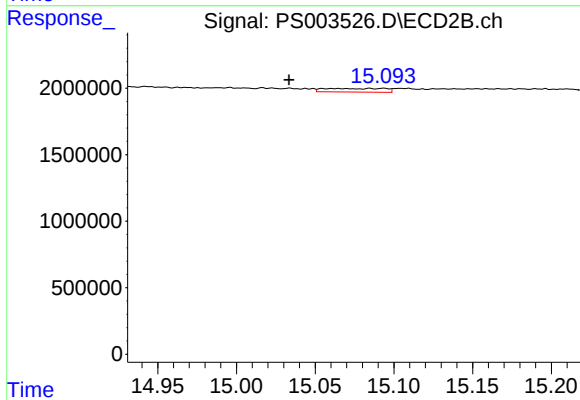


#13 2,4-DB

R.T.: 15.063 min
Delta R.T.: 0.030 min
Response: 730195
Conc: 2.86 ng/ml

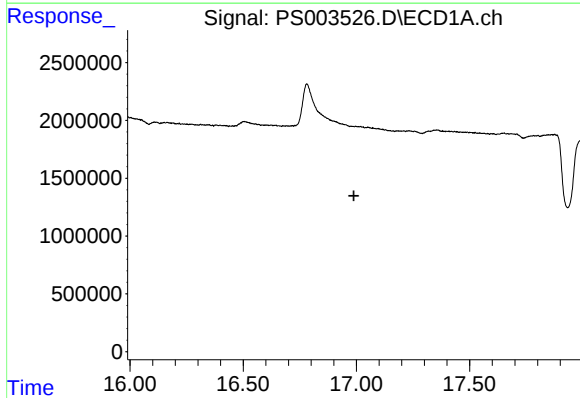


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

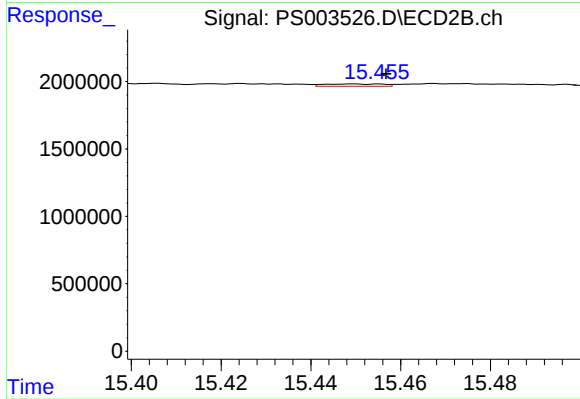

#14 DINOSEB


R.T.: 15.450 min
Delta R.T.: -0.007 min
Response: 158924
Conc: 0.09 ng/ml

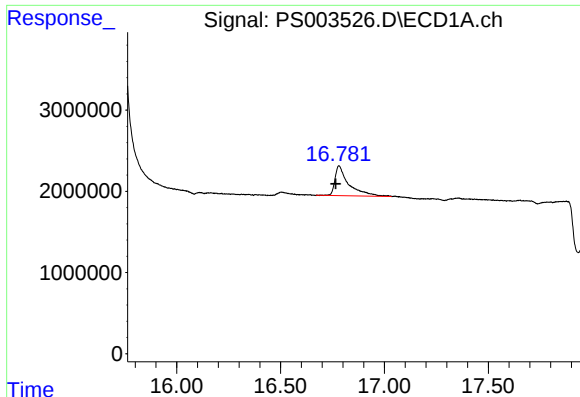

#15 Picloram


R.T.: 16.781 min
Delta R.T.: 0.016 min
Response: 17048831
Conc: 6.93 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

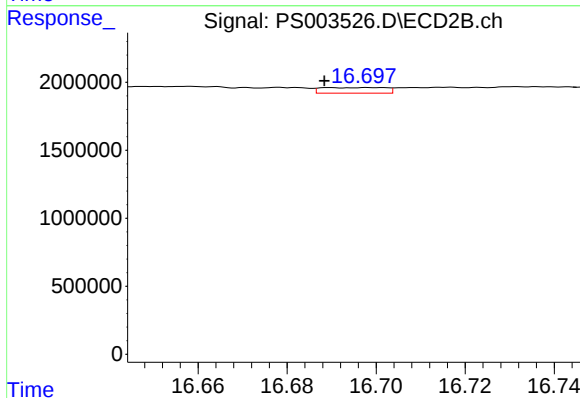


#15 Picloram

R.T.: 16.699 min
Delta R.T.: 0.011 min
Response: 409331
Conc: 0.16 ng/ml

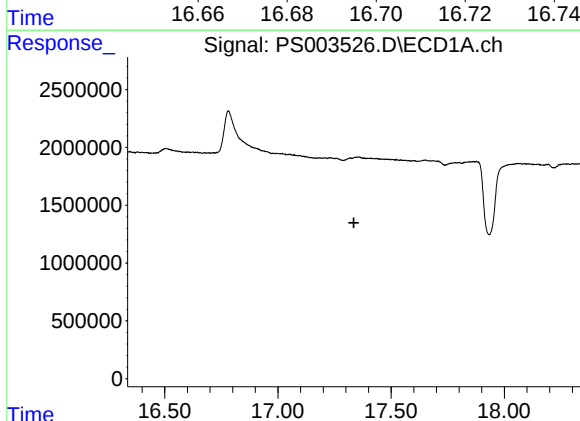

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.335 min
Response: 0
Conc: N.D.

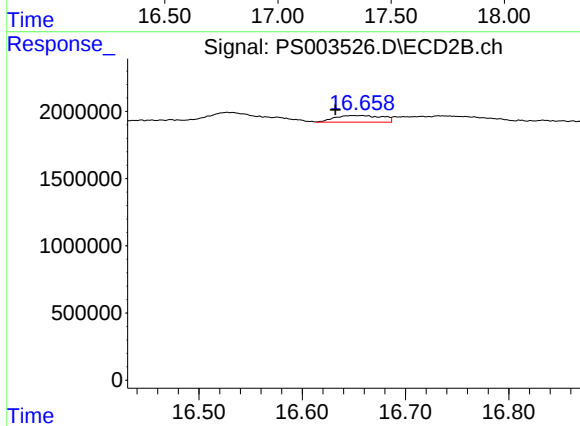

#16 DCPA

R.T.: 16.653 min
Delta R.T.: 0.021 min
Response: 1606667
Conc: 0.52 ng/ml