

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031319\
 Data File : PS003527.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2019 08:55
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 15:10:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.282	10.780	239.3E6	204.0E6	544.960	434.347
Target Compounds							
3) T	4-Nitroph...	0.000	9.960	0	459190	N.D.	2.042 #
8) T	DICHLORPROP	0.000	12.192	0	1668857	N.D.	4.038 #
10) T	Pentachlo...	0.000	13.197	0	616693	N.D.	0.094 #
11) T	2,4,5-TP ...	0.000	13.793	0	352673	N.D.	0.138 #
13) T	2,4-DB	0.000	15.043	0	1010046	N.D.	3.955 #
14) T	DINOSEB	0.000	15.459	0	1538633	N.D.	0.862 #
15) T	Picloram	16.790	16.634	11267988	1055378	4.578	0.416 #
16) T	DCPA	0.000	16.634	0	1055378	N.D.	0.339 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031319\
Data File : PS003527.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2019 08:55
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 15:10:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

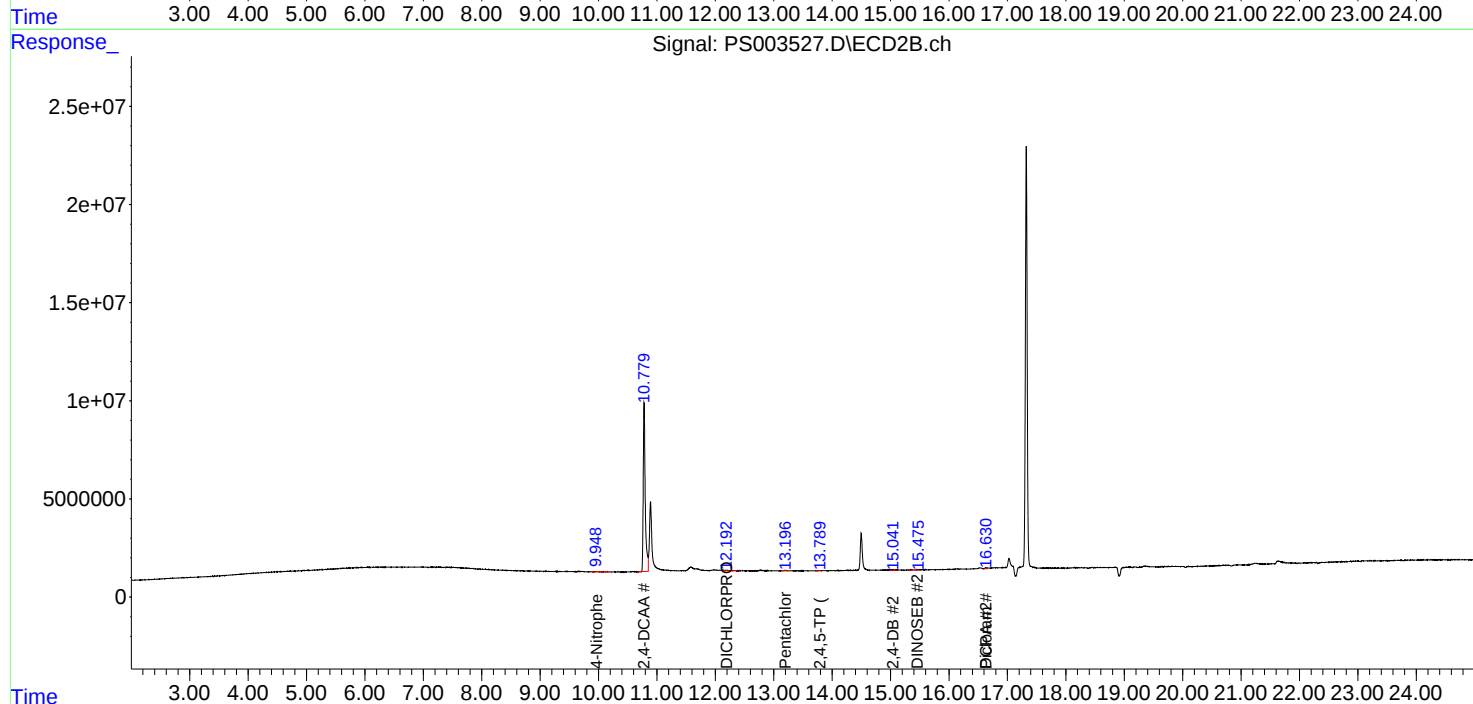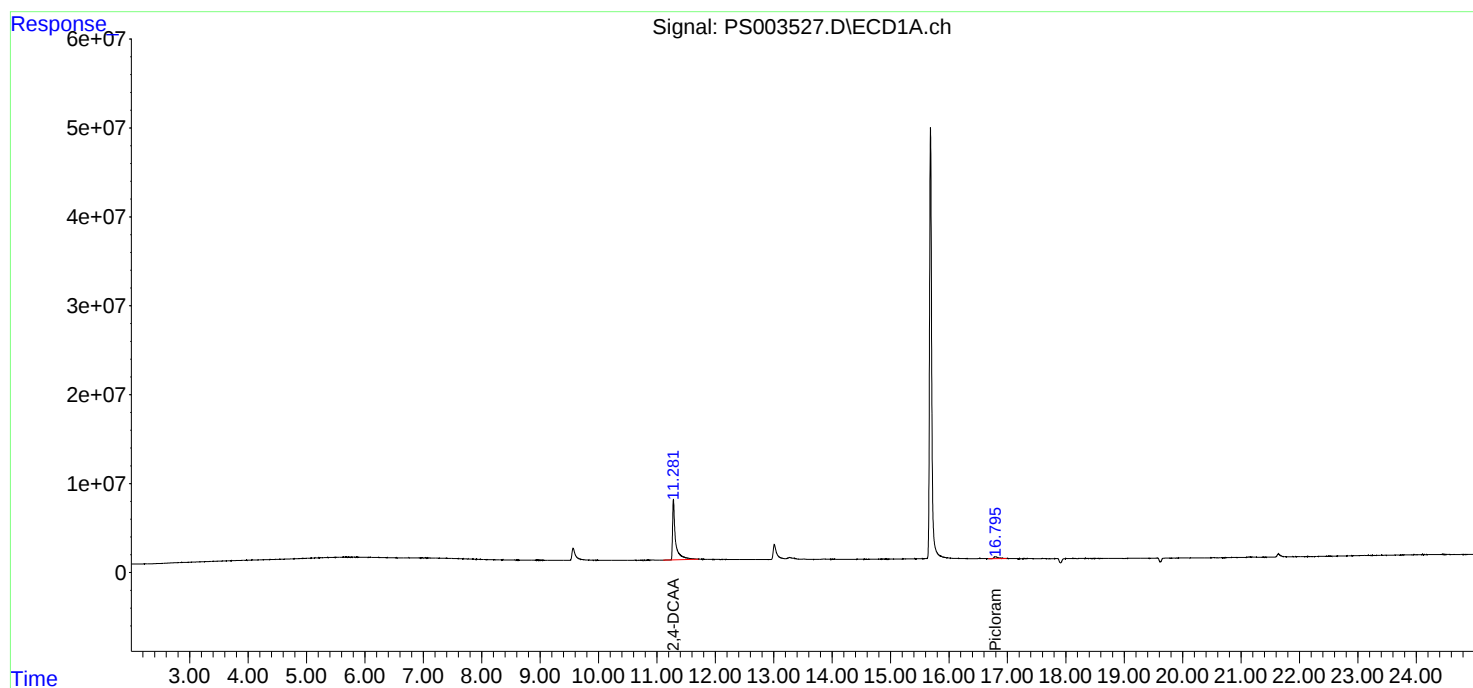


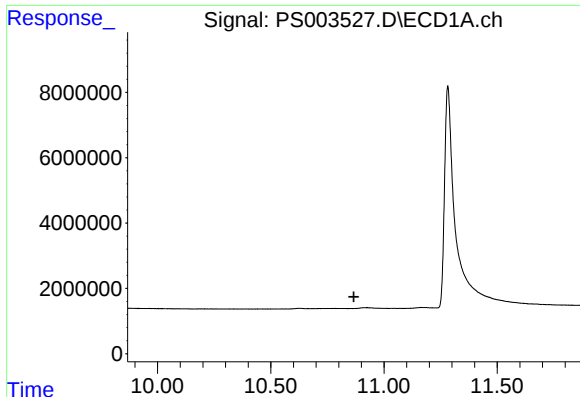

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

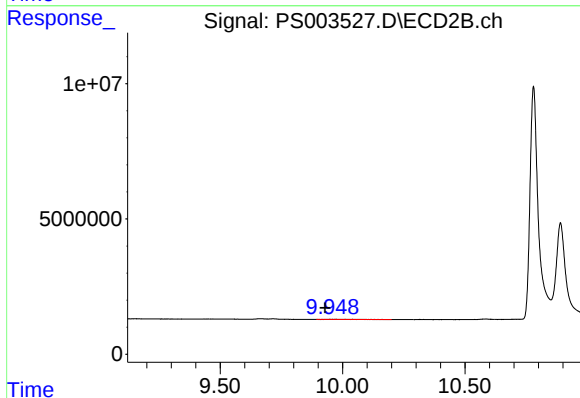


#3 4-Nitrophenol

R.T.: 9.960 min
Delta R.T.: 0.031 min
Response: 459190
Conc: 2.04 ng/ml

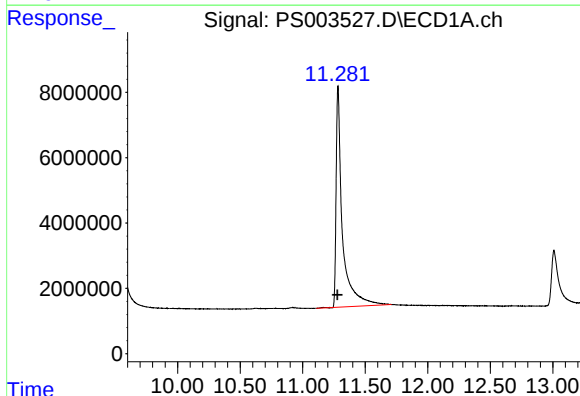


#4 2,4-DCAA

R.T.: 11.282 min
Delta R.T.: 0.004 min
Response: 239250625
Conc: 544.96 ng/ml

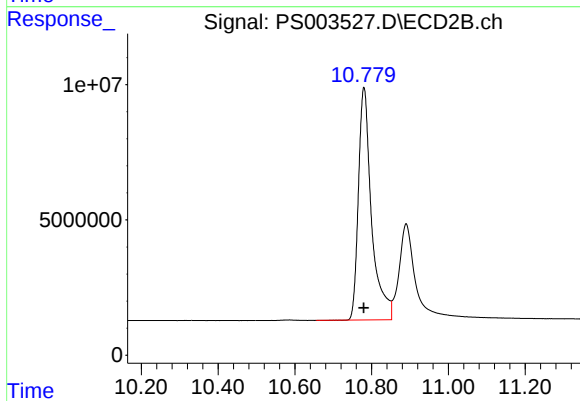

#4 2,4-DCAA


R.T.: 10.780 min
Delta R.T.: 0.000 min
Response: 203956074
Conc: 434.35 ng/ml

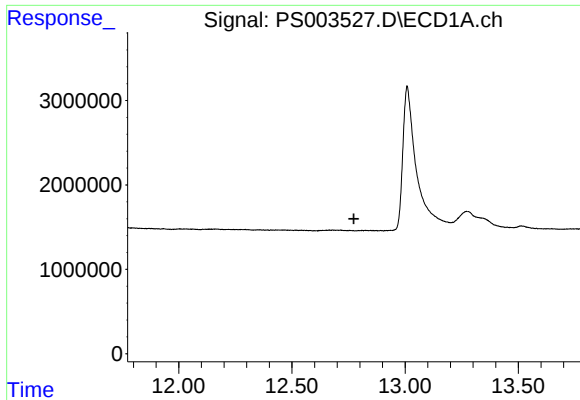

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 12.773 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

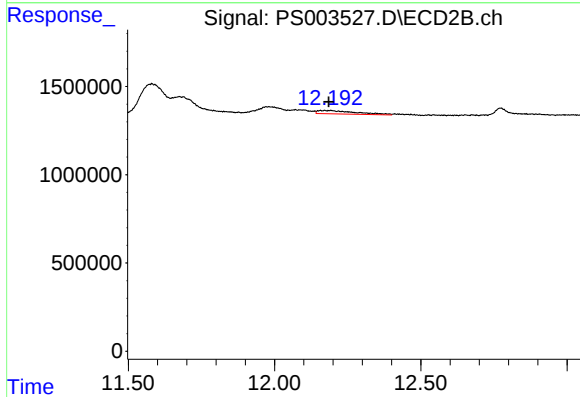


#8 DICHLORPROP

R.T.: 12.192 min
Delta R.T.: 0.007 min
Response: 1668857
Conc: 4.04 ng/ml

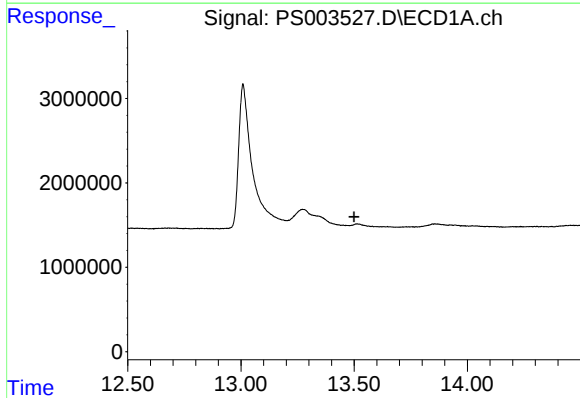


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.499 min
Response: 0
Conc: N.D.

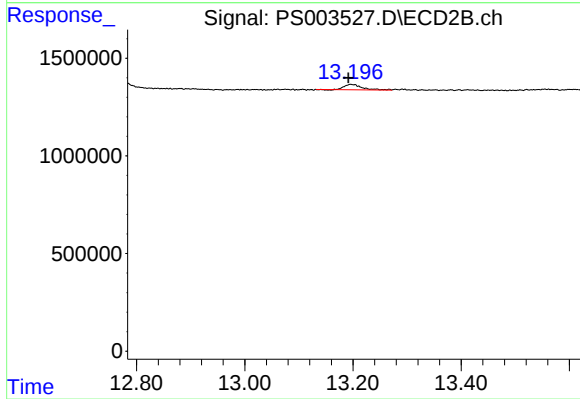

#10 Pentachlorophenol


R.T.: 13.197 min
Delta R.T.: 0.006 min
Response: 616693
Conc: 0.09 ng/ml

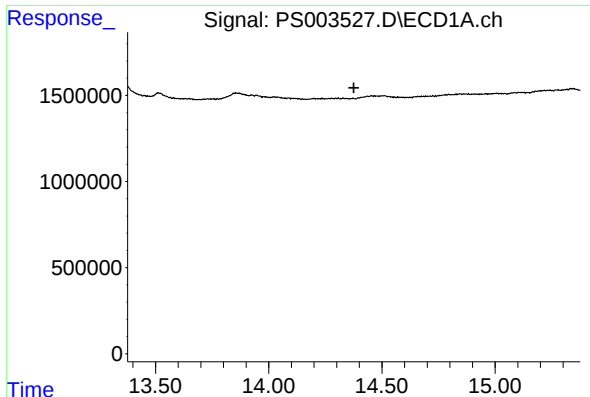

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

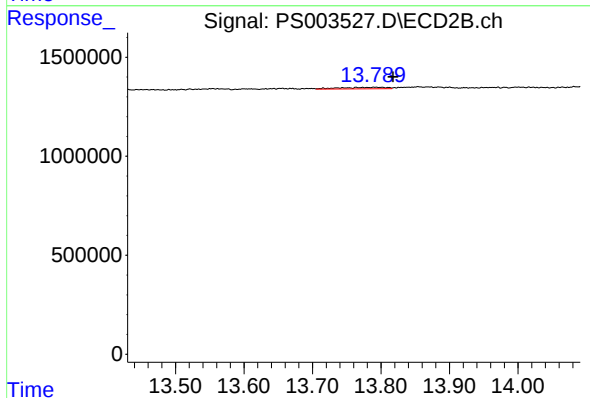


#11 2,4,5-TP (SILVEX)

R.T.: 13.793 min
Delta R.T.: -0.024 min
Response: 352673
Conc: 0.14 ng/ml

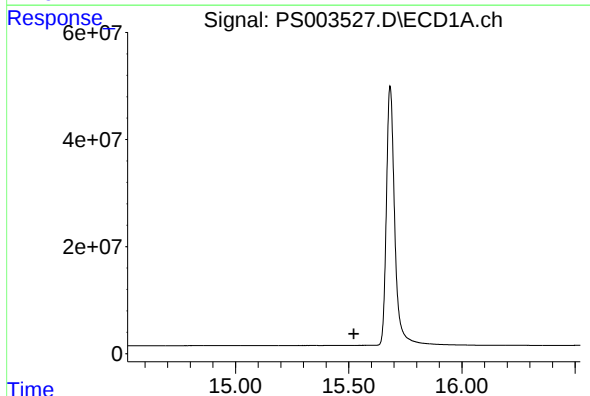


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.523 min
Response: 0
Conc: N.D.

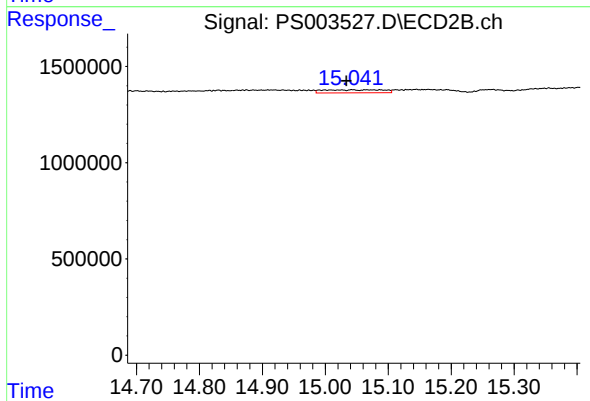

#13 2,4-DB


R.T.: 15.043 min
Delta R.T.: 0.010 min
Response: 1010046
Conc: 3.96 ng/ml

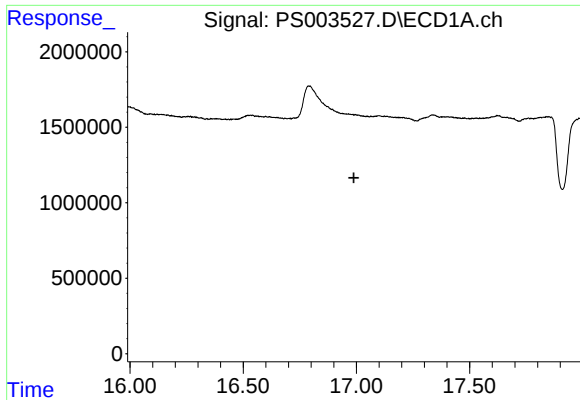

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

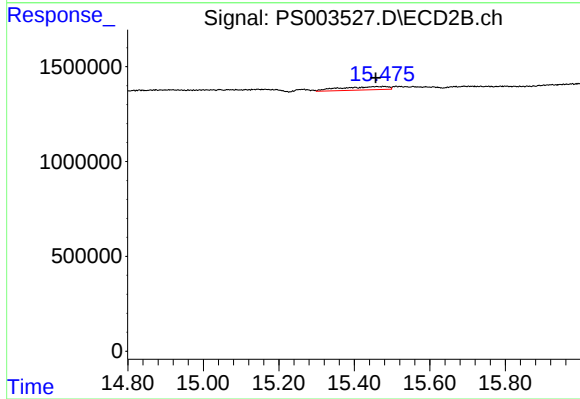


#14 DINOSEB

R.T.: 15.459 min
Delta R.T.: 0.002 min
Response: 1538633
Conc: 0.86 ng/ml

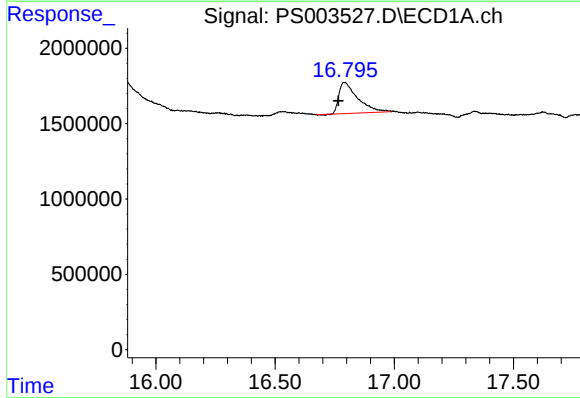


#15 Picloram

R.T.: 16.790 min
Delta R.T.: 0.025 min
Response: 11267988
Conc: 4.58 ng/ml

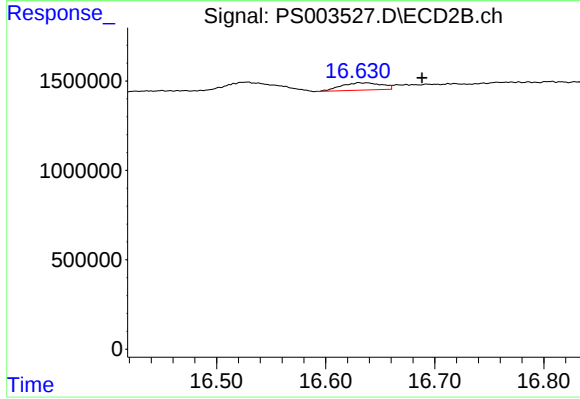

#15 Picloram


R.T.: 16.634 min
Delta R.T.: -0.054 min
Response: 1055378
Conc: 0.42 ng/ml

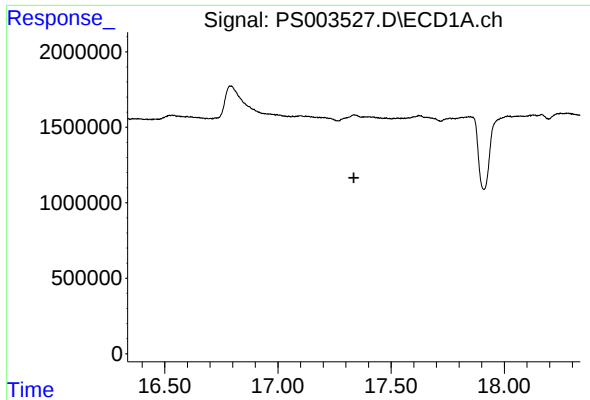

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.335 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

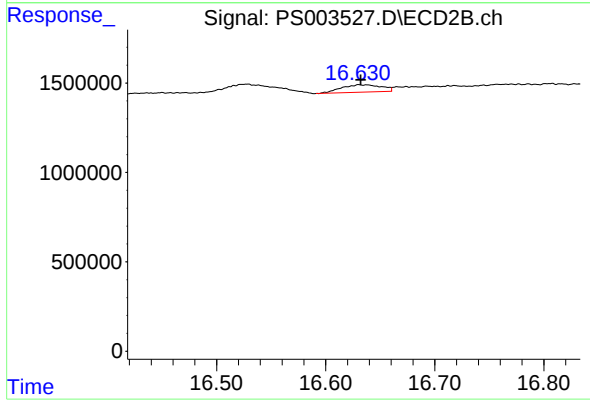

#16 DCPA

R.T.: 16.634 min
Delta R.T.: 0.003 min
Response: 1055378
Conc: 0.34 ng/ml