

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031319\
 Data File : PS003530.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2019 14:46
 Operator : EI\SJ
 Sample : K1808-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 FK-BPM-01-AA0-BB0-AA0A-BB0A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 01:06:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.299	10.804	222.2E6	174.9E6	506.233	372.422 #
Target Compounds							
1) T	Dalapon	2.820	2.309	44796597	16888290	68.924	26.672 #
2) T	3,5-DICHL...	0.000	8.994	0	1724209	N.D.	2.792 #
5) T	DICAMBA	11.626	11.041	17826160	4005985	10.113	2.398 #
6) T	MCP	11.973	11.288	1441980	1442665	1.098	1.222
7) T	MCPA	0.000	11.658	0	4794234	N.D.	2.779 #
8) T	DICHLORPROP	0.000	12.214	0	6306366	N.D.	15.261 #
9) T	2,4-D	13.157	12.667	13819974	438347	29.796	0.835 #
10) T	Pentachlo...	13.525	0.000	9282644	0	1.314	N.D. #
11) T	2,4,5-TP ...	0.000	13.816	0	3123591	N.D.	1.227 #
12) T	2,4,5-T	14.763	14.403	10570369	21626364	4.001	10.723 #
13) T	2,4-DB	15.569	15.059	147.7E6	144.4E6	623.824	565.502
14) T	DINOSEB	0.000	15.468	0	19518711	N.D.	10.936 #
15) T	Picloram	16.781	16.725	32650535	43404909	13.266	17.101 #
16) T	DCPA	17.320	16.579	26676594	27388779	8.096	8.806



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031319\
Data File : PS003530.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2019 14:46
Operator : EI\SJ
Sample : K1808-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-AA0-BB0-AA0A-BB0A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 01:06:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

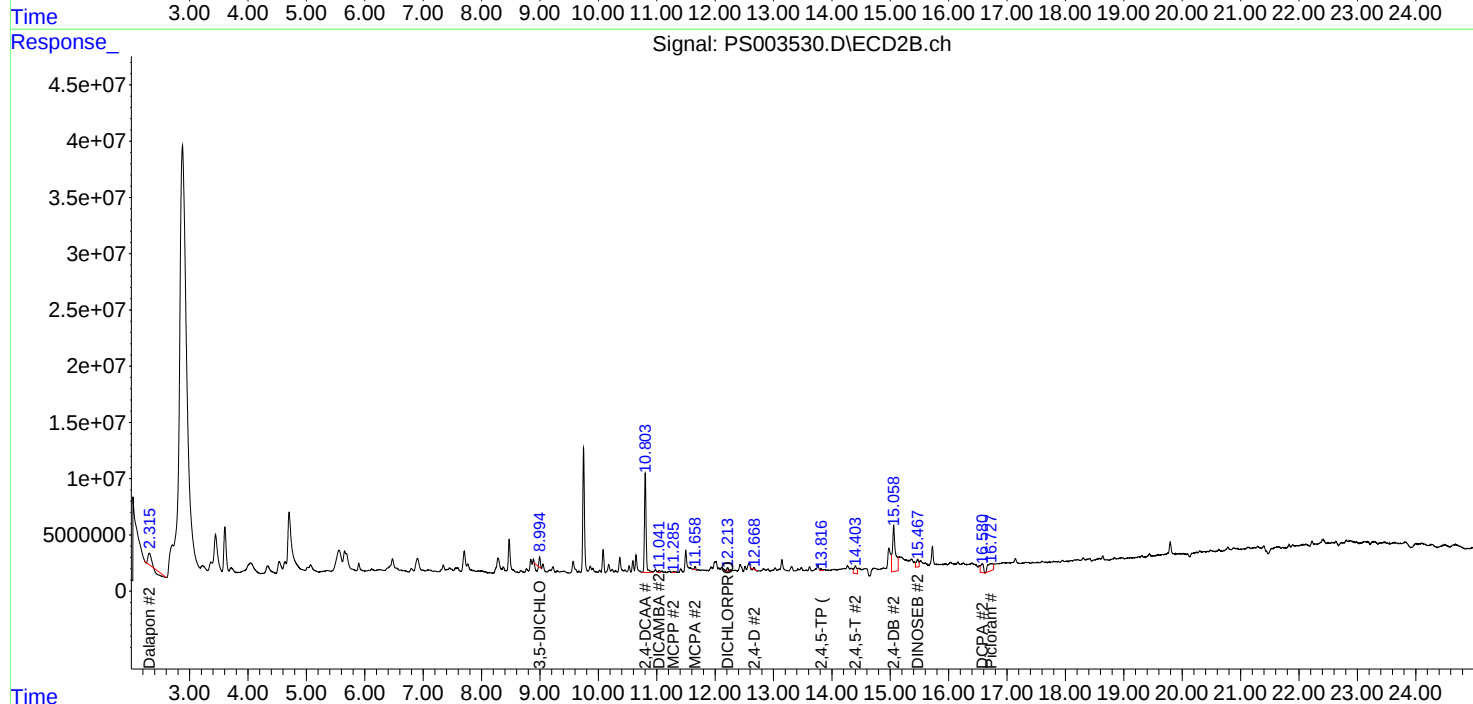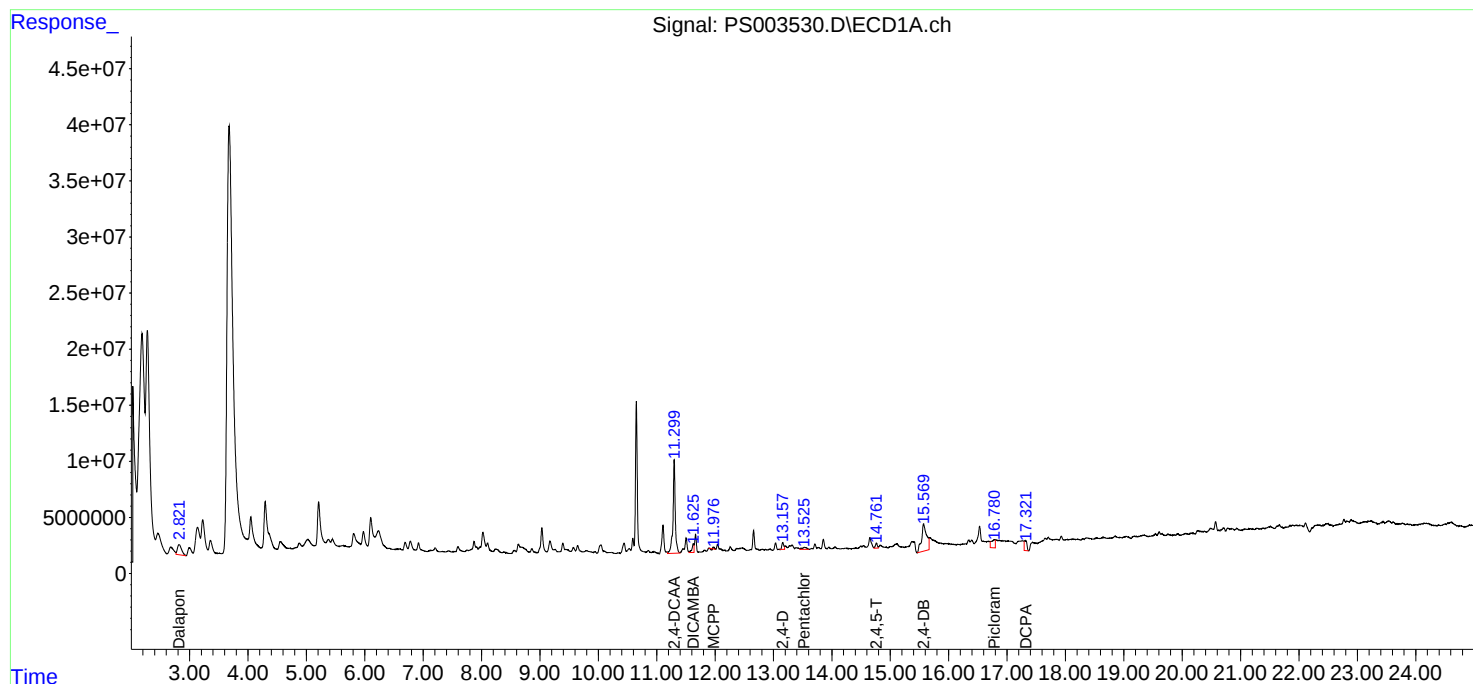


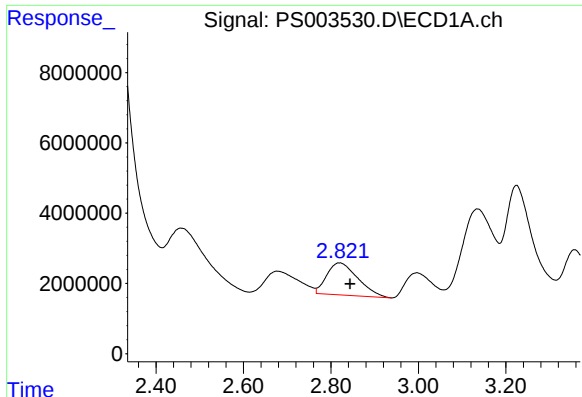

#1 Dalapon


R.T.: 2.820 min
Delta R.T.: -0.024 min
Response: 44796597
Conc: 68.92 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-AA0-BB0-AA0A-BB0A

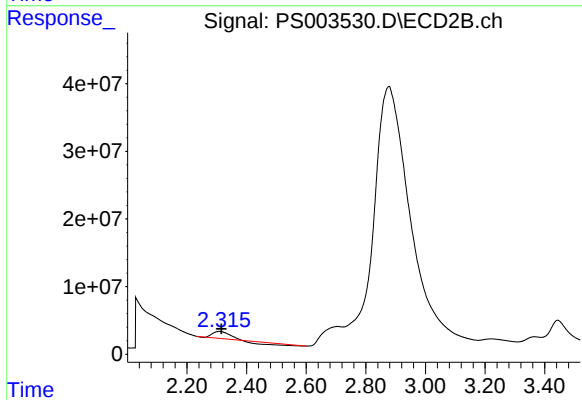


#1 Dalapon

R.T.: 2.309 min
Delta R.T.: -0.007 min
Response: 16888290
Conc: 26.67 ng/ml

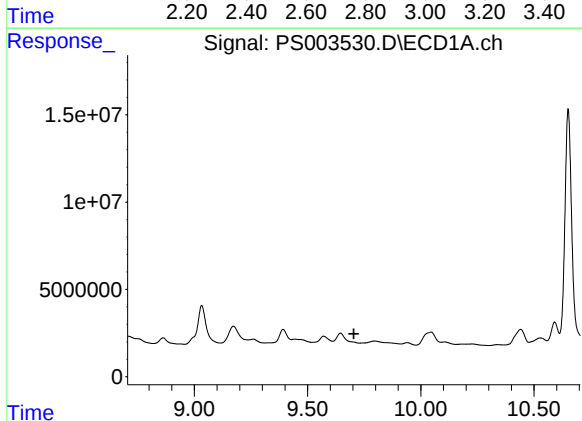


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.705 min
Response: 0
Conc: N.D.

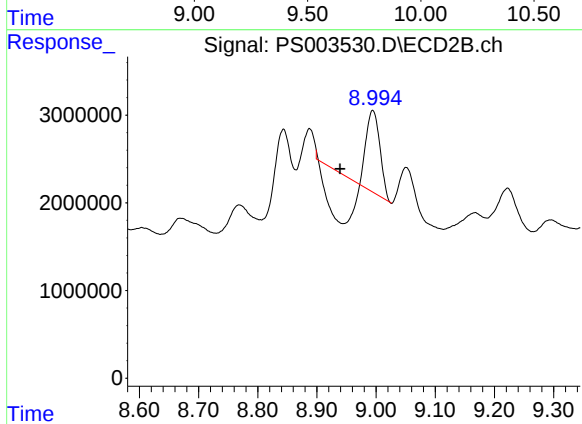

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.994 min
Delta R.T.: 0.055 min
Response: 1724209
Conc: 2.79 ng/ml

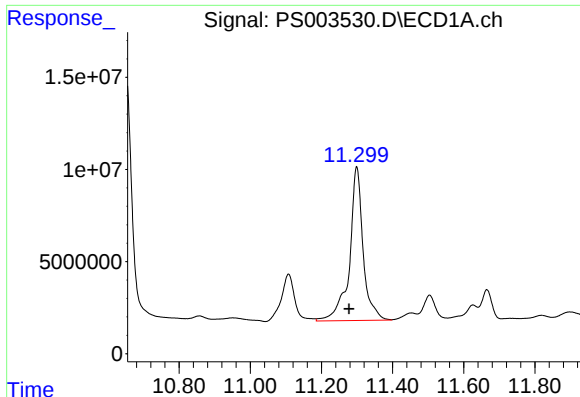

#4 2,4-DCAA


R.T.: 11.299 min
Delta R.T.: 0.022 min
Response: 222248549
Conc: 506.23 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-AA0-BB0-AA0A-BB0A

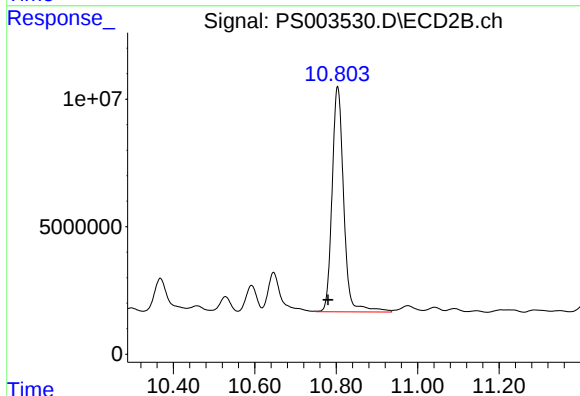


#4 2,4-DCAA

R.T.: 10.804 min
Delta R.T.: 0.024 min
Response: 174878047
Conc: 372.42 ng/ml

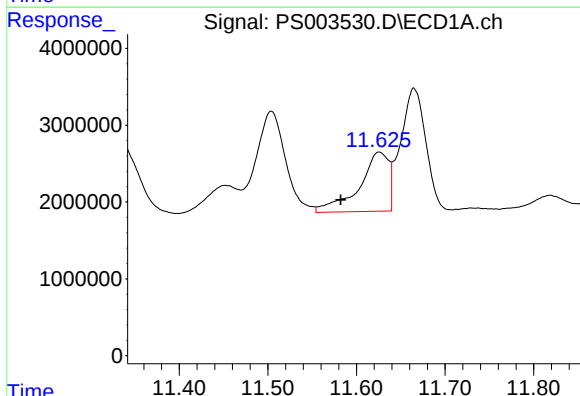


#5 DICAMBA

R.T.: 11.626 min
Delta R.T.: 0.044 min
Response: 17826160
Conc: 10.11 ng/ml

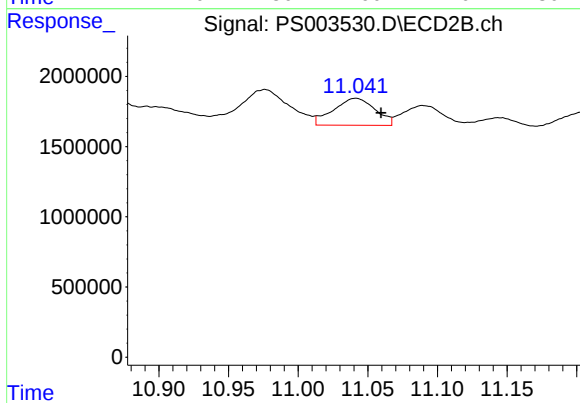

#5 DICAMBA


R.T.: 11.041 min
Delta R.T.: -0.018 min
Response: 4005985
Conc: 2.40 ng/ml

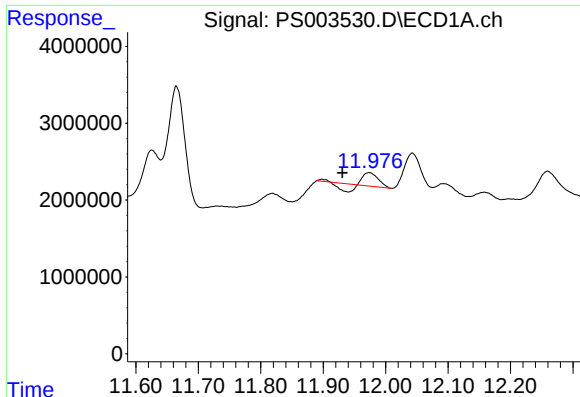

#6 MCPP


R.T.: 11.973 min
Delta R.T.: 0.043 min
Response: 1441980
Conc: 1.10 ug/ml

Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-AA0-BB0-AA0A-BB0A

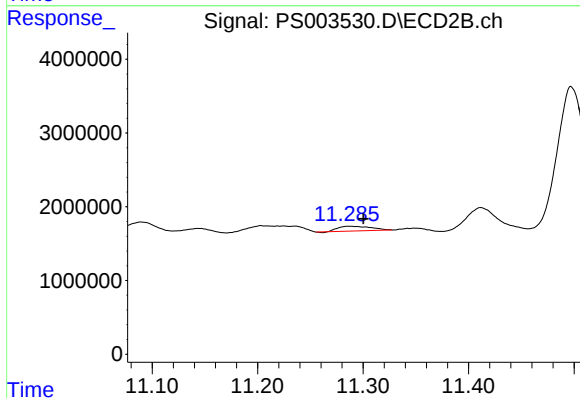


#6 MCPP

R.T.: 11.288 min
Delta R.T.: -0.013 min
Response: 1442665
Conc: 1.22 ug/ml

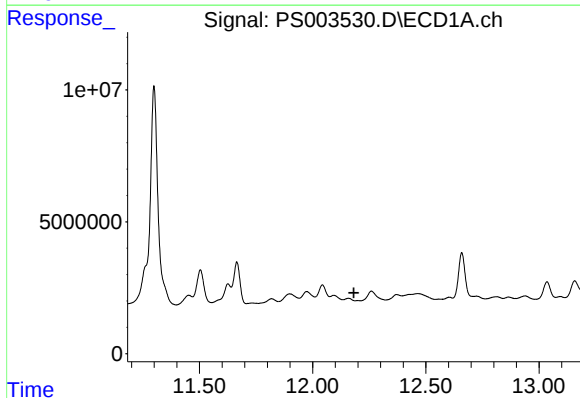


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.182 min
Response: 0
Conc: N.D.

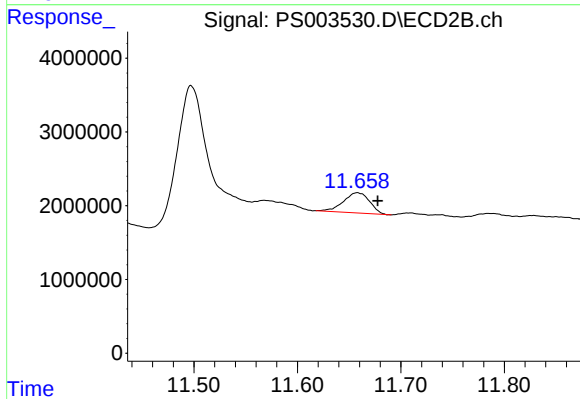

#7 MCPA


R.T.: 11.658 min
Delta R.T.: -0.019 min
Response: 4794234
Conc: 2.78 ug/ml

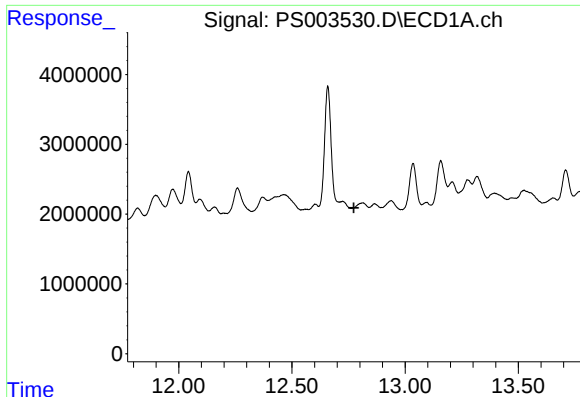

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.773 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-AA0-BB0-AA0A-BB0A

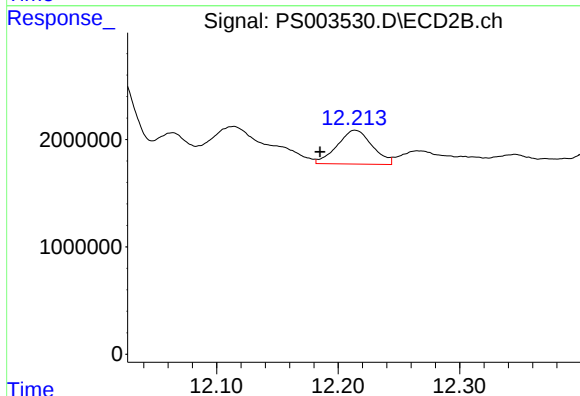


#8 DICHLORPROP

R.T.: 12.214 min
Delta R.T.: 0.029 min
Response: 6306366
Conc: 15.26 ng/ml

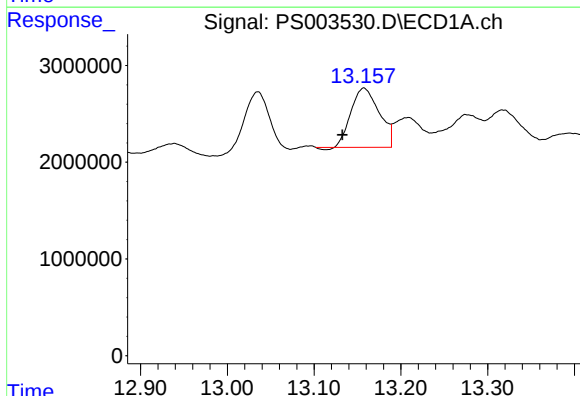


#9 2,4-D

R.T.: 13.157 min
Delta R.T.: 0.025 min
Response: 13819974
Conc: 29.80 ng/ml

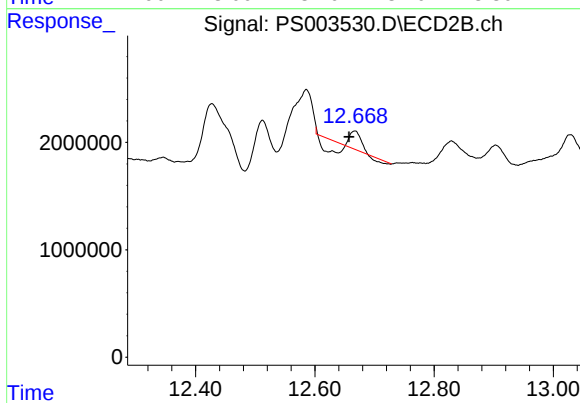

#9 2,4-D


R.T.: 12.667 min
Delta R.T.: 0.010 min
Response: 438347
Conc: 0.84 ng/ml

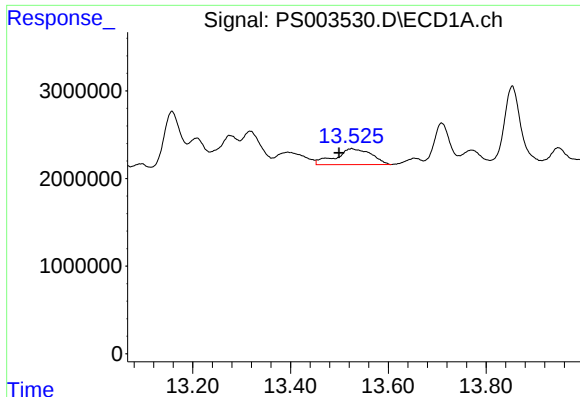

#10 Pentachlorophenol


R.T.: 13.525 min
Delta R.T.: 0.026 min
Response: 9282644
Conc: 1.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-AA0-BB0-AA0A-BB0A

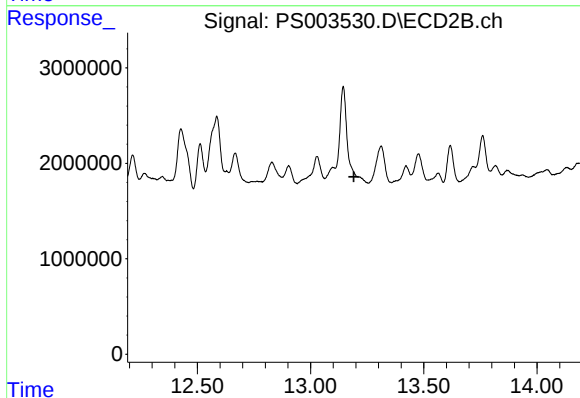


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.192 min
Response: 0
Conc: N.D.

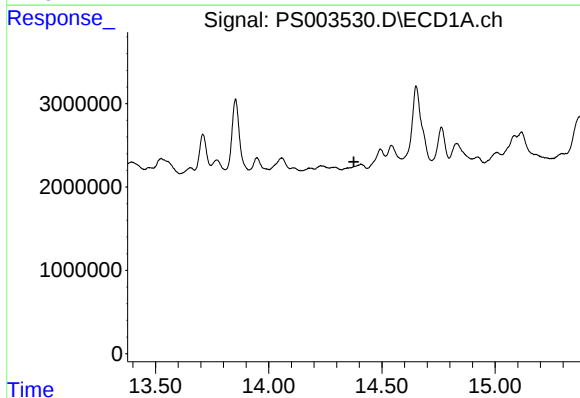


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.376 min
Response: 0
Conc: N.D.

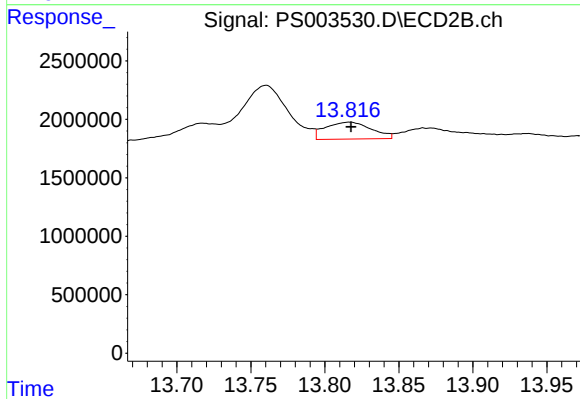

#11 2,4,5-TP (SILVEX)


R.T.: 13.816 min
Delta R.T.: -0.001 min
Response: 3123591
Conc: 1.23 ng/ml

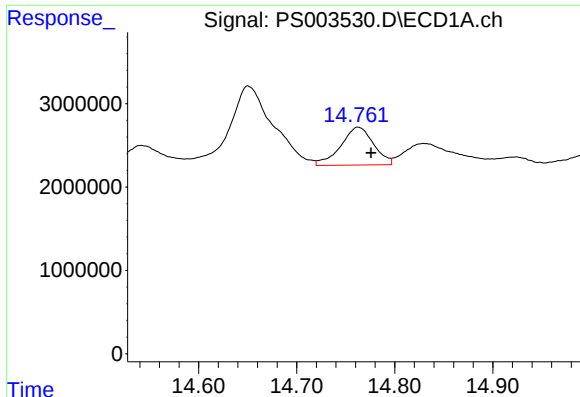

#12 2,4,5-T


R.T.: 14.763 min
Delta R.T.: -0.013 min
Response: 10570369
Conc: 4.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-AA0-BB0-AA0A-BB0A

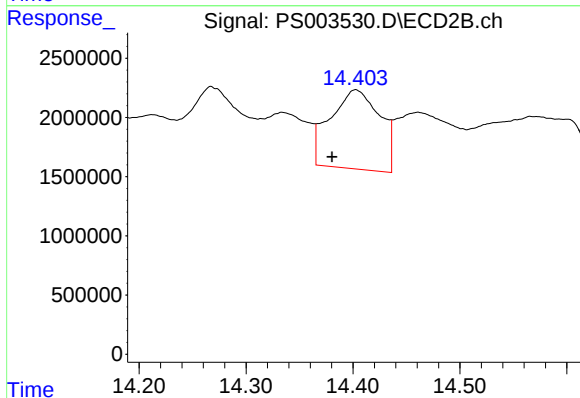


#12 2,4,5-T

R.T.: 14.403 min
Delta R.T.: 0.022 min
Response: 21626364
Conc: 10.72 ng/ml

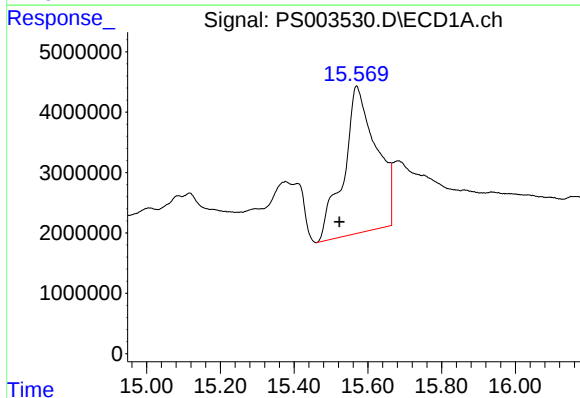


#13 2,4-DB

R.T.: 15.569 min
Delta R.T.: 0.046 min
Response: 147718864
Conc: 623.82 ng/ml

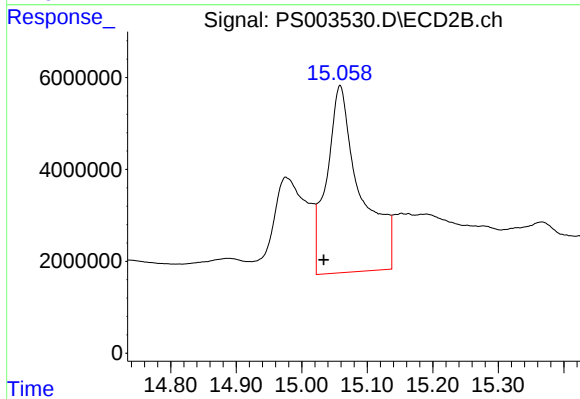

#13 2,4-DB


R.T.: 15.059 min
Delta R.T.: 0.025 min
Response: 144404911
Conc: 565.50 ng/ml

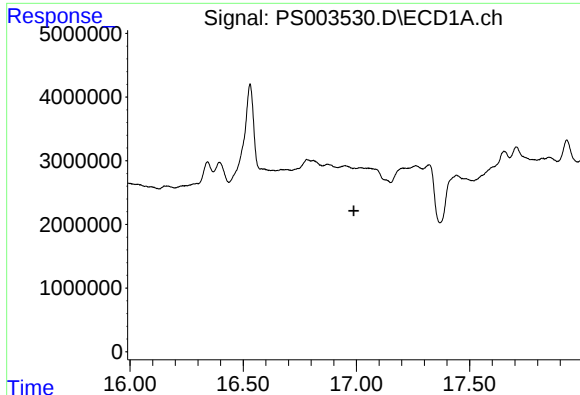

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-AA0-BB0-AA0A-BB0A

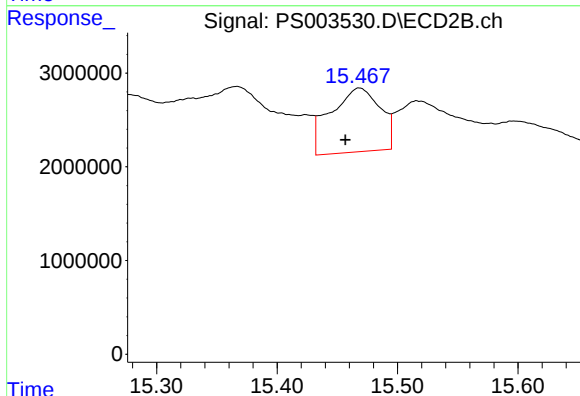


#14 DINOSEB

R.T.: 15.468 min
Delta R.T.: 0.012 min
Response: 19518711
Conc: 10.94 ng/ml

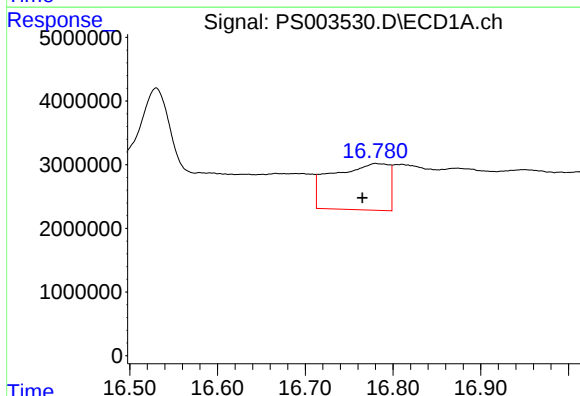


#15 Picloram

R.T.: 16.781 min
Delta R.T.: 0.016 min
Response: 32650535
Conc: 13.27 ng/ml

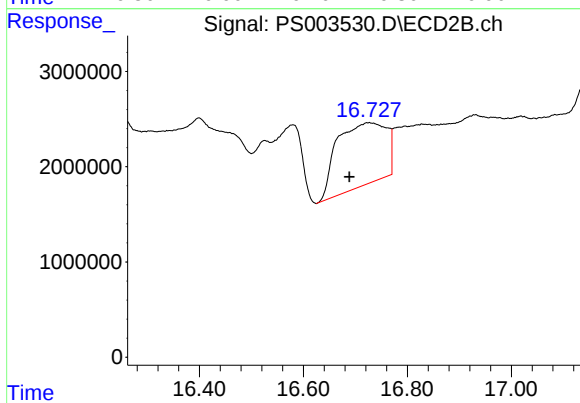

#15 Picloram


R.T.: 16.725 min
Delta R.T.: 0.037 min
Response: 43404909
Conc: 17.10 ng/ml

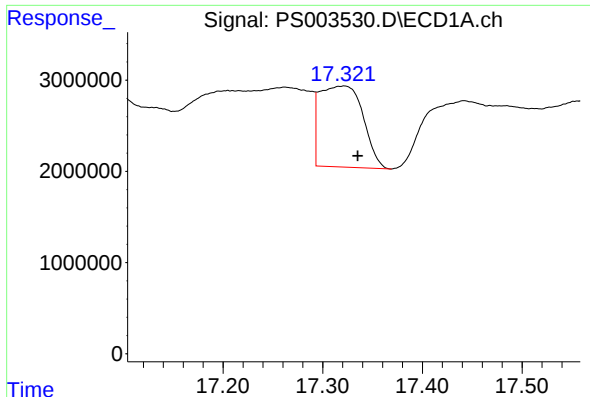

#16 DCPA

R.T.: 17.320 min
Delta R.T.: -0.015 min
Response: 26676594
Conc: 8.10 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-AA0-BB0-AA0A-BB0A

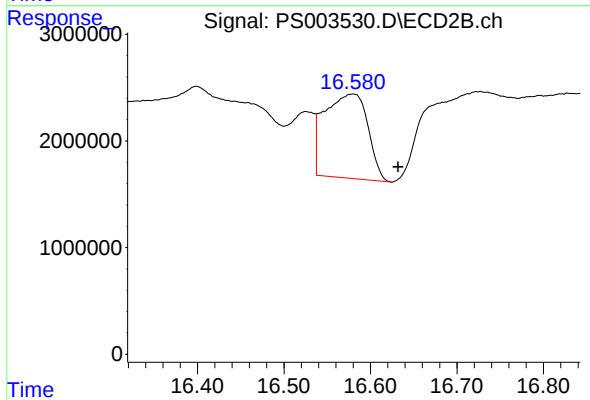

#16 DCPA

R.T.: 16.579 min
Delta R.T.: -0.053 min
Response: 27388779
Conc: 8.81 ng/ml