

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031319\
 Data File : PS003536.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2019 18:49
 Operator : EI\SJ
 Sample : PB117886TB
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB117886TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 01:08:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.293	10.795	233.4E6	235.6E6	531.594	501.690
Target Compounds							
1) T	Dalapon	2.809	2.296	21141089	18916144	32.528	29.875
2) T	3,5-DICHL...	0.000	8.961	0	5632422	N.D.	9.122 #
5) T	DICAMBA	0.000	11.036	0	4960481	N.D.	2.969 #
6) T	MCP	0.000	11.281	0	273525	N.D.	0.232 #
9) T	2,4-D	13.148	12.656	6003264	959806	12.943	1.829 #
11) T	2,4,5-TP ...	0.000	13.803	0	1262904	N.D.	0.496 #
12) T	2,4,5-T	0.000	14.395	0	8975126	N.D.	4.450 #
13) T	2,4-DB	15.486	15.018	-1755120	3755998	N.D.	14.709
14) T	DINOSEB	0.000	15.433	0	1925123	N.D.	1.079 #
15) T	Picloram	16.767	16.740	5070415	24674119	2.060	9.721 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031319\
Data File : PS003536.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2019 18:49
Operator : EI\SJ
Sample : PB117886TB
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB117886TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 01:08:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

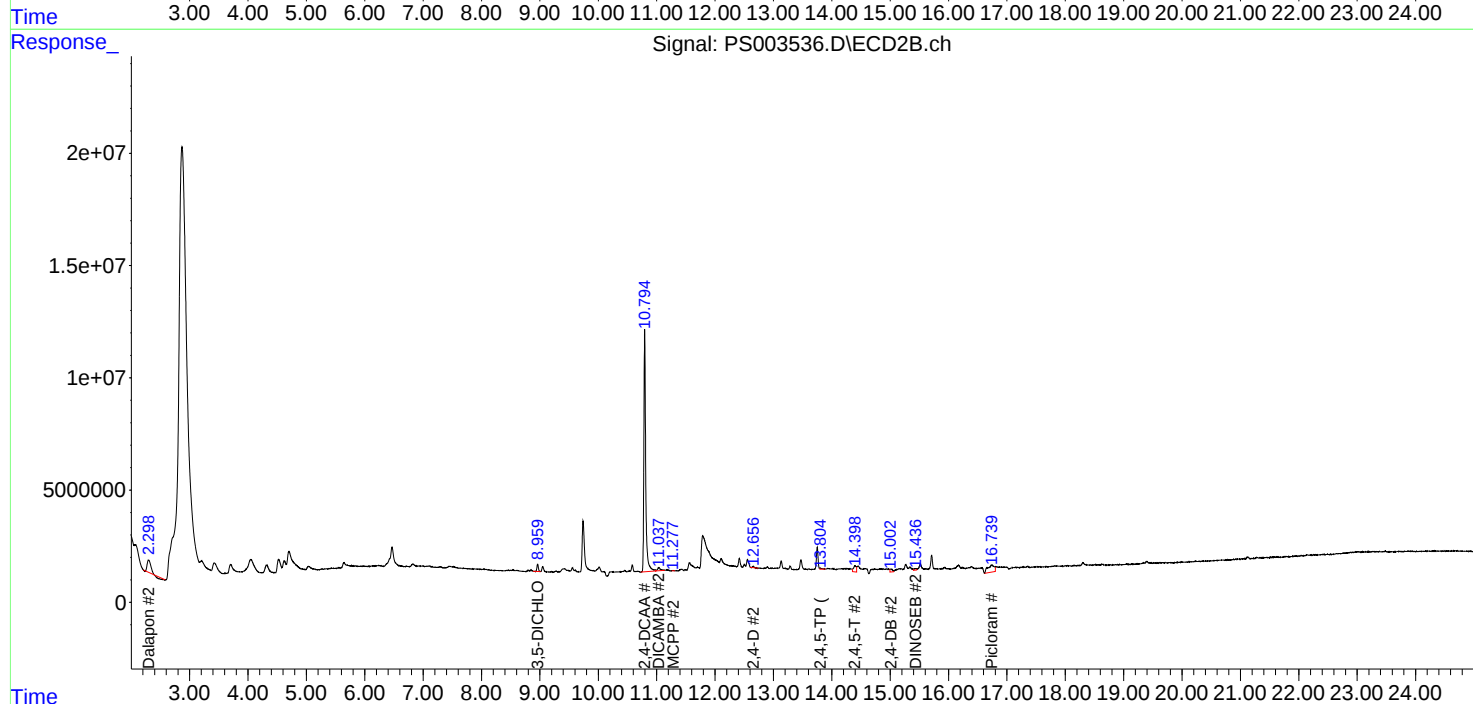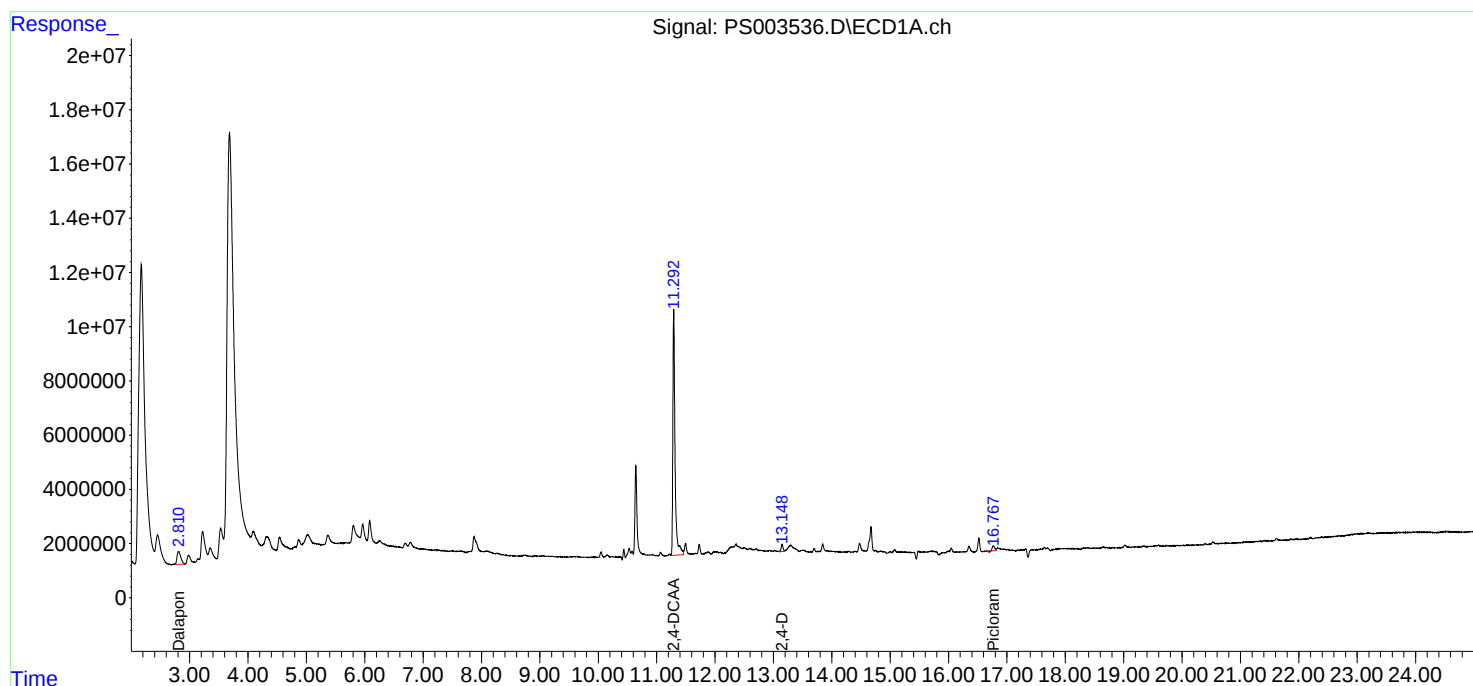


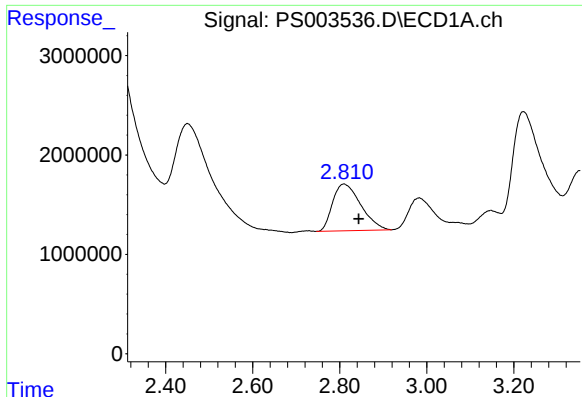

#1 Dalapon


R.T.: 2.809 min
Delta R.T.: -0.035 min
Response: 21141089
Conc: 32.53 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB117886TB

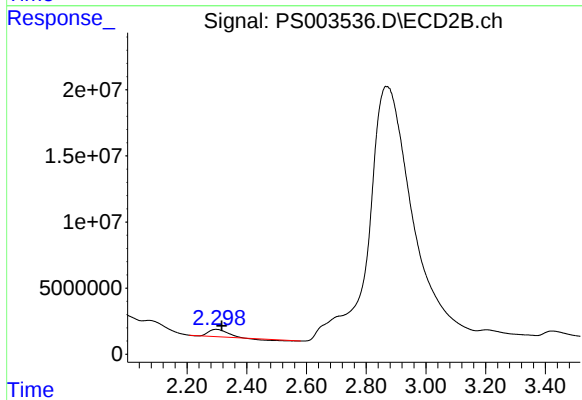


#1 Dalapon

R.T.: 2.296 min
Delta R.T.: -0.020 min
Response: 18916144
Conc: 29.87 ng/ml

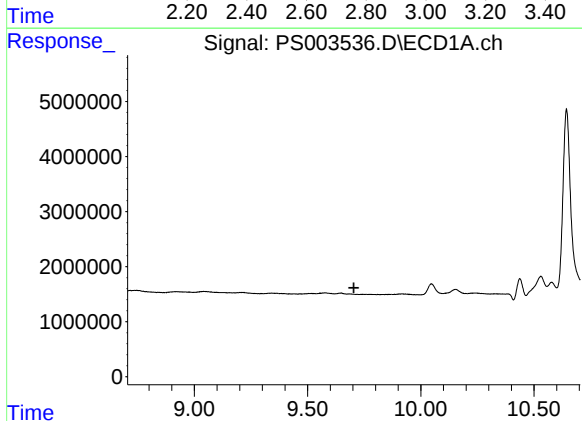


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.705 min
Response: 0
Conc: N.D.

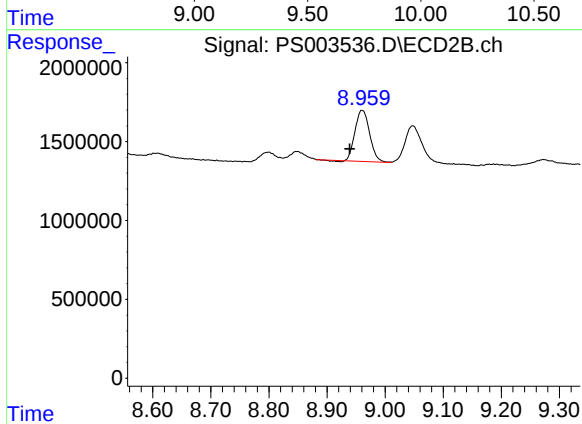

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.961 min
Delta R.T.: 0.021 min
Response: 5632422
Conc: 9.12 ng/ml

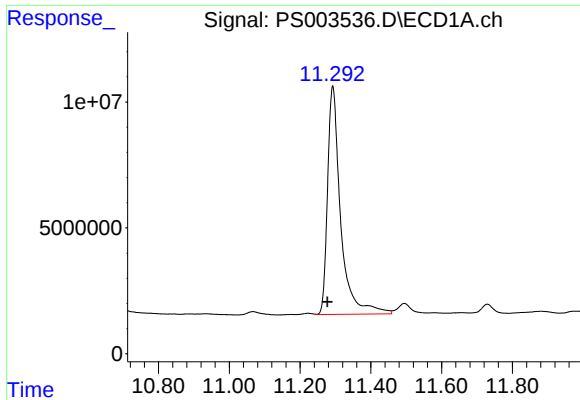

#4 2,4-DCAA


R.T.: 11.293 min
Delta R.T.: 0.015 min
Response: 233382929
Conc: 531.59 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB117886TB

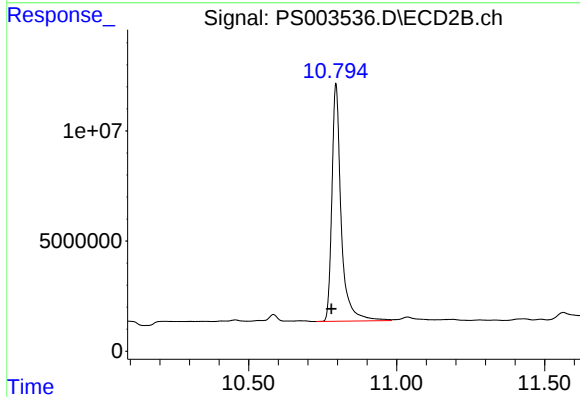


#4 2,4-DCAA

R.T.: 10.795 min
Delta R.T.: 0.015 min
Response: 235578344
Conc: 501.69 ng/ml

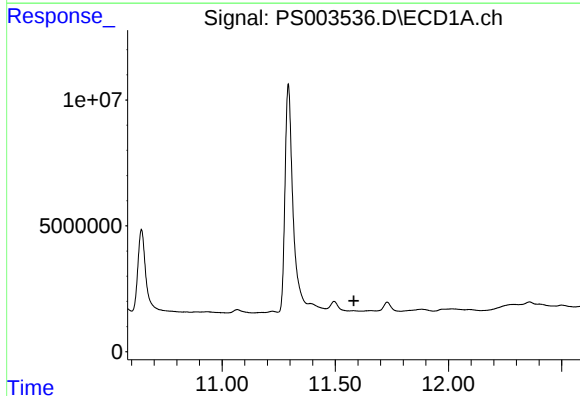


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.582 min
Response: 0
Conc: N.D.

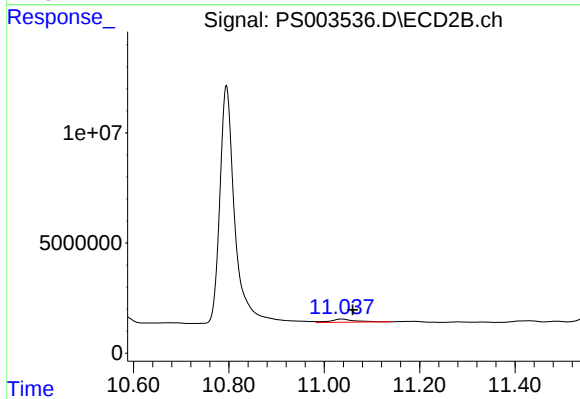

#5 DICAMBA


R.T.: 11.036 min
Delta R.T.: -0.023 min
Response: 4960481
Conc: 2.97 ng/ml

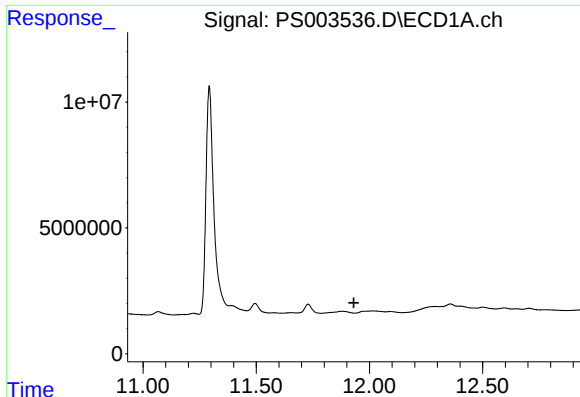

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.931 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB117886TB

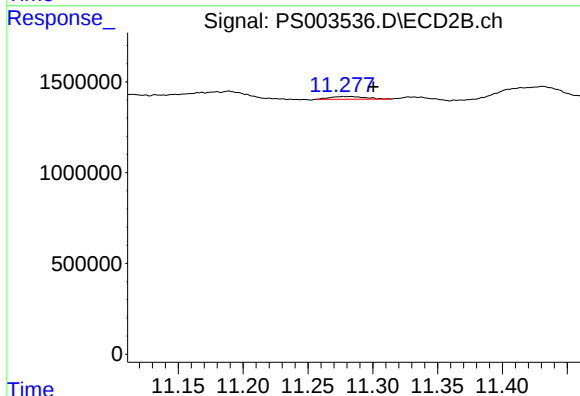


#6 MCP

R.T.: 11.281 min
Delta R.T.: -0.020 min
Response: 273525
Conc: 0.23 ug/ml

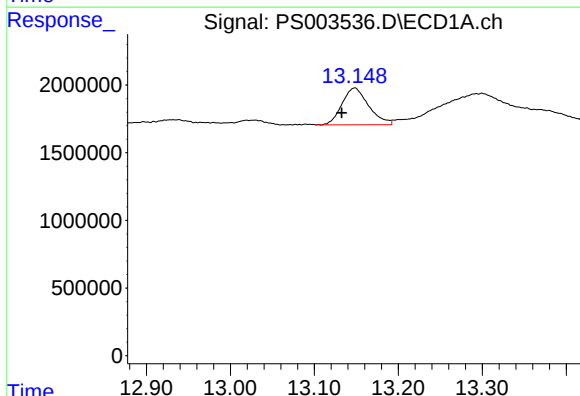


#9 2,4-D

R.T.: 13.148 min
Delta R.T.: 0.015 min
Response: 6003264
Conc: 12.94 ng/ml

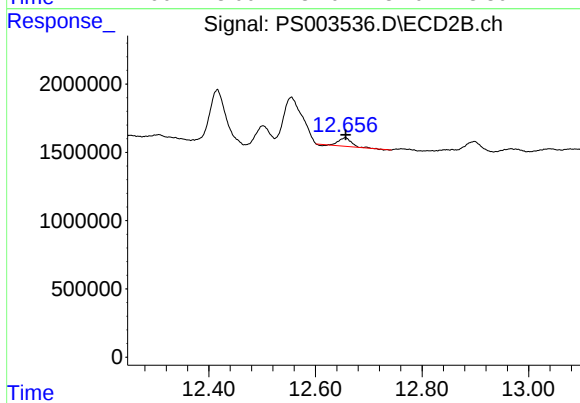

#9 2,4-D


R.T.: 12.656 min
Delta R.T.: -0.001 min
Response: 959806
Conc: 1.83 ng/ml

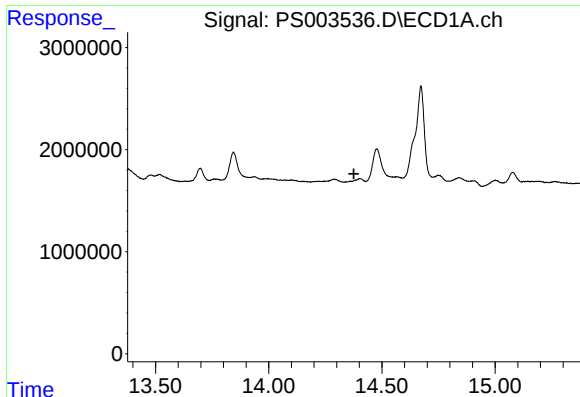

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB117886TB

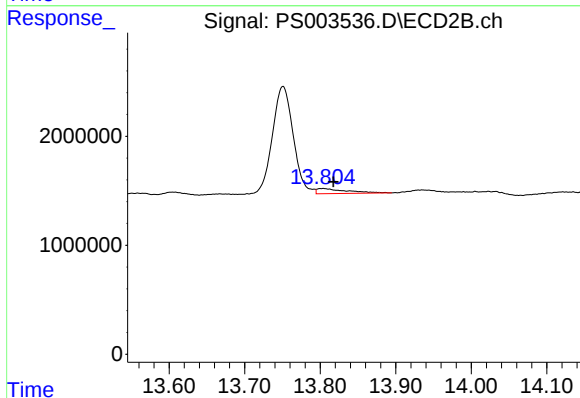


#11 2,4,5-TP (SILVEX)

R.T.: 13.803 min
Delta R.T.: -0.014 min
Response: 1262904
Conc: 0.50 ng/ml

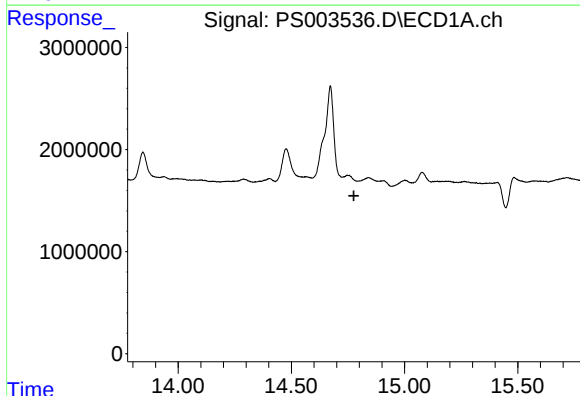


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

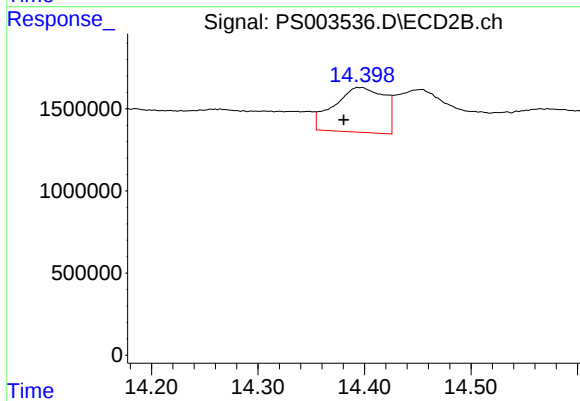

#12 2,4,5-T


R.T.: 14.395 min
Delta R.T.: 0.015 min
Response: 8975126
Conc: 4.45 ng/ml

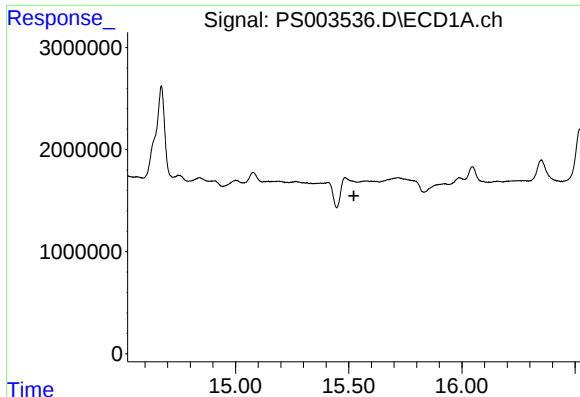

#13 2,4-DB


R.T.: 15.486 min
Delta R.T.: -0.037 min
Response: -1755120
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB117886TB

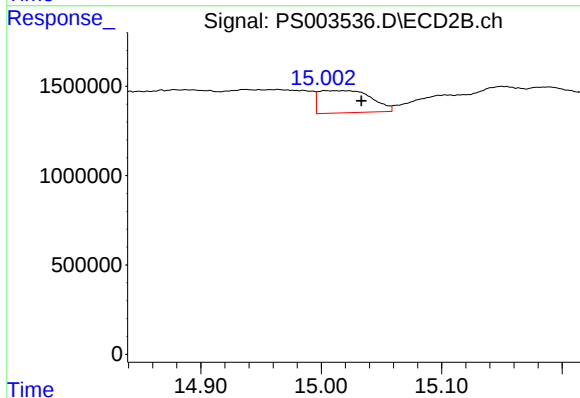


#13 2,4-DB

R.T.: 15.018 min
Delta R.T.: -0.015 min
Response: 3755998
Conc: 14.71 ng/ml

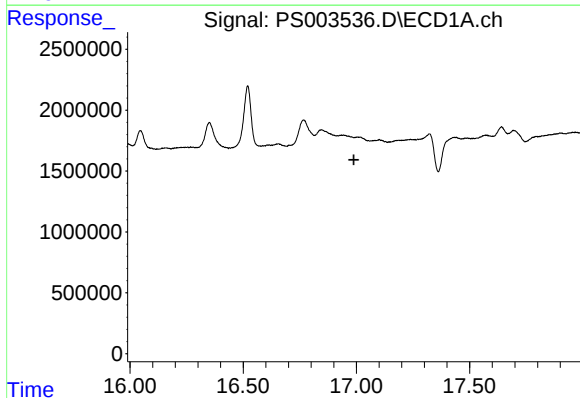


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 16.989 min
Response: 0
Conc: N.D.

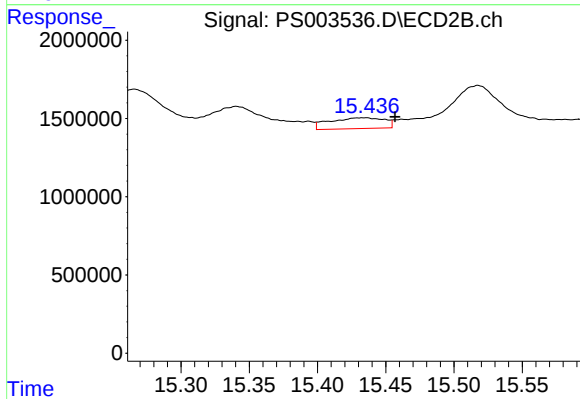

#14 DINOSEB


R.T.: 15.433 min
Delta R.T.: -0.024 min
Response: 1925123
Conc: 1.08 ng/ml

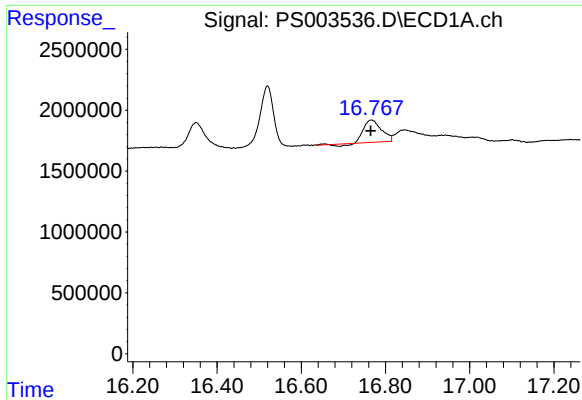

#15 Picloram

R.T.: 16.767 min
Delta R.T.: 0.001 min
Response: 5070415
Conc: 2.06 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB117886TB

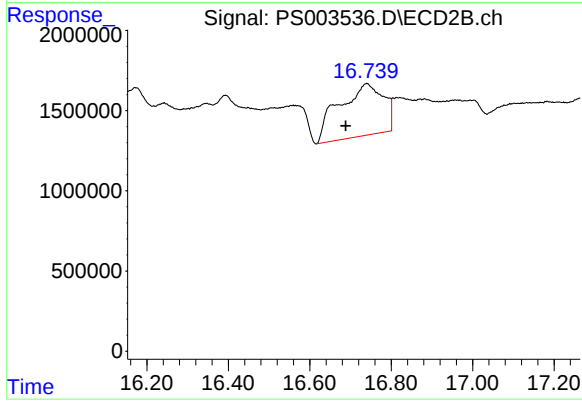

#15 Picloram

R.T.: 16.740 min
Delta R.T.: 0.051 min
Response: 24674119
Conc: 9.72 ng/ml