

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031319\
 Data File : PS003539.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2019 20:23
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 01:09:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.278	10.783	249.8E6	227.6E6	568.989	484.756
Target Compounds							
2) T	3,5-DICHL...	0.000	8.940	0	13831	N.D.	0.022 #
6) T	MCP	0.000	11.306	0	67608	N.D.	0.057 #
7) T	MCPA	0.000	11.675	0	419097	N.D.	0.243 #
10) T	Pentachlo...	0.000	13.195	0	992036	N.D.	0.151 #
11) T	2,4,5-TP ...	0.000	13.862	0	609490	N.D.	0.239 #
13) T	2,4-DB	0.000	15.009	0	1546039	N.D.	6.054 #
15) T	Picloram	16.738	16.708	17114037	3308217	6.953	1.303 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031319\
Data File : PS003539.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2019 20:23
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 01:09:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

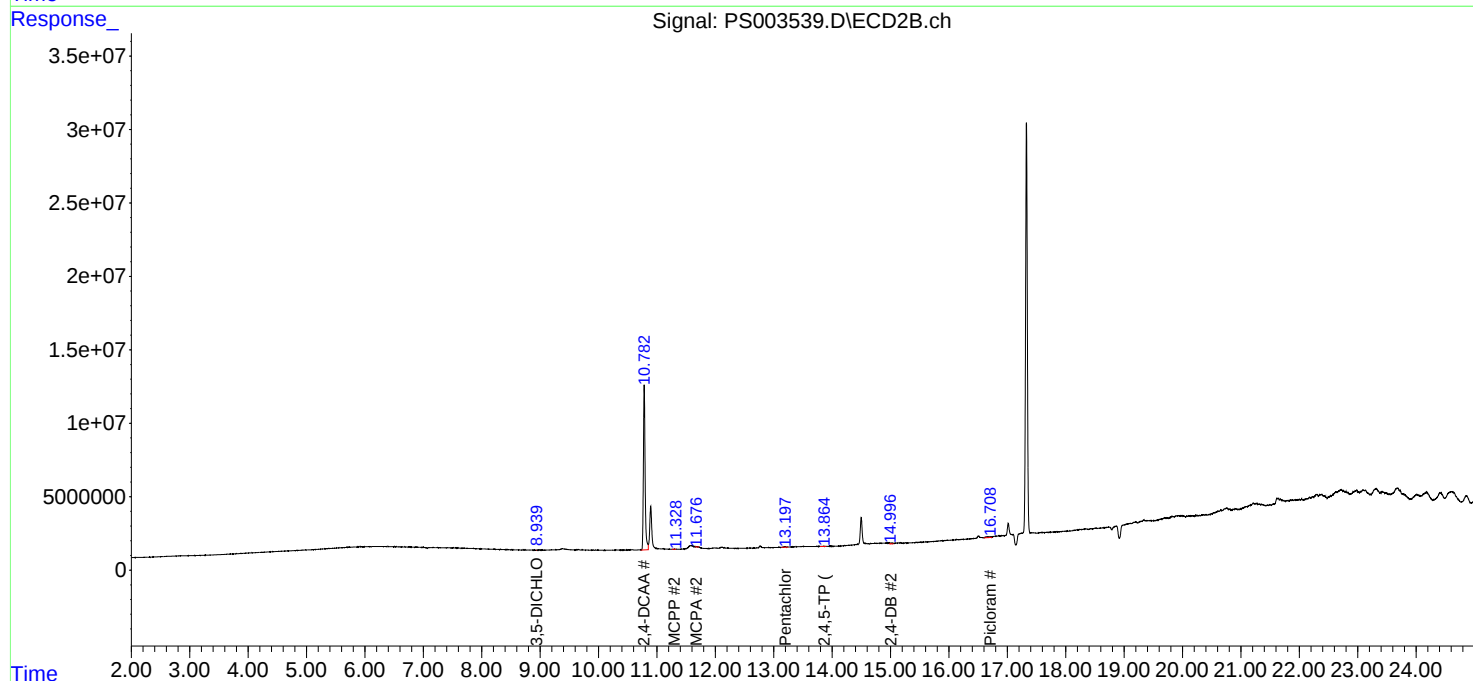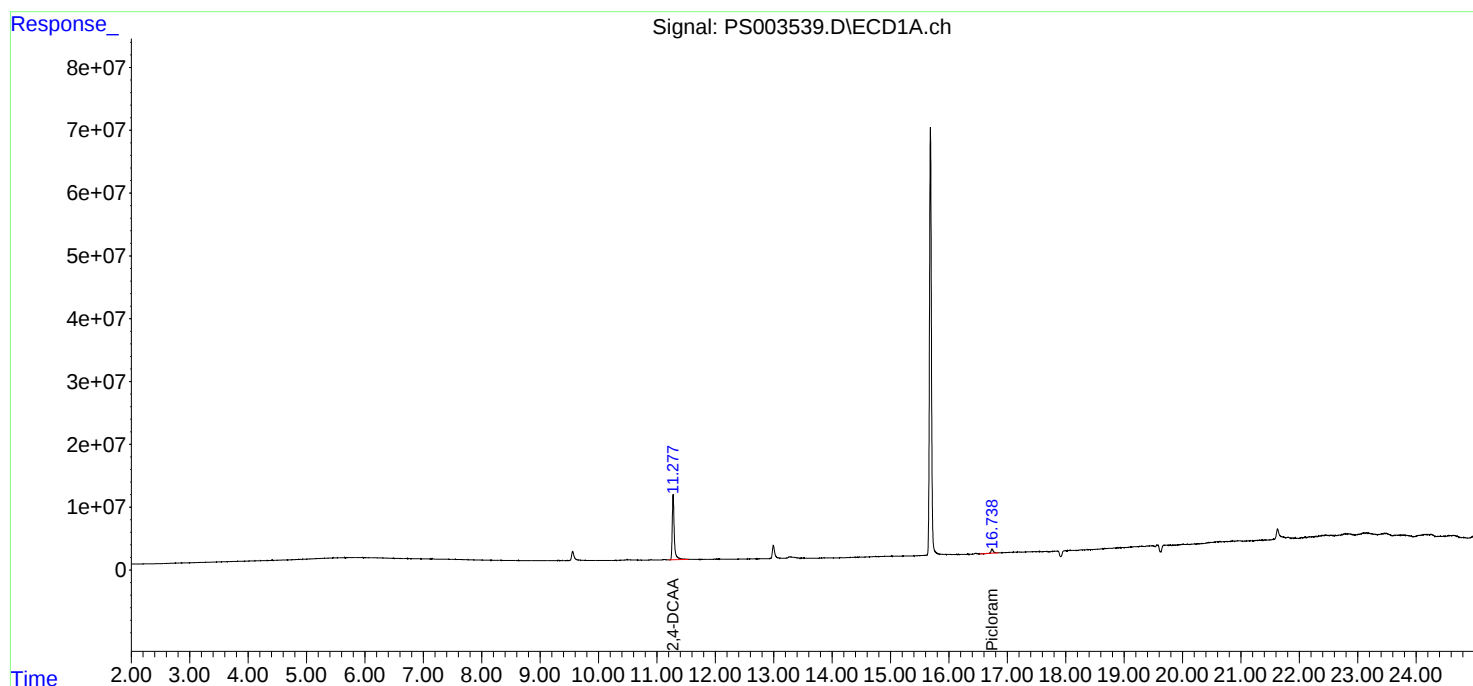


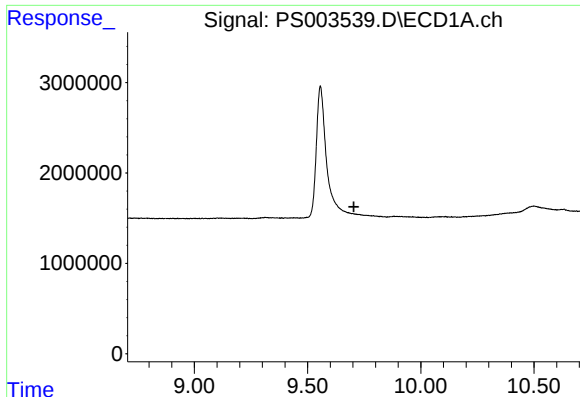

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.705 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

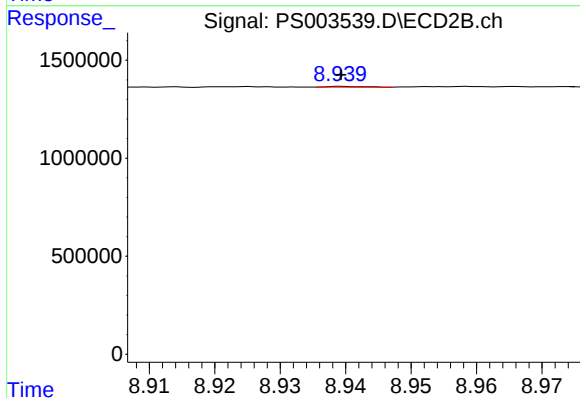


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 8.940 min
Delta R.T.: 0.000 min
Response: 13831
Conc: 0.02 ng/ml

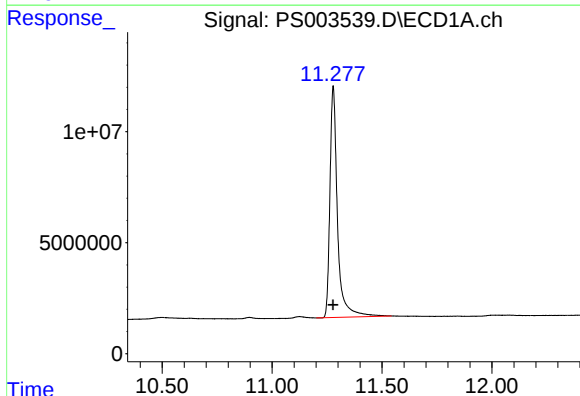


#4 2,4-DCAA

R.T.: 11.278 min
Delta R.T.: 0.000 min
Response: 249800245
Conc: 568.99 ng/ml

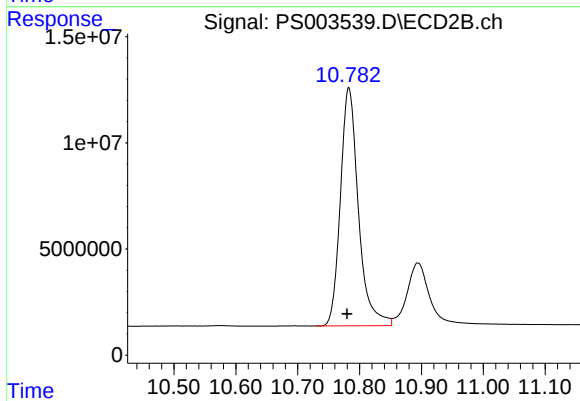

#4 2,4-DCAA


R.T.: 10.783 min
Delta R.T.: 0.003 min
Response: 227626395
Conc: 484.76 ng/ml

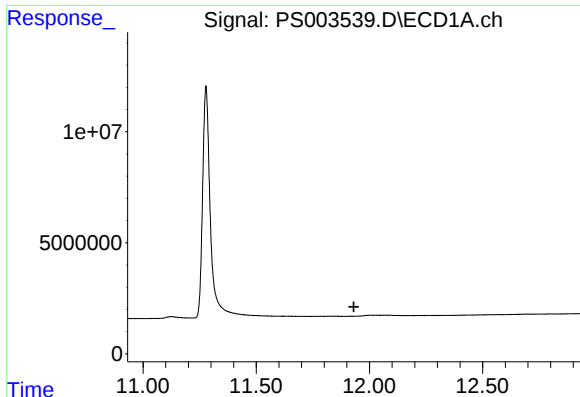

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 11.931 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

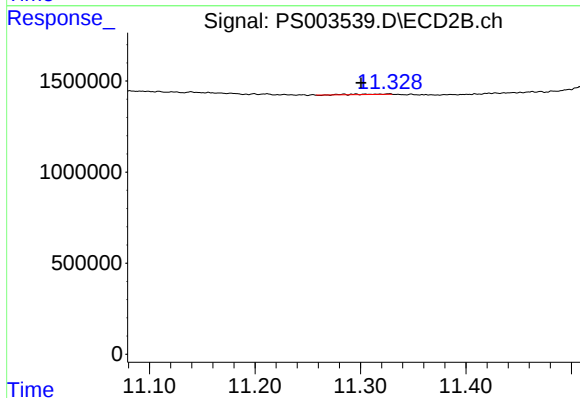


#6 MCPP

R.T.: 11.306 min
Delta R.T.: 0.005 min
Response: 67608
Conc: 0.06 ug/ml

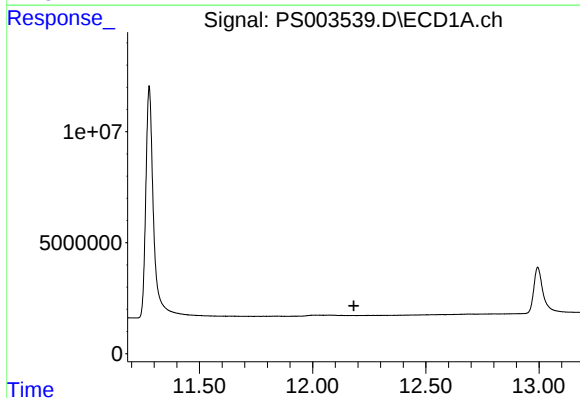


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 12.182 min
Response: 0
Conc: N.D.

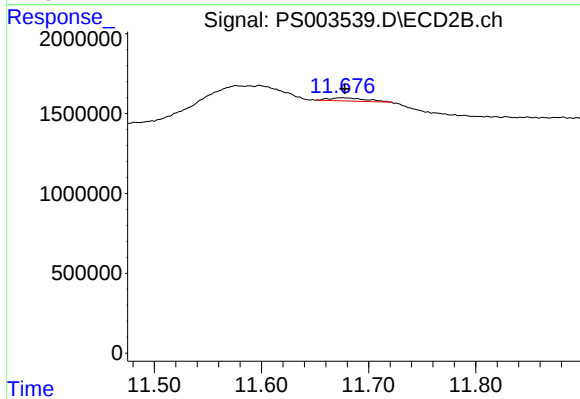

#7 MCPA


R.T.: 11.675 min
Delta R.T.: -0.003 min
Response: 419097
Conc: 0.24 ug/ml

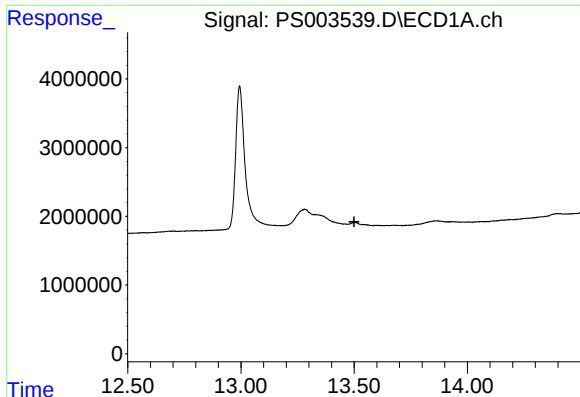

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.499 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

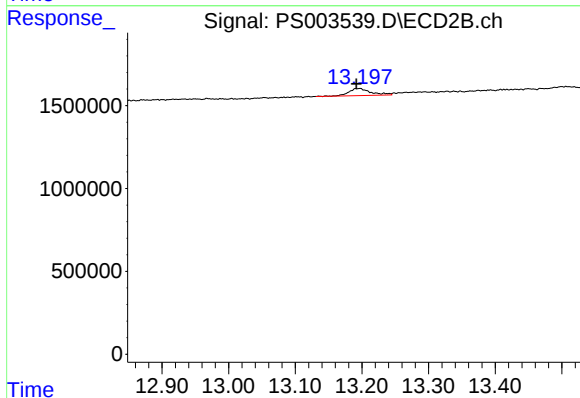


#10 Pentachlorophenol

R.T.: 13.195 min
Delta R.T.: 0.003 min
Response: 992036
Conc: 0.15 ng/ml

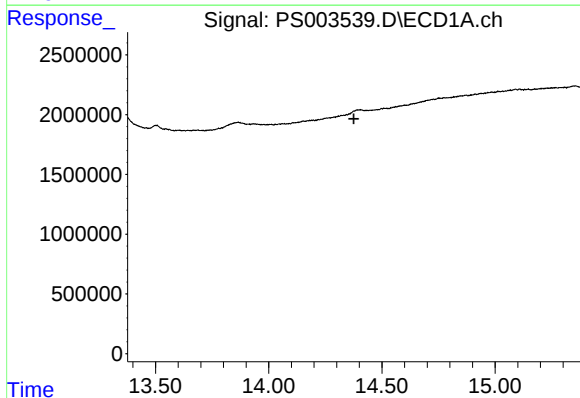


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

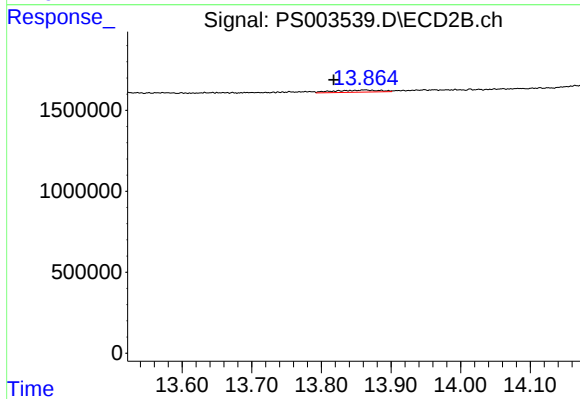

#11 2,4,5-TP (SILVEX)


R.T.: 13.862 min
Delta R.T.: 0.045 min
Response: 609490
Conc: 0.24 ng/ml

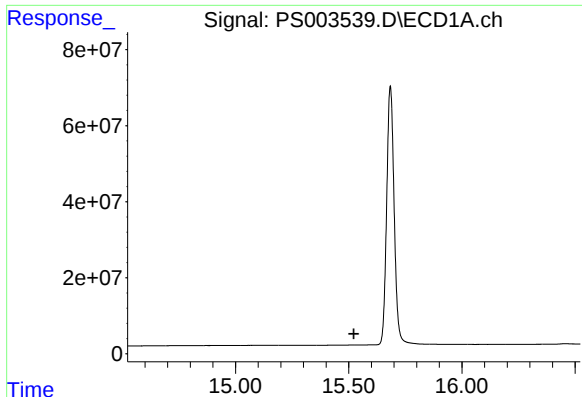

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.523 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

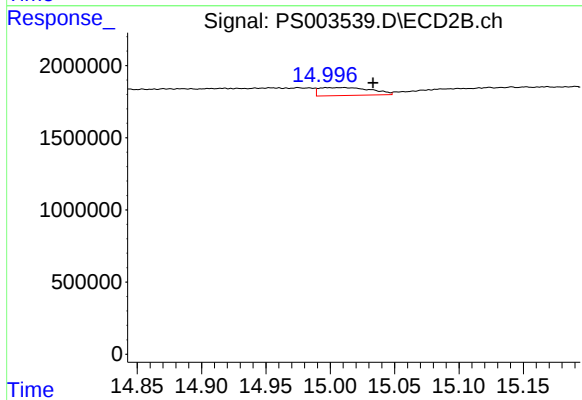


#13 2,4-DB

R.T.: 15.009 min
Delta R.T.: -0.024 min
Response: 1546039
Conc: 6.05 ng/ml

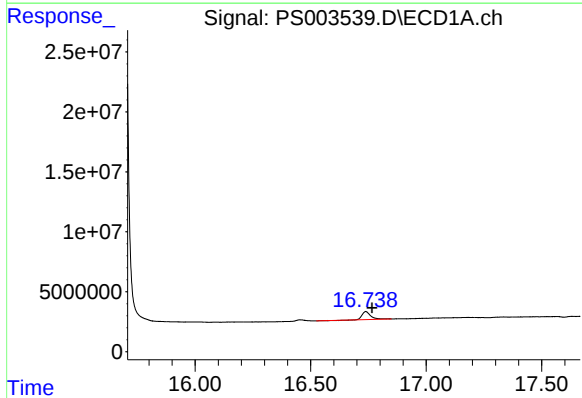

#15 Picloram

R.T.: 16.738 min
Delta R.T.: -0.027 min
Response: 17114037
Conc: 6.95 ng/ml

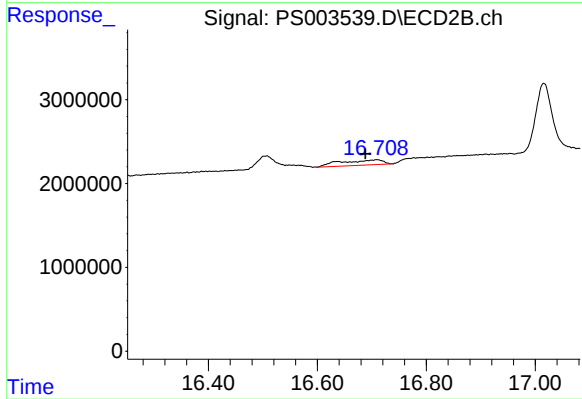

#15 Picloram

R.T.: 16.708 min
Delta R.T.: 0.019 min
Response: 3308217
Conc: 1.30 ng/ml