

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031319\
 Data File : PS003548.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2019 01:03
 Operator : EI\SJ
 Sample : K1870-12
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 04:15:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.272	10.775	195.5E6	196.3E6	445.272	418.025
Target Compounds							
1) T	Dalapon	0.000	2.281	0	21357691	N.D.	33.731 #
2) T	3,5-DICHL...	0.000	8.941	0	4857518	N.D.	7.867 #
3) T	4-Nitroph...	0.000	9.961	0	2921365	N.D.	12.994 #
5) T	DICAMBA	0.000	11.014	0	4108998	N.D.	2.459 #
6) T	MCP	11.971	11.310	5819207	479174	4.432	0.406 #
9) T	2,4-D	13.127	12.636	3692586	1542796	7.961	2.939 #
11) T	2,4,5-TP ...	0.000	13.842	0	260157	N.D.	0.102 #
12) T	2,4,5-T	0.000	14.374	0	8814202	N.D.	4.370 #
14) T	DINOSEB	0.000	15.495	0	17938047	N.D.	10.050 #
15) T	Picloram	16.741	16.737	16921841	20849926	6.875	8.215



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031319\
Data File : PS003548.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2019 01:03
Operator : EI\SJ
Sample : K1870-12
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
SP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 04:15:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

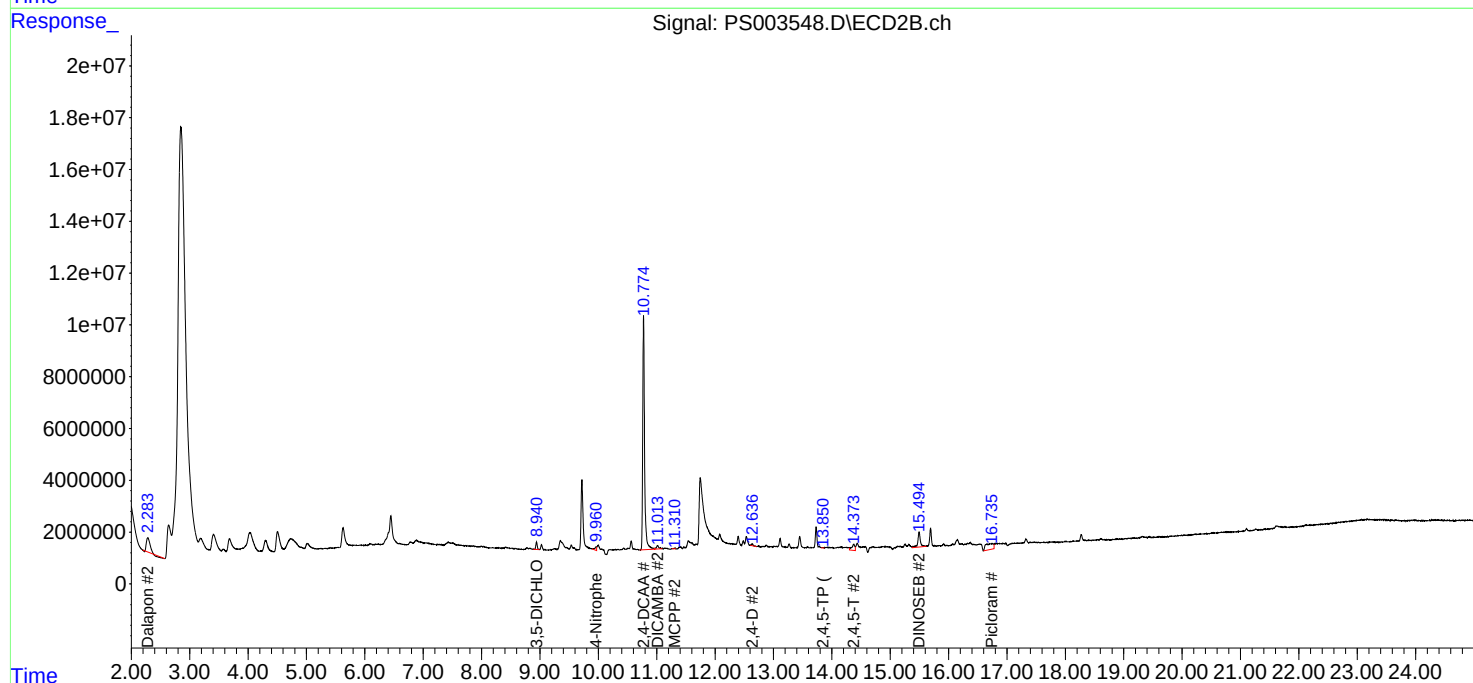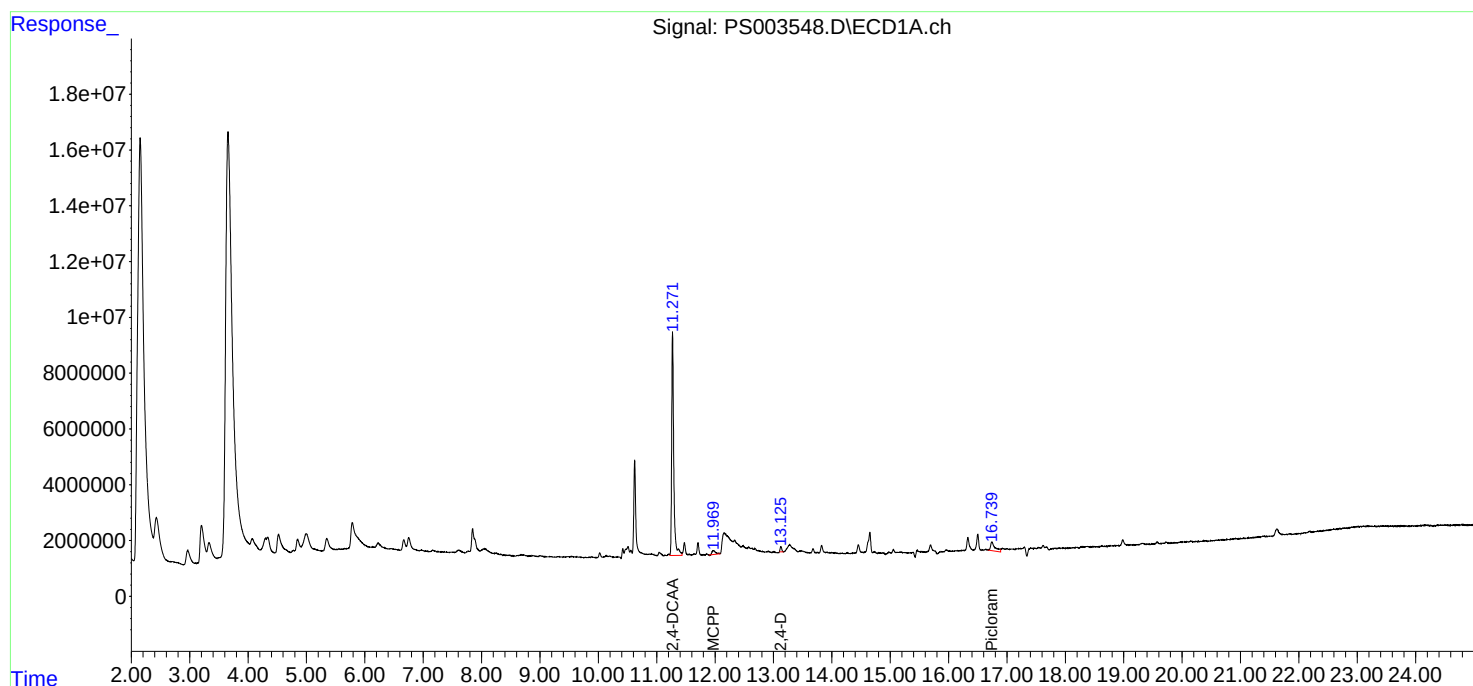


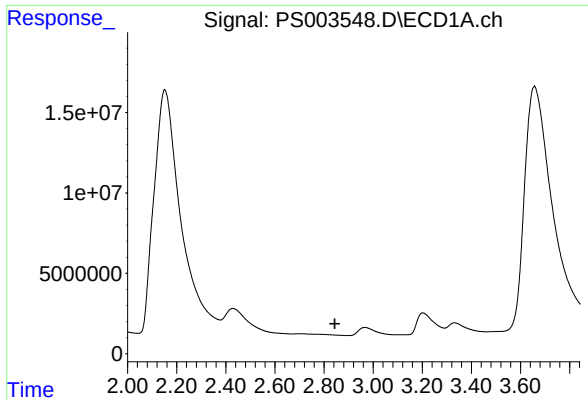

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 2.844 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SP-3

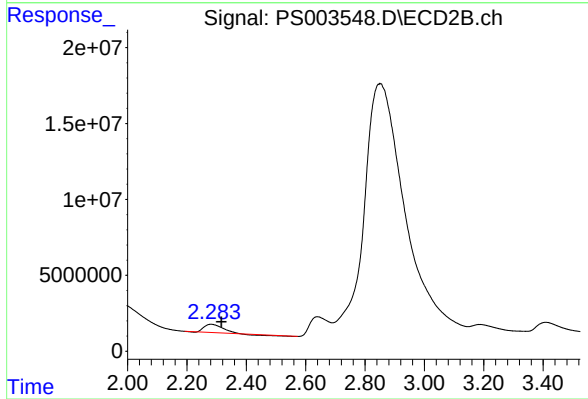


#1 Dalapon

R.T.: 2.281 min
Delta R.T.: -0.035 min
Response: 21357691
Conc: 33.73 ng/ml

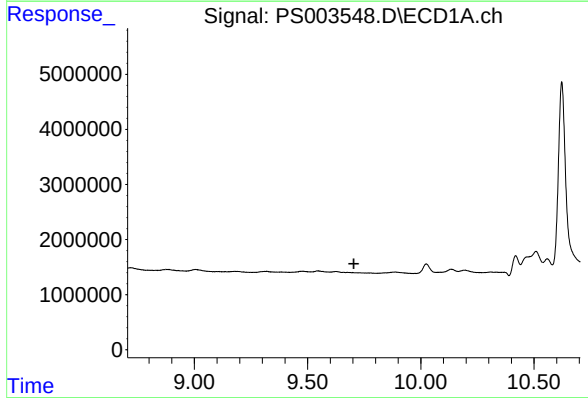


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.705 min
Response: 0
Conc: N.D.

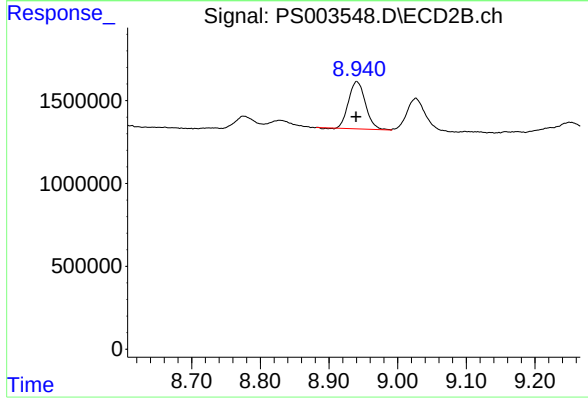

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.941 min
Delta R.T.: 0.001 min
Response: 4857518
Conc: 7.87 ng/ml

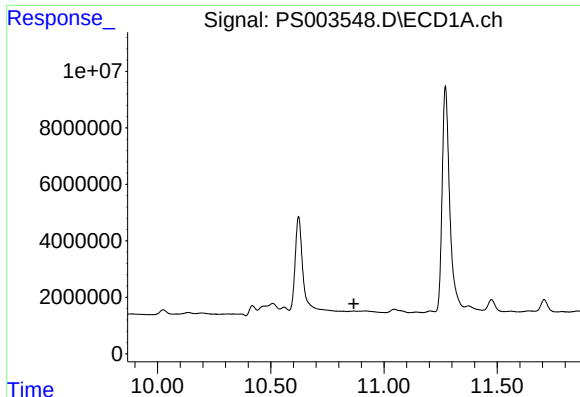

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SP-3

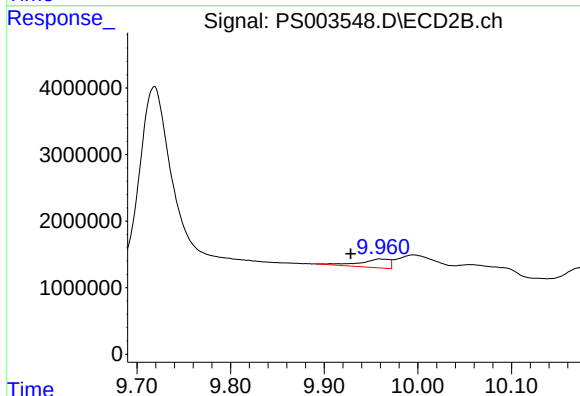


#3 4-Nitrophenol

R.T.: 9.961 min
Delta R.T.: 0.032 min
Response: 2921365
Conc: 12.99 ng/ml

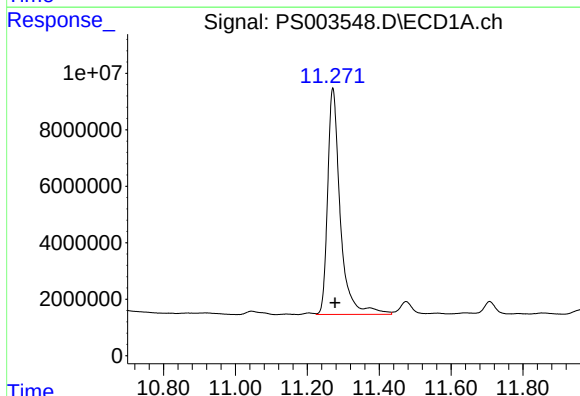


#4 2,4-DCAA

R.T.: 11.272 min
Delta R.T.: -0.006 min
Response: 195485190
Conc: 445.27 ng/ml

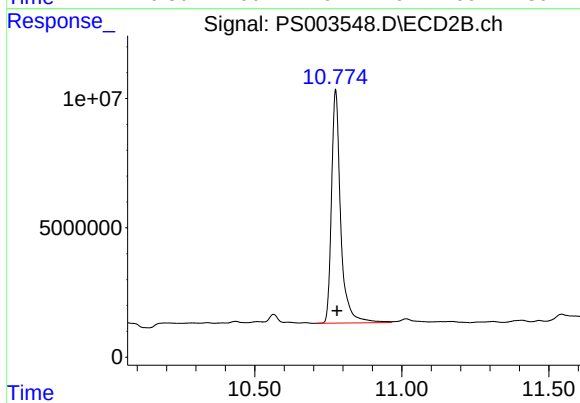

#4 2,4-DCAA


R.T.: 10.775 min
Delta R.T.: -0.005 min
Response: 196291713
Conc: 418.03 ng/ml

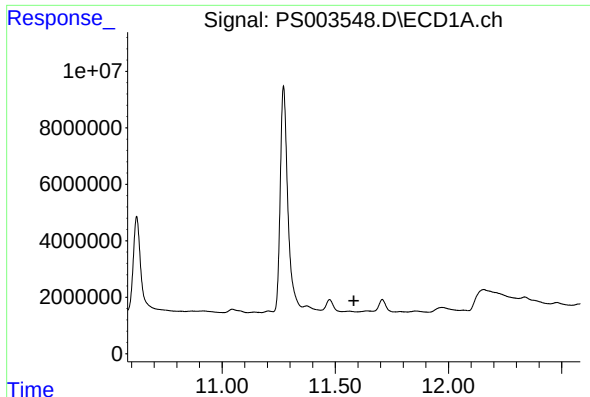

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.582 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SP-3

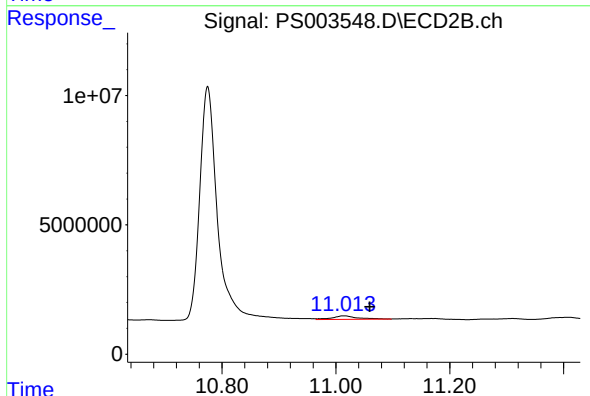


#5 DICAMBA

R.T.: 11.014 min
Delta R.T.: -0.045 min
Response: 4108998
Conc: 2.46 ng/ml

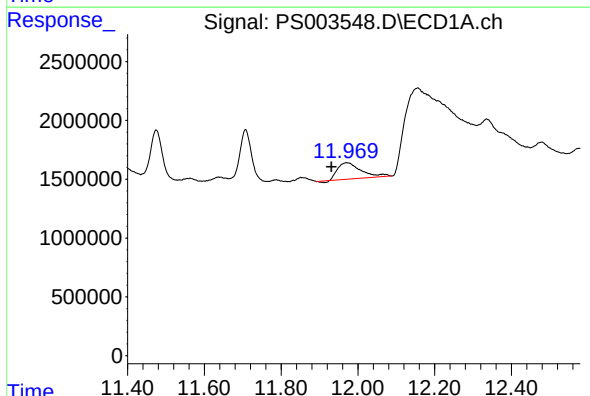


#6 MCP

R.T.: 11.971 min
Delta R.T.: 0.040 min
Response: 5819207
Conc: 4.43 ug/ml

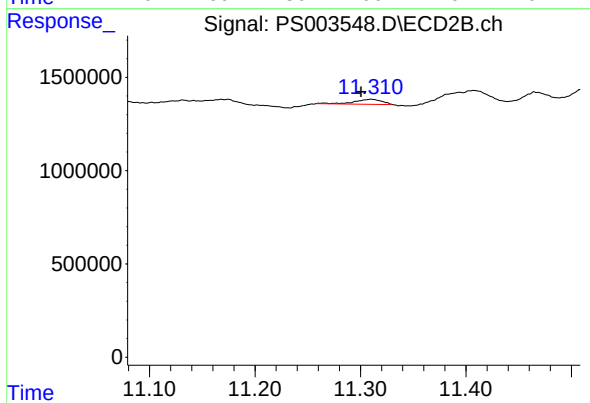

#6 MCP


R.T.: 11.310 min
Delta R.T.: 0.010 min
Response: 479174
Conc: 0.41 ug/ml

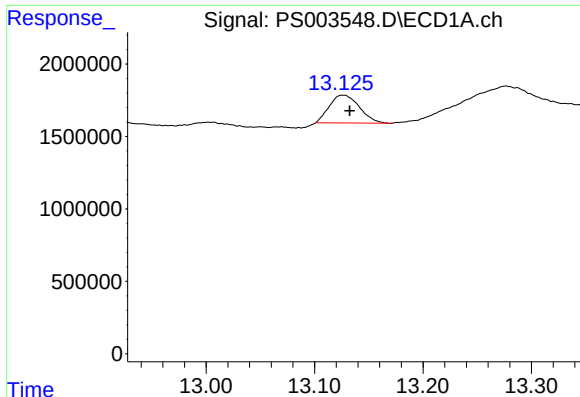

#9 2,4-D


R.T.: 13.127 min
Delta R.T.: -0.006 min
Response: 3692586
Conc: 7.96 ng/ml

Instrument :
ECD_S
ClientSampleId :
SP-3

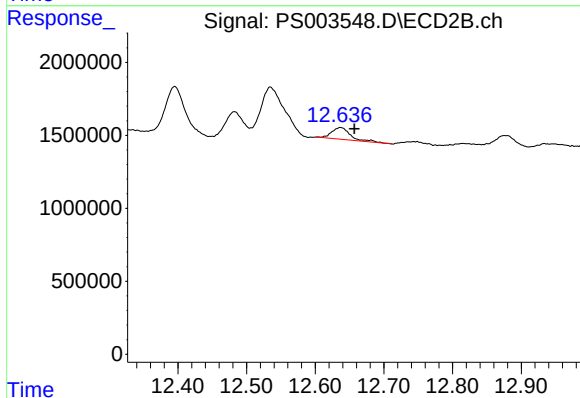


#9 2,4-D

R.T.: 12.636 min
Delta R.T.: -0.021 min
Response: 1542796
Conc: 2.94 ng/ml

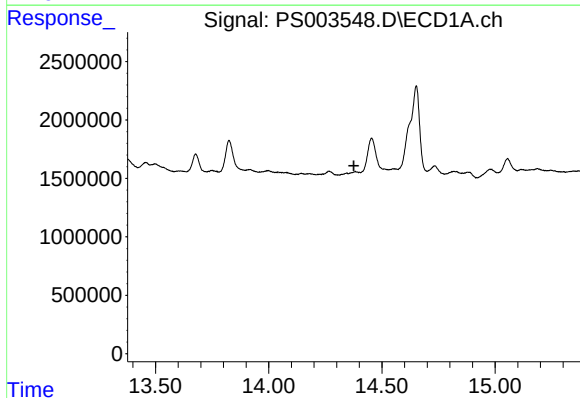


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.376 min
Response: 0
Conc: N.D.

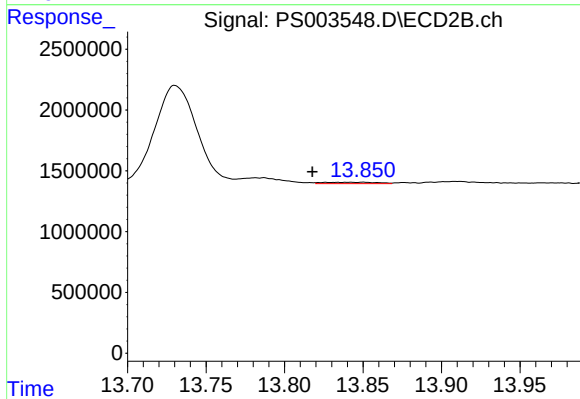

#11 2,4,5-TP (SILVEX)


R.T.: 13.842 min
Delta R.T.: 0.025 min
Response: 260157
Conc: 0.10 ng/ml

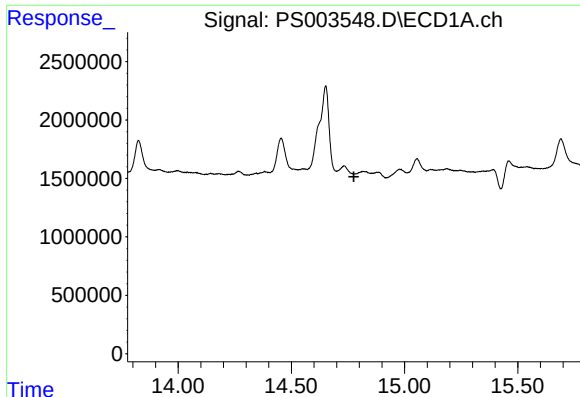

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SP-3

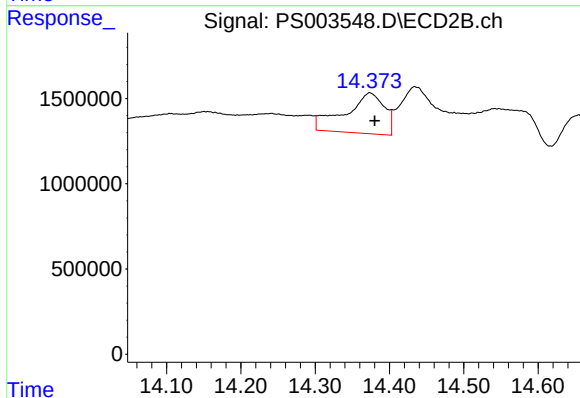


#12 2,4,5-T

R.T.: 14.374 min
Delta R.T.: -0.006 min
Response: 8814202
Conc: 4.37 ng/ml

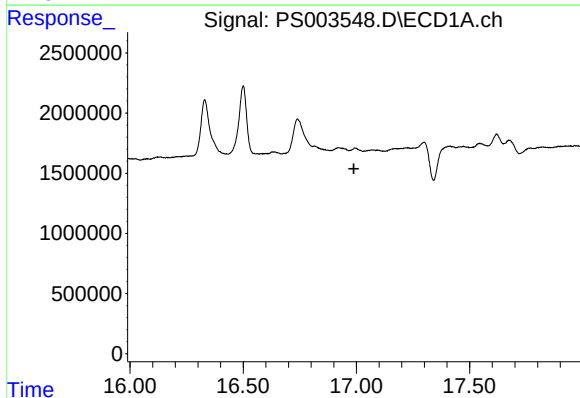


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

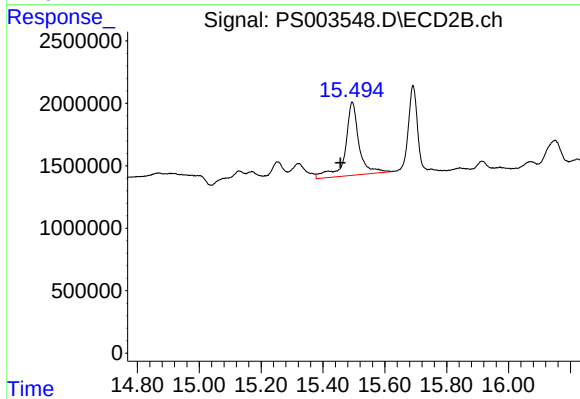

#14 DINOSEB


R.T.: 15.495 min
Delta R.T.: 0.038 min
Response: 17938047
Conc: 10.05 ng/ml

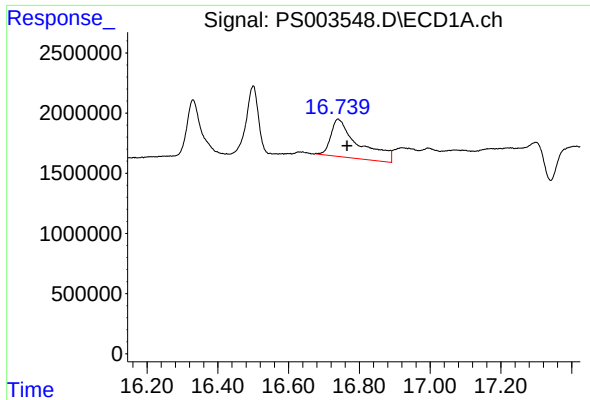

#15 Picloram

R.T.: 16.741 min
Delta R.T.: -0.024 min
Response: 16921841
Conc: 6.88 ng/ml

Instrument :
ECD_S
ClientSampleId :
SP-3

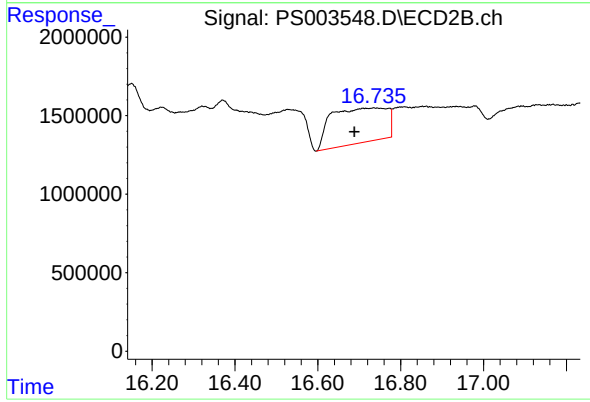

#15 Picloram

R.T.: 16.737 min
Delta R.T.: 0.049 min
Response: 20849926
Conc: 8.21 ng/ml