

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031319\
 Data File : PS003549.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2019 01:35
 Operator : EI\SJ
 Sample : K1871-04
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 04:16:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.274	10.778	181.1E6	186.5E6	412.498	397.102
Target Compounds							
1) T	Dalapon	0.000	2.288	0	25944006	N.D.	40.974 #
2) T	3,5-DICHL...	0.000	8.943	0	4479213	N.D.	7.254 #
3) T	4-Nitroph...	0.000	9.997	0	9359094	N.D.	41.628 #
5) T	DICAMBA	0.000	11.017	0	3957405	N.D.	2.369 #
6) T	MCP	11.966	11.314	2942823	238066	2.241	0.202 #
9) T	2,4-D	13.130	12.639	4516432	1313764	9.738	2.503 #
12) T	2,4,5-T	0.000	14.378	0	7524943	N.D.	3.731 #
13) T	2,4-DB	15.466	0.000	3775574	0	15.944	N.D. #
14) T	DINOSEB	0.000	15.498	0	15014165	N.D.	8.412 #
15) T	Picloram	16.743	16.738	9424290	18977920	3.829	7.477 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031319\
Data File : PS003549.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2019 01:35
Operator : EI\SJ
Sample : K1871-04
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 04:16:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

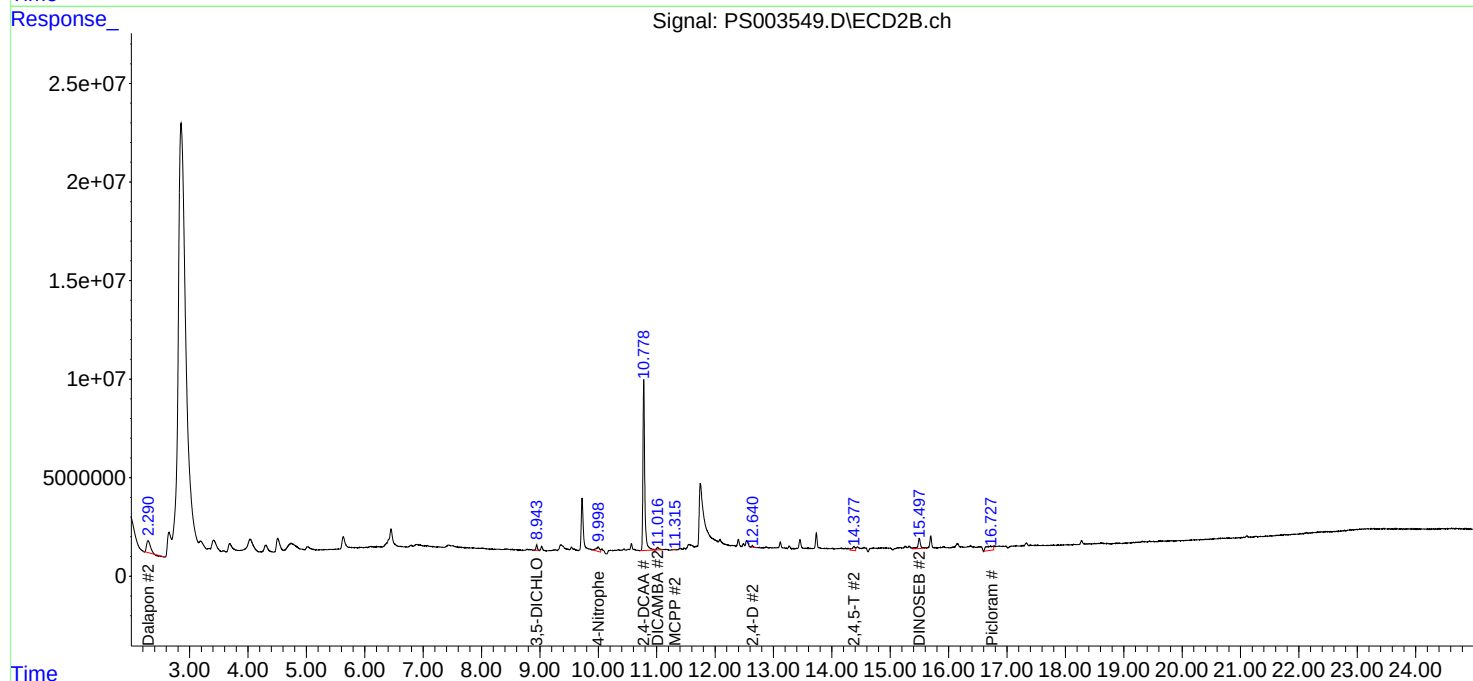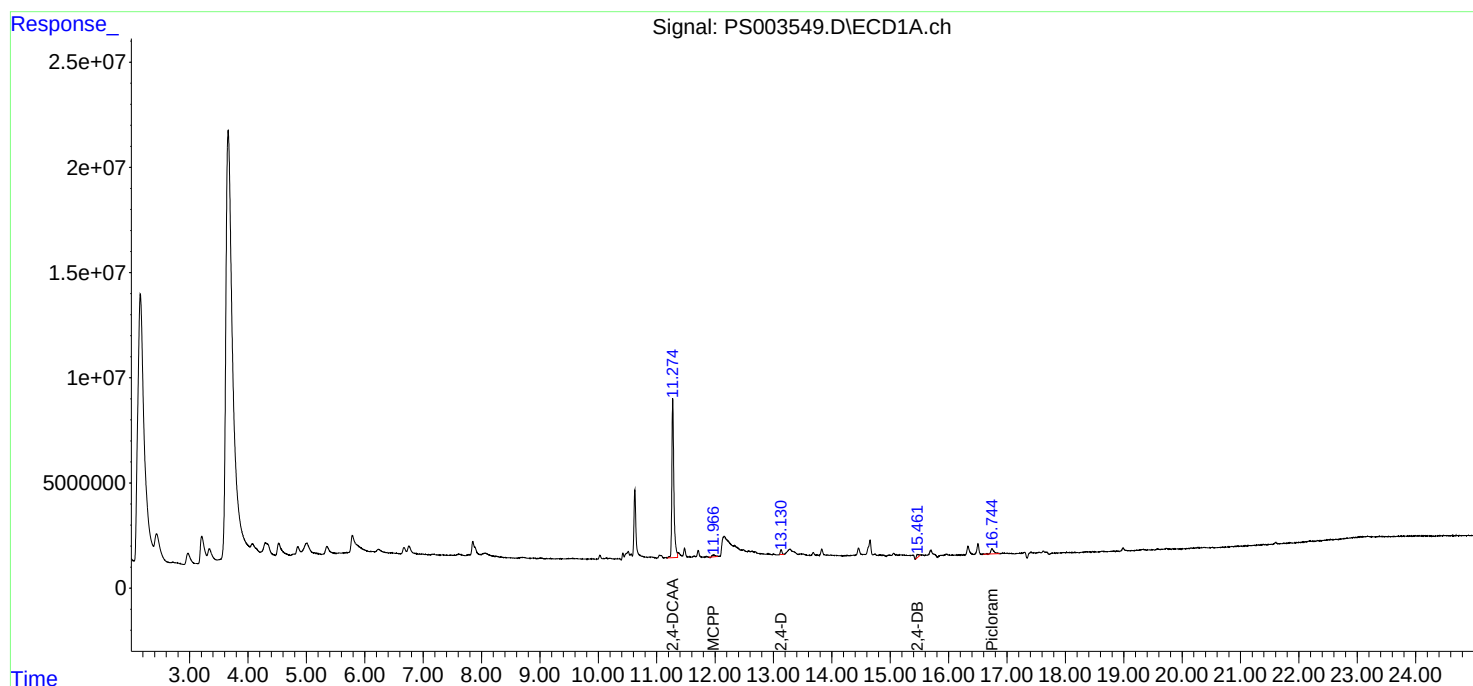


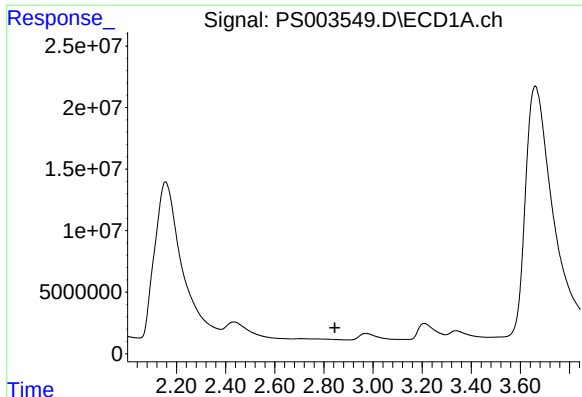

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 2.844 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-1

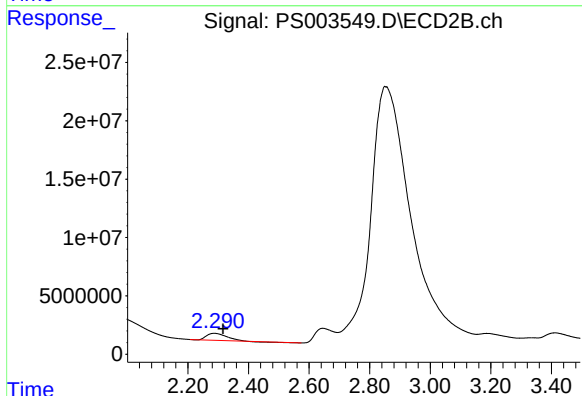


#1 Dalapon

R.T.: 2.288 min
Delta R.T.: -0.029 min
Response: 25944006
Conc: 40.97 ng/ml

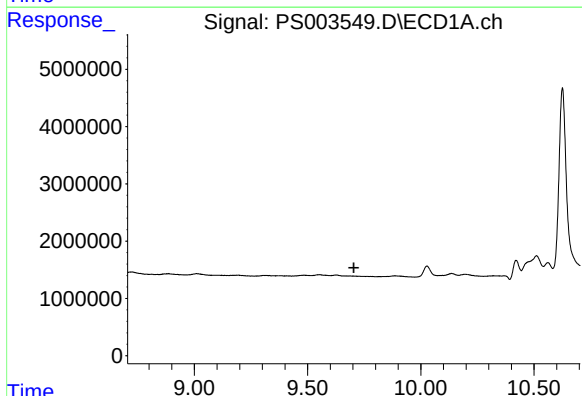


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.705 min
Response: 0
Conc: N.D.

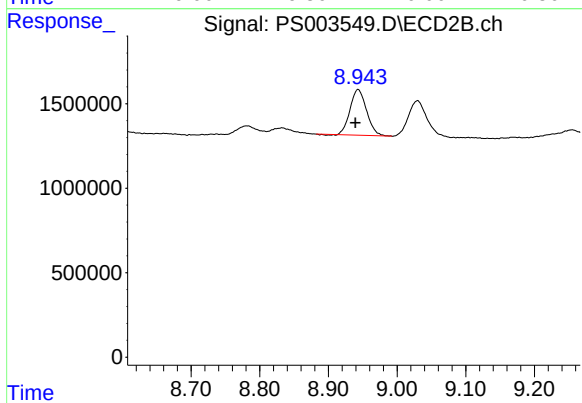

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.943 min
Delta R.T.: 0.004 min
Response: 4479213
Conc: 7.25 ng/ml

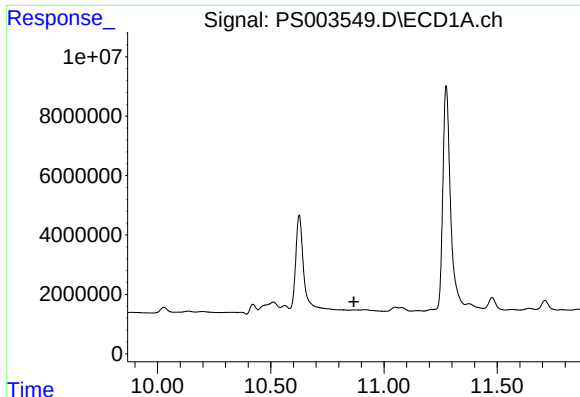

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-1

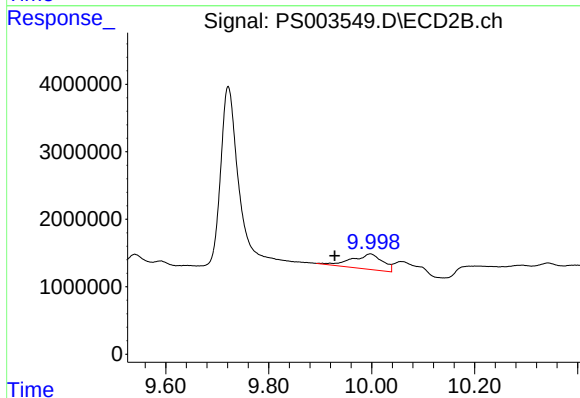


#3 4-Nitrophenol

R.T.: 9.997 min
Delta R.T.: 0.069 min
Response: 9359094
Conc: 41.63 ng/ml

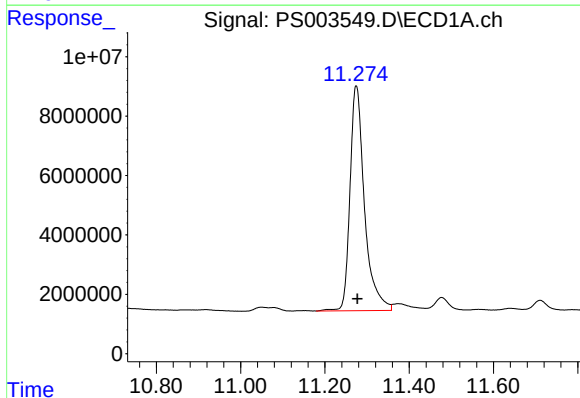


#4 2,4-DCAA

R.T.: 11.274 min
Delta R.T.: -0.003 min
Response: 181096671
Conc: 412.50 ng/ml

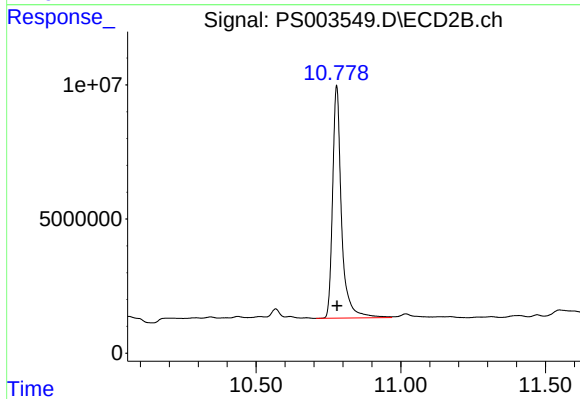

#4 2,4-DCAA


R.T.: 10.778 min
Delta R.T.: -0.002 min
Response: 186466684
Conc: 397.10 ng/ml

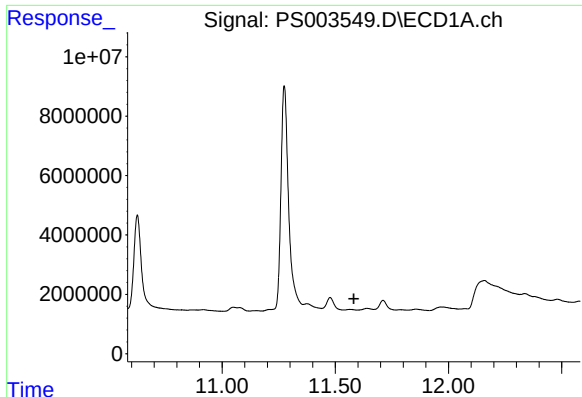

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.582 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-1

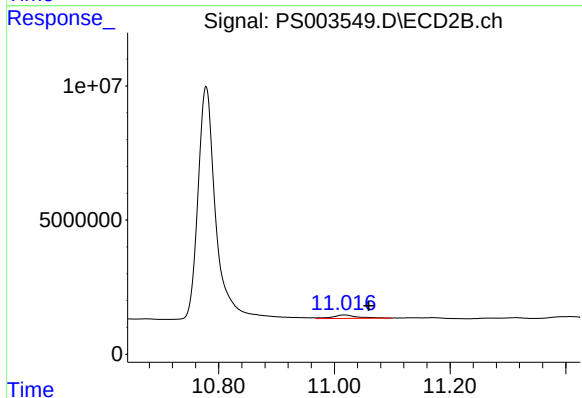


#5 DICAMBA

R.T.: 11.017 min
Delta R.T.: -0.042 min
Response: 3957405
Conc: 2.37 ng/ml

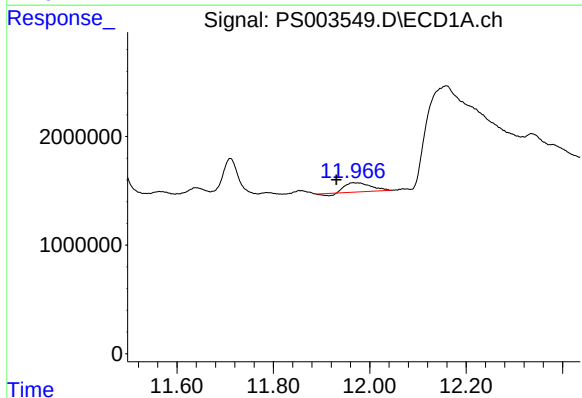


#6 MCP

R.T.: 11.966 min
Delta R.T.: 0.035 min
Response: 2942823
Conc: 2.24 ug/ml

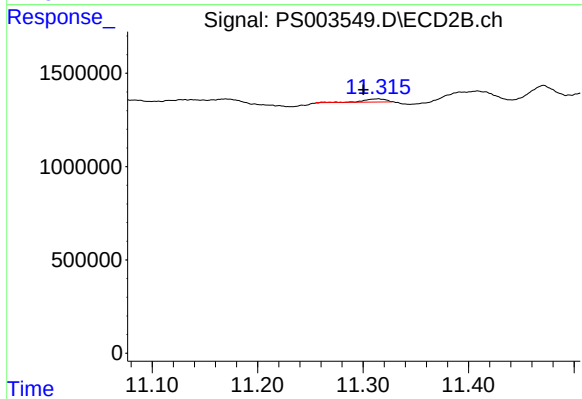

#6 MCP


R.T.: 11.314 min
Delta R.T.: 0.013 min
Response: 238066
Conc: 0.20 ug/ml

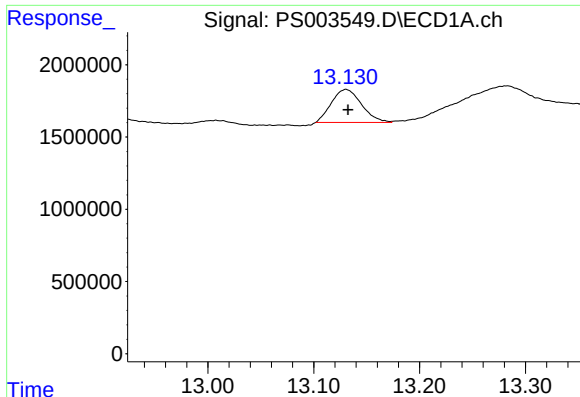

#9 2,4-D


R.T.: 13.130 min
Delta R.T.: -0.002 min
Response: 4516432
Conc: 9.74 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-1

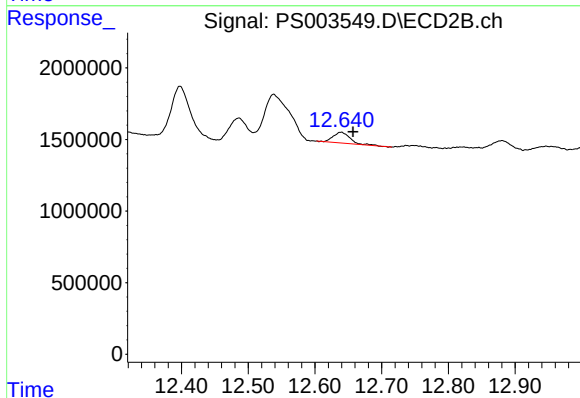


#9 2,4-D

R.T.: 12.639 min
Delta R.T.: -0.018 min
Response: 1313764
Conc: 2.50 ng/ml

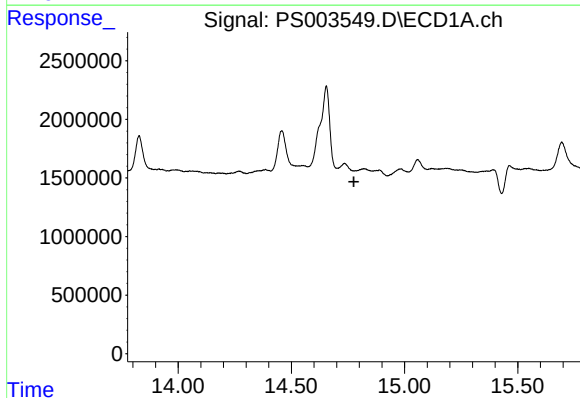


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.776 min
Response: 0
Conc: N.D.

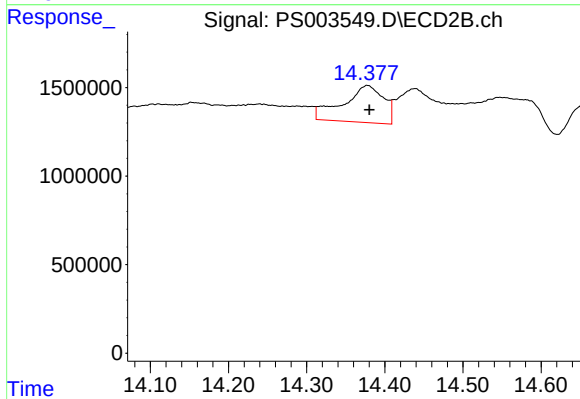

#12 2,4,5-T


R.T.: 14.378 min
Delta R.T.: -0.003 min
Response: 7524943
Conc: 3.73 ng/ml

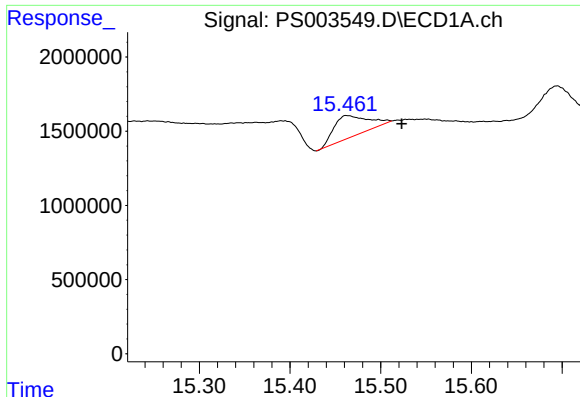

#13 2,4-DB


R.T.: 15.466 min
Delta R.T.: -0.057 min
Response: 3775574
Conc: 15.94 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-1

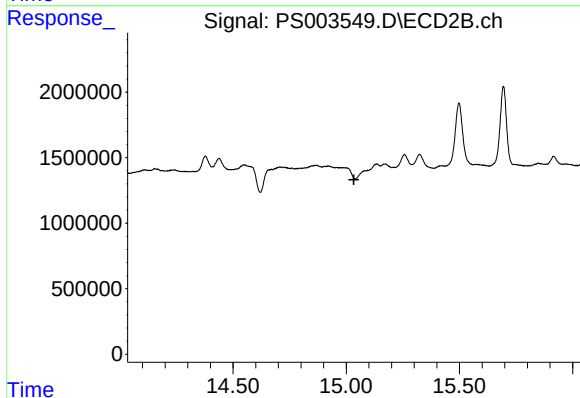


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 15.033 min
Response: 0
Conc: N.D.

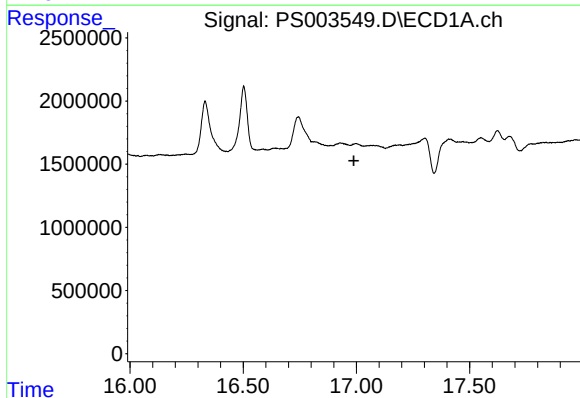


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 16.989 min
Response: 0
Conc: N.D.

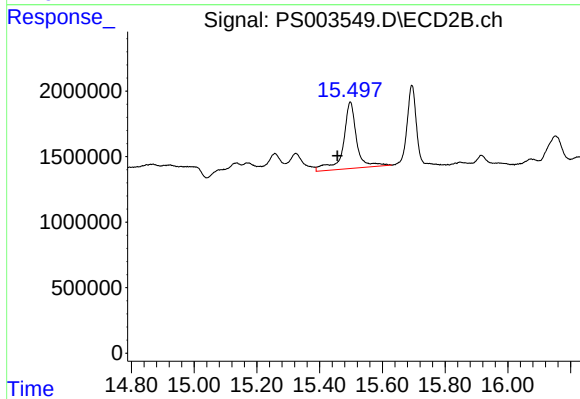

#14 DINOSEB


R.T.: 15.498 min
Delta R.T.: 0.041 min
Response: 15014165
Conc: 8.41 ng/ml

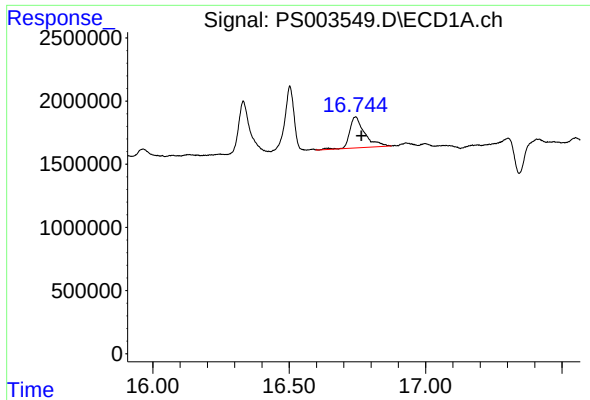

#15 Picloram

R.T.: 16.743 min
Delta R.T.: -0.022 min
Response: 9424290
Conc: 3.83 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-1

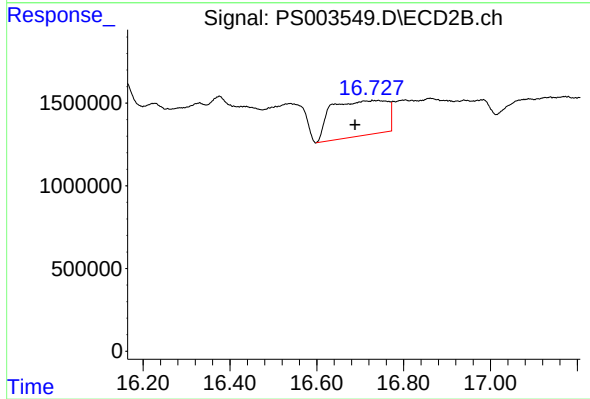

#15 Picloram

R.T.: 16.738 min
Delta R.T.: 0.049 min
Response: 18977920
Conc: 7.48 ng/ml