

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031319\
 Data File : PS003552.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2019 03:08
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 04:17:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.300	10.802	256.6E6	223.1E6	584.404	475.154
Target Compounds							
3) T	4-Nitroph...	0.000	9.952	0	38797	N.D.	0.173 #
7) T	MCPA	0.000	11.694	0	461967	N.D.	0.268 #
8) T	DICHLORPROP	0.000	12.163	0	2385517	N.D.	5.773 #
10) T	Pentachlo...	0.000	13.218	0	904568	N.D.	0.137 #
11) T	2,4,5-TP ...	0.000	13.756	0	62851	N.D.	0.025 #
12) T	2,4,5-T	0.000	14.397	0	322965	N.D.	0.160 #
13) T	2,4-DB	0.000	15.008	0	354424	N.D.	1.388 #
14) T	DINOSEB	0.000	15.452	0	140155	N.D.	0.079 #
15) T	Picloram	16.775	16.698	18642178	1115754	7.574	0.440 #
16) T	DCPA	0.000	16.651	0	3112997	N.D.	1.001 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031319\
Data File : PS003552.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2019 03:08
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 04:17:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

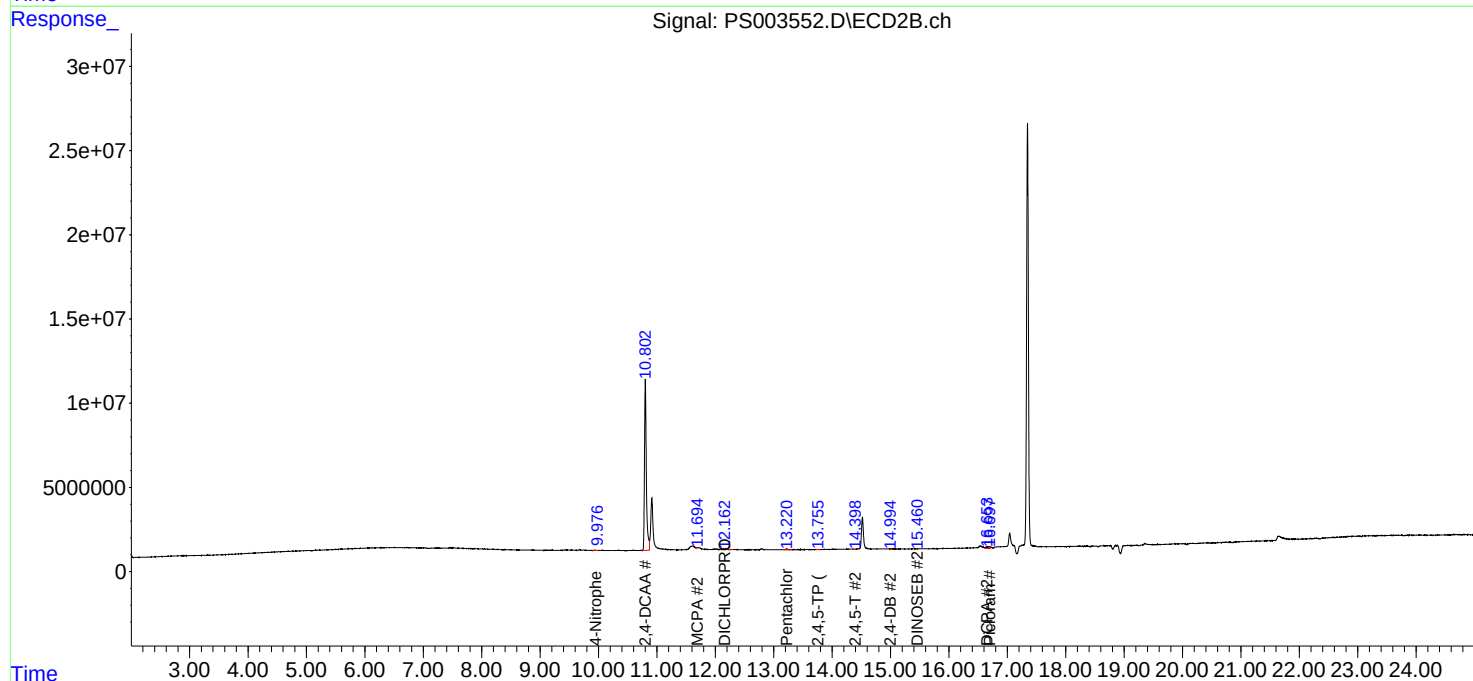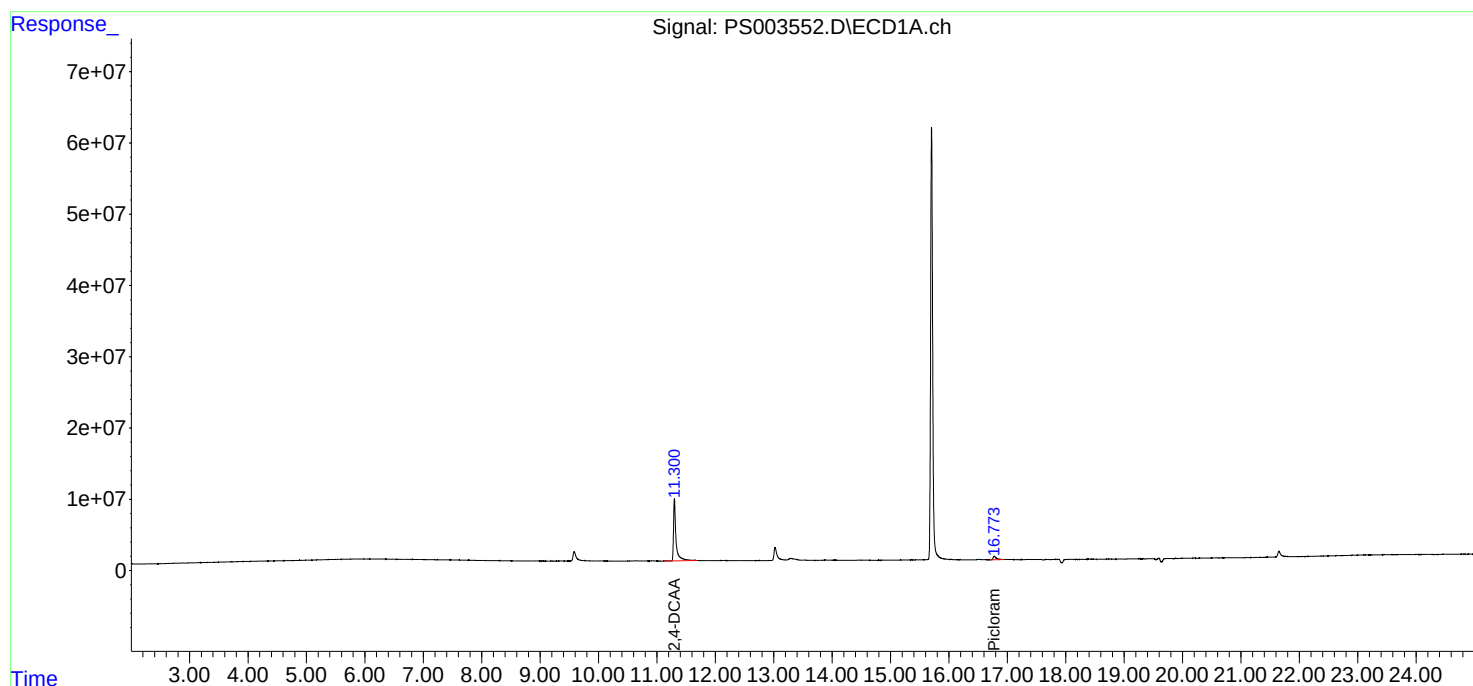


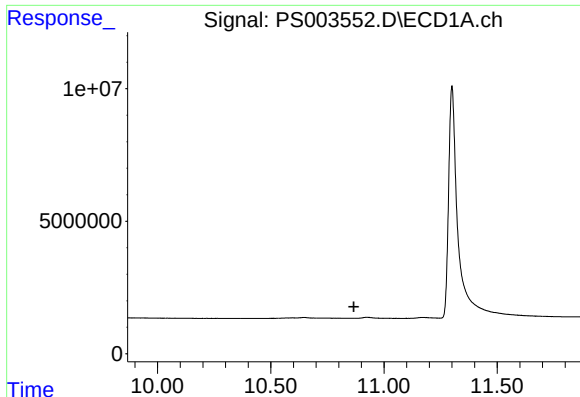

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

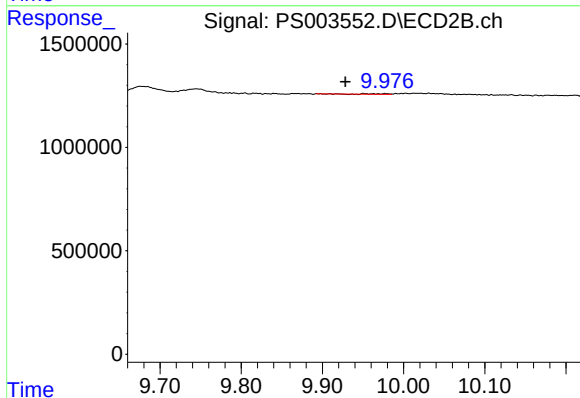


#3 4-Nitrophenol

R.T.: 9.952 min
Delta R.T.: 0.024 min
Response: 38797
Conc: 0.17 ng/ml

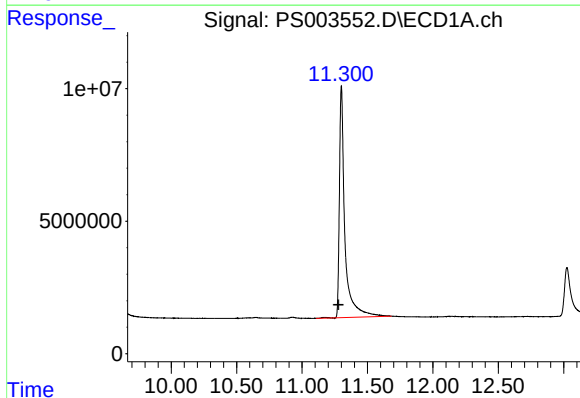


#4 2,4-DCAA

R.T.: 11.300 min
Delta R.T.: 0.022 min
Response: 256567743
Conc: 584.40 ng/ml

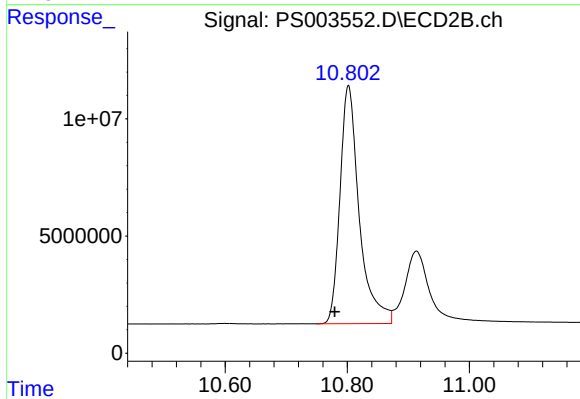

#4 2,4-DCAA


R.T.: 10.802 min
Delta R.T.: 0.022 min
Response: 223117739
Conc: 475.15 ng/ml

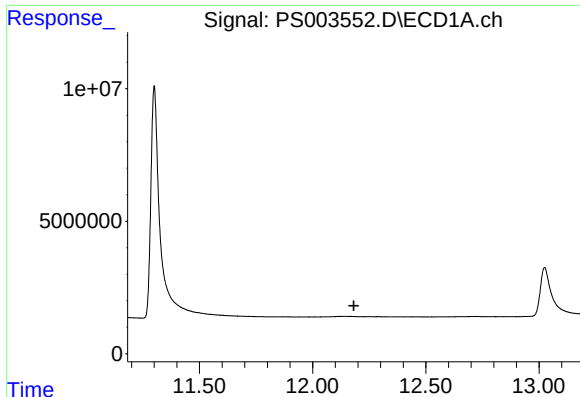

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 12.182 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

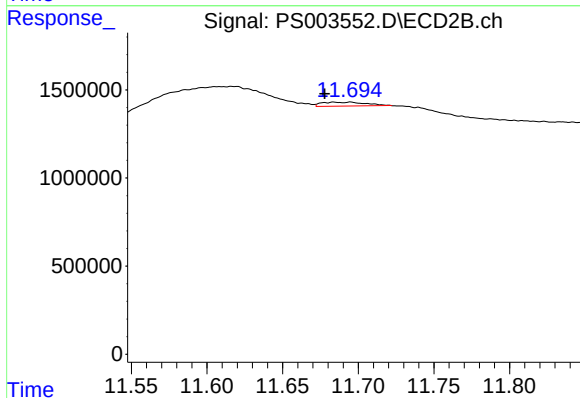


#7 MCPA

R.T.: 11.694 min
Delta R.T.: 0.017 min
Response: 461967
Conc: 0.27 ug/ml

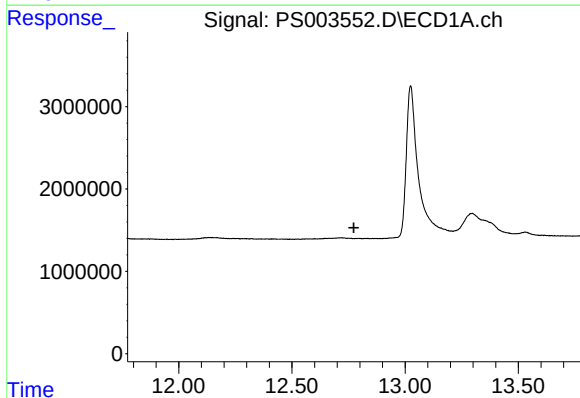


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.773 min
Response: 0
Conc: N.D.

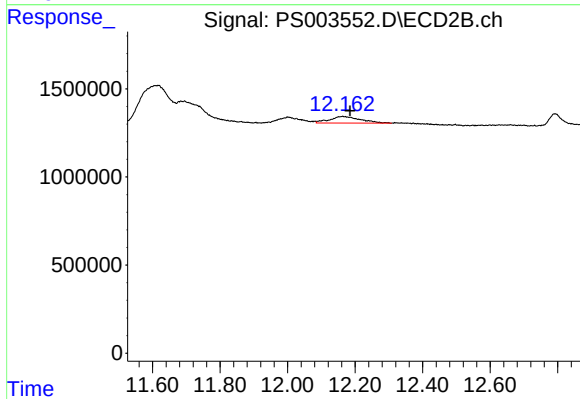

#8 DICHLORPROP


R.T.: 12.163 min
Delta R.T.: -0.022 min
Response: 2385517
Conc: 5.77 ng/ml

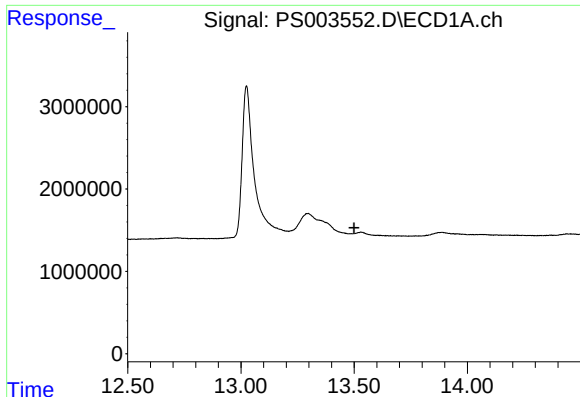

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.499 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

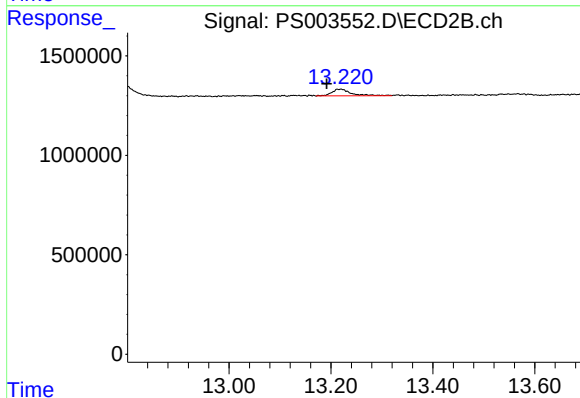


#10 Pentachlorophenol

R.T.: 13.218 min
Delta R.T.: 0.027 min
Response: 904568
Conc: 0.14 ng/ml

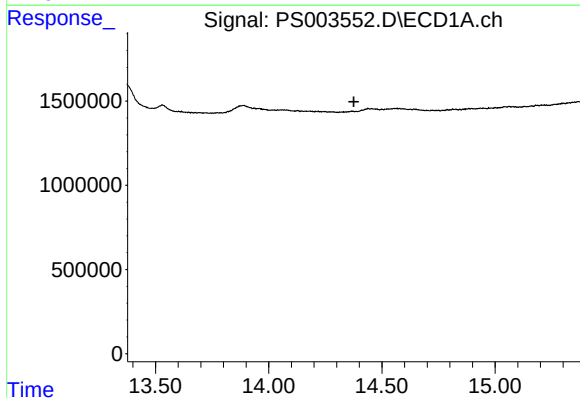


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

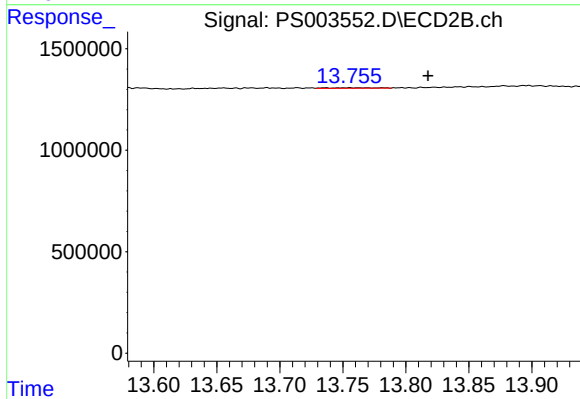

#11 2,4,5-TP (SILVEX)


R.T.: 13.756 min
Delta R.T.: -0.062 min
Response: 62851
Conc: 0.02 ng/ml

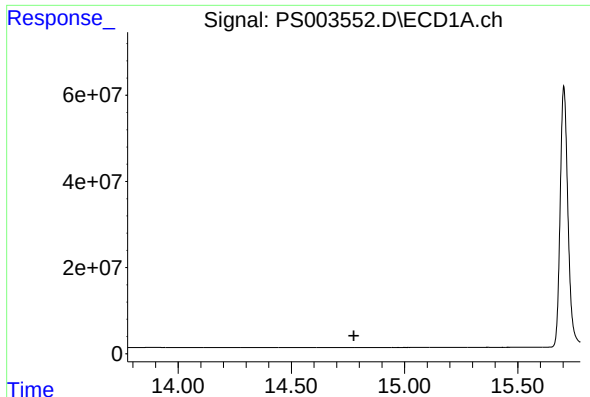

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

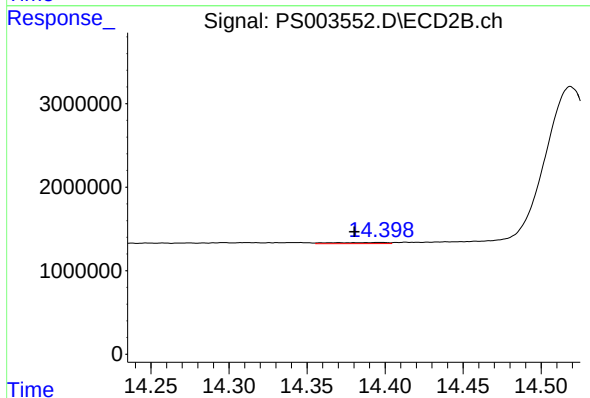


#12 2,4,5-T

R.T.: 14.397 min
Delta R.T.: 0.017 min
Response: 322965
Conc: 0.16 ng/ml

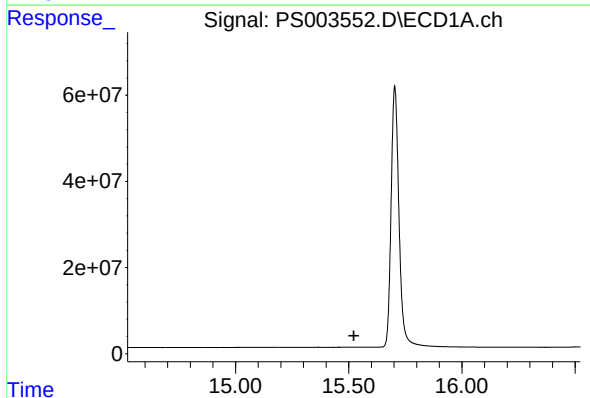


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.523 min
Response: 0
Conc: N.D.

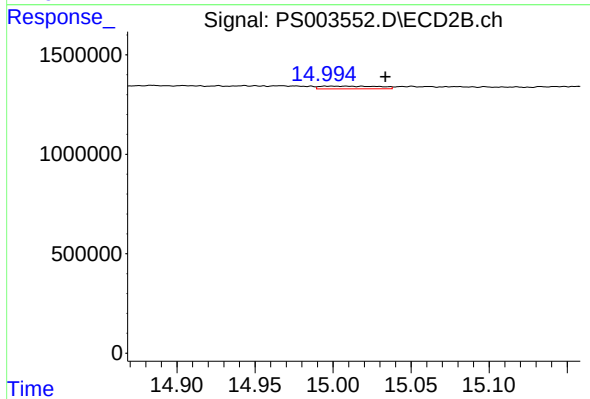

#13 2,4-DB


R.T.: 15.008 min
Delta R.T.: -0.025 min
Response: 354424
Conc: 1.39 ng/ml

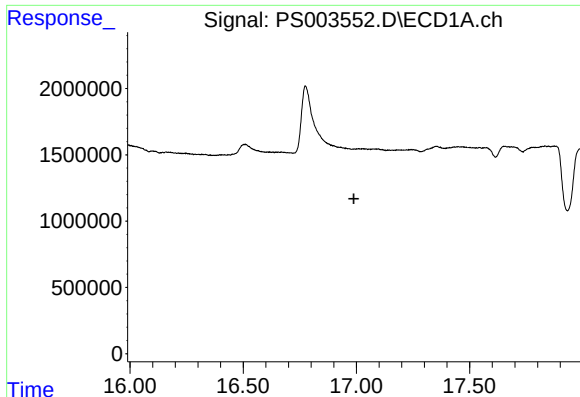

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

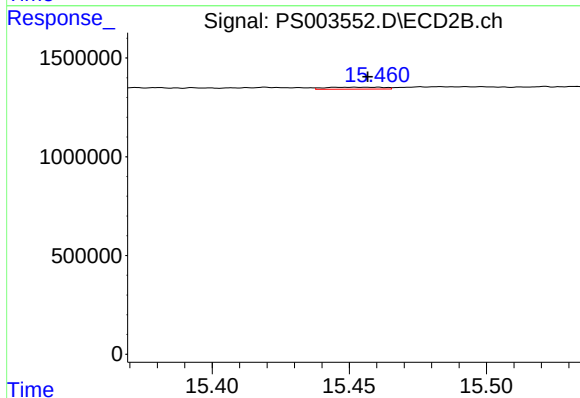


#14 DINOSEB

R.T.: 15.452 min
Delta R.T.: -0.004 min
Response: 140155
Conc: 0.08 ng/ml

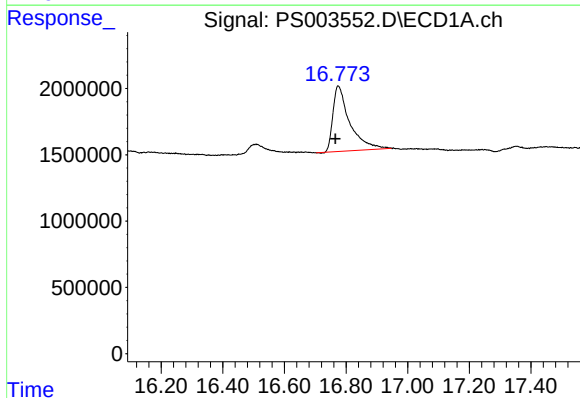


#15 Picloram

R.T.: 16.775 min
Delta R.T.: 0.009 min
Response: 18642178
Conc: 7.57 ng/ml

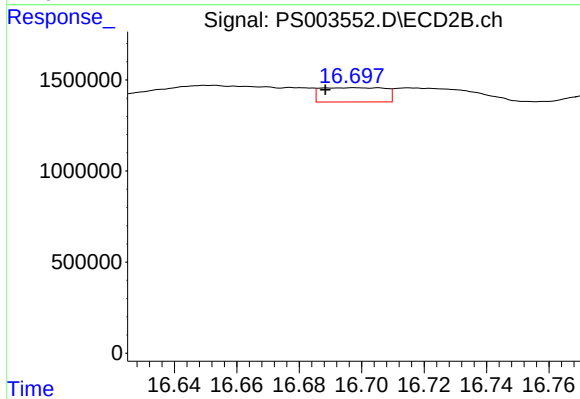

#15 Picloram


R.T.: 16.698 min
Delta R.T.: 0.009 min
Response: 1115754
Conc: 0.44 ng/ml

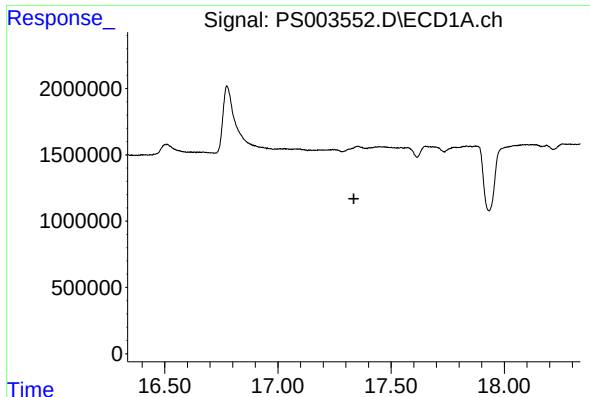

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.335 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

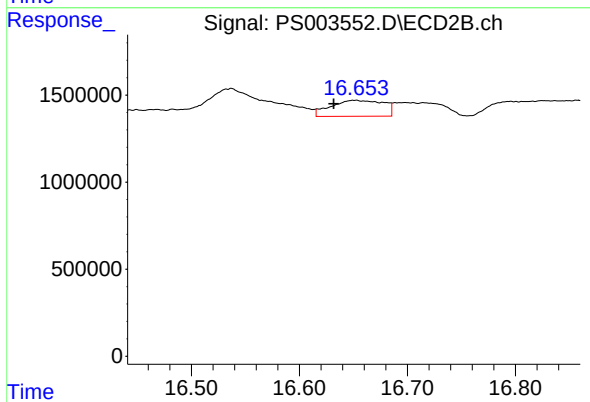

#16 DCPA

R.T.: 16.651 min
Delta R.T.: 0.019 min
Response: 3112997
Conc: 1.00 ng/ml