

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031320\
 Data File : PS009268.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2020 16:36
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 17:55:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.243	6.935	247.1E6	277.0E6	446.706	504.309
Target Compounds							
12) T	2,4,5-T	0.000	9.255	0	7862255	N.D.	2.663
15) T	Picloram	11.039	11.025	24244537	35913266	7.989	8.819
16) T	DCPA	0.000	11.025	0	35913266	N.D.	9.273



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031320\
Data File : PS009268.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2020 16:36
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 17:55:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

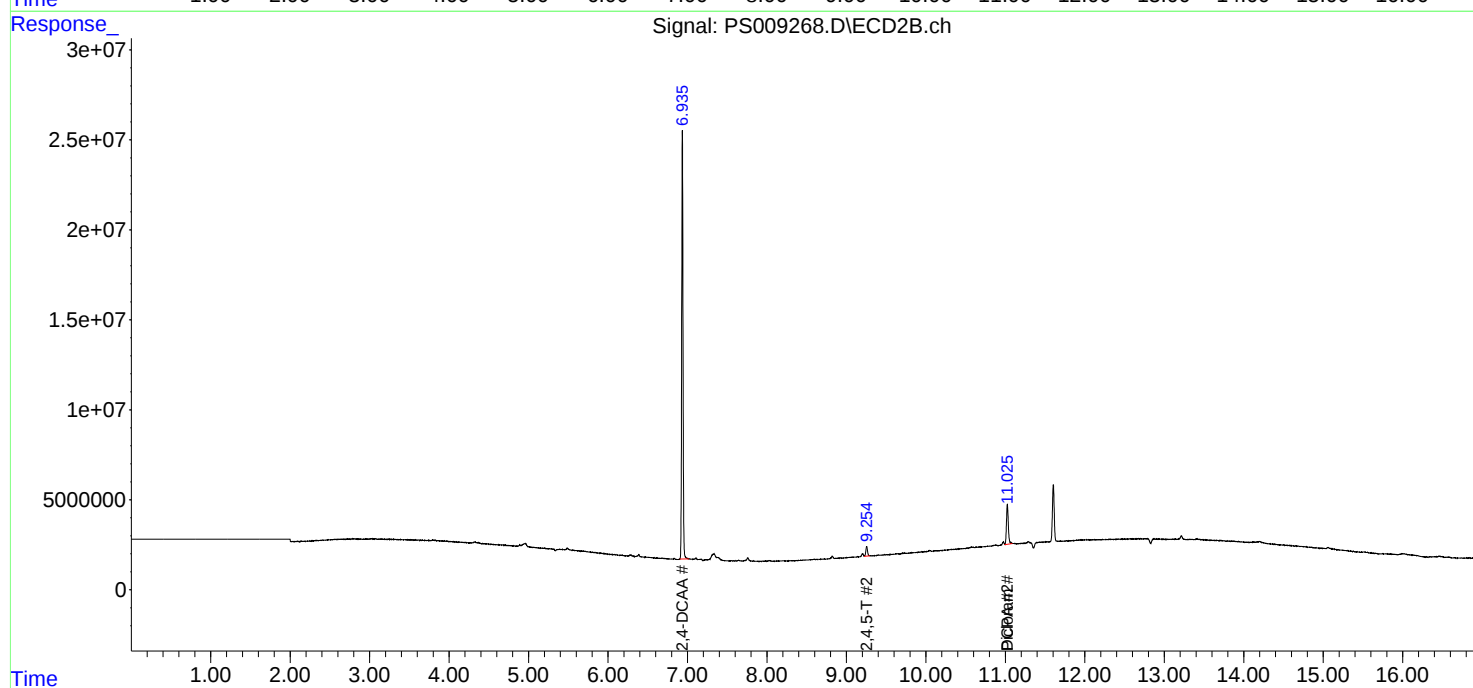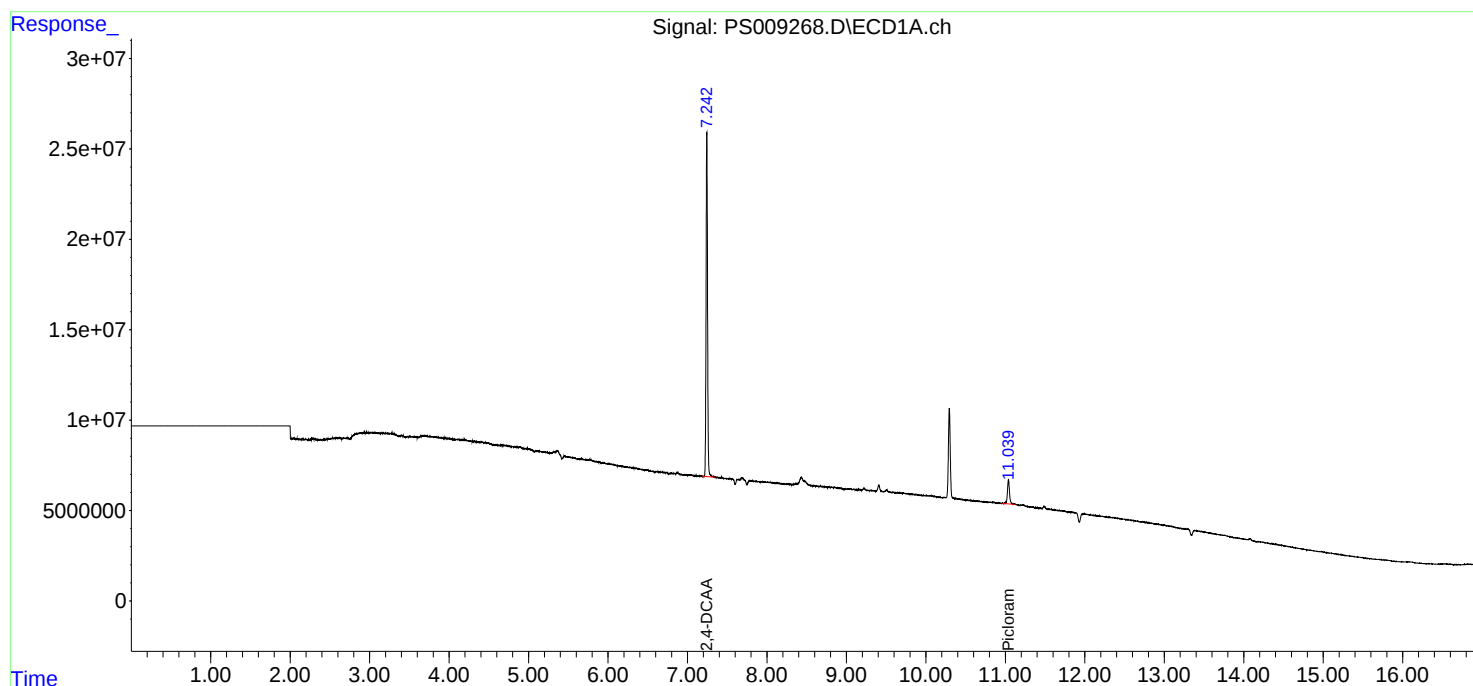


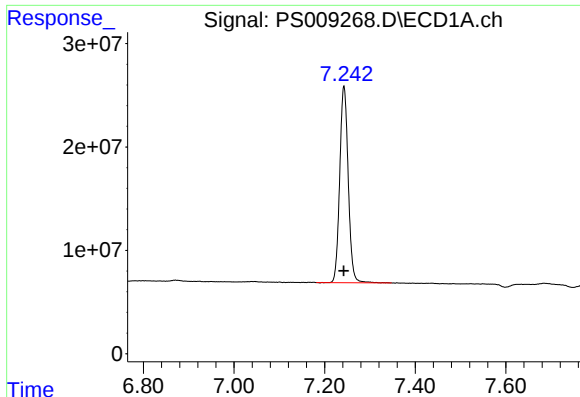

#4 2,4-DCAA


R.T.: 7.243 min
Delta R.T.: 0.000 min
Response: 247104640
Conc: 446.71 ng/ml

Instrument :
ECD_S
ClientSampleId :

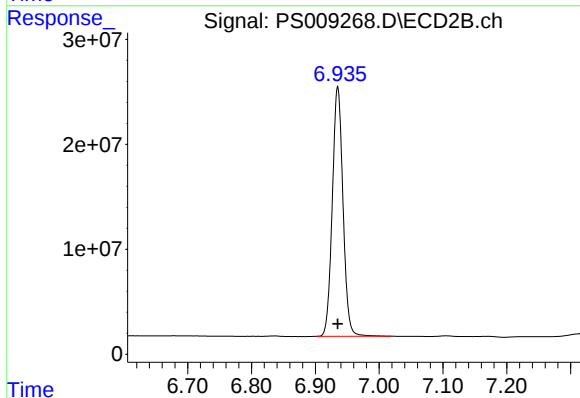


#4 2,4-DCAA

R.T.: 6.935 min
Delta R.T.: 0.000 min
Response: 276965202
Conc: 504.31 ng/ml

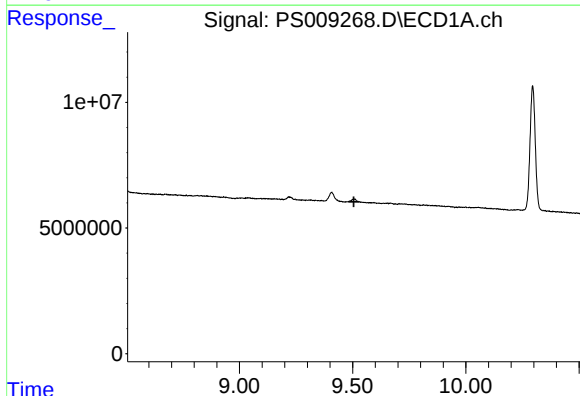


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.505 min
Response: 0
Conc: N.D.

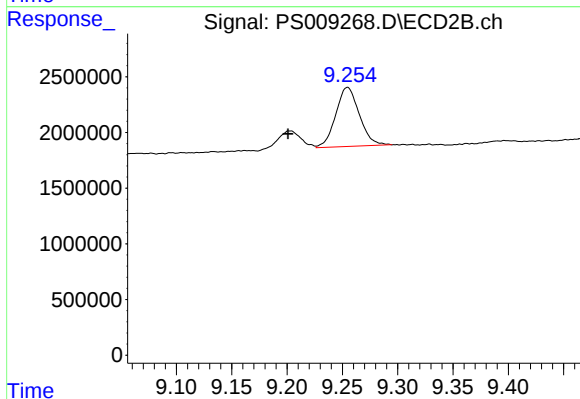

#12 2,4,5-T


R.T.: 9.255 min
Delta R.T.: 0.054 min
Response: 7862255
Conc: 2.66 ng/ml

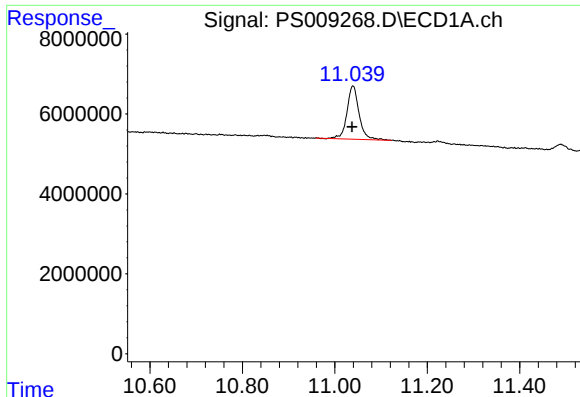

#15 Picloram


R.T.: 11.039 min
Delta R.T.: 0.002 min
Response: 24244537
Conc: 7.99 ng/ml

Instrument :
ECD_S
ClientSampleId :

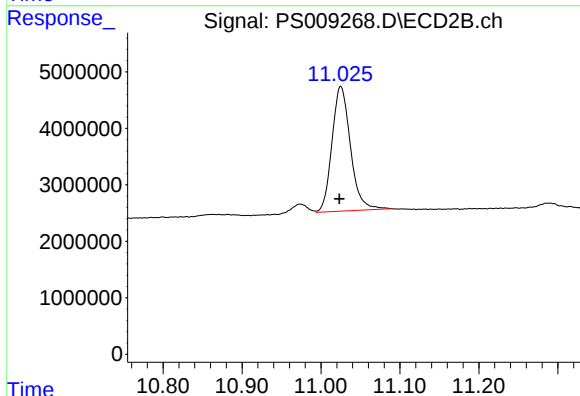


#15 Picloram

R.T.: 11.025 min
Delta R.T.: 0.002 min
Response: 35913266
Conc: 8.82 ng/ml

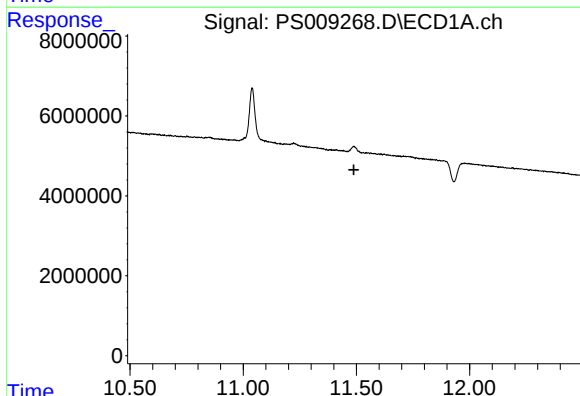

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.489 min
Response: 0
Conc: N.D.

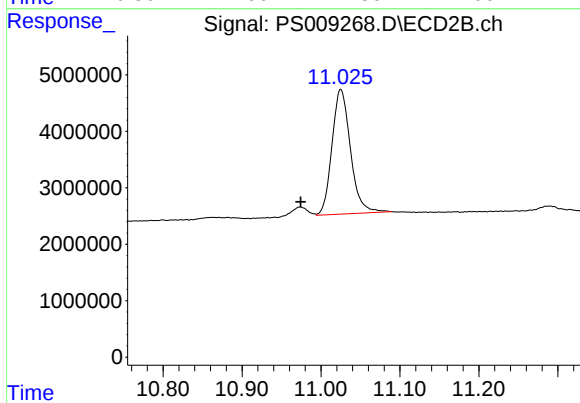

#16 DCPA

R.T.: 11.025 min
Delta R.T.: 0.051 min
Response: 35913266
Conc: 9.27 ng/ml