

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031320\
 Data File : PS009272.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2020 18:08
 Operator : DD\AJ
 Sample : L1752-04
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 01:01:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.242	6.934	229.1E6	231.9E6	414.175	422.281
Target Compounds							
1) T	Dalapon	3.007	2.590	14214711	64035430	18.228	81.329 #
2) T	3,5-DICHL...	0.000	6.110	0	59840888	N.D.	73.577
3) T	4-Nitroph...	7.010	6.592	16235873	10159618	68.014	31.929 #
8) T	DICHLORPROP	8.120	7.754	-626108	45314294	N.D.	81.674
12) T	2,4,5-T	9.445	0.000	28943766	0	11.378	N.D. #
15) T	Picloram	11.037	11.023	13160367	37663565	4.336	9.249 #
16) T	DCPA	0.000	11.023	0	37663565	N.D.	9.725



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031320\
Data File : PS009272.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2020 18:08
Operator : DD\AJ
Sample : L1752-04
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 01:01:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

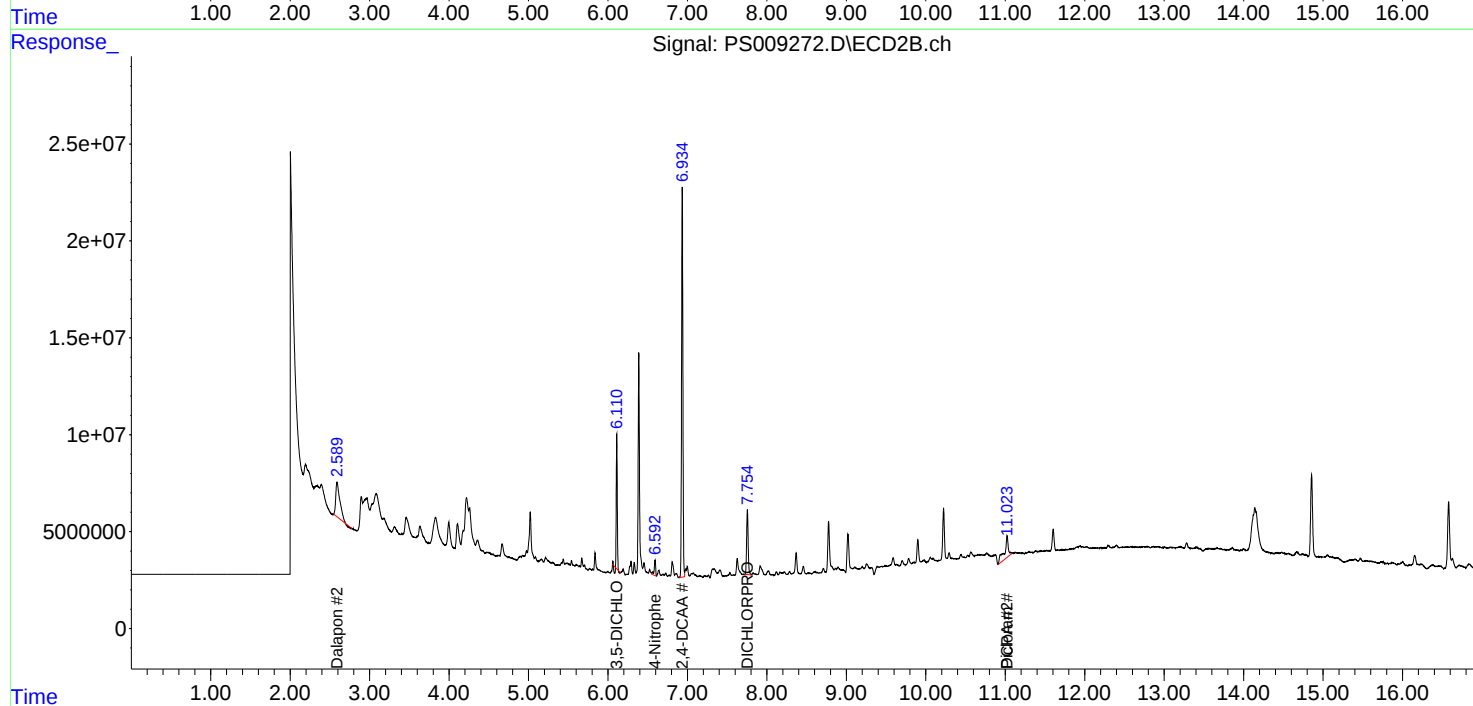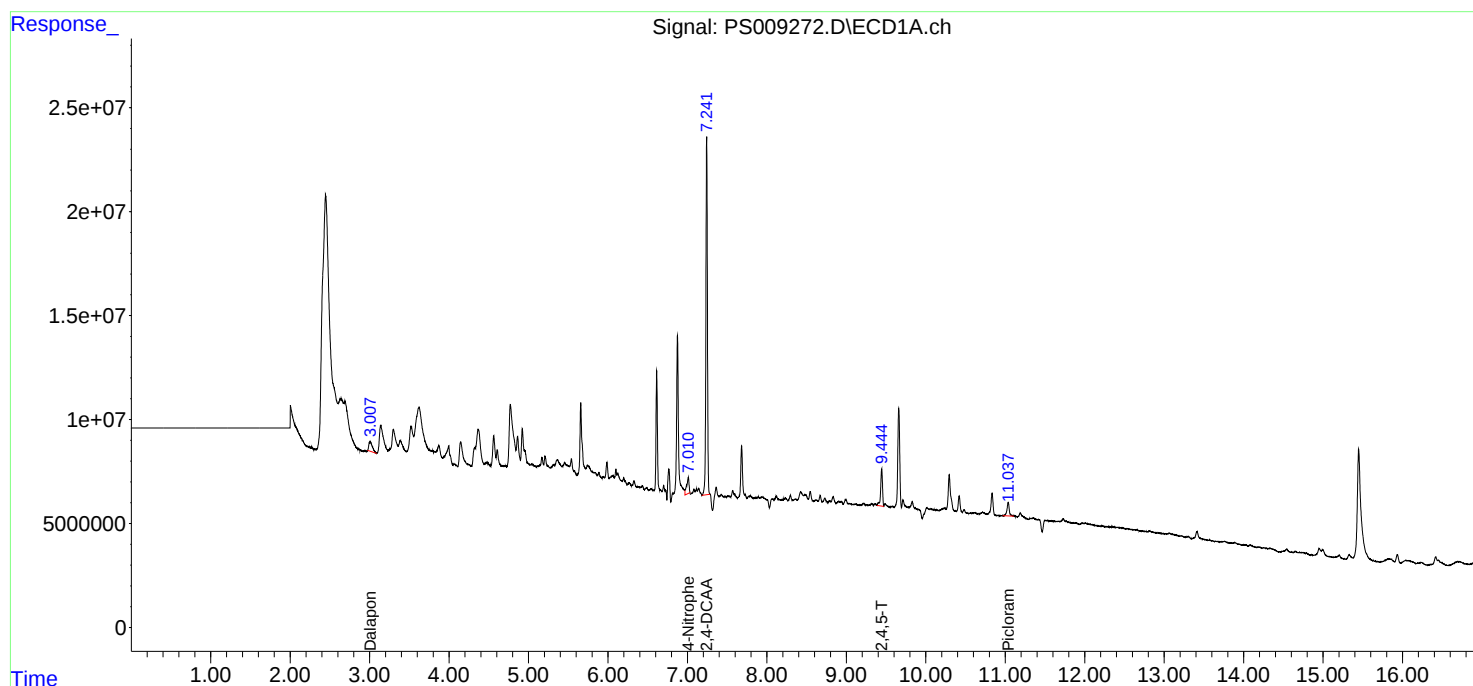


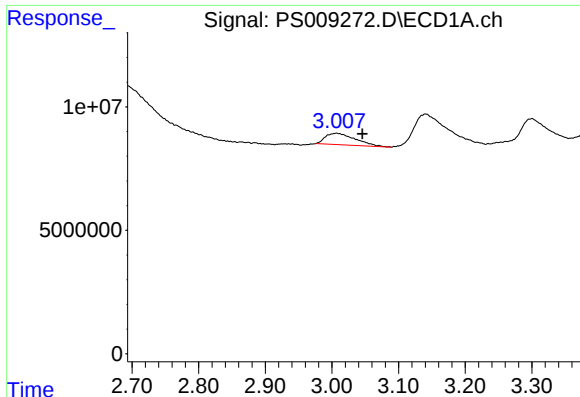

#1 Dalapon


R.T.: 3.007 min
Delta R.T.: -0.039 min
Response: 14214711
Conc: 18.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

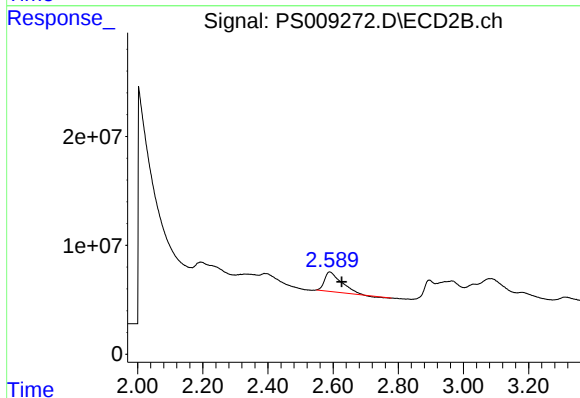


#1 Dalapon

R.T.: 2.590 min
Delta R.T.: -0.037 min
Response: 64035430
Conc: 81.33 ng/ml

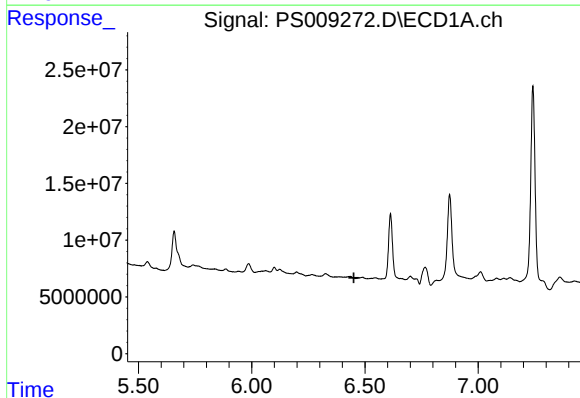


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

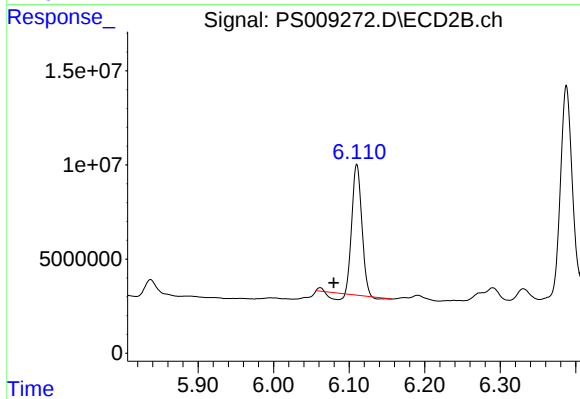

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.110 min
Delta R.T.: 0.031 min
Response: 59840888
Conc: 73.58 ng/ml

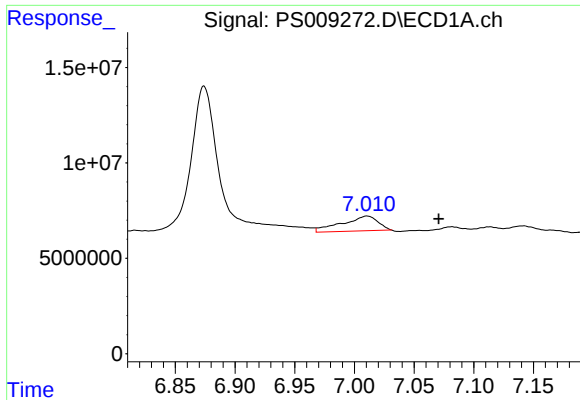

#3 4-Nitrophenol


R.T.: 7.010 min
Delta R.T.: -0.060 min
Response: 16235873
Conc: 68.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

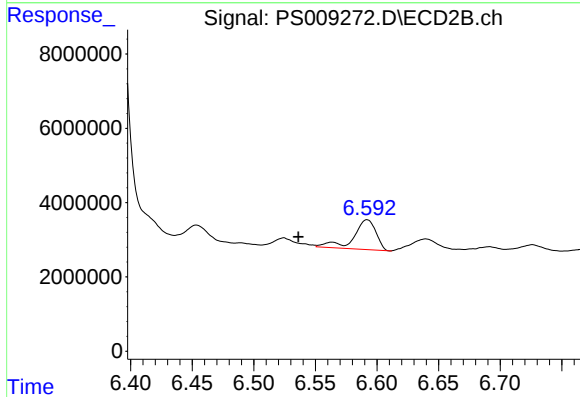


#3 4-Nitrophenol

R.T.: 6.592 min
Delta R.T.: 0.056 min
Response: 10159618
Conc: 31.93 ng/ml

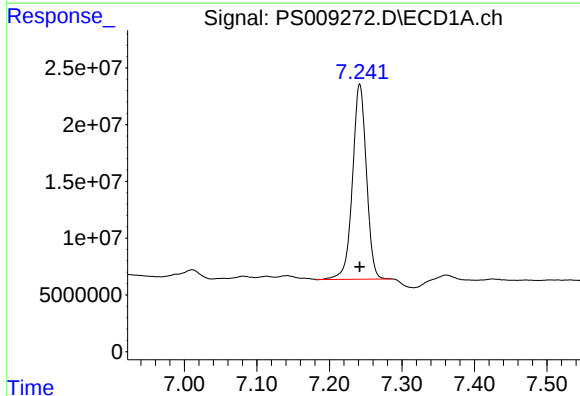


#4 2,4-DCAA

R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 229108964
Conc: 414.17 ng/ml

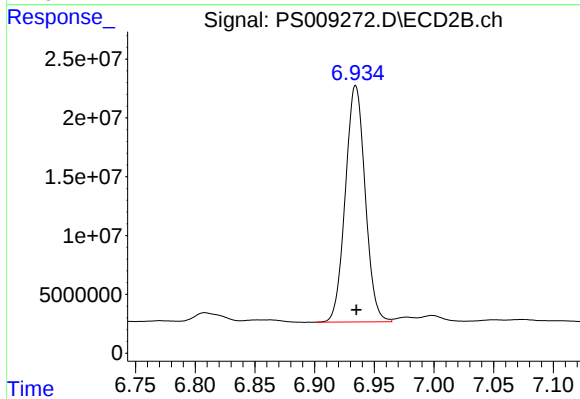

#4 2,4-DCAA


R.T.: 6.934 min
Delta R.T.: 0.000 min
Response: 231915920
Conc: 422.28 ng/ml

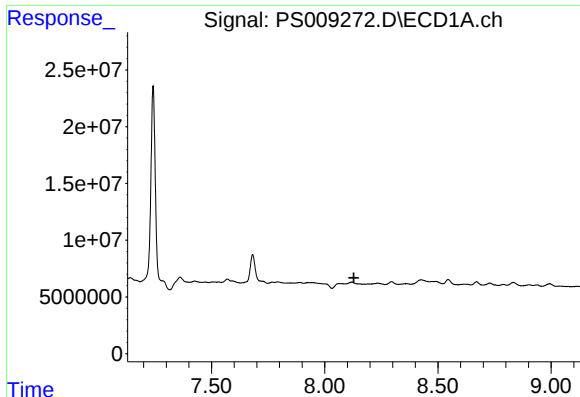

#8 DICHLORPROP


R.T.: 8.120 min
Delta R.T.: -0.009 min
Response: -626108
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

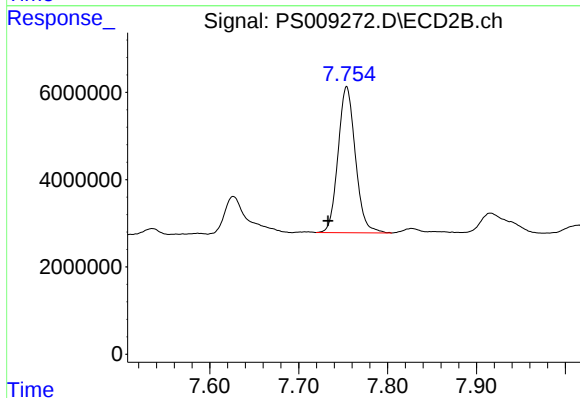


#8 DICHLORPROP

R.T.: 7.754 min
Delta R.T.: 0.021 min
Response: 45314294
Conc: 81.67 ng/ml

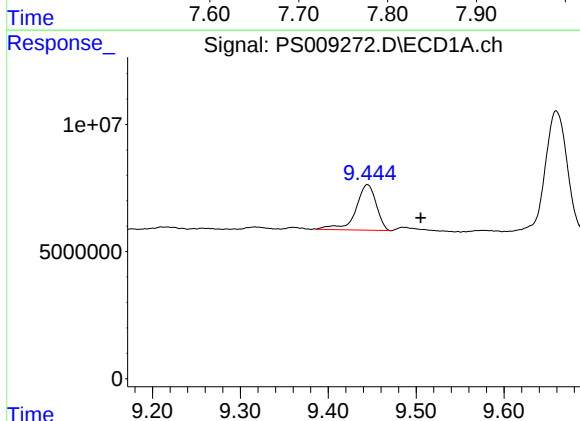


#12 2,4,5-T

R.T.: 9.445 min
Delta R.T.: -0.060 min
Response: 28943766
Conc: 11.38 ng/ml

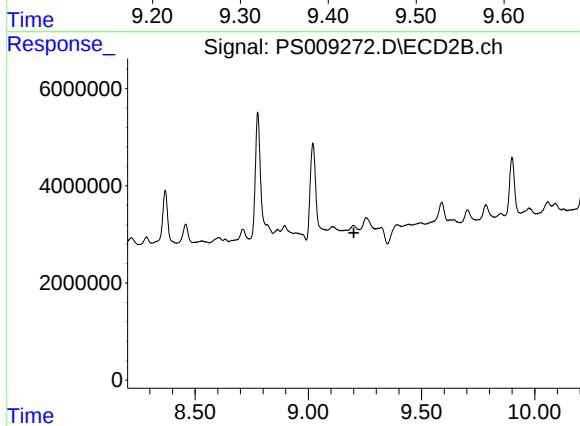

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.201 min
Response: 0
Conc: N.D.

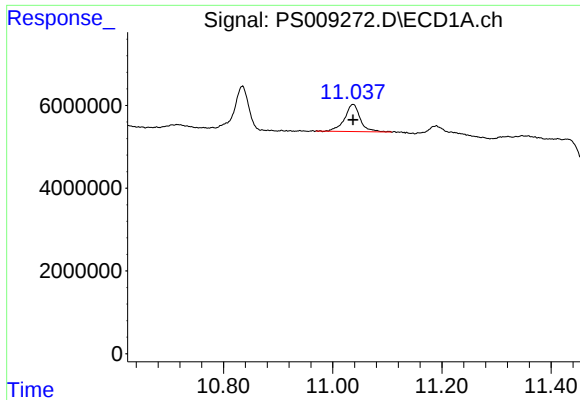

#15 Picloram


R.T.: 11.037 min
Delta R.T.: 0.000 min
Response: 13160367
Conc: 4.34 ng/ml

Instrument :
ECD_S
ClientSampleId :

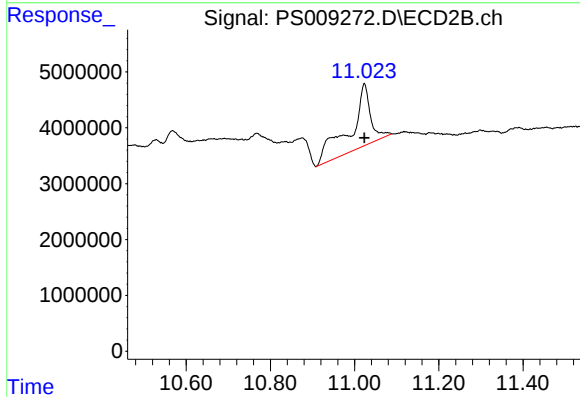


#15 Picloram

R.T.: 11.023 min
Delta R.T.: 0.000 min
Response: 37663565
Conc: 9.25 ng/ml

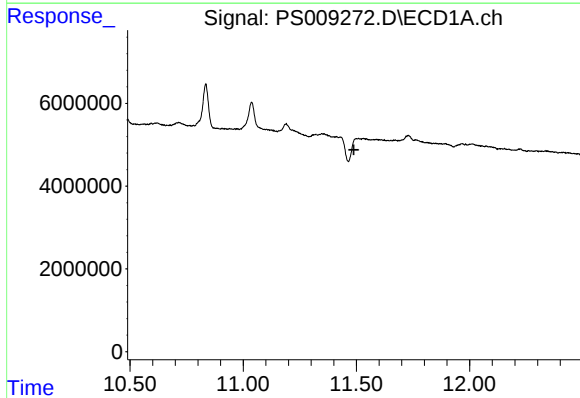

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.489 min
Response: 0
Conc: N.D.

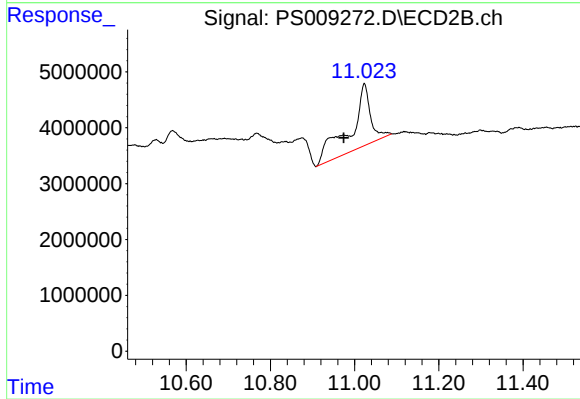

#16 DCPA

R.T.: 11.023 min
Delta R.T.: 0.049 min
Response: 37663565
Conc: 9.72 ng/ml