

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031320\
 Data File : PS009276.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2020 19:39
 Operator : DD\AJ
 Sample : L1893-04
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 01:02:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.242	6.934	232.6E6	231.2E6	420.555	421.059
Target Compounds							
1) T	Dalapon	3.006	2.591	14553219	95346784	18.662	121.096 #
2) T	3,5-DICHL...	0.000	6.110	0	62662718	N.D.	77.047
3) T	4-Nitroph...	7.010	6.592	14283595	8402424	59.836	26.406 #
8) T	DICHLORPROP	8.118	7.754	-2267196	37005517	N.D.	66.698
9) T	2,4-D	8.427	0.000	5465062	0	10.366	N.D. #
12) T	2,4,5-T	9.443	0.000	18533615	0	7.286	N.D. #
15) T	Picloram	0.000	11.024	0	25138872	N.D.	6.173
16) T	DCPA	0.000	11.024	0	25138872	N.D.	6.491



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031320\
Data File : PS009276.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2020 19:39
Operator : DD\AJ
Sample : L1893-04
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 01:02:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

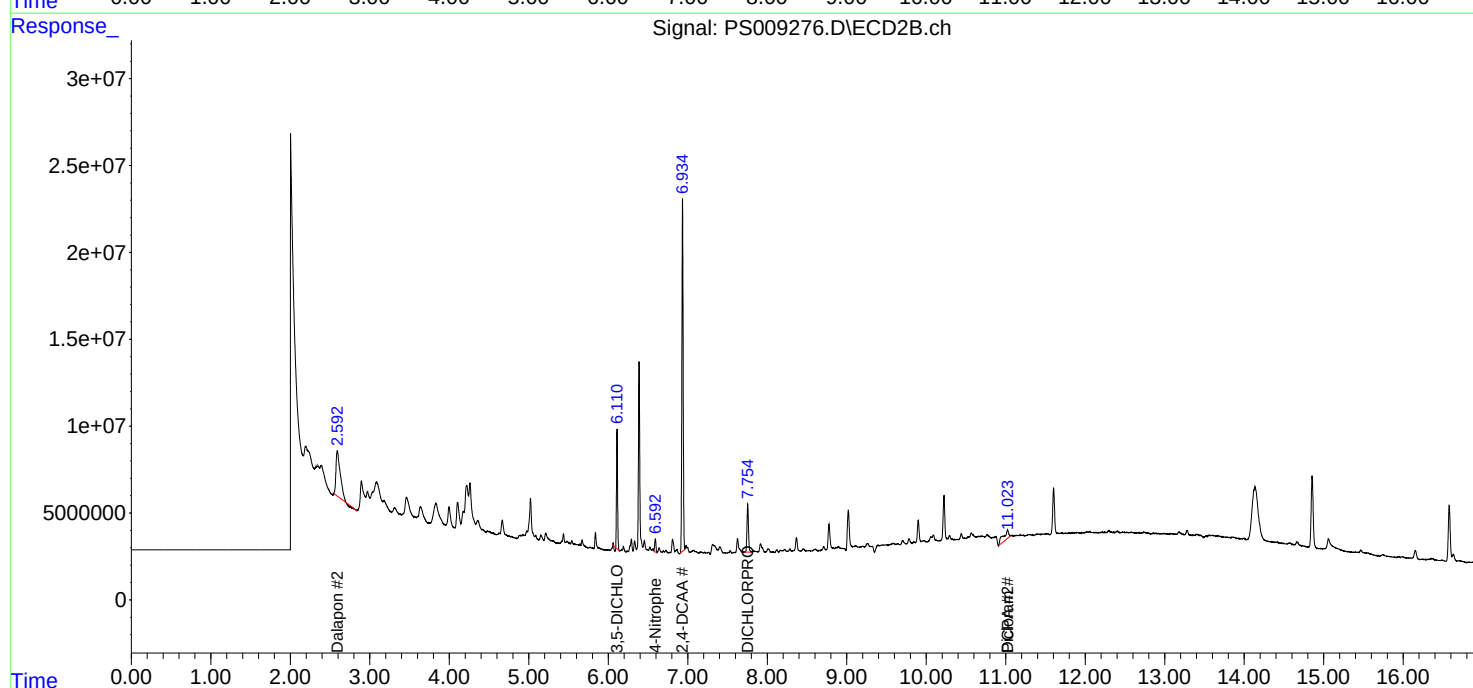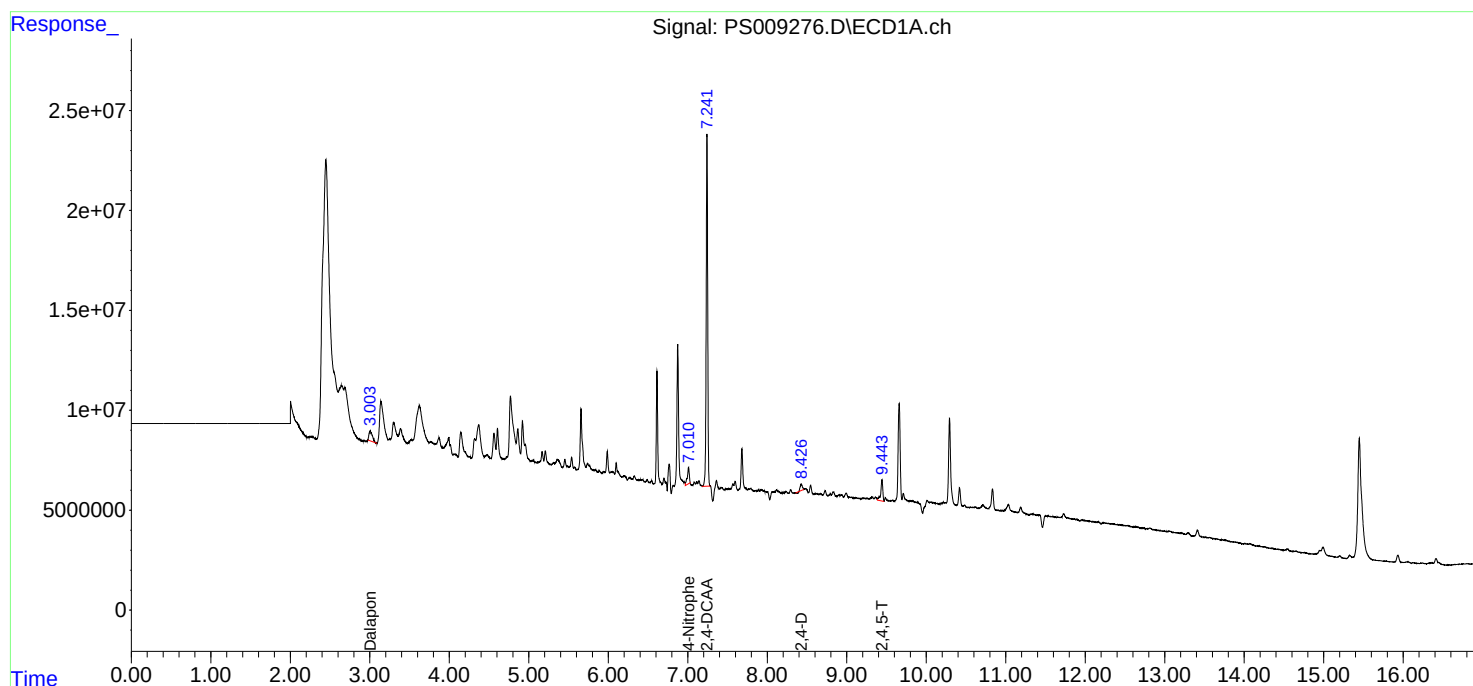


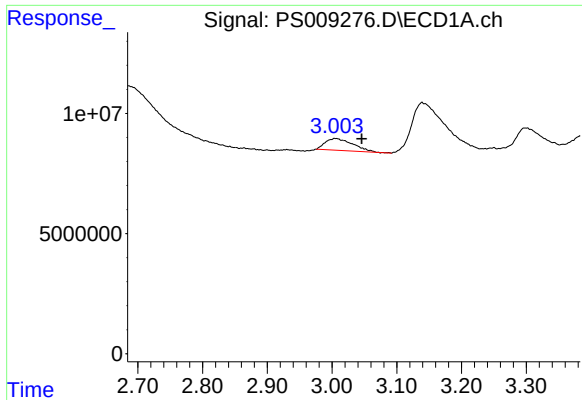

#1 Dalapon


R.T.: 3.006 min
Delta R.T.: -0.040 min
Response: 14553219
Conc: 18.66 ng/ml

Instrument :
ECD_S
ClientSampleId :

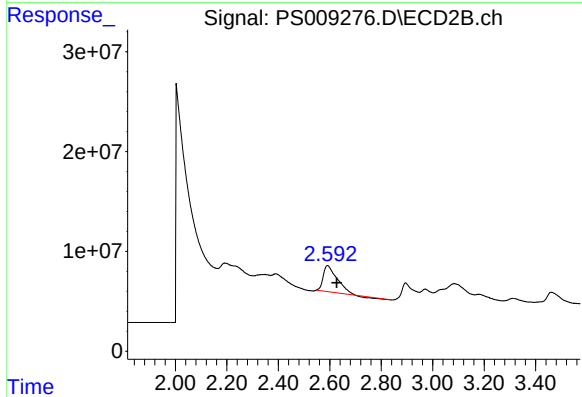


#1 Dalapon

R.T.: 2.591 min
Delta R.T.: -0.035 min
Response: 95346784
Conc: 121.10 ng/ml

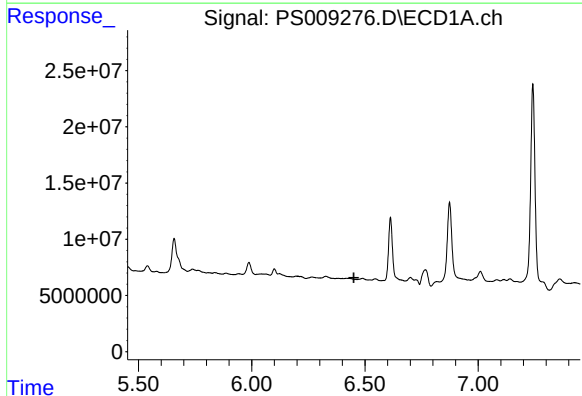


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

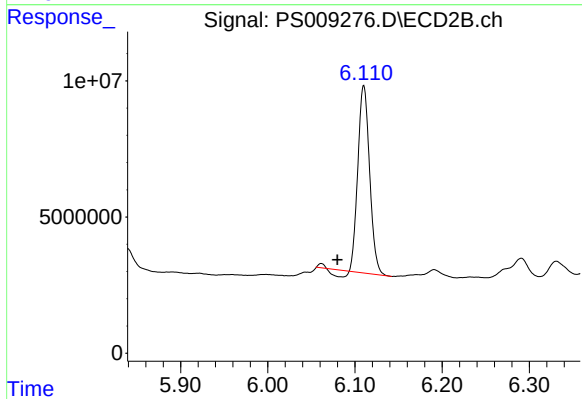

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.110 min
Delta R.T.: 0.030 min
Response: 62662718
Conc: 77.05 ng/ml

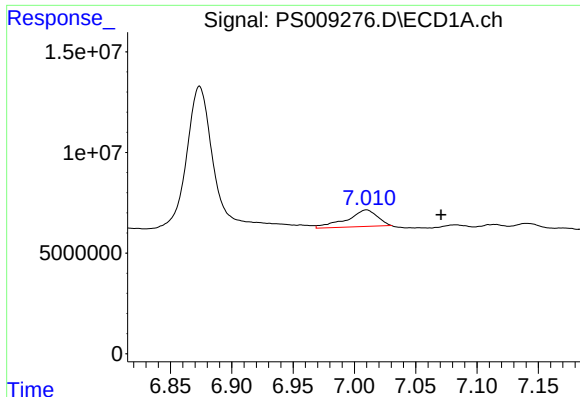

#3 4-Nitrophenol


R.T.: 7.010 min
Delta R.T.: -0.061 min
Response: 14283595
Conc: 59.84 ng/ml

Instrument :
ECD_S
ClientSampleId :

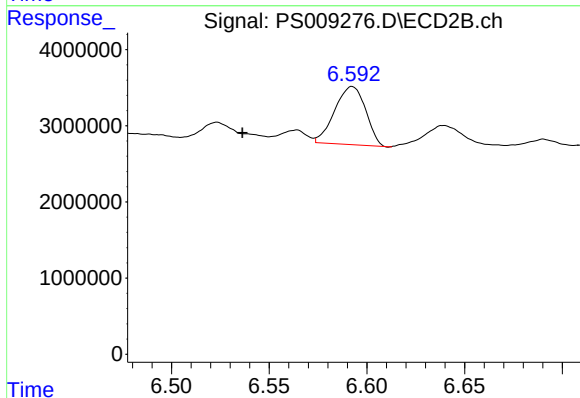


#3 4-Nitrophenol

R.T.: 6.592 min
Delta R.T.: 0.056 min
Response: 8402424
Conc: 26.41 ng/ml

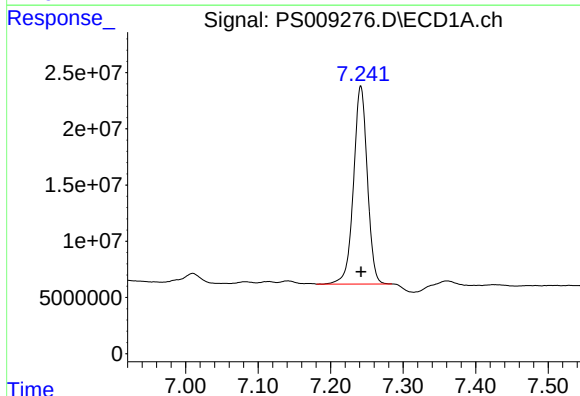


#4 2,4-DCAA

R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 232638313
Conc: 420.55 ng/ml

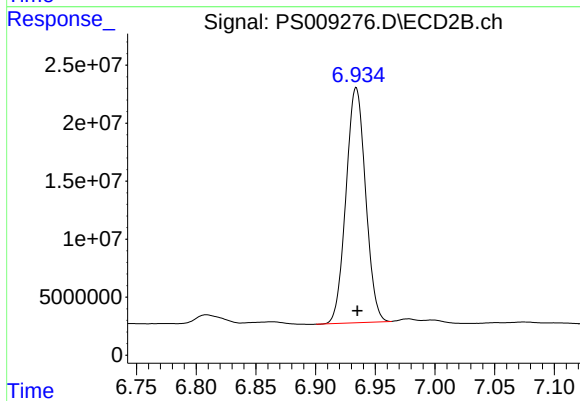

#4 2,4-DCAA


R.T.: 6.934 min
Delta R.T.: -0.001 min
Response: 231244865
Conc: 421.06 ng/ml

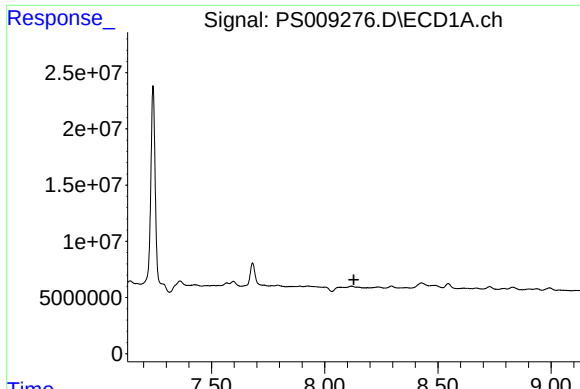

#8 DICHLORPROP


R.T.: 8.118 min
Delta R.T.: -0.011 min
Response: -2267196
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

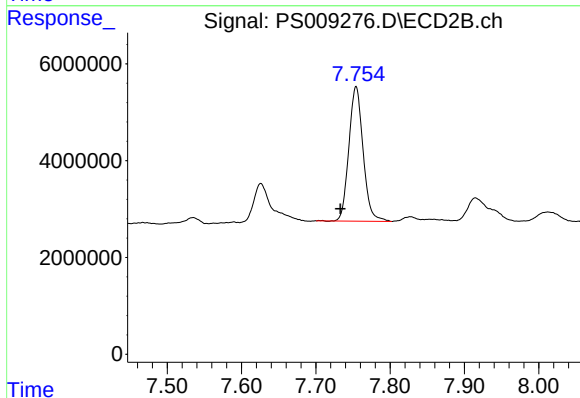


#8 DICHLORPROP

R.T.: 7.754 min
Delta R.T.: 0.021 min
Response: 37005517
Conc: 66.70 ng/ml

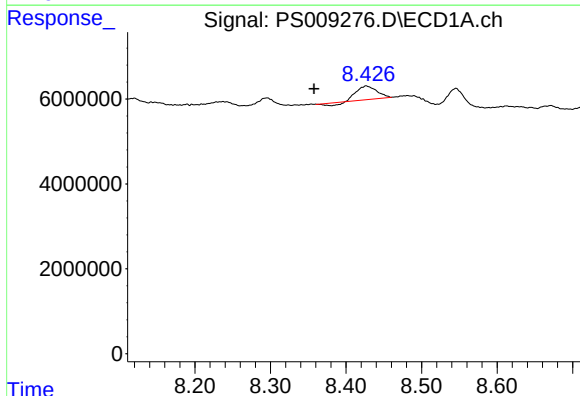


#9 2,4-D

R.T.: 8.427 min
Delta R.T.: 0.069 min
Response: 5465062
Conc: 10.37 ng/ml

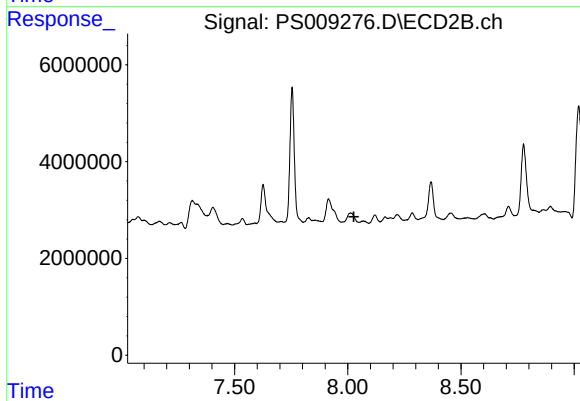

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.027 min
Response: 0
Conc: N.D.

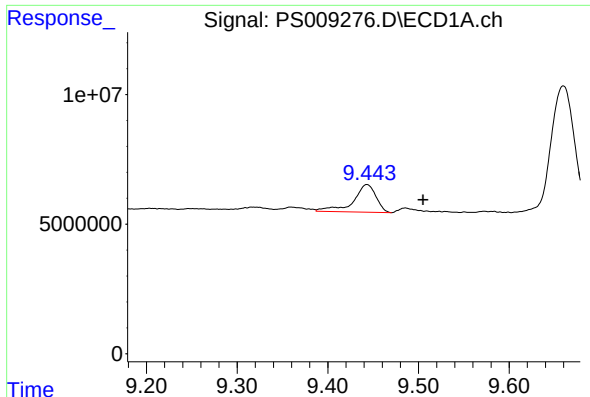

#12 2,4,5-T


R.T.: 9.443 min
Delta R.T.: -0.062 min
Response: 18533615
Conc: 7.29 ng/ml

Instrument :
ECD_S
ClientSampleId :

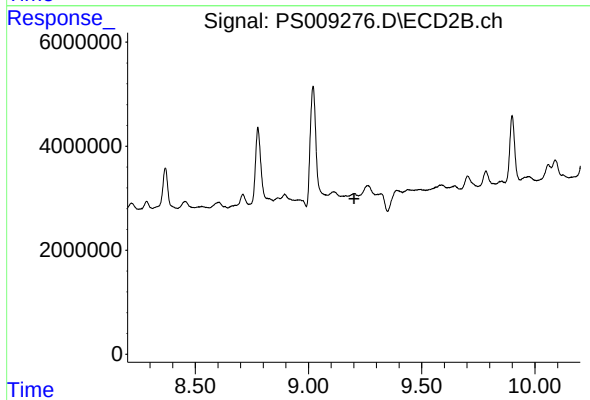


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.201 min
Response: 0
Conc: N.D.

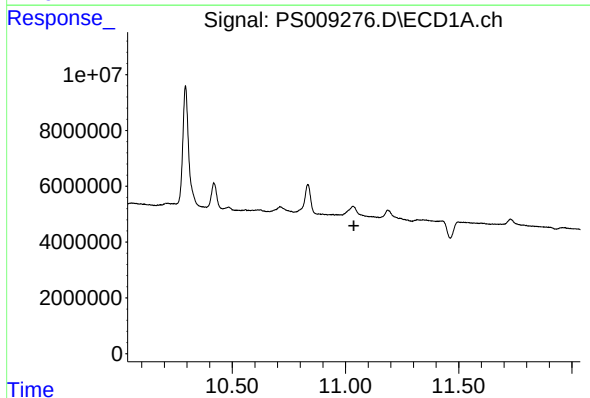


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.037 min
Response: 0
Conc: N.D.

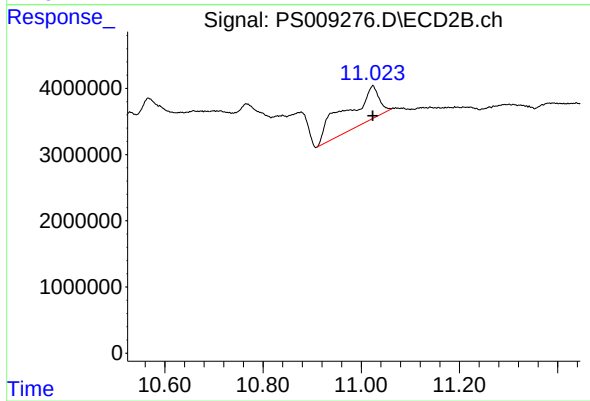

#15 Picloram


R.T.: 11.024 min
Delta R.T.: 0.000 min
Response: 25138872
Conc: 6.17 ng/ml

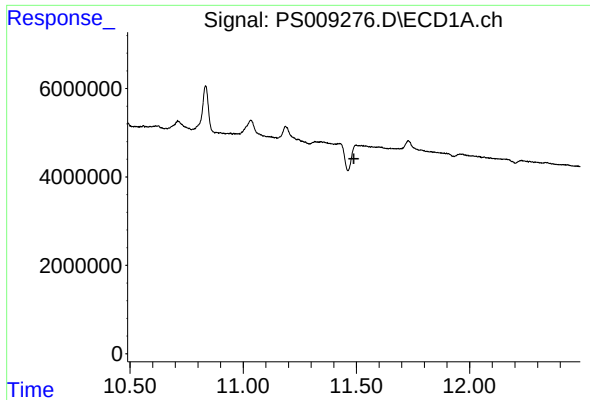

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.489 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

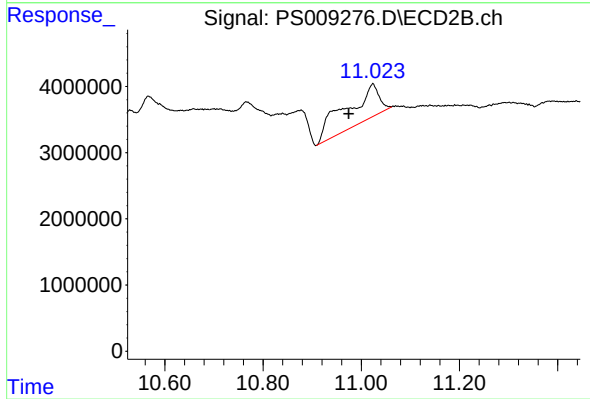

#16 DCPA

R.T.: 11.024 min
Delta R.T.: 0.049 min
Response: 25138872
Conc: 6.49 ng/ml