

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031320\
 Data File : PS009277.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2020 20:02
 Operator : DD\AJ
 Sample : L1893-08
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 01:03:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.242	6.934	253.4E6	250.6E6	458.081	456.228
Target Compounds							
1) T	Dalapon	3.004	2.589	14620507	92658479	18.748	117.682 #
2) T	3,5-DICHL...	0.000	6.110	0	64892140	N.D.	79.788
3) T	4-Nitroph...	7.010	6.592	18851674	11418214	78.972	35.884 #
8) T	DICHLORPROP	8.117	7.753	-2948	35939174	N.D.	64.776
9) T	2,4-D	8.295	0.000	6590380	0	12.500	N.D. #
12) T	2,4,5-T	9.443	0.000	14038028	0	5.518	N.D. #
15) T	Picloram	0.000	11.024	0	26586726	N.D.	6.529
16) T	DCPA	0.000	11.024	0	26586726	N.D.	6.865



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031320\
Data File : PS009277.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2020 20:02
Operator : DD\AJ
Sample : L1893-08
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 01:03:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

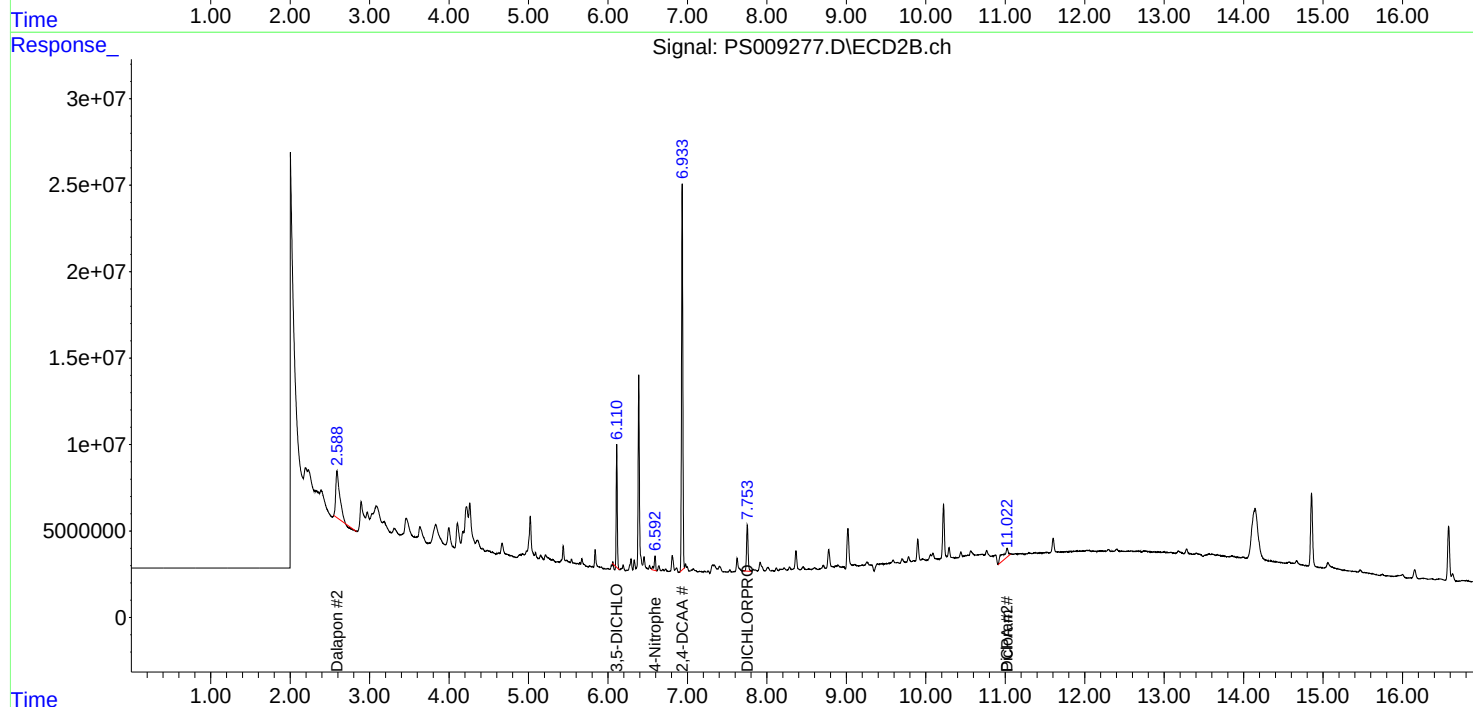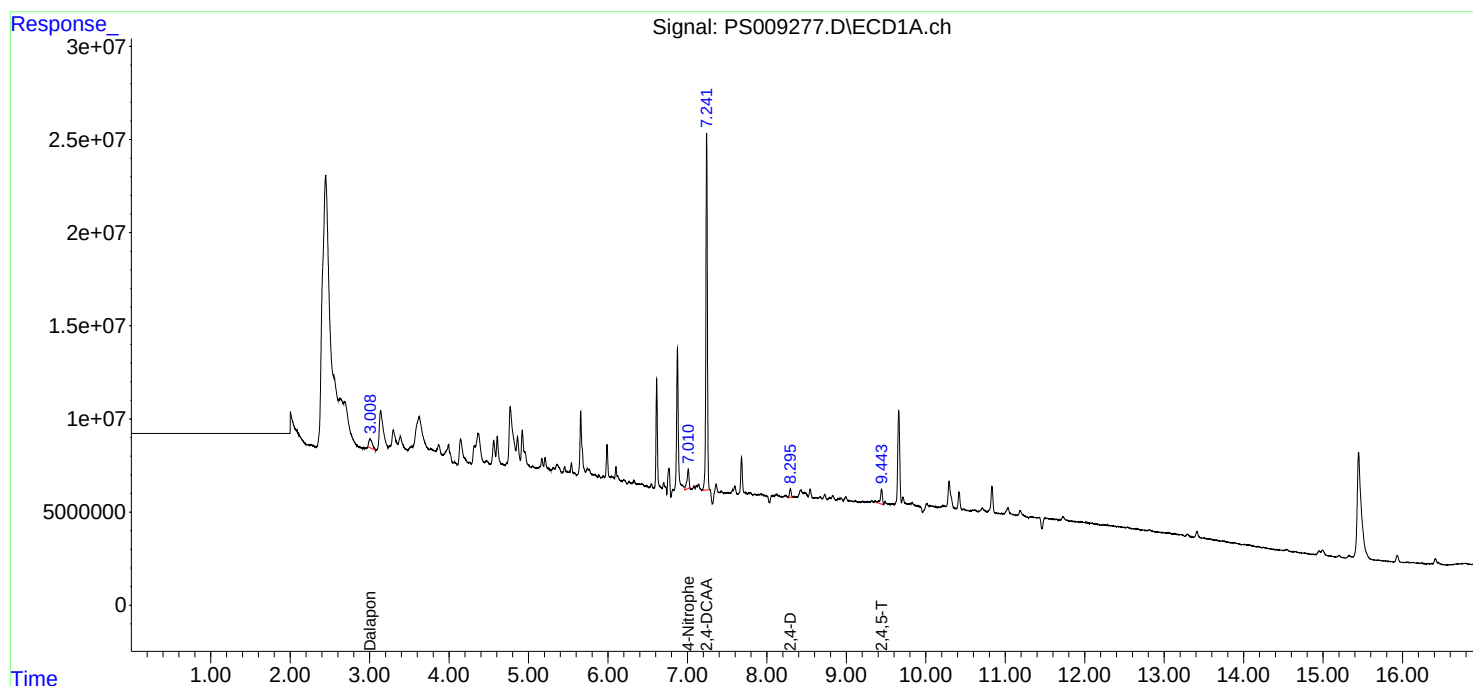


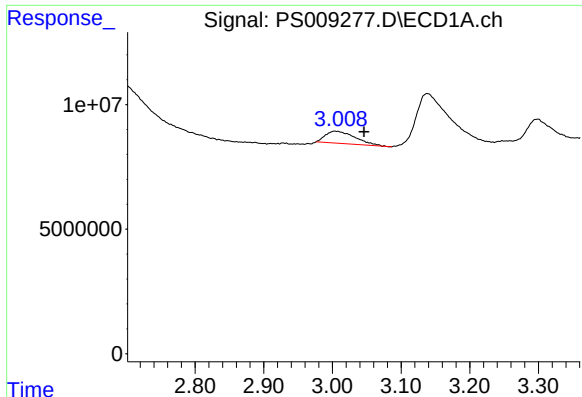

#1 Dalapon


R.T.: 3.004 min
Delta R.T.: -0.042 min
Response: 14620507
Conc: 18.75 ng/ml

Instrument :
ECD_S
ClientSampleId :

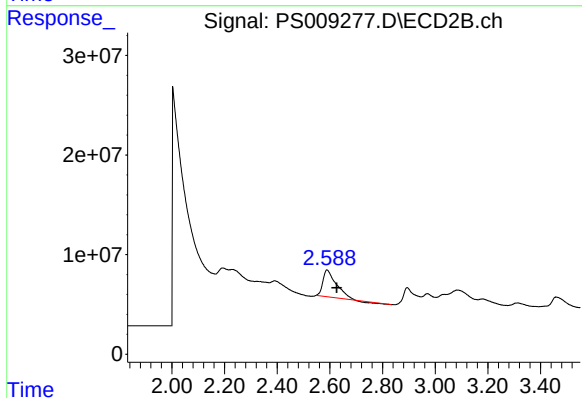


#1 Dalapon

R.T.: 2.589 min
Delta R.T.: -0.037 min
Response: 92658479
Conc: 117.68 ng/ml

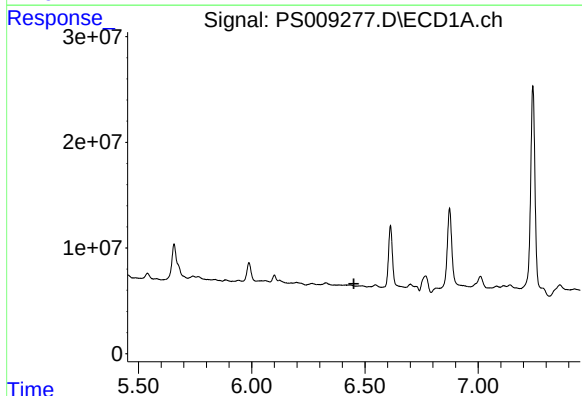


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

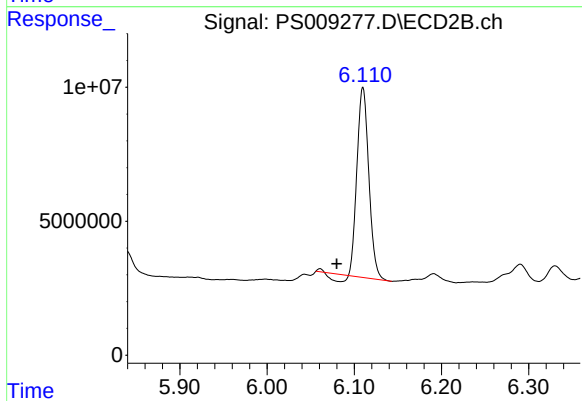

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.110 min
Delta R.T.: 0.030 min
Response: 64892140
Conc: 79.79 ng/ml

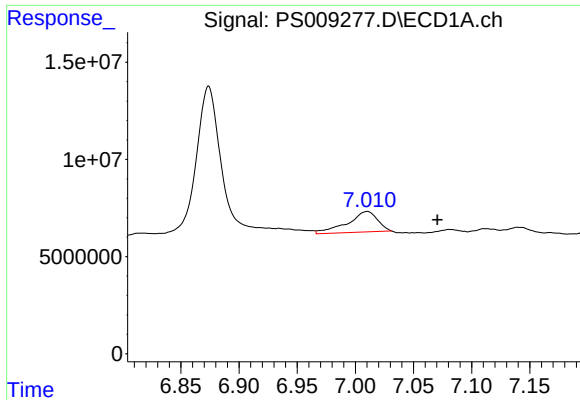

#3 4-Nitrophenol


R.T.: 7.010 min
Delta R.T.: -0.061 min
Response: 18851674
Conc: 78.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

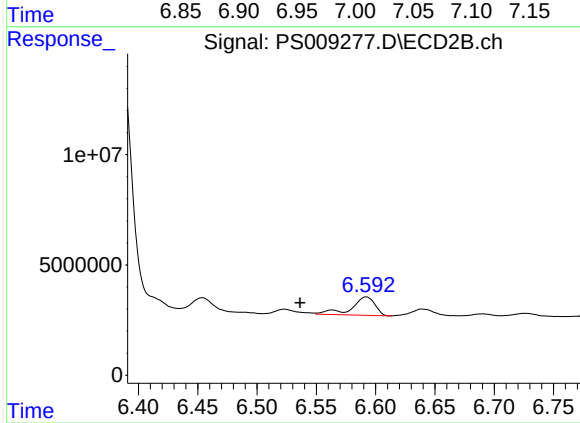


#3 4-Nitrophenol

R.T.: 6.592 min
Delta R.T.: 0.056 min
Response: 11418214
Conc: 35.88 ng/ml

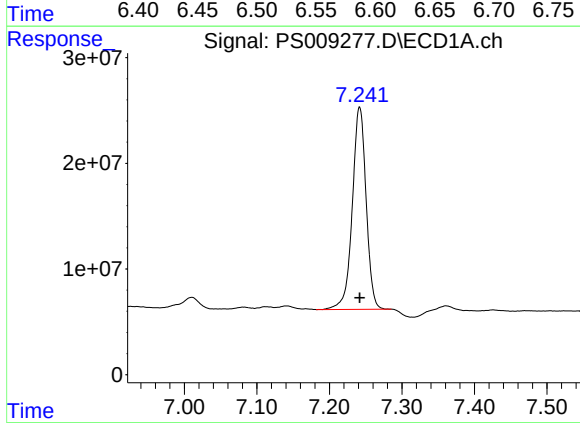


#4 2,4-DCAA

R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 253396900
Conc: 458.08 ng/ml

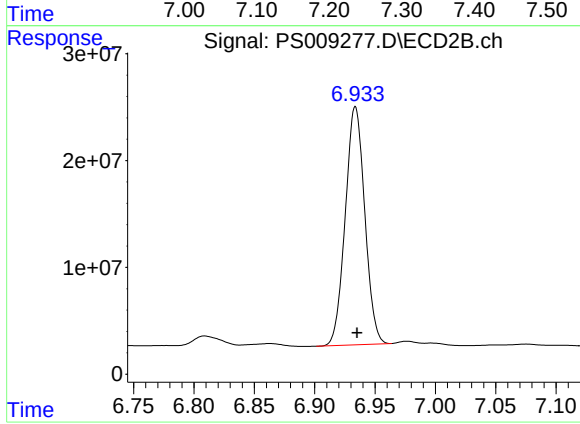

#4 2,4-DCAA


R.T.: 6.934 min
Delta R.T.: -0.001 min
Response: 250559168
Conc: 456.23 ng/ml

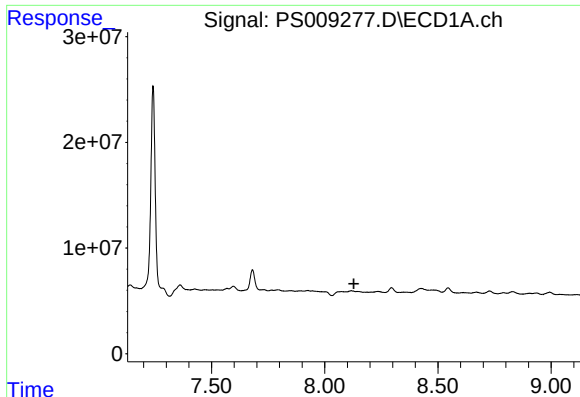

#8 DICHLORPROP


R.T.: 8.117 min
Delta R.T.: -0.012 min
Response: -2948
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

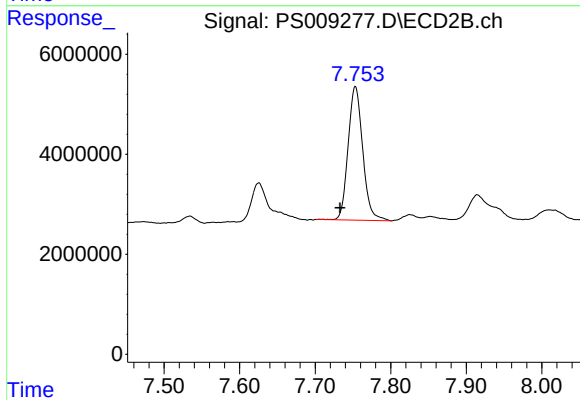


#8 DICHLORPROP

R.T.: 7.753 min
Delta R.T.: 0.020 min
Response: 35939174
Conc: 64.78 ng/ml

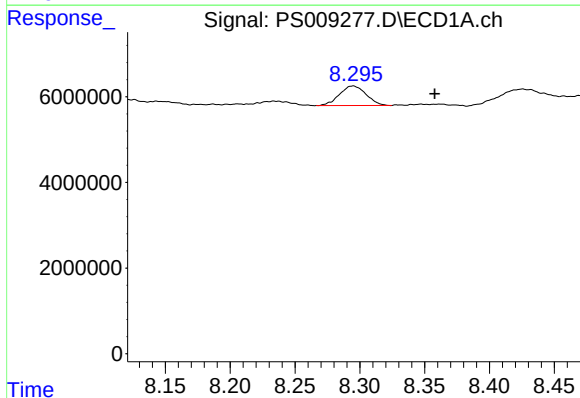


#9 2,4-D

R.T.: 8.295 min
Delta R.T.: -0.063 min
Response: 6590380
Conc: 12.50 ng/ml

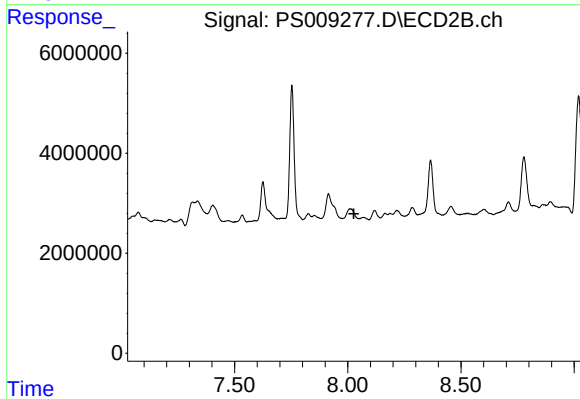

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.027 min
Response: 0
Conc: N.D.

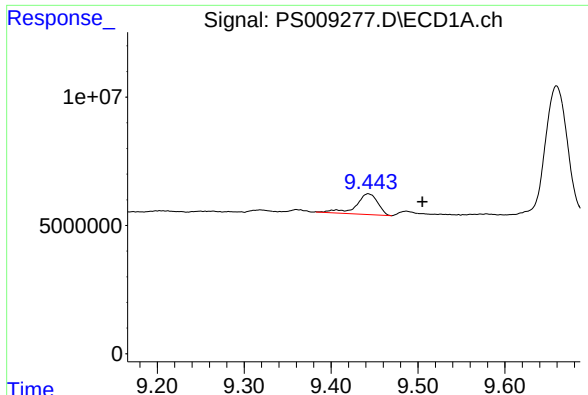

#12 2,4,5-T


R.T.: 9.443 min
Delta R.T.: -0.062 min
Response: 14038028
Conc: 5.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

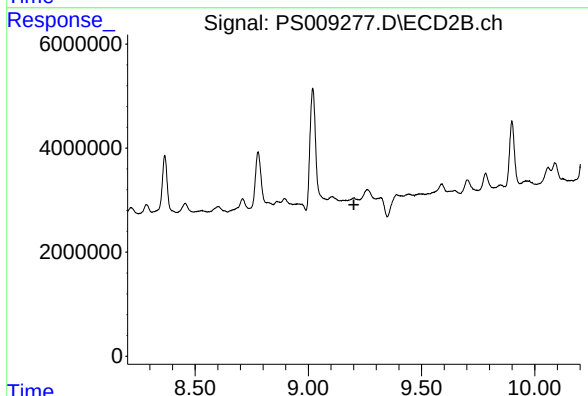


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.201 min
Response: 0
Conc: N.D.

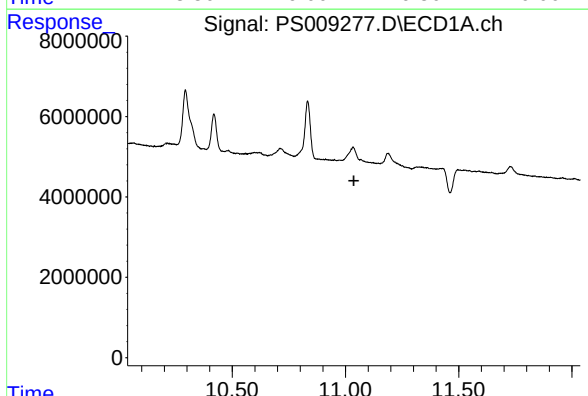


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.037 min
Response: 0
Conc: N.D.

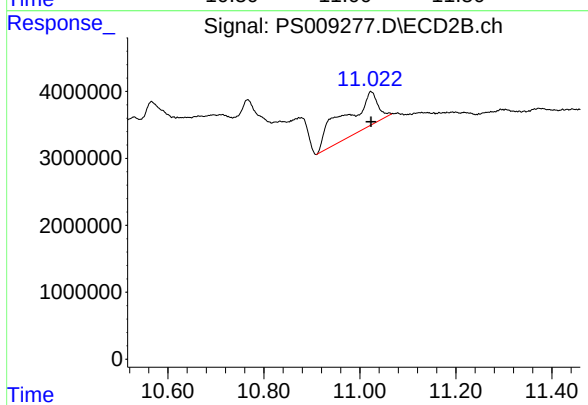

#15 Picloram


R.T.: 11.024 min
Delta R.T.: 0.000 min
Response: 26586726
Conc: 6.53 ng/ml

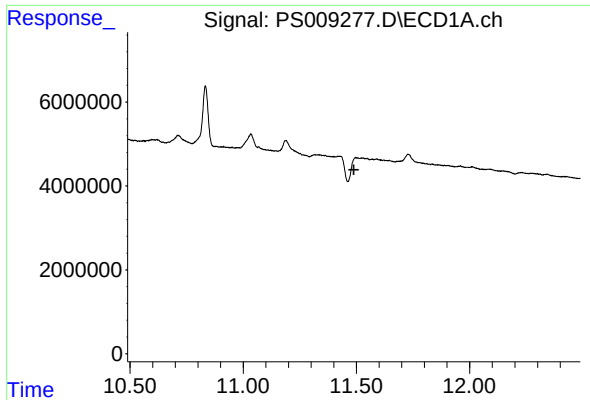

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.489 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

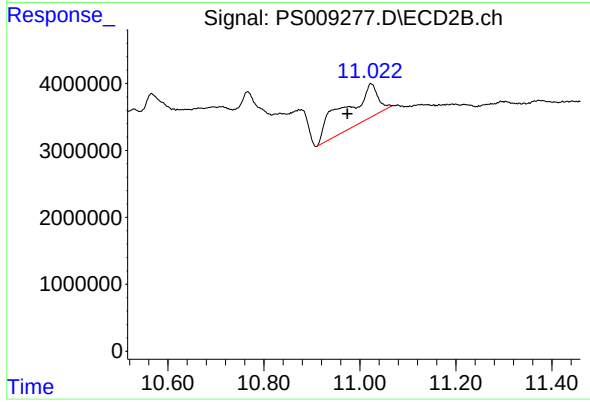

#16 DCPA

R.T.: 11.024 min
Delta R.T.: 0.050 min
Response: 26586726
Conc: 6.86 ng/ml