

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031320\
 Data File : PS009278.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2020 20:25
 Operator : DD\AJ
 Sample : L1893-12
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 01:03:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.241	6.934	216.5E6	215.6E6	391.386	392.654
Target Compounds							
1) T	Dalapon	0.000	2.590	0	61005138	N.D.	77.480
2) T	3,5-DICHL...	0.000	6.110	0	53062614	N.D.	65.243
3) T	4-Nitroph...	7.009	6.592	12789174	7603403	53.576	23.895 #
8) T	DICHLORPROP	8.116	7.753	-138243	40492941	N.D.	72.984
10) T	Pentachlo...	8.670	8.458	192.1E6	207.3E6	27.324	27.315
12) T	2,4,5-T	9.444	0.000	17001247	0	6.683	N.D. #
15) T	Picloram	0.000	11.023	0	26626188	N.D.	6.539
16) T	DCPA	0.000	11.023	0	26626188	N.D.	6.875



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031320\
Data File : PS009278.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2020 20:25
Operator : DD\AJ
Sample : L1893-12
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 01:03:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

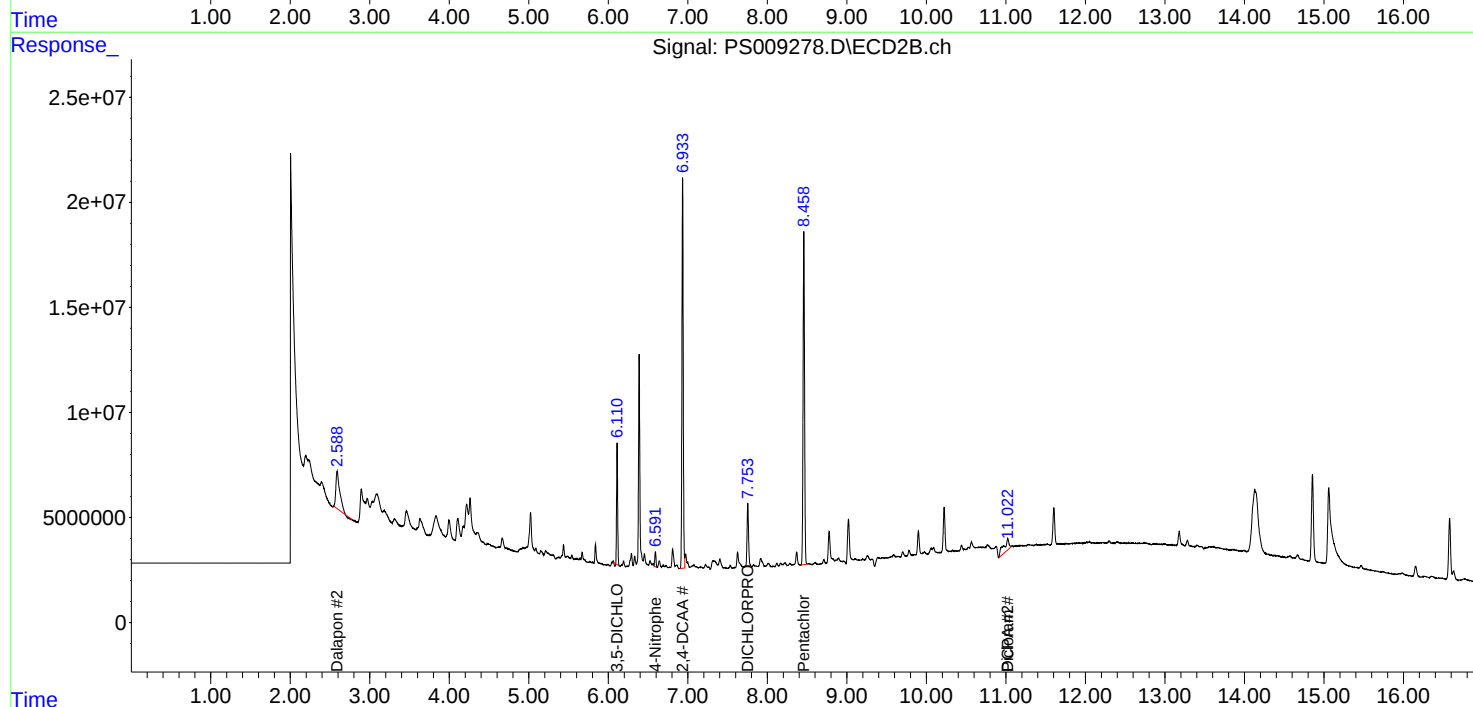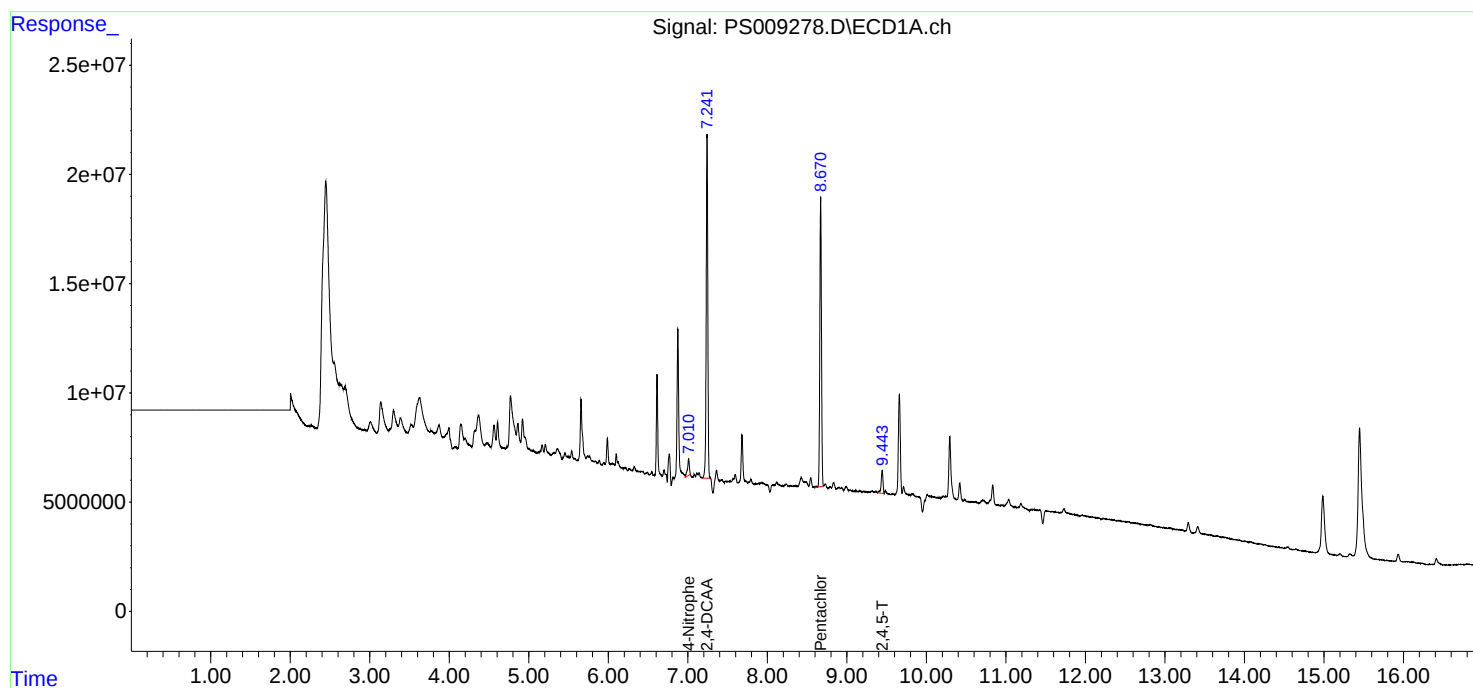


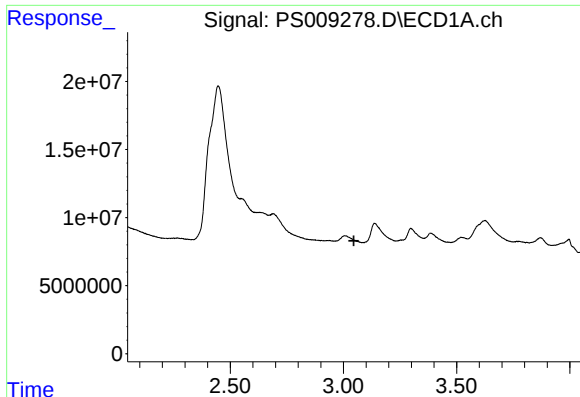

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 3.046 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

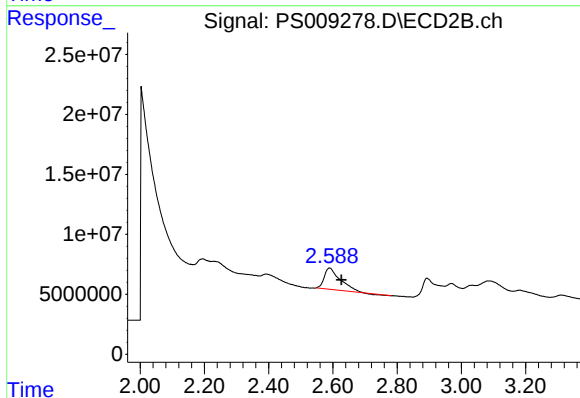


#1 Dalapon

R.T.: 2.590 min
Delta R.T.: -0.037 min
Response: 61005138
Conc: 77.48 ng/ml

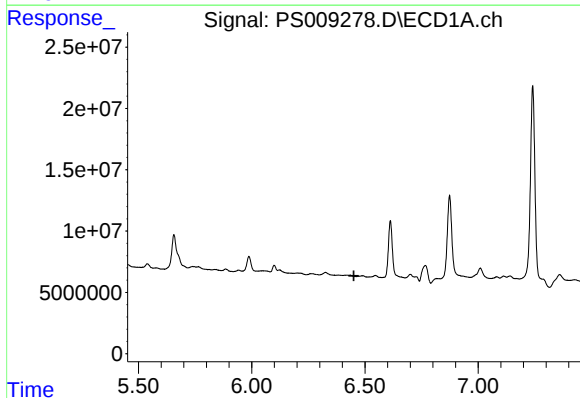


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

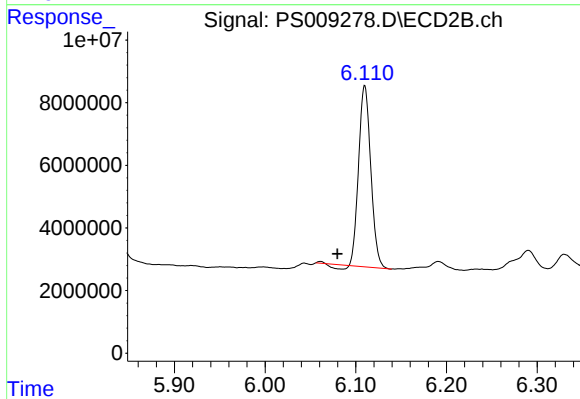

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.110 min
Delta R.T.: 0.030 min
Response: 53062614
Conc: 65.24 ng/ml

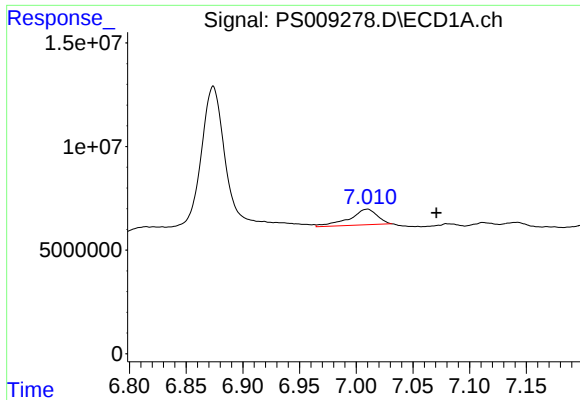

#3 4-Nitrophenol


R.T.: 7.009 min
Delta R.T.: -0.061 min
Response: 12789174
Conc: 53.58 ng/ml

Instrument :
ECD_S
ClientSampleId :

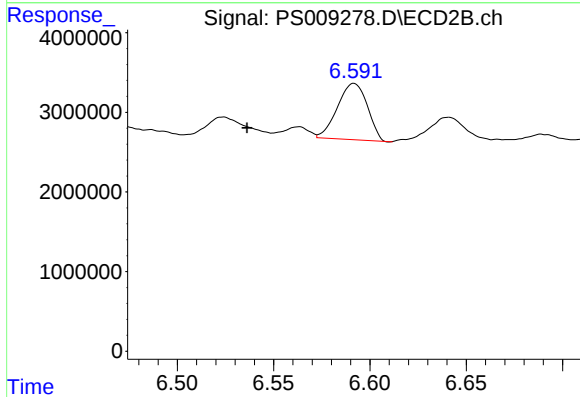


#3 4-Nitrophenol

R.T.: 6.592 min
Delta R.T.: 0.055 min
Response: 7603403
Conc: 23.90 ng/ml

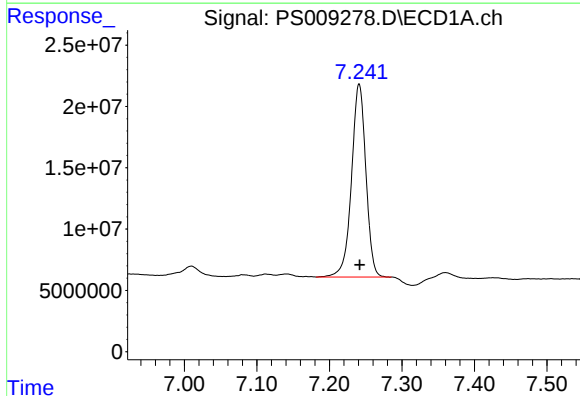


#4 2,4-DCAA

R.T.: 7.241 min
Delta R.T.: 0.000 min
Response: 216502795
Conc: 391.39 ng/ml

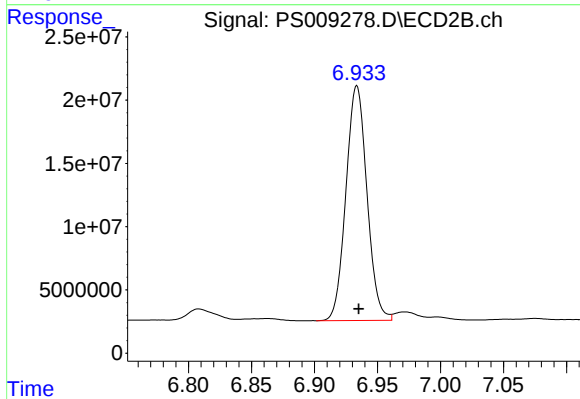

#4 2,4-DCAA


R.T.: 6.934 min
Delta R.T.: -0.001 min
Response: 215644664
Conc: 392.65 ng/ml

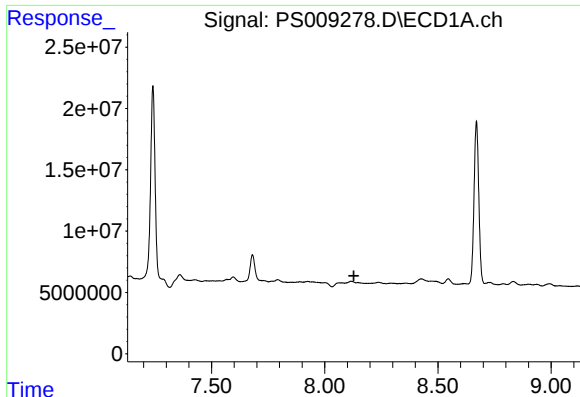

#8 DICHLORPROP


R.T.: 8.116 min
Delta R.T.: -0.013 min
Response: -138243
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

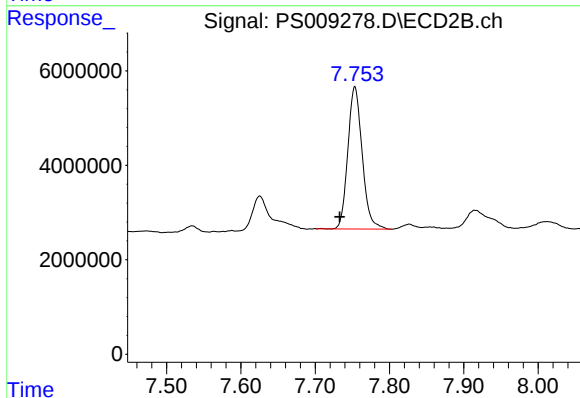


#8 DICHLORPROP

R.T.: 7.753 min
Delta R.T.: 0.020 min
Response: 40492941
Conc: 72.98 ng/ml

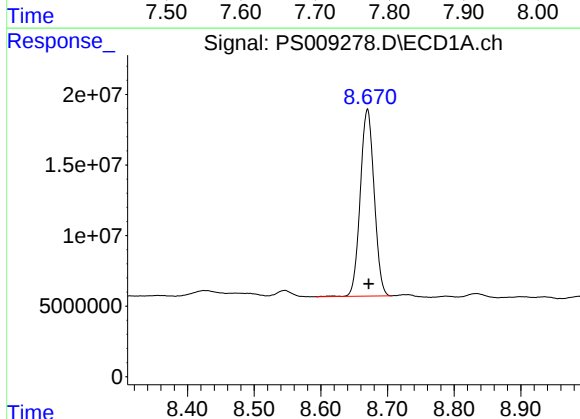


#10 Pentachlorophenol

R.T.: 8.670 min
Delta R.T.: -0.002 min
Response: 192120668
Conc: 27.32 ng/ml

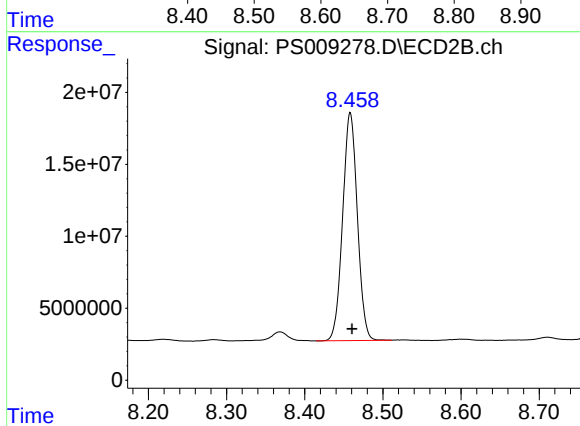

#10 Pentachlorophenol


R.T.: 8.458 min
Delta R.T.: -0.002 min
Response: 207319015
Conc: 27.31 ng/ml

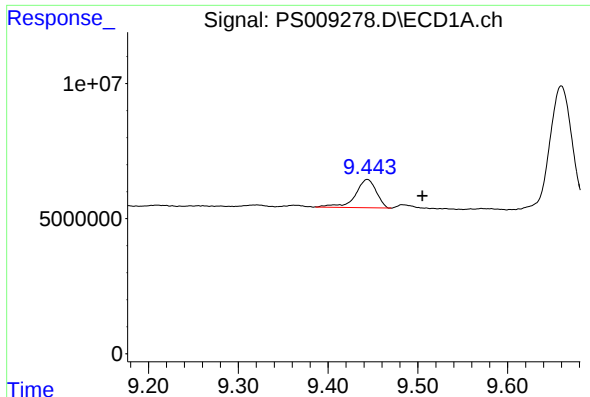

#12 2,4,5-T


R.T.: 9.444 min
Delta R.T.: -0.061 min
Response: 17001247
Conc: 6.68 ng/ml

Instrument :
ECD_S
ClientSampleId :

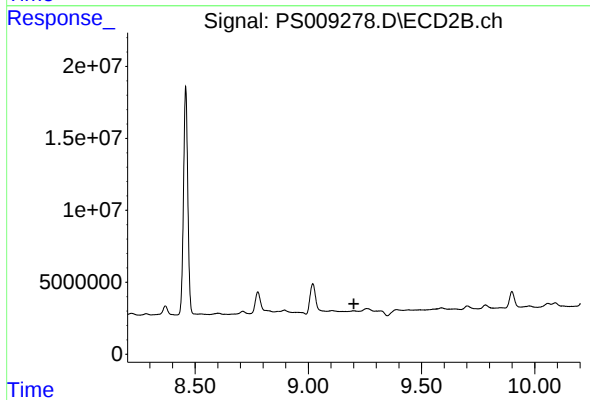


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.201 min
Response: 0
Conc: N.D.

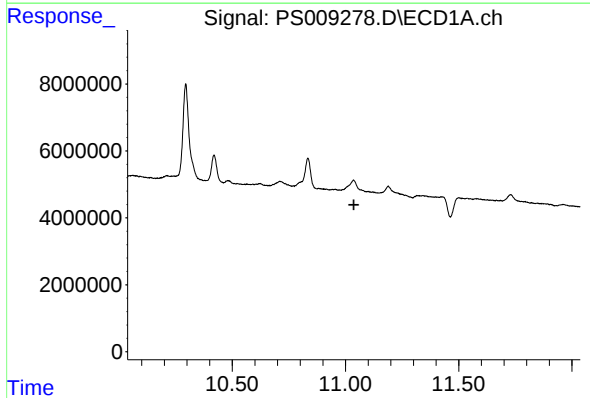


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.037 min
Response: 0
Conc: N.D.

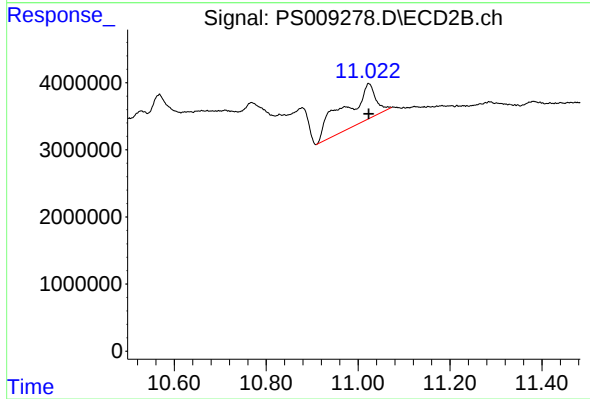

#15 Picloram


R.T.: 11.023 min
Delta R.T.: 0.000 min
Response: 26626188
Conc: 6.54 ng/ml

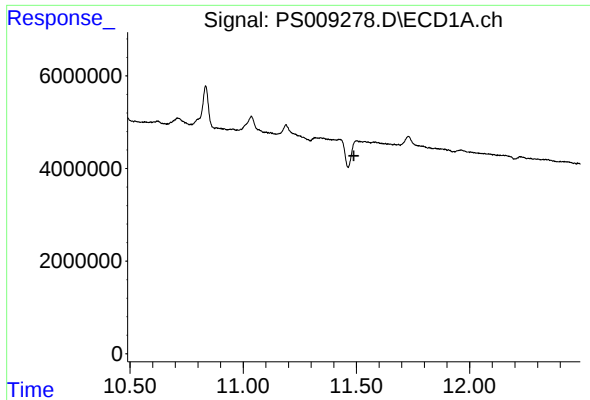

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.489 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

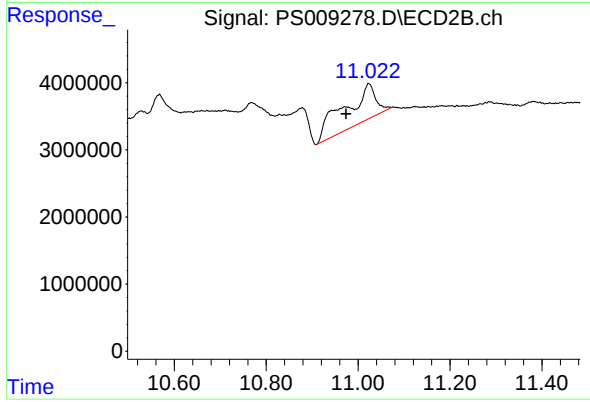

#16 DCPA

R.T.: 11.023 min
Delta R.T.: 0.049 min
Response: 26626188
Conc: 6.87 ng/ml