

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031320\
 Data File : PS009279.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2020 20:48
 Operator : DD\AJ
 Sample : L1893-16
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 01:03:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.241	6.934	249.5E6	255.1E6	451.027	464.486
Target Compounds							
1) T	Dalapon	0.000	2.589	0 47470700		N.D.	60.291
2) T	3,5-DICHL...	0.000	6.110	0 66392724		N.D.	81.633
3) T	4-Nitroph...	7.010	6.592	14032049	9647589	58.782	30.319 #
8) T	DICHLORPROP	8.116	7.753	39307	42346689	<MDL	76.325 #
9) T	2,4-D	8.294	0.000	19328576	0	36.661	N.D. #
12) T	2,4,5-T	9.443	0.000	25751066	0	10.123	N.D. #
15) T	Picloram	0.000	11.023	0 25459183		N.D.	6.252
16) T	DCPA	11.524	11.023	-1899748	25459183	N.D.	6.573



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031320\
Data File : PS009279.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2020 20:48
Operator : DD\AJ
Sample : L1893-16
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 01:03:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

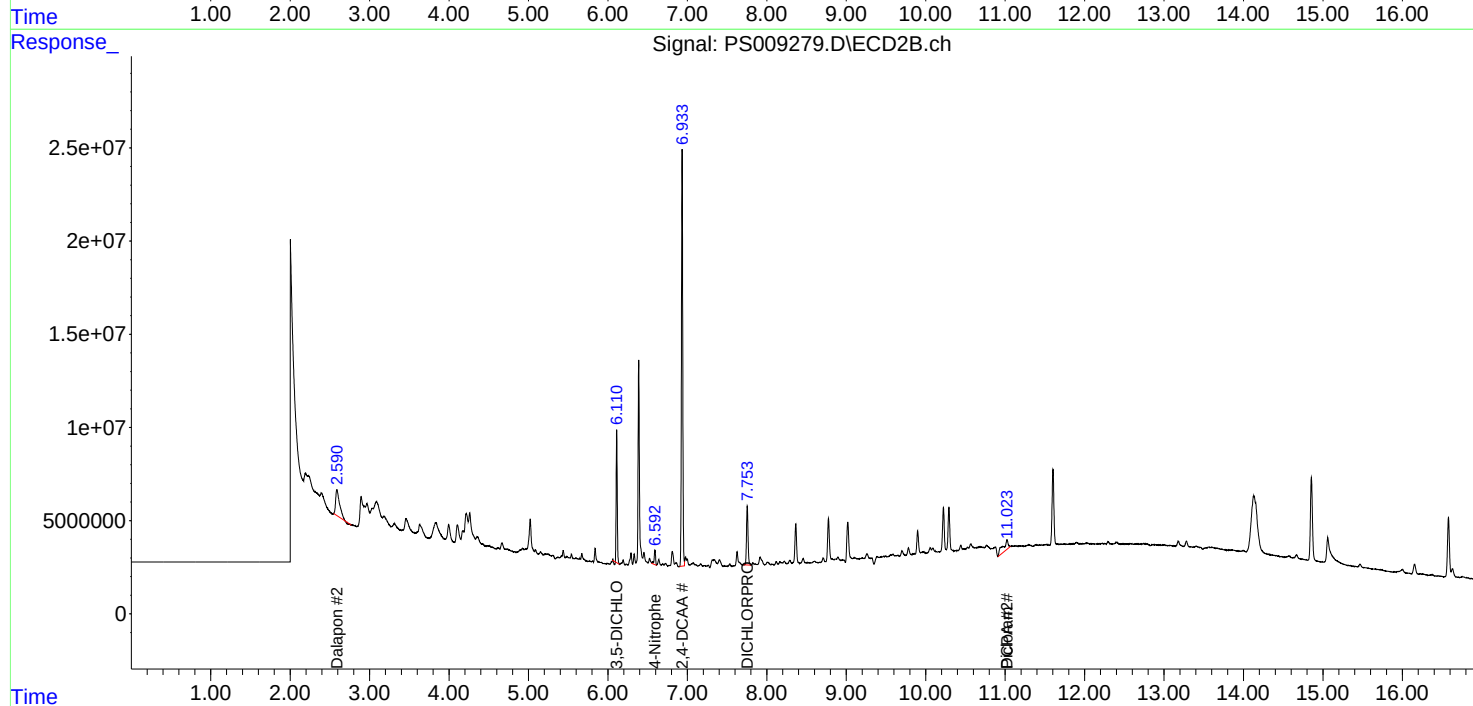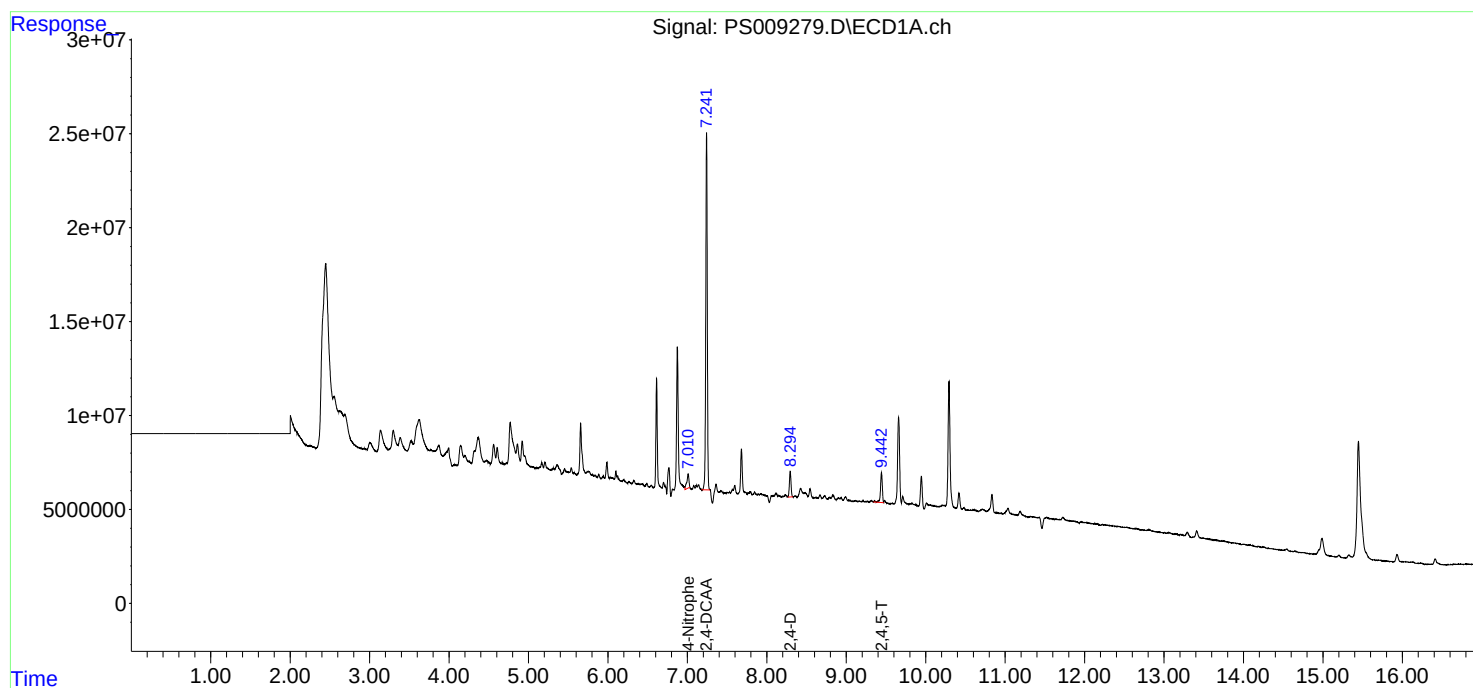


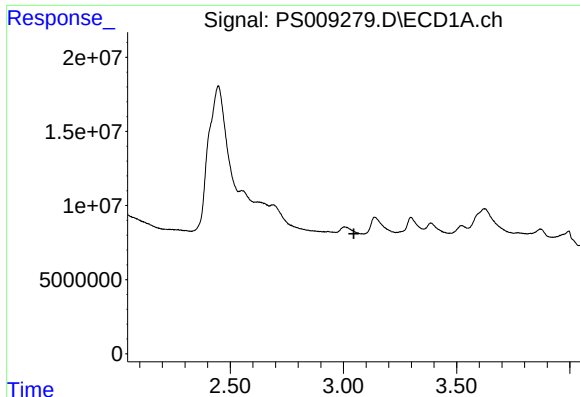

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.046 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

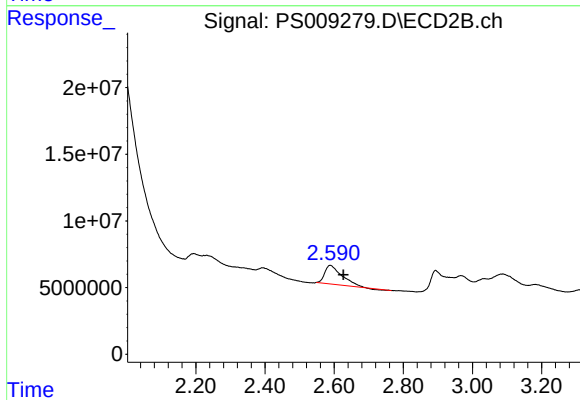


#1 Dalapon

R.T.: 2.589 min
Delta R.T.: -0.038 min
Response: 47470700
Conc: 60.29 ng/ml

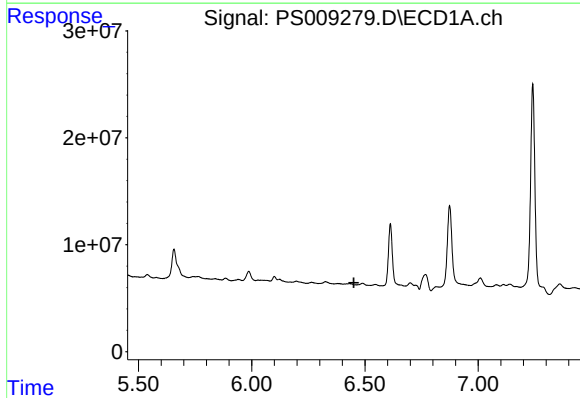


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.451 min
Response: 0
Conc: N.D.

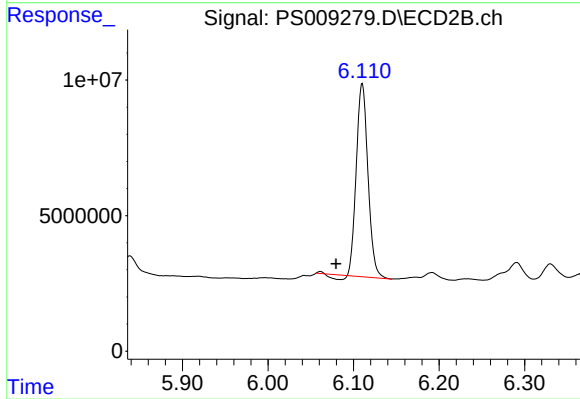

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.110 min
Delta R.T.: 0.030 min
Response: 66392724
Conc: 81.63 ng/ml

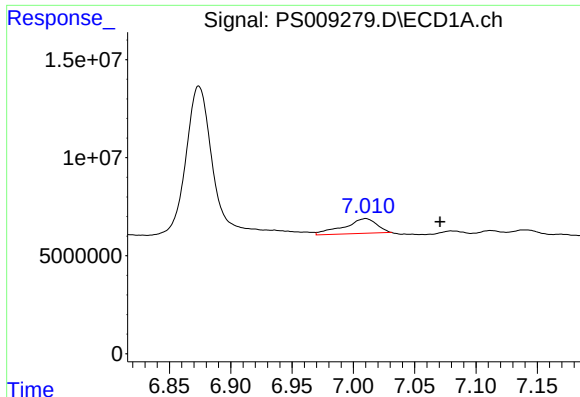

#3 4-Nitrophenol


R.T.: 7.010 min
Delta R.T.: -0.061 min
Response: 14032049
Conc: 58.78 ng/ml

Instrument :
ECD_S
ClientSampleId :

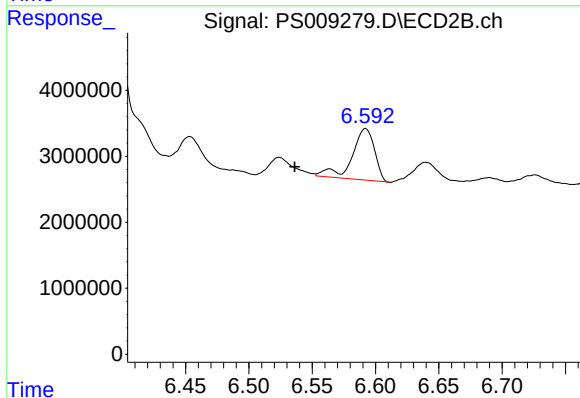


#3 4-Nitrophenol

R.T.: 6.592 min
Delta R.T.: 0.056 min
Response: 9647589
Conc: 30.32 ng/ml

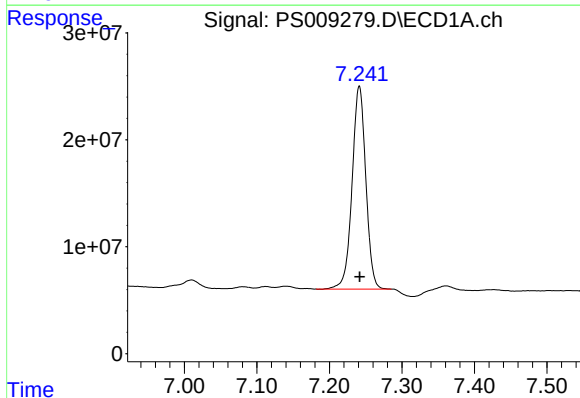


#4 2,4-DCAA

R.T.: 7.241 min
Delta R.T.: 0.000 min
Response: 249494647
Conc: 451.03 ng/ml

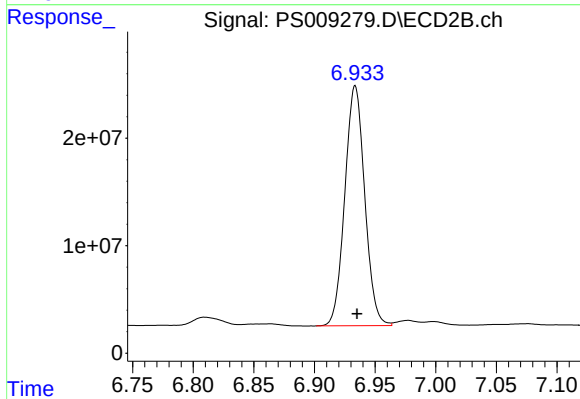

#4 2,4-DCAA


R.T.: 6.934 min
Delta R.T.: -0.002 min
Response: 255094645
Conc: 464.49 ng/ml

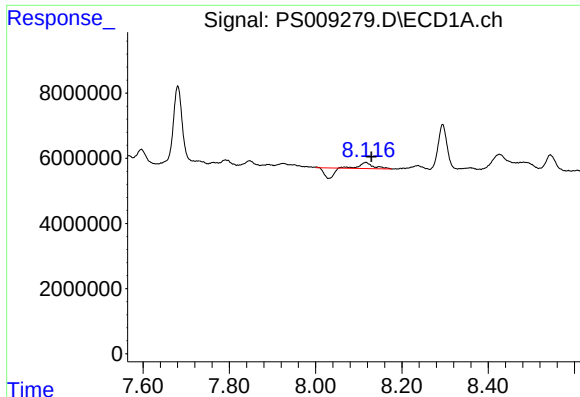

#8 DICHLORPROP


R.T.: 8.116 min
Delta R.T.: -0.013 min
Response: 39307
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

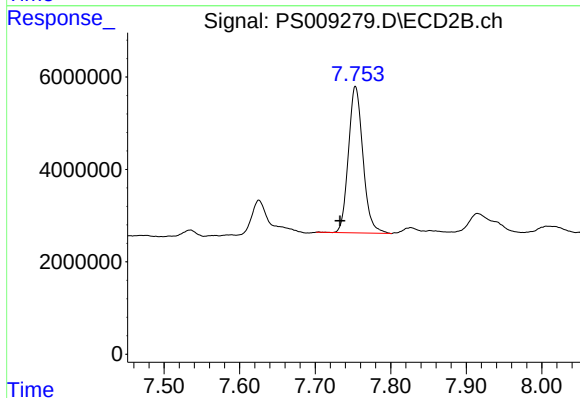


#8 DICHLORPROP

R.T.: 7.753 min
Delta R.T.: 0.020 min
Response: 42346689
Conc: 76.32 ng/ml

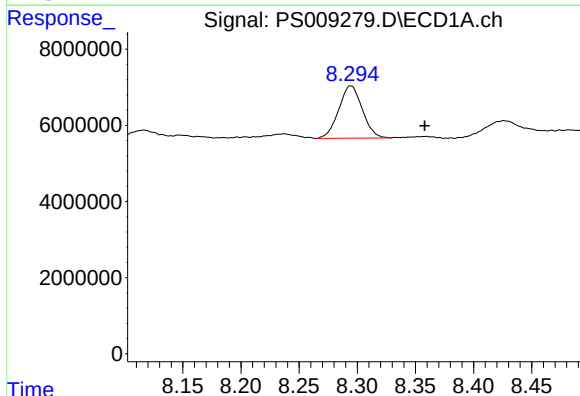


#9 2,4-D

R.T.: 8.294 min
Delta R.T.: -0.063 min
Response: 19328576
Conc: 36.66 ng/ml

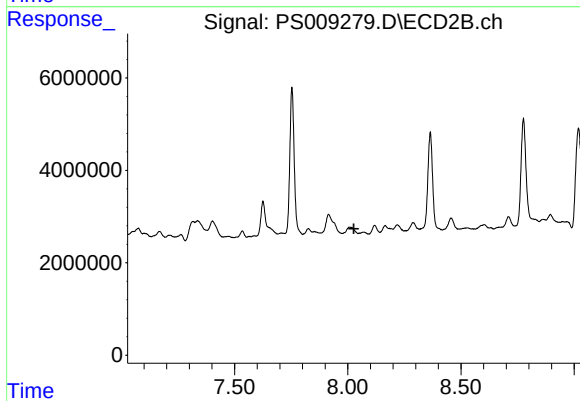

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.027 min
Response: 0
Conc: N.D.

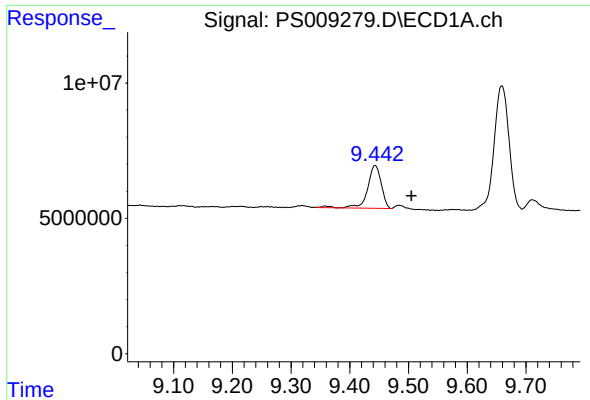

#12 2,4,5-T


R.T.: 9.443 min
Delta R.T.: -0.062 min
Response: 25751066
Conc: 10.12 ng/ml

Instrument :
ECD_S
ClientSampleId :

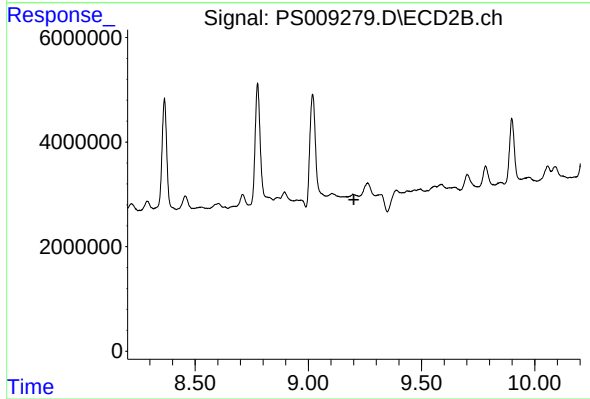


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.201 min
Response: 0
Conc: N.D.

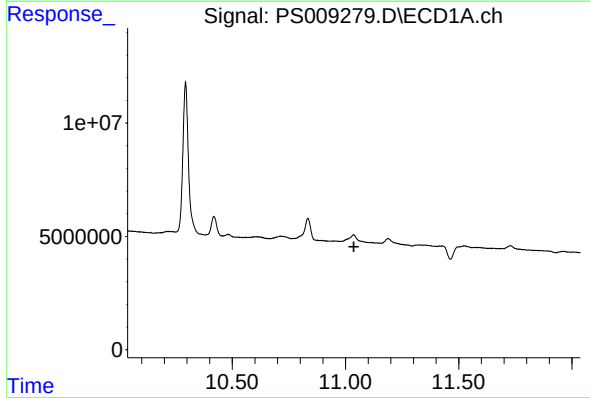


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.037 min
Response: 0
Conc: N.D.

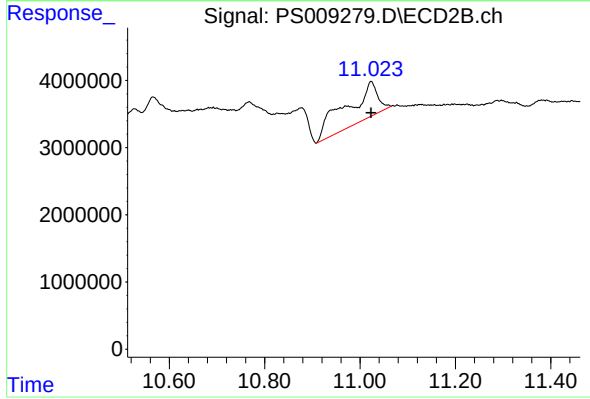

#15 Picloram


R.T.: 11.023 min
Delta R.T.: 0.000 min
Response: 25459183
Conc: 6.25 ng/ml

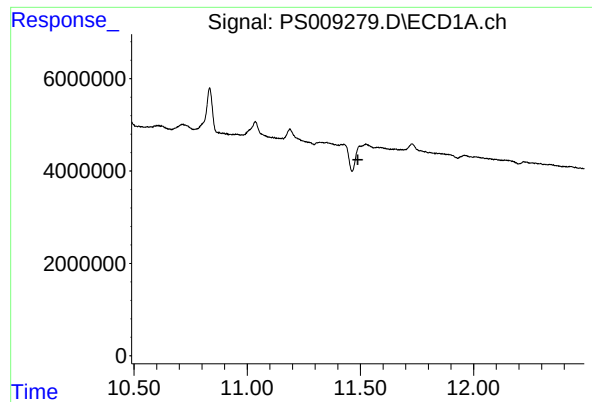

#16 DCPA

R.T.: 11.524 min
Delta R.T.: 0.035 min
Response: -1899748
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

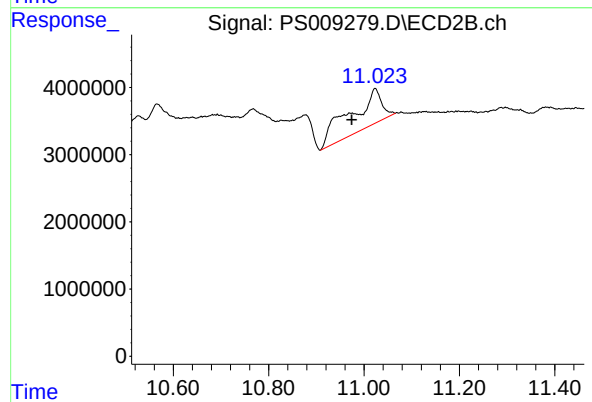

#16 DCPA

R.T.: 11.023 min
Delta R.T.: 0.049 min
Response: 25459183
Conc: 6.57 ng/ml