

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031320\
 Data File : PS009282.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2020 21:57
 Operator : DD\AJ
 Sample : L1893-20
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 01:04:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.242	6.934	246.0E6	243.4E6	444.677	443.179
Target Compounds							
1) T	Dalapon	0.000	2.590	0 70480846		N.D.	89.515
2) T	3,5-DICHL...	0.000	6.110	0 75575634		N.D.	92.924
3) T	4-Nitroph...	7.009	6.592	11222510	9513804	47.013	29.899 #
8) T	DICHLORPROP	8.116	7.754	3089937	51107878	5.991	92.116 #
9) T	2,4-D	8.294	0.000	7178232	0	13.615	N.D. #
12) T	2,4,5-T	9.444	9.253	22381735	20798728	8.798	7.045
15) T	Picloram	11.037	11.022	65853567	112.0E6	21.699	27.499 #
16) T	DCPA	0.000	11.022	0 112.0E6		N.D.	28.913



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031320\
Data File : PS009282.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2020 21:57
Operator : DD\AJ
Sample : L1893-20
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 01:04:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

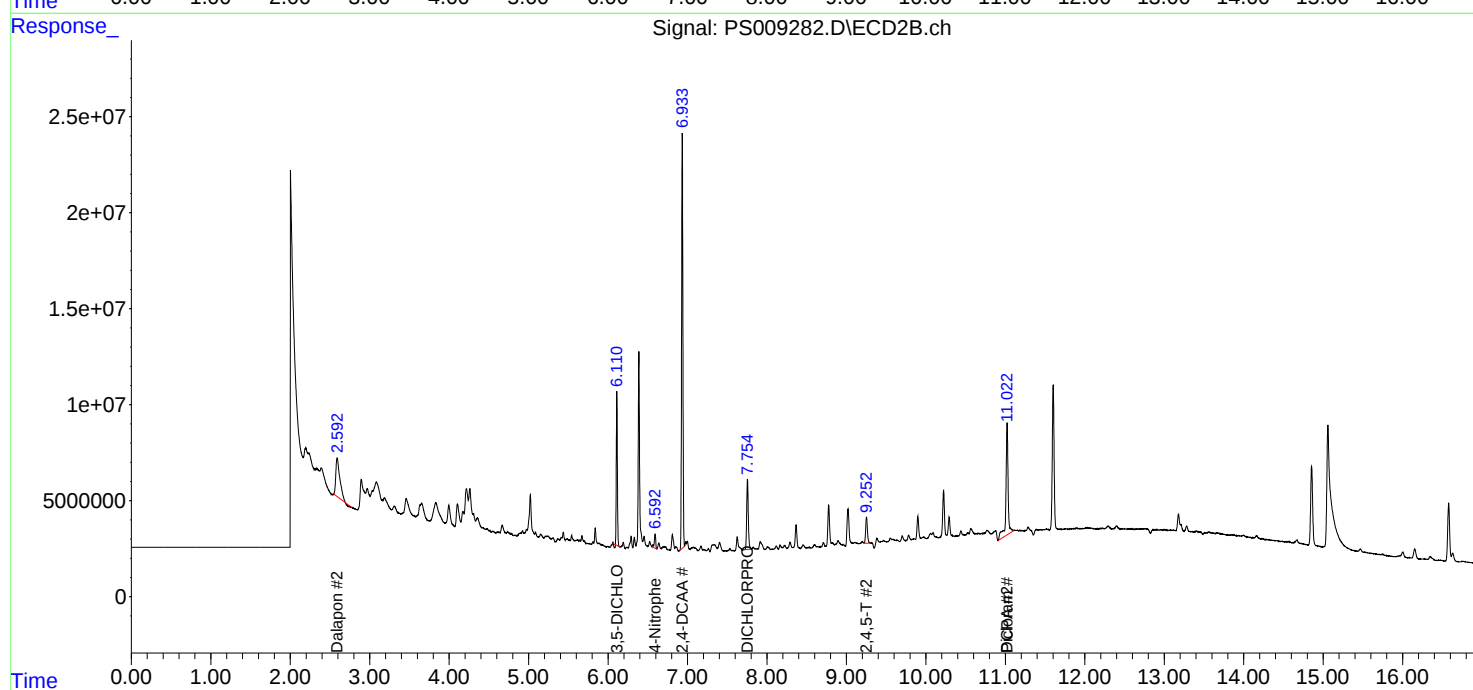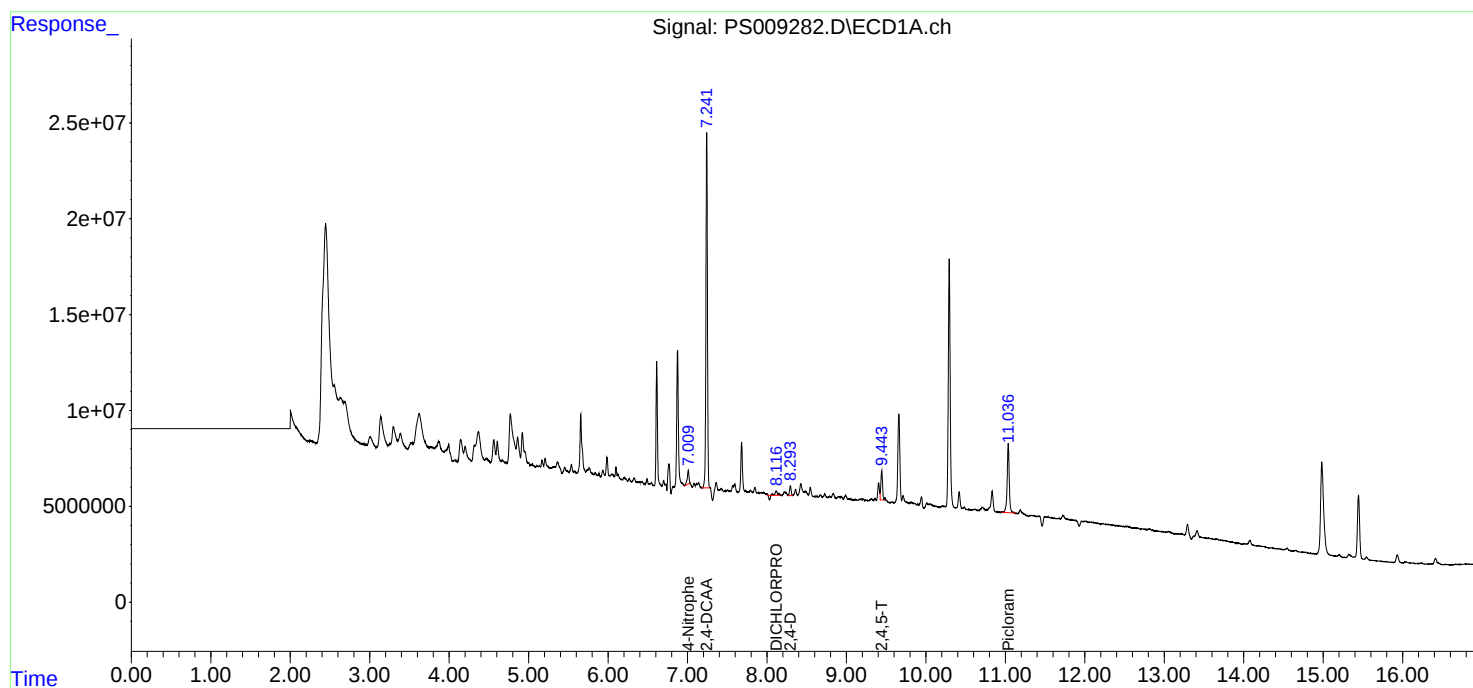


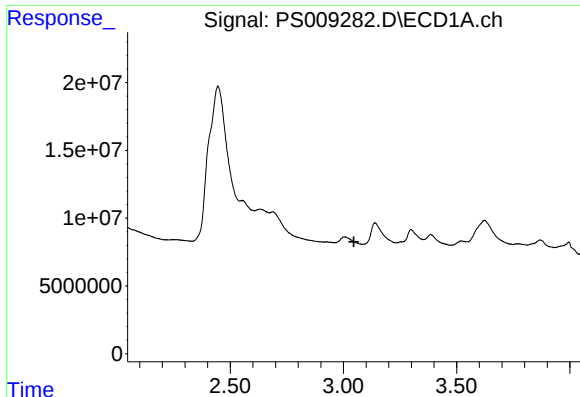

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 3.046 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

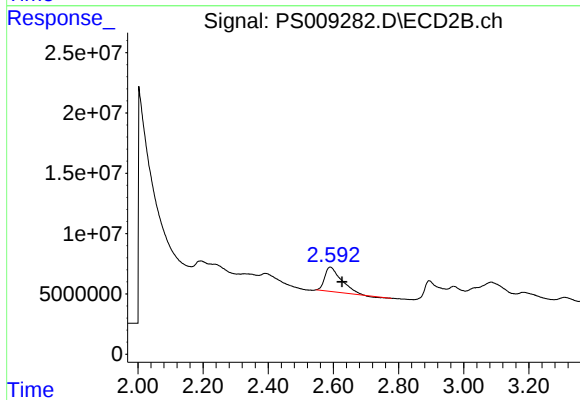


#1 Dalapon

R.T.: 2.590 min
Delta R.T.: -0.036 min
Response: 70480846
Conc: 89.52 ng/ml

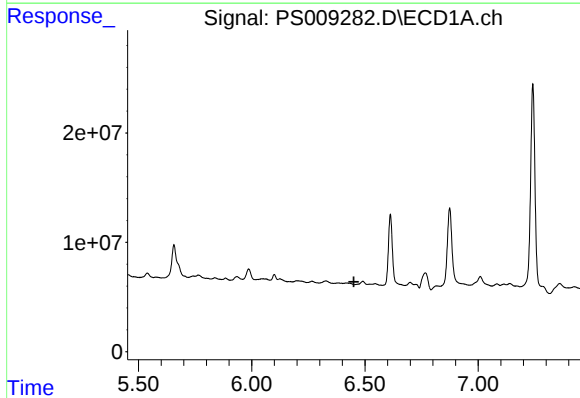


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

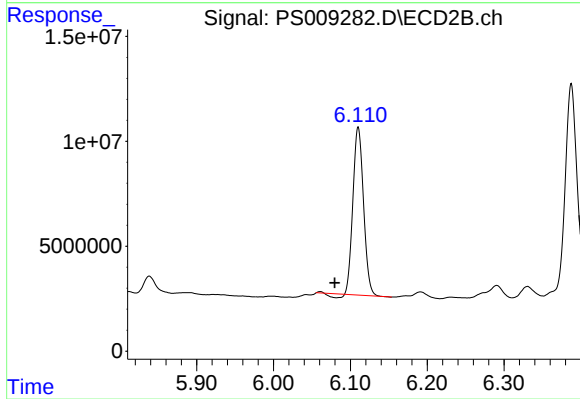

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.110 min
Delta R.T.: 0.031 min
Response: 75575634
Conc: 92.92 ng/ml

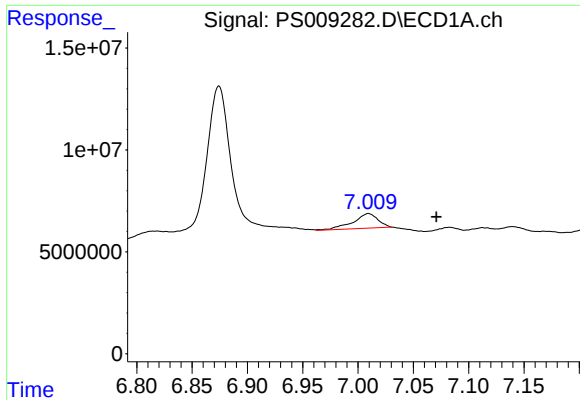

#3 4-Nitrophenol


R.T.: 7.009 min
Delta R.T.: -0.061 min
Response: 11222510
Conc: 47.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

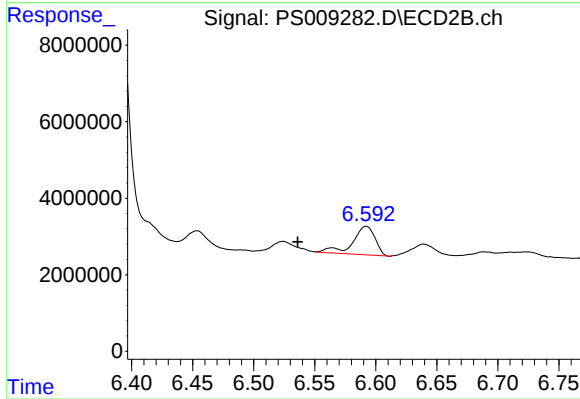


#3 4-Nitrophenol

R.T.: 6.592 min
Delta R.T.: 0.056 min
Response: 9513804
Conc: 29.90 ng/ml

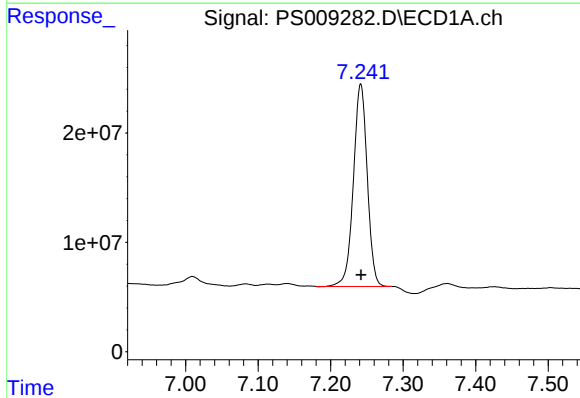


#4 2,4-DCAA

R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 245981995
Conc: 444.68 ng/ml

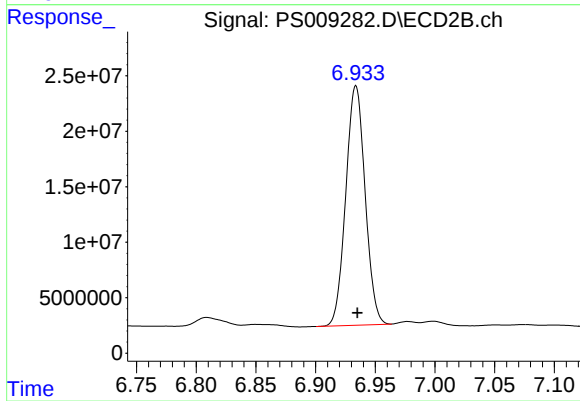

#4 2,4-DCAA


R.T.: 6.934 min
Delta R.T.: -0.001 min
Response: 243393010
Conc: 443.18 ng/ml

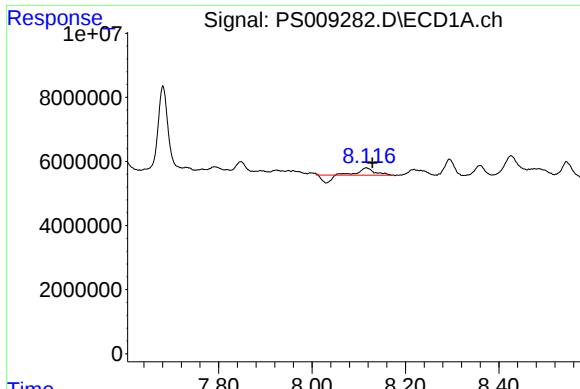

#8 DICHLORPROP


R.T.: 8.116 min
Delta R.T.: -0.013 min
Response: 3089937
Conc: 5.99 ng/ml

Instrument :
ECD_S
ClientSampleId :

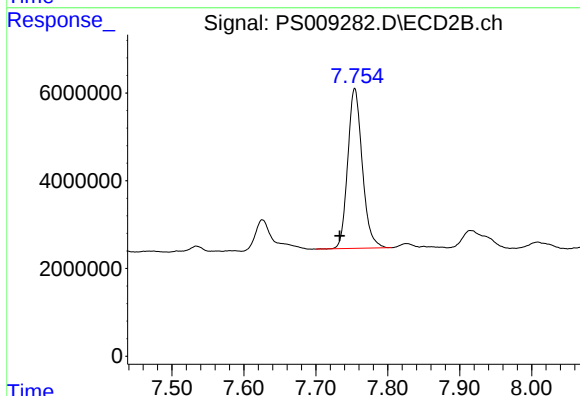


#8 DICHLORPROP

R.T.: 7.754 min
Delta R.T.: 0.021 min
Response: 51107878
Conc: 92.12 ng/ml

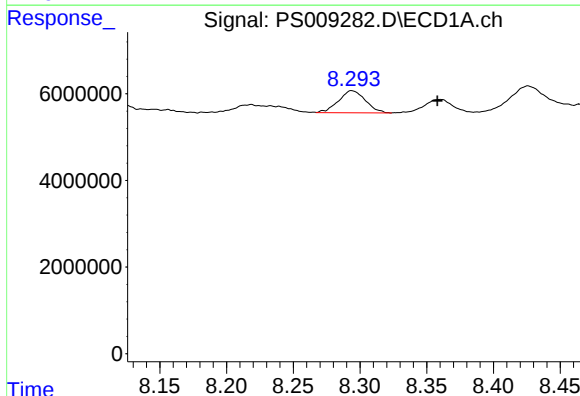


#9 2,4-D

R.T.: 8.294 min
Delta R.T.: -0.064 min
Response: 7178232
Conc: 13.62 ng/ml

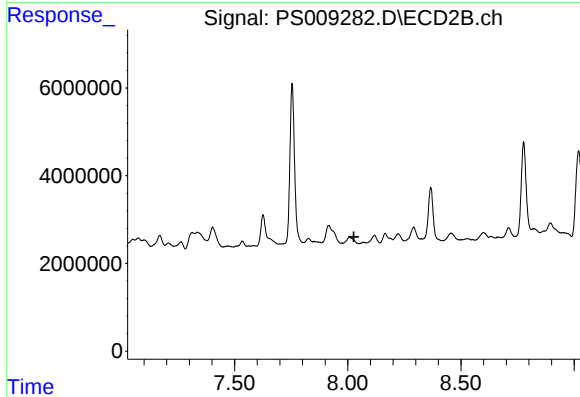

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.027 min
Response: 0
Conc: N.D.

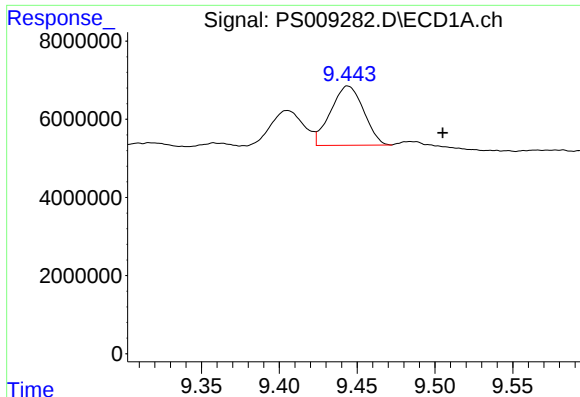

#12 2,4,5-T


R.T.: 9.444 min
Delta R.T.: -0.061 min
Response: 22381735
Conc: 8.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

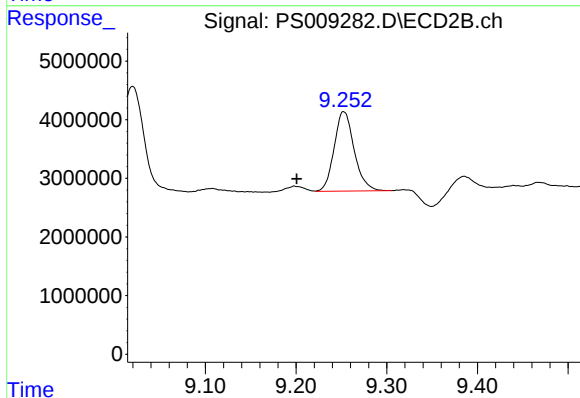


#12 2,4,5-T

R.T.: 9.253 min
Delta R.T.: 0.052 min
Response: 20798728
Conc: 7.05 ng/ml

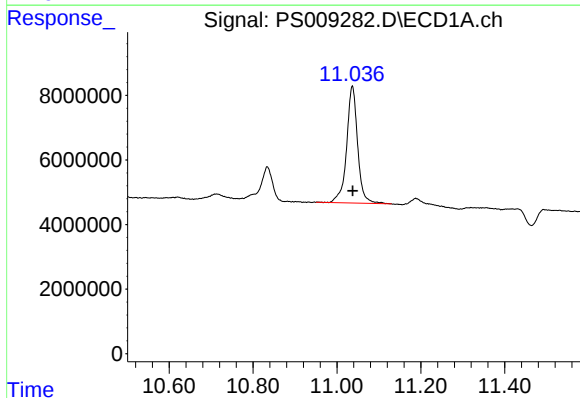


#15 Picloram

R.T.: 11.037 min
Delta R.T.: 0.000 min
Response: 65853567
Conc: 21.70 ng/ml

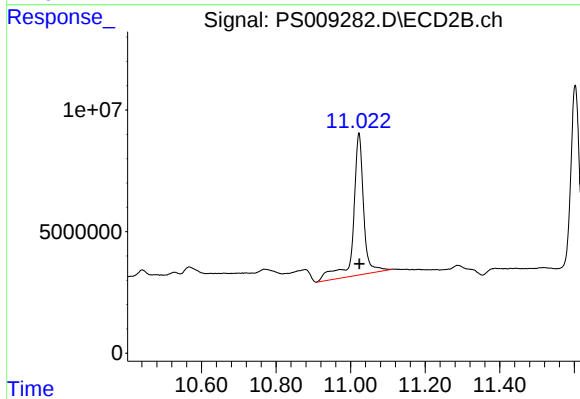

#15 Picloram


R.T.: 11.022 min
Delta R.T.: -0.001 min
Response: 111979763
Conc: 27.50 ng/ml

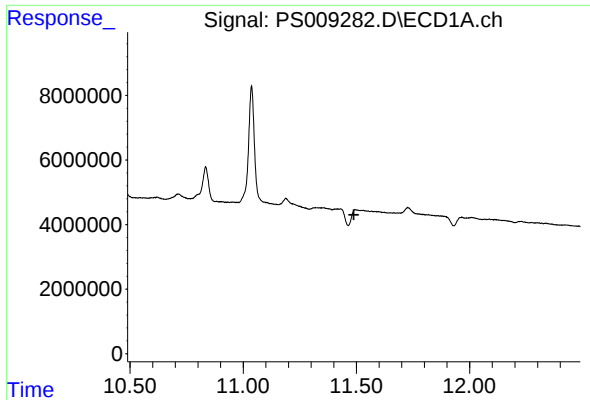

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.489 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

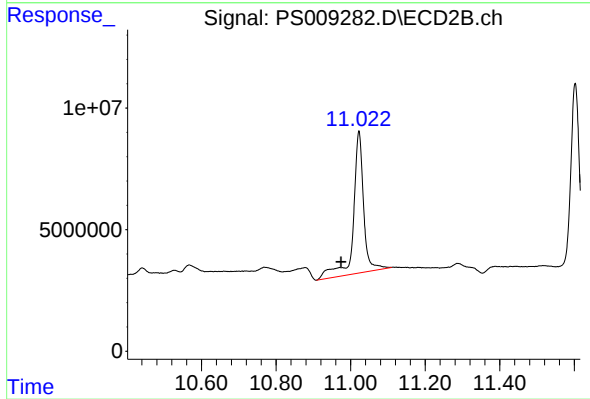

#16 DCPA

R.T.: 11.022 min
Delta R.T.: 0.048 min
Response: 111979763
Conc: 28.91 ng/ml