

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031320\
 Data File : PS009283.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2020 22:20
 Operator : DD\AJ
 Sample : L1893-24
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 01:04:35 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.242	6.934	263.3E6	269.1E6	475.921	490.007
Target Compounds							
1) T	Dalapon	3.005	2.588	15416931	83354318	19.770	105.865 #
2) T	3,5-DICHL...	0.000	6.110	0	69605620	N.D.	85.583
3) T	4-Nitroph...	7.010	6.592	13978762	8269843	58.559	25.990 #
8) T	DICHLORPROP	8.117	7.754	76745	43355694	<MDL	78.143 #
9) T	2,4-D	8.427	0.000	9921574	0	18.818	N.D. #
12) T	2,4,5-T	9.444	0.000	25293132	0	9.943	N.D. #
15) T	Picloram	11.036	11.023	12370906	33788424	4.076	8.297 #
16) T	DCPA	0.000	11.023	0	33788424	N.D.	8.724



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031320\
Data File : PS009283.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2020 22:20
Operator : DD\AJ
Sample : L1893-24
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 01:04:35 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

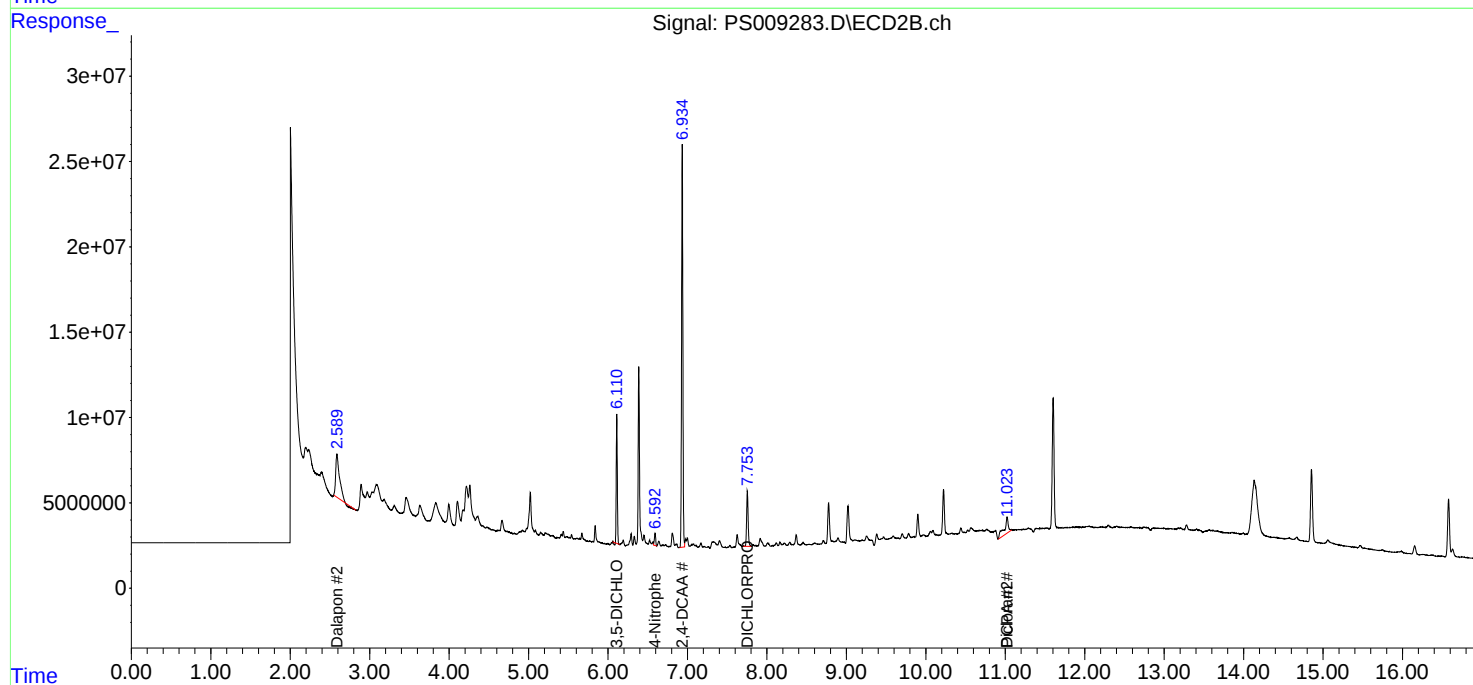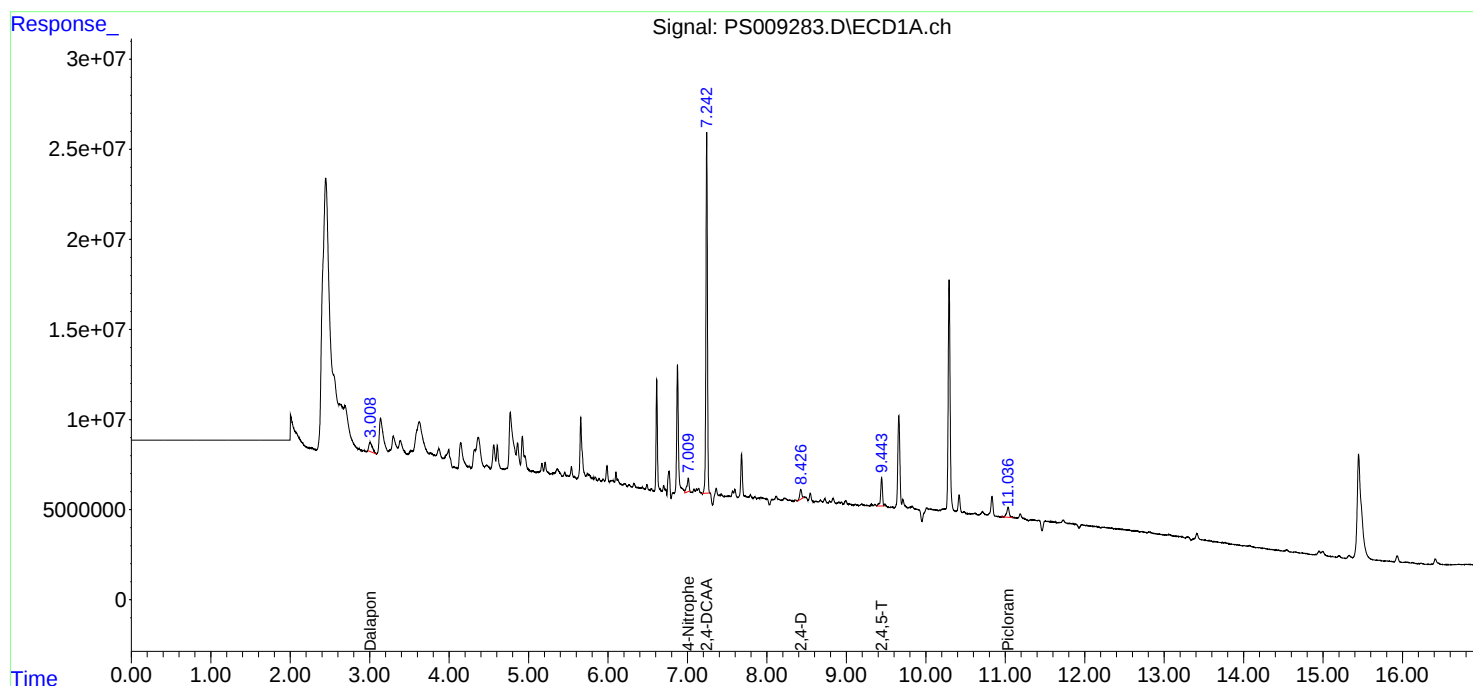


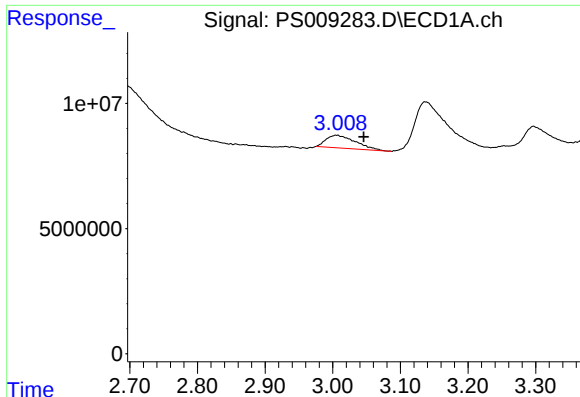

#1 Dalapon


R.T.: 3.005 min
Delta R.T.: -0.041 min
Response: 15416931
Conc: 19.77 ng/ml

Instrument :
ECD_S
ClientSampleId :

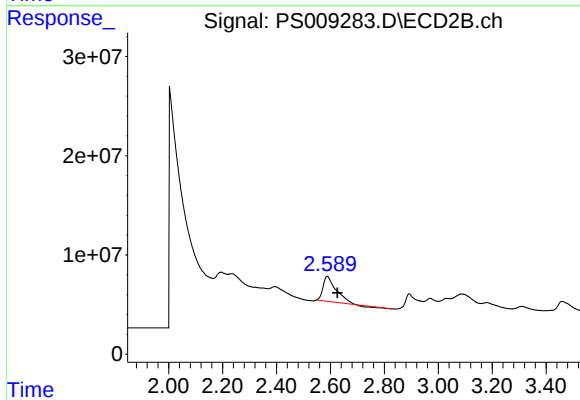


#1 Dalapon

R.T.: 2.588 min
Delta R.T.: -0.038 min
Response: 83354318
Conc: 105.87 ng/ml

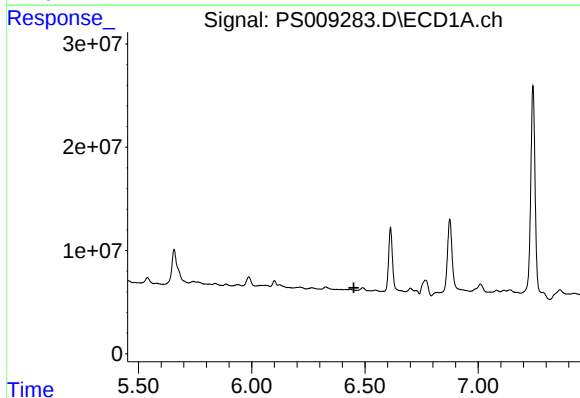


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

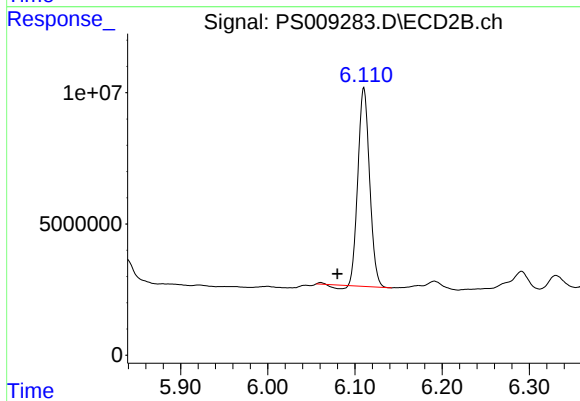

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.110 min
Delta R.T.: 0.031 min
Response: 69605620
Conc: 85.58 ng/ml

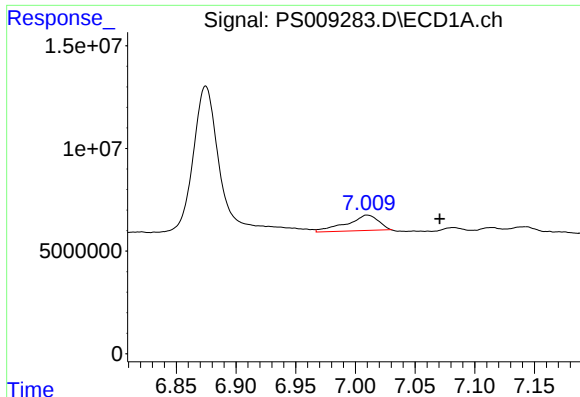

#3 4-Nitrophenol


R.T.: 7.010 min
Delta R.T.: -0.061 min
Response: 13978762
Conc: 58.56 ng/ml

Instrument :
ECD_S
ClientSampleId :

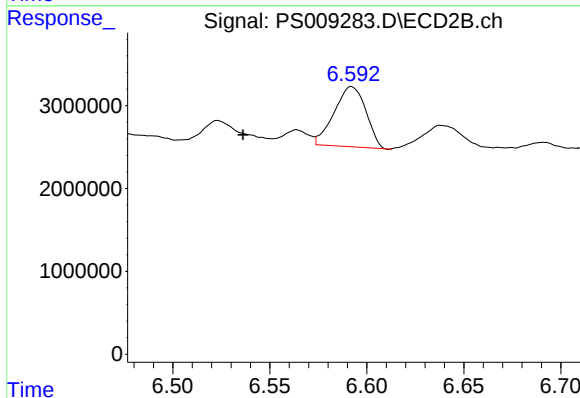


#3 4-Nitrophenol

R.T.: 6.592 min
Delta R.T.: 0.056 min
Response: 8269843
Conc: 25.99 ng/ml

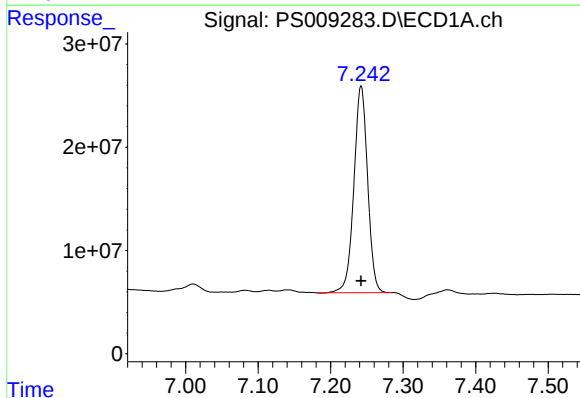


#4 2,4-DCAA

R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 263265179
Conc: 475.92 ng/ml

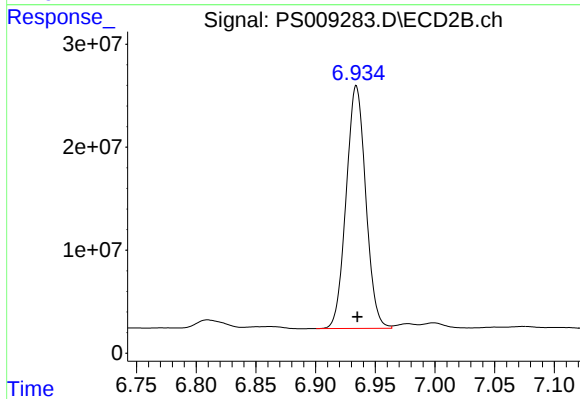

#4 2,4-DCAA


R.T.: 6.934 min
Delta R.T.: 0.000 min
Response: 269110591
Conc: 490.01 ng/ml

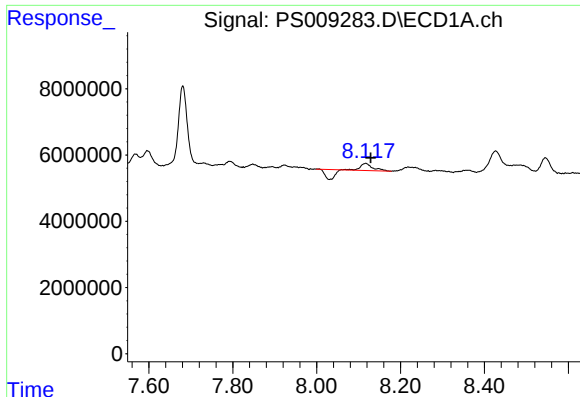

#8 DICHLORPROP


R.T.: 8.117 min
Delta R.T.: -0.012 min
Response: 76745
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

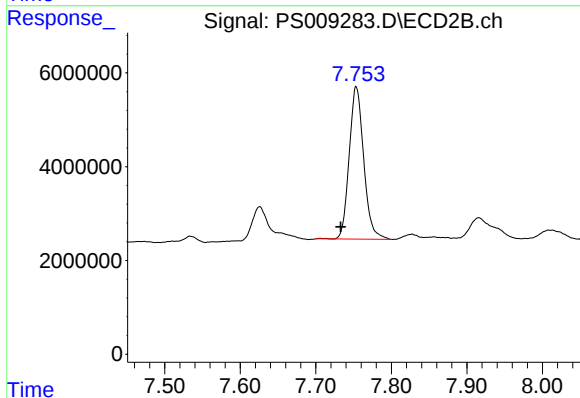


#8 DICHLORPROP

R.T.: 7.754 min
Delta R.T.: 0.021 min
Response: 43355694
Conc: 78.14 ng/ml

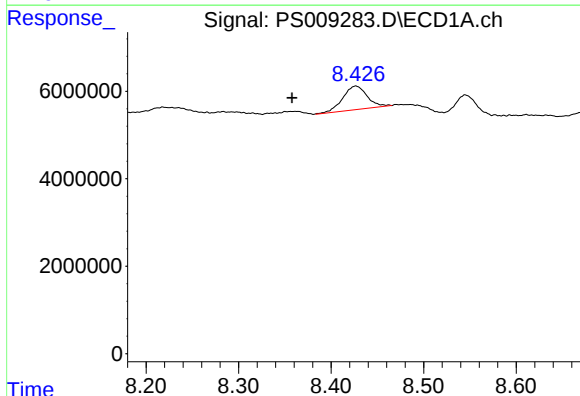


#9 2,4-D

R.T.: 8.427 min
Delta R.T.: 0.069 min
Response: 9921574
Conc: 18.82 ng/ml

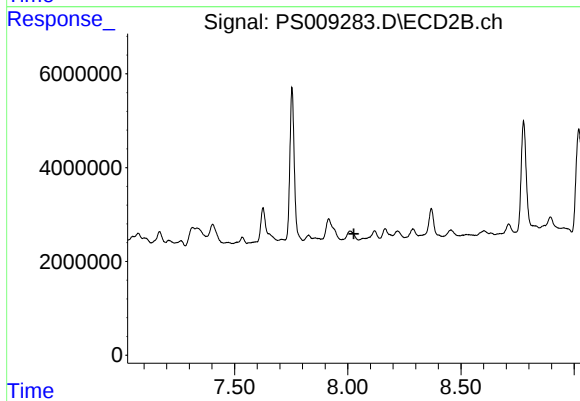

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.027 min
Response: 0
Conc: N.D.

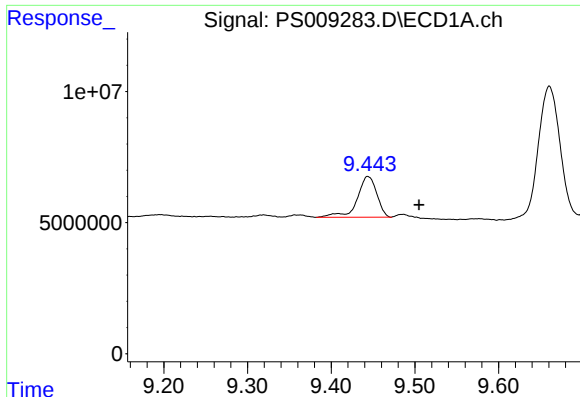

#12 2,4,5-T


R.T.: 9.444 min
Delta R.T.: -0.061 min
Response: 25293132
Conc: 9.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

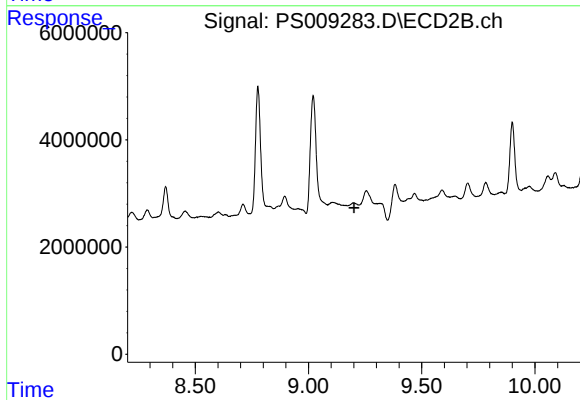


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.201 min
Response: 0
Conc: N.D.

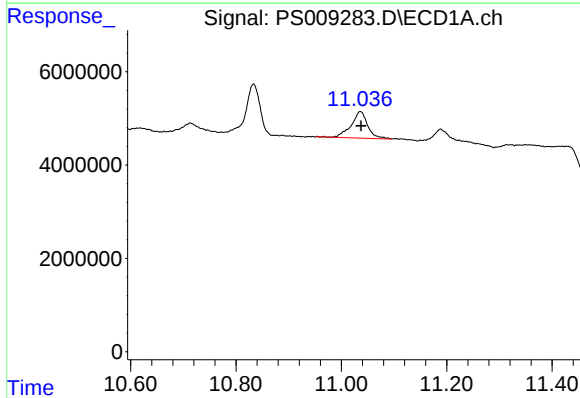


#15 Picloram

R.T.: 11.036 min
Delta R.T.: -0.001 min
Response: 12370906
Conc: 4.08 ng/ml

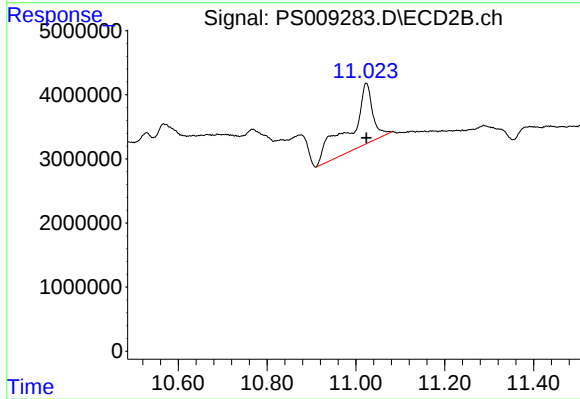

#15 Picloram


R.T.: 11.023 min
Delta R.T.: 0.000 min
Response: 33788424
Conc: 8.30 ng/ml

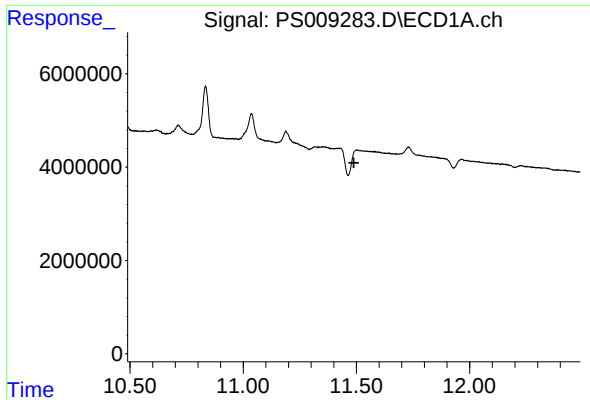

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.489 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

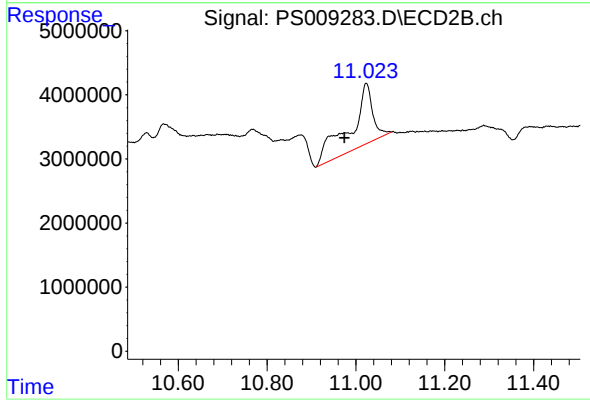

#16 DCPA

R.T.: 11.023 min
Delta R.T.: 0.049 min
Response: 33788424
Conc: 8.72 ng/ml