

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031325\
 Data File : PS029439.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2025 01:10
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 11:07:36 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022125.M
 Quant Title : 8080.M
 QLast Update : Sat Feb 22 01:02:20 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.155	7.617	2143.4E6	478.2E6	520.169	508.579
Target Compounds							
1) T	Dalapon	0.000	2.684f	0	6904729	N.D.	3.261
2) T	3,5-DICHL...	6.324	0.000	4640804	0	<MDL	N.D. #
3) T	4-Nitroph...	6.943	0.000	18936647	0	8.092	N.D. #
5) T	DICAMBA	0.000	7.832	0	2975801	N.D.	<MDL
8) T	DICHLORPROP	8.044	8.572f	4996498	9181981	1.087	7.180 #
9) T	2,4-D	8.266	0.000	189685	0	<MDL	N.D. #
10) T	Pentachlo...	8.555	0.000	5350915	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.118	0.000	3869872	0	<MDL	N.D. #
12) T	2,4,5-T	9.454f	10.172	9084269	5849695	<MDL	<MDL #
13) T	2,4-DB	9.999	0.000	1101783	0	<MDL	N.D. #
14) T	DINOSEB	11.187	0.000	1475233	0	<MDL	N.D. #
15) T	Picloram	10.998	0.000	3775822	0	<MDL	N.D. #
16) T	DCPA	11.483	0.000	4915051	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031325\
Data File : PS029439.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2025 01:10
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 11:07:36 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022125.M
Quant Title : 8080.M
QLast Update : Sat Feb 22 01:02:20 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

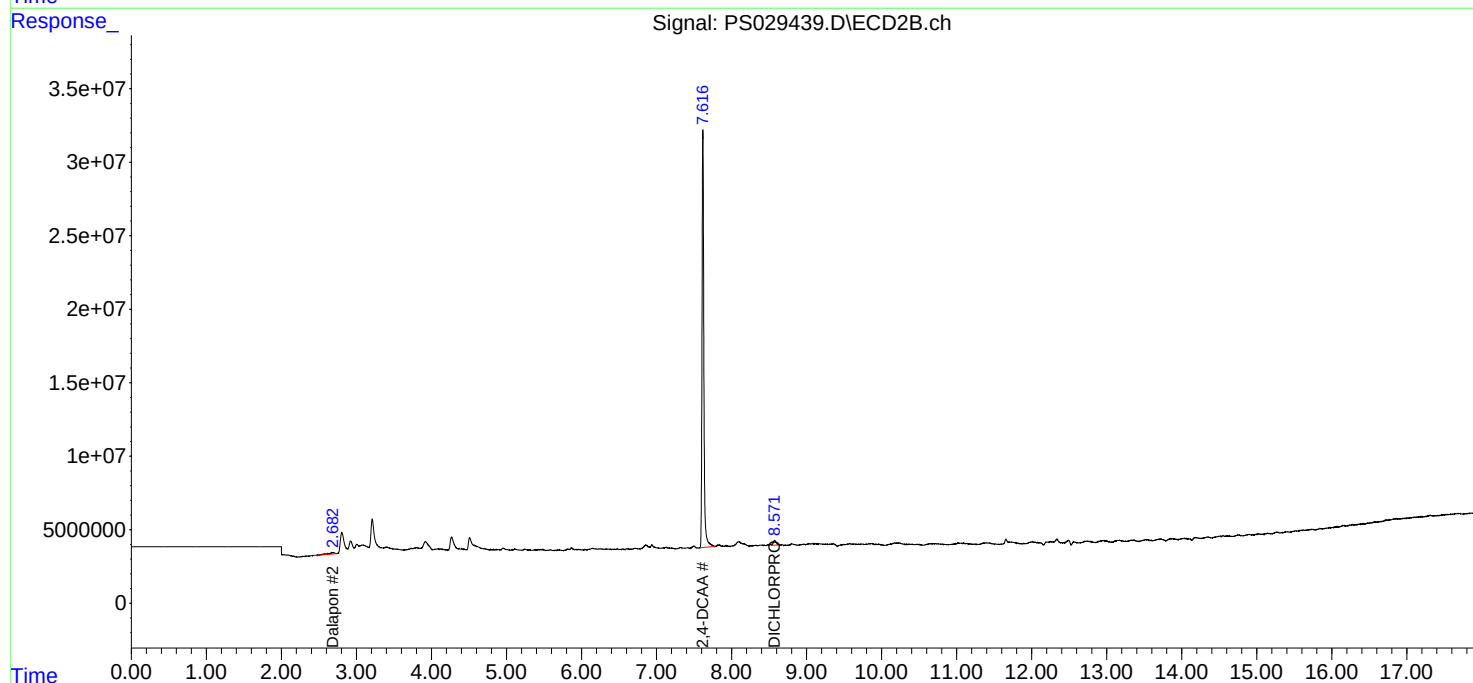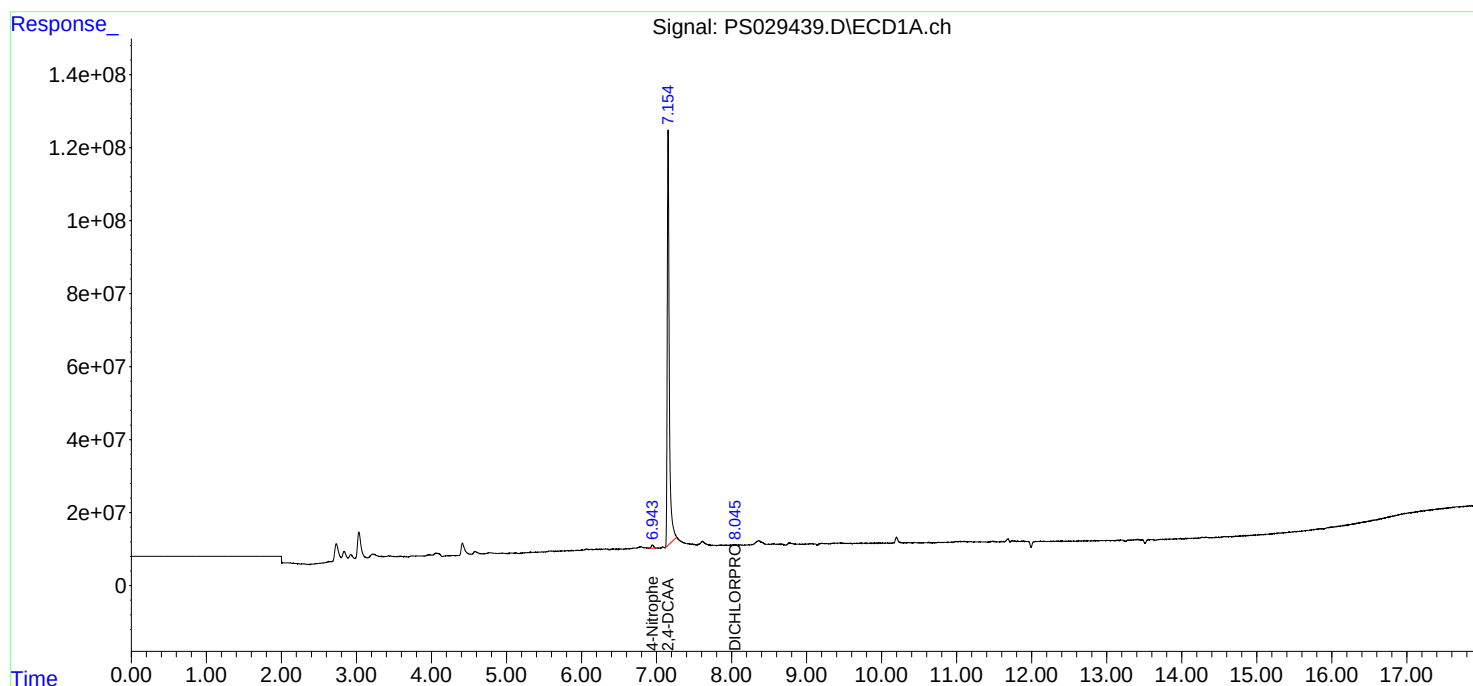


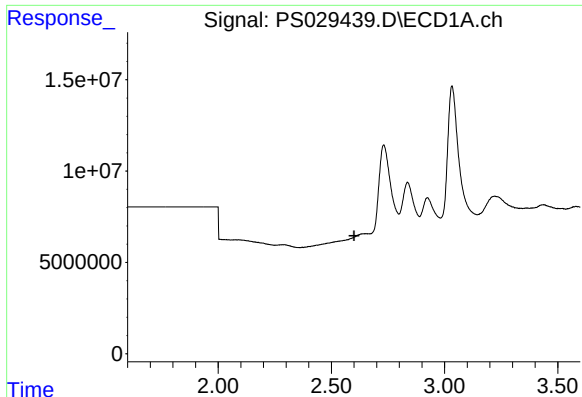

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.600 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

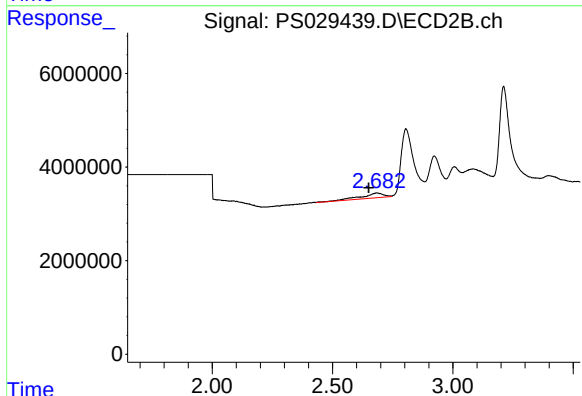


#1 Dalapon

R.T.: 2.684 min
Delta R.T.: 0.033 min
Response: 6904729
Conc: 3.26 ng/ml

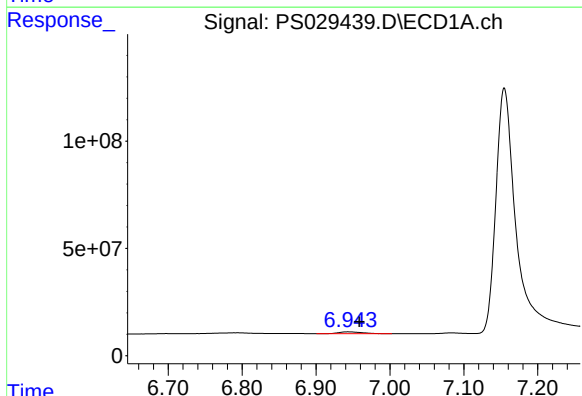


#3 4-Nitrophenol

R.T.: 6.943 min
Delta R.T.: -0.015 min
Response: 18936647
Conc: 8.09 ng/ml

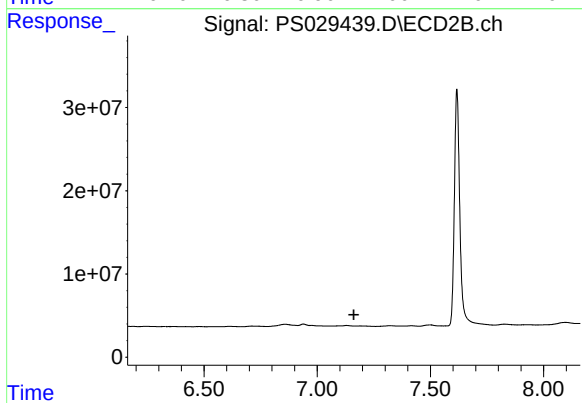

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.162 min
Response: 0
Conc: N.D.

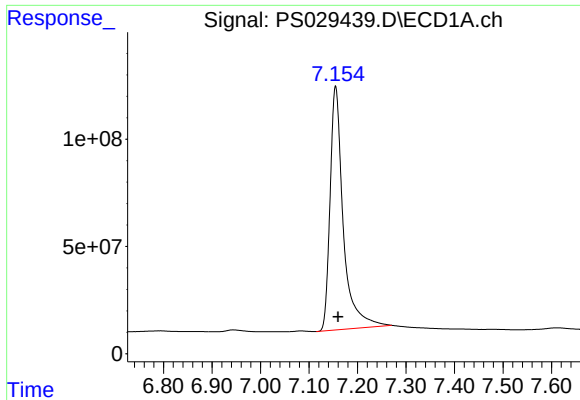

#4 2,4-DCAA


R.T.: 7.155 min
Delta R.T.: -0.005 min
Response: 2143397466
Conc: 520.17 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

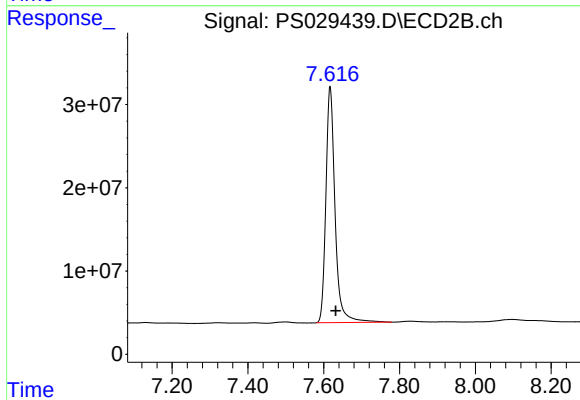


#4 2,4-DCAA

R.T.: 7.617 min
Delta R.T.: -0.015 min
Response: 478233098
Conc: 508.58 ng/ml

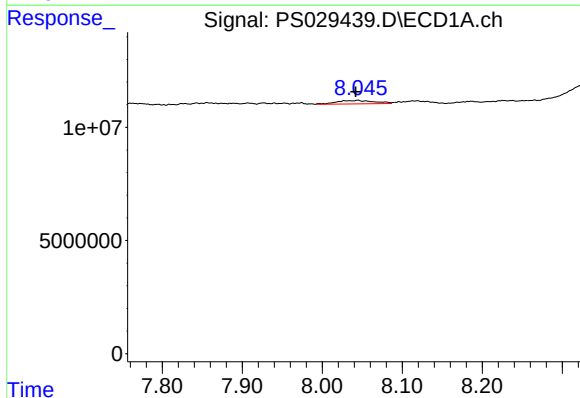

#8 DICHLORPROP

R.T.: 8.044 min
Delta R.T.: 0.003 min
Response: 4996498
Conc: 1.09 ng/ml

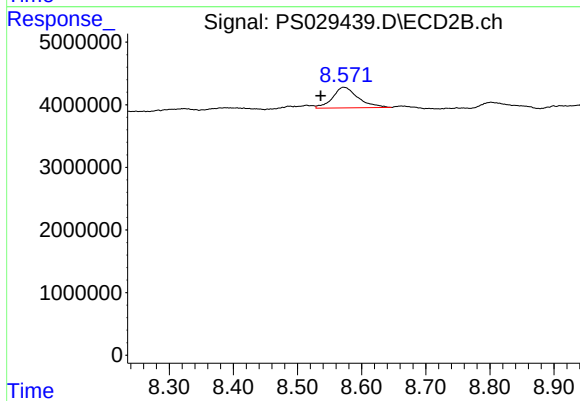

#8 DICHLORPROP

R.T.: 8.572 min
Delta R.T.: 0.036 min
Response: 9181981
Conc: 7.18 ng/ml