

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031419\
 Data File : PS003554.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2019 11:00
 Operator : EI\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 01:08:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.763	0	221085	N.D.	0.471 #
Target Compounds							
3) T	4-Nitroph...	0.000	9.959	0	746410	N.D.	3.320 #
5) T	DICAMBA	0.000	11.047	0	846260	N.D.	0.507 #
7) T	MCPA	0.000	11.700	0	376088	N.D.	0.218 #
10) T	Pentachlo...	0.000	13.177	0	209684	N.D.	0.032 #
11) T	2,4,5-TP ...	0.000	13.814	0	1015869	N.D.	0.399 #
13) T	2,4-DB	0.000	15.072	0	5335743	N.D.	20.895 #
14) T	DINOSEB	0.000	15.447	0	1970444	N.D.	1.104 #
15) T	Picloram	16.737	16.701	36560717	9992156	14.855	3.937 #
16) T	DCPA	0.000	16.629	0	6075492	N.D.	1.953 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031419\
Data File : PS003554.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2019 11:00
Operator : EI\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 01:08:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

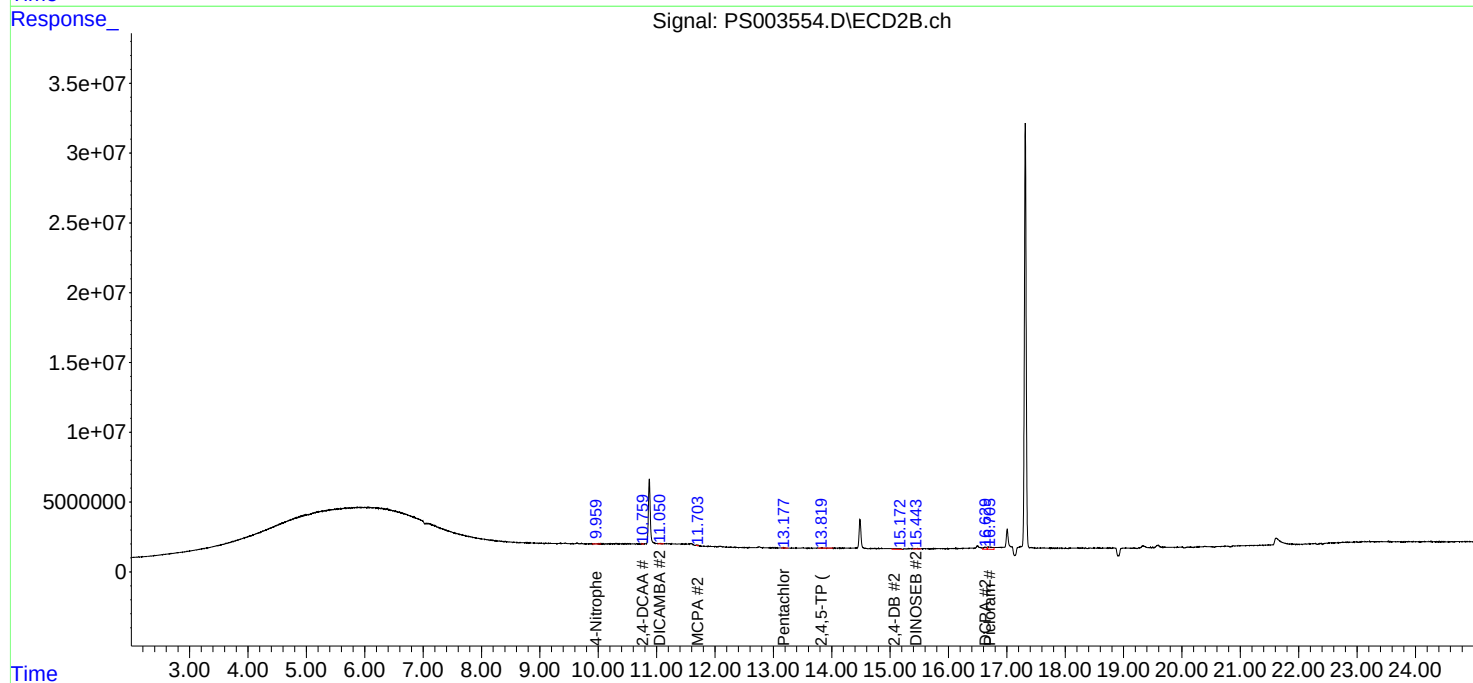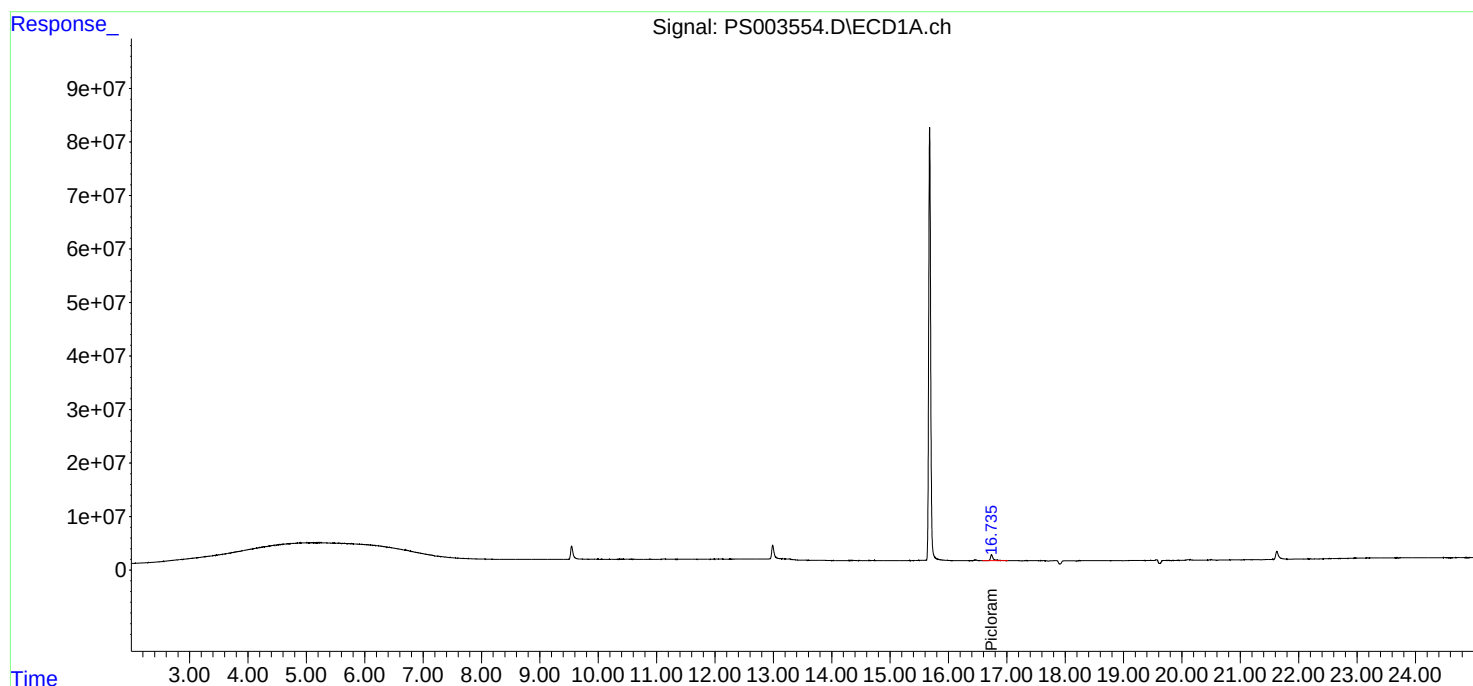


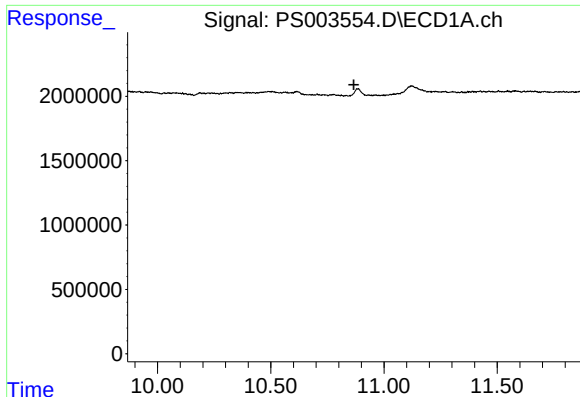

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

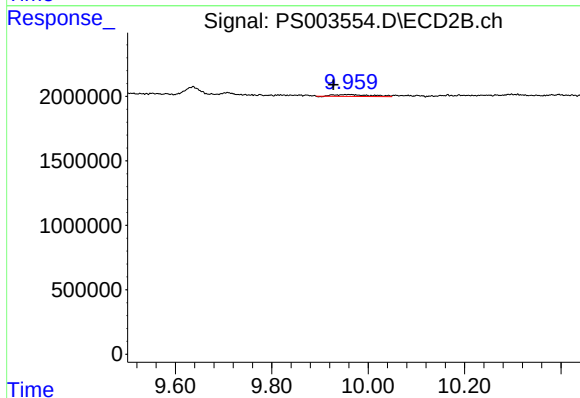


#3 4-Nitrophenol

R.T.: 9.959 min
Delta R.T.: 0.030 min
Response: 746410
Conc: 3.32 ng/ml

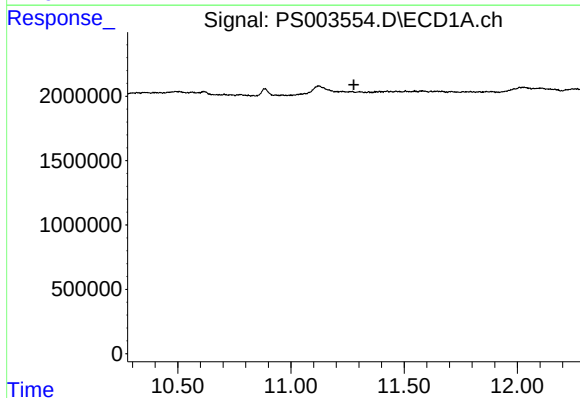


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 11.278 min
Response: 0
Conc: N.D.

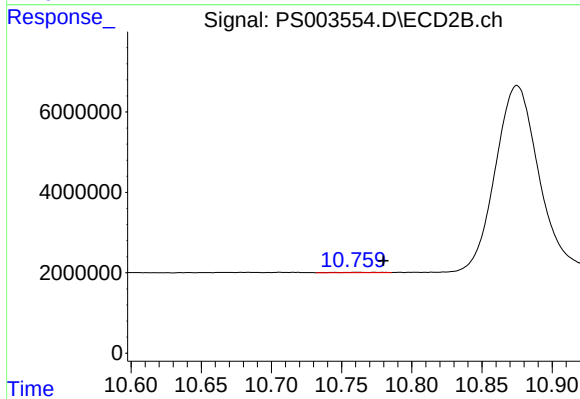

#4 2,4-DCAA


R.T.: 10.763 min
Delta R.T.: -0.017 min
Response: 221085
Conc: 0.47 ng/ml

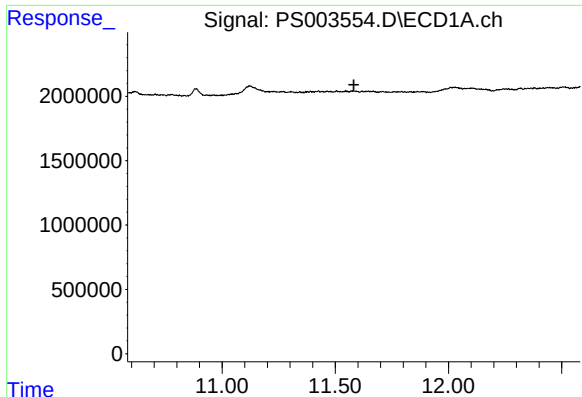

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 11.582 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

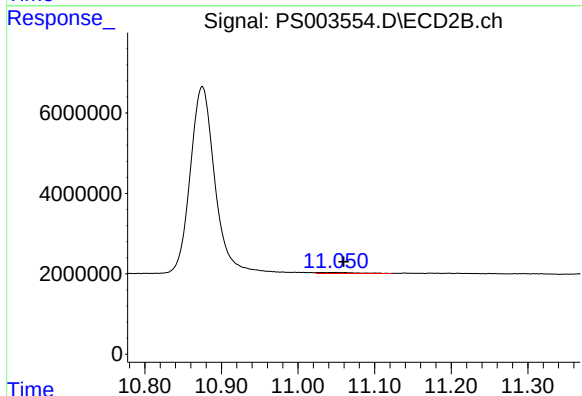


#5 DICAMBA

R.T.: 11.047 min
Delta R.T.: -0.012 min
Response: 846260
Conc: 0.51 ng/ml

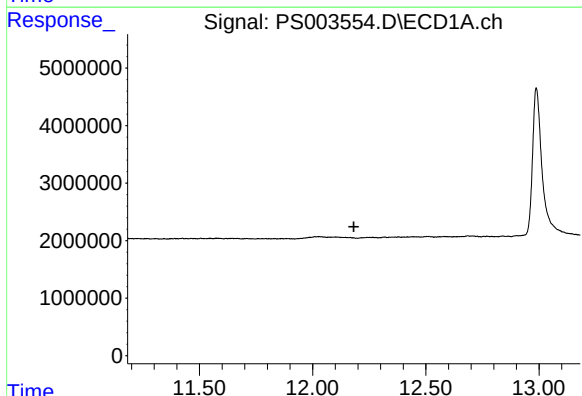


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.182 min
Response: 0
Conc: N.D.

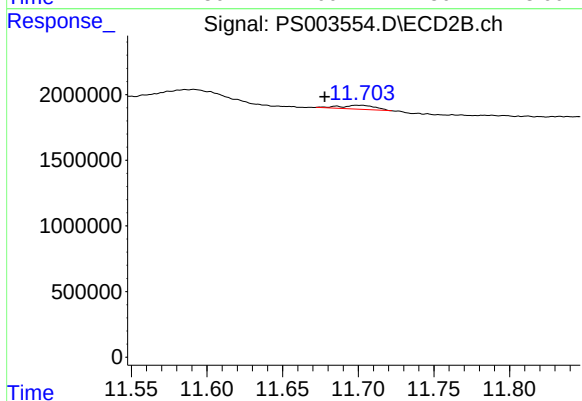

#7 MCPA


R.T.: 11.700 min
Delta R.T.: 0.022 min
Response: 376088
Conc: 0.22 ug/ml

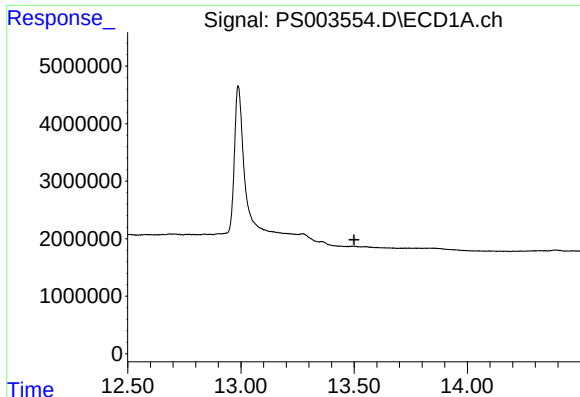

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.499 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

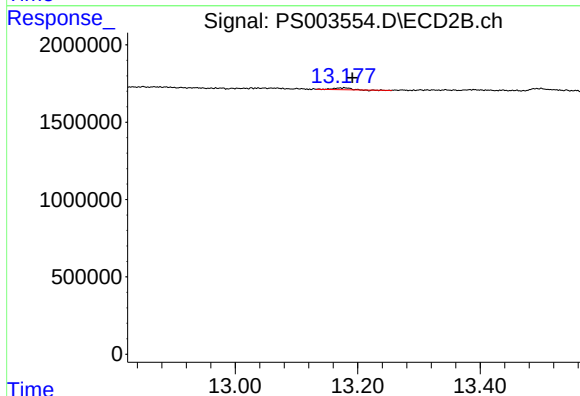


#10 Pentachlorophenol

R.T.: 13.177 min
Delta R.T.: -0.014 min
Response: 209684
Conc: 0.03 ng/ml

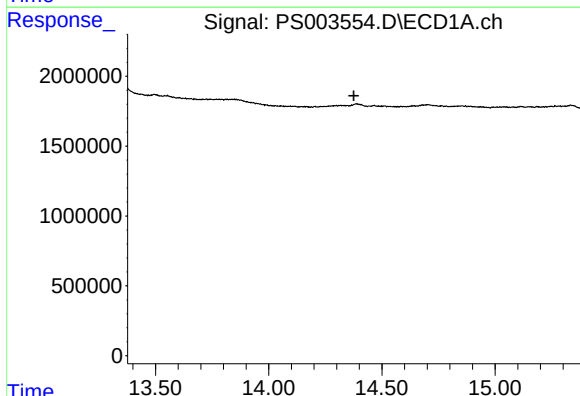


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

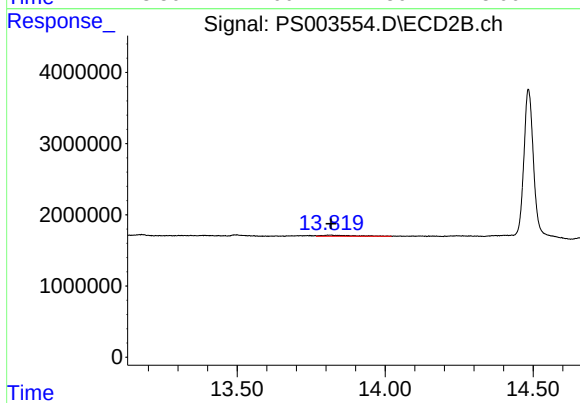

#11 2,4,5-TP (SILVEX)


R.T.: 13.814 min
Delta R.T.: -0.004 min
Response: 1015869
Conc: 0.40 ng/ml

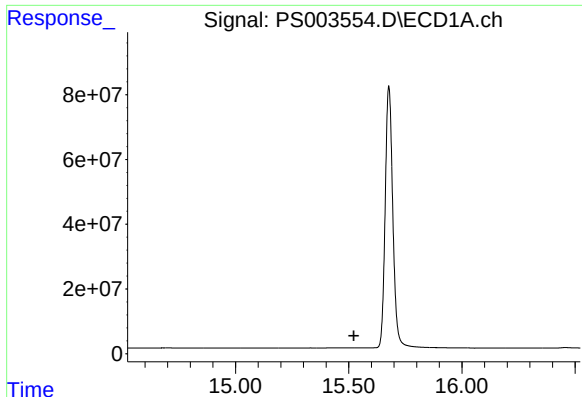

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.523 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

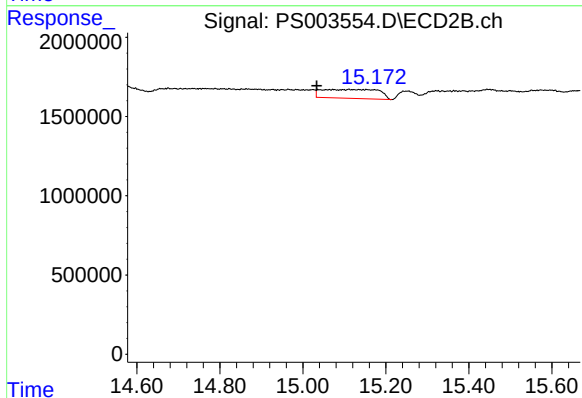


#13 2,4-DB

R.T.: 15.072 min
Delta R.T.: 0.038 min
Response: 5335743
Conc: 20.90 ng/ml

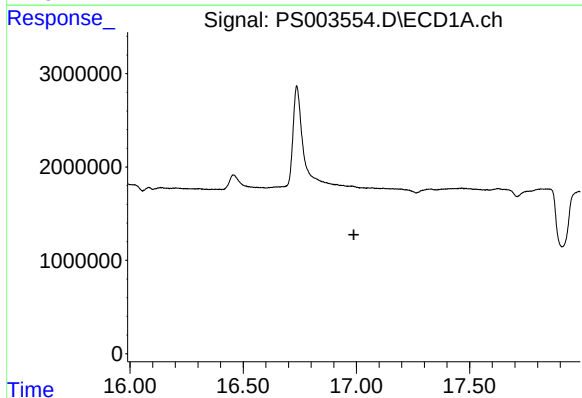


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

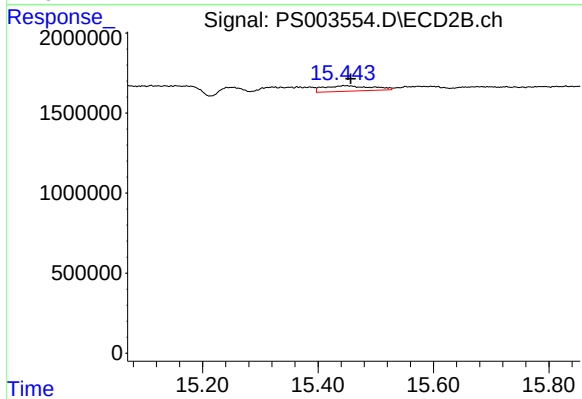

#14 DINOSEB


R.T.: 15.447 min
Delta R.T.: -0.010 min
Response: 1970444
Conc: 1.10 ng/ml

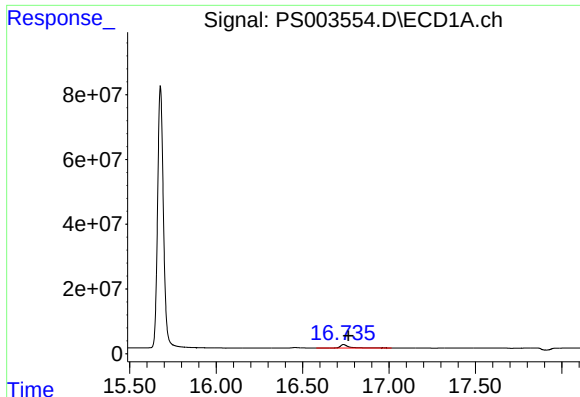

#15 Picloram


R.T.: 16.737 min
Delta R.T.: -0.028 min
Response: 36560717
Conc: 14.85 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

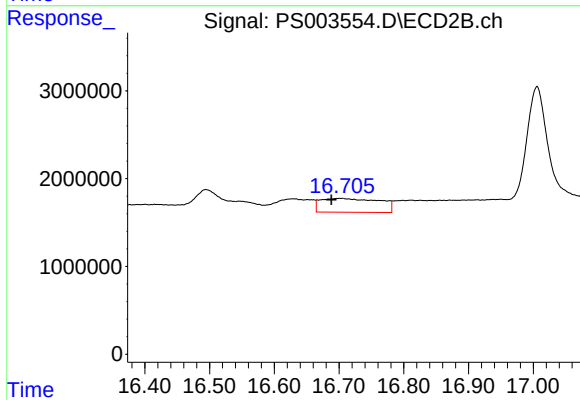


#15 Picloram

R.T.: 16.701 min
Delta R.T.: 0.013 min
Response: 9992156
Conc: 3.94 ng/ml

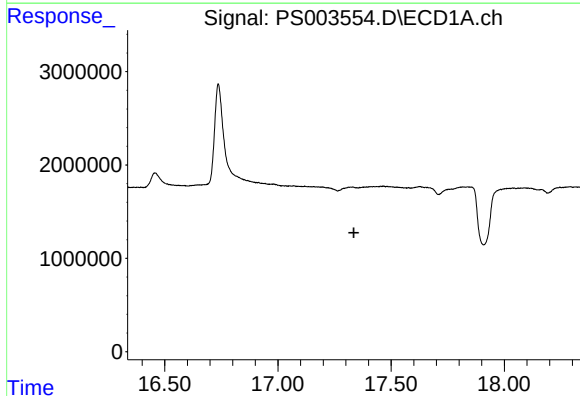

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.335 min
Response: 0
Conc: N.D.

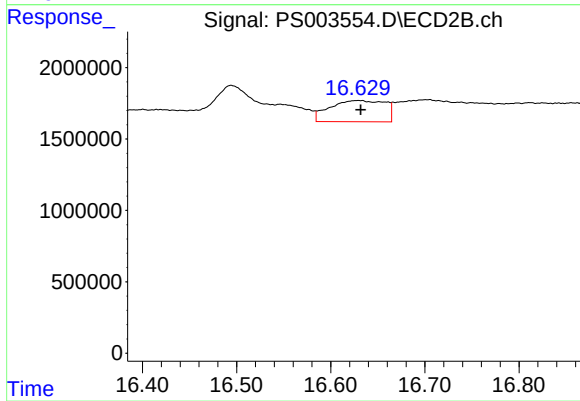

#16 DCPA

R.T.: 16.629 min
Delta R.T.: -0.003 min
Response: 6075492
Conc: 1.95 ng/ml