

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031419\
 Data File : PS003563.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2019 17:32
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 01:11:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.297	10.800	260.4E6	234.3E6	593.233	498.920
Target Compounds							
3) T	4-Nitroph...	0.000	9.994	0	31885	N.D.	0.142 #
7) T	MCPA	0.000	11.693	0	430898	N.D.	0.250 #
8) T	DICHLORPROP	0.000	12.139	0	6547758	N.D.	15.845 #
9) T	2,4-D	0.000	12.637	0	96257	N.D.	0.183 #
10) T	Pentachlo...	0.000	13.212	0	982094	N.D.	0.149 #
11) T	2,4,5-TP ...	0.000	13.756	0	357356	N.D.	0.140 #
12) T	2,4,5-T	0.000	14.333	0	1137969	N.D.	0.564 #
13) T	2,4-DB	0.000	15.051	0	3295845	N.D.	12.907 #
14) T	DINOSEB	0.000	15.474	0	3709488	N.D.	2.078 #
15) T	Picloram	16.758	16.706	54037310	15450190	21.955	6.087 #
16) T	DCPA	0.000	16.655	0	16022297	N.D.	5.151 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031419\
Data File : PS003563.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2019 17:32
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 01:11:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

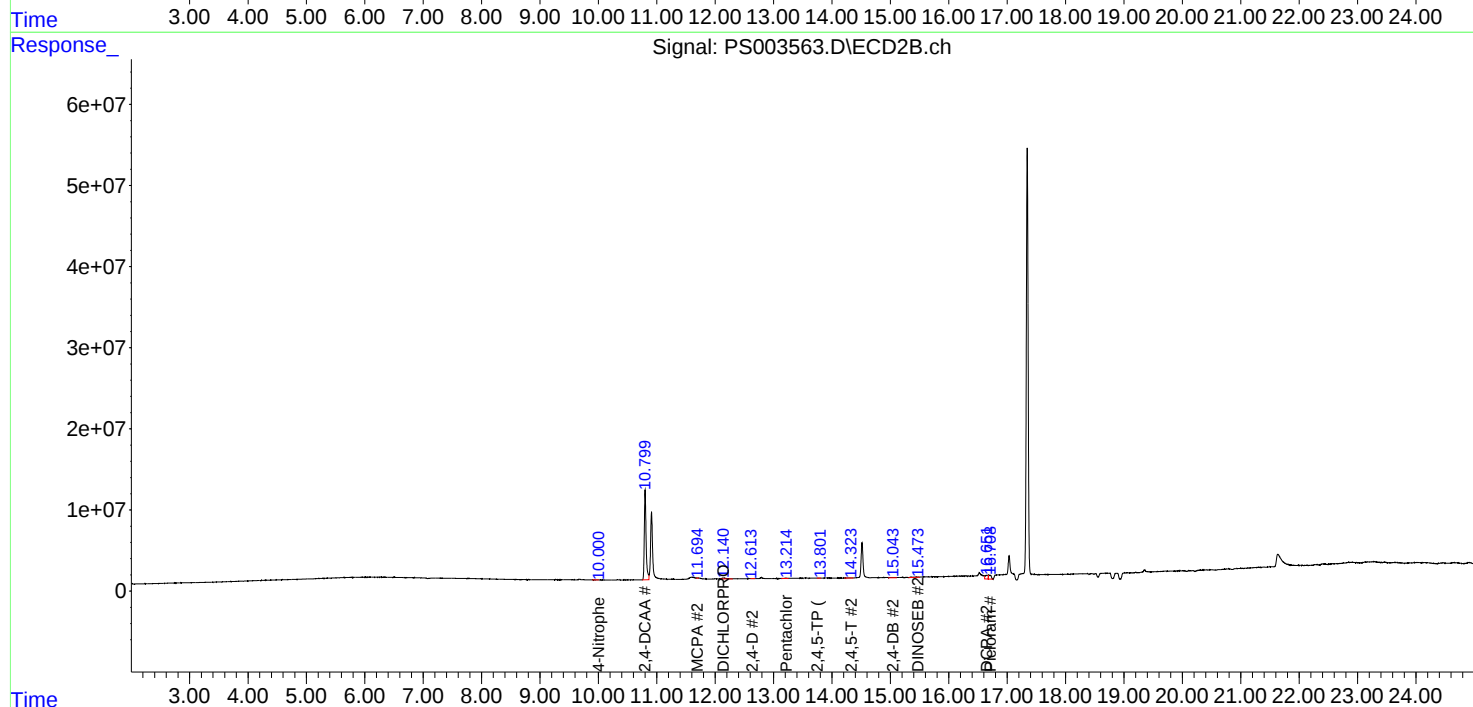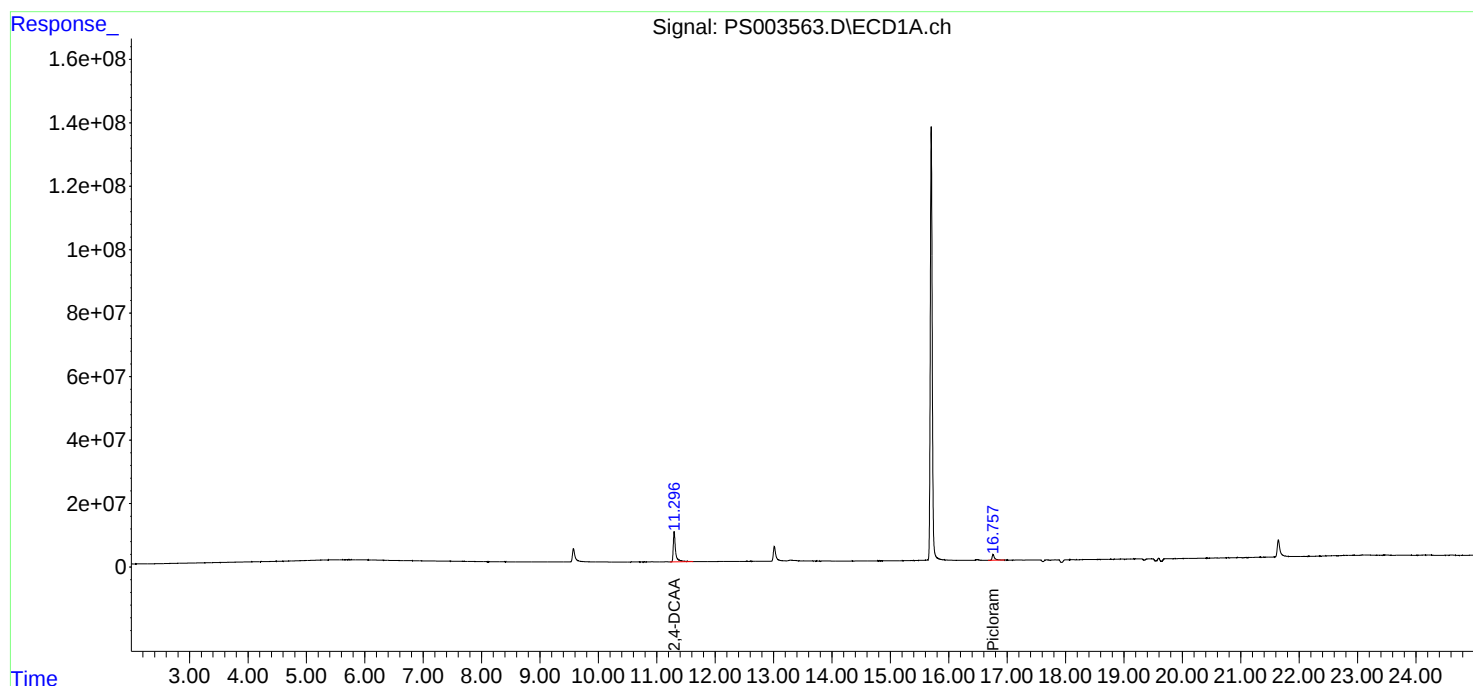


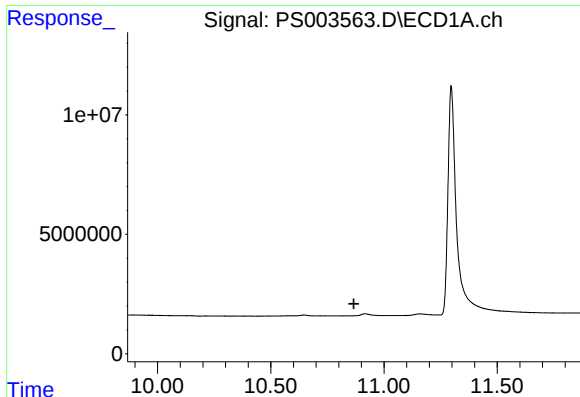

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

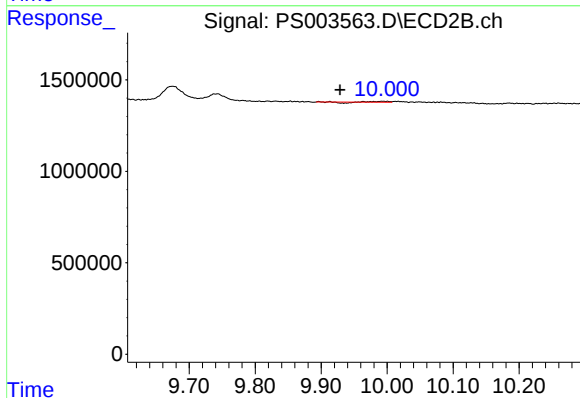


#3 4-Nitrophenol

R.T.: 9.994 min
Delta R.T.: 0.065 min
Response: 31885
Conc: 0.14 ng/ml

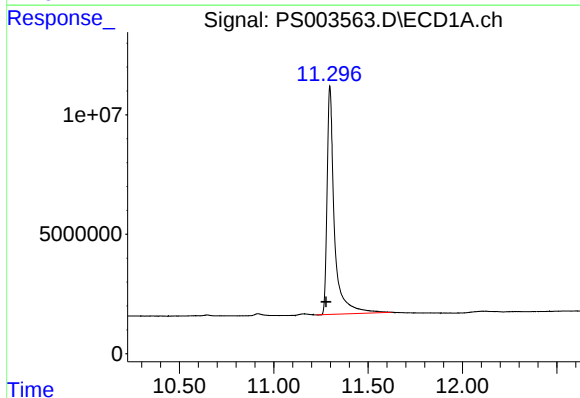


#4 2,4-DCAA

R.T.: 11.297 min
Delta R.T.: 0.019 min
Response: 260443832
Conc: 593.23 ng/ml

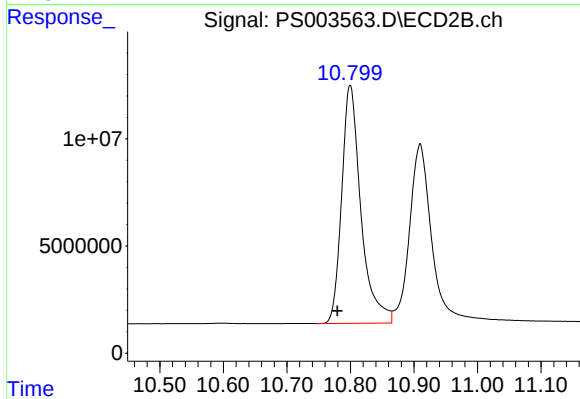

#4 2,4-DCAA


R.T.: 10.800 min
Delta R.T.: 0.020 min
Response: 234277653
Conc: 498.92 ng/ml

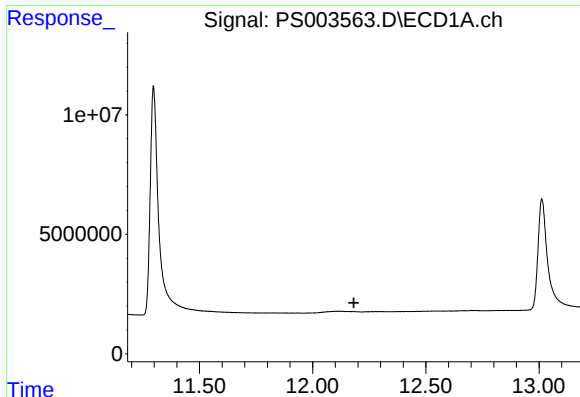

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.182 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

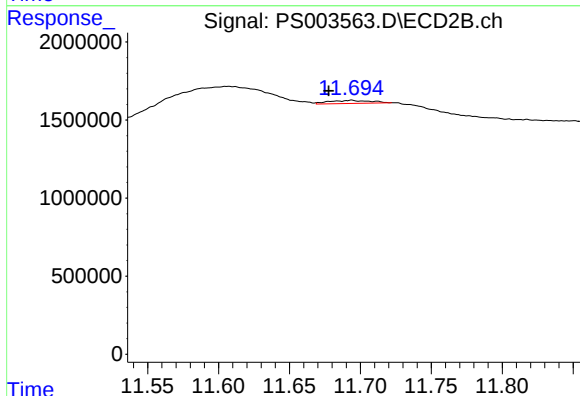


#7 MCPA

R.T.: 11.693 min
Delta R.T.: 0.016 min
Response: 430898
Conc: 0.25 ug/ml

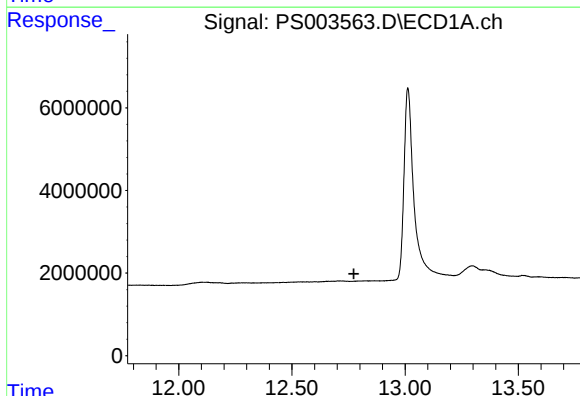


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 12.773 min
Response: 0
Conc: N.D.

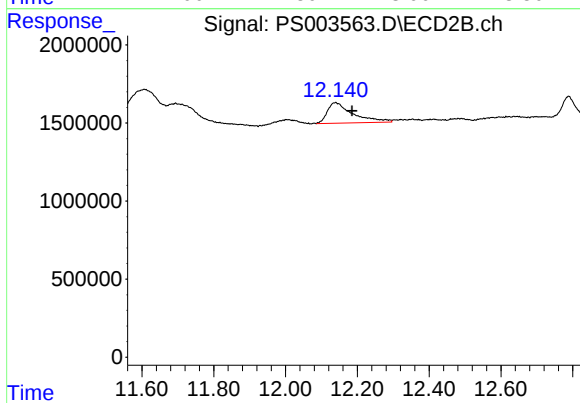

#8 DICHLORPROP


R.T.: 12.139 min
Delta R.T.: -0.046 min
Response: 6547758
Conc: 15.84 ng/ml

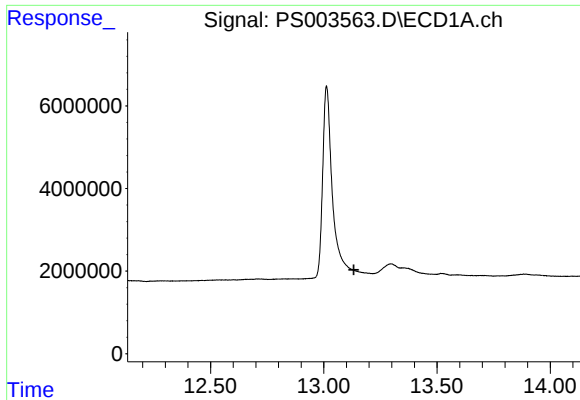

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.133 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

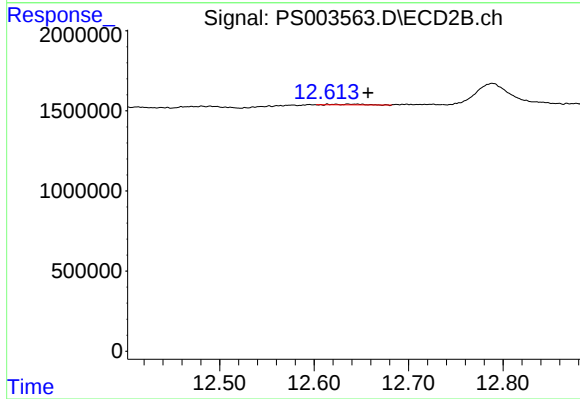


#9 2,4-D

R.T.: 12.637 min
Delta R.T.: -0.020 min
Response: 96257
Conc: 0.18 ng/ml

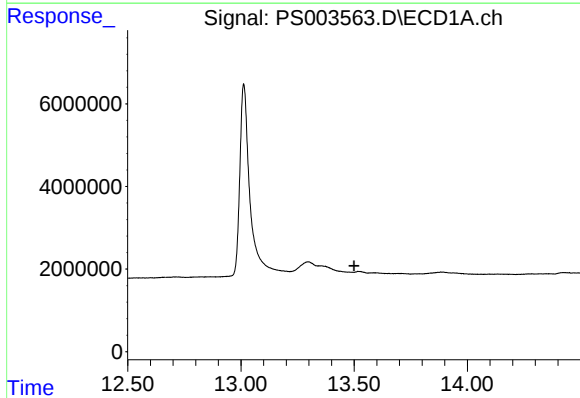


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 13.499 min
Response: 0
Conc: N.D.

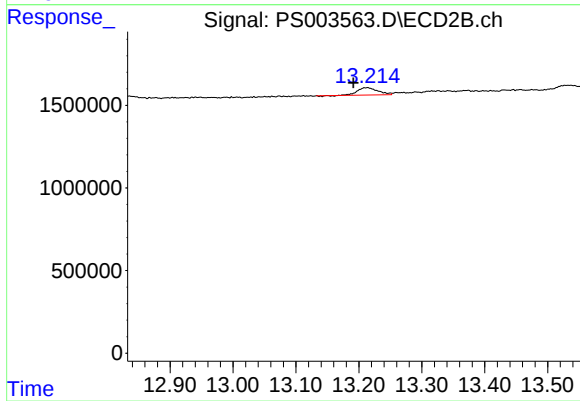

#10 Pentachlorophenol


R.T.: 13.212 min
Delta R.T.: 0.021 min
Response: 982094
Conc: 0.15 ng/ml

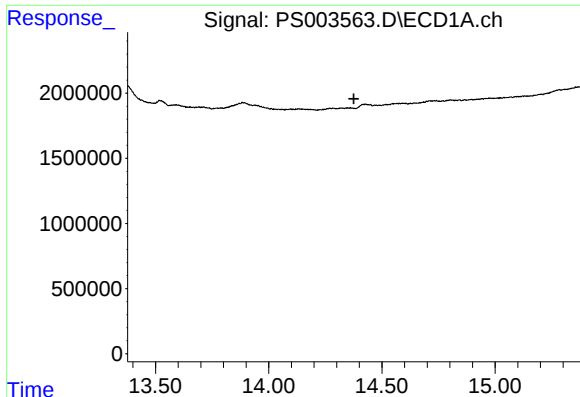

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

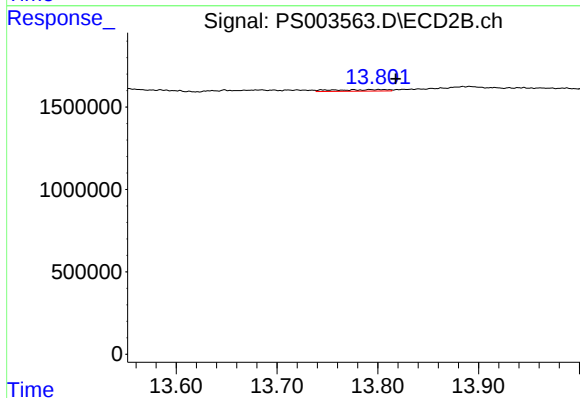


#11 2,4,5-TP (SILVEX)

R.T.: 13.756 min
Delta R.T.: -0.062 min
Response: 357356
Conc: 0.14 ng/ml

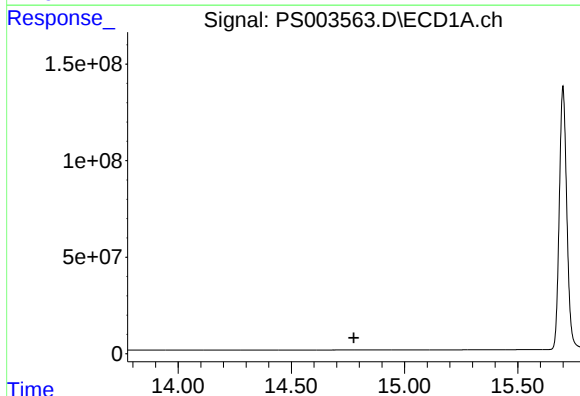


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

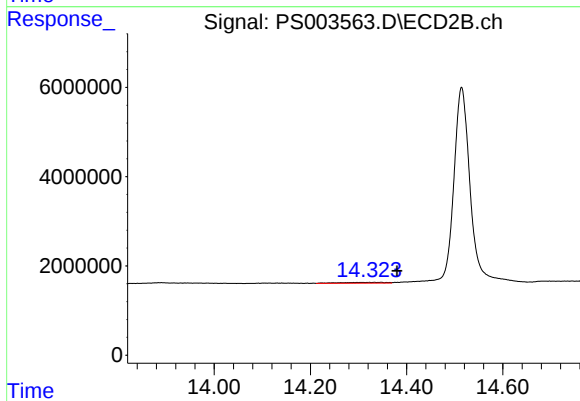

#12 2,4,5-T


R.T.: 14.333 min
Delta R.T.: -0.047 min
Response: 1137969
Conc: 0.56 ng/ml

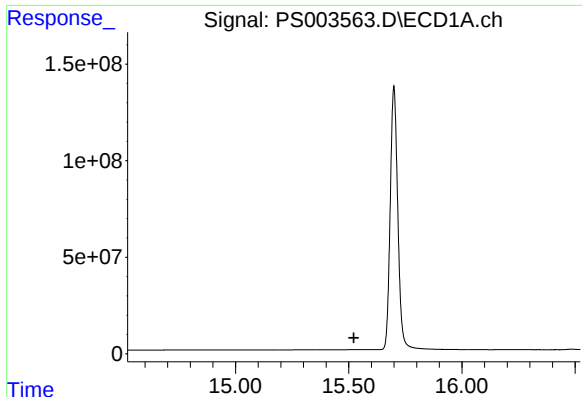

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.523 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

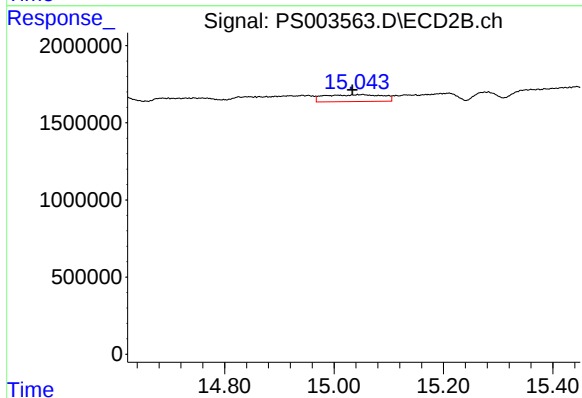


#13 2,4-DB

R.T.: 15.051 min
Delta R.T.: 0.017 min
Response: 3295845
Conc: 12.91 ng/ml

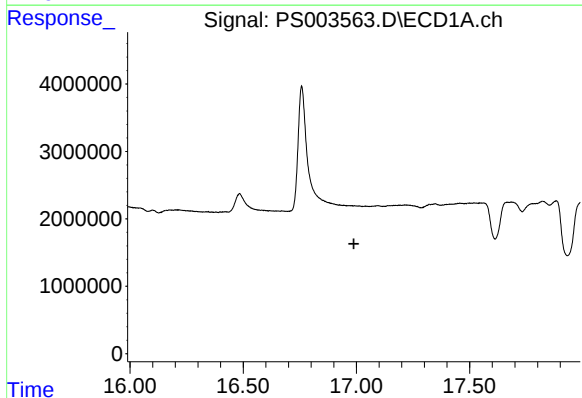


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

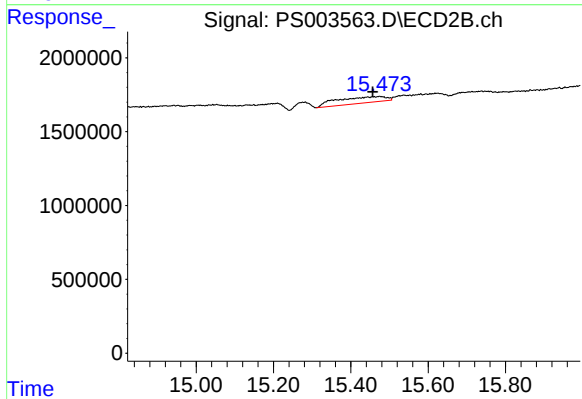

#14 DINOSEB


R.T.: 15.474 min
Delta R.T.: 0.017 min
Response: 3709488
Conc: 2.08 ng/ml

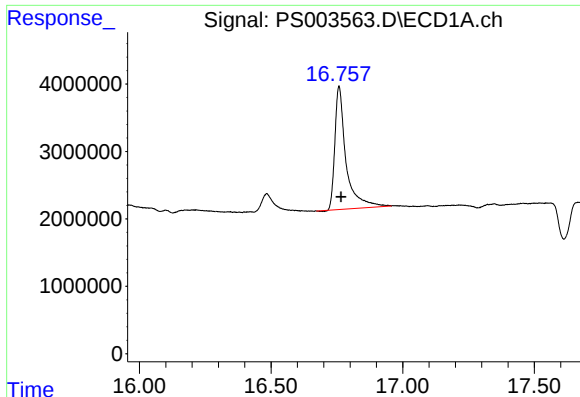

#15 Picloram


R.T.: 16.758 min
Delta R.T.: -0.007 min
Response: 54037310
Conc: 21.96 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

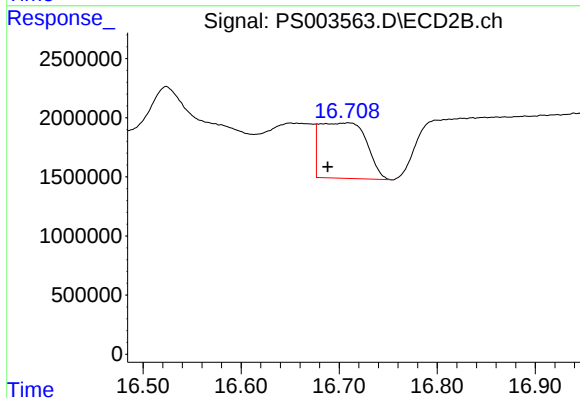


#15 Picloram

R.T.: 16.706 min
Delta R.T.: 0.018 min
Response: 15450190
Conc: 6.09 ng/ml

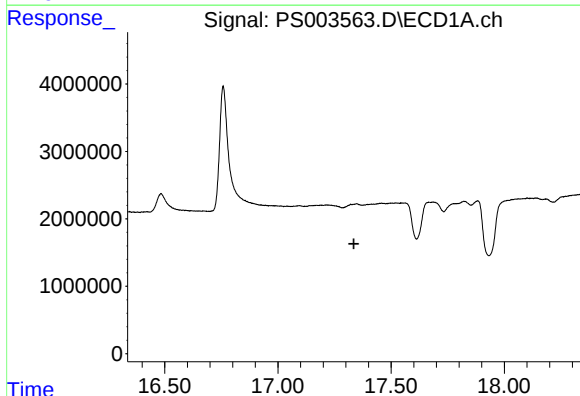

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.335 min
Response: 0
Conc: N.D.

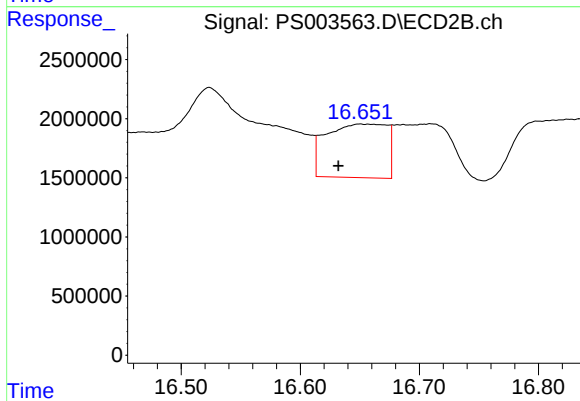

#16 DCPA

R.T.: 16.655 min
Delta R.T.: 0.023 min
Response: 16022297
Conc: 5.15 ng/ml