

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031419\
 Data File : PS003566.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2019 19:05
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 01:12:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.291	10.776	271.1E6	236.1E6	617.423	502.897
Target Compounds							
2) T	3,5-DICHL...	0.000	8.979	0	40911	N.D.	0.066 #
3) T	4-Nitroph...	0.000	9.977	0	72631	N.D.	0.323 #
7) T	MCPA	0.000	11.667	0	555213	N.D.	0.322 #
8) T	DICHLORPROP	0.000	12.118	0	8841725	N.D.	21.396 #
10) T	Pentachlo...	0.000	13.190	0	1156821	N.D.	0.176 #
11) T	2,4,5-TP ...	0.000	13.862	0	486919	N.D.	0.191 #
13) T	2,4-DB	0.000	15.020	0	3269305	N.D.	12.803 #
14) T	DINOSEB	0.000	15.414	0	3360715	N.D.	1.883 #
15) T	Picloram	16.752	16.629	57857064	27885687	23.507	10.987 #
16) T	DCPA	0.000	16.629	0	27885687	N.D.	8.965 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031419\
Data File : PS003566.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2019 19:05
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 01:12:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

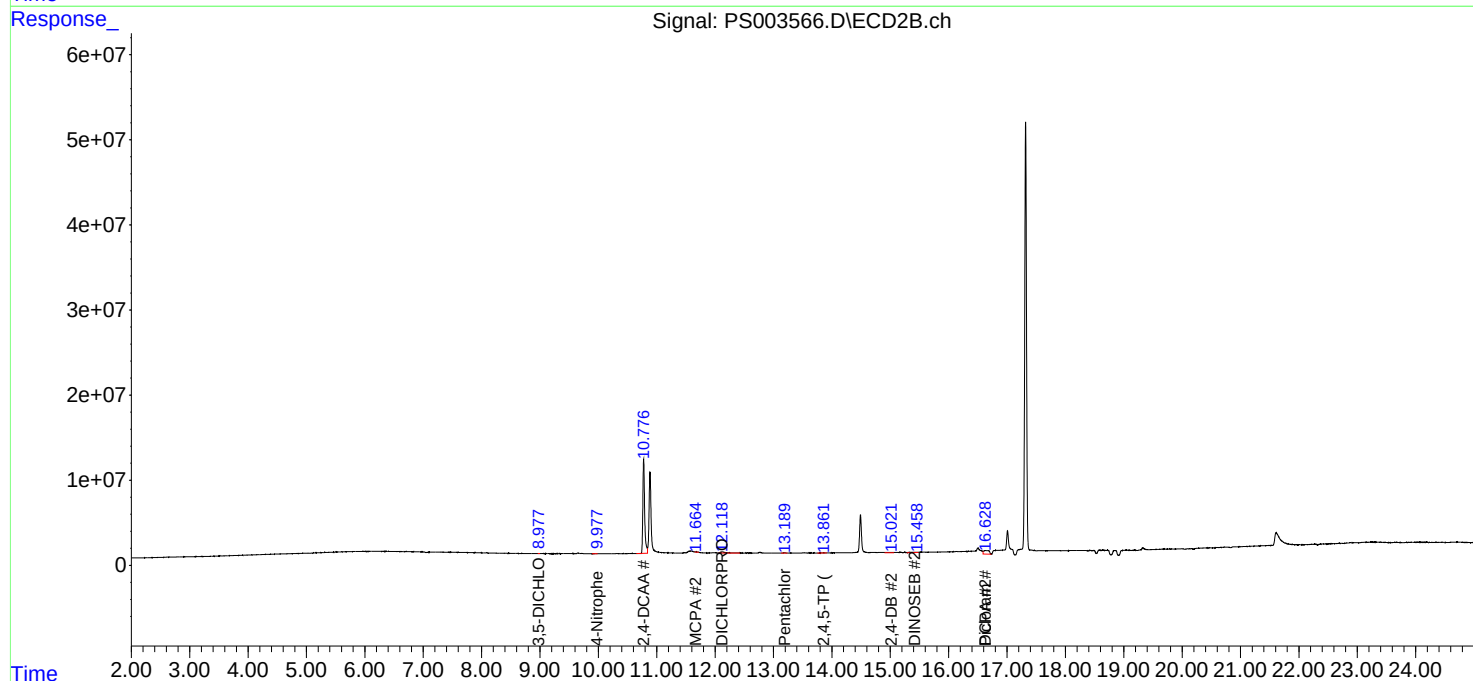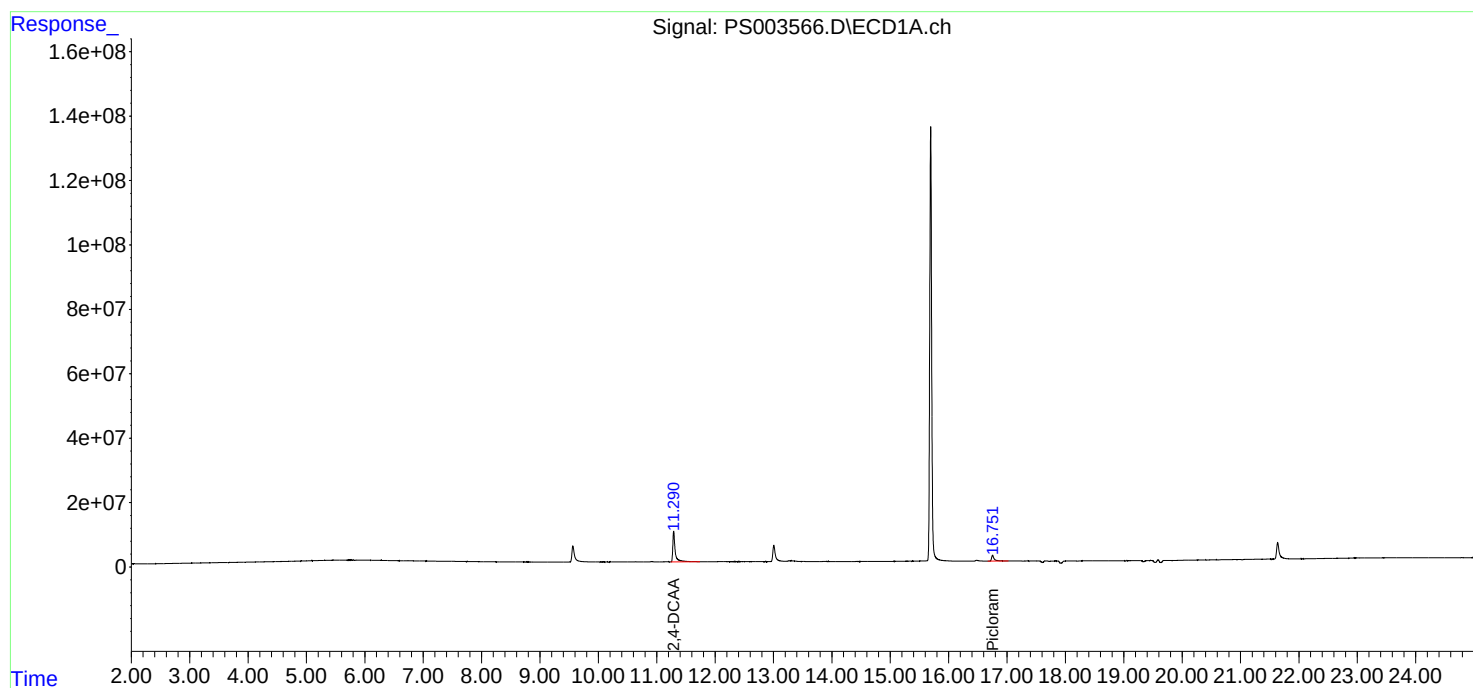


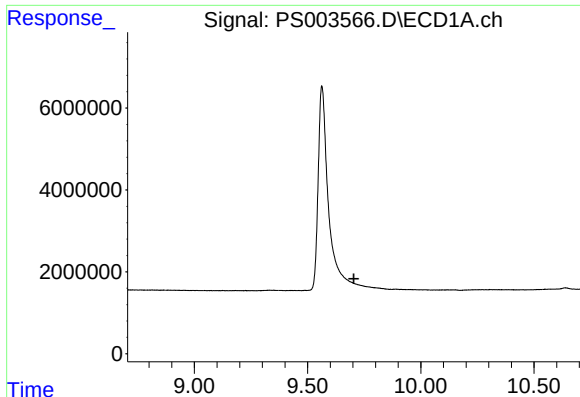

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.705 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

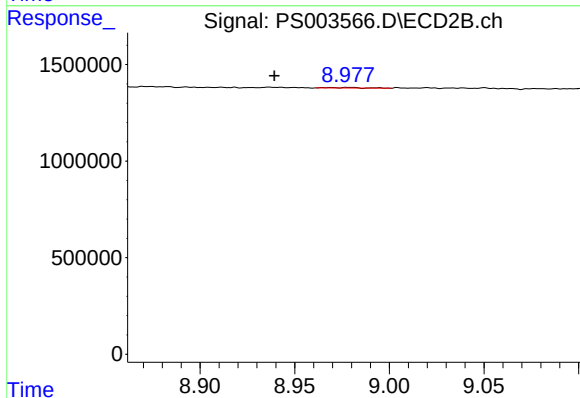


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 8.979 min
Delta R.T.: 0.039 min
Response: 40911
Conc: 0.07 ng/ml

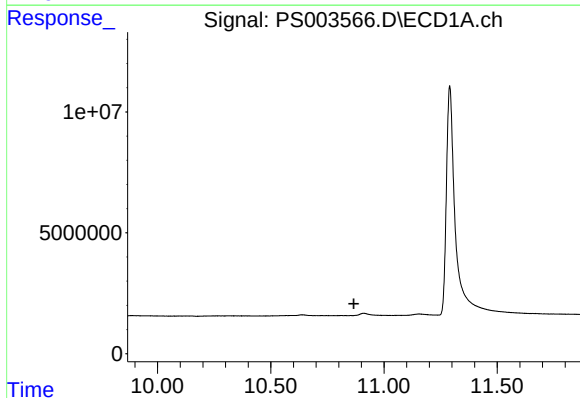


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

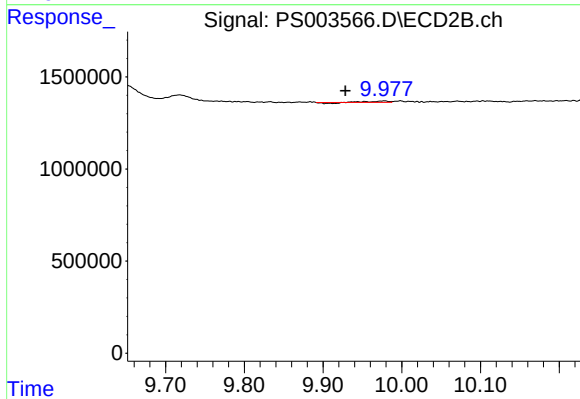

#3 4-Nitrophenol


R.T.: 9.977 min
Delta R.T.: 0.049 min
Response: 72631
Conc: 0.32 ng/ml

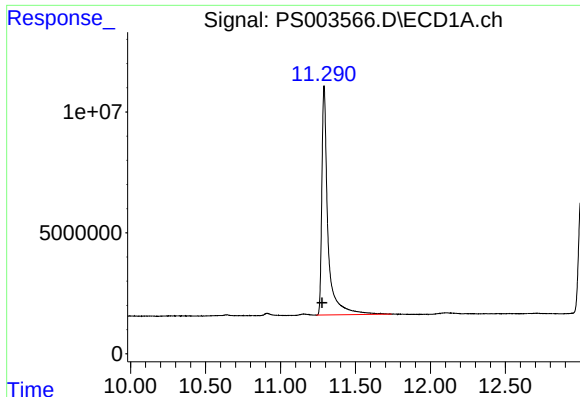

#4 2,4-DCAA


R.T.: 11.291 min
Delta R.T.: 0.013 min
Response: 271063639
Conc: 617.42 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

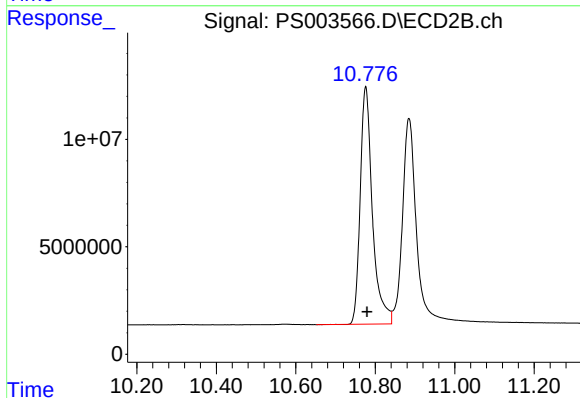


#4 2,4-DCAA

R.T.: 10.776 min
Delta R.T.: -0.004 min
Response: 236144896
Conc: 502.90 ng/ml

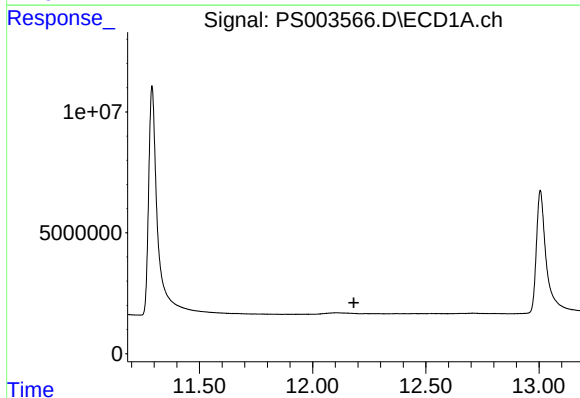


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.182 min
Response: 0
Conc: N.D.

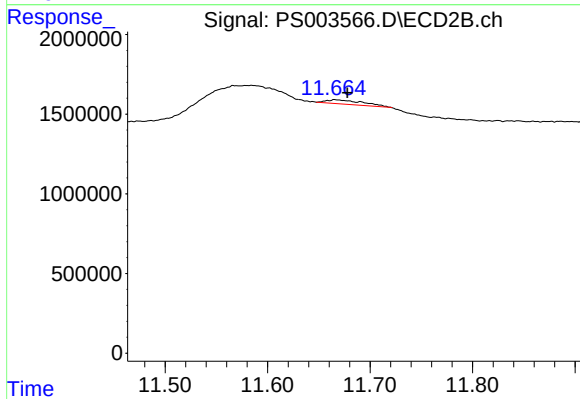

#7 MCPA


R.T.: 11.667 min
Delta R.T.: -0.011 min
Response: 555213
Conc: 0.32 ug/ml

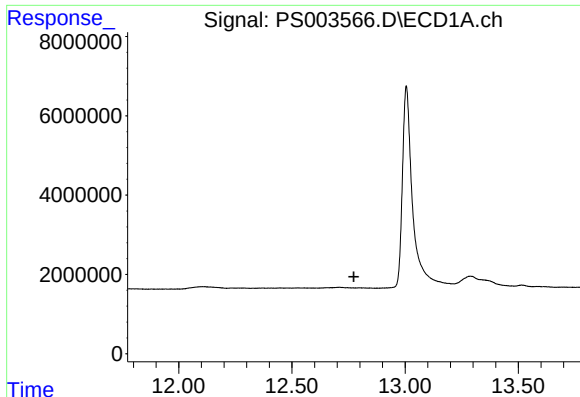

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 12.773 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

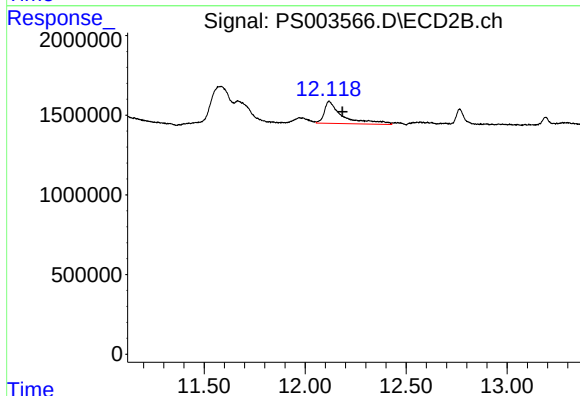


#8 DICHLORPROP

R.T.: 12.118 min
Delta R.T.: -0.067 min
Response: 8841725
Conc: 21.40 ng/ml

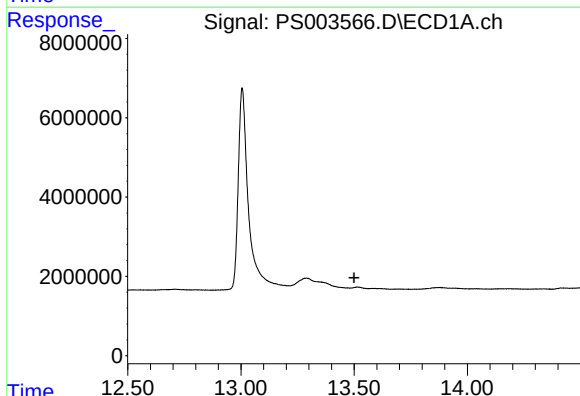


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.499 min
Response: 0
Conc: N.D.

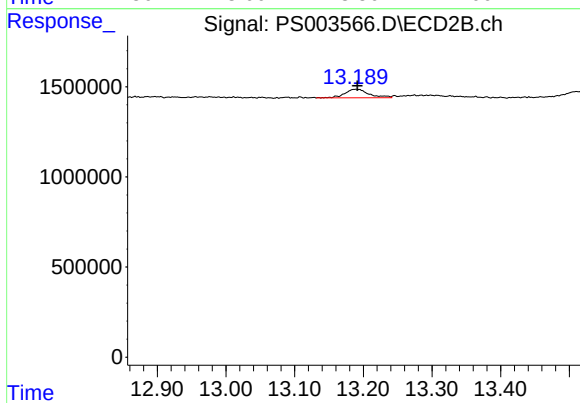

#10 Pentachlorophenol


R.T.: 13.190 min
Delta R.T.: -0.002 min
Response: 1156821
Conc: 0.18 ng/ml

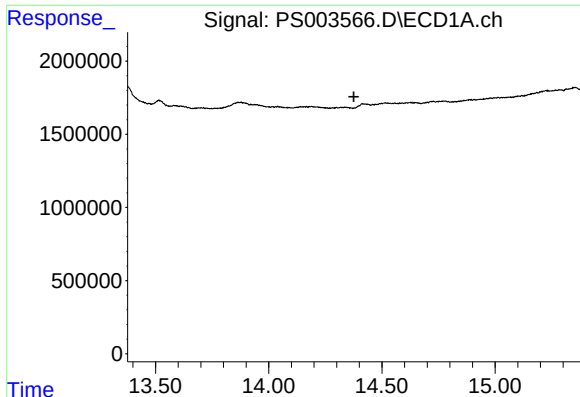

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

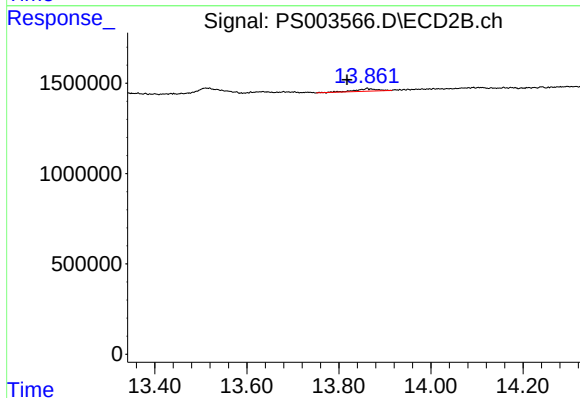


#11 2,4,5-TP (SILVEX)

R.T.: 13.862 min
Delta R.T.: 0.045 min
Response: 486919
Conc: 0.19 ng/ml

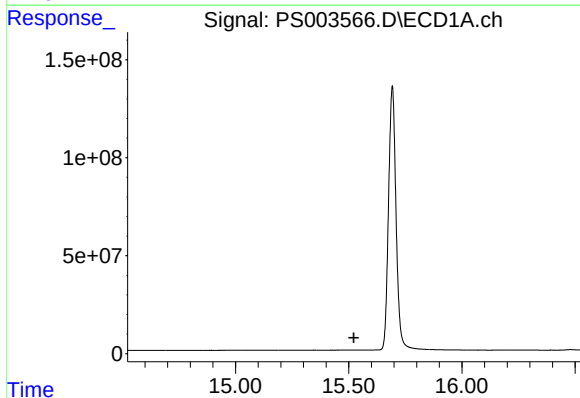


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.523 min
Response: 0
Conc: N.D.

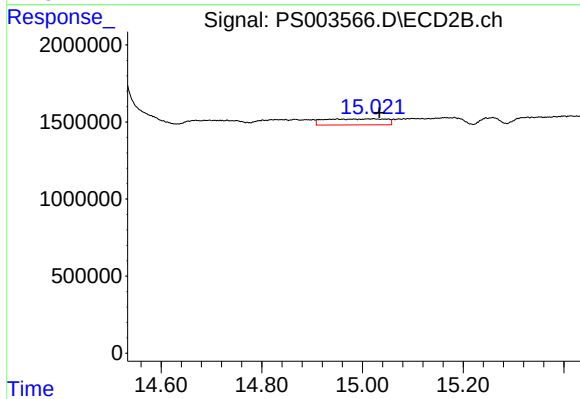

#13 2,4-DB


R.T.: 15.020 min
Delta R.T.: -0.013 min
Response: 3269305
Conc: 12.80 ng/ml

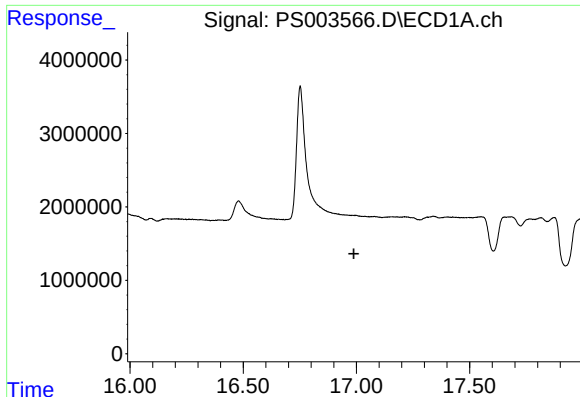

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

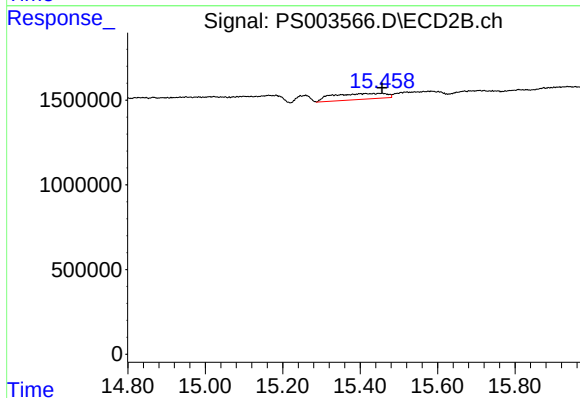


#14 DINOSEB

R.T.: 15.414 min
Delta R.T.: -0.042 min
Response: 3360715
Conc: 1.88 ng/ml

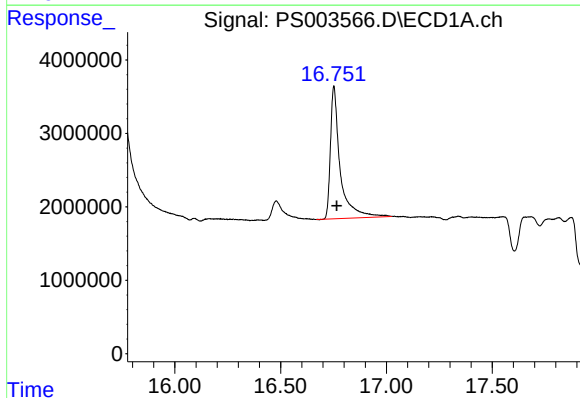


#15 Picloram

R.T.: 16.752 min
Delta R.T.: -0.013 min
Response: 57857064
Conc: 23.51 ng/ml

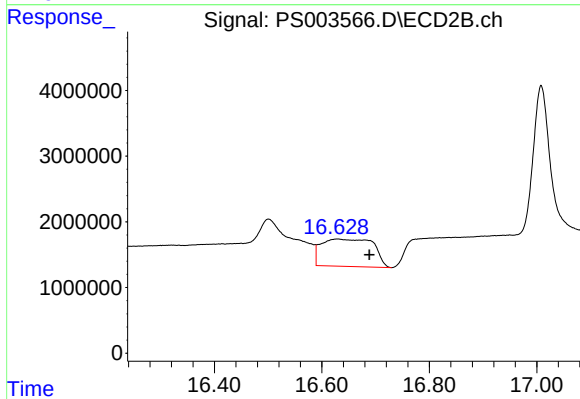

#15 Picloram


R.T.: 16.629 min
Delta R.T.: -0.059 min
Response: 27885687
Conc: 10.99 ng/ml

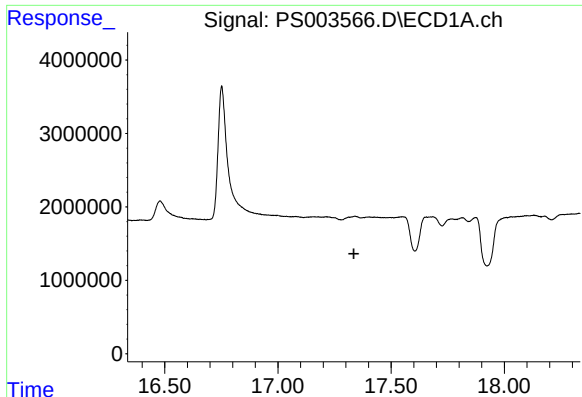

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.335 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

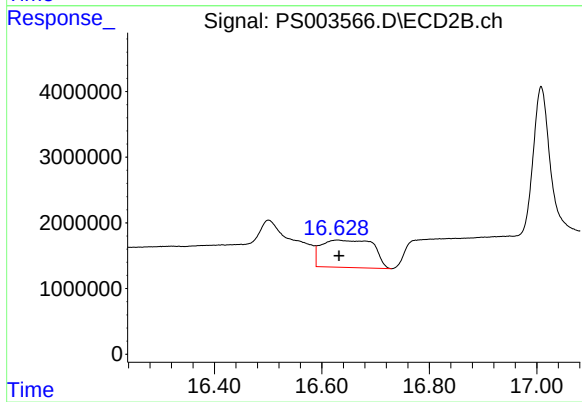

#16 DCPA

R.T.: 16.629 min
Delta R.T.: -0.003 min
Response: 27885687
Conc: 8.97 ng/ml